

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032221\
 Data File : PL065467.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2021 13:27
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:02:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.786	135.9E6	121.5E6	57.228	44.278
28)	SA Decachlor...	7.929	8.736	105.3E6	91961732	43.596	46.396
Target Compounds							
23)	Chlordane-1	4.126	4.751	46534222	47116079	540.156	417.730
24)	Chlordane-2	4.613	5.213	54803285	48469359	505.281	445.028
25)	Chlordane-3	5.164	5.850	145.1E6	176.9E6	486.397	434.026
26)	Chlordane-4	5.220	5.921	131.7E6	210.9E6	483.474	438.473
27)	Chlordane-5	6.032	6.718	45938275	34108546	459.486	426.259



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032221\
Data File : PL065467.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2021 13:27
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:02:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

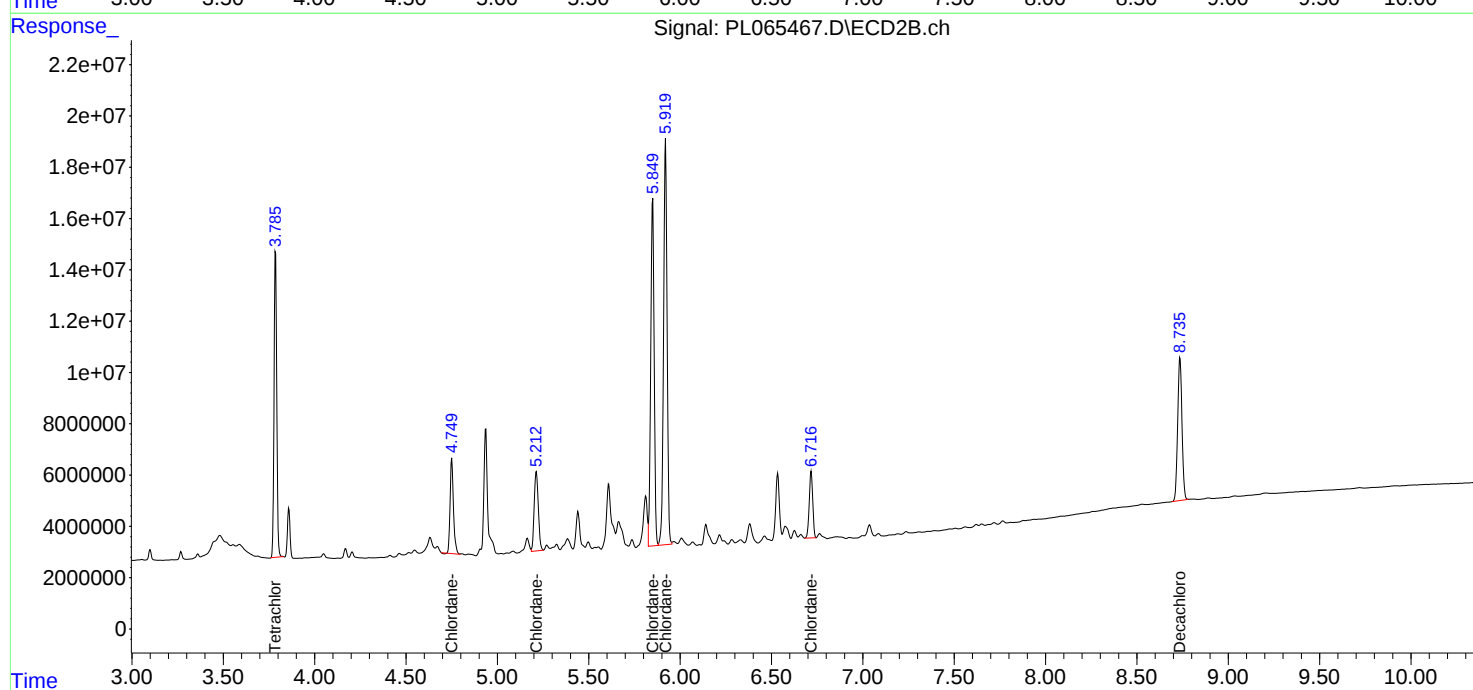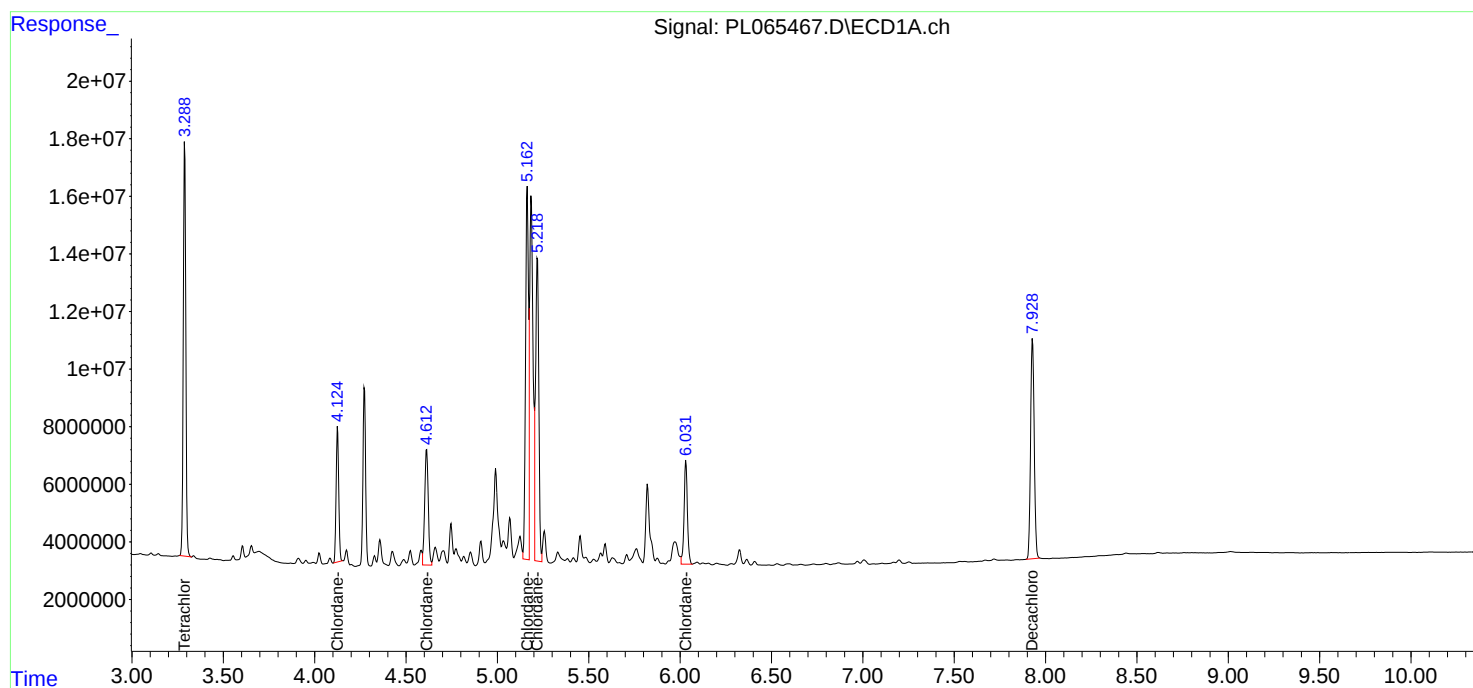


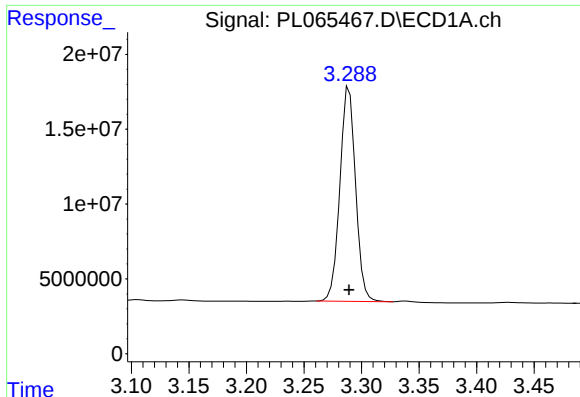

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 135904697
Conc: 57.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

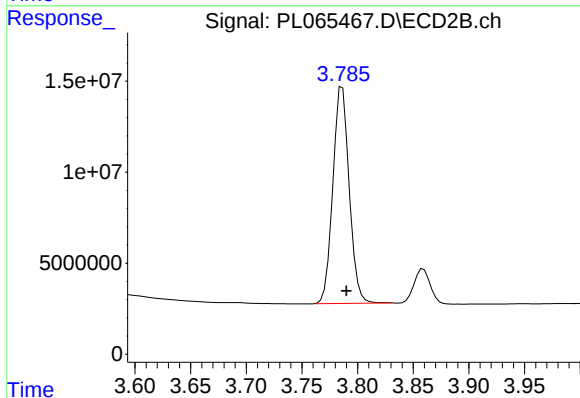


#1 Tetrachloro-m-xylene

R.T.: 3.786 min
Delta R.T.: -0.004 min
Response: 121531810
Conc: 44.28 ng/ml

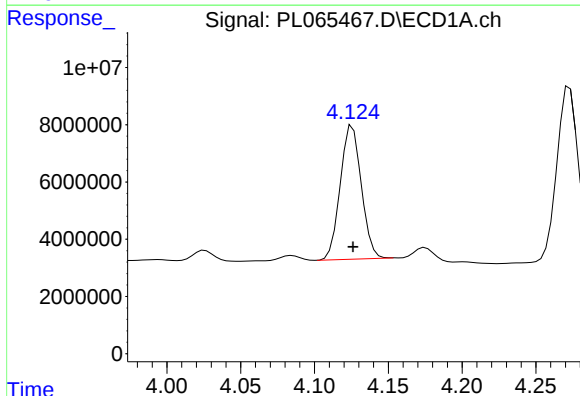


#23 Chlordane-1

R.T.: 4.126 min
Delta R.T.: 0.000 min
Response: 46534222
Conc: 540.16 ng/ml

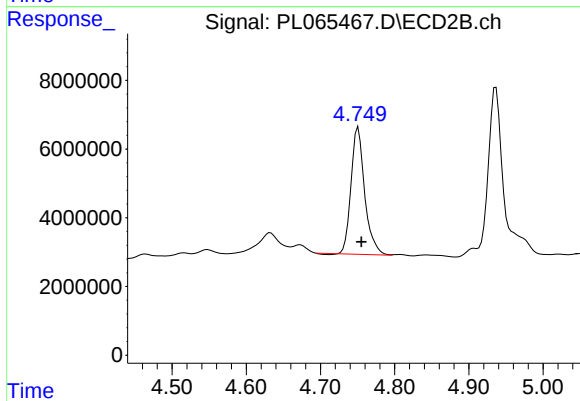

#23 Chlordane-1


R.T.: 4.751 min
Delta R.T.: -0.004 min
Response: 47116079
Conc: 417.73 ng/ml

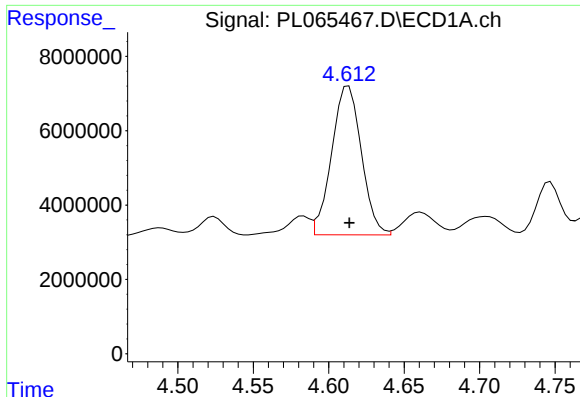

#24 Chlordane-2


R.T.: 4.613 min
Delta R.T.: 0.000 min
Response: 54803285
Conc: 505.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

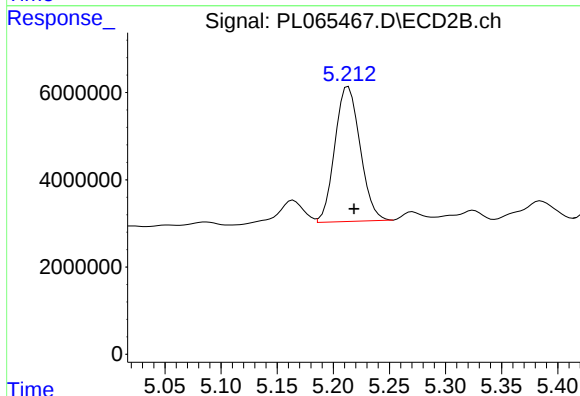


#24 Chlordane-2

R.T.: 5.213 min
Delta R.T.: -0.005 min
Response: 48469359
Conc: 445.03 ng/ml

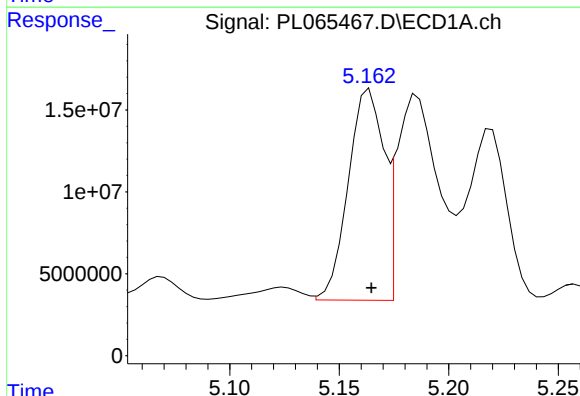


#25 Chlordane-3

R.T.: 5.164 min
Delta R.T.: 0.000 min
Response: 145126647
Conc: 486.40 ng/ml

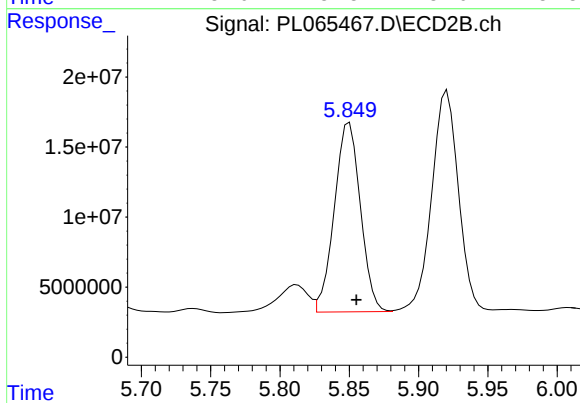

#25 Chlordane-3


R.T.: 5.850 min
Delta R.T.: -0.005 min
Response: 176920507
Conc: 434.03 ng/ml

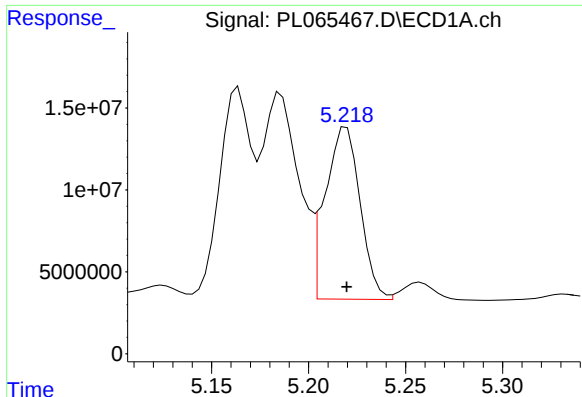

#26 Chlordane-4


R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 131714841
Conc: 483.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

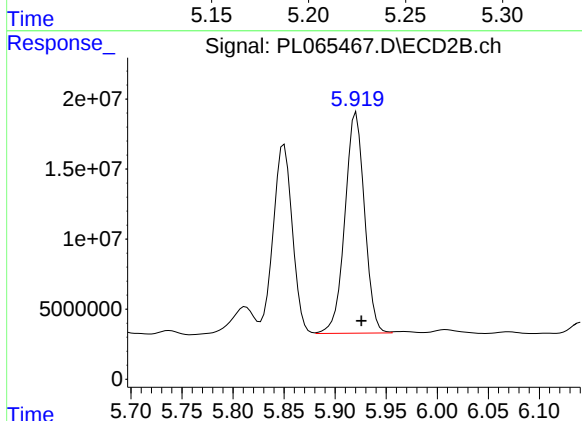


#26 Chlordane-4

R.T.: 5.921 min
Delta R.T.: -0.005 min
Response: 210937221
Conc: 438.47 ng/ml

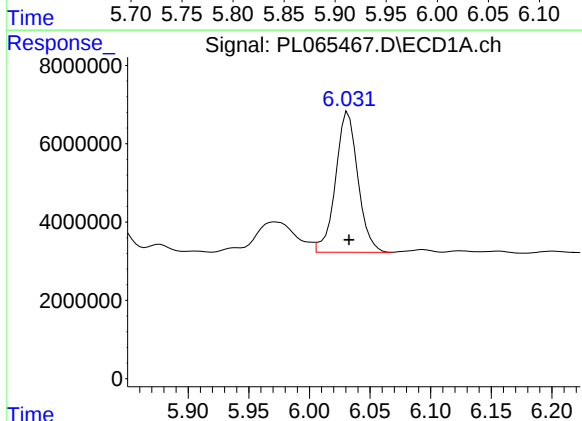


#27 Chlordane-5

R.T.: 6.032 min
Delta R.T.: 0.000 min
Response: 45938275
Conc: 459.49 ng/ml

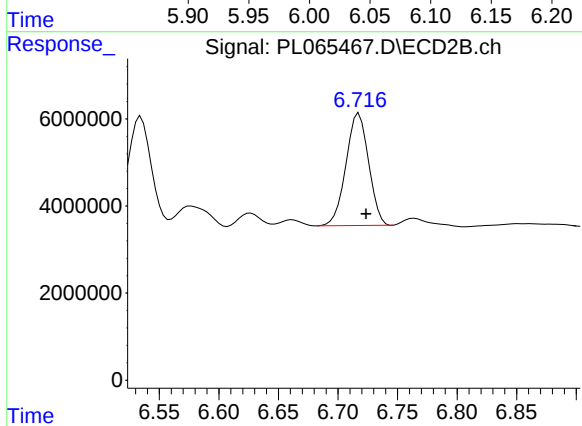

#27 Chlordane-5

R.T.: 6.718 min
Delta R.T.: -0.006 min
Response: 34108546
Conc: 426.26 ng/ml

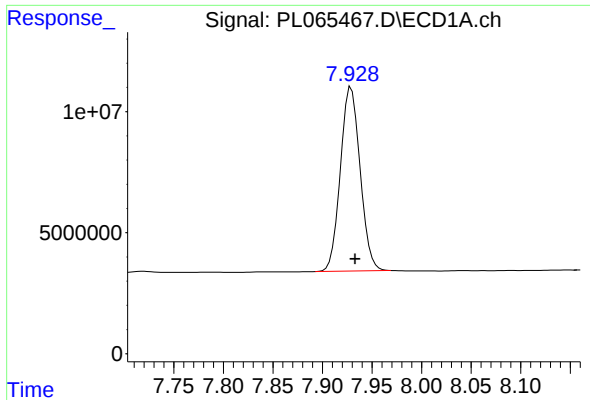

#28 Decachlorobiphenyl


R.T.: 7.929 min

Delta R.T.: -0.004 min

Response: 105329410

Conc: 43.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

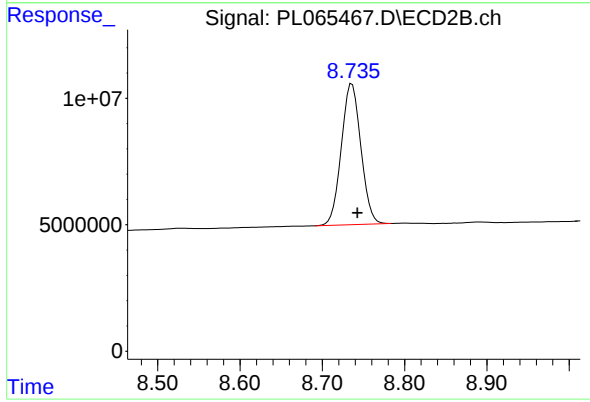

#28 Decachlorobiphenyl

R.T.: 8.736 min

Delta R.T.: -0.007 min

Response: 91961732

Conc: 46.40 ng/ml