

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032221\
 Data File : PL065469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2021 14:30
 Operator : AR\AJ
 Sample : PB135246BS
 Misc : CHLORDANE BS
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB135246BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:02:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.291	3.786	65775700	60593728	27.697	22.076
28)	SA Decachlor...	7.932	8.736	58558693	50293825	24.237	25.374
Target Compounds							
23)	Chlordane-1	4.128	4.750	22126575	23050670	256.839	204.367
24)	Chlordane-2	4.615	5.214	27266092	24028488	251.391	220.621
25)	Chlordane-3	5.166	5.850	69673169	84039097	233.512	206.167
26)	Chlordane-4	5.221	5.920	63827016	101.2E6	234.284	210.284
27)	Chlordane-5	6.033	6.718	21417993	16349024	214.228	204.316



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032221\
Data File : PL065469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2021 14:30
Operator : AR\AJ
Sample : PB135246BS
Misc : CHLORDANE BS
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB135246BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:02:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

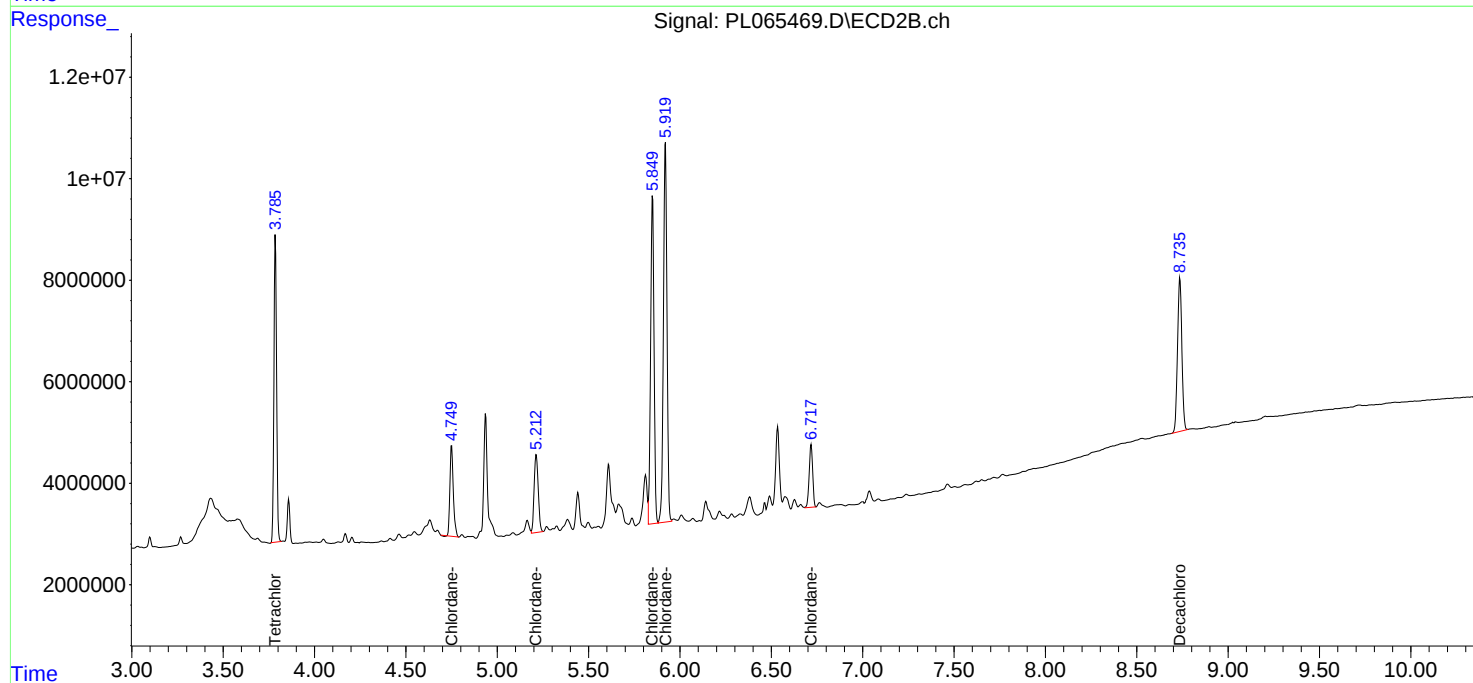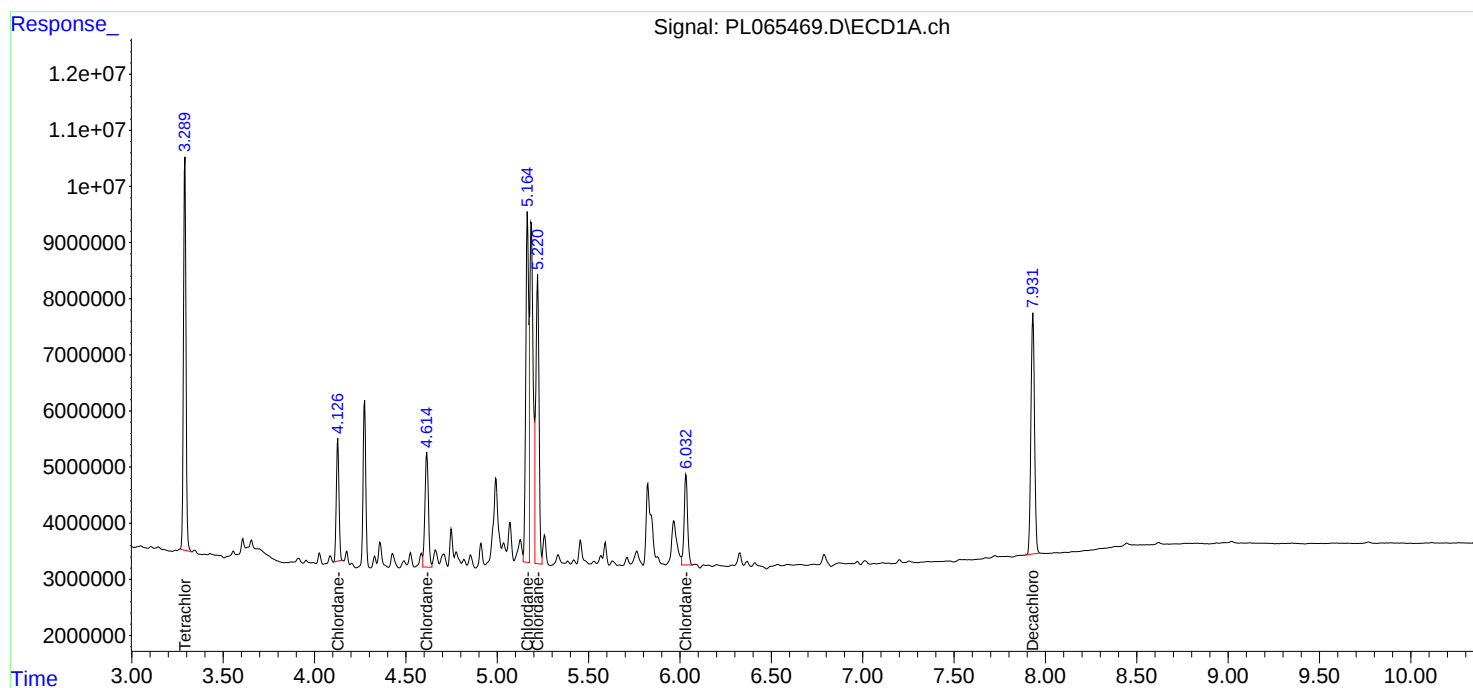


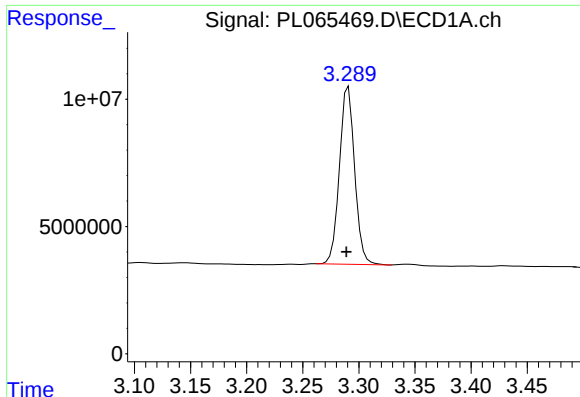

#1 Tetrachloro-m-xylene


R.T.: 3.291 min
Delta R.T.: 0.002 min
Response: 65775700
Conc: 27.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135246BS

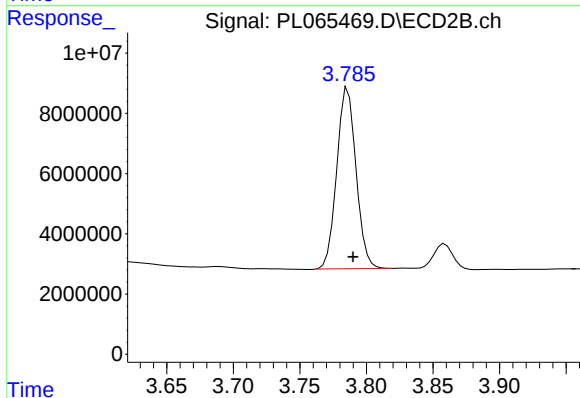


#1 Tetrachloro-m-xylene

R.T.: 3.786 min
Delta R.T.: -0.004 min
Response: 60593728
Conc: 22.08 ng/ml

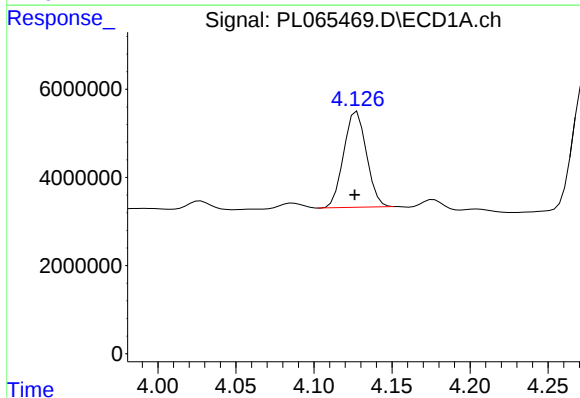


#23 Chlordane-1

R.T.: 4.128 min
Delta R.T.: 0.001 min
Response: 22126575
Conc: 256.84 ng/ml

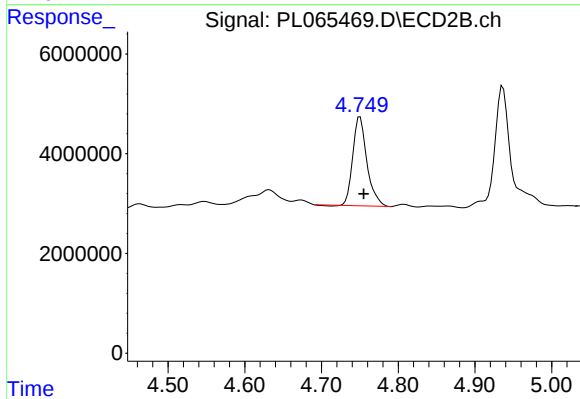

#23 Chlordane-1


R.T.: 4.750 min
Delta R.T.: -0.005 min
Response: 23050670
Conc: 204.37 ng/ml

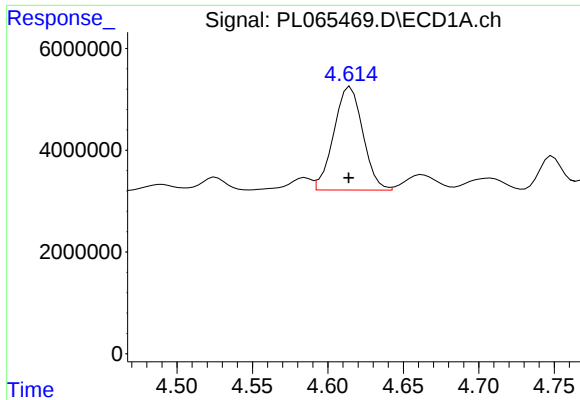

#24 Chlordane-2


R.T.: 4.615 min
Delta R.T.: 0.001 min
Response: 27266092
Conc: 251.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135246BS

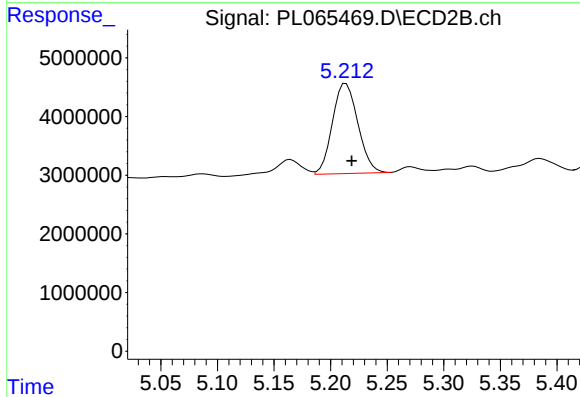


#24 Chlordane-2

R.T.: 5.214 min
Delta R.T.: -0.005 min
Response: 24028488
Conc: 220.62 ng/ml

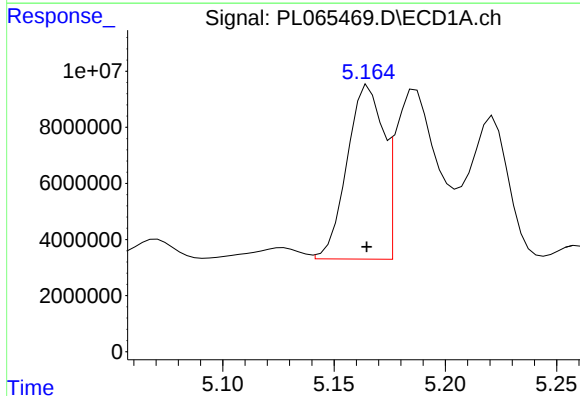


#25 Chlordane-3

R.T.: 5.166 min
Delta R.T.: 0.000 min
Response: 69673169
Conc: 233.51 ng/ml

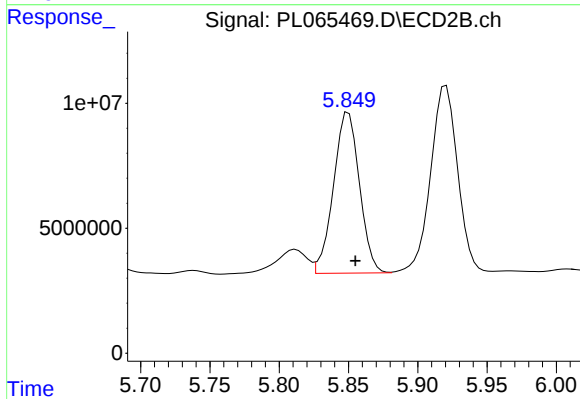

#25 Chlordane-3


R.T.: 5.850 min
Delta R.T.: -0.005 min
Response: 84039097
Conc: 206.17 ng/ml

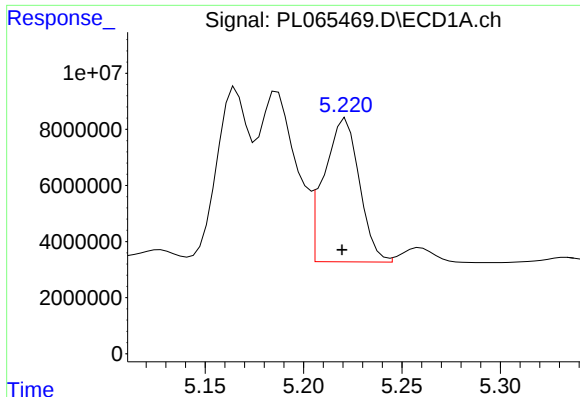

#26 Chlordane-4


R.T.: 5.221 min
Delta R.T.: 0.002 min
Response: 63827016
Conc: 234.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135246BS

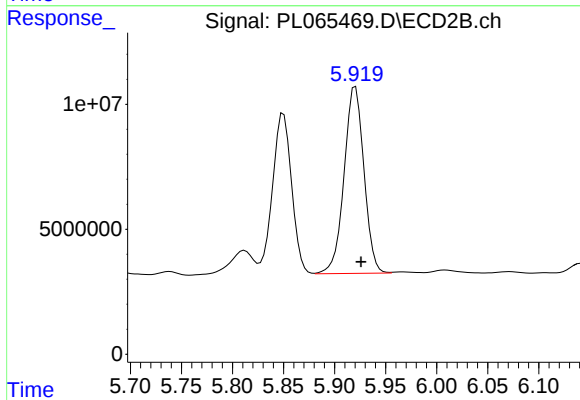


#26 Chlordane-4

R.T.: 5.920 min
Delta R.T.: -0.005 min
Response: 101161899
Conc: 210.28 ng/ml

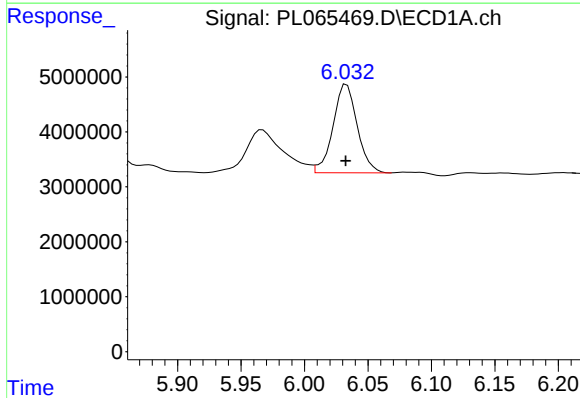


#27 Chlordane-5

R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 21417993
Conc: 214.23 ng/ml

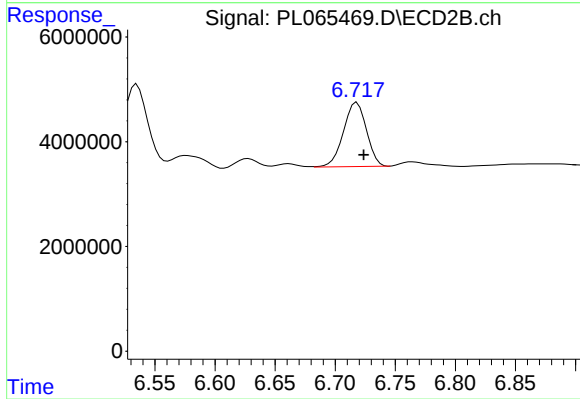

#27 Chlordane-5


R.T.: 6.718 min
Delta R.T.: -0.005 min
Response: 16349024
Conc: 204.32 ng/ml

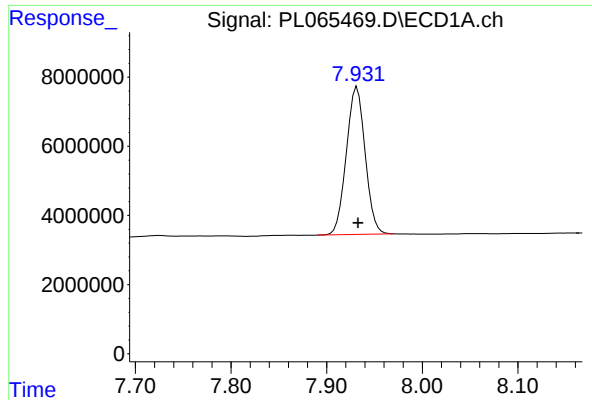

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: -0.001 min
Response: 58558693
Conc: 24.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135246BS

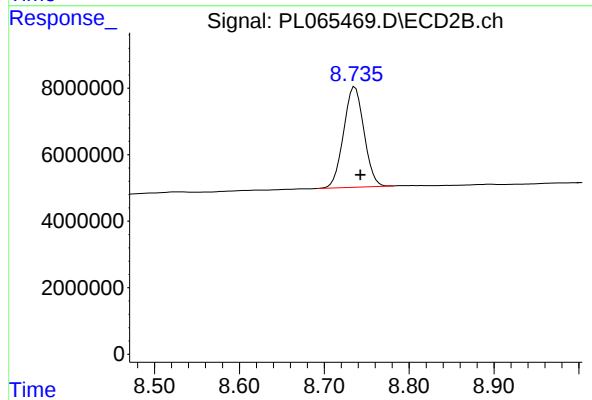

#28 Decachlorobiphenyl

R.T.: 8.736 min
Delta R.T.: -0.007 min
Response: 50293825
Conc: 25.37 ng/ml