

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032222\
 Data File : PL073557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 08:39
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:38:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

3) MA	gamma-BHC...	0.000	6.459f	0	68669	N.D.	0.032 #
5) MB	Aldrin	0.000	7.491f	0	79430	N.D.	0.038 #
8) B	Heptachlo...	0.000	7.925	0	1827905	N.D.	0.915 #
10) B	gamma-Chl...	0.000	8.185	0	1440980	N.D.	0.706 #
12) B	4,4'-DDE	0.000	8.469	0	53234	N.D.	0.030 #
13) MA	Dieldrin	7.792	0.000	146020	0	0.350	N.D. #
14) MA	Endrin	8.047f	8.861f	79711	52155	0.205	0.034 #
15) B	Endosulfa...	0.000	9.097f	0	2269079	N.D.	1.477 #
16) A	4,4'-DDD	0.000	8.999	0	2383402	N.D.	1.633 #
19) B	Endosulfa...	0.000	9.466f	0	332468	N.D.	0.211 #
21) B	Endrin ke...	0.000	9.927	0	127080	N.D.	0.077 #
25)	Chlordane-3	0.000	8.204	0	986781	N.D.	3.639 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032222\
Data File : PL073557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 08:39
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:38:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

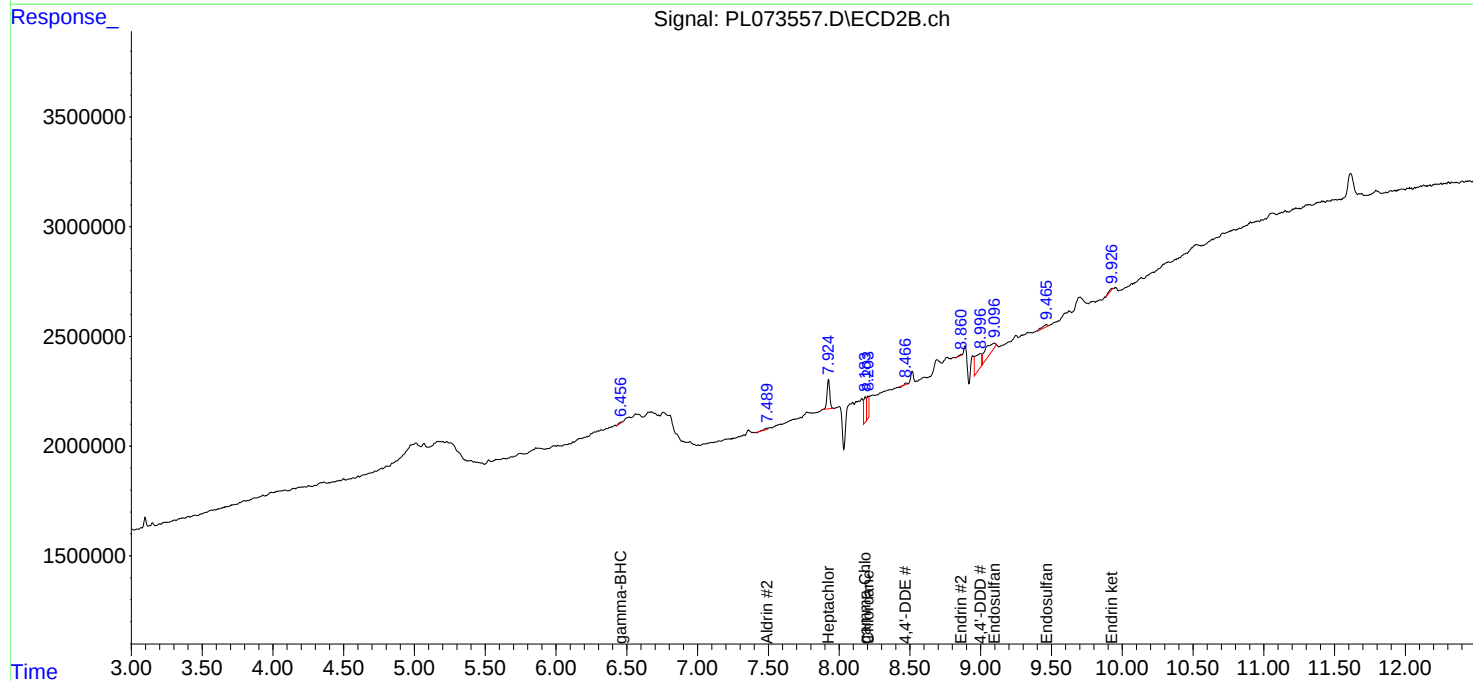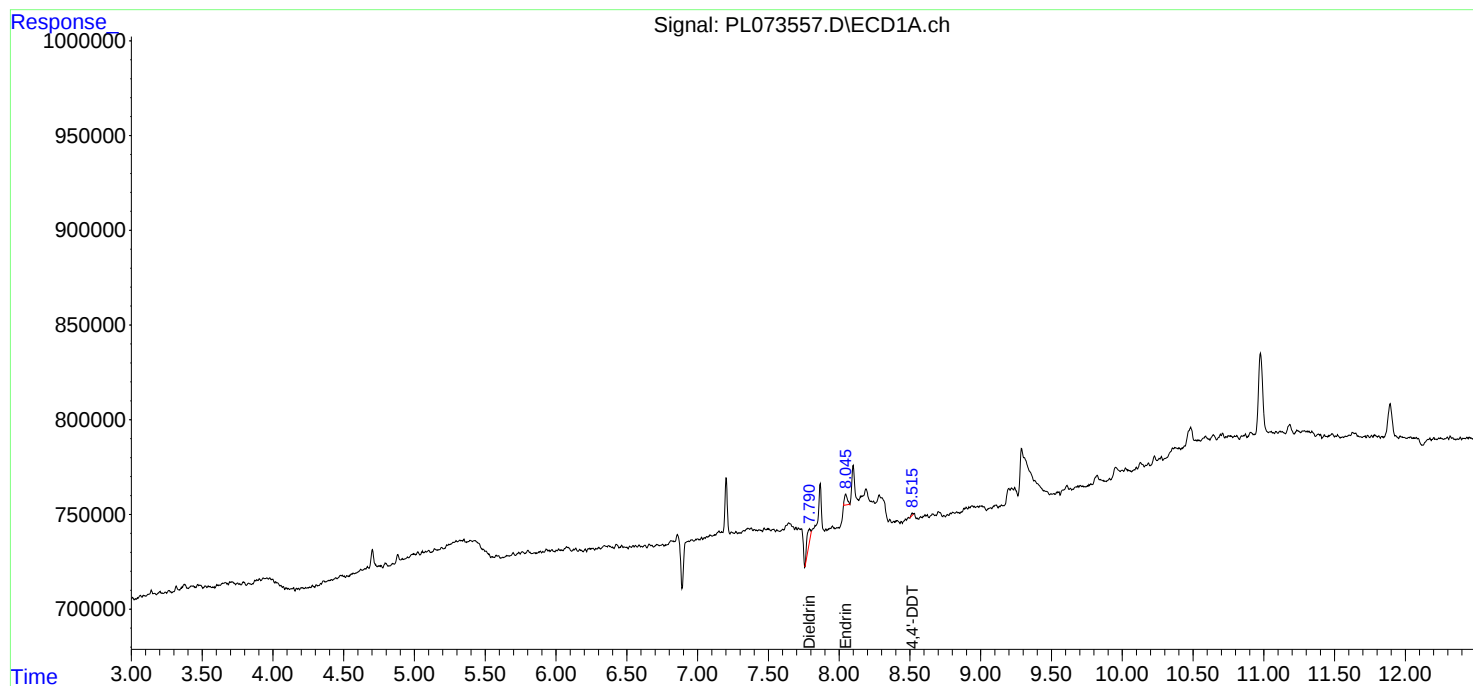


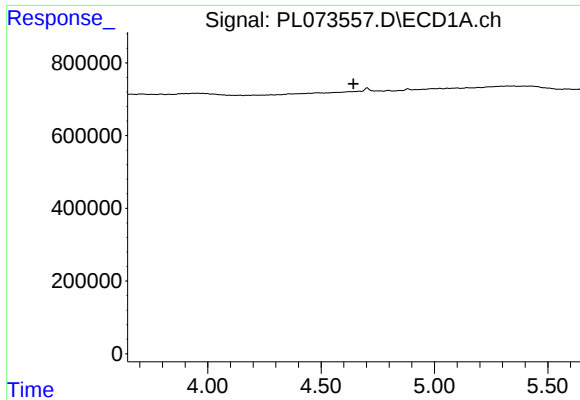

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

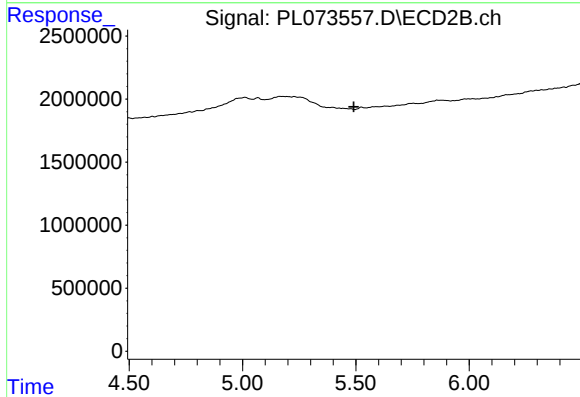


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.491 min
Response: 0
Conc: N.D.

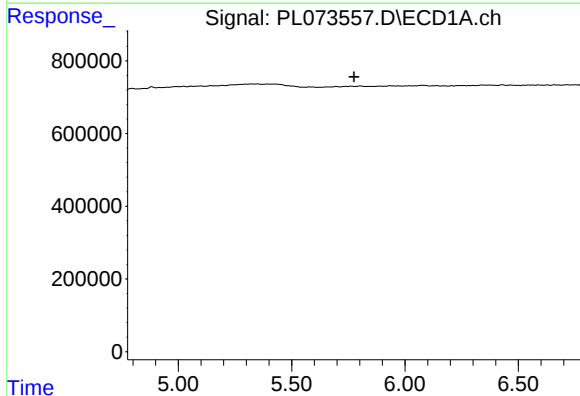


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 5.775 min
Response: 0
Conc: N.D.

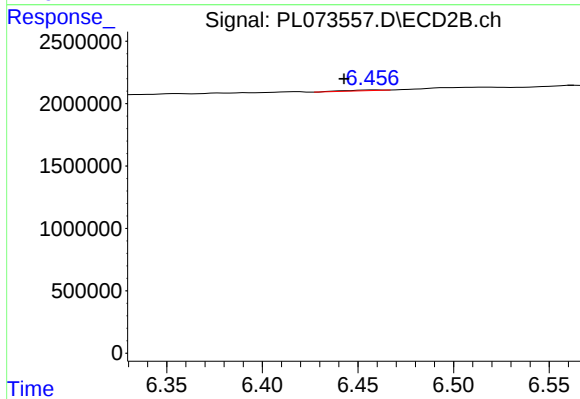

#3 gamma-BHC (Lindane)


R.T.: 6.459 min
Delta R.T.: 0.016 min
Response: 68669
Conc: 0.03 ng/ml

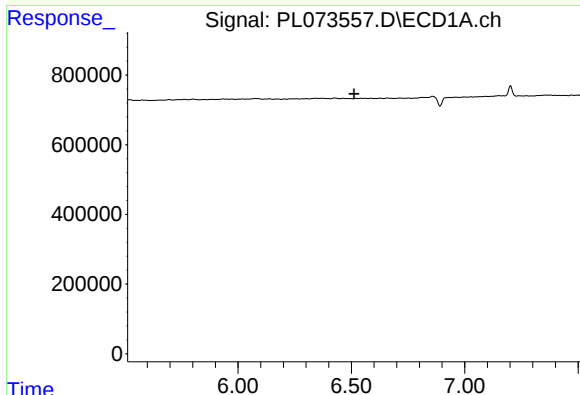

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.513 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

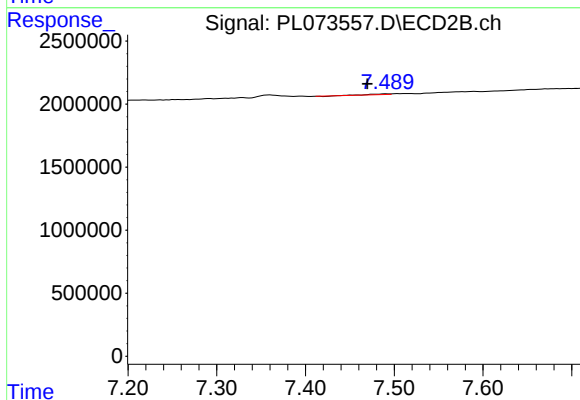


#5 Aldrin

R.T.: 7.491 min
Delta R.T.: 0.021 min
Response: 79430
Conc: 0.04 ng/ml

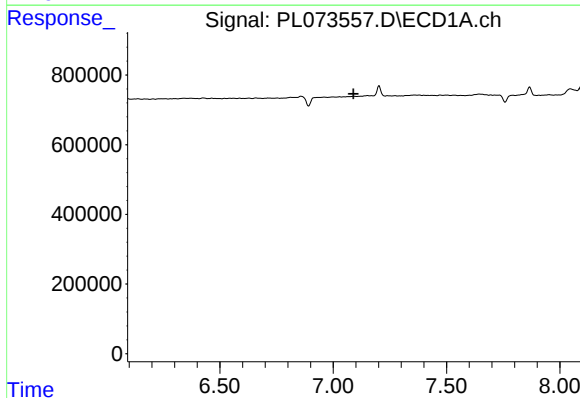


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

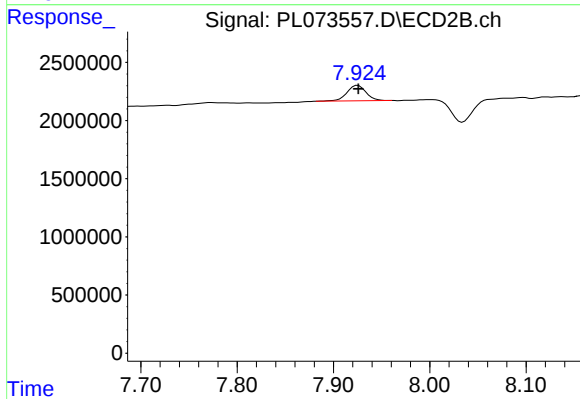

#8 Heptachlor epoxide


R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 1827905
Conc: 0.92 ng/ml

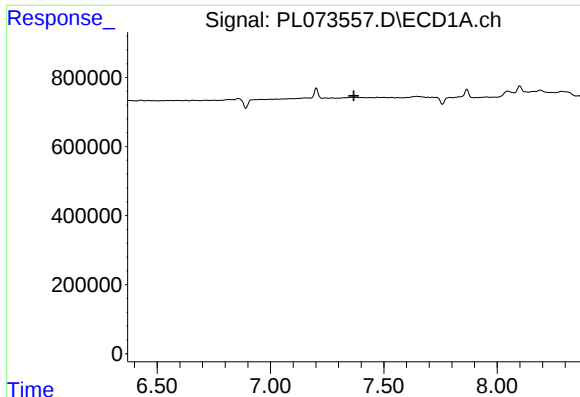

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

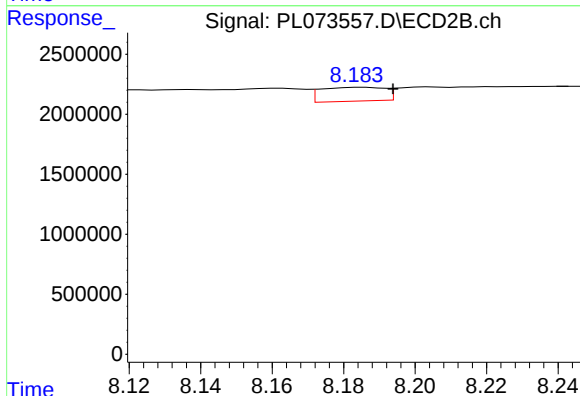


#10 gamma-Chlordane

R.T.: 8.185 min
Delta R.T.: -0.008 min
Response: 1440980
Conc: 0.71 ng/ml

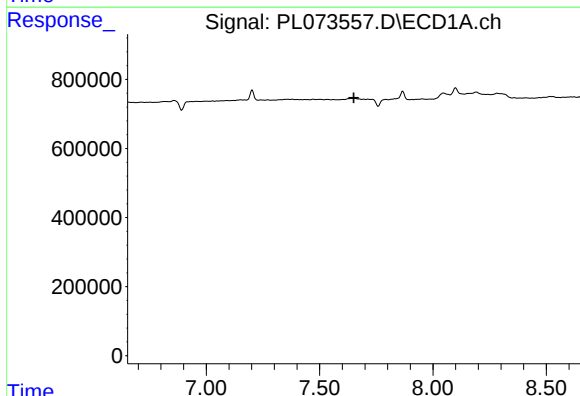


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.651 min
Response: 0
Conc: N.D.

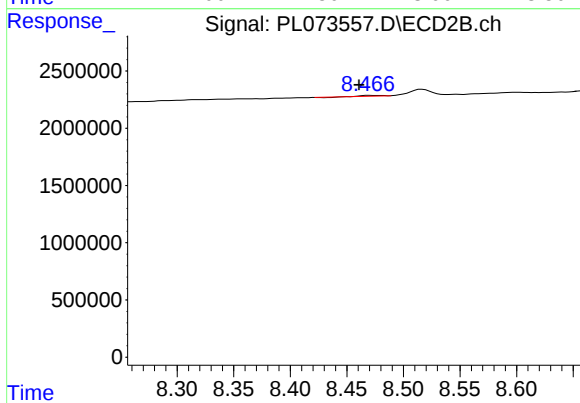

#12 4,4'-DDE


R.T.: 8.469 min
Delta R.T.: 0.009 min
Response: 53234
Conc: 0.03 ng/ml

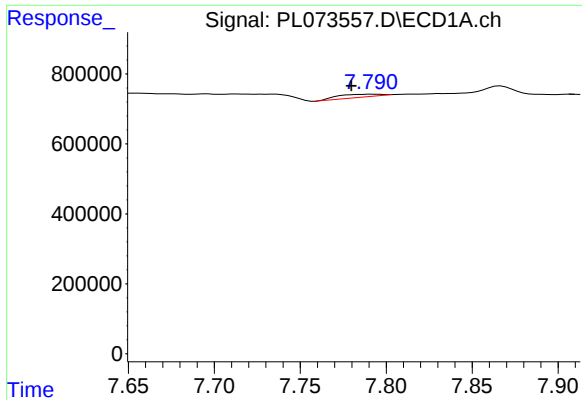

#13 Dieldrin


R.T.: 7.792 min
Delta R.T.: 0.012 min
Response: 146020
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

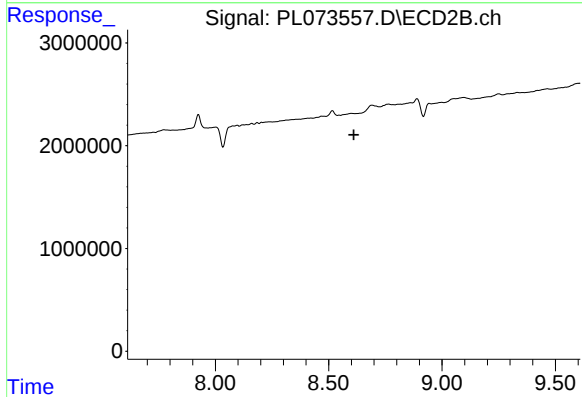


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.611 min
Response: 0
Conc: N.D.

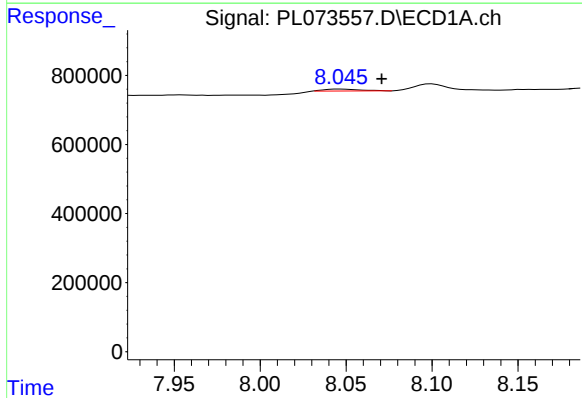


#14 Endrin

R.T.: 8.047 min
Delta R.T.: -0.024 min
Response: 79711
Conc: 0.21 ng/ml

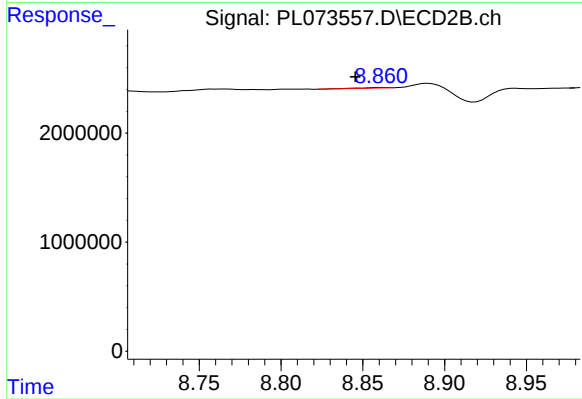

#14 Endrin


R.T.: 8.861 min
Delta R.T.: 0.016 min
Response: 52155
Conc: 0.03 ng/ml

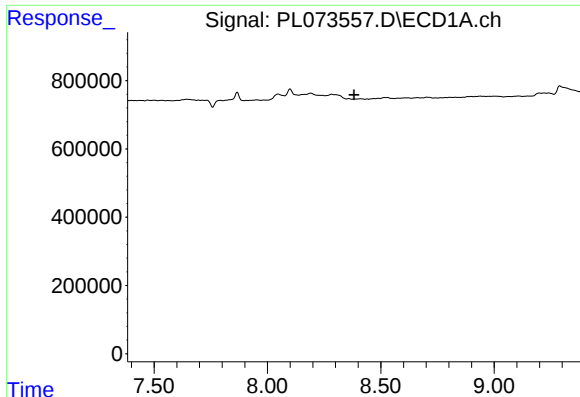

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

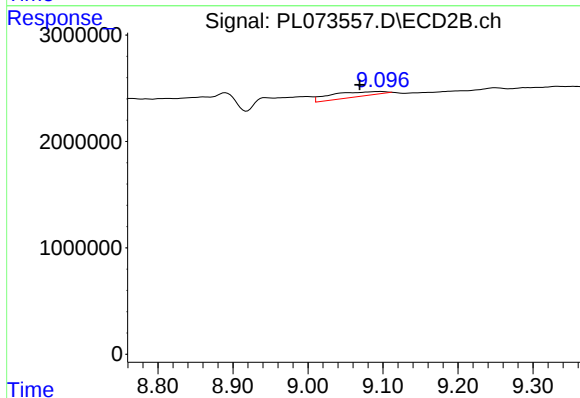


#15 Endosulfan II

R.T.: 9.097 min
Delta R.T.: 0.028 min
Response: 2269079
Conc: 1.48 ng/ml

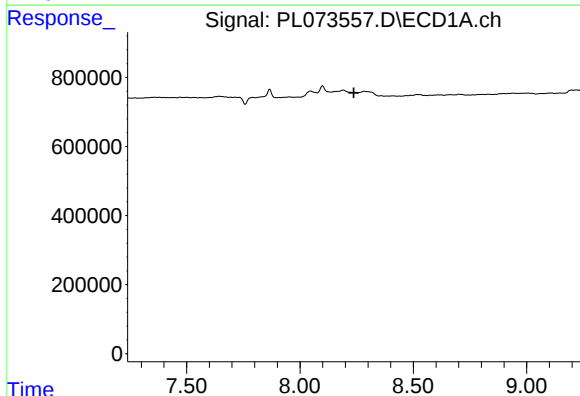


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.237 min
Response: 0
Conc: N.D.

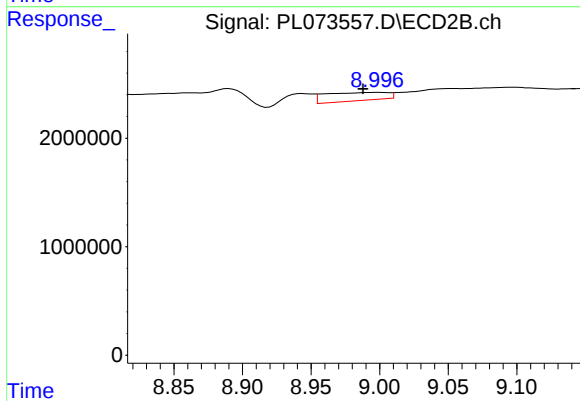

#16 4,4'-DDD


R.T.: 8.999 min
Delta R.T.: 0.011 min
Response: 2383402
Conc: 1.63 ng/ml

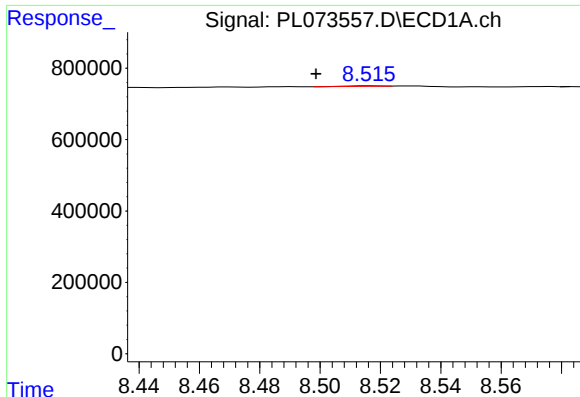

#17 4,4'-DDT


R.T.: 8.517 min
Delta R.T.: 0.018 min
Response: 8842
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

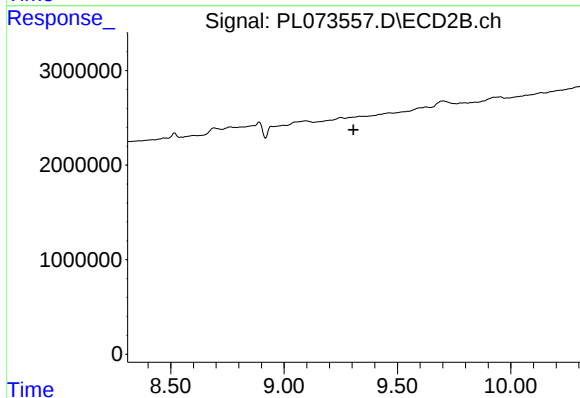


#17 4,4'-DDT

R.T.: 9.333 min
Delta R.T.: 0.026 min
Response: -184254
Conc: N.D.

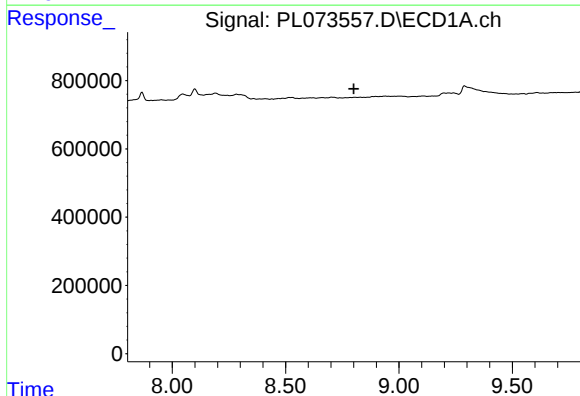


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.801 min
Response: 0
Conc: N.D.

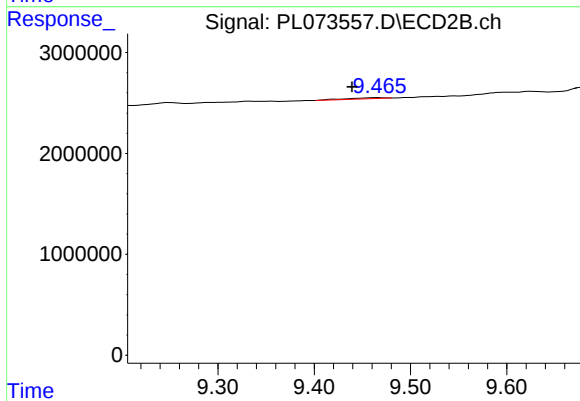

#19 Endosulfan Sulfate


R.T.: 9.466 min
Delta R.T.: 0.027 min
Response: 332468
Conc: 0.21 ng/ml

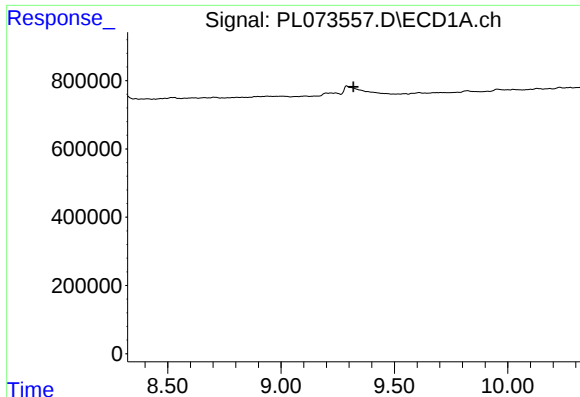

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

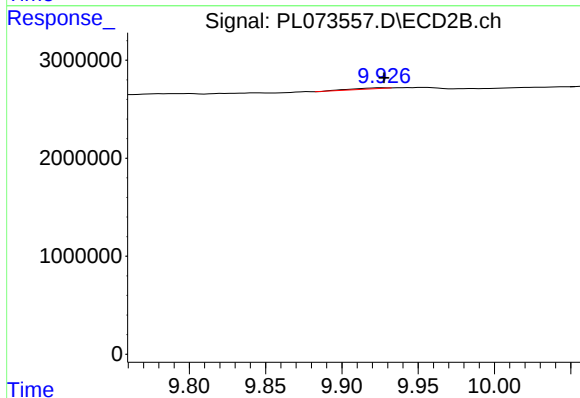


#21 Endrin ketone

R.T.: 9.927 min
Delta R.T.: 0.000 min
Response: 127080
Conc: 0.08 ng/ml

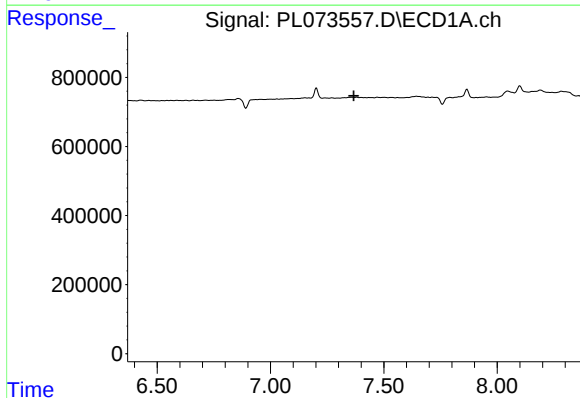


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

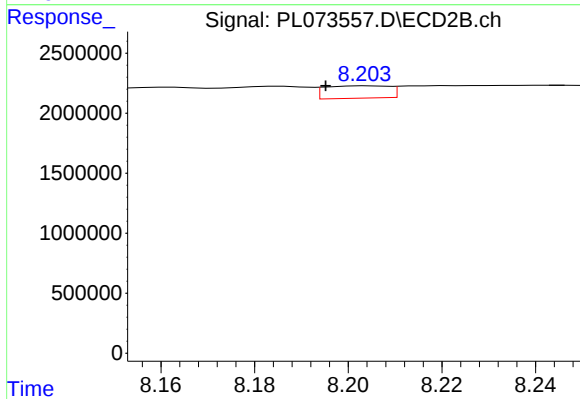

#25 Chlordane-3


R.T.: 8.204 min
Delta R.T.: 0.009 min
Response: 986781
Conc: 3.64 ng/ml

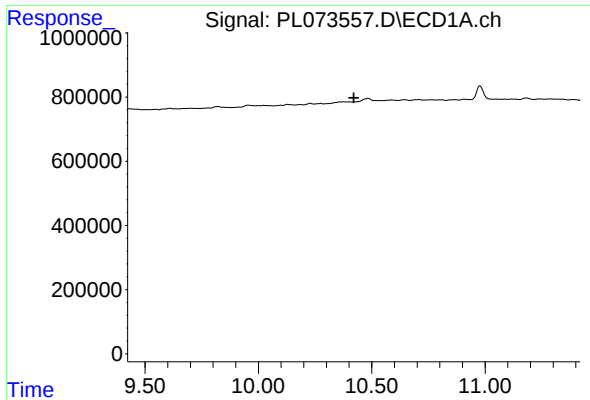

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.421 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

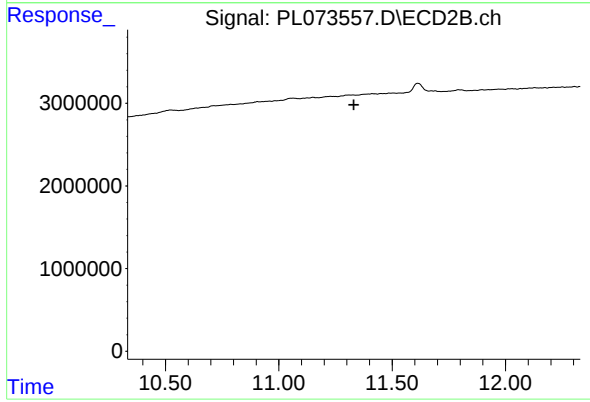

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 11.331 min
Response: 0
Conc: N.D.