

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032222\
 Data File : PL073564.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 12:48
 Operator : AR\AJ
 Sample : PB143350BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:41:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.652	5.488	5878082	32524446	18.353	19.817
28)	SA Decachlor...	10.421	11.333	10389130	35984464	20.431	20.124
Target Compounds							
3)	MA gamma-BHC...	5.786	0.000	9684	0	0.023	N.D. #
6)	B beta-BHC	6.136f	6.704f	55130	545095	0.268	0.523 #
7)	B delta-BHC	0.000	6.958	0	664142	N.D.	0.308 #
8)	B Heptachlo...	0.000	7.927	0	206763	N.D.	0.104 #
10)	B gamma-Chl...	0.000	8.189	0	1141816	N.D.	0.559 #
11)	B alpha-Chl...	0.000	8.276	0	96201	N.D.	0.048 #
14)	MA Endrin	8.100f	0.000	107856	0	0.278	N.D. #
19)	B Endosulfa...	0.000	9.437	0	45606	N.D.	0.029 #
25)	Chlordane-3	0.000	8.189	0	1141816	N.D.	4.211 #
26)	Chlordane-4	0.000	8.276	0	96201	N.D.	0.290 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032222\
Data File : PL073564.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 12:48
Operator : AR\AJ
Sample : PB143350BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:41:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

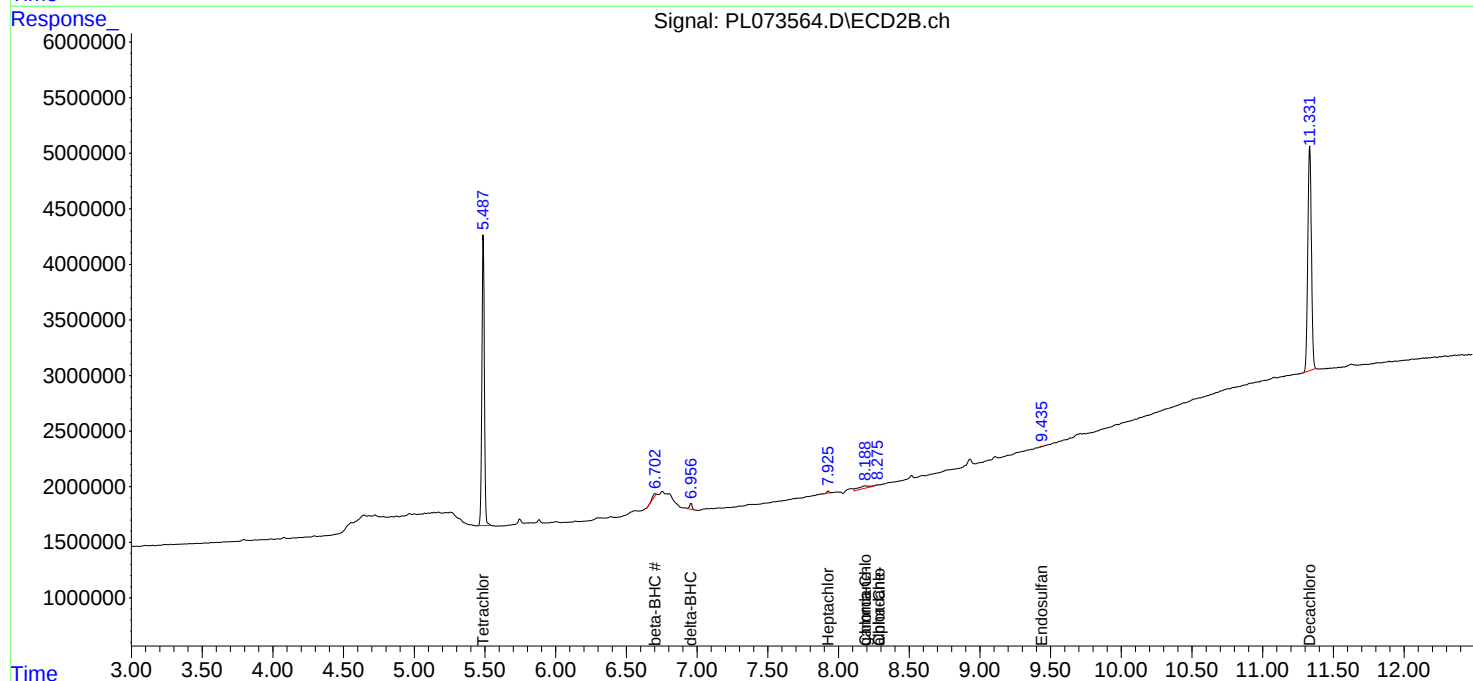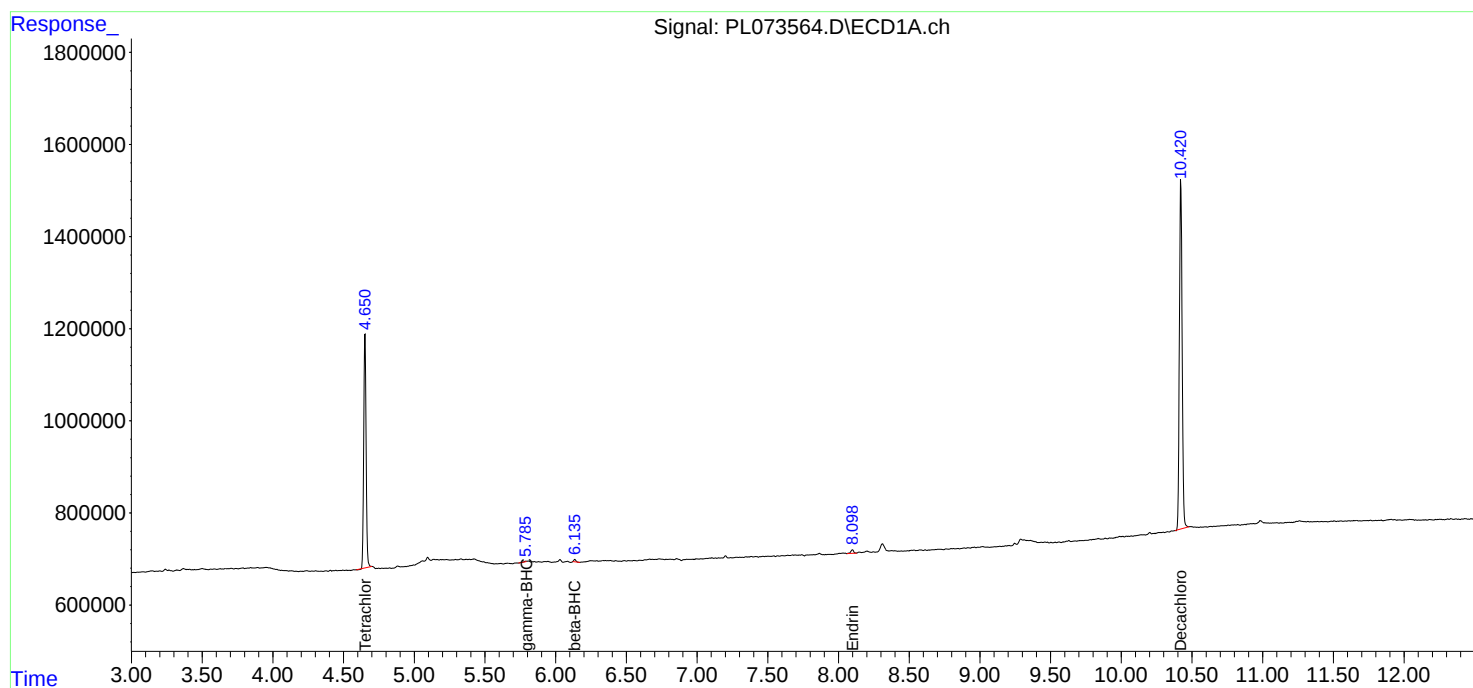


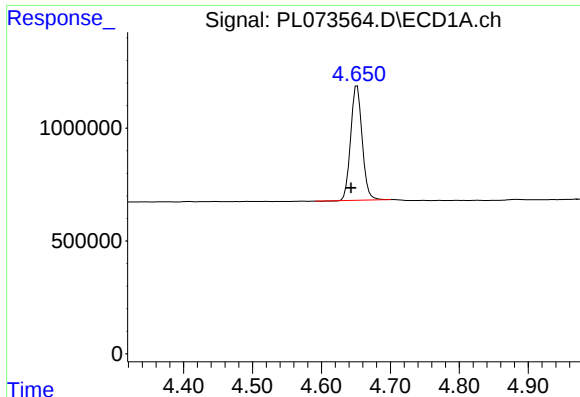

#1 Tetrachloro-m-xylene


R.T.: 4.652 min
Delta R.T.: 0.009 min
Response: 5878082
Conc: 18.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

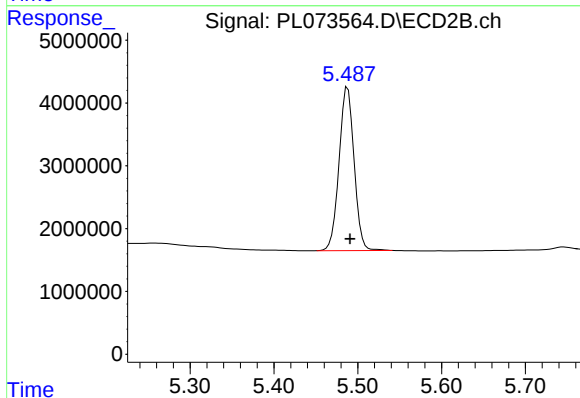


#1 Tetrachloro-m-xylene

R.T.: 5.488 min
Delta R.T.: -0.003 min
Response: 32524446
Conc: 19.82 ng/ml

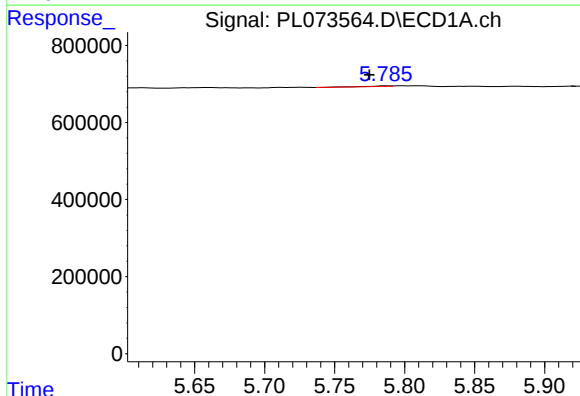


#3 gamma-BHC (Lindane)

R.T.: 5.786 min
Delta R.T.: 0.011 min
Response: 9684
Conc: 0.02 ng/ml

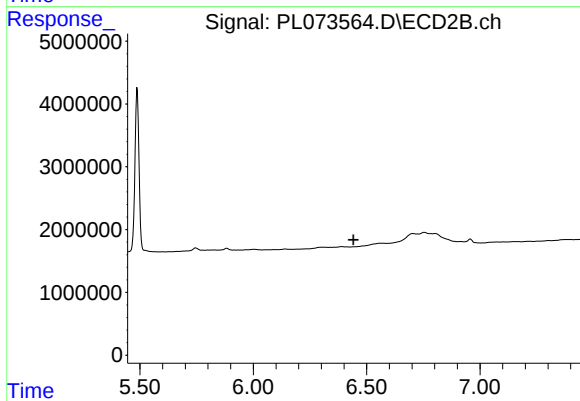

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.443 min
Response: 0
Conc: N.D.

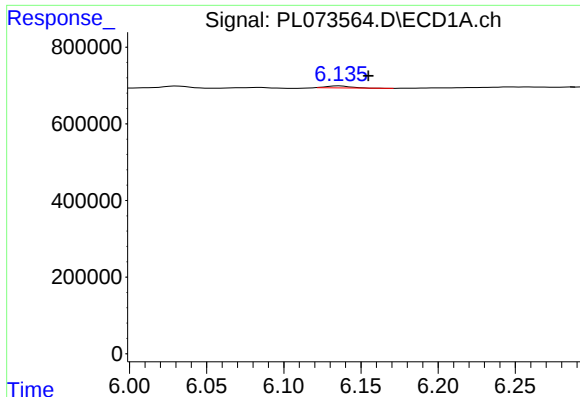

#6 beta-BHC


R.T.: 6.136 min
Delta R.T.: -0.019 min
Response: 55130
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

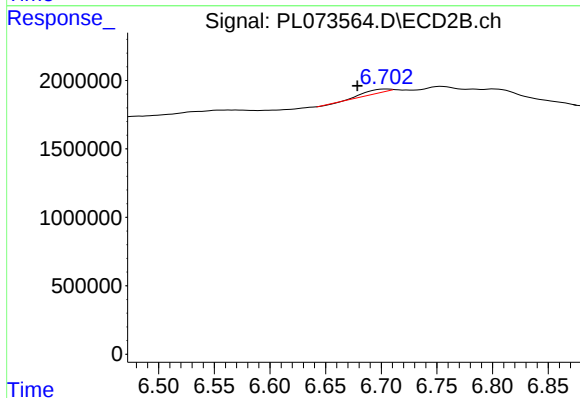


#6 beta-BHC

R.T.: 6.704 min
Delta R.T.: 0.025 min
Response: 545095
Conc: 0.52 ng/ml

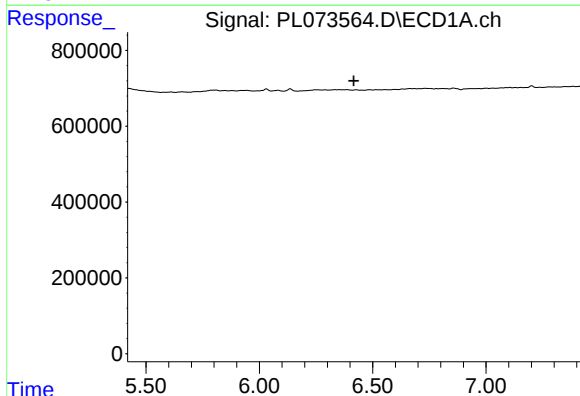


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

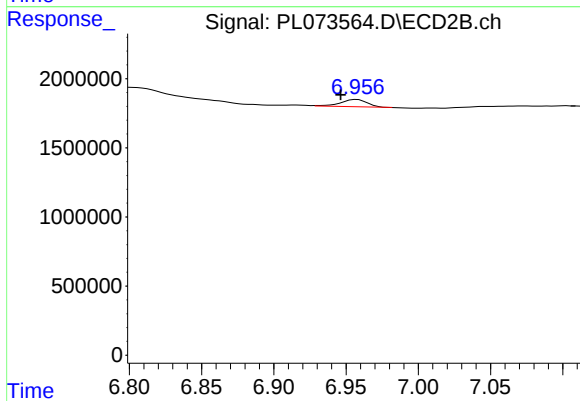

#7 delta-BHC


R.T.: 6.958 min
Delta R.T.: 0.011 min
Response: 664142
Conc: 0.31 ng/ml

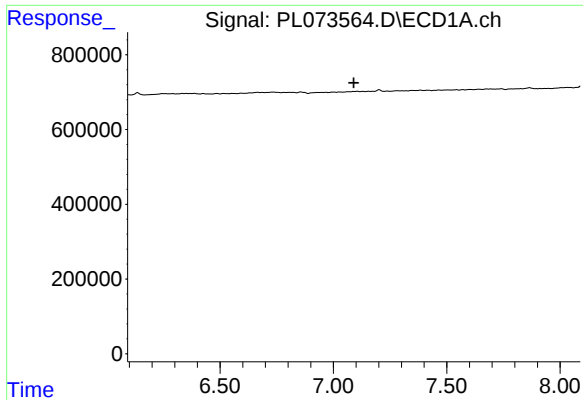

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

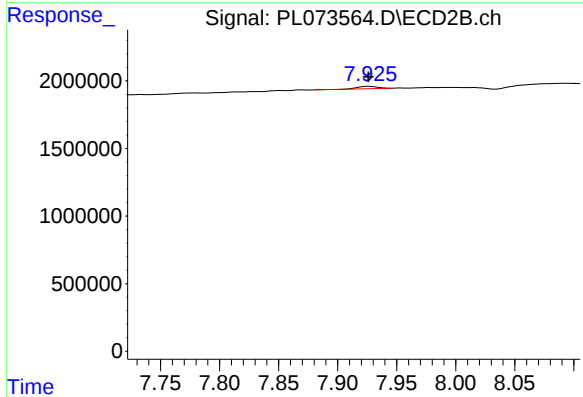


#8 Heptachlor epoxide

R.T.: 7.927 min
Delta R.T.: 0.000 min
Response: 206763
Conc: 0.10 ng/ml

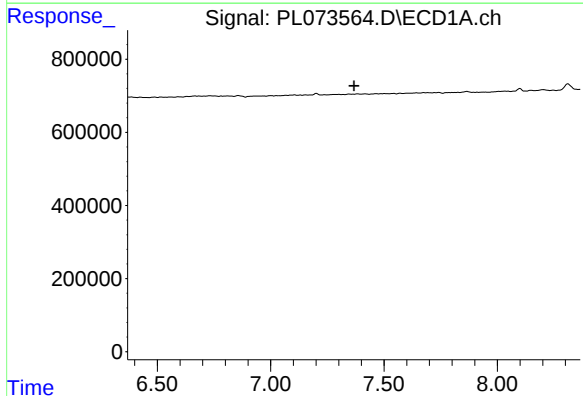


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

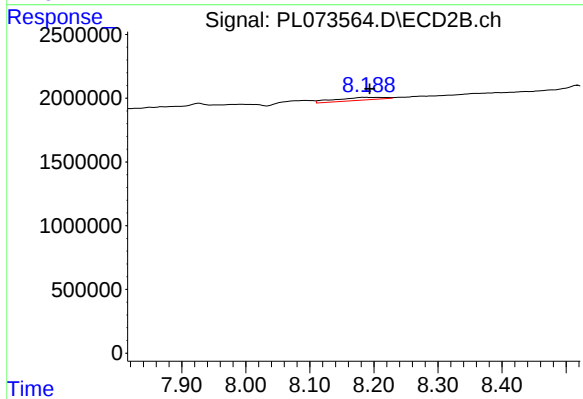

#10 gamma-Chlordane


R.T.: 8.189 min
Delta R.T.: -0.005 min
Response: 1141816
Conc: 0.56 ng/ml

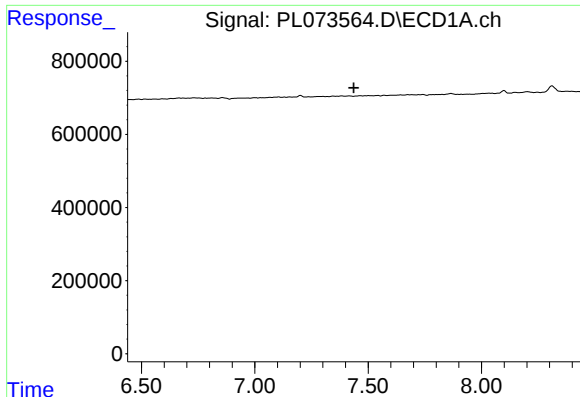

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

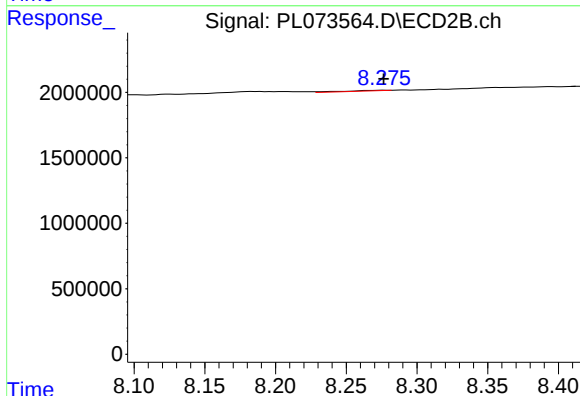


#11 alpha-Chlordane

R.T.: 8.276 min
Delta R.T.: 0.000 min
Response: 96201
Conc: 0.05 ng/ml

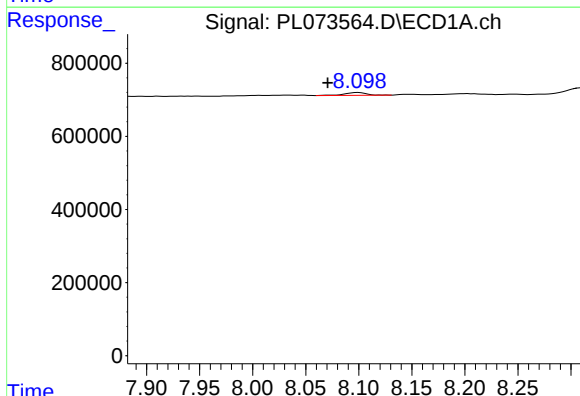


#14 Endrin

R.T.: 8.100 min
Delta R.T.: 0.029 min
Response: 107856
Conc: 0.28 ng/ml

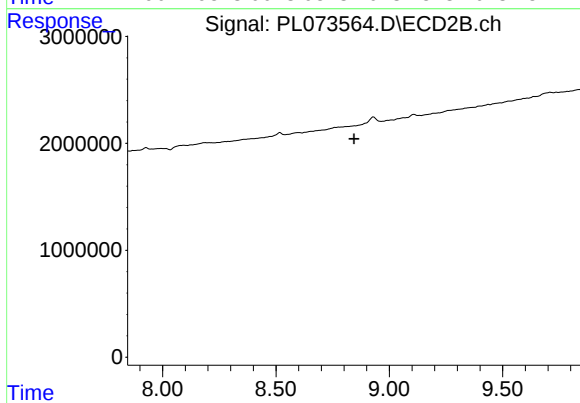

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.845 min
Response: 0
Conc: N.D.

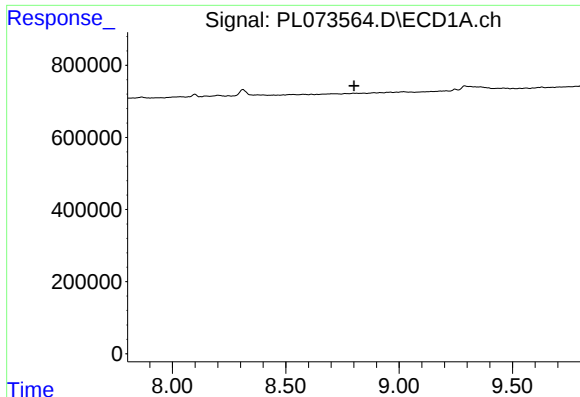

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

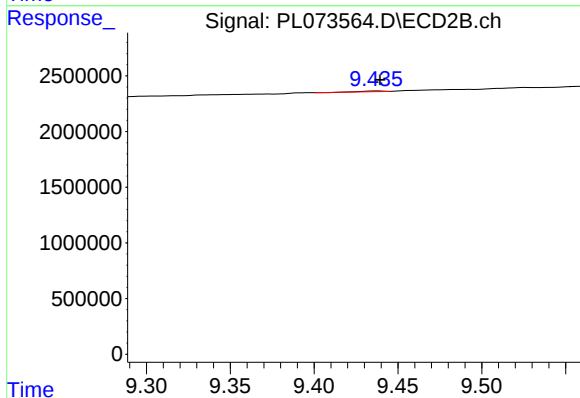


#19 Endosulfan Sulfate

R.T.: 9.437 min
Delta R.T.: -0.002 min
Response: 45606
Conc: 0.03 ng/ml

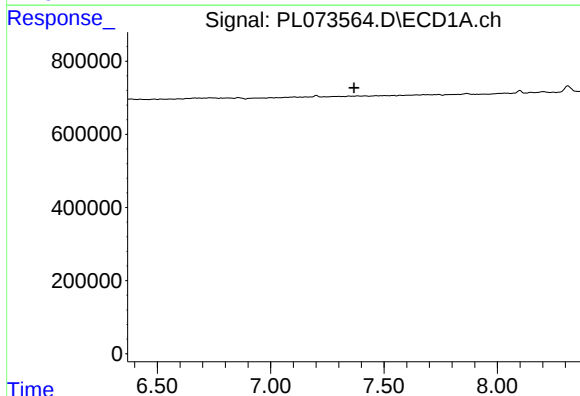


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

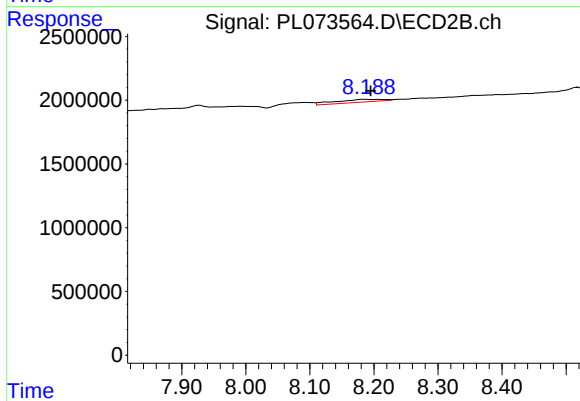

#25 Chlordane-3


R.T.: 8.189 min
Delta R.T.: -0.006 min
Response: 1141816
Conc: 4.21 ng/ml

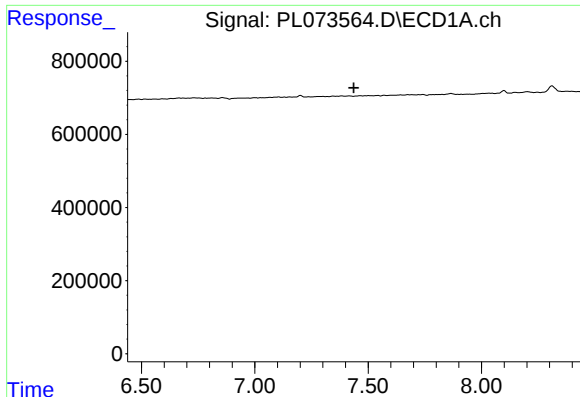

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

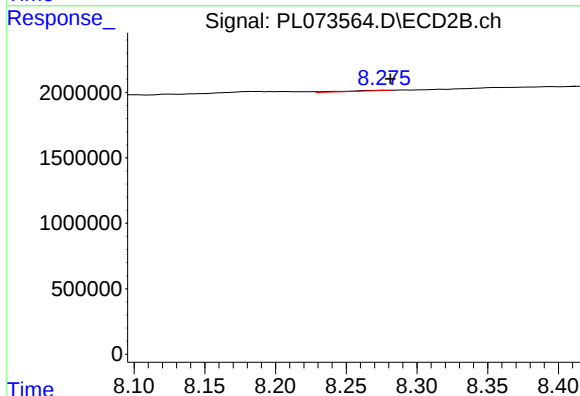


#26 Chlordane-4

R.T.: 8.276 min
Delta R.T.: -0.005 min
Response: 96201
Conc: 0.29 ng/ml

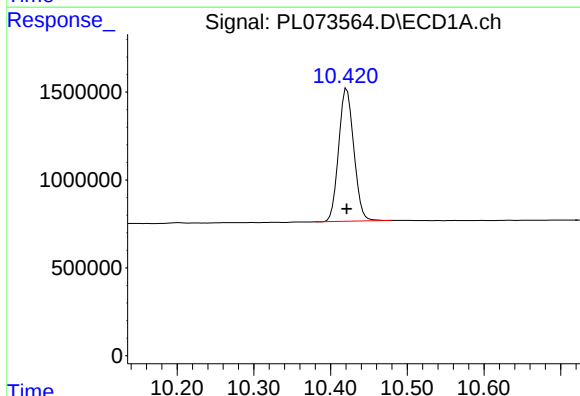

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: 0.000 min
Response: 10389130
Conc: 20.43 ng/ml

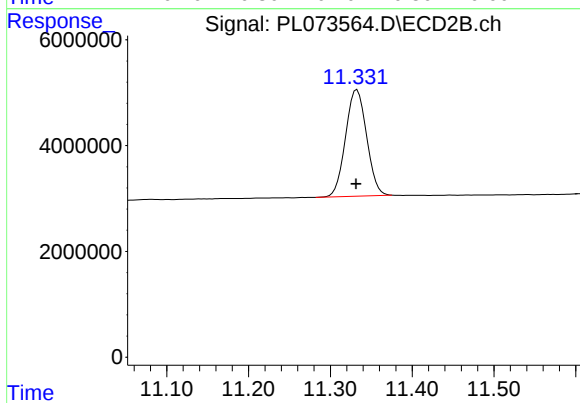

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: 0.001 min
Response: 35984464
Conc: 20.12 ng/ml