

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032222\
 Data File : PL073580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 17:16
 Operator : AR\AJ
 Sample : PB143516BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:49:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.491	5660902	30136825	17.675	18.362
28)	SA Decachlor...	10.415	11.332	9757994	34306657	19.190	19.185
Target Compounds							
6)	B beta-BHC	0.000	6.675	0	761485	N.D.	0.731 #
7)	B delta-BHC	0.000	6.955	0	1311551	N.D.	0.609 #
10)	B gamma-Chl...	0.000	8.196	0	455209	N.D.	0.223 #
11)	B alpha-Chl...	0.000	8.267	0	60176	N.D.	0.030 #
14)	MA Endrin	8.092f	0.000	30000	0	0.077	N.D. #
19)	B Endosulfa...	0.000	9.437	0	15957	N.D.	0.010 #
23)	Chlordane-1	0.000	6.852	0	945697	N.D.	13.844 #
25)	Chlordane-3	0.000	8.196	0	455209	N.D.	1.679 #
26)	Chlordane-4	0.000	8.267	0	60176	N.D.	0.182 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032222\
Data File : PL073580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 17:16
Operator : AR\AJ
Sample : PB143516BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:49:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

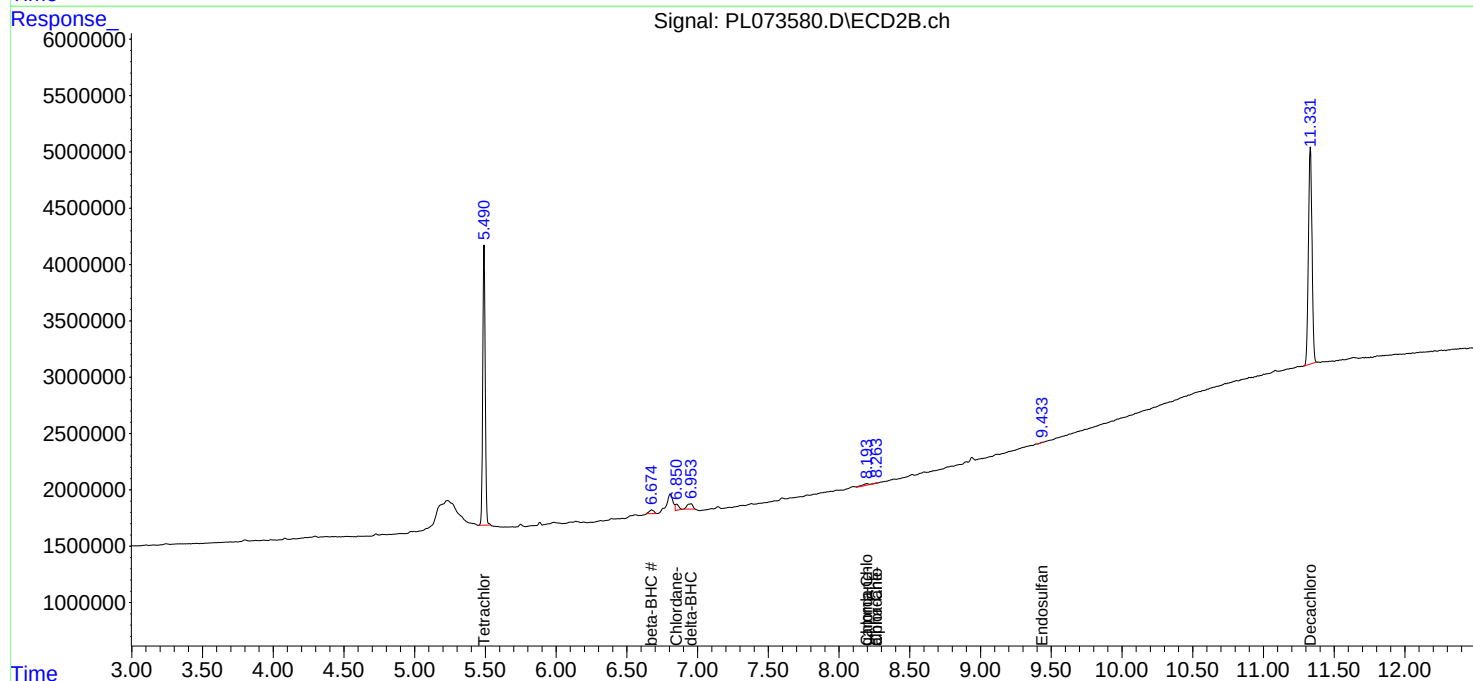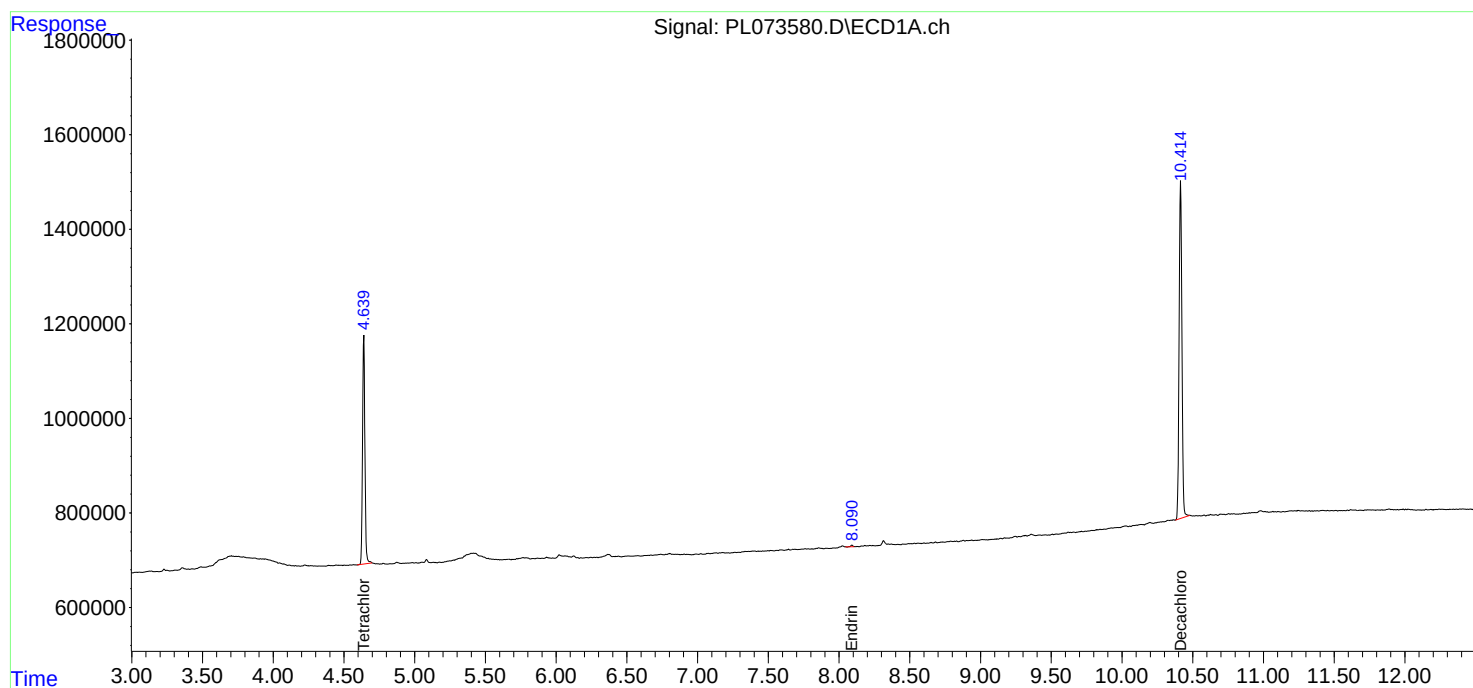


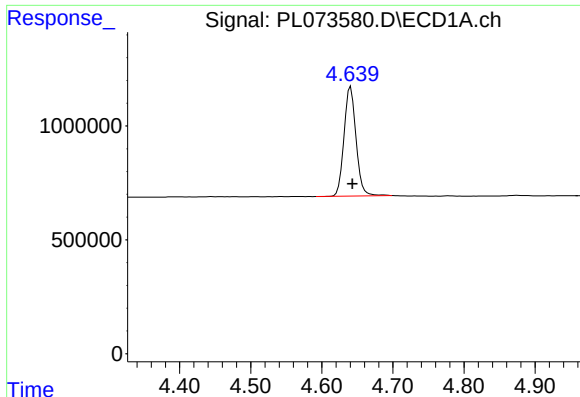

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.002 min
Response: 5660902
Conc: 17.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

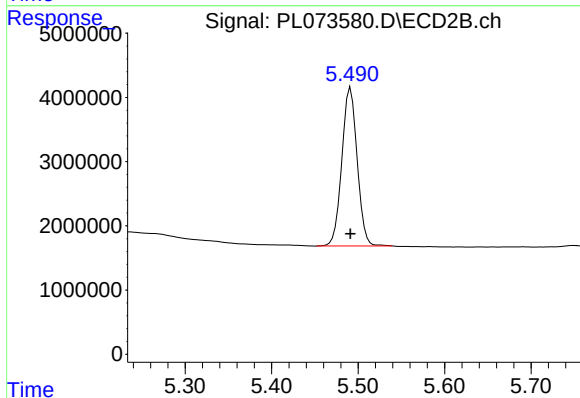


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 30136825
Conc: 18.36 ng/ml

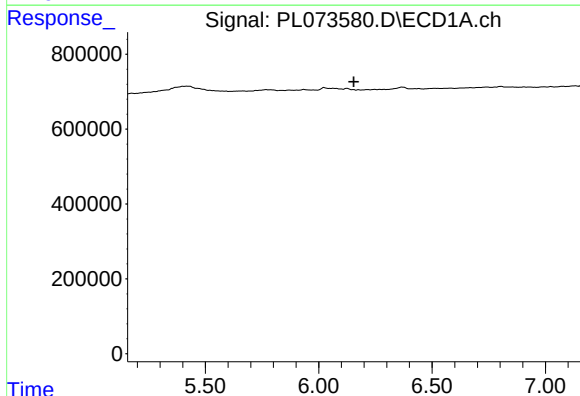


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

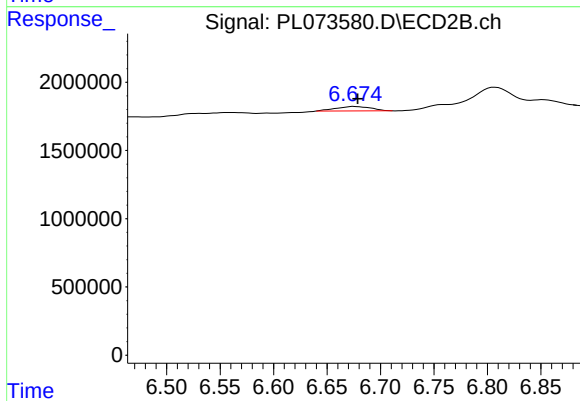

#6 beta-BHC


R.T.: 6.675 min
Delta R.T.: -0.003 min
Response: 761485
Conc: 0.73 ng/ml

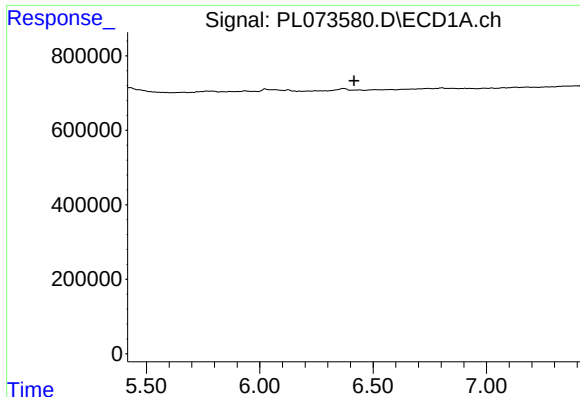

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

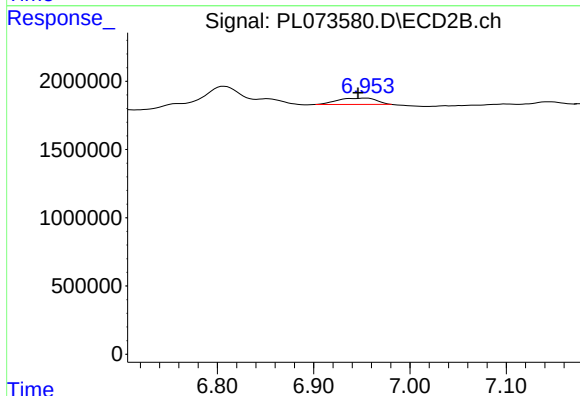


#7 delta-BHC

R.T.: 6.955 min
Delta R.T.: 0.009 min
Response: 1311551
Conc: 0.61 ng/ml

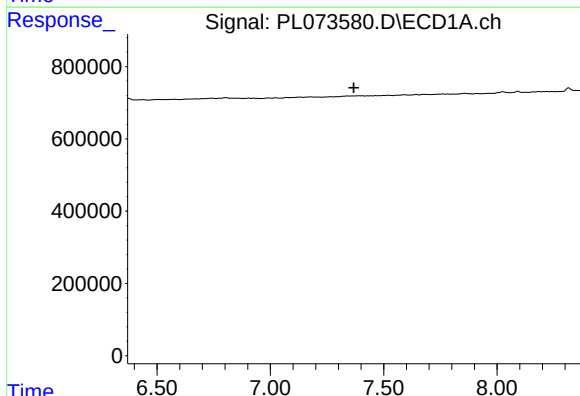


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.368 min
Response: 0
Conc: N.D.

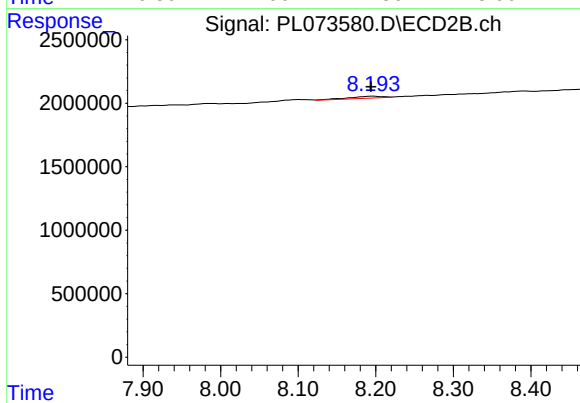

#10 gamma-Chlordane


R.T.: 8.196 min
Delta R.T.: 0.002 min
Response: 455209
Conc: 0.22 ng/ml

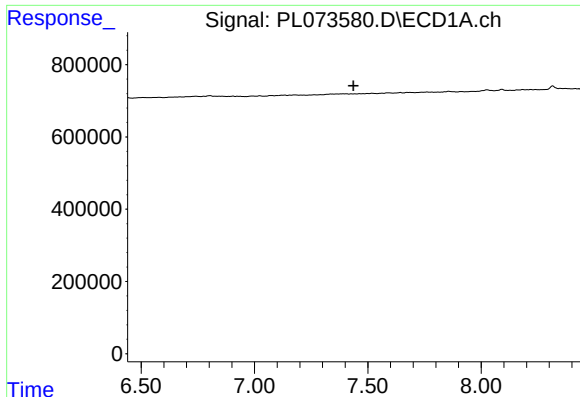

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

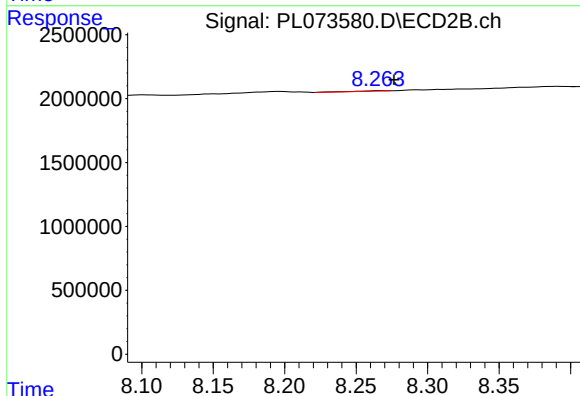


#11 alpha-Chlordane

R.T.: 8.267 min
Delta R.T.: -0.010 min
Response: 60176
Conc: 0.03 ng/ml

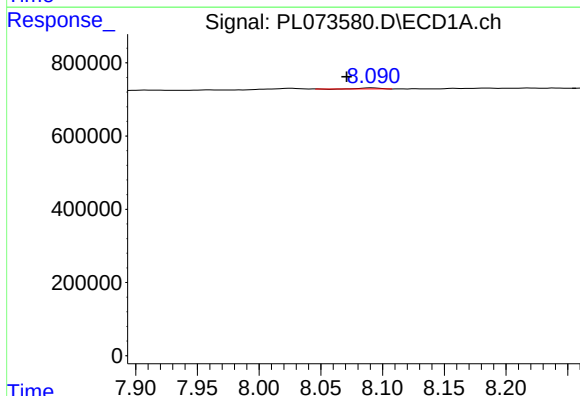


#14 Endrin

R.T.: 8.092 min
Delta R.T.: 0.021 min
Response: 30000
Conc: 0.08 ng/ml

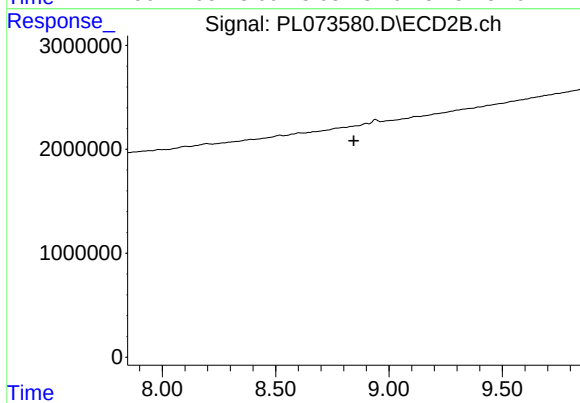

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.845 min
Response: 0
Conc: N.D.

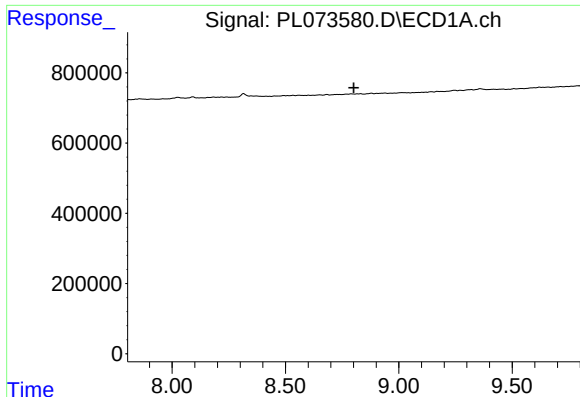

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

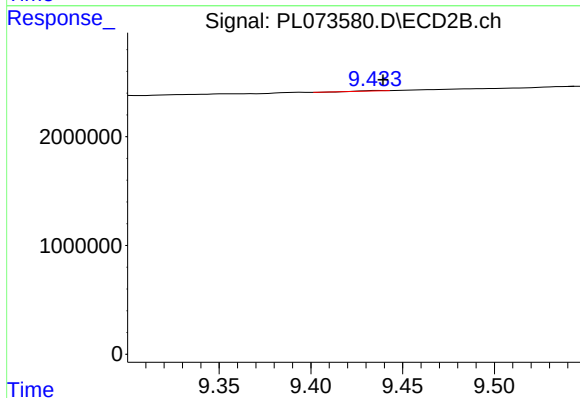


#19 Endosulfan Sulfate

R.T.: 9.437 min
Delta R.T.: -0.002 min
Response: 15957
Conc: 0.01 ng/ml

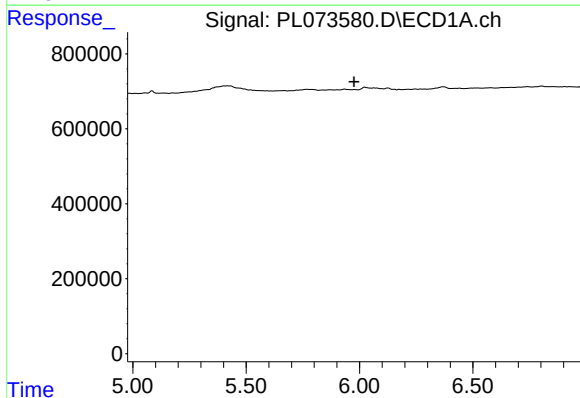


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

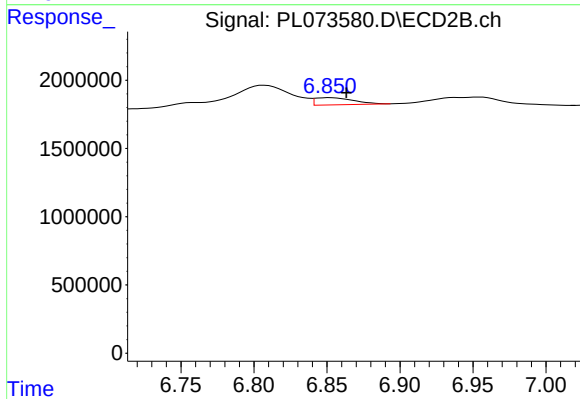

#23 Chlordane-1


R.T.: 6.852 min
Delta R.T.: -0.011 min
Response: 945697
Conc: 13.84 ng/ml

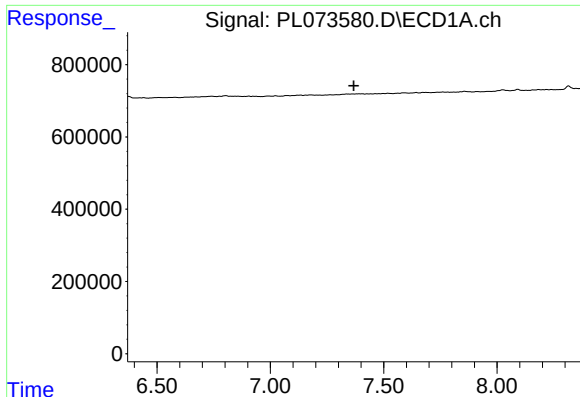

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

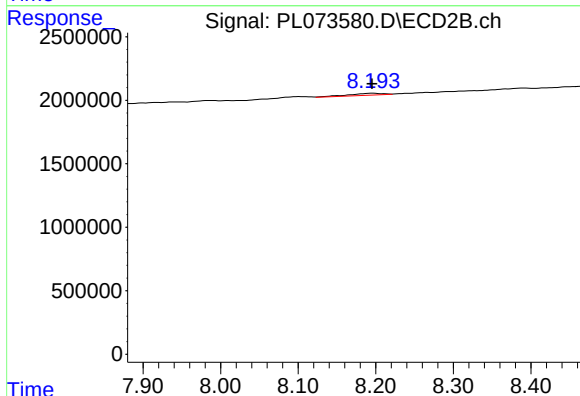


#25 Chlordane-3

R.T.: 8.196 min
Delta R.T.: 0.001 min
Response: 455209
Conc: 1.68 ng/ml

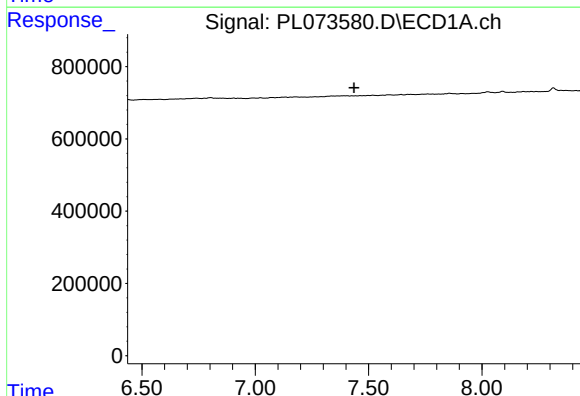


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

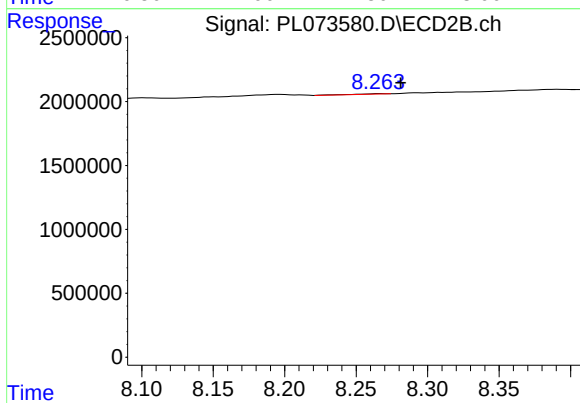

#26 Chlordane-4


R.T.: 8.267 min
Delta R.T.: -0.015 min
Response: 60176
Conc: 0.18 ng/ml

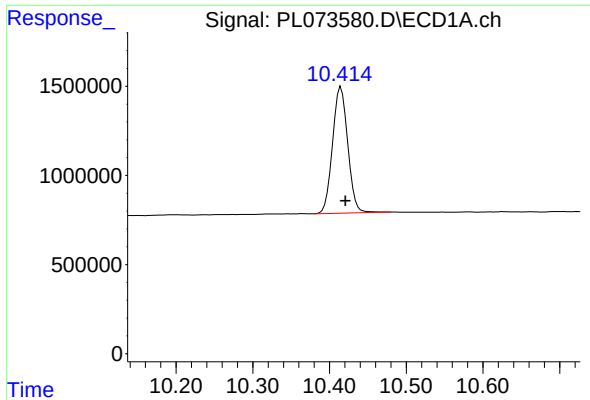

#28 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.006 min
Response: 9757994
Conc: 19.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

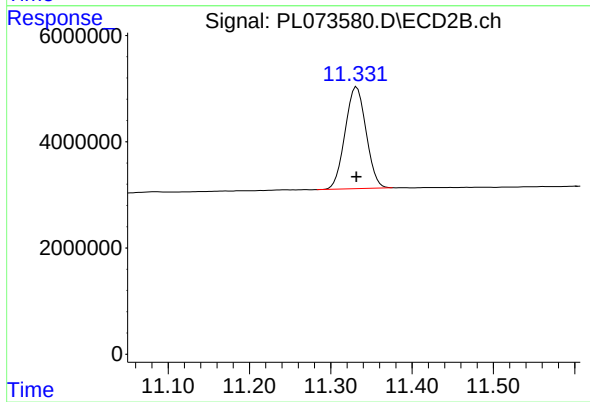

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 34306657
Conc: 19.19 ng/ml