

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032222\
 Data File : PL073574.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2022 15:37
 Operator : AR\AJ
 Sample : N1908-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-8-9-2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/23/2022
 Supervised By : mohammad ahmed 03/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:45:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.490	6083323	32269322	18.993m	19.661m
28)	SA Decachlor...	10.416	11.332	9570339	34088441	18.821	19.063

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032222\
Data File : PL073574.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2022 15:37
Operator : AR\AJ
Sample : N1908-04
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-8-9-2


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/23/2022
Supervised By : mohammad ahmed 03/23/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:45:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

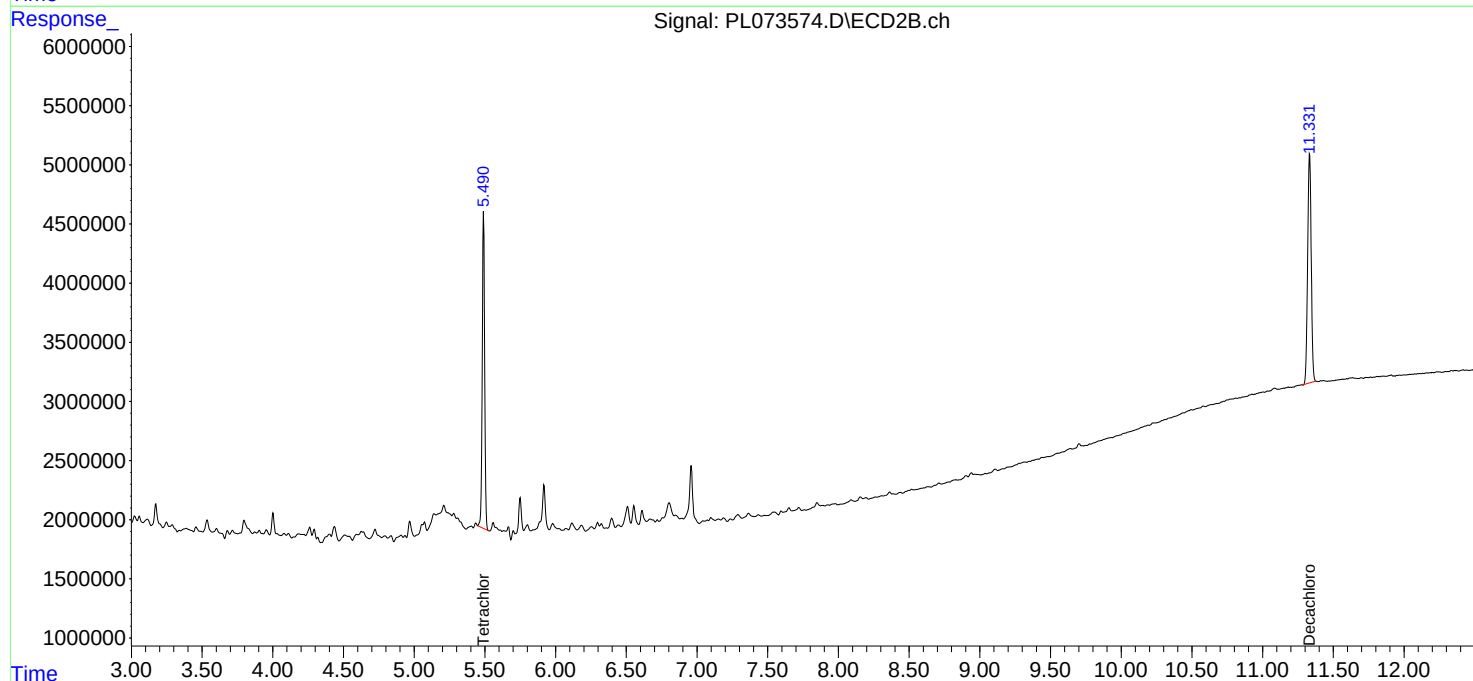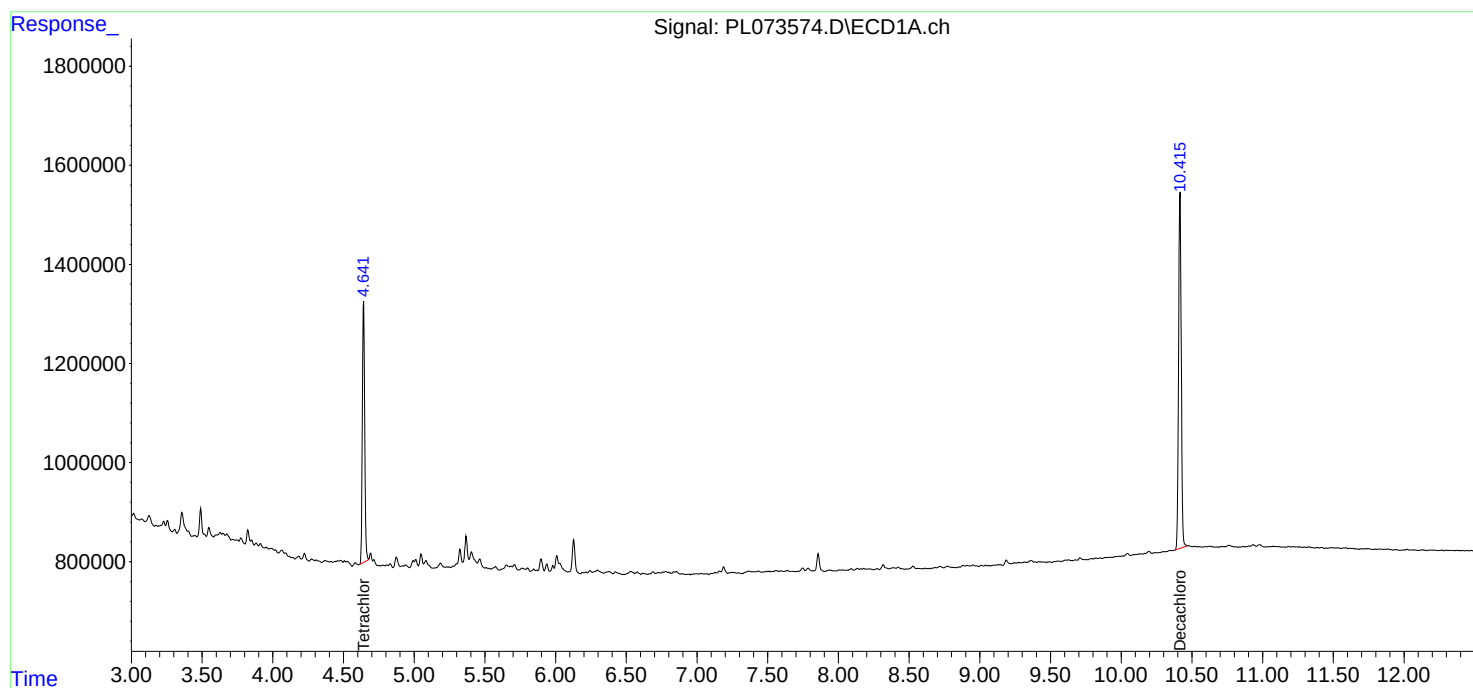

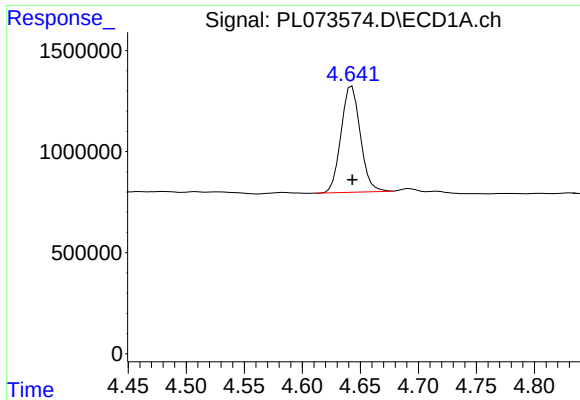


#1 Tetrachloro-m-xylene

R.T.: 4.641 min
Delta R.T.: -0.002 min
Response: 6083323
Conc: 18.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-8-9-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/23/2022
Supervised By :mohammad ahmed 03/23/2022

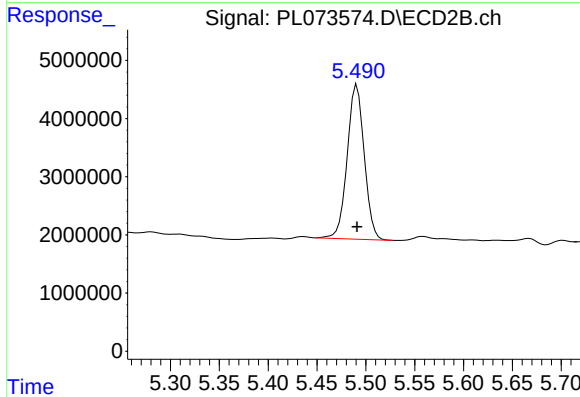


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.001 min
Response: 32269322
Conc: 19.66 ng/ml m

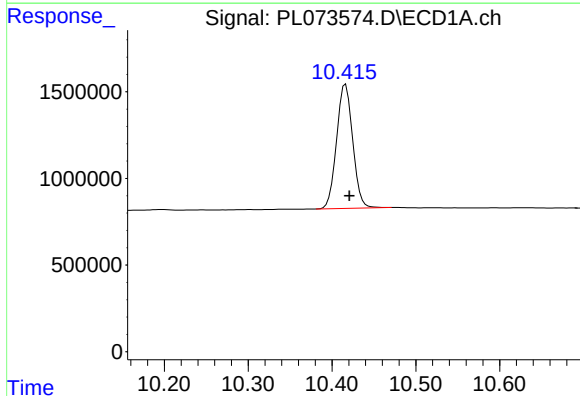

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.005 min
Response: 9570339
Conc: 18.82 ng/ml

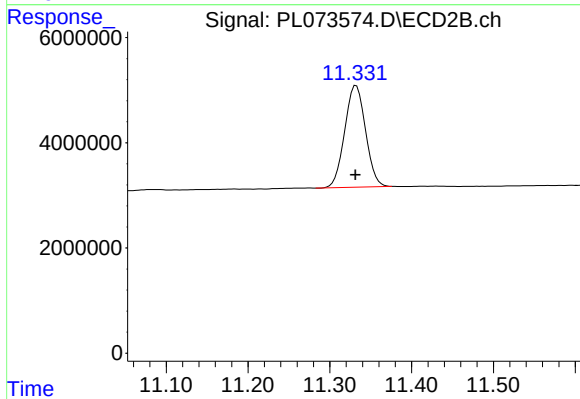

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 34088441
Conc: 19.06 ng/ml