

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032223\
 Data File : PL081611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2023 20:07
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 21:26:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 22 21:23:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	2.658	163.0E6	180.4E6	72.494	72.479
28)	SA Decachlor...	8.748	7.776	118.0E6	134.0E6	70.313	70.857
Target Compounds							
23)	Chlordane-1	4.473	3.646	73403157	56925531	722.036	722.910
24)	Chlordane-2	5.000	4.221	75641642	66743421	706.091	708.613
25)	Chlordane-3	5.704	4.848	296.9E6	194.1E6	733.693	740.428
26)	Chlordane-4	5.785	4.909	355.0E6	196.7E6	727.639	729.563
27)	Chlordane-5	6.626	5.575	60297709	50622403	716.544	733.165



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032223\
Data File : PL081611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2023 20:07
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 21:26:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Wed Mar 22 21:23:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

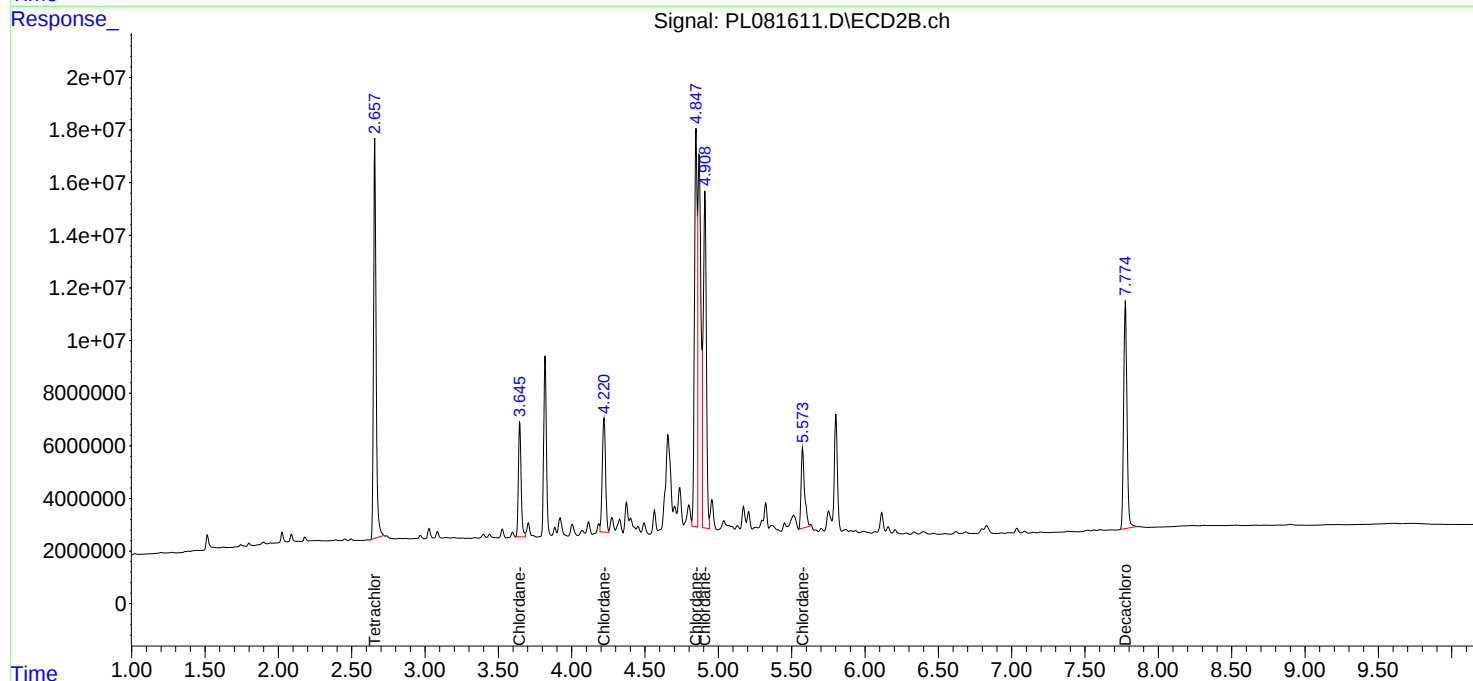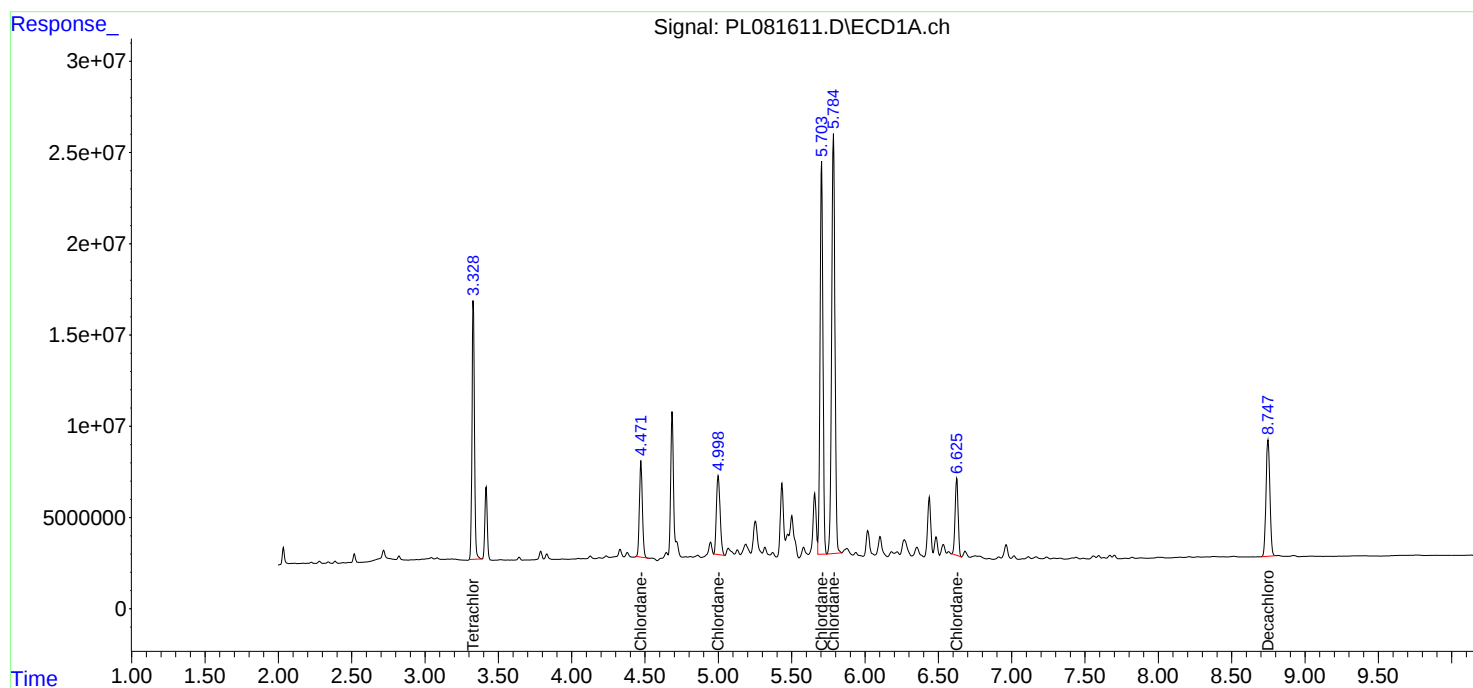


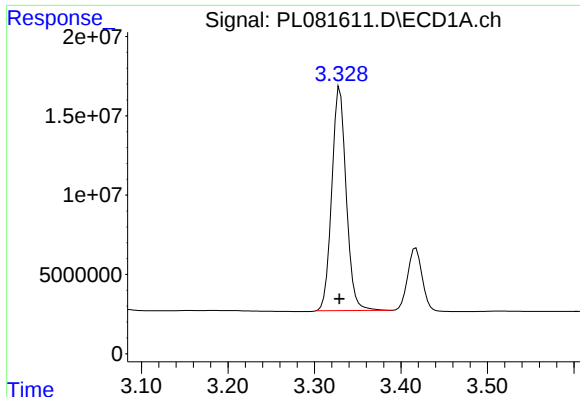

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 162976470
Conc: 72.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

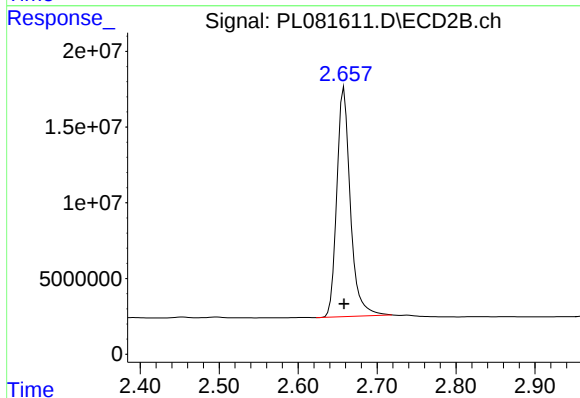


#1 Tetrachloro-m-xylene

R.T.: 2.658 min
Delta R.T.: 0.000 min
Response: 180369444
Conc: 72.48 ng/ml

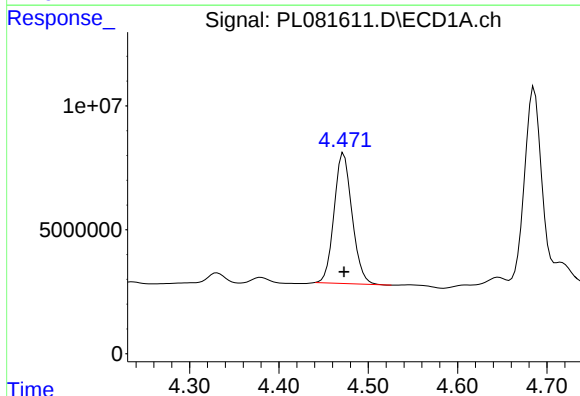


#23 Chlordane-1

R.T.: 4.473 min
Delta R.T.: 0.000 min
Response: 73403157
Conc: 722.04 ng/ml

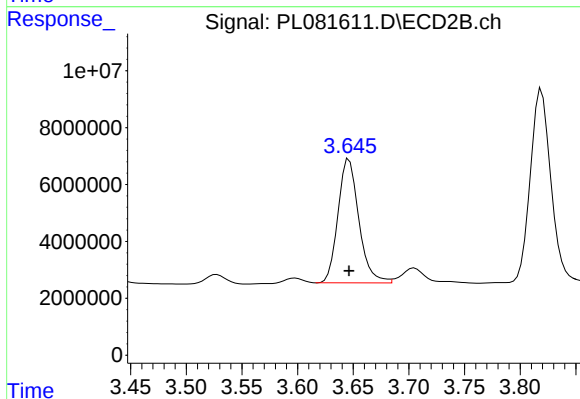

#23 Chlordane-1


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 56925531
Conc: 722.91 ng/ml

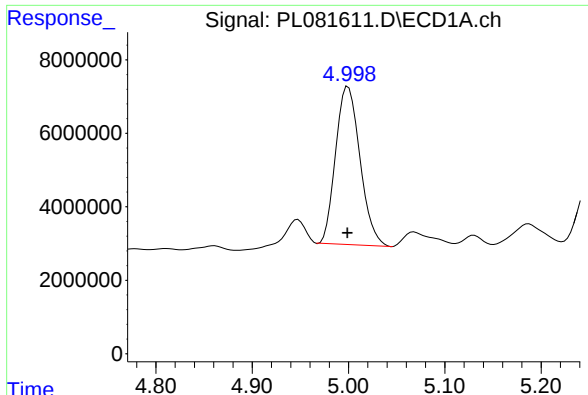

#24 Chlordane-2


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 75641642
Conc: 706.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

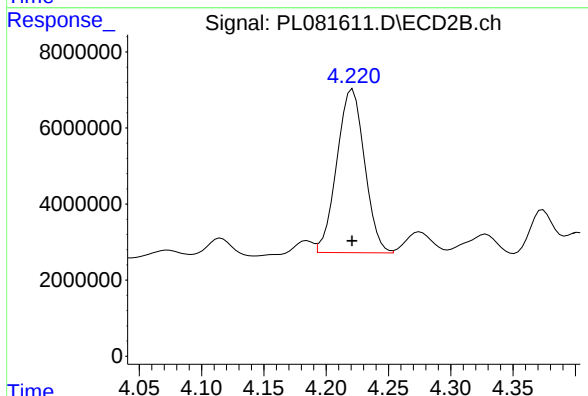


#24 Chlordane-2

R.T.: 4.221 min
Delta R.T.: 0.000 min
Response: 66743421
Conc: 708.61 ng/ml

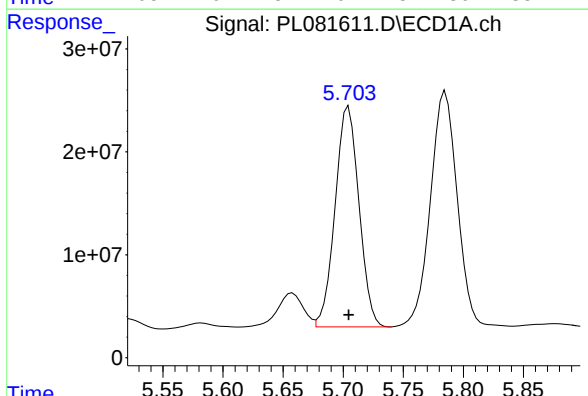


#25 Chlordane-3

R.T.: 5.704 min
Delta R.T.: 0.000 min
Response: 296883659
Conc: 733.69 ng/ml

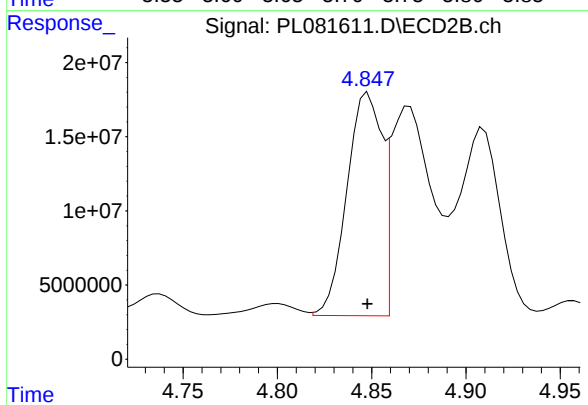

#25 Chlordane-3


R.T.: 4.848 min
Delta R.T.: 0.000 min
Response: 194094575
Conc: 740.43 ng/ml

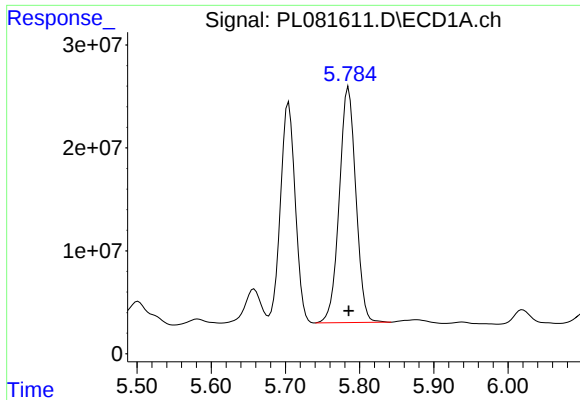

#26 Chlordane-4


R.T.: 5.785 min
Delta R.T.: 0.000 min
Response: 354956002
Conc: 727.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

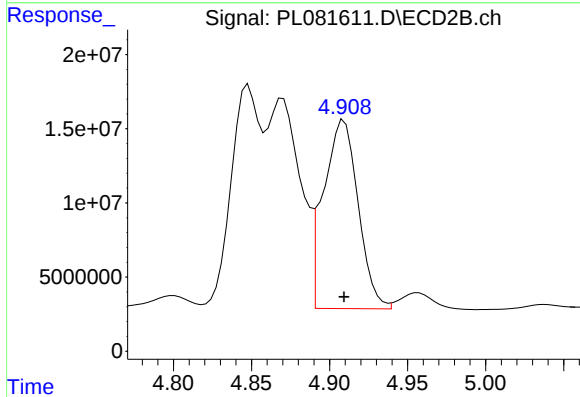


#26 Chlordane-4

R.T.: 4.909 min
Delta R.T.: 0.000 min
Response: 196739298
Conc: 729.56 ng/ml

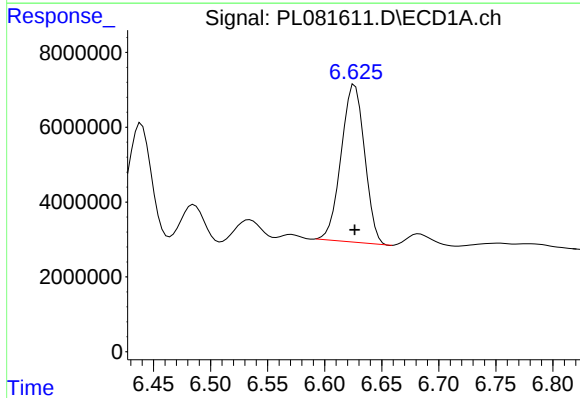


#27 Chlordane-5

R.T.: 6.626 min
Delta R.T.: 0.000 min
Response: 60297709
Conc: 716.54 ng/ml

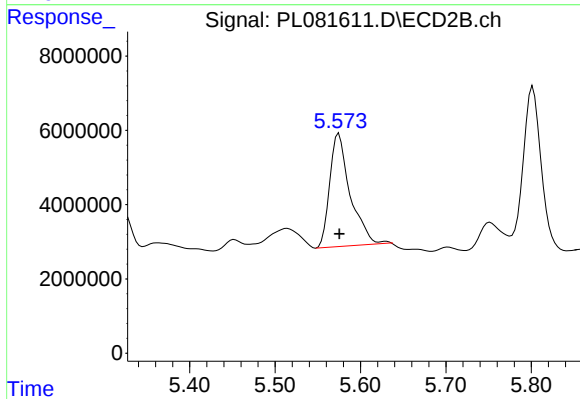

#27 Chlordane-5


R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 50622403
Conc: 733.17 ng/ml

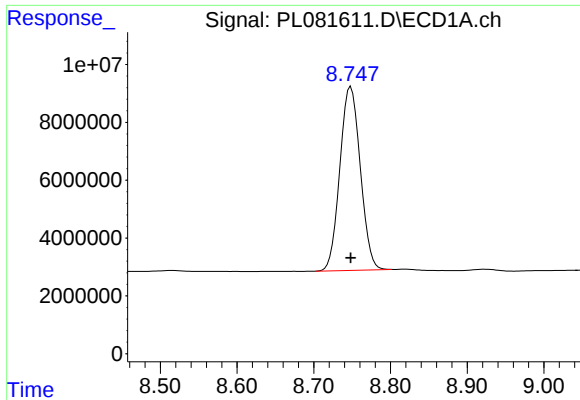

#28 Decachlorobiphenyl

R.T.: 8.748 min
Delta R.T.: 0.000 min
Response: 118035827
Conc: 70.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

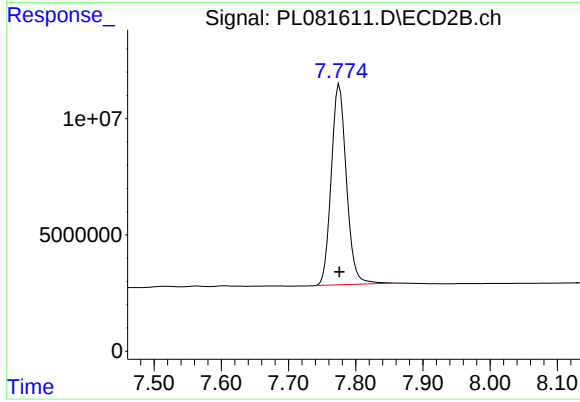

#28 Decachlorobiphenyl

R.T.: 7.776 min
Delta R.T.: 0.000 min
Response: 134011928
Conc: 70.86 ng/ml