

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032223\
 Data File : PL081612.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2023 20:21
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 21:26:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 22 21:23:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	2.658	112.4E6	124.4E6	50.000	50.000
28)	SA Decachlor...	8.748	7.776	83936554	94565523	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.473	3.646	50830669	39372480	500.000	500.000
24)	Chlordane-2	4.999	4.221	53563687	47094400	500.000	500.000
25)	Chlordane-3	5.705	4.848	202.3E6	131.1E6	500.000	500.000
26)	Chlordane-4	5.785	4.909	243.9E6	134.8E6	500.000	500.000
27)	Chlordane-5	6.626	5.575	42075393	34523197	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032223\
Data File : PL081612.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2023 20:21
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 21:26:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Wed Mar 22 21:23:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

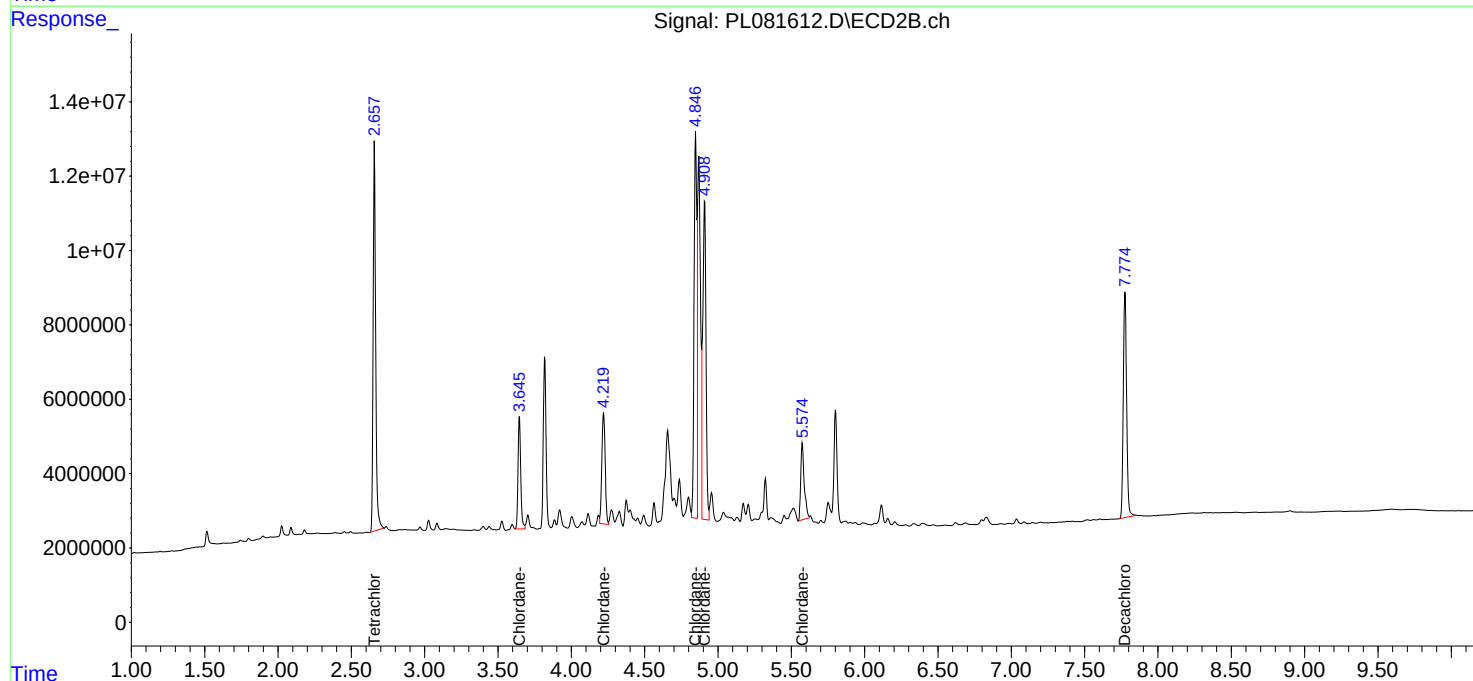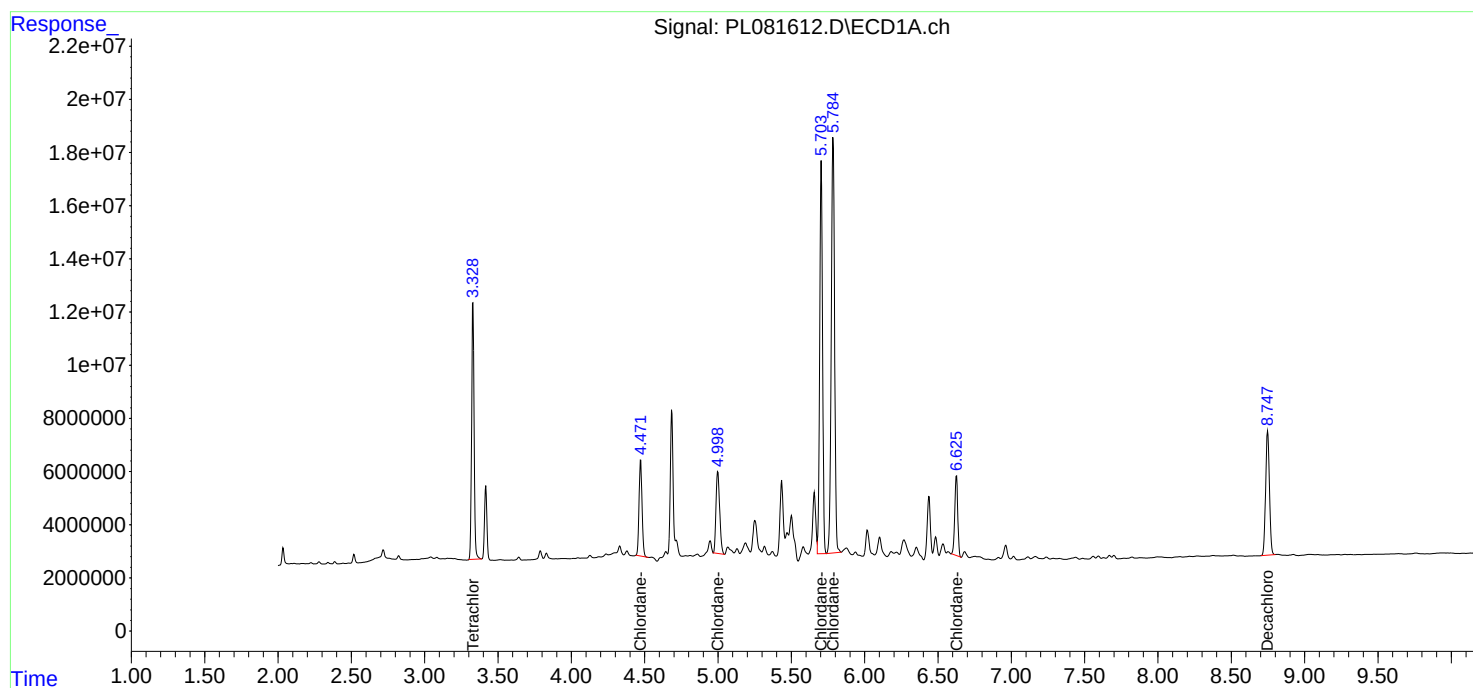


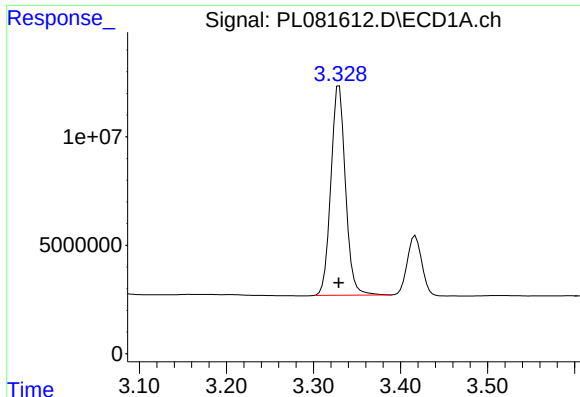

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 112407053
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

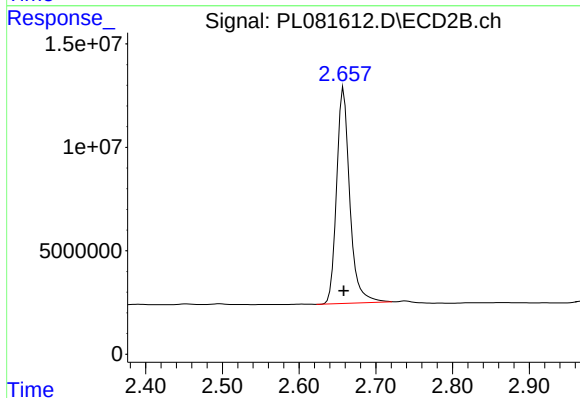


#1 Tetrachloro-m-xylene

R.T.: 2.658 min
Delta R.T.: 0.000 min
Response: 124429279
Conc: 50.00 ng/ml

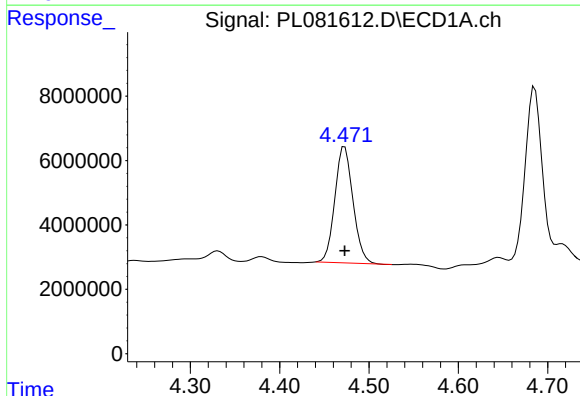


#23 Chlordane-1

R.T.: 4.473 min
Delta R.T.: 0.000 min
Response: 50830669
Conc: 500.00 ng/ml

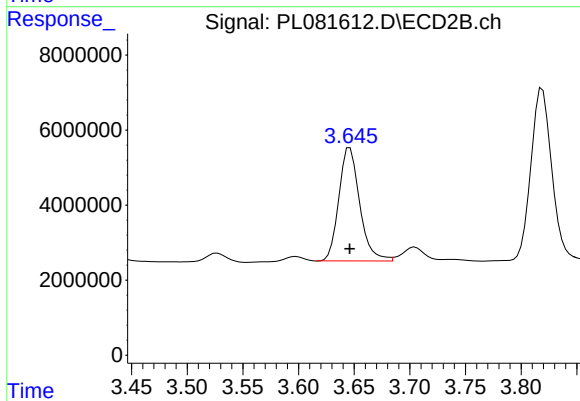

#23 Chlordane-1


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 39372480
Conc: 500.00 ng/ml

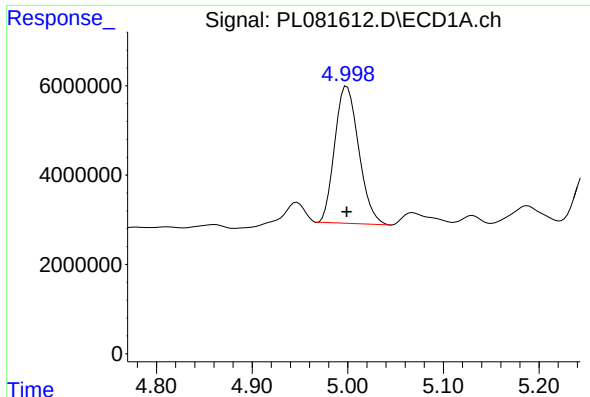

#24 Chlordane-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 53563687
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

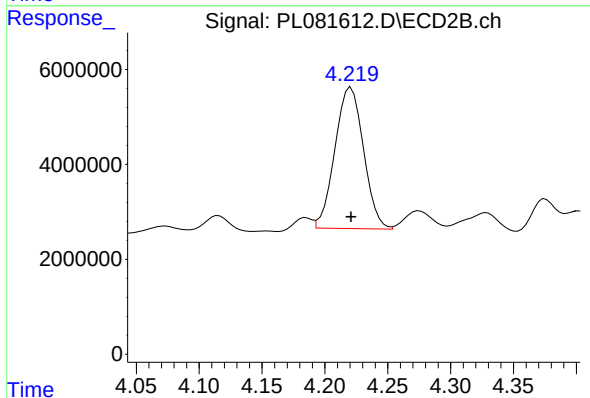


#24 Chlordane-2

R.T.: 4.221 min
Delta R.T.: 0.000 min
Response: 47094400
Conc: 500.00 ng/ml

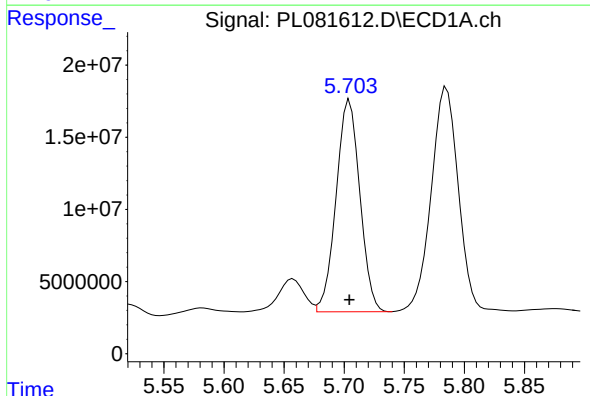


#25 Chlordane-3

R.T.: 5.705 min
Delta R.T.: 0.000 min
Response: 202321323
Conc: 500.00 ng/ml

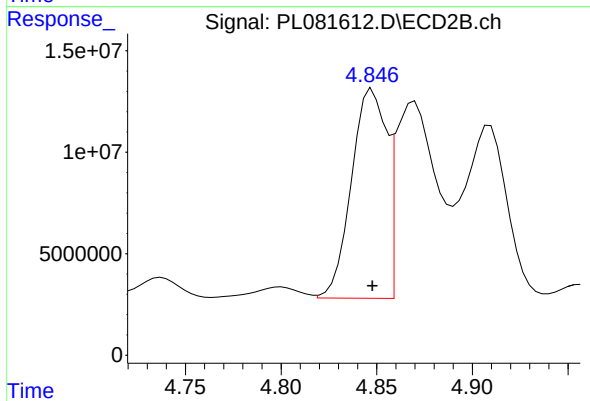

#25 Chlordane-3


R.T.: 4.848 min
Delta R.T.: 0.000 min
Response: 131069248
Conc: 500.00 ng/ml

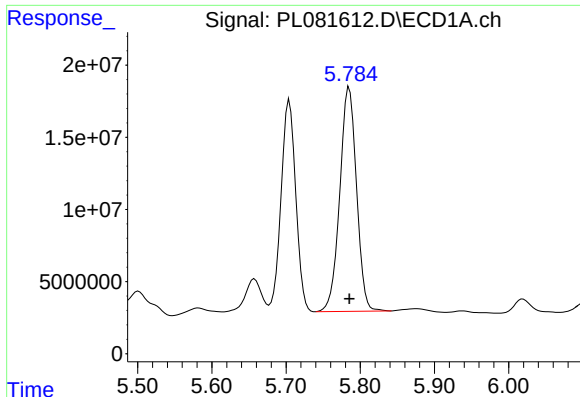

#26 Chlordane-4


R.T.: 5.785 min
Delta R.T.: 0.000 min
Response: 243909526
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

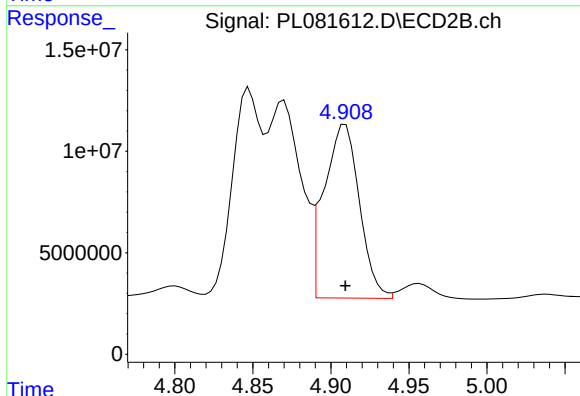


#26 Chlordane-4

R.T.: 4.909 min
Delta R.T.: 0.000 min
Response: 134833724
Conc: 500.00 ng/ml

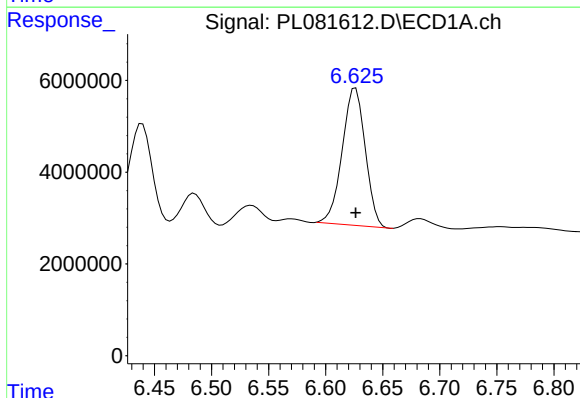


#27 Chlordane-5

R.T.: 6.626 min
Delta R.T.: 0.000 min
Response: 42075393
Conc: 500.00 ng/ml

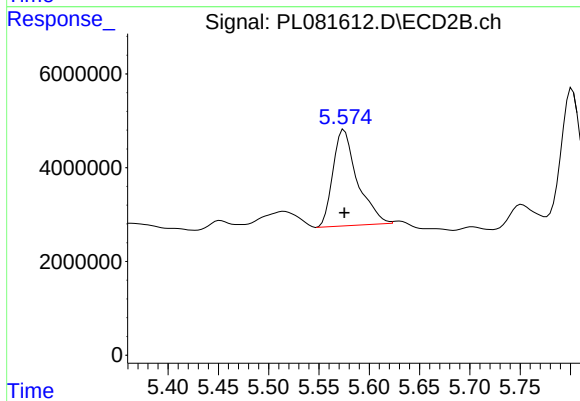

#27 Chlordane-5


R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 34523197
Conc: 500.00 ng/ml

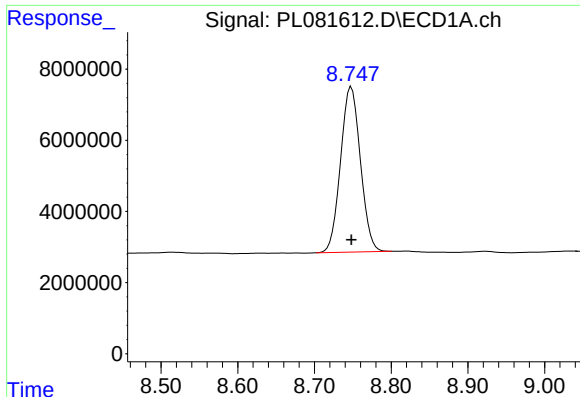

#28 Decachlorobiphenyl

R.T.: 8.748 min
Delta R.T.: 0.000 min
Response: 83936554
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

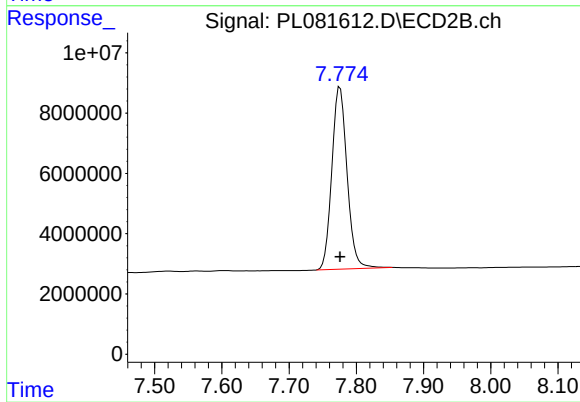

#28 Decachlorobiphenyl

R.T.: 7.776 min
Delta R.T.: 0.000 min
Response: 94565523
Conc: 50.00 ng/ml