

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032223\
 Data File : PL081613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2023 20:35
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 21:27:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 22 21:23:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	2.658	54379642	59743494	24.189	24.007
28)	SA Decachlor...	8.749	7.776	42948170	47992856	25.584	25.375
Target Compounds							
23)	Chlordane-1	4.473	3.646	24764833	19380578	243.601	246.118
24)	Chlordane-2	4.999	4.220	26647386	23416737	248.745	248.615
25)	Chlordane-3	5.704	4.847	95818136	59562903	236.797	227.219
26)	Chlordane-4	5.785	4.909	117.1E6	63560285	240.012	235.699
27)	Chlordane-5	6.625	5.574	20956907	17316380	249.040	250.793


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032223\
Data File : PL081613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2023 20:35
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 21:27:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Wed Mar 22 21:23:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

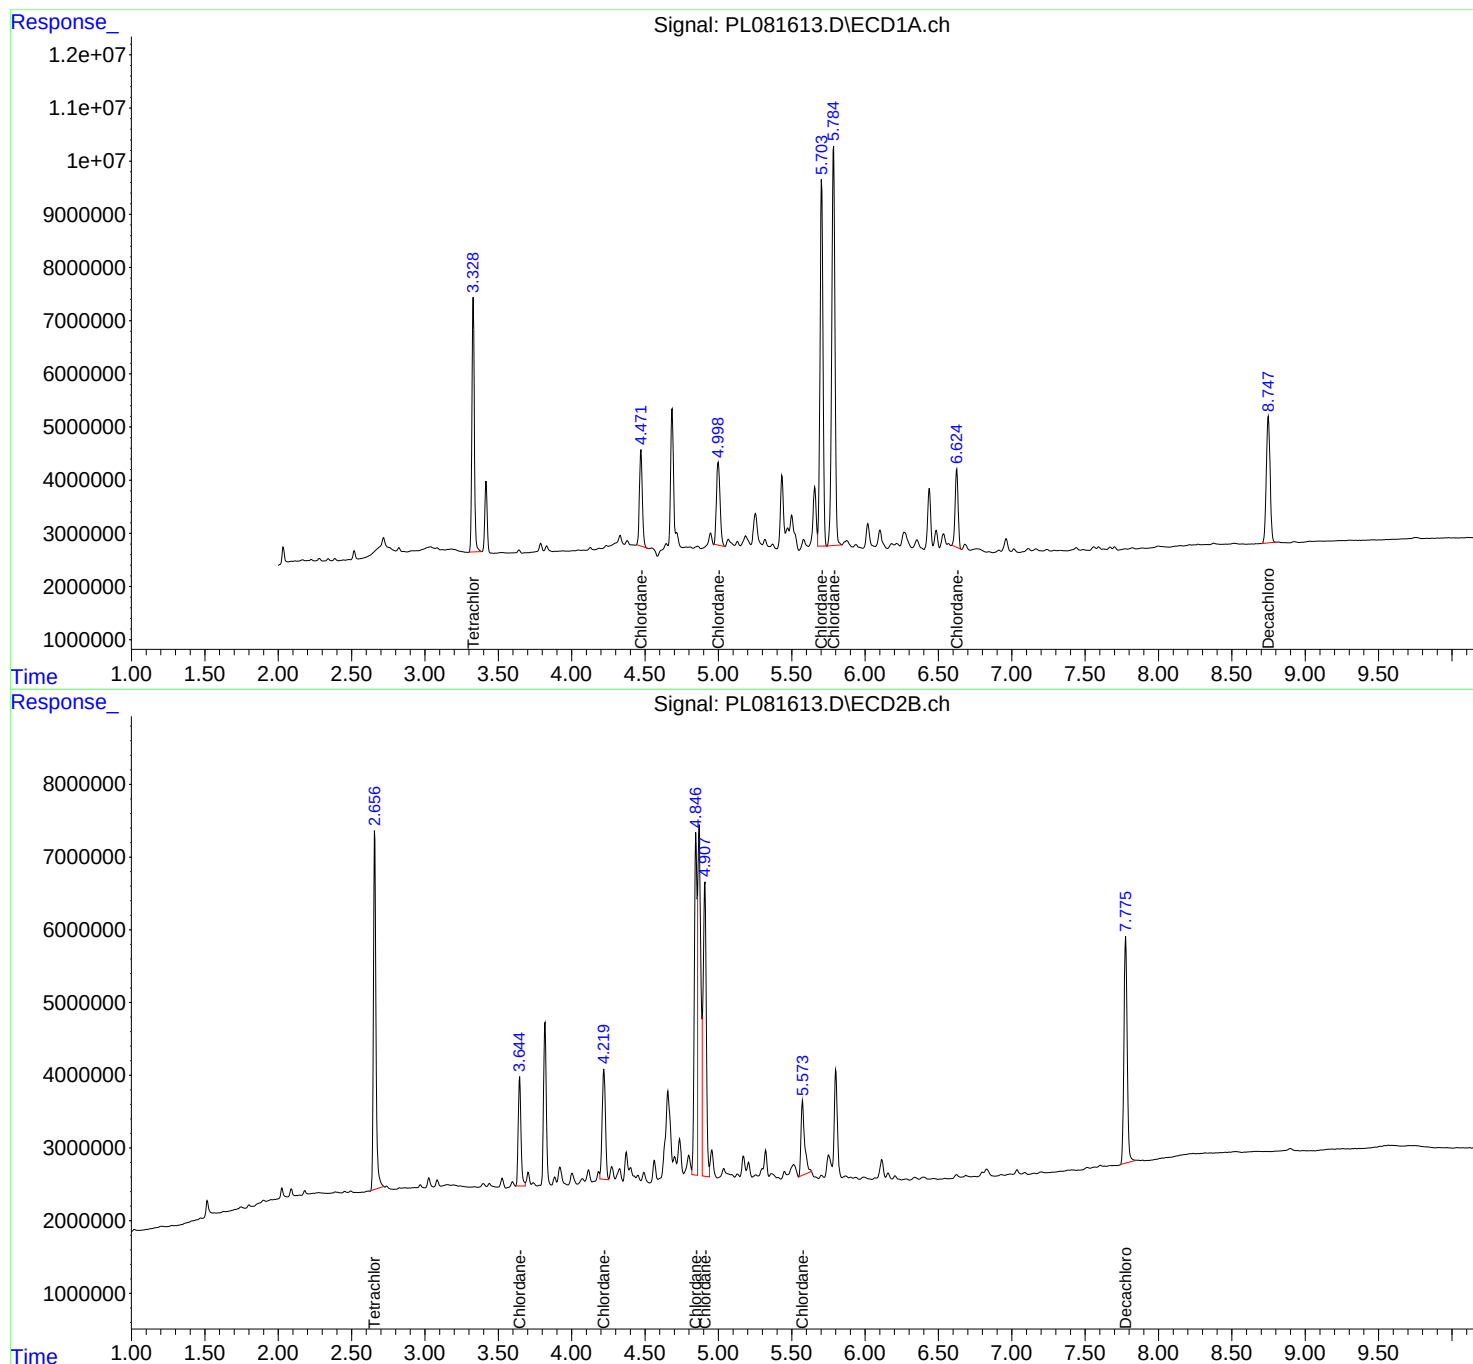


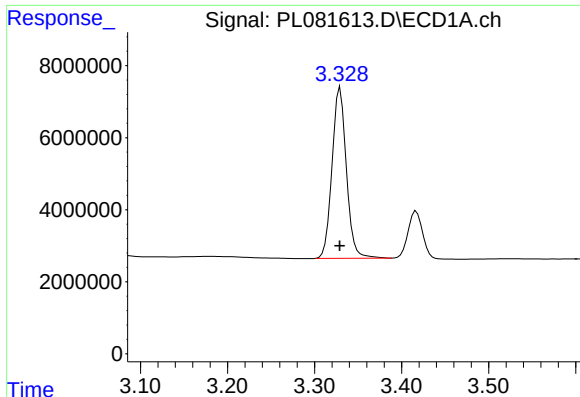

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 54379642
Conc: 24.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

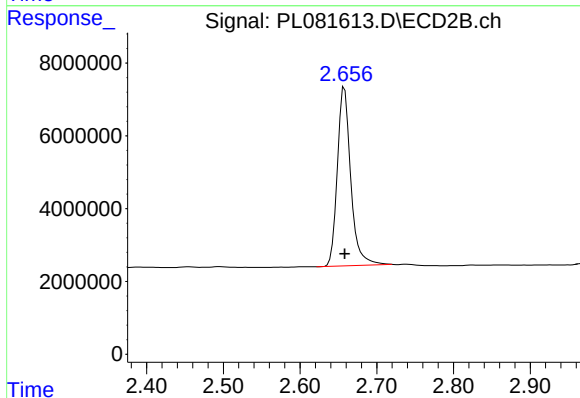


#1 Tetrachloro-m-xylene

R.T.: 2.658 min
Delta R.T.: 0.000 min
Response: 59743494
Conc: 24.01 ng/ml

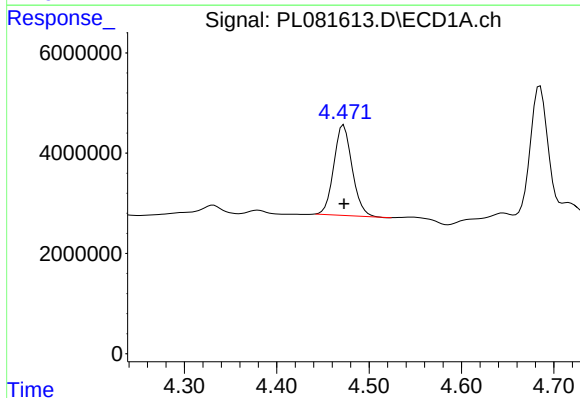


#23 Chlordane-1

R.T.: 4.473 min
Delta R.T.: 0.000 min
Response: 24764833
Conc: 243.60 ng/ml

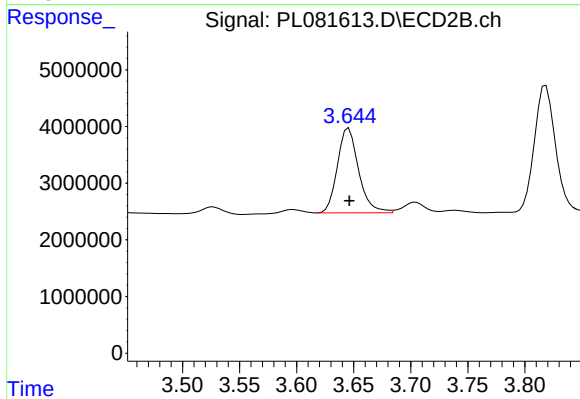

#23 Chlordane-1


R.T.: 3.646 min
Delta R.T.: 0.000 min
Response: 19380578
Conc: 246.12 ng/ml

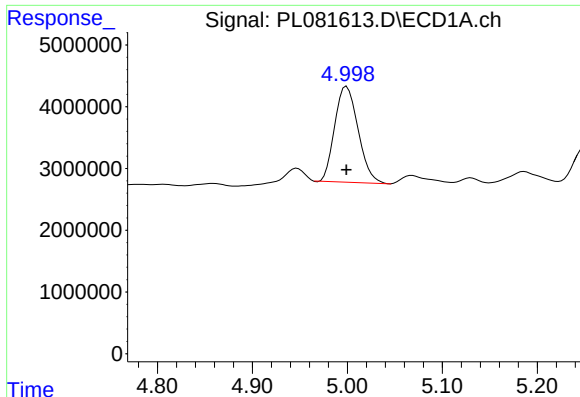

#24 Chlordane-2


R.T.: 4.999 min
Delta R.T.: 0.000 min
Response: 26647386
Conc: 248.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

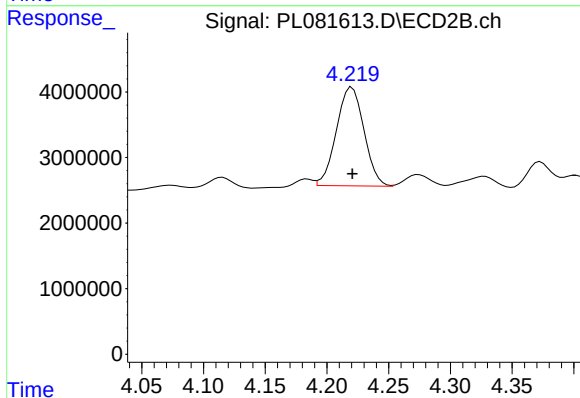


#24 Chlordane-2

R.T.: 4.220 min
Delta R.T.: 0.000 min
Response: 23416737
Conc: 248.61 ng/ml

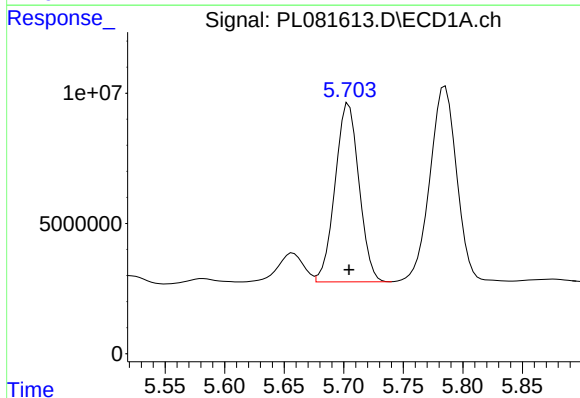


#25 Chlordane-3

R.T.: 5.704 min
Delta R.T.: 0.000 min
Response: 95818136
Conc: 236.80 ng/ml

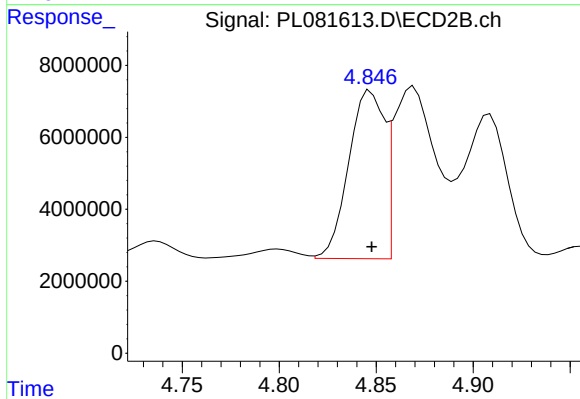

#25 Chlordane-3


R.T.: 4.847 min
Delta R.T.: 0.000 min
Response: 59562903
Conc: 227.22 ng/ml

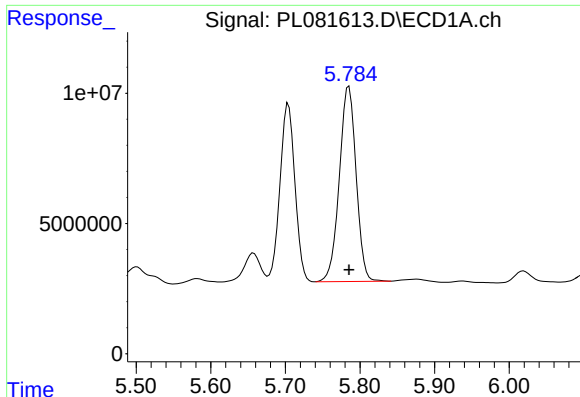

#26 Chlordane-4


R.T.: 5.785 min
Delta R.T.: 0.000 min
Response: 117082265
Conc: 240.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

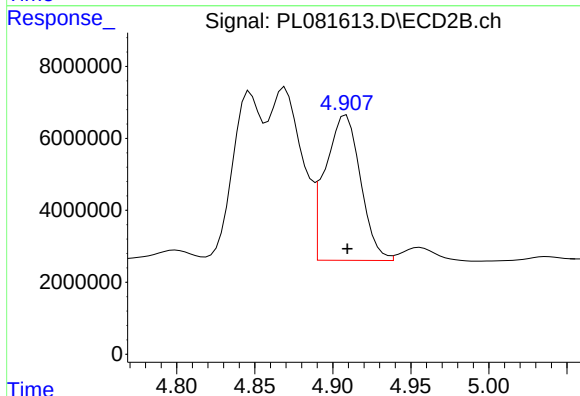


#26 Chlordane-4

R.T.: 4.909 min
Delta R.T.: 0.000 min
Response: 63560285
Conc: 235.70 ng/ml

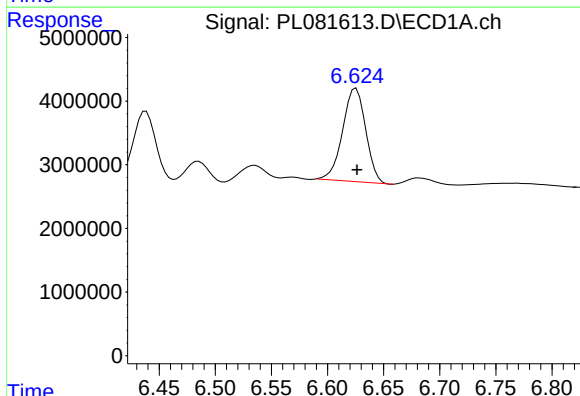


#27 Chlordane-5

R.T.: 6.625 min
Delta R.T.: 0.000 min
Response: 20956907
Conc: 249.04 ng/ml

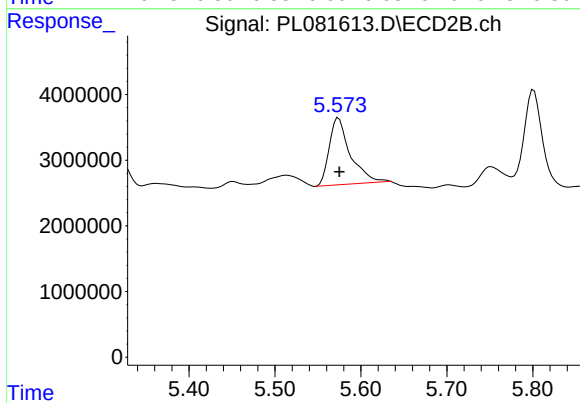

#27 Chlordane-5


R.T.: 5.574 min
Delta R.T.: 0.000 min
Response: 17316380
Conc: 250.79 ng/ml

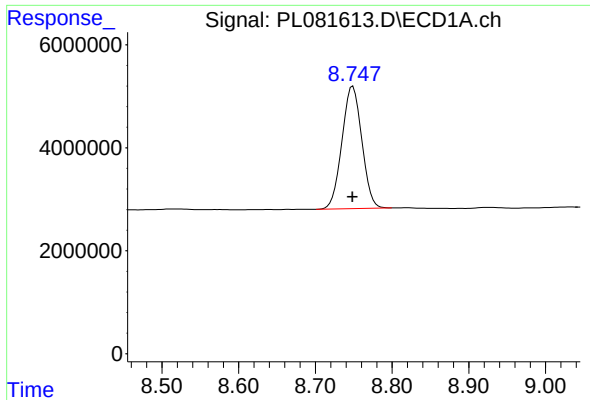

#28 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: 0.000 min
Response: 42948170
Conc: 25.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

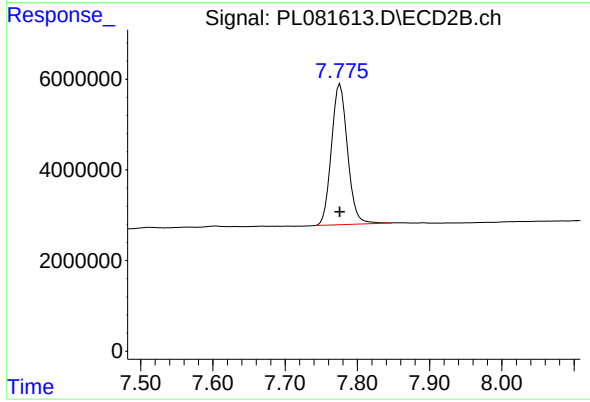

#28 Decachlorobiphenyl

R.T.: 7.776 min
Delta R.T.: 0.000 min
Response: 47992856
Conc: 25.38 ng/ml