

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032223\
 Data File : PL081651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2023 07:20
 Operator : AR\AJ
 Sample : 02020-01
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 08:53:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.329	2.658	23740407	19942488	10.207	9.990
28) SA Decachlor...	8.749	7.775	14888736	16853218	8.319	8.498
Target Compounds						
17) MA 4,4'-DDT	6.786	5.903	1050829	1228910	0.518	0.713 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032223\
Data File : PL081651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2023 07:20
Operator : AR\AJ
Sample : 02020-01
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 08:53:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

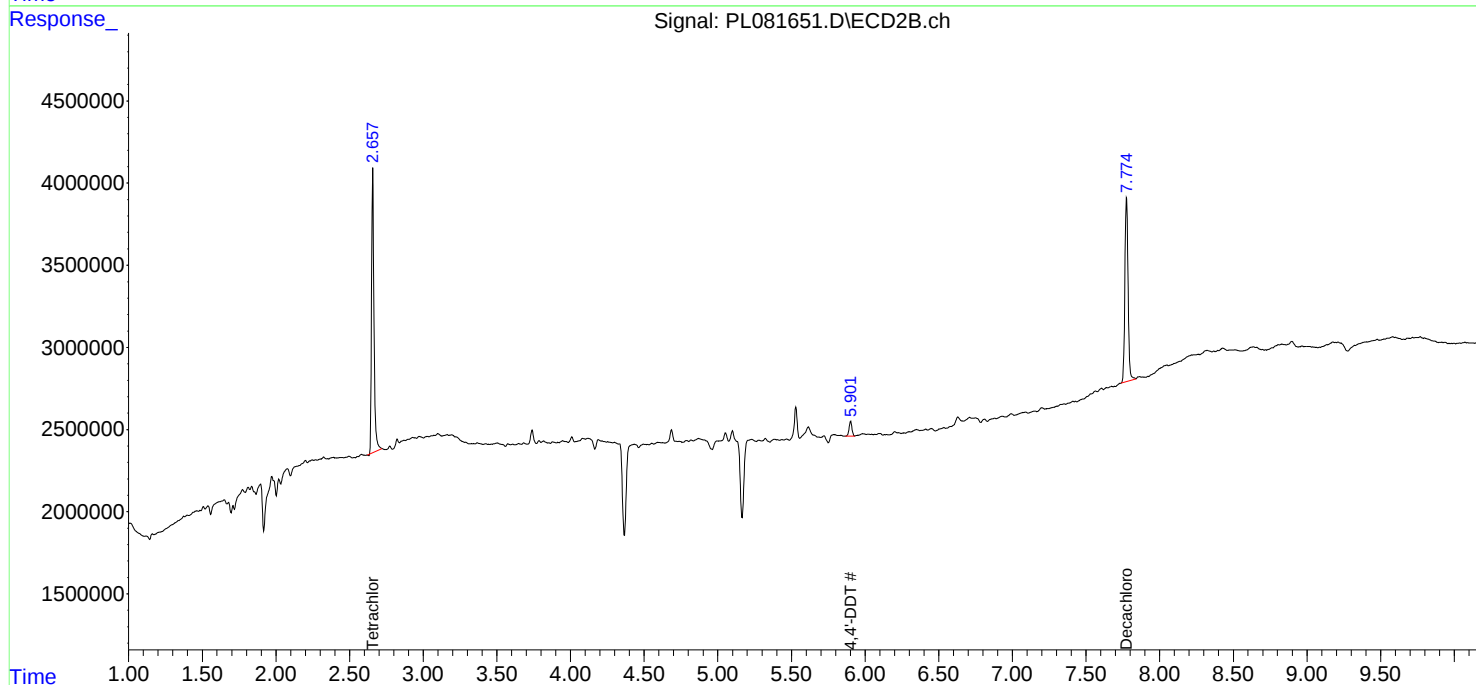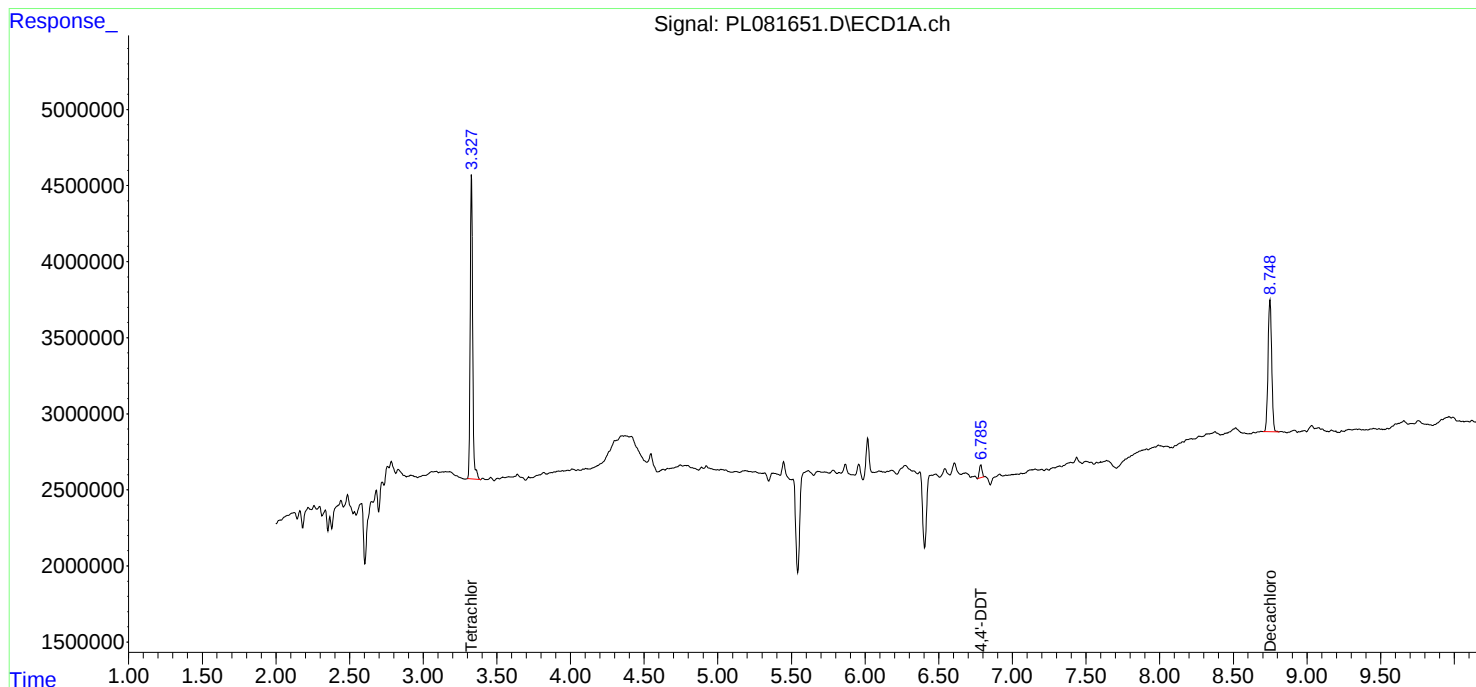


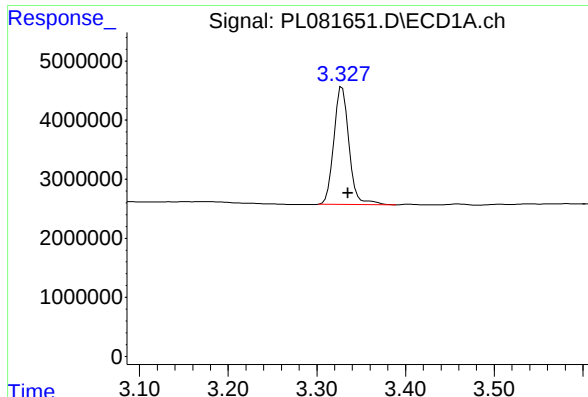

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: -0.006 min
Response: 23740407
Conc: 10.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1

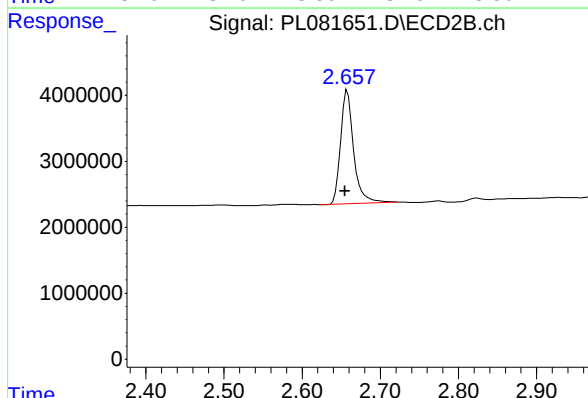


#1 Tetrachloro-m-xylene

R.T.: 2.658 min
Delta R.T.: 0.003 min
Response: 19942488
Conc: 9.99 ng/ml

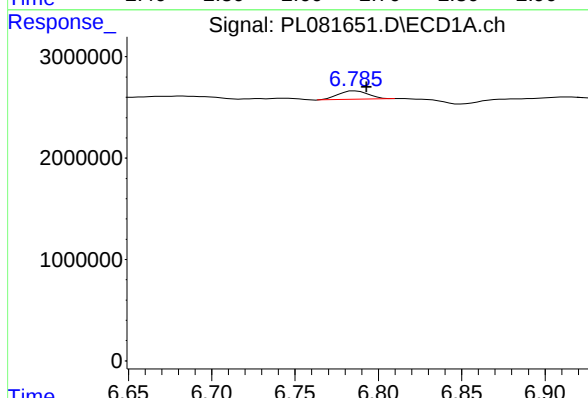


#17 4,4'-DDT

R.T.: 6.786 min
Delta R.T.: -0.007 min
Response: 1050829
Conc: 0.52 ng/ml

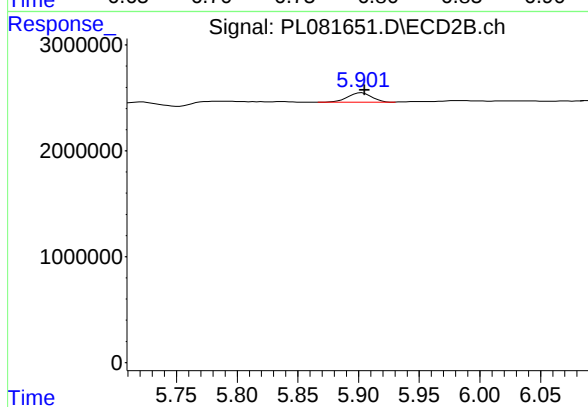

#17 4,4'-DDT


R.T.: 5.903 min
Delta R.T.: -0.002 min
Response: 1228910
Conc: 0.71 ng/ml

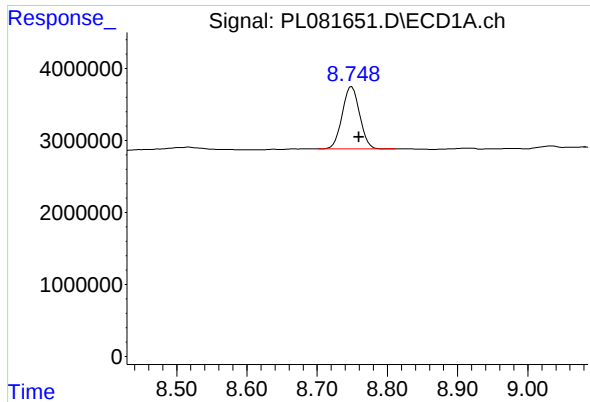

#28 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.010 min
Response: 14888736
Conc: 8.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1

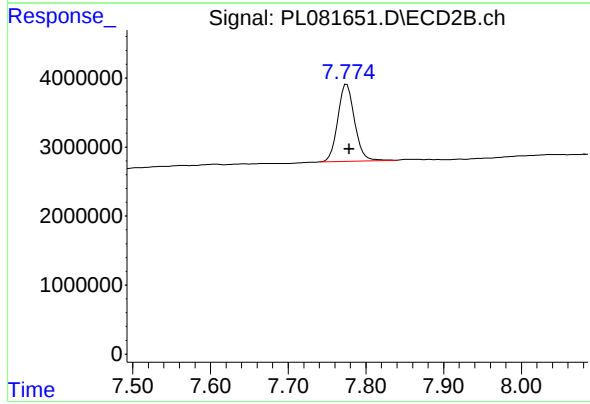

#28 Decachlorobiphenyl

R.T.: 7.775 min
Delta R.T.: -0.003 min
Response: 16853218
Conc: 8.50 ng/ml