

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032224\
 Data File : PL088743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2024 12:56
 Operator : AR\AJ
 Sample : P1786-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WASTE-COMPOSITE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/25/2024
 Supervised By :Ankita Jodhani 03/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 22:54:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.634	2.851	52127234	27064232	19.671	20.307m
28) SA Decachlor...	9.296	8.077	42154827	25179173	17.054	18.570

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032224\
Data File : PL088743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2024 12:56
Operator : AR\AJ
Sample : P1786-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WASTE-COMPOSITE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/25/2024
Supervised By : Ankita Jodhani 03/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 22:54:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

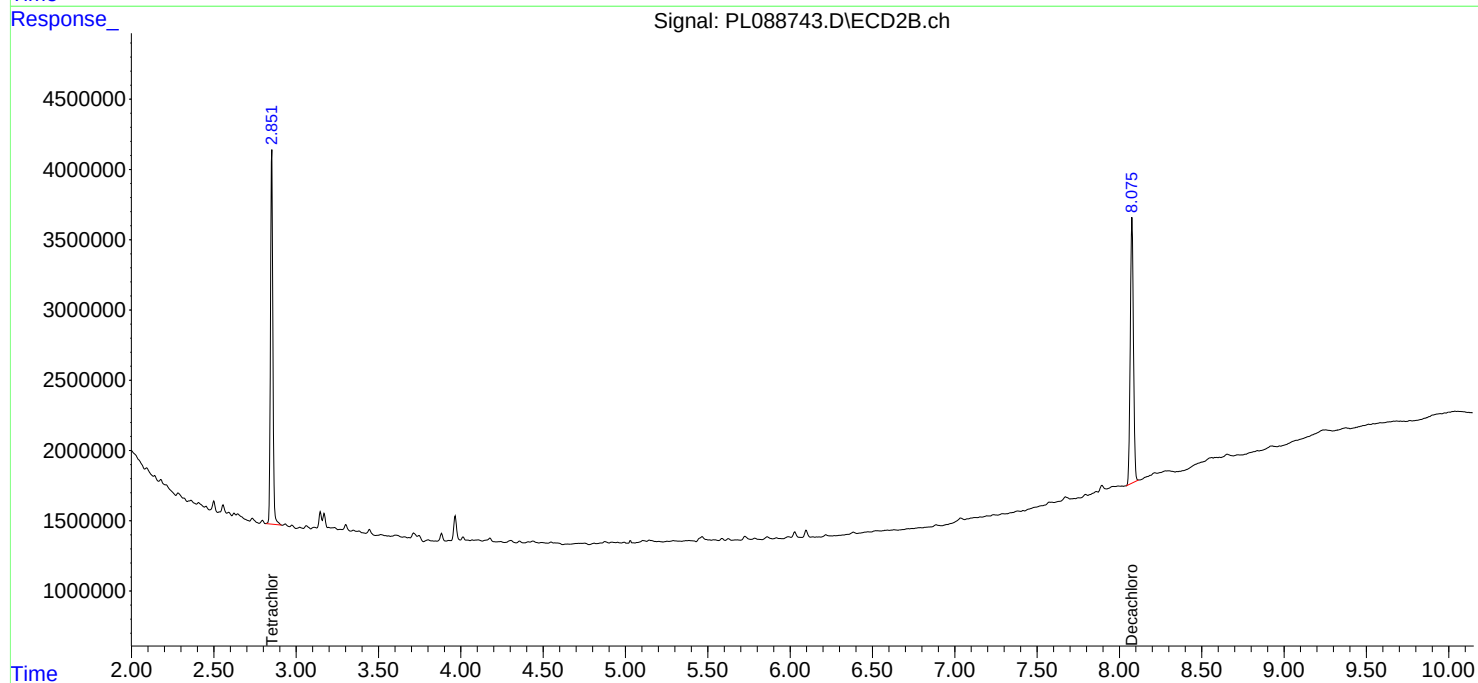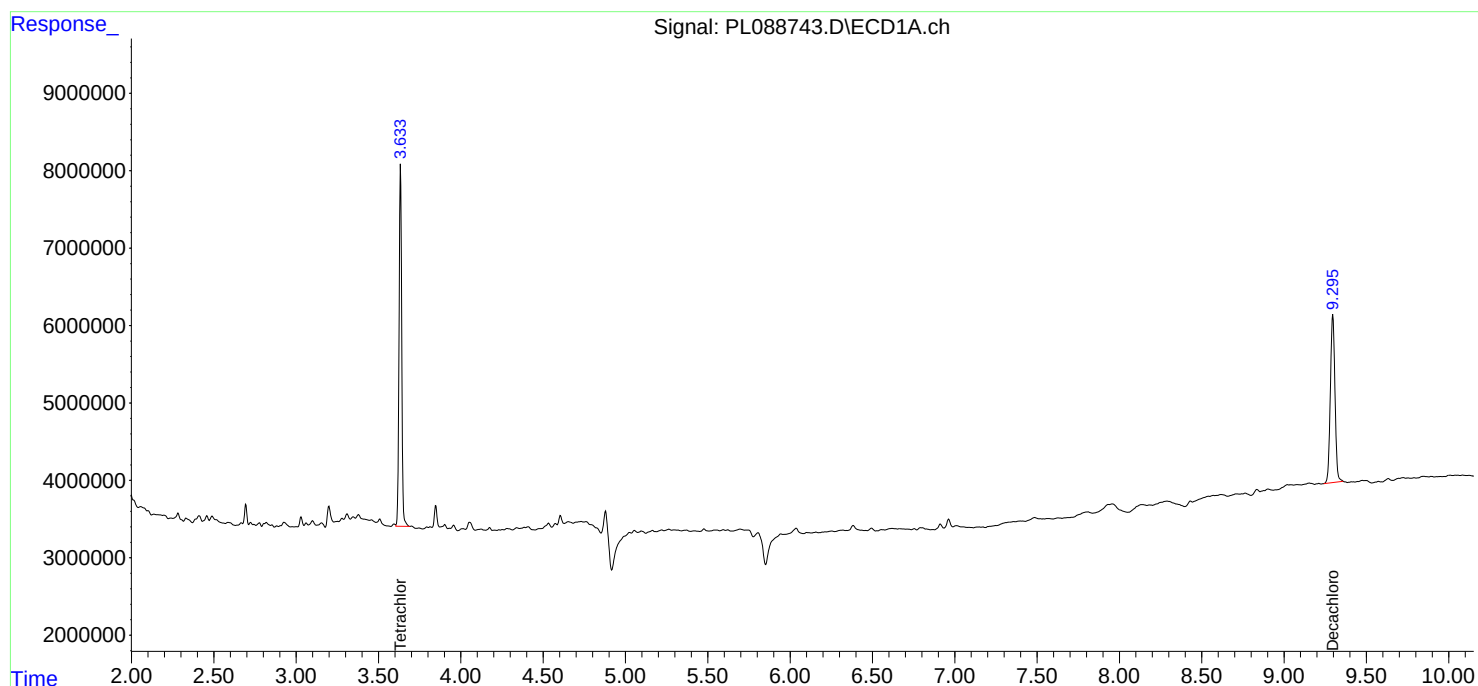

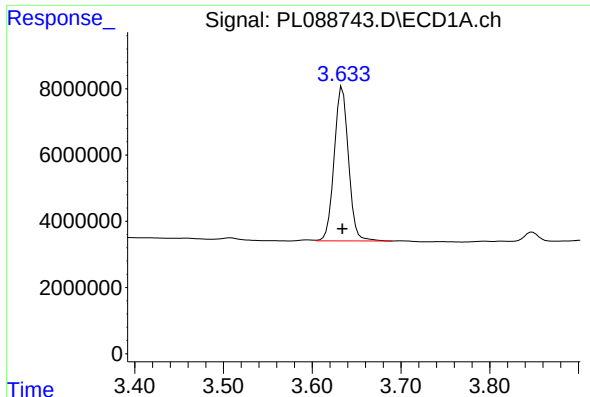


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 52127234
Conc: 19.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
WASTE-COMPOSITE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/25/2024
Supervised By :Ankita Jodhani 03/25/2024

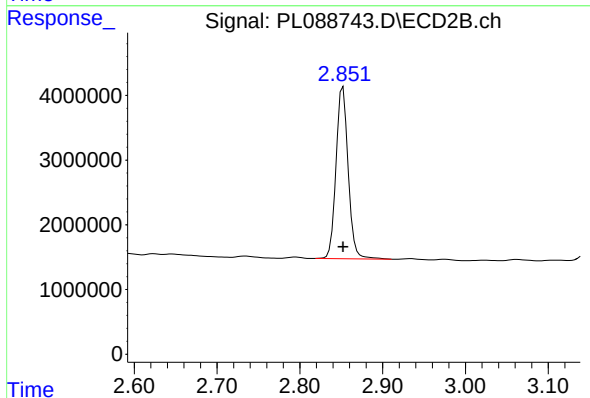


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: -0.002 min
Response: 27064232
Conc: 20.31 ng/ml m

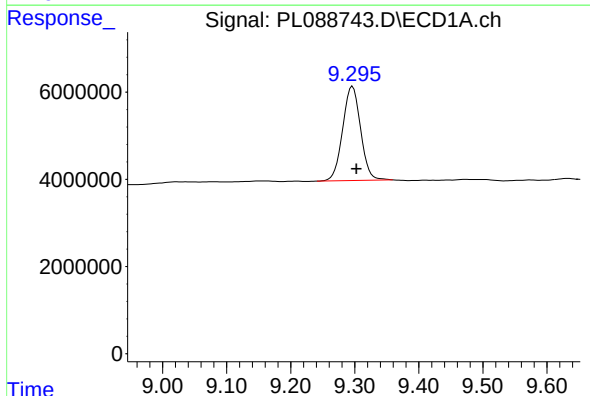

#28 Decachlorobiphenyl

R.T.: 9.296 min
Delta R.T.: -0.006 min
Response: 42154827
Conc: 17.05 ng/ml

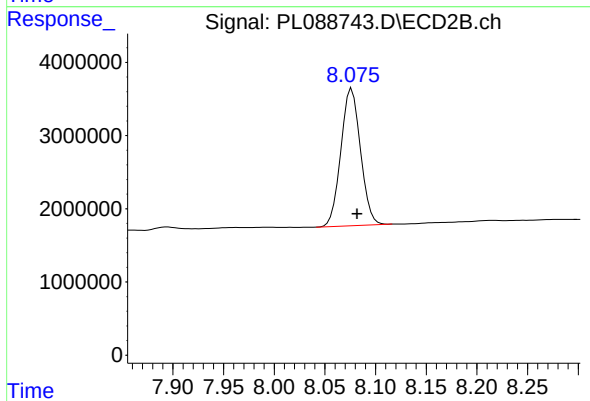

#28 Decachlorobiphenyl

R.T.: 8.077 min
Delta R.T.: -0.005 min
Response: 25179173
Conc: 18.57 ng/ml