

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032319\
 Data File : PL046371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2019 18:32
 Operator : AJ\SJ
 Sample : K2014-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-026-SW075-031819

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 04:34:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.979	121.2E6	37615525	16.660	16.429
28)	SA Decachlor...	8.039	9.034	105.5E6	32922284	12.544	14.200
Target Compounds							
10)	B gamma-Chl...	0.000	6.072f	0	2359710	N.D.	0.831 #
19)	B Endosulfa...	6.490f	7.235	7974220	2672290	0.971	1.133
25)	Chlordane-3	0.000	6.072f	0	2359710	N.D.	6.189 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032319\
Data File : PL046371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2019 18:32
Operator : AJ\SJ
Sample : K2014-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-026-SW075-031819

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 04:34:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

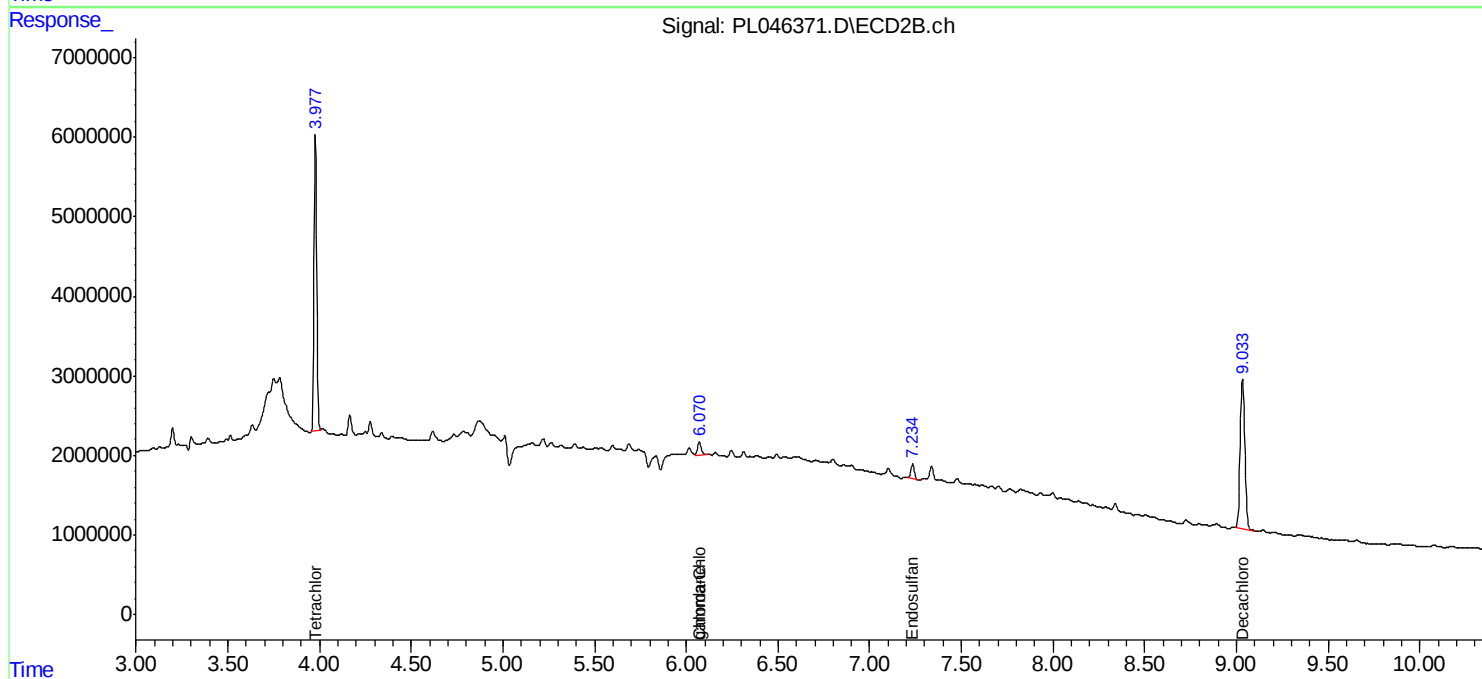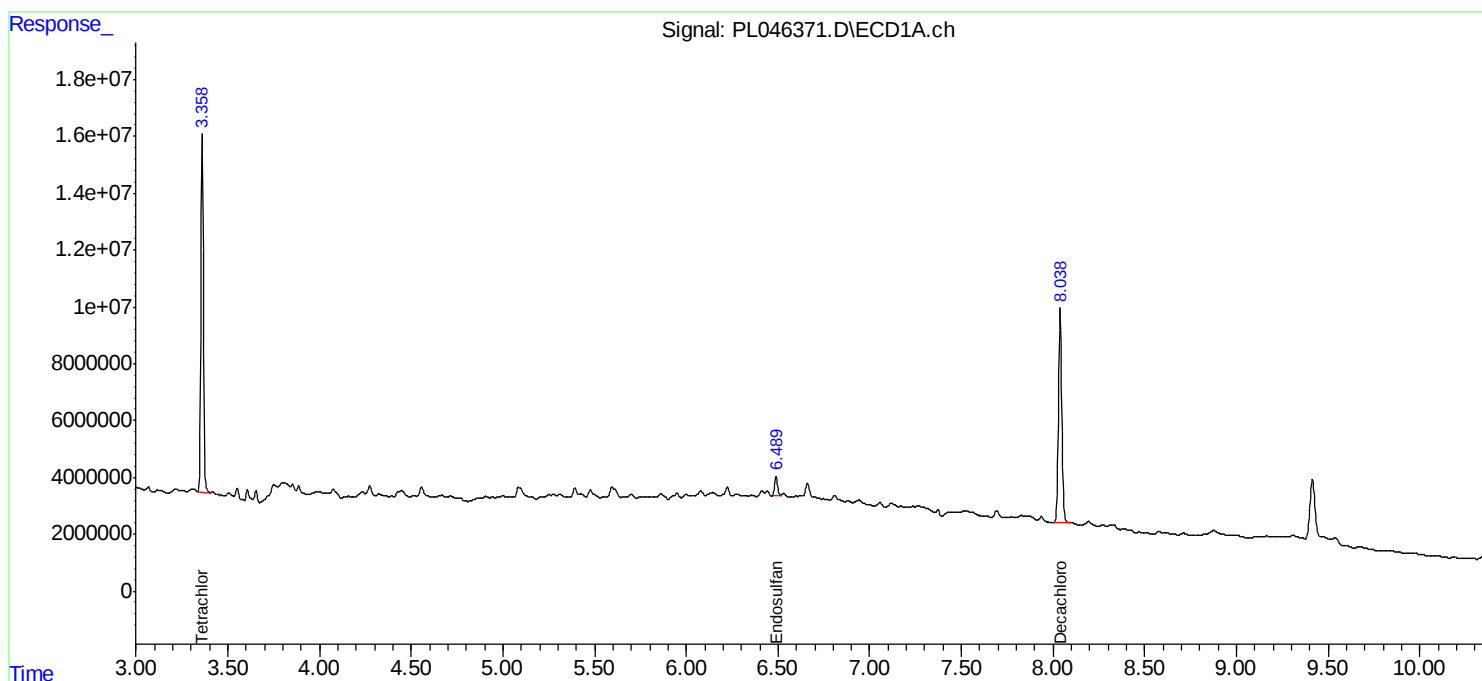


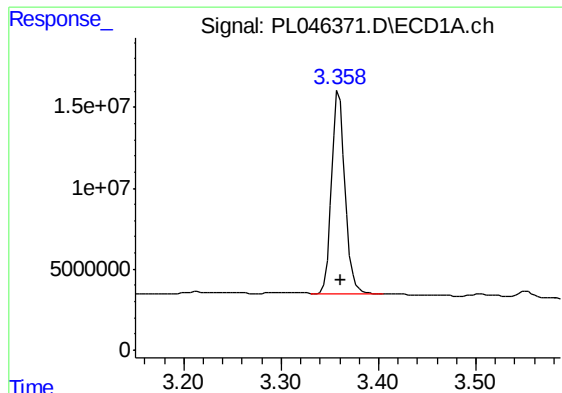

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 121193747
Conc: 16.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-026-SW075-031819

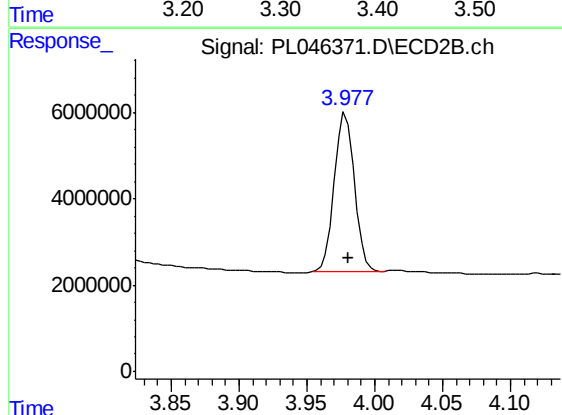


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 37615525
Conc: 16.43 ng/ml

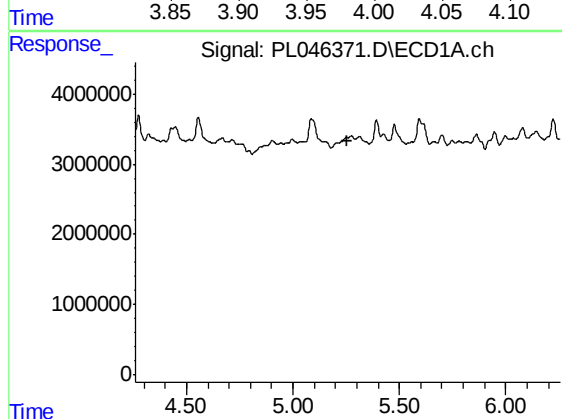


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

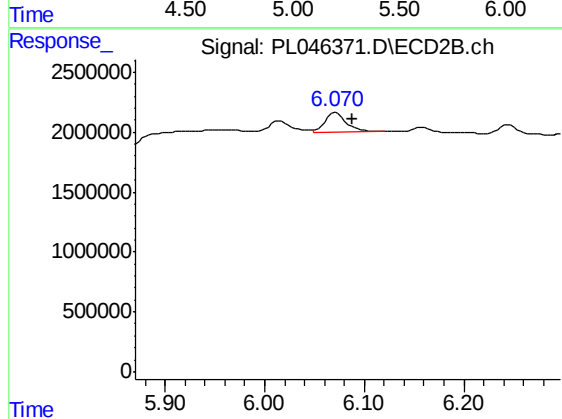

#10 gamma-Chlordane


R.T.: 6.072 min
Delta R.T.: -0.016 min
Response: 2359710
Conc: 0.83 ng/ml

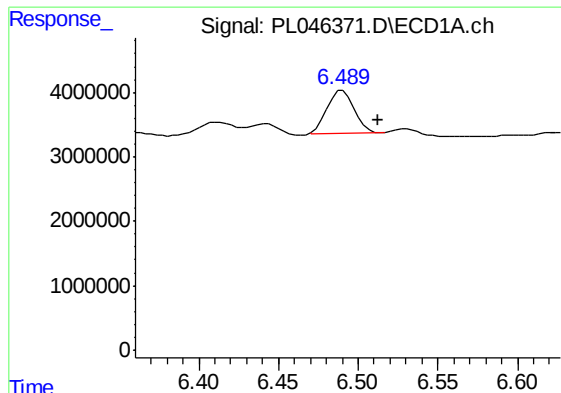

#19 Endosulfan Sulfate


R.T.: 6.490 min
Delta R.T.: -0.022 min
Response: 7974220
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-026-SW075-031819

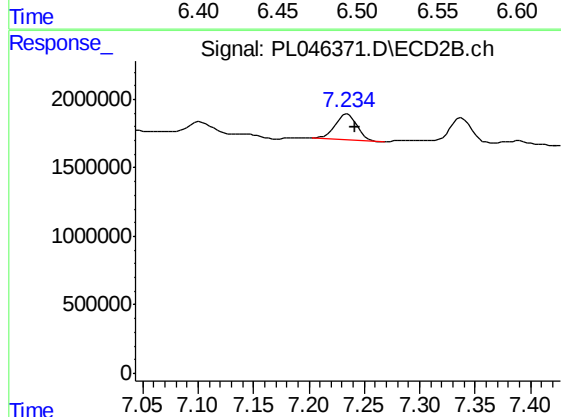


#19 Endosulfan Sulfate

R.T.: 7.235 min
Delta R.T.: -0.007 min
Response: 2672290
Conc: 1.13 ng/ml

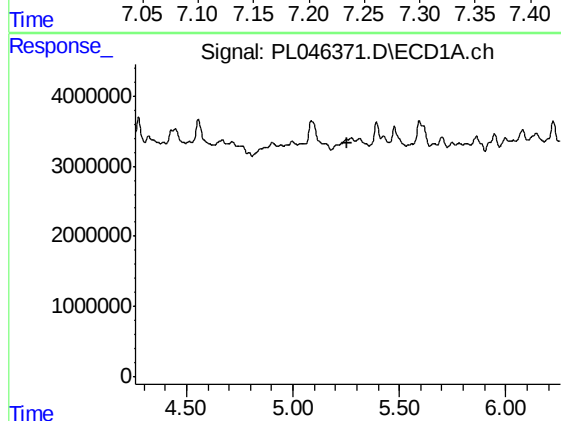


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

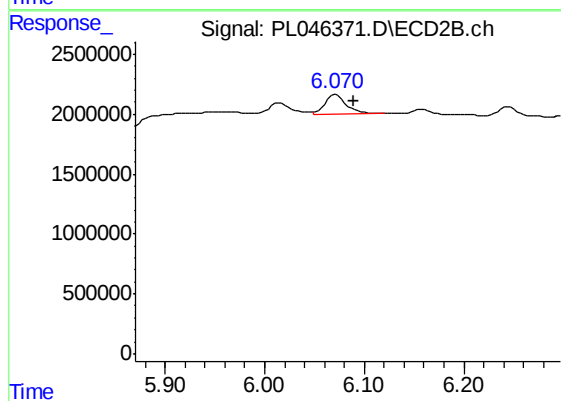

#25 Chlordane-3


R.T.: 6.072 min
Delta R.T.: -0.017 min
Response: 2359710
Conc: 6.19 ng/ml

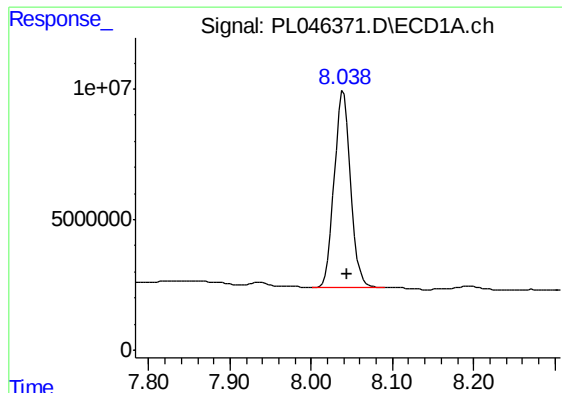

#28 Decachlorobiphenyl

R.T.: 8.039 min
Delta R.T.: -0.005 min
Response: 105511738
Conc: 12.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-026-SW075-031819

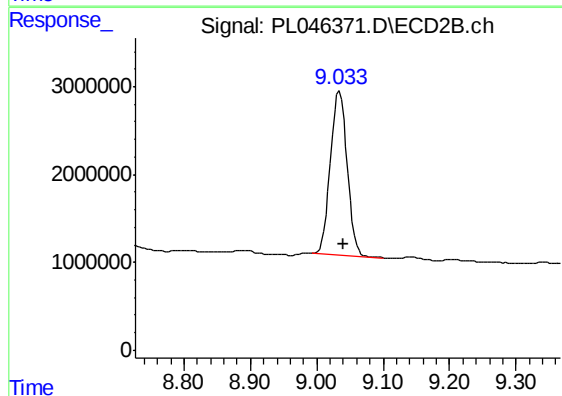

#28 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: -0.006 min
Response: 32922284
Conc: 14.20 ng/ml