

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032319\
 Data File : PL046386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2019 22:21
 Operator : AJ\SJ
 Sample : K2014-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-026-B121-031919

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 04:38:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.978	114.1E6	34936160	15.685	15.259
28)	SA Decachlor...	8.038	9.033	92578777	27711932	11.007	11.953
Target Compounds							
9)	A Endosulfan I	5.392f	0.000	4687883	0	0.499	N.D. #
10)	B gamma-Chl...	0.000	6.070f	0	3037080	N.D.	1.070 #
25)	Chlordane-3	0.000	6.070f	0	3037080	N.D.	7.966 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032319\
Data File : PL046386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2019 22:21
Operator : AJ\SJ
Sample : K2014-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-026-B121-031919

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 04:38:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

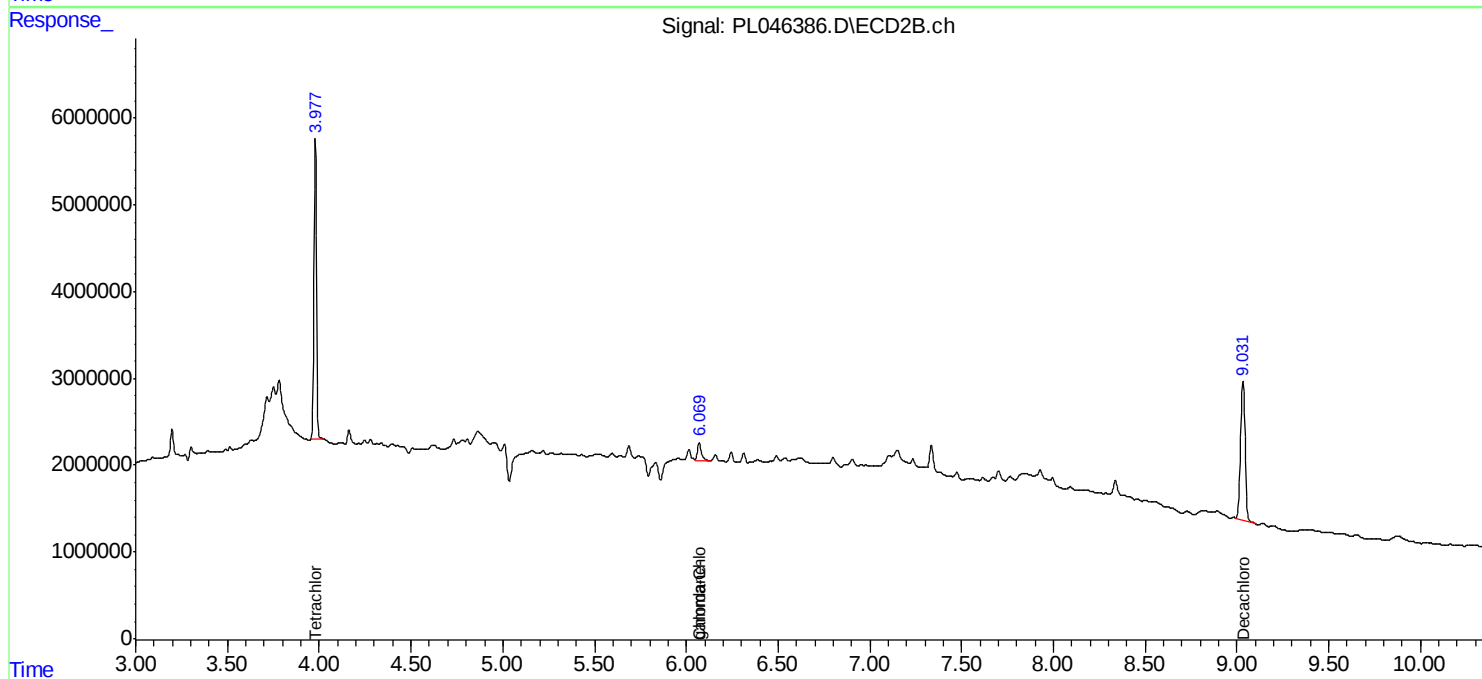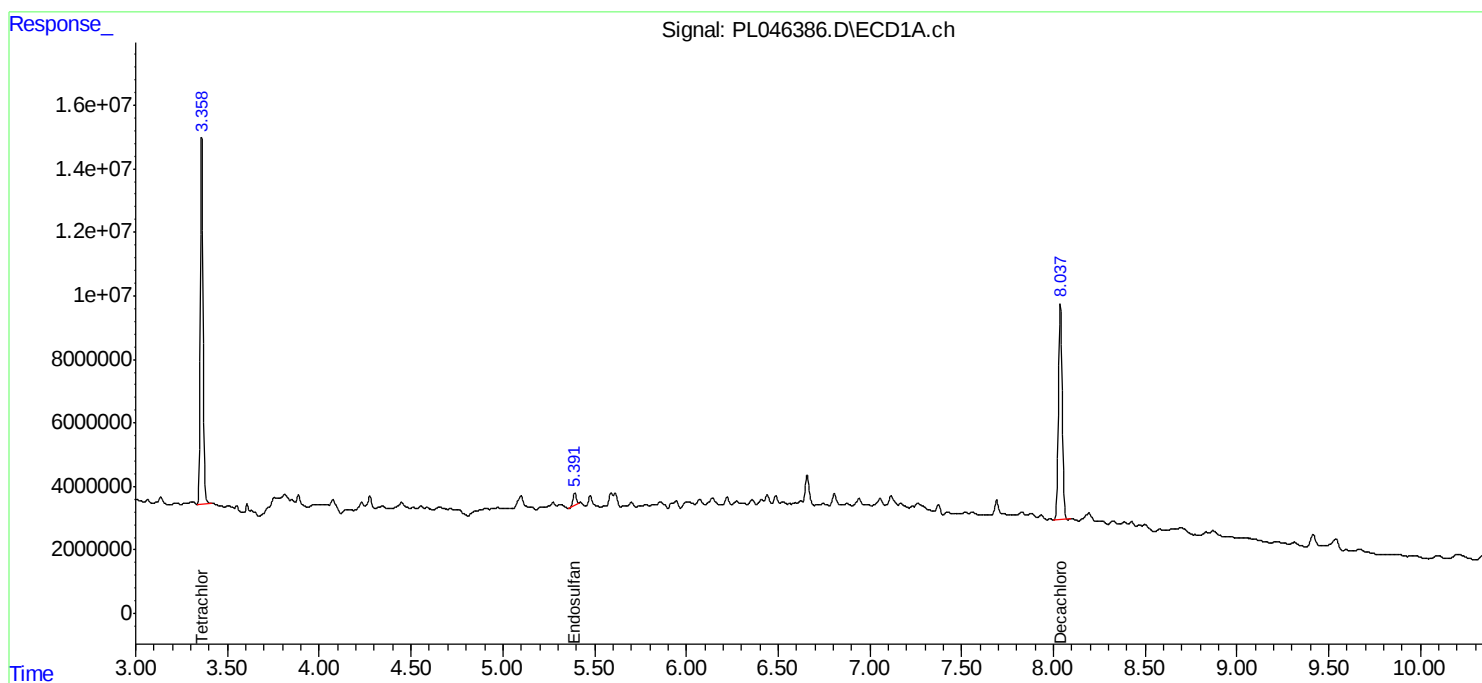


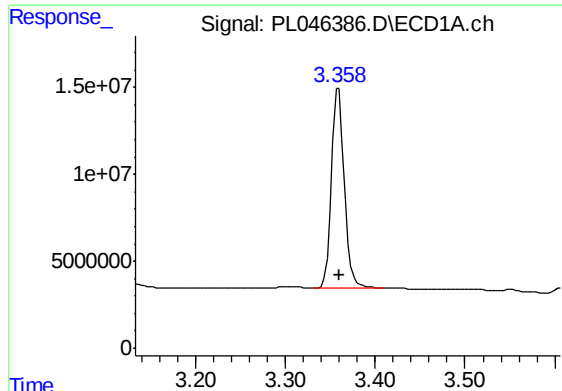

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 114102253
Conc: 15.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-026-B121-031919

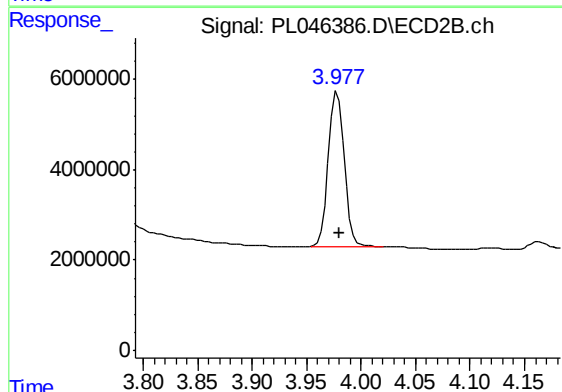


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.002 min
Response: 34936160
Conc: 15.26 ng/ml

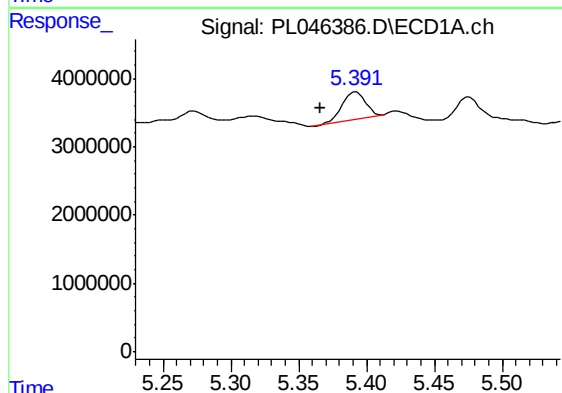


#9 Endosulfan I

R.T.: 5.392 min
Delta R.T.: 0.026 min
Response: 4687883
Conc: 0.50 ng/ml

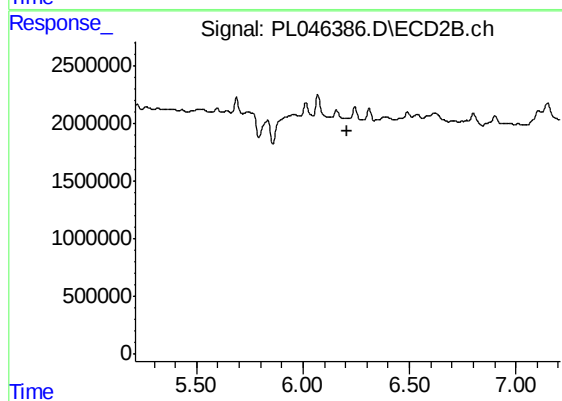

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

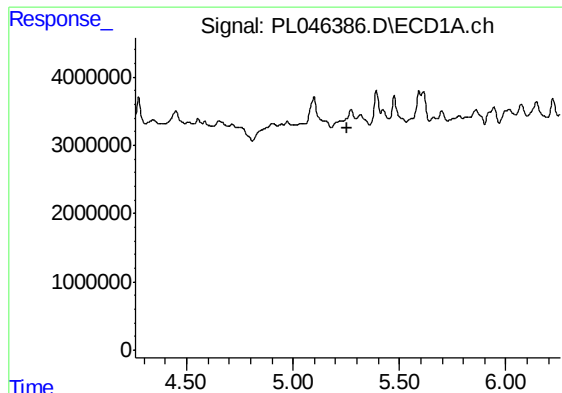

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-026-B121-031919

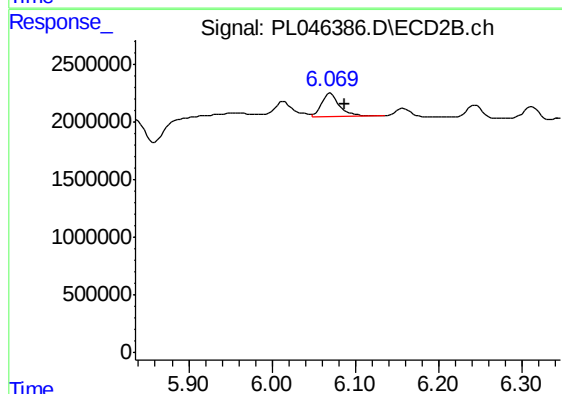


#10 gamma-Chlordane

R.T.: 6.070 min
Delta R.T.: -0.017 min
Response: 3037080
Conc: 1.07 ng/ml

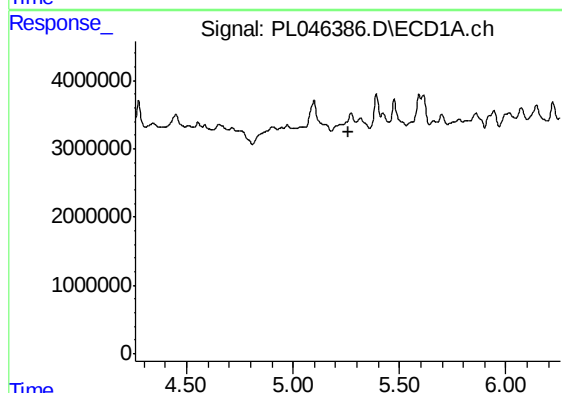


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

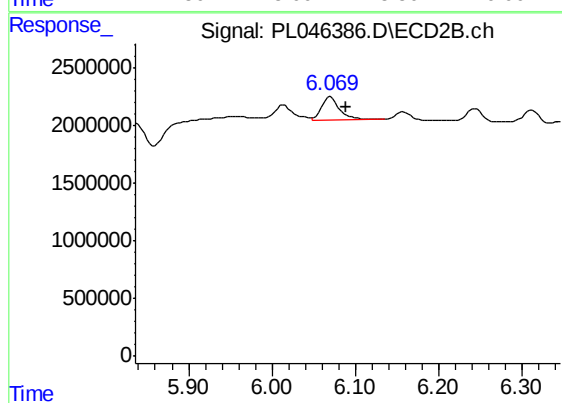

#25 Chlordane-3


R.T.: 6.070 min
Delta R.T.: -0.019 min
Response: 3037080
Conc: 7.97 ng/ml

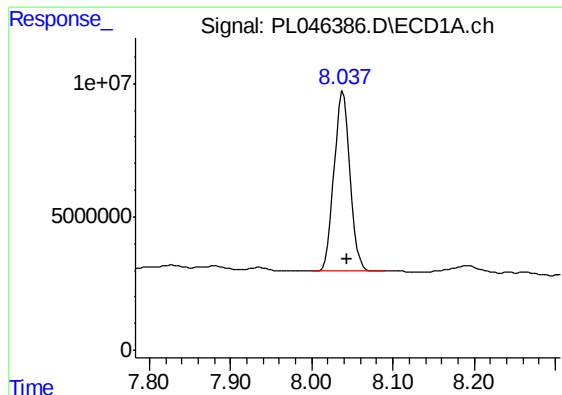

#28 Decachlorobiphenyl

R.T.: 8.038 min
Delta R.T.: -0.006 min
Response: 92578777
Conc: 11.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-026-B121-031919

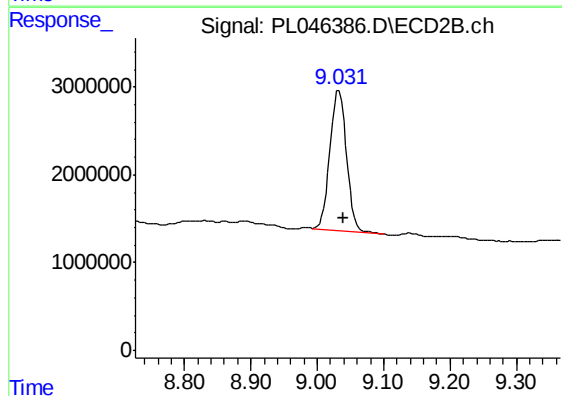

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: -0.007 min
Response: 27711932
Conc: 11.95 ng/ml