

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032319\
 Data File : PL046419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2019 06:55
 Operator : AJ\SJ
 Sample : K2015-14
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-025-B029-031919

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 04:46:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.978	68538722	22088110	9.422	9.647
28)	SA Decachlor...	8.037	9.031	75803466	24293220	9.012	10.478
Target Compounds							
10)	B gamma-Chl...	0.000	6.084	0	1452919	N.D.	0.512 #
12)	B 4,4'-DDE	5.477	6.309	4846543	1922204	0.526	0.774 #
25)	Chlordane-3	0.000	6.084	0	1452919	N.D.	3.811 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032319\
Data File : PL046419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2019 06:55
Operator : AJ\SJ
Sample : K2015-14
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-025-B029-031919

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 04:46:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

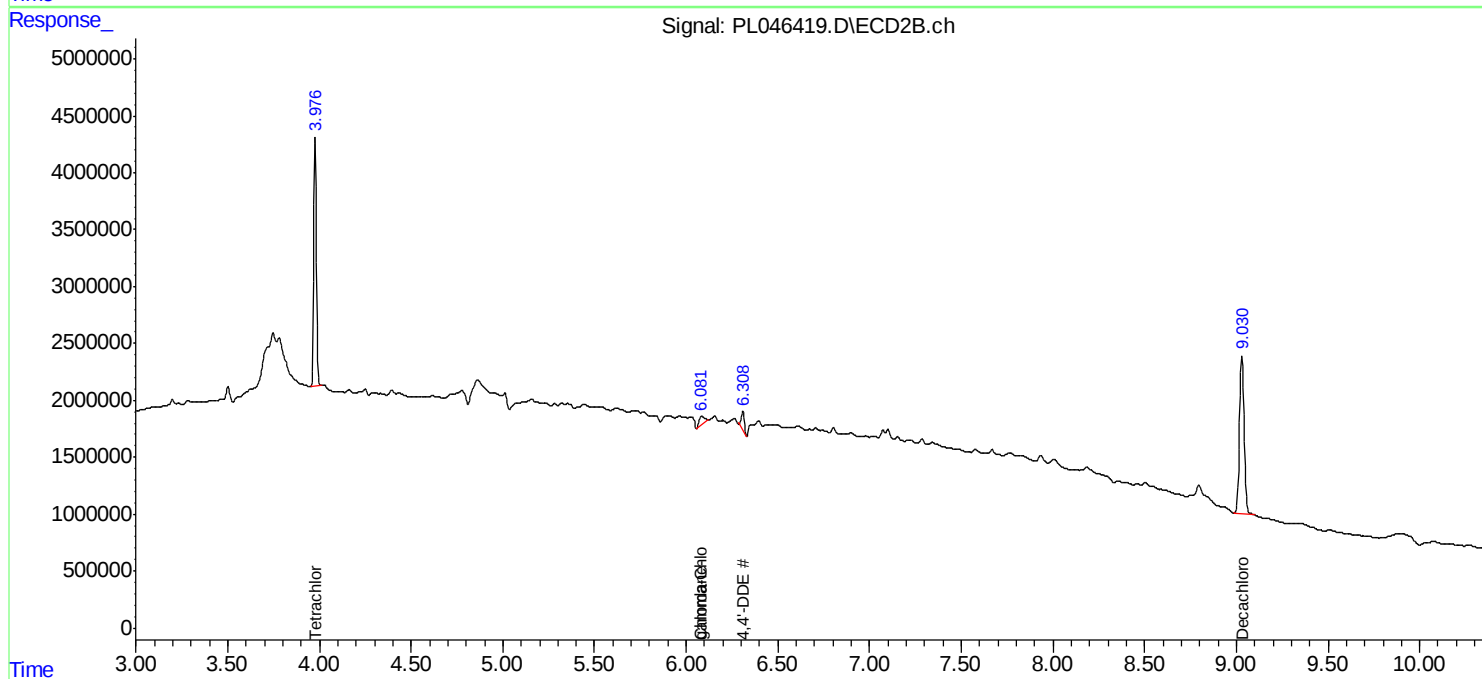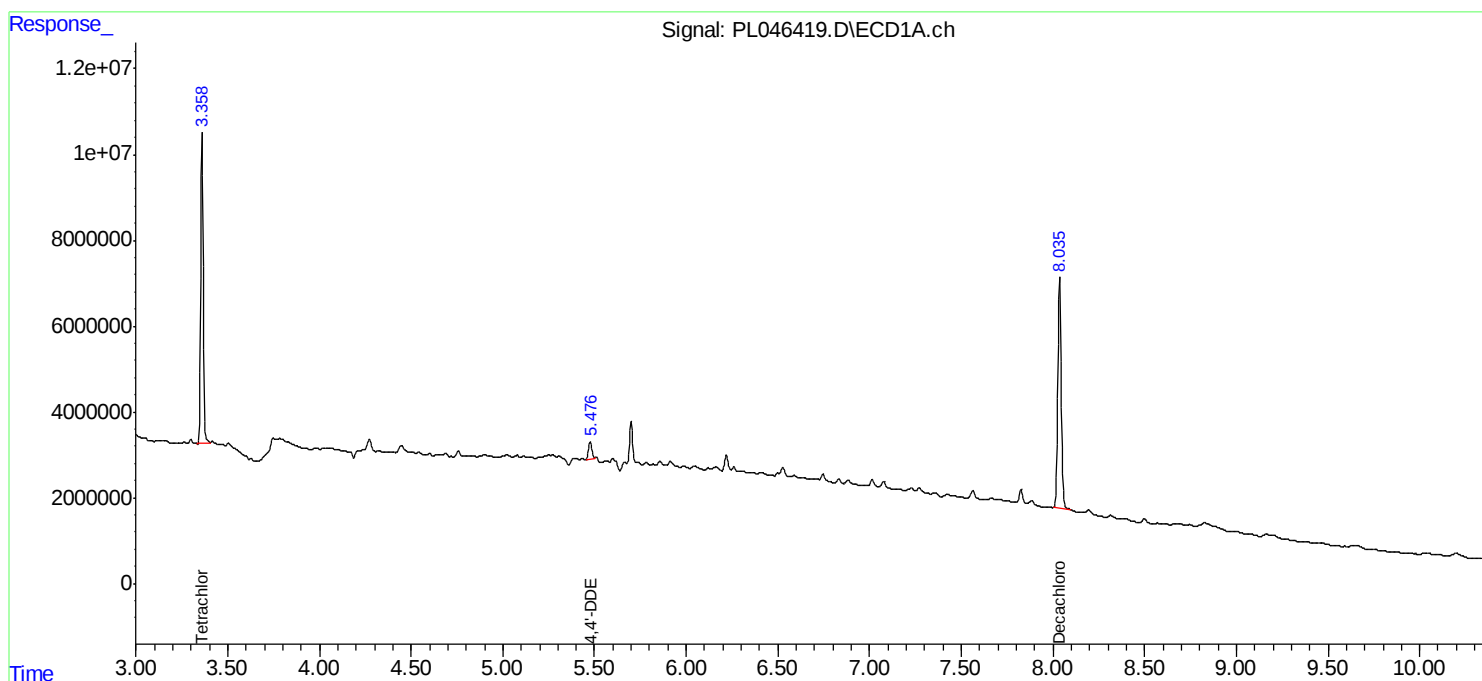


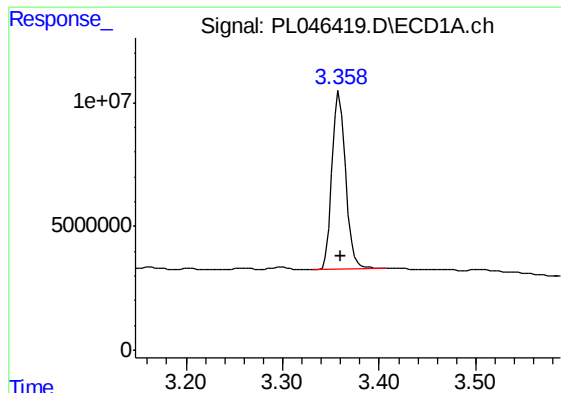

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 68538722
Conc: 9.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-025-B029-031919

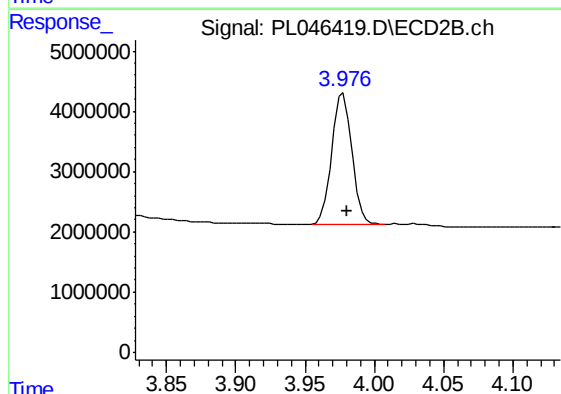


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 22088110
Conc: 9.65 ng/ml

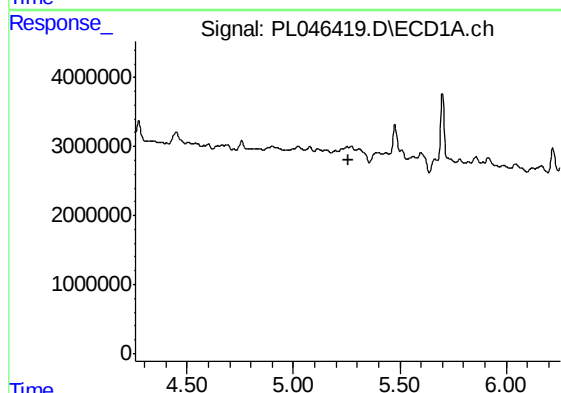


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

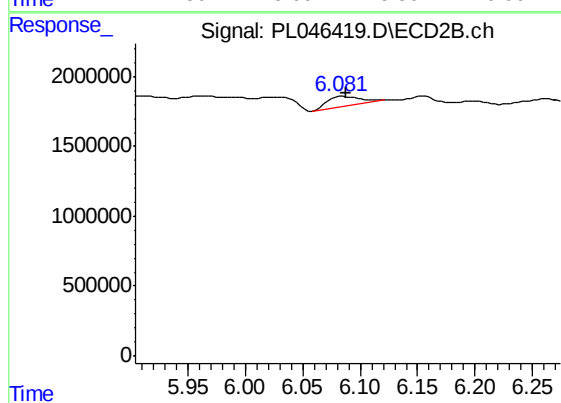

#10 gamma-Chlordane


R.T.: 6.084 min
Delta R.T.: -0.004 min
Response: 1452919
Conc: 0.51 ng/ml

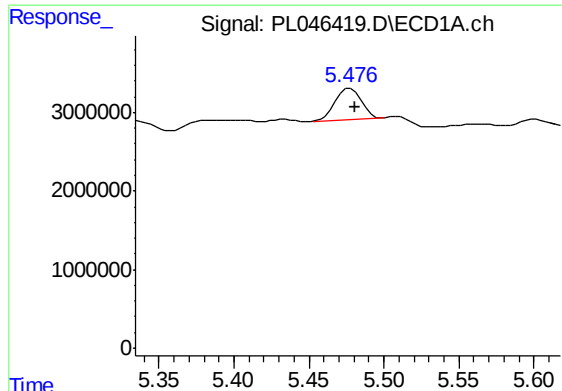

#12 4,4'-DDE


R.T.: 5.477 min
Delta R.T.: -0.003 min
Response: 4846543
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-025-B029-031919

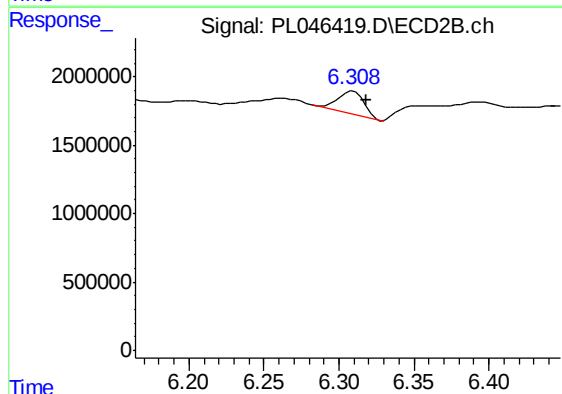


#12 4,4'-DDE

R.T.: 6.309 min
Delta R.T.: -0.009 min
Response: 1922204
Conc: 0.77 ng/ml

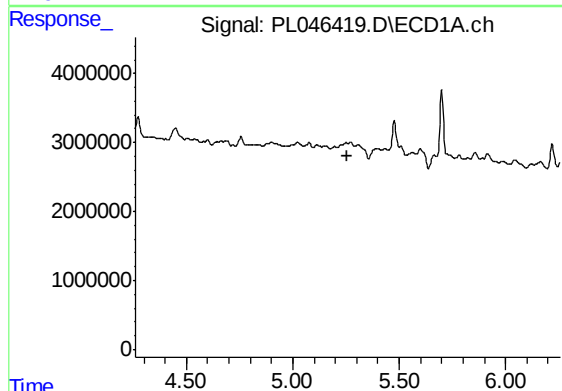


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

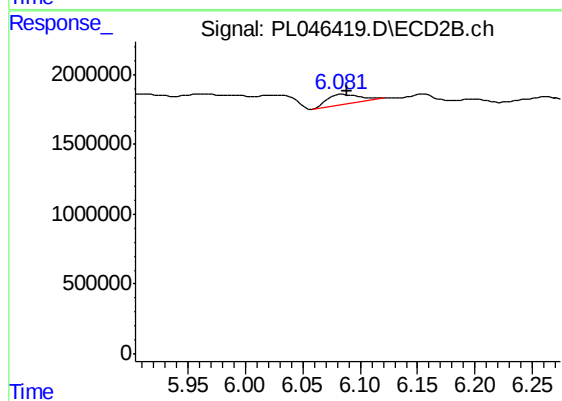

#25 Chlordane-3


R.T.: 6.084 min
Delta R.T.: -0.005 min
Response: 1452919
Conc: 3.81 ng/ml

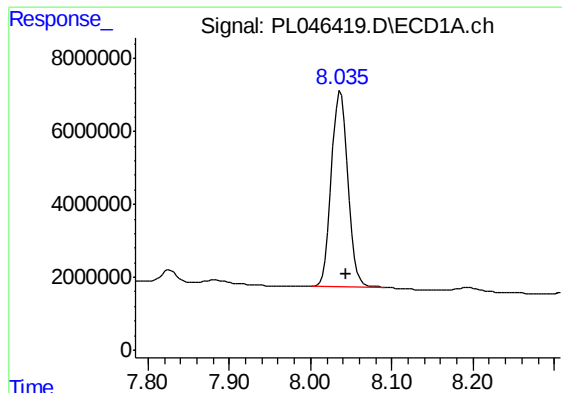

#28 Decachlorobiphenyl

R.T.: 8.037 min
Delta R.T.: -0.008 min
Response: 75803466
Conc: 9.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-025-B029-031919

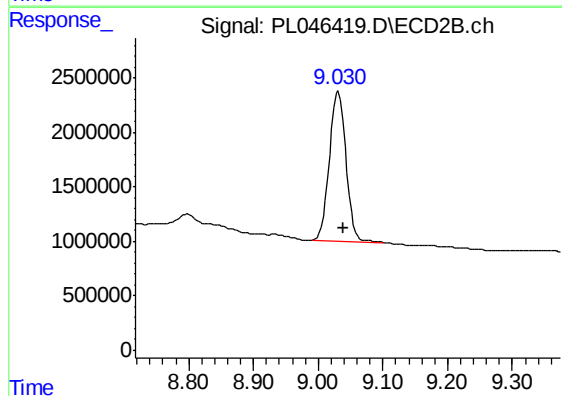

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: -0.009 min
Response: 24293220
Conc: 10.48 ng/ml