

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032319\
 Data File : PL046420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2019 07:10
 Operator : AJ\SJ
 Sample : K2015-15
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-025-B030-031919

Manual Integrations
 APPROVED

Sohil
 3/25/2019 11:32:31 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 04:47:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.359	3.977	69870650	22600237	9.605	9.871
28) SA Decachlor...	8.037	9.030	79487924	25170003	9.450	10.856
Target Compounds						
12) B 4,4'-DDE	5.477	6.311	12766590	3968471	1.387m	1.599m
17) MA 4,4'-DDT	6.220	7.099	17084801	4043983	2.256	1.929m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032319\
Data File : PL046420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2019 07:10
Operator : AJ\SJ
Sample : K2015-15
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PST-025-B030-031919


Manual Integrations
APPROVED

Sohil
3/25/2019 11:32:31 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 04:47:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

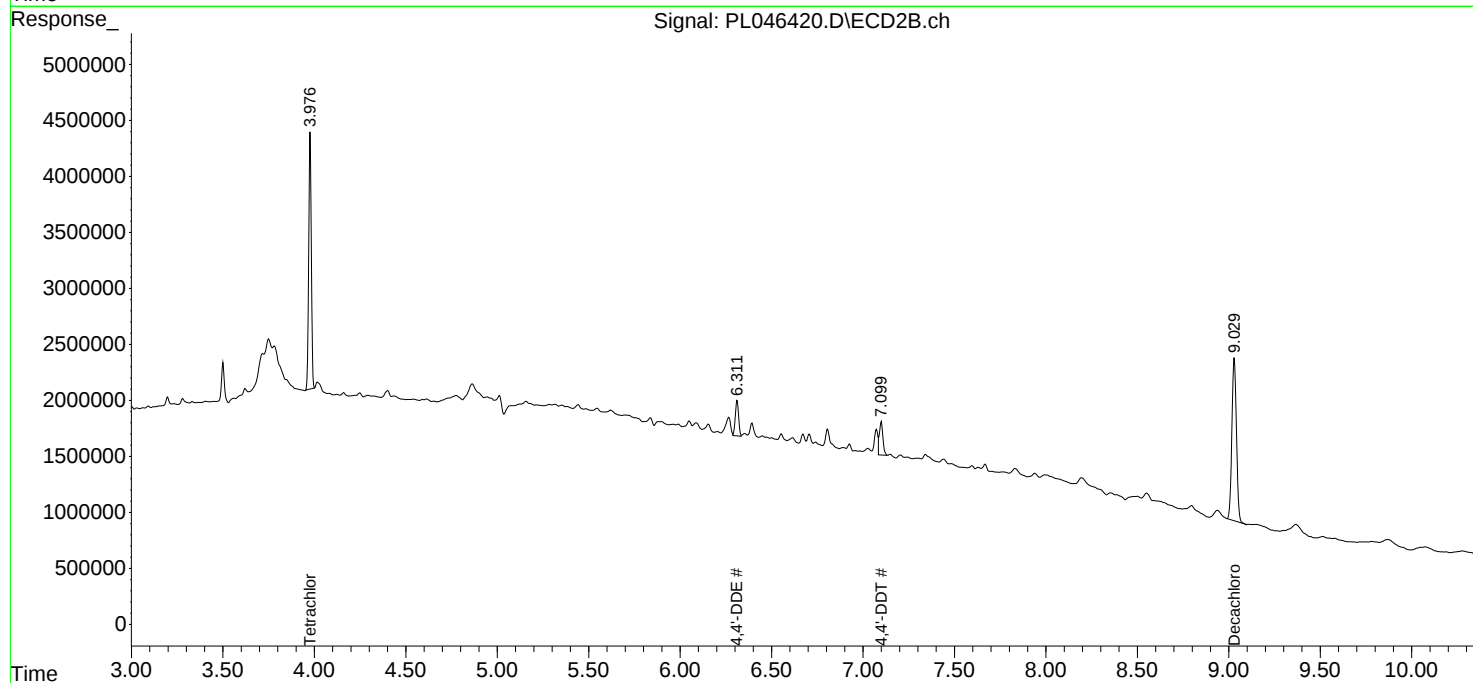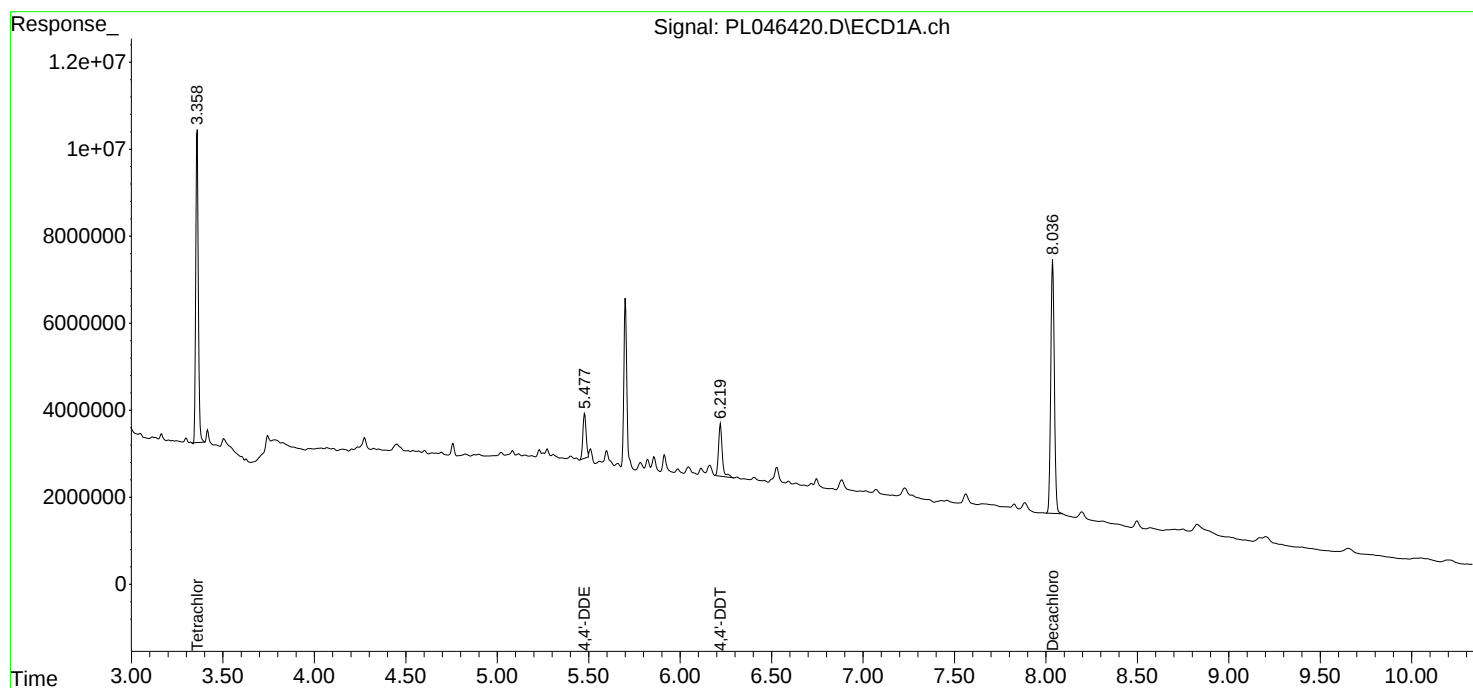

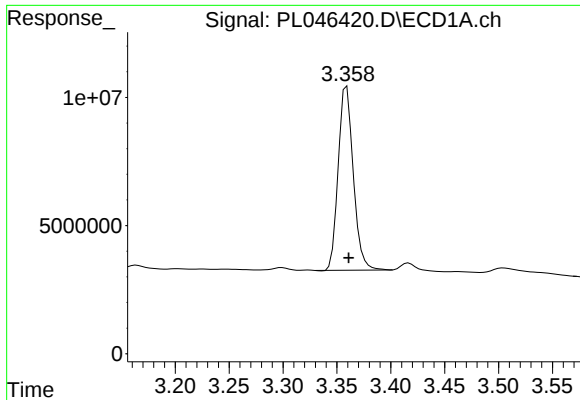


#1 Tetrachloro-m-xylene

R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 69870650
Conc: 9.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-025-B030-031919


Manual Integrations
APPROVED

Sohil
3/25/2019 11:32:31 AM

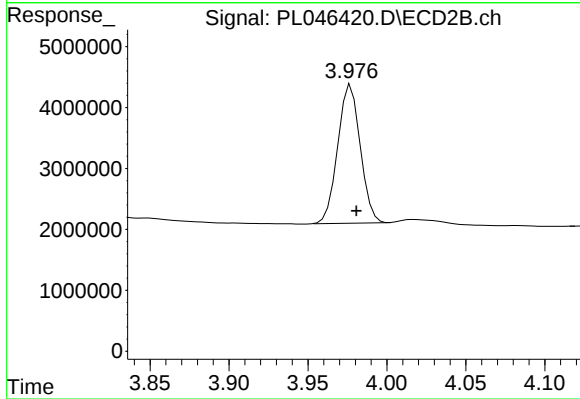


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 22600237
Conc: 9.87 ng/ml

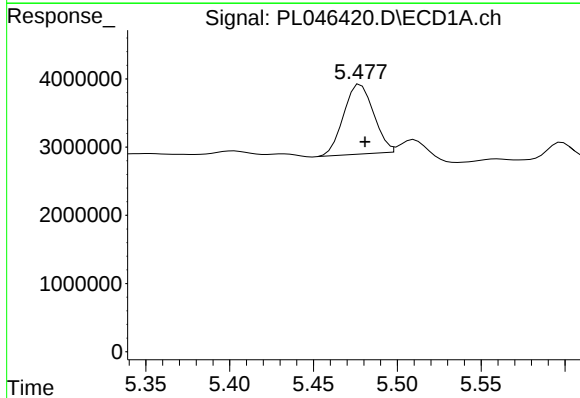


#12 4,4'-DDE

R.T.: 5.477 min
Delta R.T.: -0.004 min
Response: 12766590
Conc: 1.39 ng/ml m

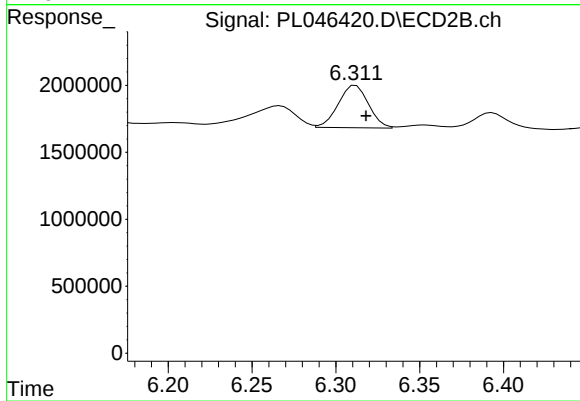

#12 4,4'-DDE

R.T.: 6.311 min
Delta R.T.: -0.007 min
Response: 3968471
Conc: 1.60 ng/ml m

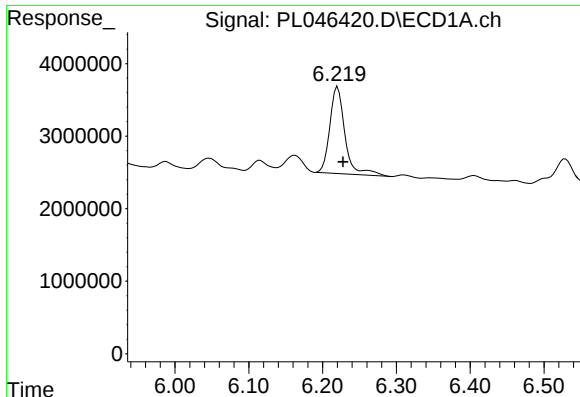


#17 4,4'-DDT

R.T.: 6.220 min
Delta R.T.: -0.007 min
Response: 17084801
Conc: 2.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-025-B030-031919


Manual Integrations
APPROVED

Sohil
3/25/2019 11:32:31 AM

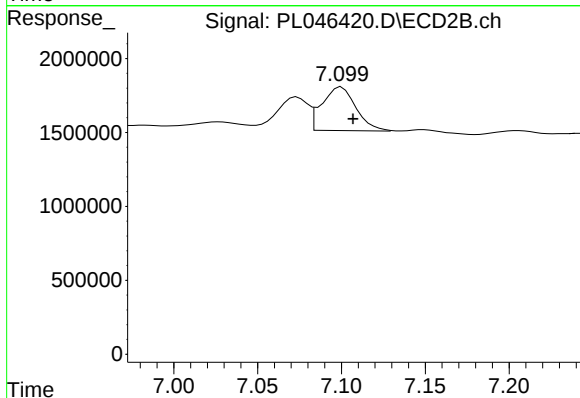


#17 4,4'-DDT

R.T.: 7.099 min
Delta R.T.: -0.008 min
Response: 4043983
Conc: 1.93 ng/ml m

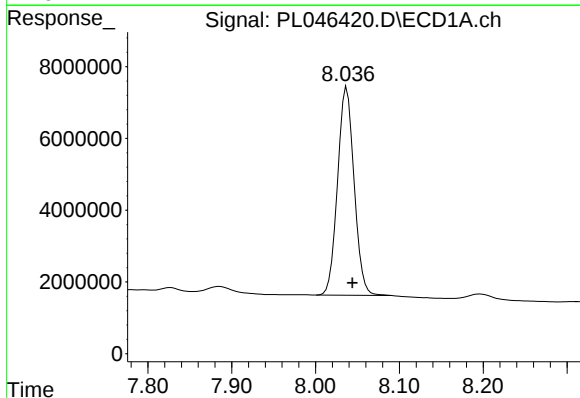

#28 Decachlorobiphenyl

R.T.: 8.037 min
Delta R.T.: -0.007 min
Response: 79487924
Conc: 9.45 ng/ml

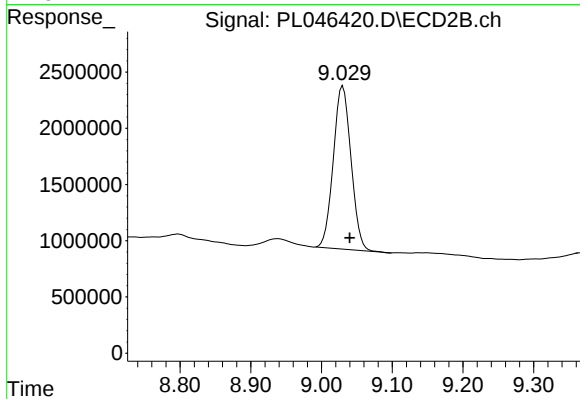

#28 Decachlorobiphenyl

R.T.: 9.030 min
Delta R.T.: -0.010 min
Response: 25170003
Conc: 10.86 ng/ml