

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032320\
 Data File : PL057517.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2020 16:25
 Operator : AJ\MA
 Sample : L1755-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-031920

Manual Integrations
 APPROVED

mohammad
 3/24/2020 3:41:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:42:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.458	3.957	131.4E6	31500740	14.175	14.519
28) SA Decachlor...	8.205	8.979	126.8E6	32824973	11.988	14.804
Target Compounds						
10) B gamma-Chl...	5.397	6.046	56021199	30137477	4.296m	9.778m#
11) B alpha-Chl...	5.454	6.121	144.2E6	86320890	11.155	27.732 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032320\
Data File : PL057517.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2020 16:25
Operator : AJ\MA
Sample : L1755-05
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-01-031920


Manual Integrations
APPROVED

mohammad
3/24/2020 3:41:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:42:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

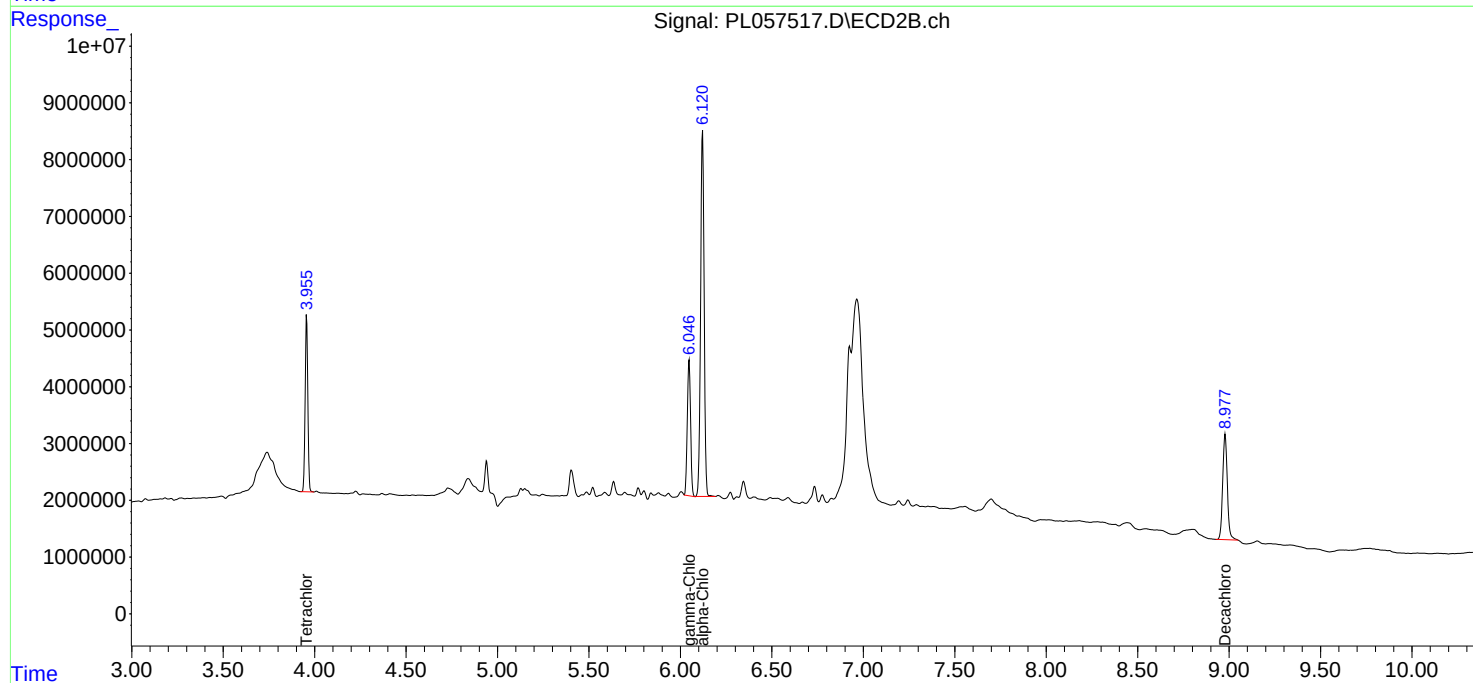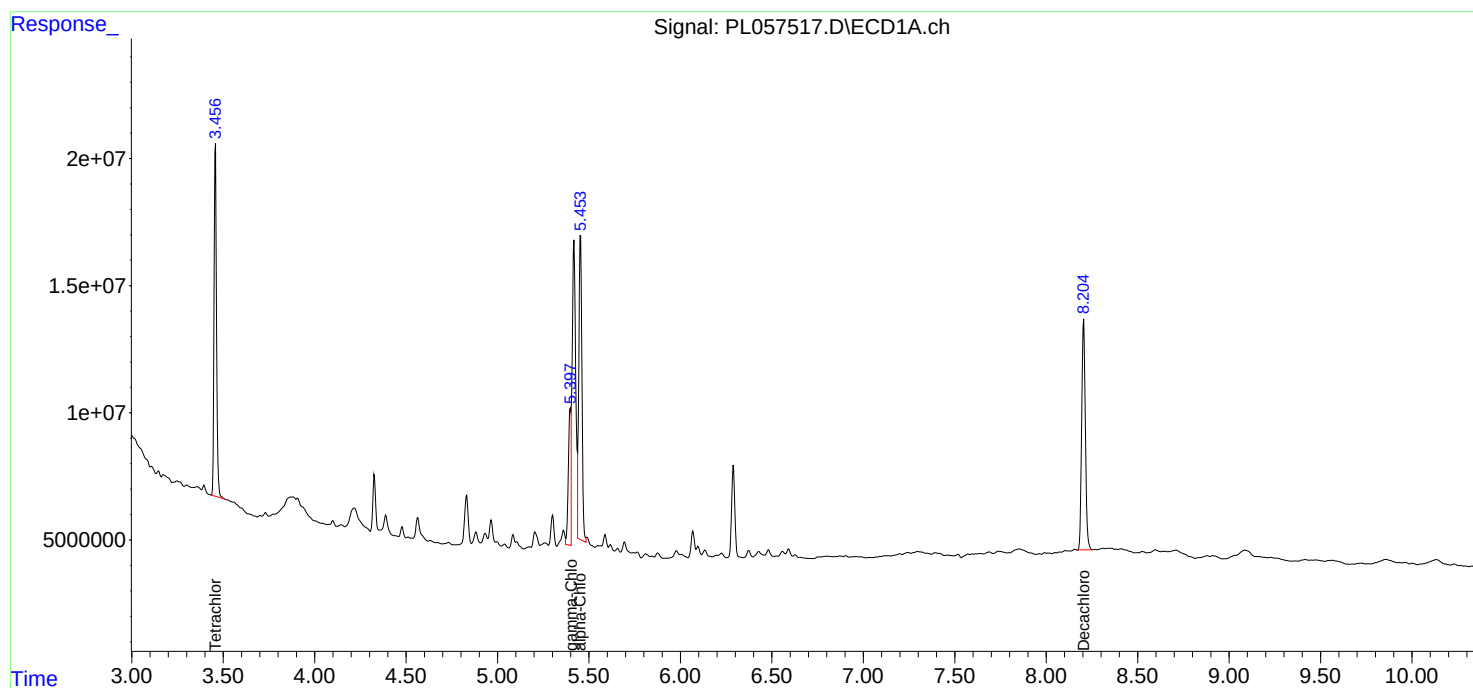

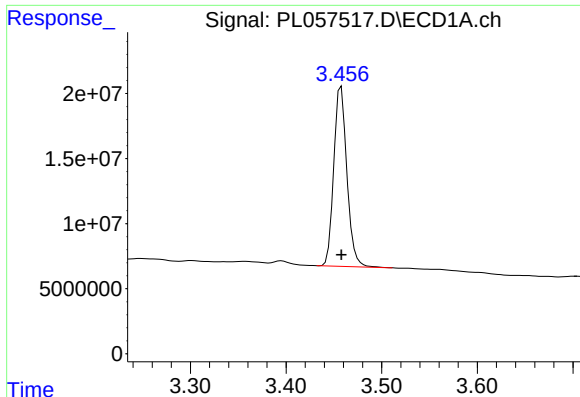


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 131395250
Conc: 14.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-031920


Manual Integrations
APPROVED

mohammad
3/24/2020 3:41:54 PM

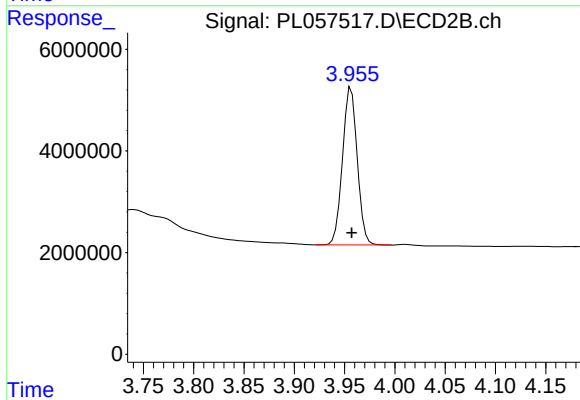


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 31500740
Conc: 14.52 ng/ml

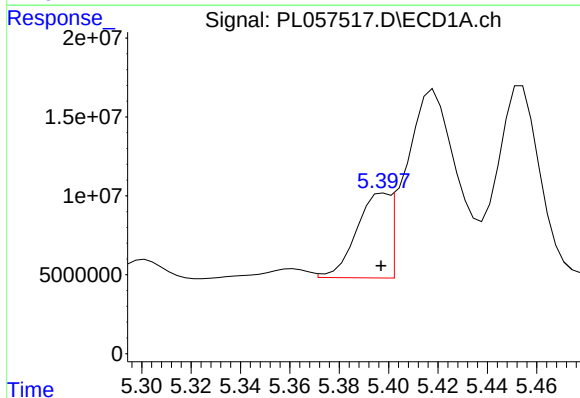


#10 gamma-Chlordane

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 56021199
Conc: 4.30 ng/ml m

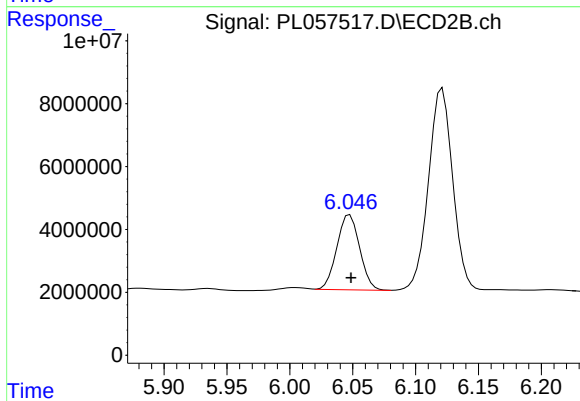

#10 gamma-Chlordane

R.T.: 6.046 min
Delta R.T.: -0.002 min
Response: 30137477
Conc: 9.78 ng/ml m

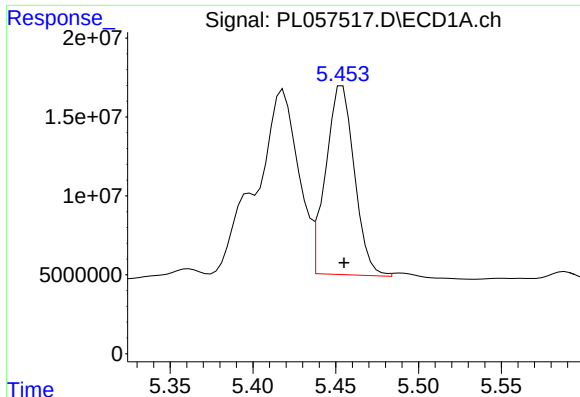


#11 alpha-Chlordane

R.T.: 5.454 min
Delta R.T.: -0.001 min
Response: 144151506
Conc: 11.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-031920


Manual Integrations
APPROVED

mohammad
3/24/2020 3:41:54 PM

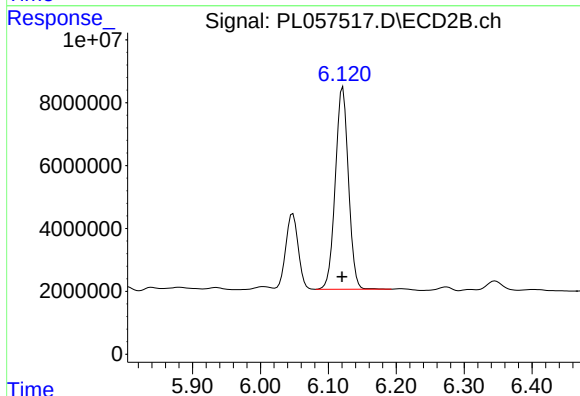


#11 alpha-Chlordane

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 86320890
Conc: 27.73 ng/ml

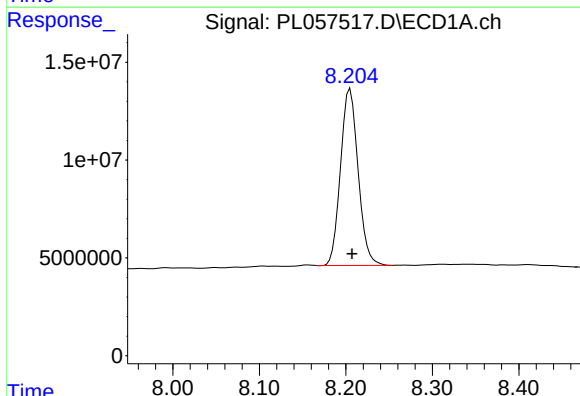

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 126848963
Conc: 11.99 ng/ml

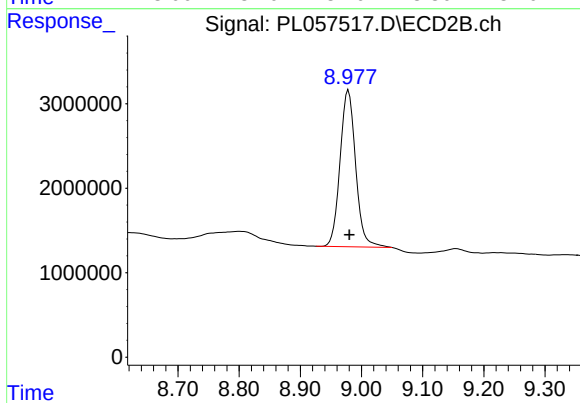

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: -0.001 min
Response: 32824973
Conc: 14.80 ng/ml