

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032320\
 Data File : PL057518.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2020 16:39
 Operator : AJ\MA
 Sample : L1762-18
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-031920

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:42:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.458	3.956	131.4E6	30935538	14.174	14.259
28)	SA Decachlor...	8.205	8.978	132.8E6	34273862	12.554	15.457
Target Compounds							
12)	B 4,4'-DDE	5.617	6.277	12987479	3326430	1.043	1.170



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032320\
Data File : PL057518.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2020 16:39
Operator : AJ\MA
Sample : L1762-18
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-05-031920

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:42:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

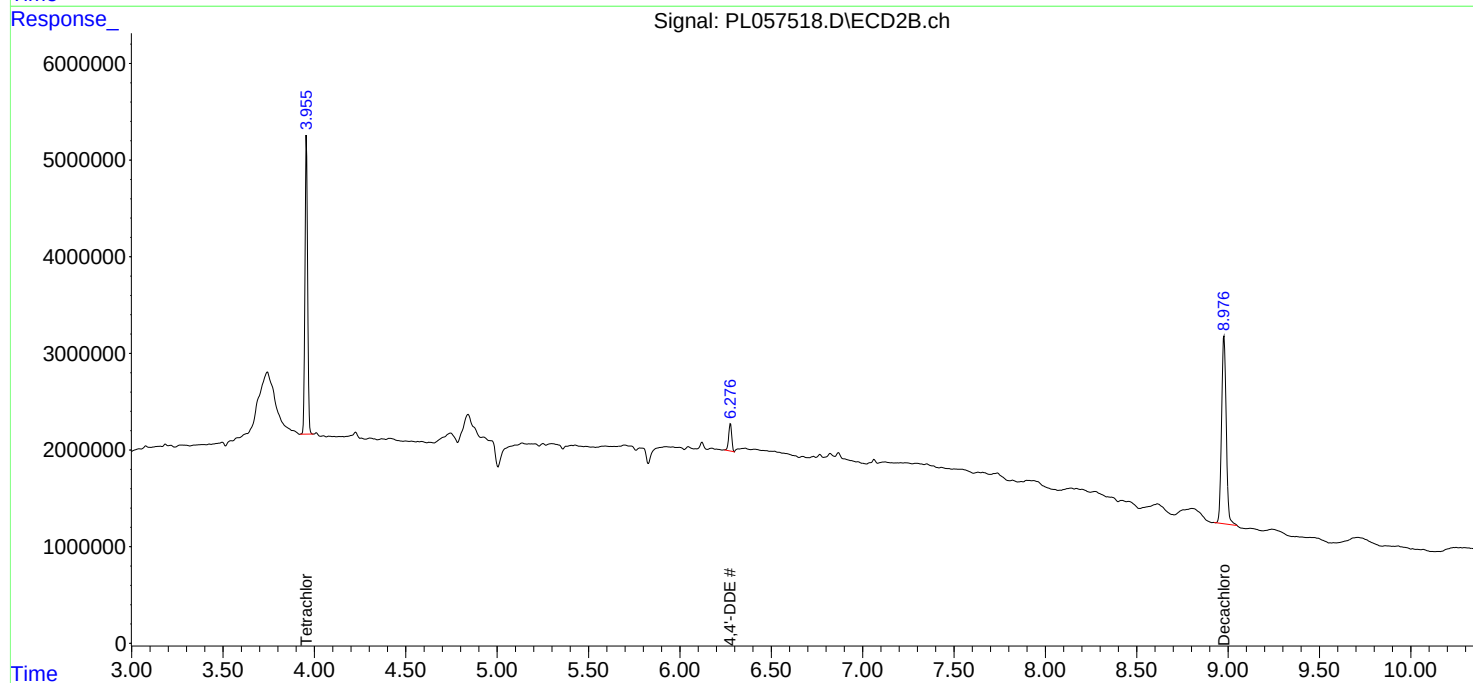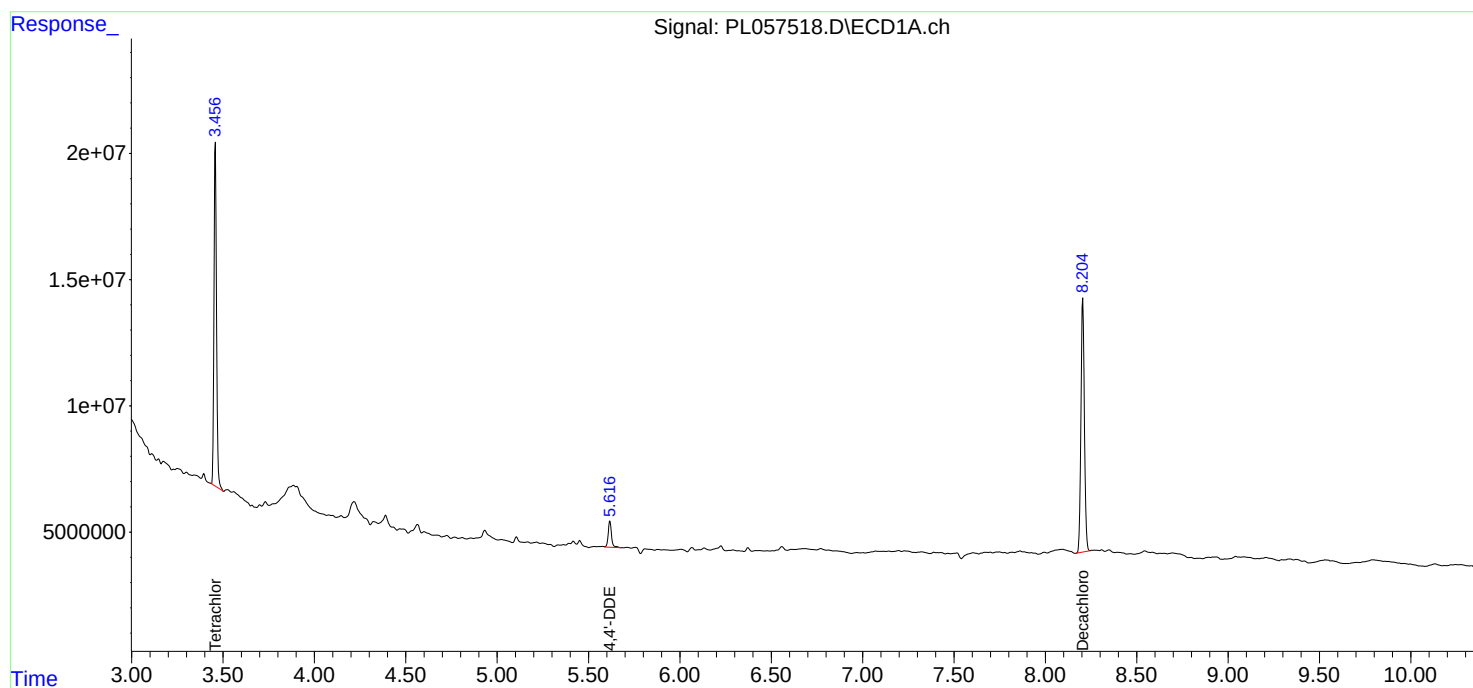


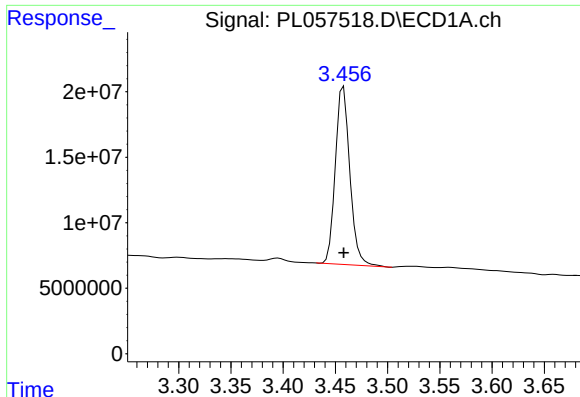

#1 Tetrachloro-m-xylene


R.T.: 3.458 min
Delta R.T.: 0.000 min
Response: 131380595
Conc: 14.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-031920

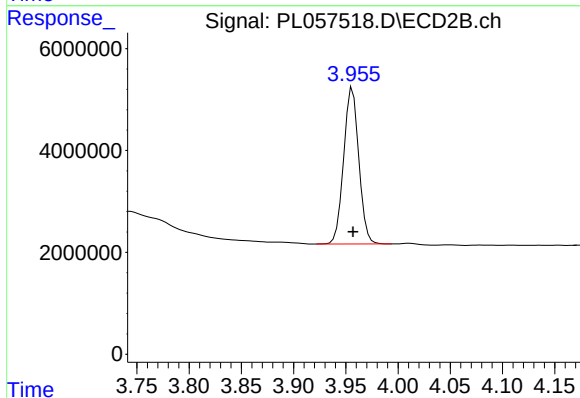


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: 0.000 min
Response: 30935538
Conc: 14.26 ng/ml

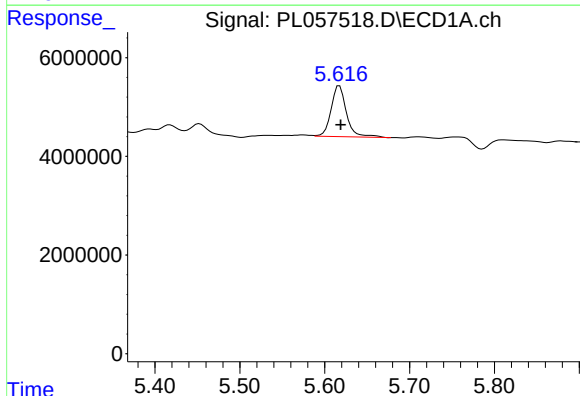


#12 4,4'-DDE

R.T.: 5.617 min
Delta R.T.: -0.002 min
Response: 12987479
Conc: 1.04 ng/ml

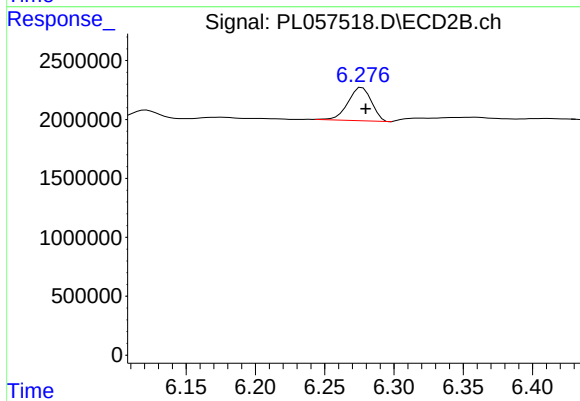

#12 4,4'-DDE

R.T.: 6.277 min
Delta R.T.: -0.003 min
Response: 3326430
Conc: 1.17 ng/ml

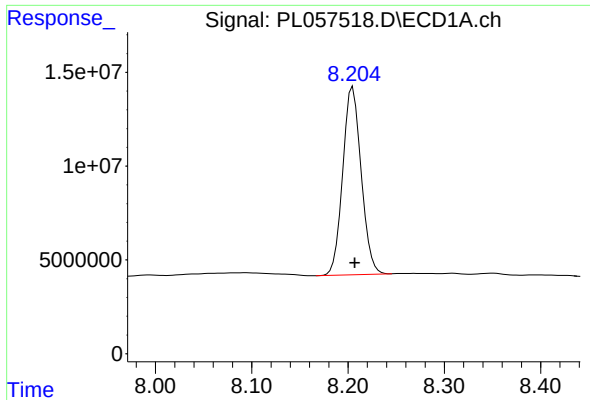

#28 Decachlorobiphenyl


R.T.: 8.205 min

Delta R.T.: -0.002 min

Response: 132833340

Conc: 12.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-031920

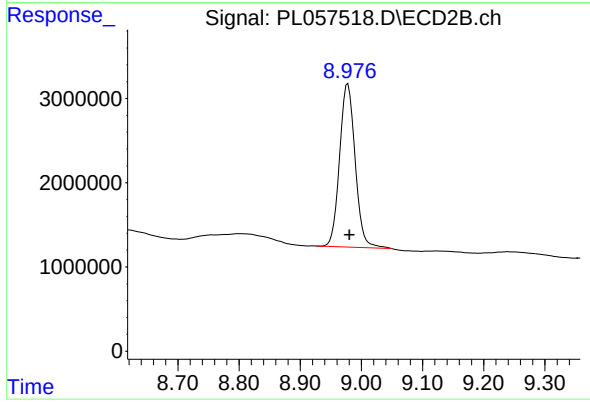

#28 Decachlorobiphenyl

R.T.: 8.978 min

Delta R.T.: -0.002 min

Response: 34273862

Conc: 15.46 ng/ml