

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032321\
 Data File : PL065495.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2021 13:32
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:12:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.785	132.7E6	121.7E6	55.874	44.351
28)	SA Decachlor...	7.925	8.734	109.7E6	96087124	45.385	48.477
Target Compounds							
23)	Chlordane-1	4.122	4.749	45951346	48178099	533.390	427.146
24)	Chlordane-2	4.609	5.212	53511906	48310093	493.375	443.566
25)	Chlordane-3	5.160	5.848	141.5E6	175.5E6	474.103	430.497
26)	Chlordane-4	5.215	5.919	132.3E6	209.1E6	485.565	434.563
27)	Chlordane-5	6.028	6.716	46557673	35169930	465.682	439.523



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032321\
Data File : PL065495.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2021 13:32
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:12:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

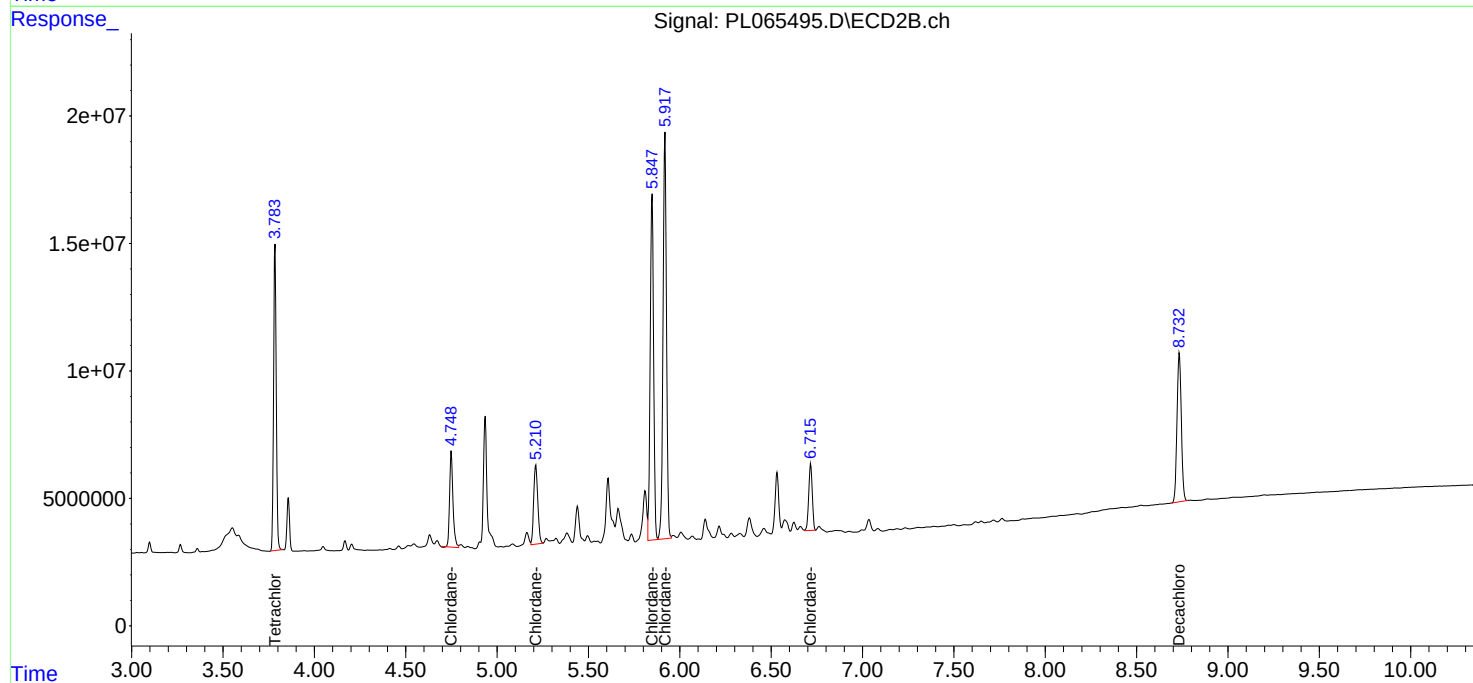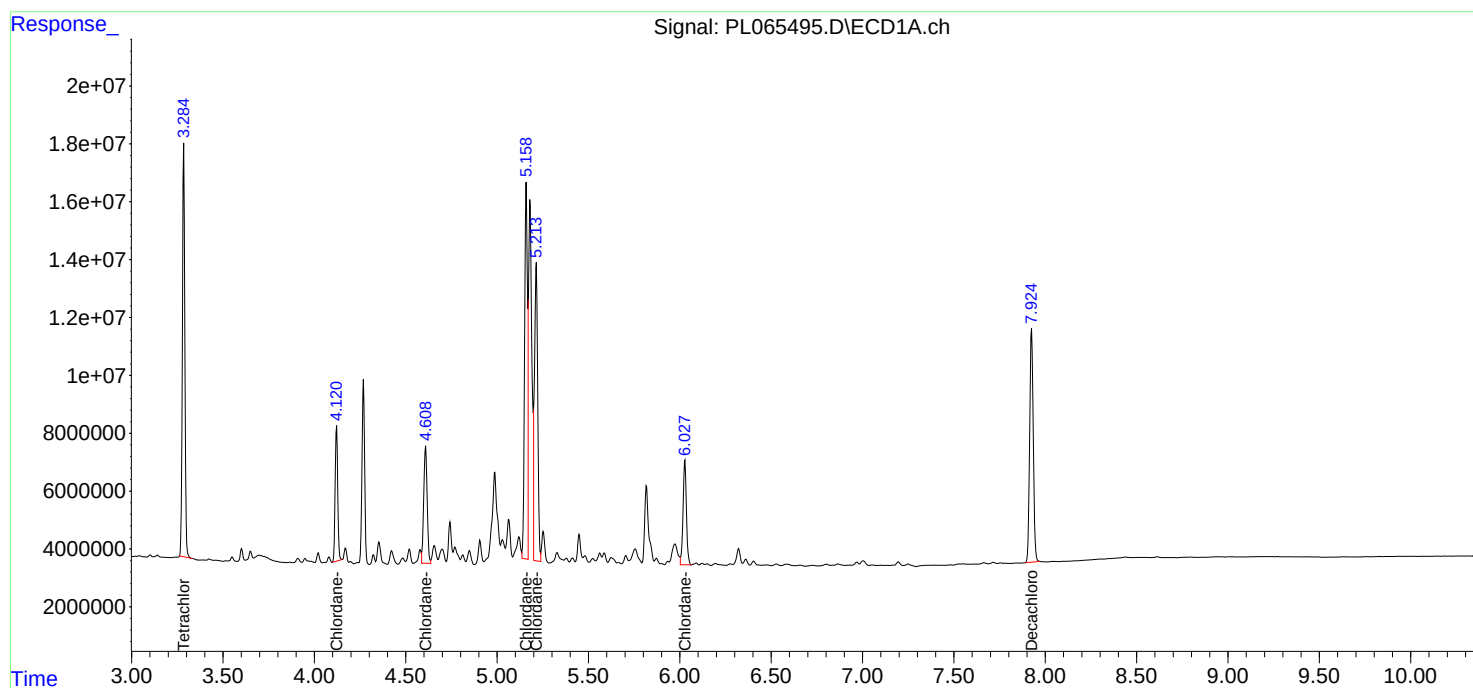


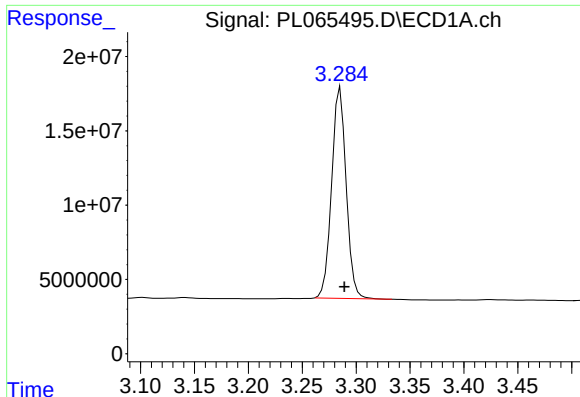

#1 Tetrachloro-m-xylene


R.T.: 3.285 min
Delta R.T.: -0.004 min
Response: 132689724
Conc: 55.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

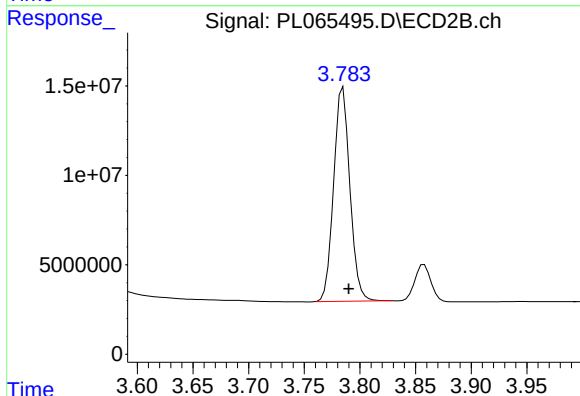


#1 Tetrachloro-m-xylene

R.T.: 3.785 min
Delta R.T.: -0.005 min
Response: 121730989
Conc: 44.35 ng/ml

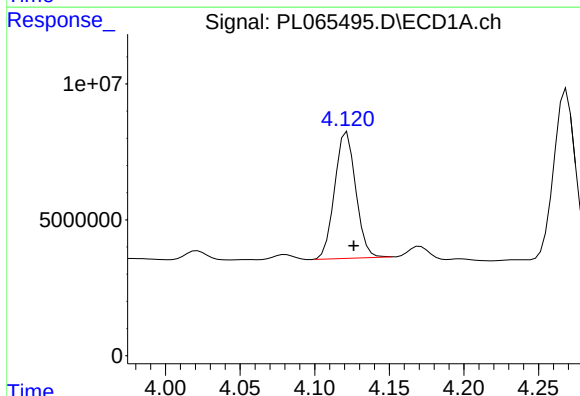


#23 Chlordane-1

R.T.: 4.122 min
Delta R.T.: -0.005 min
Response: 45951346
Conc: 533.39 ng/ml

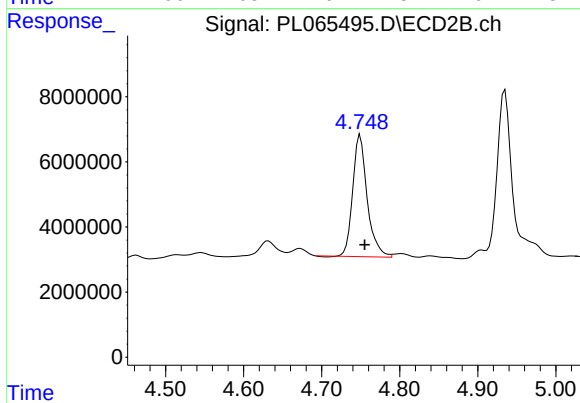

#23 Chlordane-1


R.T.: 4.749 min
Delta R.T.: -0.006 min
Response: 48178099
Conc: 427.15 ng/ml

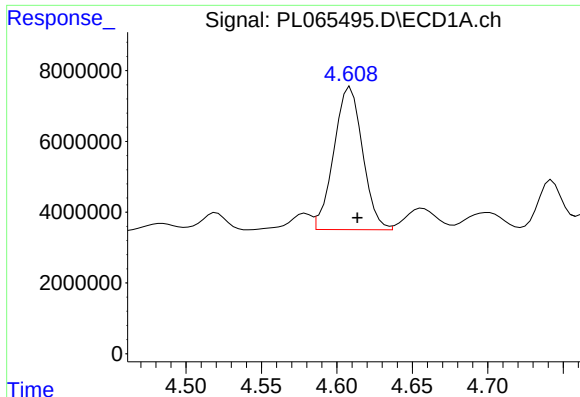

#24 Chlordane-2


R.T.: 4.609 min
Delta R.T.: -0.005 min
Response: 53511906
Conc: 493.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

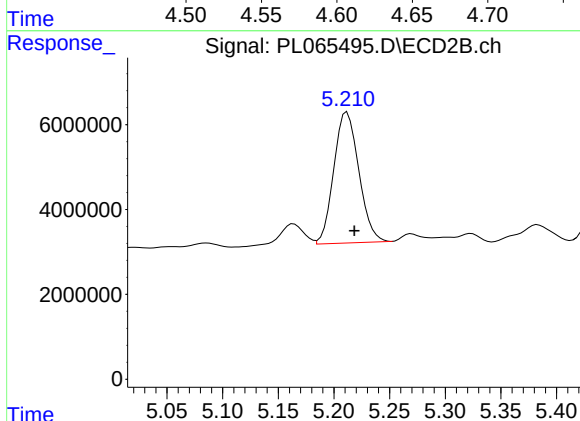


#24 Chlordane-2

R.T.: 5.212 min
Delta R.T.: -0.007 min
Response: 48310093
Conc: 443.57 ng/ml

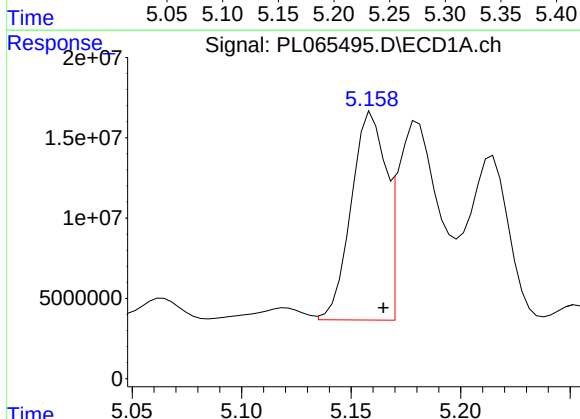


#25 Chlordane-3

R.T.: 5.160 min
Delta R.T.: -0.005 min
Response: 141458431
Conc: 474.10 ng/ml

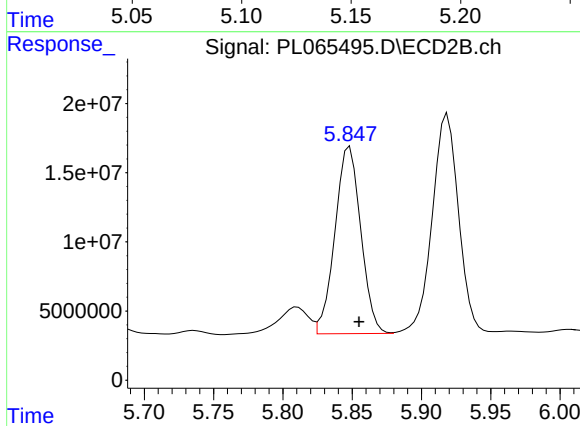

#25 Chlordane-3


R.T.: 5.848 min
Delta R.T.: -0.007 min
Response: 175481964
Conc: 430.50 ng/ml

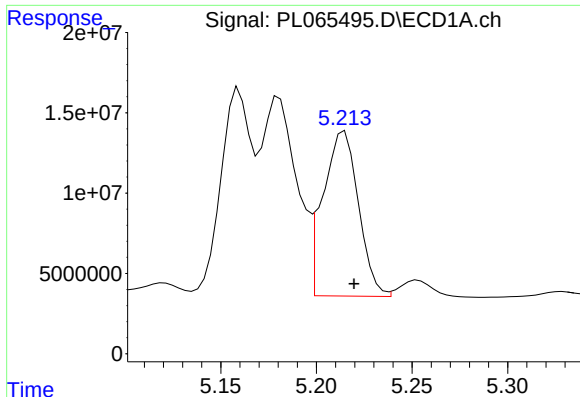

#26 Chlordane-4


R.T.: 5.215 min
Delta R.T.: -0.005 min
Response: 132284606
Conc: 485.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

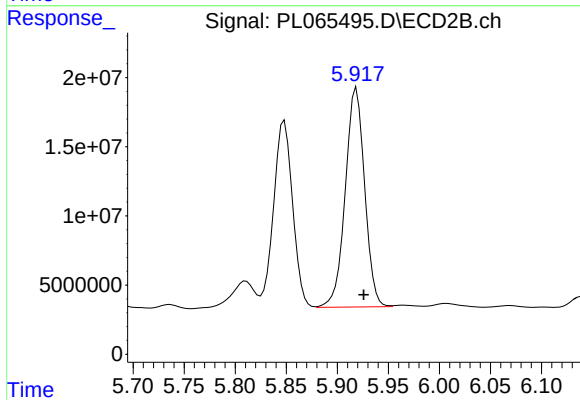


#26 Chlordane-4

R.T.: 5.919 min
Delta R.T.: -0.007 min
Response: 209056405
Conc: 434.56 ng/ml

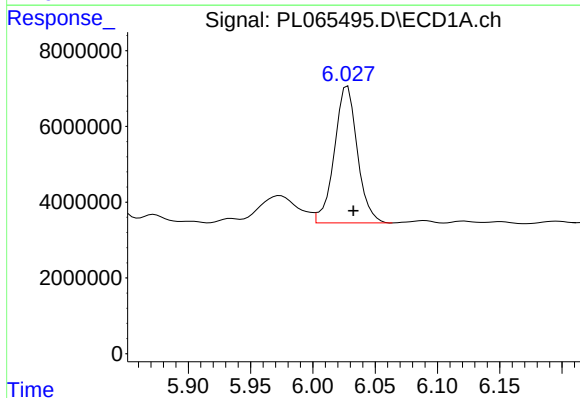


#27 Chlordane-5

R.T.: 6.028 min
Delta R.T.: -0.005 min
Response: 46557673
Conc: 465.68 ng/ml

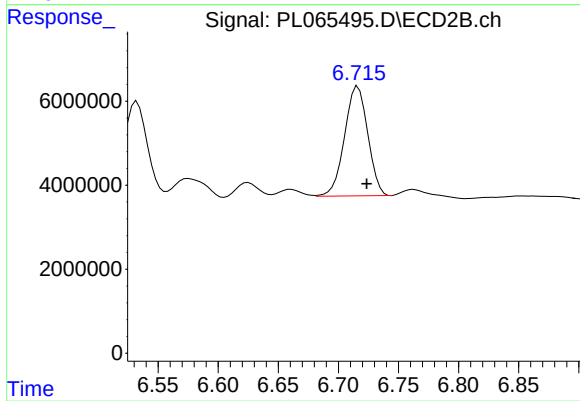

#27 Chlordane-5


R.T.: 6.716 min
Delta R.T.: -0.007 min
Response: 35169930
Conc: 439.52 ng/ml

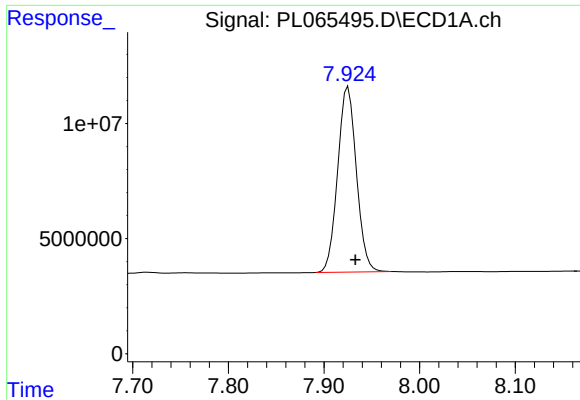

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: -0.008 min
Response: 109652448
Conc: 45.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

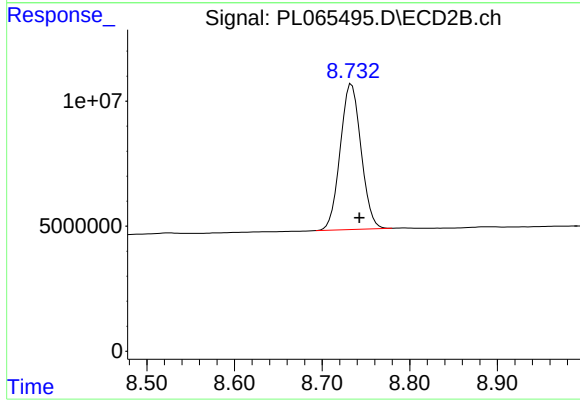

#28 Decachlorobiphenyl

R.T.: 8.734 min
Delta R.T.: -0.009 min
Response: 96087124
Conc: 48.48 ng/ml