

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032321\
 Data File : PL065496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2021 14:27
 Operator : AR\AJ
 Sample : M1746-10
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-4

Manual Integrations
 APPROVED

Ankita
 3/24/2021 11:22:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:12:39 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.293	3.784	31577153	33122273	13.297	12.068m
28)	SA Decachlor...	7.935	8.738	34185481	30262080	14.149	15.267

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032321\
Data File : PL065496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2021 14:27
Operator : AR\AJ
Sample : M1746-10
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
COMP-4


Manual Integrations
APPROVED

Ankita
3/24/2021 11:22:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:12:39 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

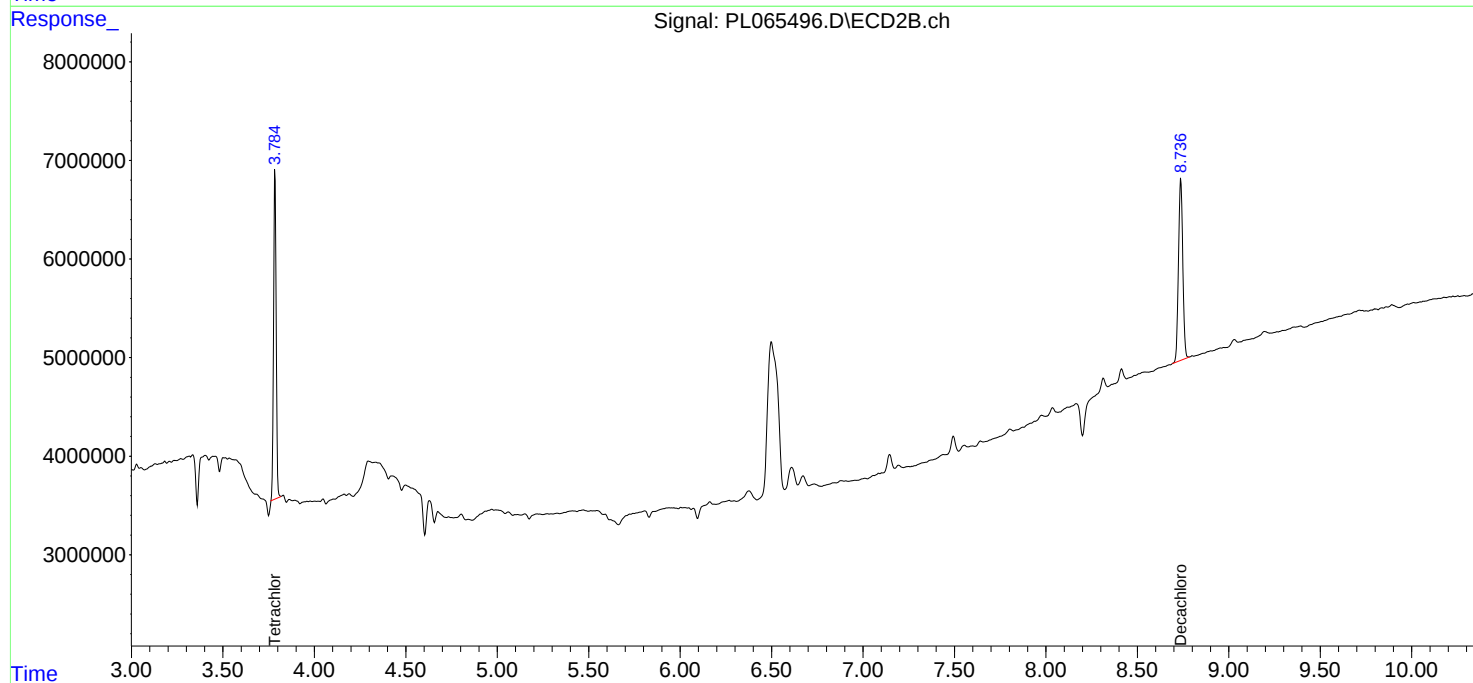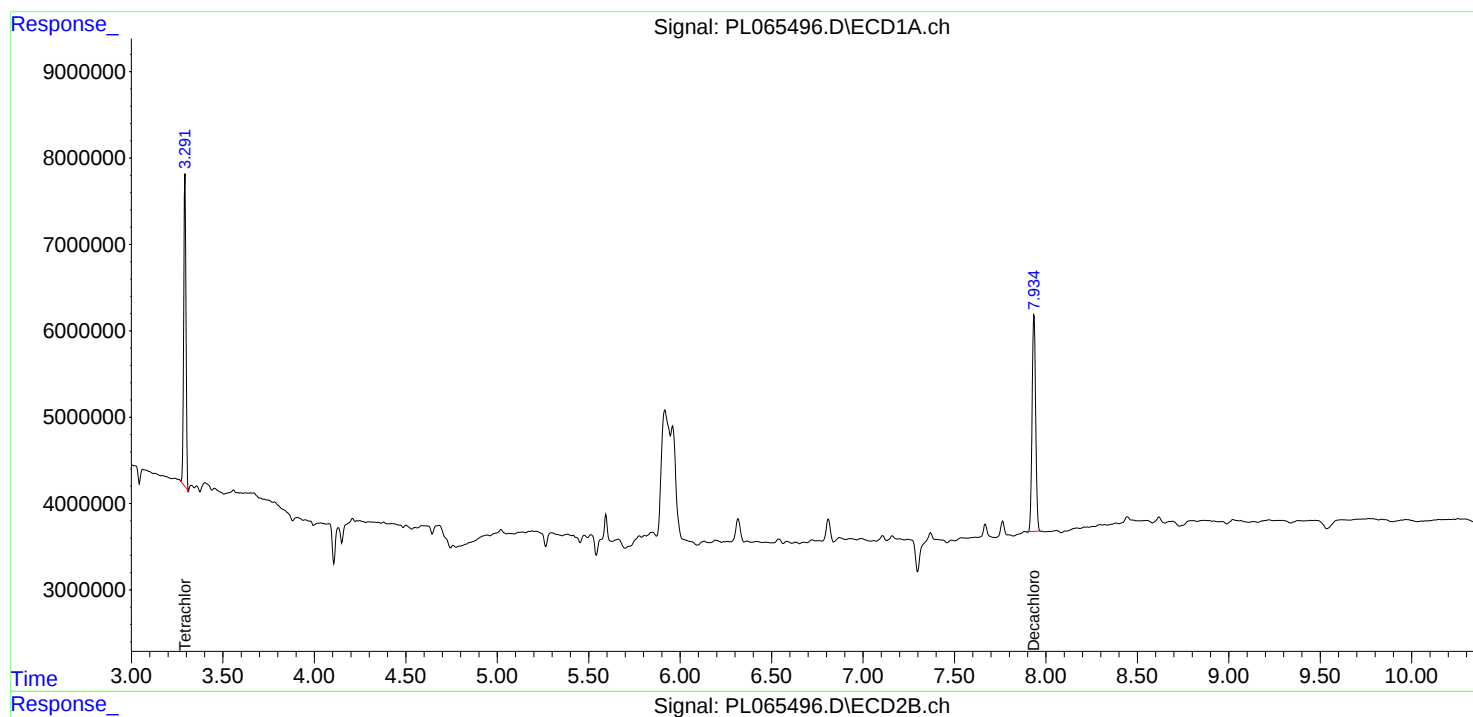

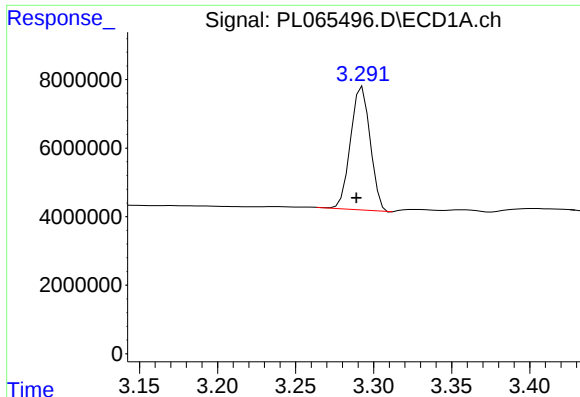


#1 Tetrachloro-m-xylene

R.T.: 3.293 min
Delta R.T.: 0.004 min
Response: 31577153
Conc: 13.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-4


Manual Integrations
APPROVED

Ankita
3/24/2021 11:22:14 AM

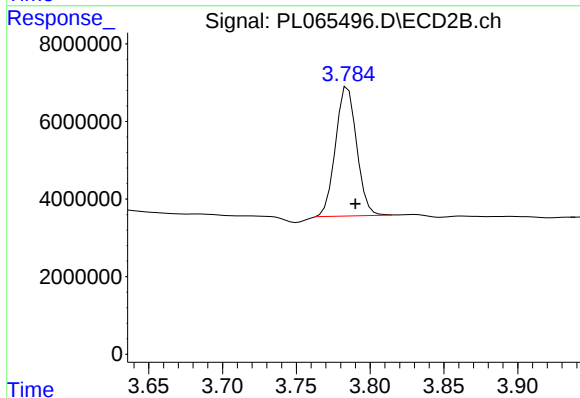


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: -0.006 min
Response: 33122273
Conc: 12.07 ng/ml m

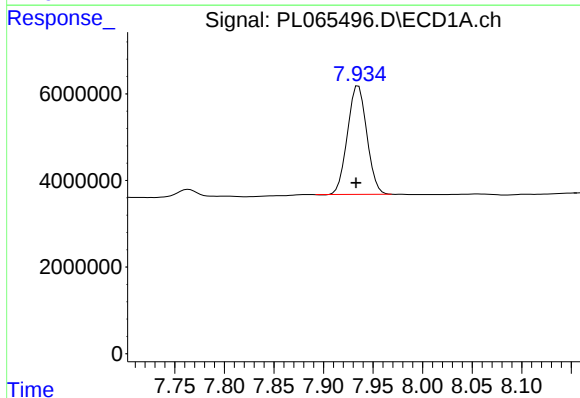

#28 Decachlorobiphenyl

R.T.: 7.935 min
Delta R.T.: 0.002 min
Response: 34185481
Conc: 14.15 ng/ml

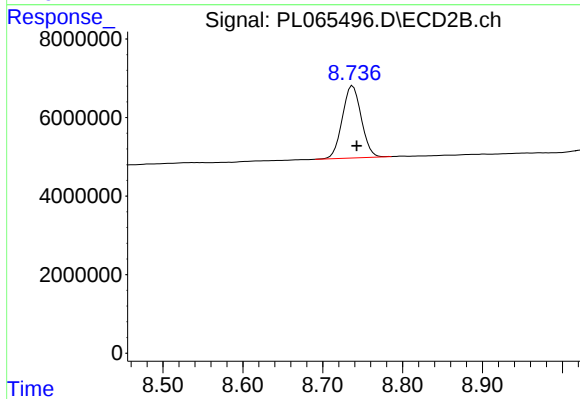

#28 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: -0.005 min
Response: 30262080
Conc: 15.27 ng/ml