

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073599.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 13:06
 Operator : AR\AJ
 Sample : PB143534BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:27:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.651	5.488	5340430	27534596	16.674	16.777
28)	SA Decachlor...	10.421	11.332	9146285	30747702	17.987	17.195
Target Compounds							
4)	MA Heptachlor	6.186	0.000	35264	0	0.078	N.D. #
6)	B beta-BHC	6.136f	6.660f	39523	221450	0.192	0.212
7)	B delta-BHC	0.000	6.956	0	411313	N.D.	0.191 #
10)	B gamma-Chl...	0.000	8.185	0	856482	N.D.	0.419 #
14)	MA Endrin	8.063	0.000	291355	0	0.751	N.D. #
15)	B Endosulfa...	0.000	9.044f	0	471978	N.D.	0.307 #
16)	A 4,4'-DDD	0.000	9.002	0	105631	N.D.	0.072 #
17)	MA 4,4'-DDT	0.000	9.302	0	285221	N.D.	0.174 #
19)	B Endosulfa...	0.000	9.469f	0	180966	N.D.	0.115 #
25)	Chlordane-3	0.000	8.204	0	232238	N.D.	0.857 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073599.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 13:06
Operator : AR\AJ
Sample : PB143534BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:27:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

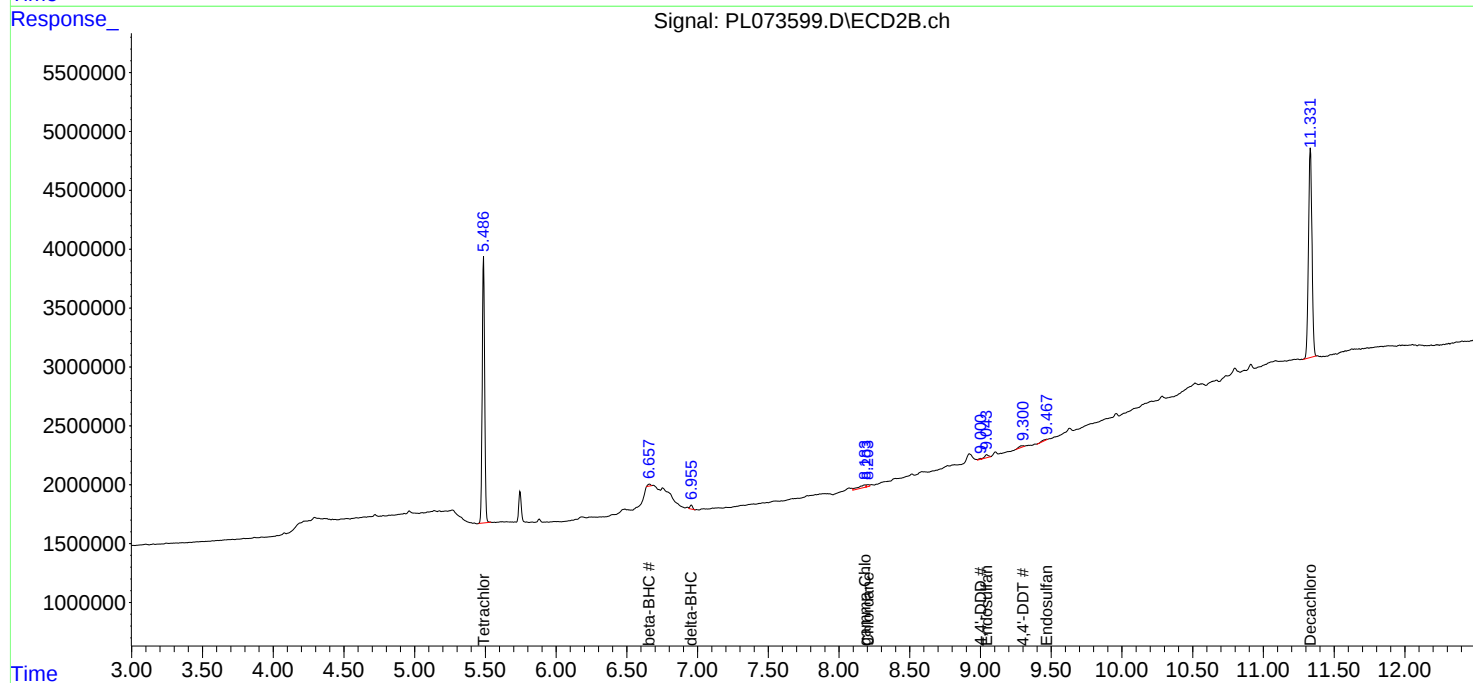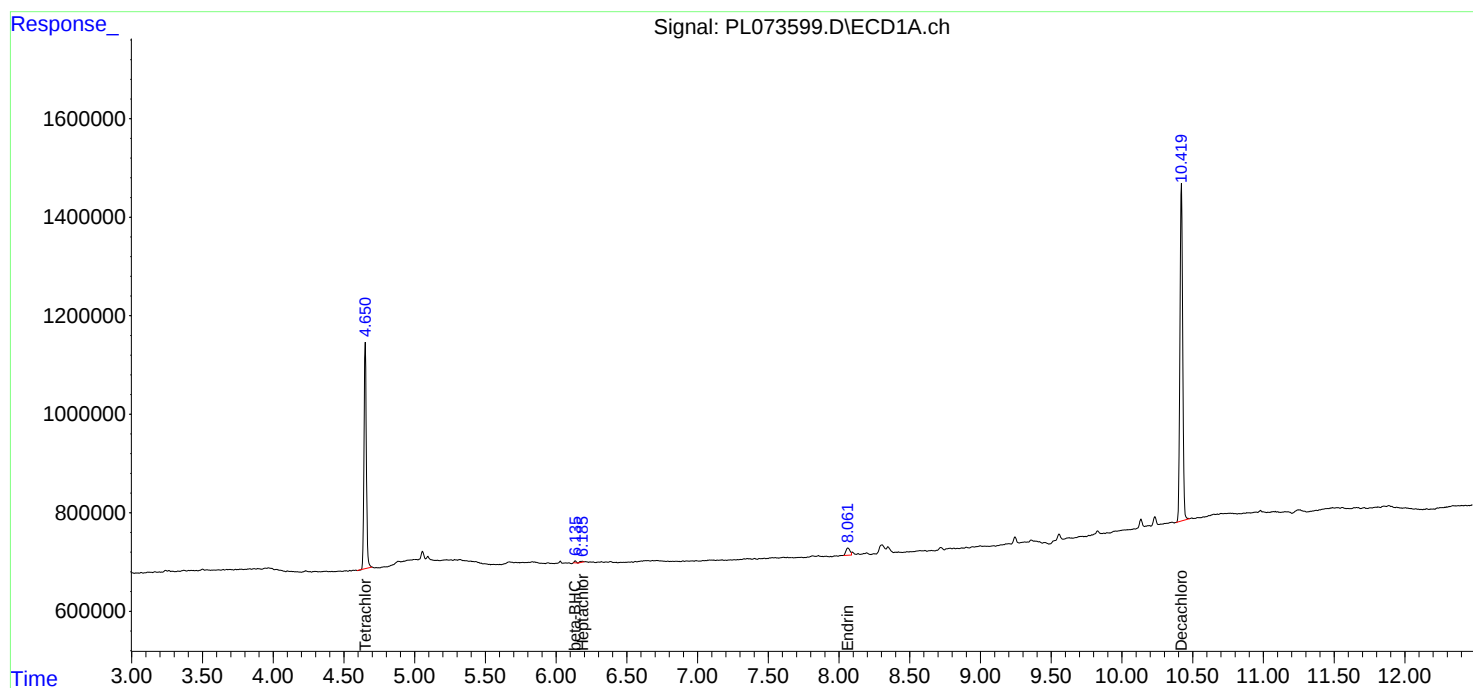


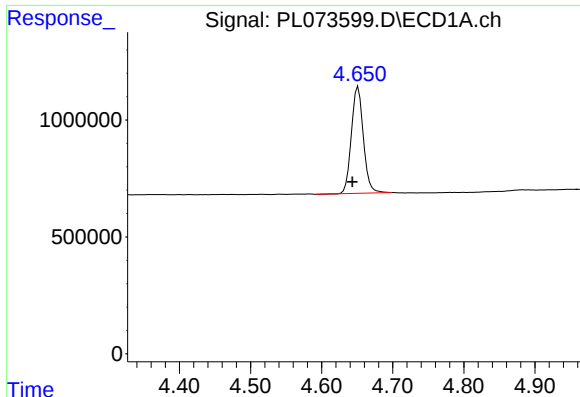

#1 Tetrachloro-m-xylene


R.T.: 4.651 min
Delta R.T.: 0.008 min
Response: 5340430
Conc: 16.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

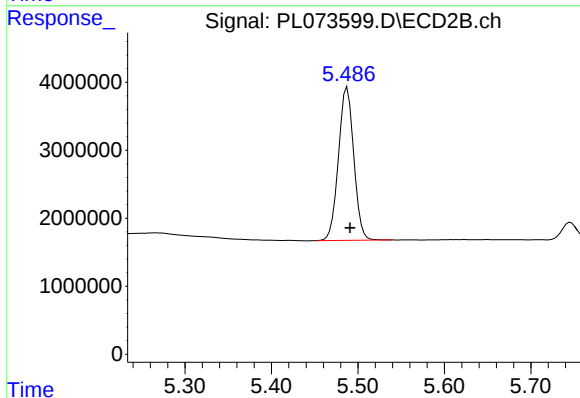


#1 Tetrachloro-m-xylene

R.T.: 5.488 min
Delta R.T.: -0.003 min
Response: 27534596
Conc: 16.78 ng/ml

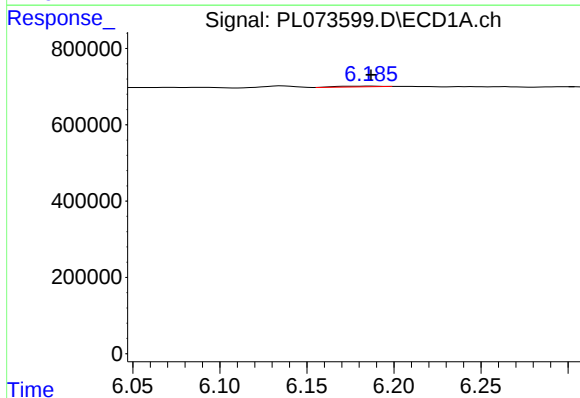


#4 Heptachlor

R.T.: 6.186 min
Delta R.T.: -0.001 min
Response: 35264
Conc: 0.08 ng/ml

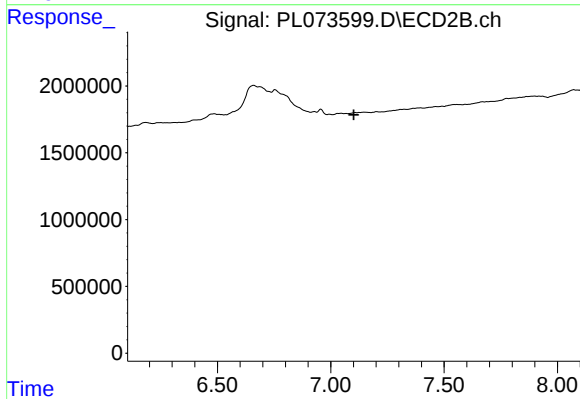

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 7.102 min
Response: 0
Conc: N.D.

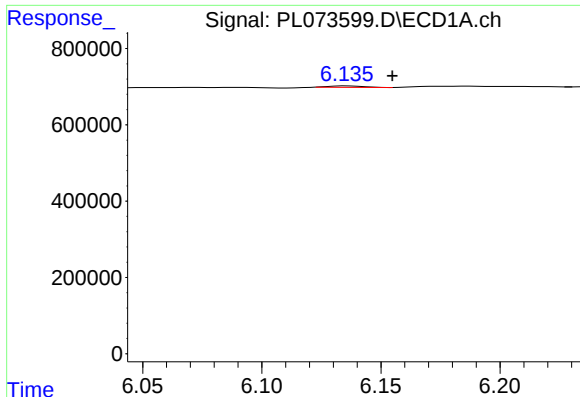

#6 beta-BHC


R.T.: 6.136 min
Delta R.T.: -0.019 min
Response: 39523
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

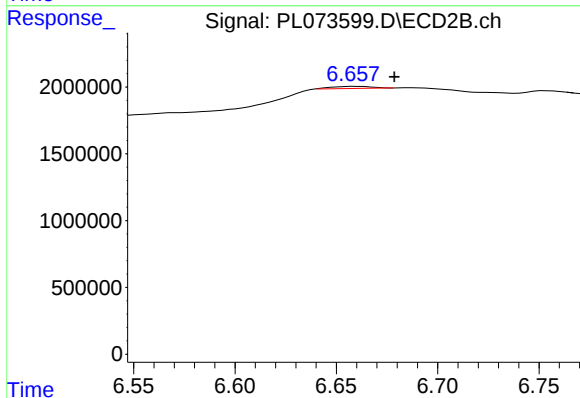


#6 beta-BHC

R.T.: 6.660 min
Delta R.T.: -0.019 min
Response: 221450
Conc: 0.21 ng/ml

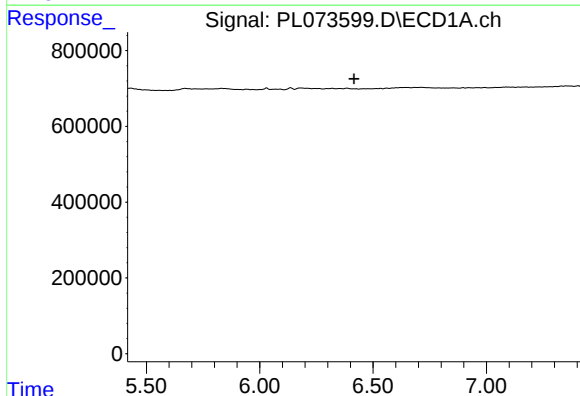


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

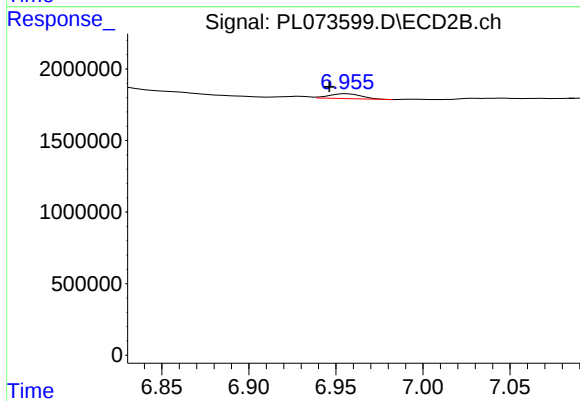

#7 delta-BHC


R.T.: 6.956 min
Delta R.T.: 0.010 min
Response: 411313
Conc: 0.19 ng/ml

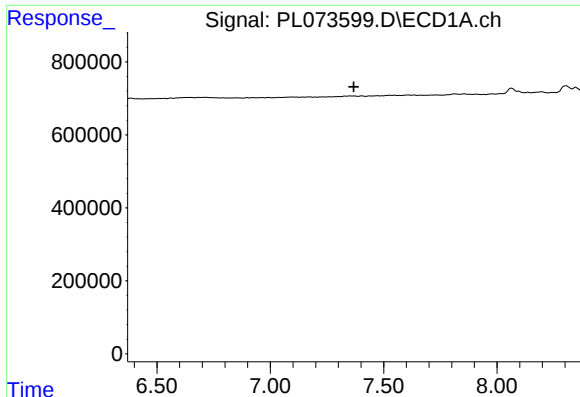

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

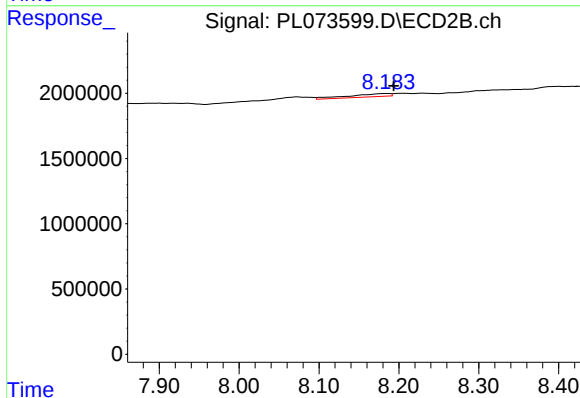


#10 gamma-Chlordane

R.T.: 8.185 min
Delta R.T.: -0.009 min
Response: 856482
Conc: 0.42 ng/ml

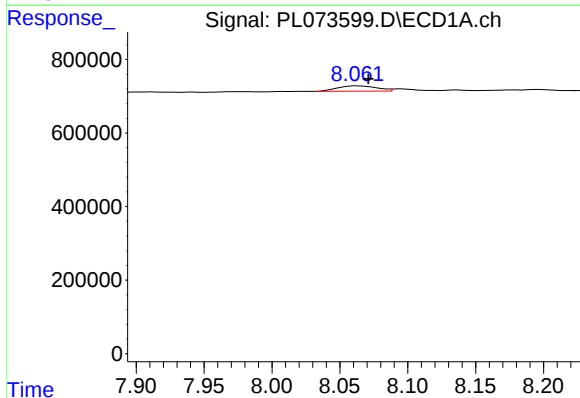


#14 Endrin

R.T.: 8.063 min
Delta R.T.: -0.008 min
Response: 291355
Conc: 0.75 ng/ml

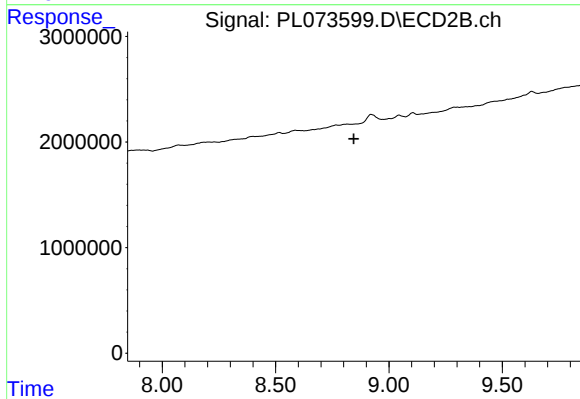

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.845 min
Response: 0
Conc: N.D.

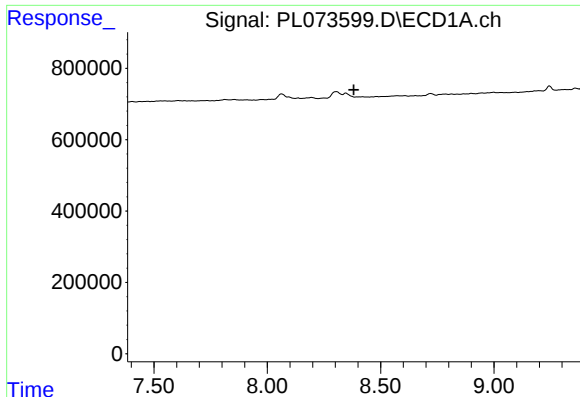

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

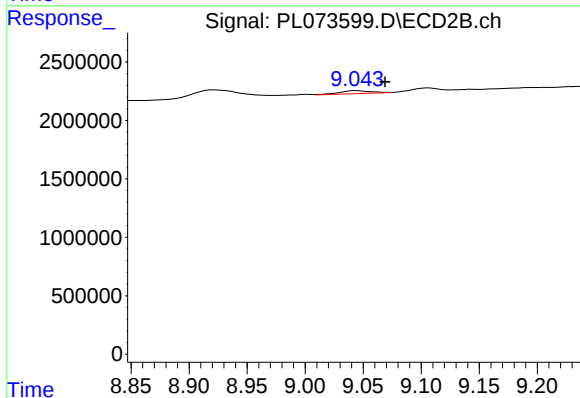


#15 Endosulfan II

R.T.: 9.044 min
Delta R.T.: -0.025 min
Response: 471978
Conc: 0.31 ng/ml

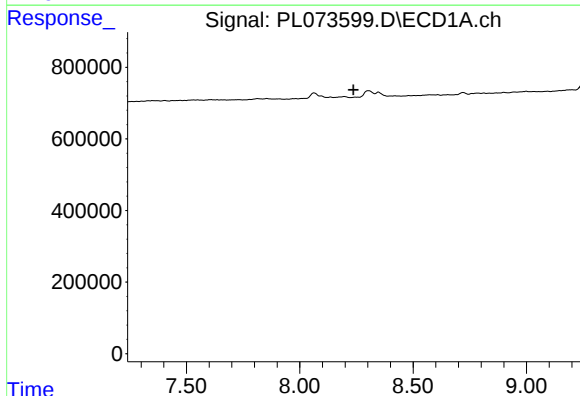


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.237 min
Response: 0
Conc: N.D.

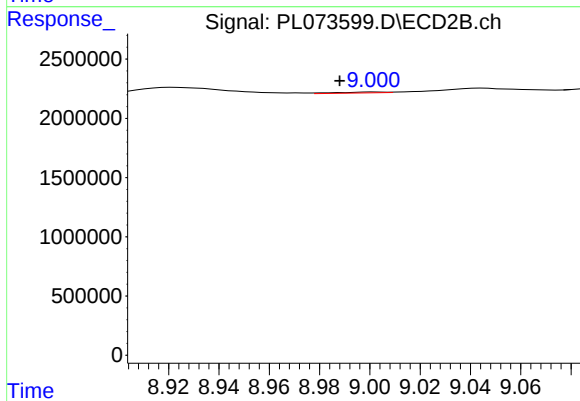

#16 4,4'-DDD


R.T.: 9.002 min
Delta R.T.: 0.014 min
Response: 105631
Conc: 0.07 ng/ml

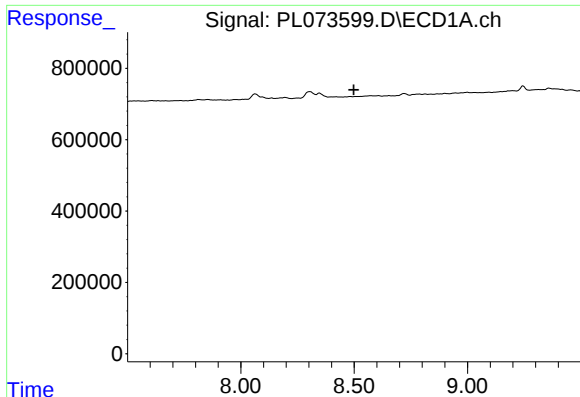

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

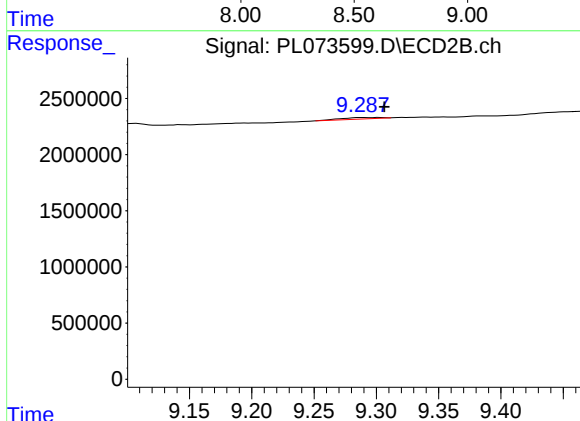


#17 4,4'-DDT

R.T.: 9.302 min
Delta R.T.: -0.004 min
Response: 285221
Conc: 0.17 ng/ml

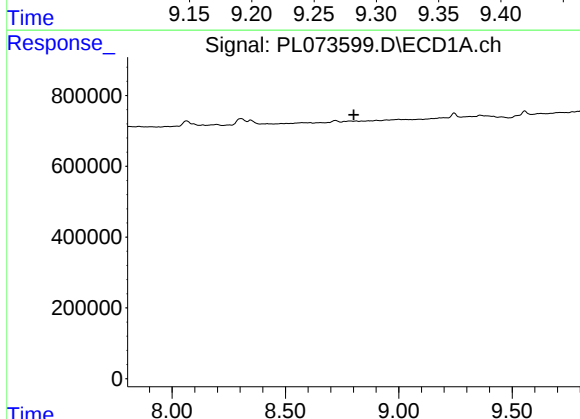


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

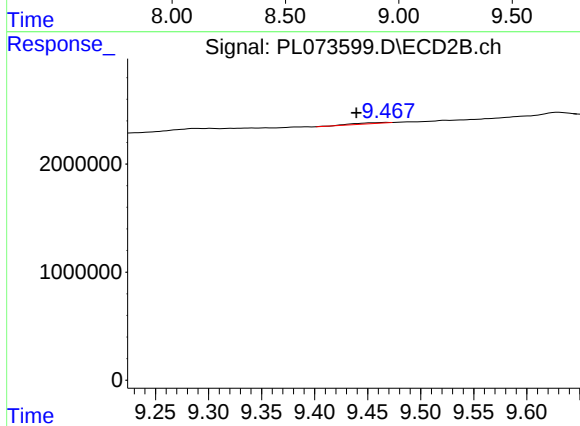

#19 Endosulfan Sulfate


R.T.: 9.469 min
Delta R.T.: 0.029 min
Response: 180966
Conc: 0.11 ng/ml

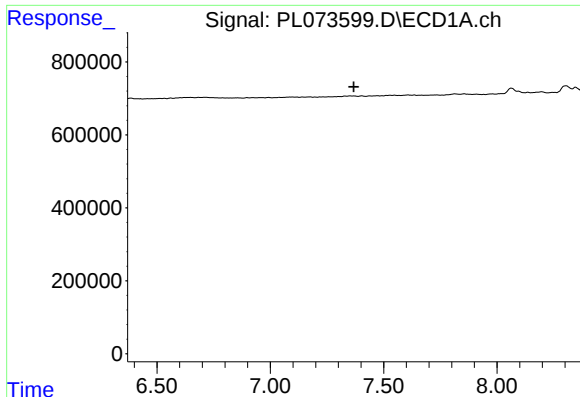

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

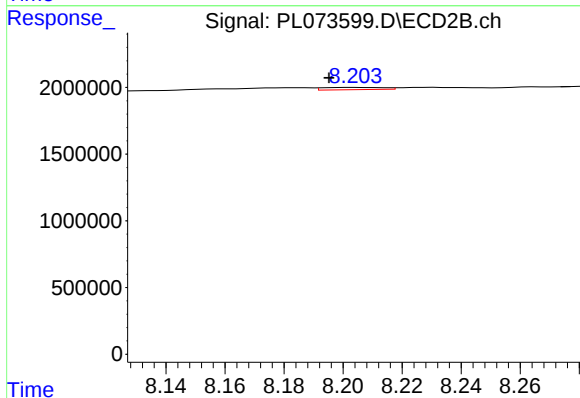


#25 Chlordane-3

R.T.: 8.204 min
Delta R.T.: 0.009 min
Response: 232238
Conc: 0.86 ng/ml

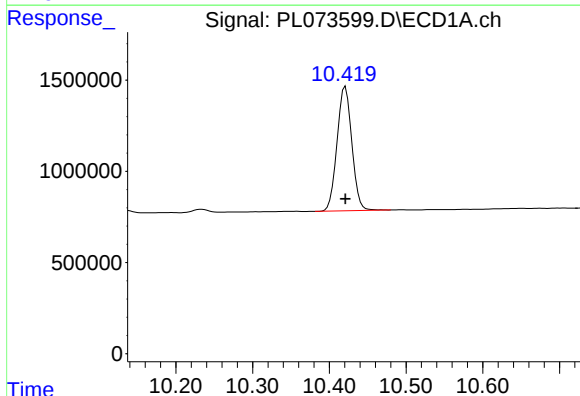

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: 0.000 min
Response: 9146285
Conc: 17.99 ng/ml

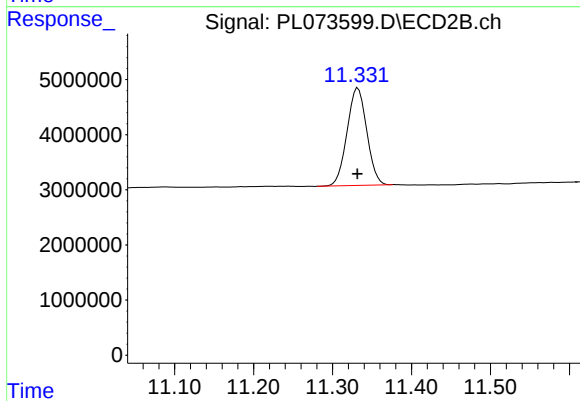

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 30747702
Conc: 17.20 ng/ml