

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 13:59
 Operator : AR\AJ
 Sample : N2063-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:28:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.651	5.487	3003014	14513715	9.376	8.843
28)	SA Decachlor...	10.423	11.333	6804148	22563376	13.381	12.618
Target Compounds							
6)	B beta-BHC	6.136f	6.654f	61585	368352	0.299	0.353
7)	B delta-BHC	0.000	6.957	0	824354	N.D.	0.383 #
8)	B Heptachlo...	0.000	7.940	0	184005	N.D.	0.092 #
10)	B gamma-Chl...	0.000	8.192	0	549780	N.D.	0.269 #
14)	MA Endrin	8.062	0.000	191451	0	0.493	N.D. #
15)	B Endosulfa...	0.000	9.048f	0	385144	N.D.	0.251 #
17)	MA 4,4'-DDT	0.000	9.282f	0	113309	N.D.	0.069 #
25)	Chlordane-3	0.000	8.192	0	549780	N.D.	2.028 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 13:59
Operator : AR\AJ
Sample : N2063-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:28:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

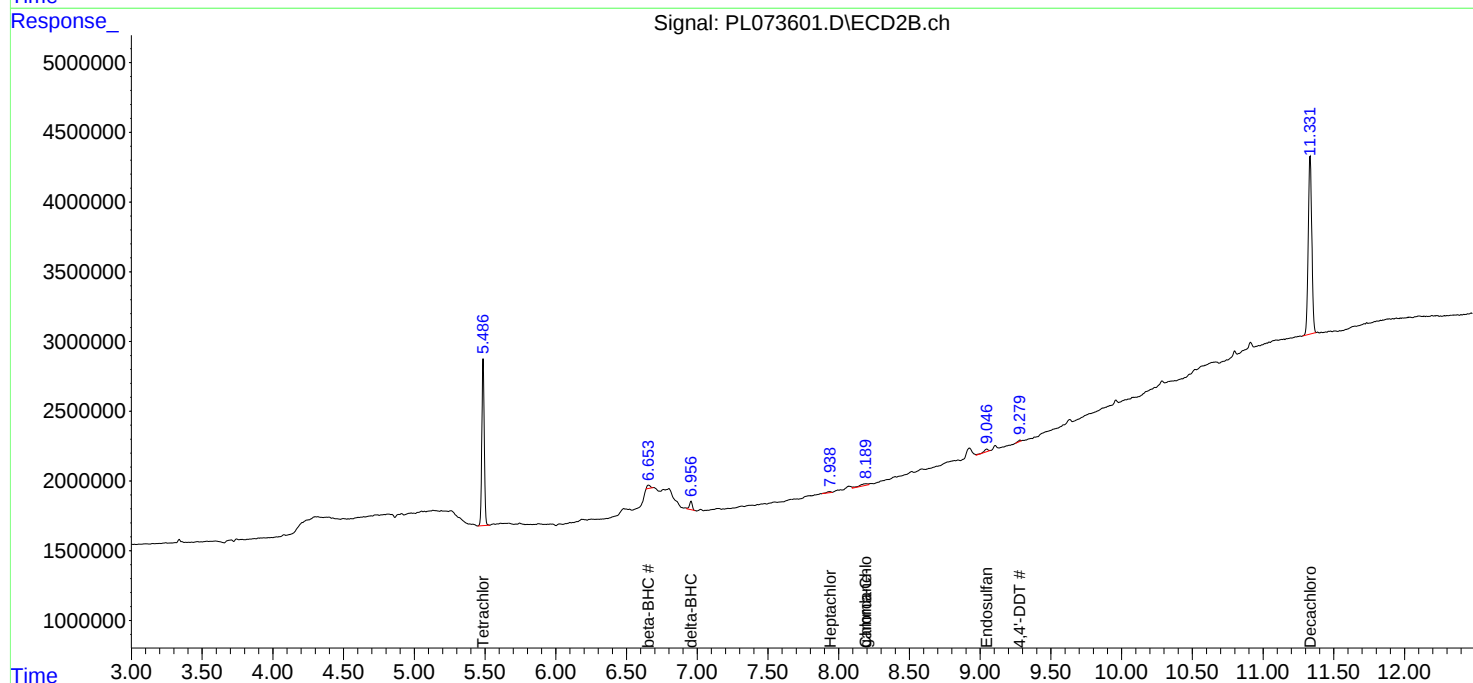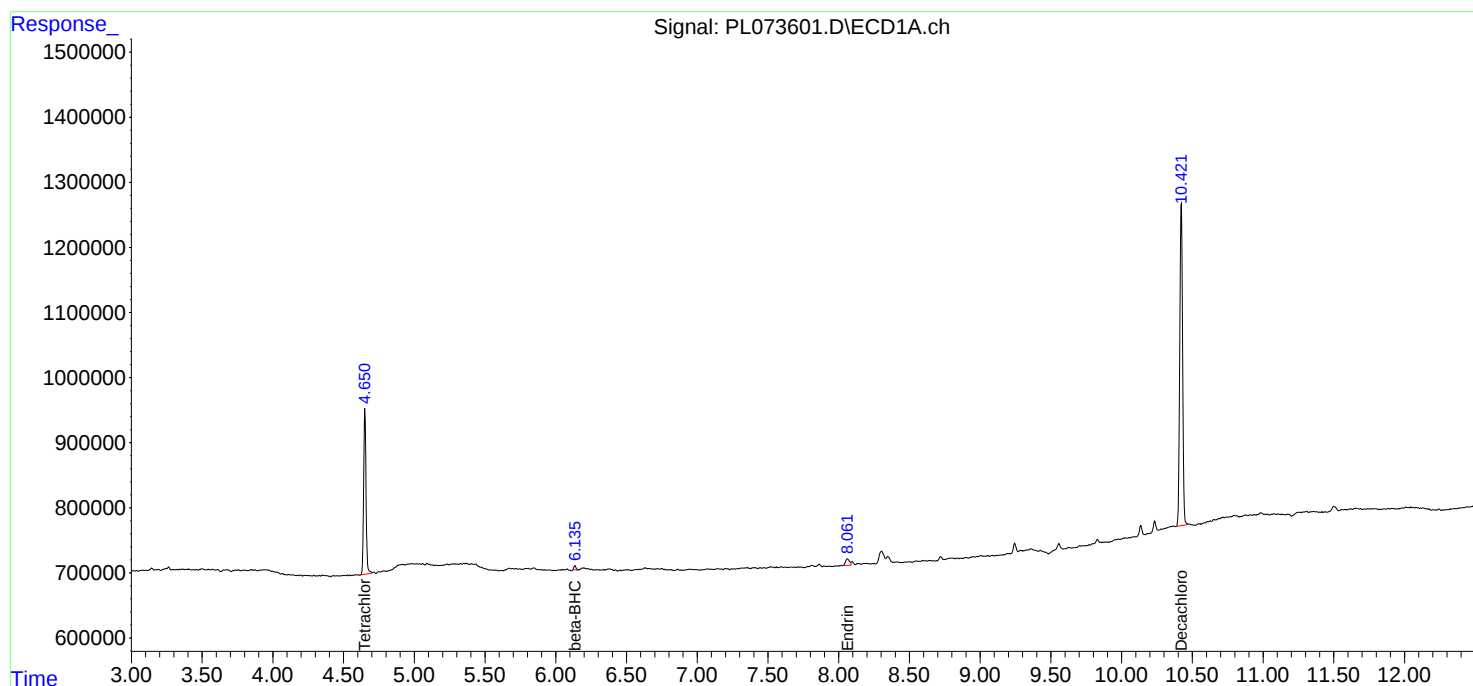


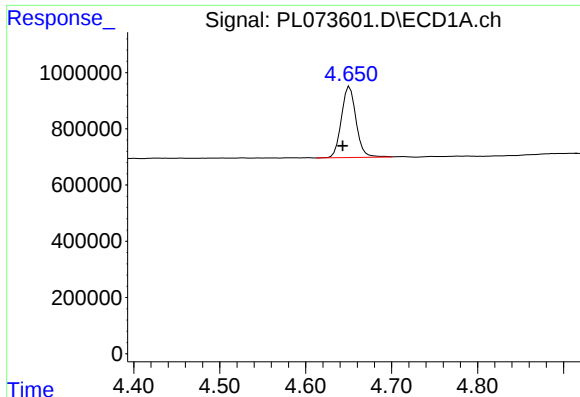

#1 Tetrachloro-m-xylene


R.T.: 4.651 min
Delta R.T.: 0.008 min
Response: 3003014
Conc: 9.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

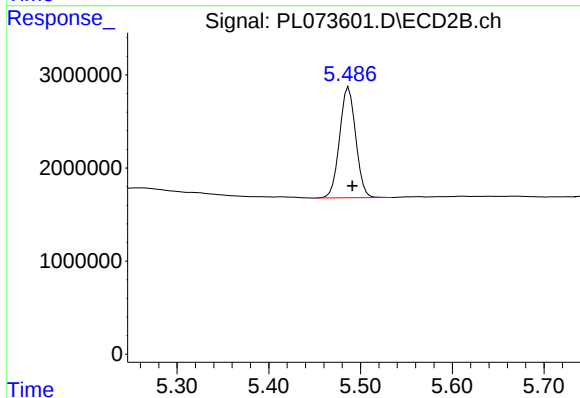


#1 Tetrachloro-m-xylene

R.T.: 5.487 min
Delta R.T.: -0.004 min
Response: 14513715
Conc: 8.84 ng/ml

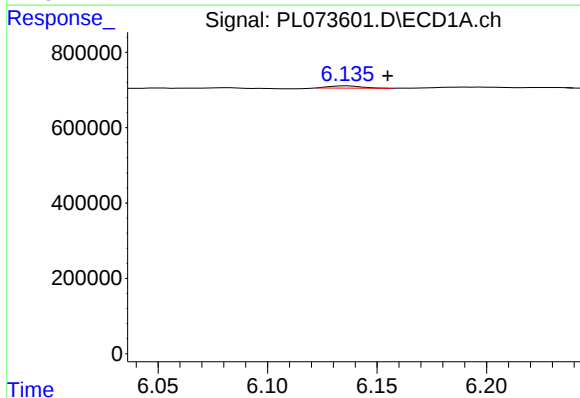


#6 beta-BHC

R.T.: 6.136 min
Delta R.T.: -0.018 min
Response: 61585
Conc: 0.30 ng/ml

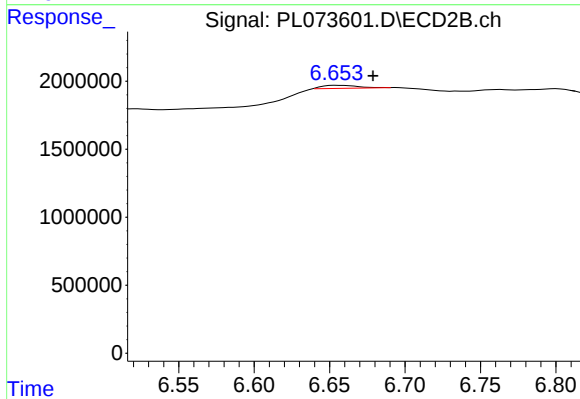

#6 beta-BHC


R.T.: 6.654 min
Delta R.T.: -0.024 min
Response: 368352
Conc: 0.35 ng/ml

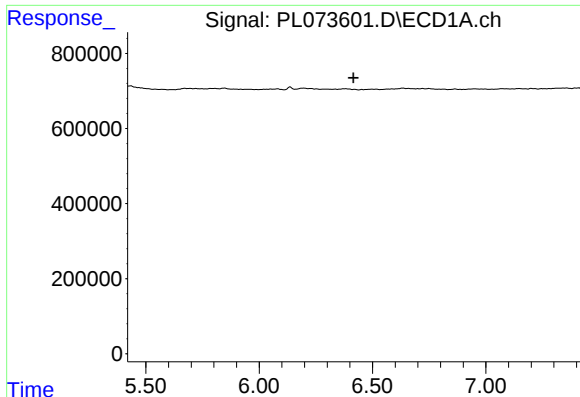

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

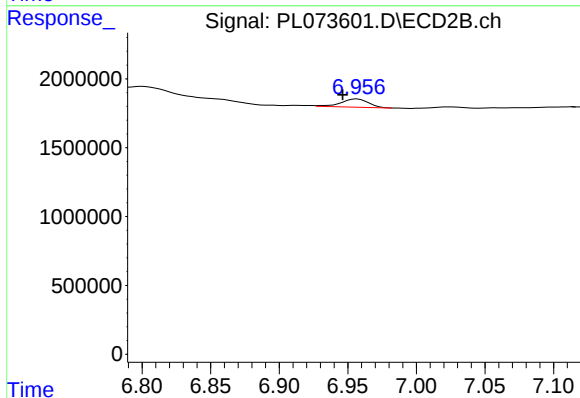


#7 delta-BHC

R.T.: 6.957 min
Delta R.T.: 0.011 min
Response: 824354
Conc: 0.38 ng/ml

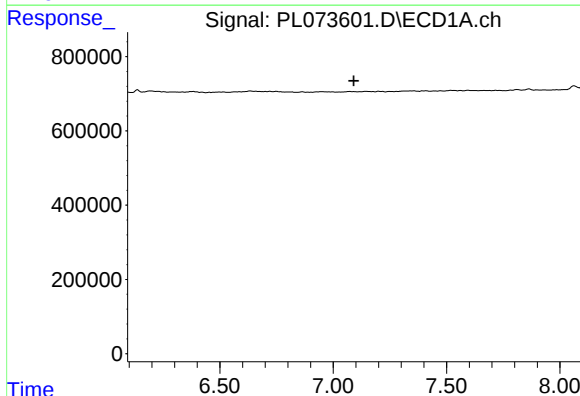


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

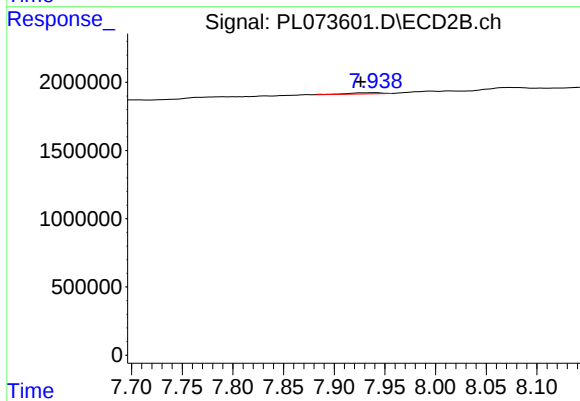

#8 Heptachlor epoxide


R.T.: 7.940 min
Delta R.T.: 0.013 min
Response: 184005
Conc: 0.09 ng/ml

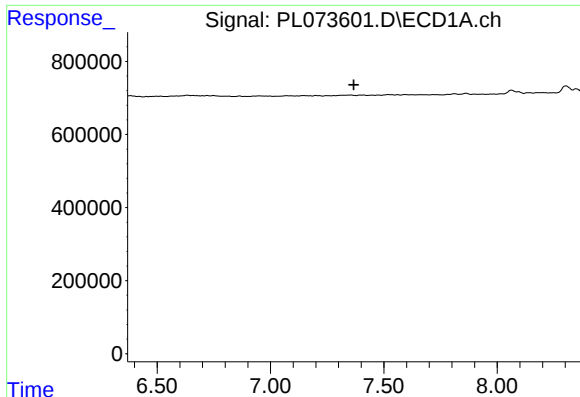

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

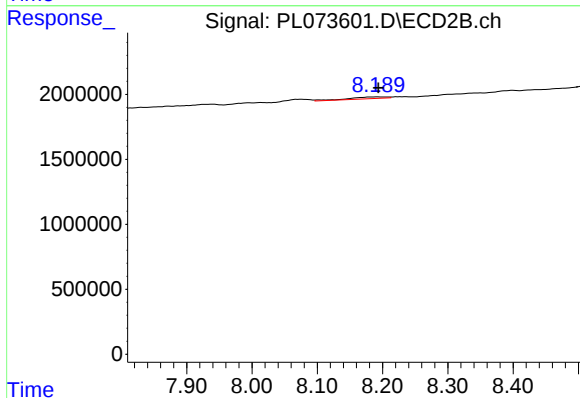


#10 gamma-Chlordane

R.T.: 8.192 min
Delta R.T.: -0.002 min
Response: 549780
Conc: 0.27 ng/ml

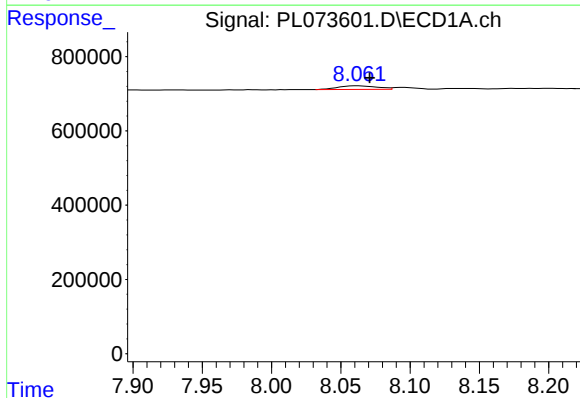


#14 Endrin

R.T.: 8.062 min
Delta R.T.: -0.008 min
Response: 191451
Conc: 0.49 ng/ml

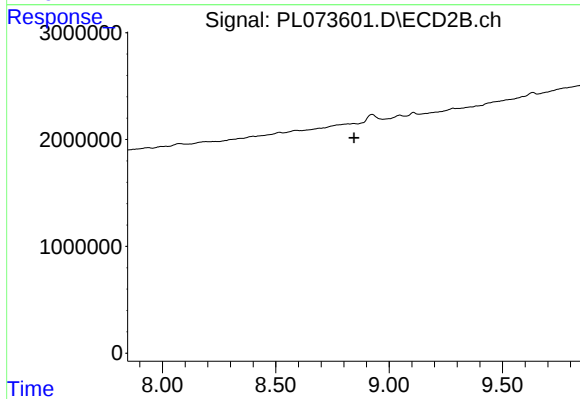

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.845 min
Response: 0
Conc: N.D.

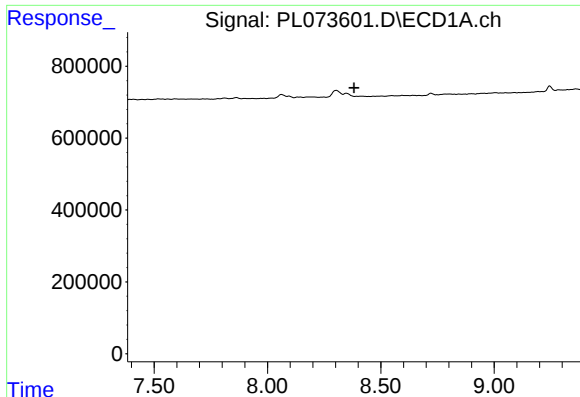

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

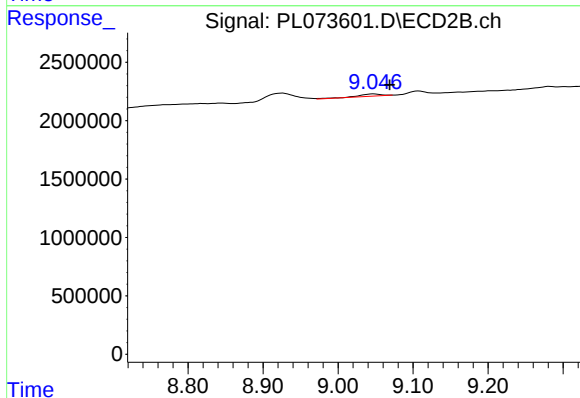


#15 Endosulfan II

R.T.: 9.048 min
Delta R.T.: -0.021 min
Response: 385144
Conc: 0.25 ng/ml

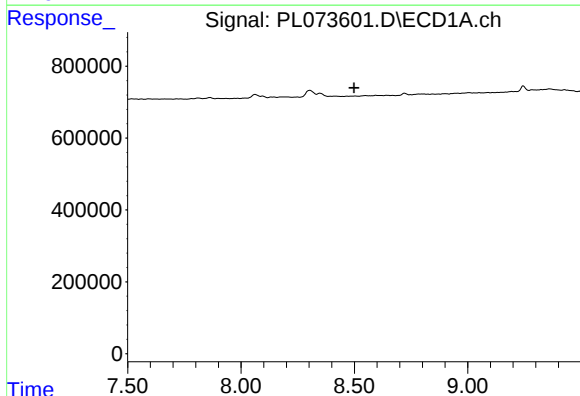


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.499 min
Response: 0
Conc: N.D.

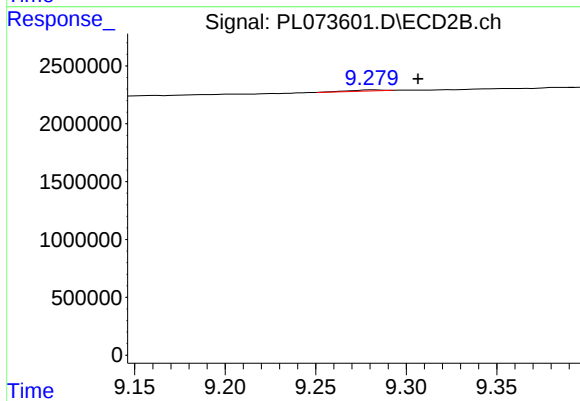

#17 4,4'-DDT


R.T.: 9.282 min
Delta R.T.: -0.025 min
Response: 113309
Conc: 0.07 ng/ml

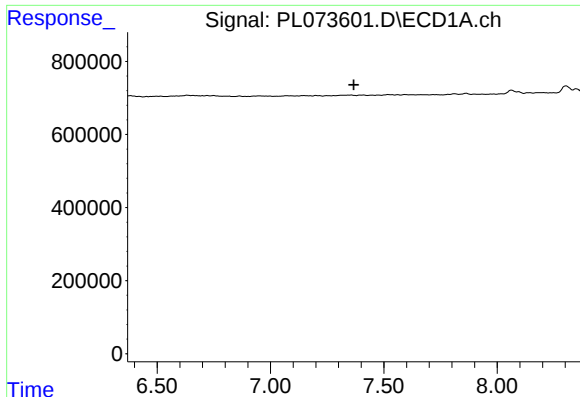

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

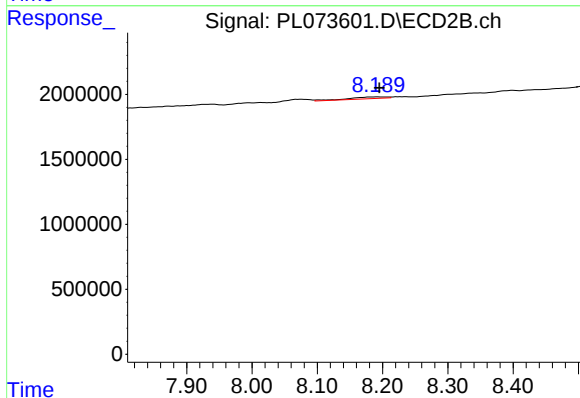


#25 Chlordane-3

R.T.: 8.192 min
Delta R.T.: -0.003 min
Response: 549780
Conc: 2.03 ng/ml

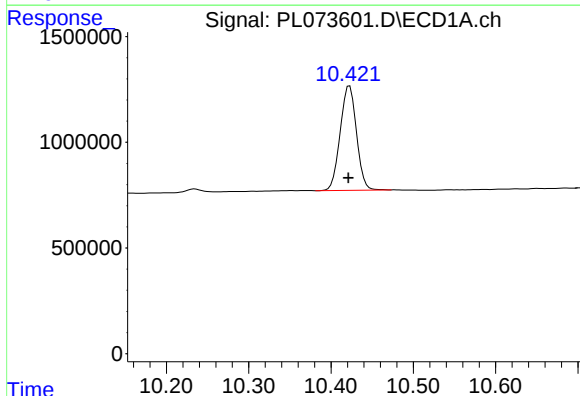

#28 Decachlorobiphenyl

R.T.: 10.423 min
Delta R.T.: 0.002 min
Response: 6804148
Conc: 13.38 ng/ml

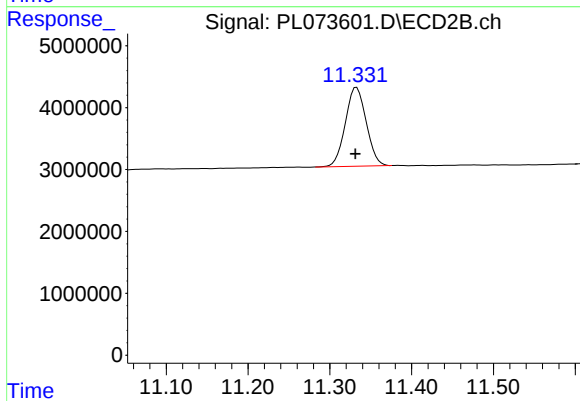

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: 0.001 min
Response: 22563376
Conc: 12.62 ng/ml