

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073607.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 15:37
 Operator : AR\AJ
 Sample : PB143539BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:29:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.492	5485666	28218554	17.127	17.193
28)	SA Decachlor...	10.414	11.332	9288177	31503665	18.266	17.618
Target Compounds							
6)	B beta-BHC	0.000	6.679	0	632461	N.D.	0.607 #
7)	B delta-BHC	0.000	6.939	0	923733	N.D.	0.429 #
8)	B Heptachlo...	0.000	7.925	0	223284	N.D.	0.112 #
9)	A Endosulfan I	0.000	8.327	0	404685	N.D.	0.222 #
10)	B gamma-Chl...	0.000	8.194	0	978636	N.D.	0.479 #
13)	MA Dieldrin	0.000	8.613	0	42464	N.D.	0.023 #
14)	MA Endrin	8.088f	8.852	159223	72071	0.410	0.047 #
17)	MA 4,4'-DDT	0.000	9.305	0	30742	N.D.	0.019 #
23)	Chlordane-1	0.000	6.854	0	718675	N.D.	10.520 #
25)	Chlordane-3	0.000	8.194	0	978636	N.D.	3.609 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073607.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 15:37
Operator : AR\AJ
Sample : PB143539BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:29:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

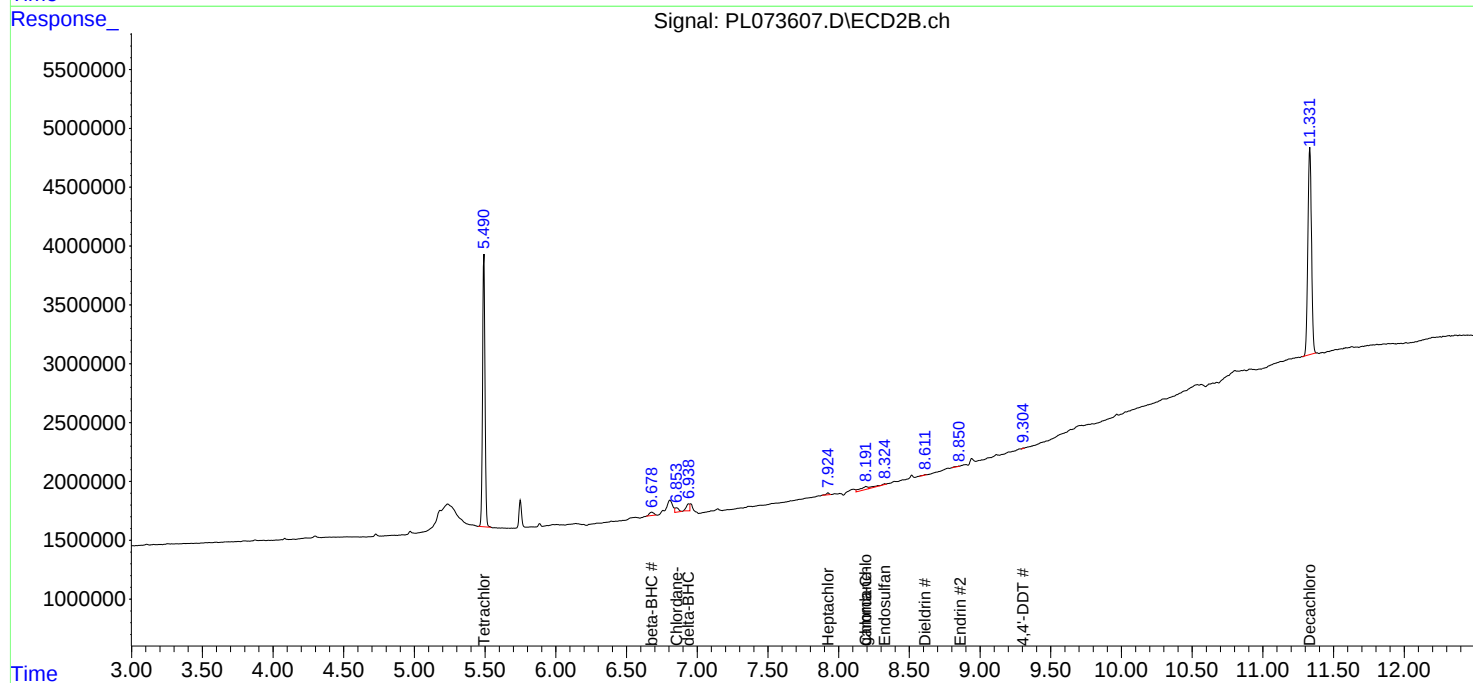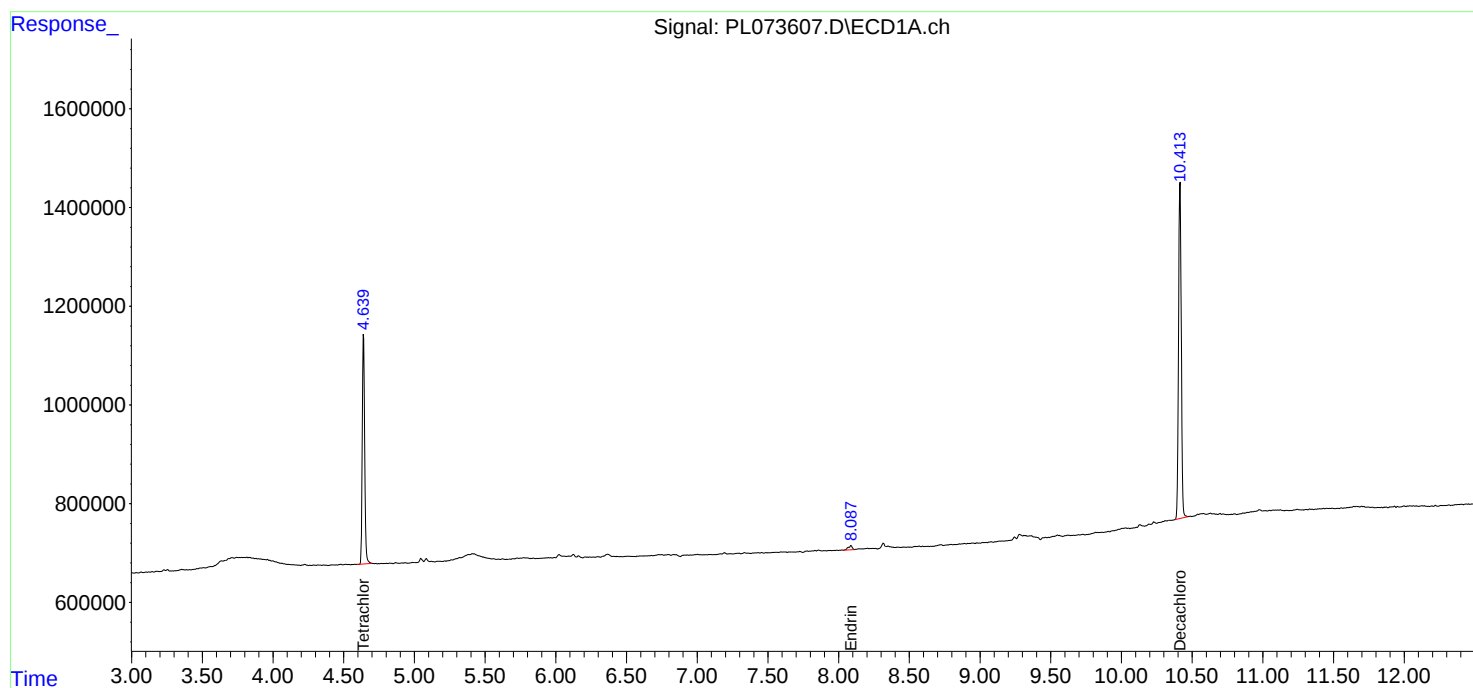


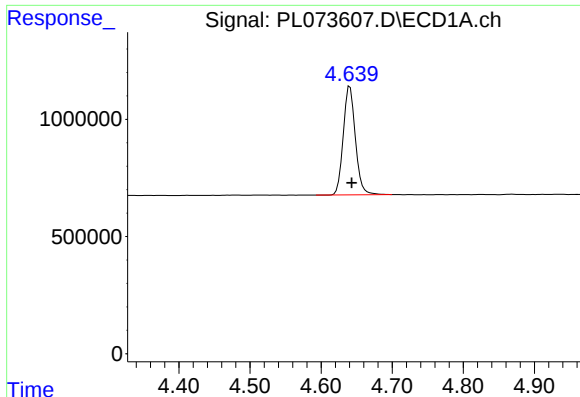

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.002 min
Response: 5485666
Conc: 17.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

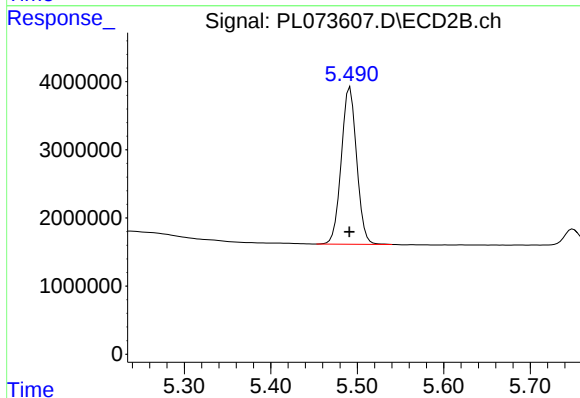


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 28218554
Conc: 17.19 ng/ml

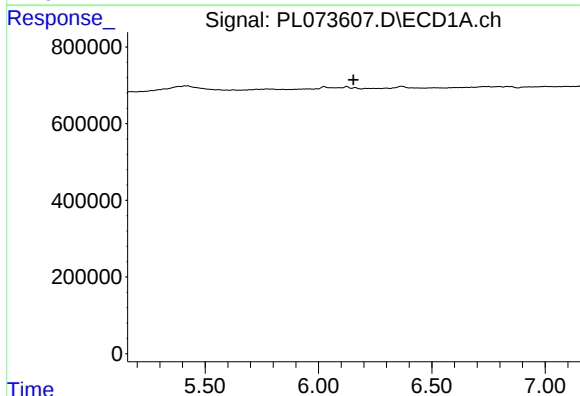


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

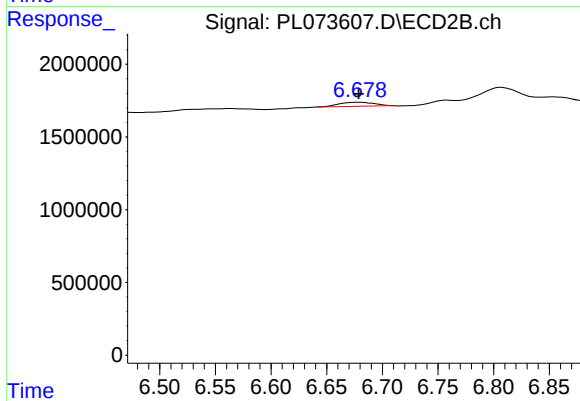

#6 beta-BHC


R.T.: 6.679 min
Delta R.T.: 0.000 min
Response: 632461
Conc: 0.61 ng/ml

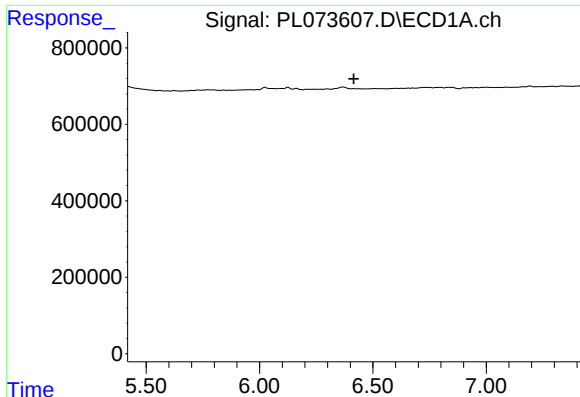

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

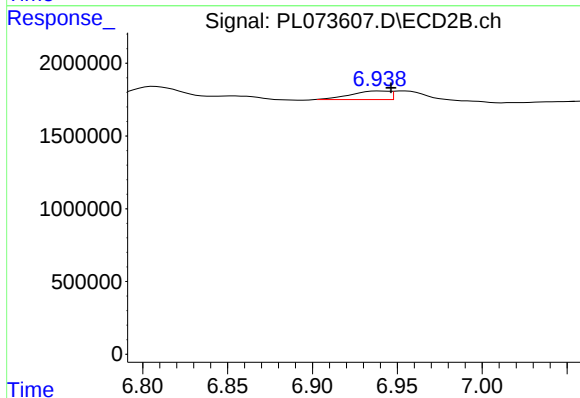


#7 delta-BHC

R.T.: 6.939 min
Delta R.T.: -0.007 min
Response: 923733
Conc: 0.43 ng/ml

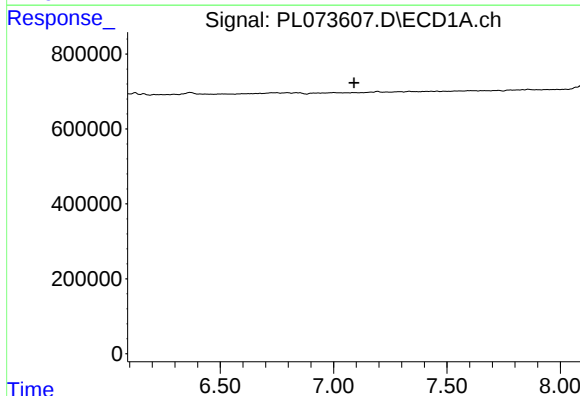


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

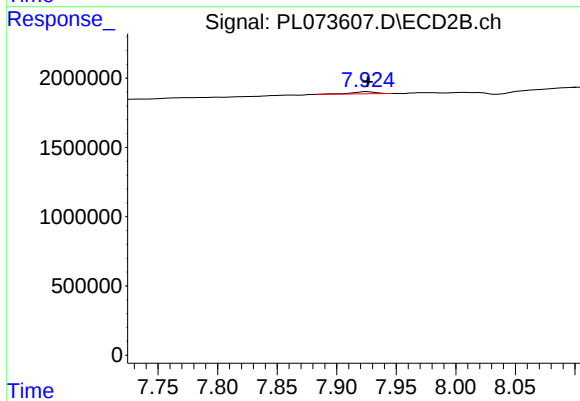

#8 Heptachlor epoxide


R.T.: 7.925 min
Delta R.T.: 0.000 min
Response: 223284
Conc: 0.11 ng/ml

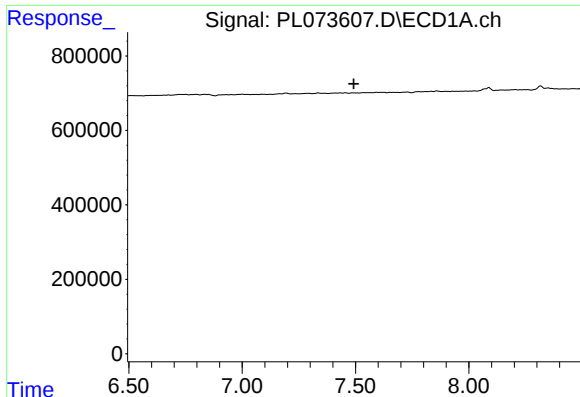

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.493 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

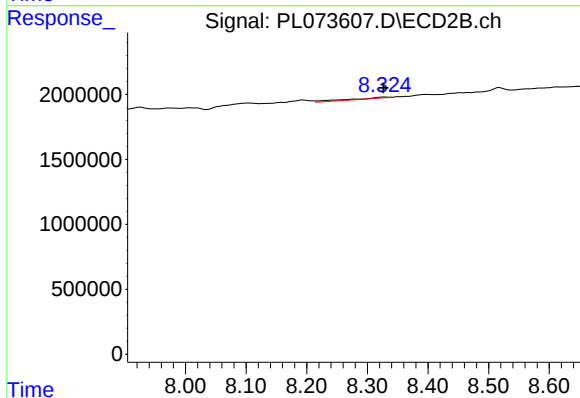


#9 Endosulfan I

R.T.: 8.327 min
Delta R.T.: 0.000 min
Response: 404685
Conc: 0.22 ng/ml

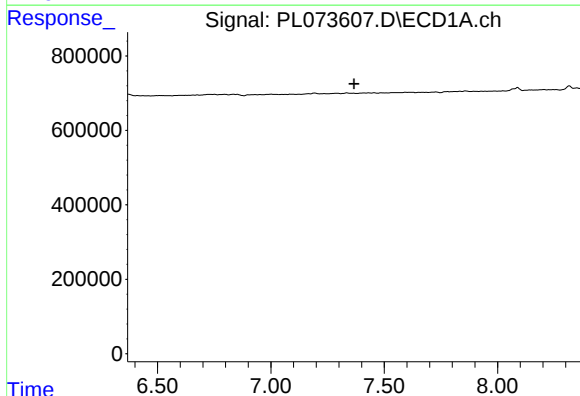


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

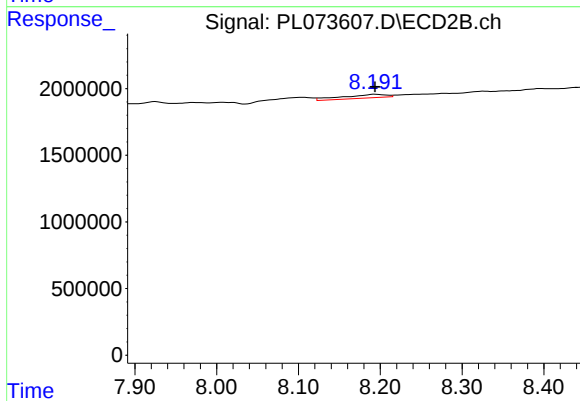

#10 gamma-Chlordane


R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 978636
Conc: 0.48 ng/ml

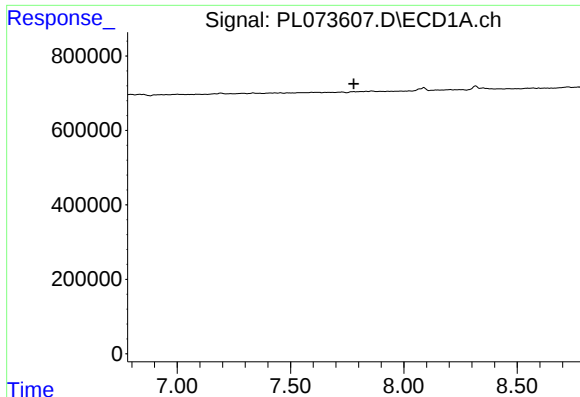

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

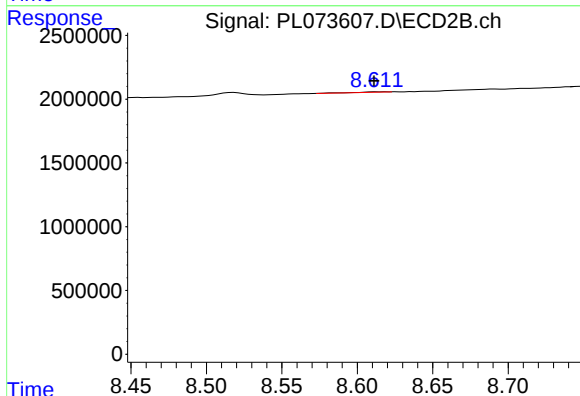


#13 Dieldrin

R.T.: 8.613 min
Delta R.T.: 0.001 min
Response: 42464
Conc: 0.02 ng/ml

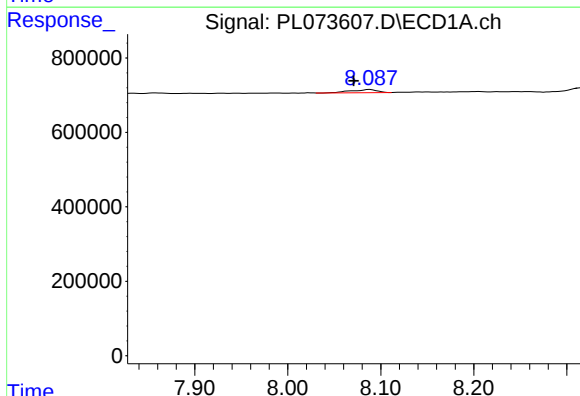


#14 Endrin

R.T.: 8.088 min
Delta R.T.: 0.017 min
Response: 159223
Conc: 0.41 ng/ml

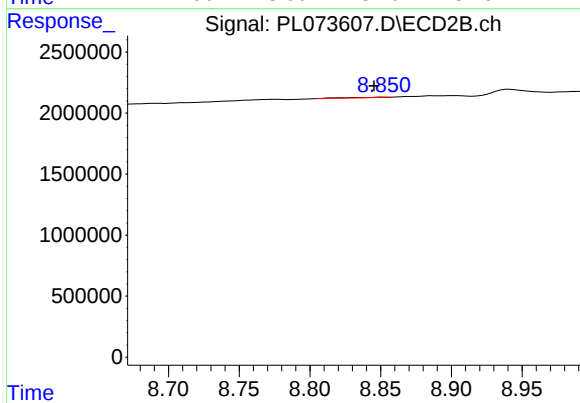

#14 Endrin


R.T.: 8.852 min
Delta R.T.: 0.006 min
Response: 72071
Conc: 0.05 ng/ml

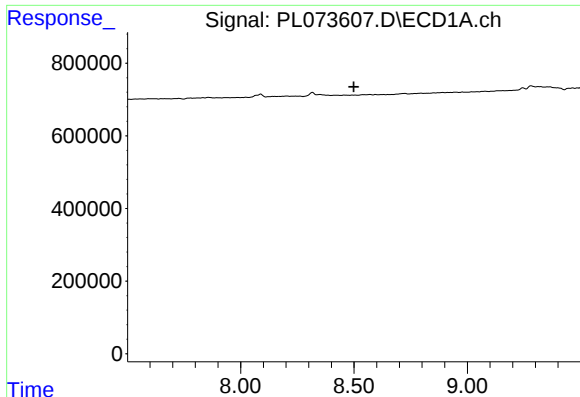

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

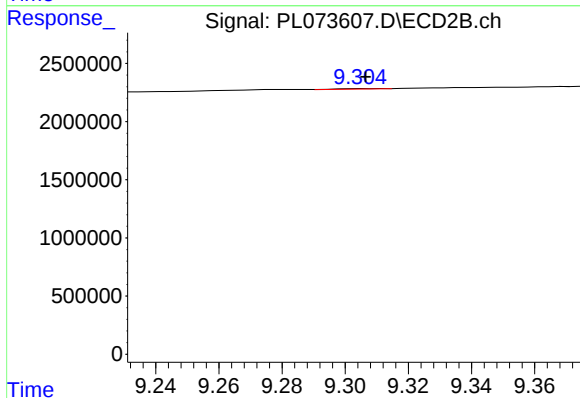


#17 4,4'-DDT

R.T.: 9.305 min
Delta R.T.: -0.001 min
Response: 30742
Conc: 0.02 ng/ml

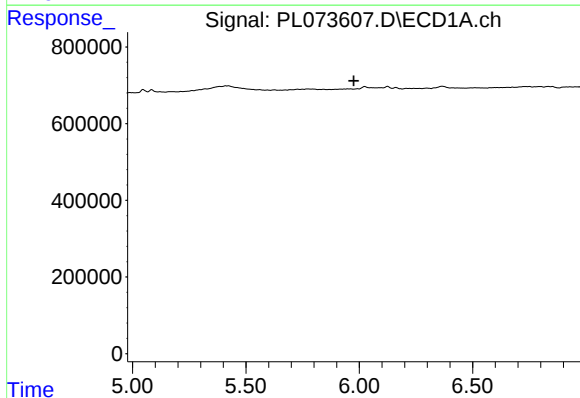


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

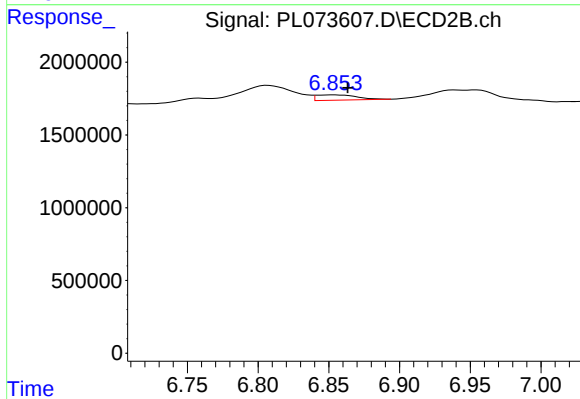

#23 Chlordane-1


R.T.: 6.854 min
Delta R.T.: -0.009 min
Response: 718675
Conc: 10.52 ng/ml

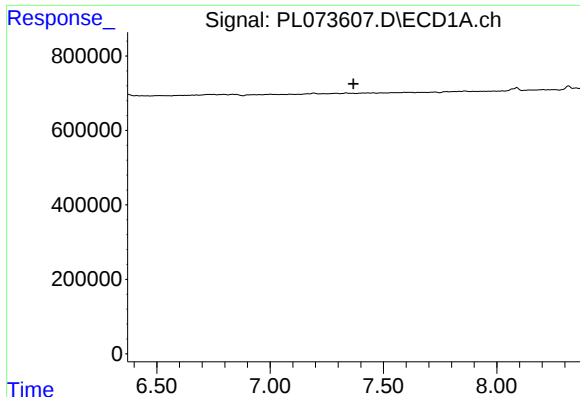

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

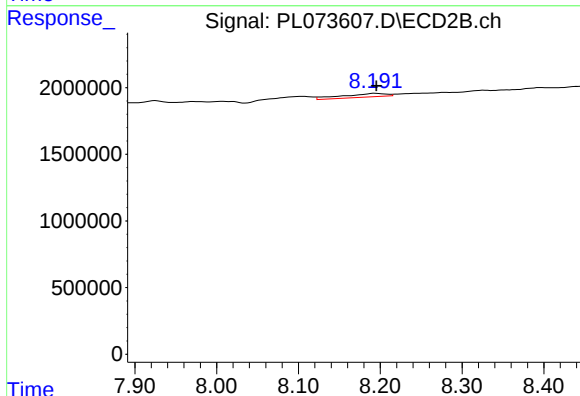


#25 Chlordane-3

R.T.: 8.194 min
Delta R.T.: -0.002 min
Response: 978636
Conc: 3.61 ng/ml

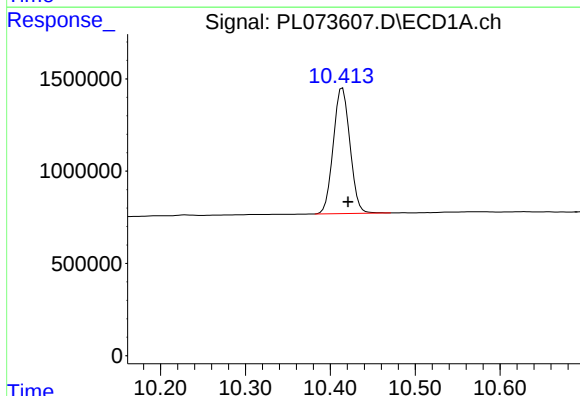

#28 Decachlorobiphenyl

R.T.: 10.414 min
Delta R.T.: -0.007 min
Response: 9288177
Conc: 18.27 ng/ml

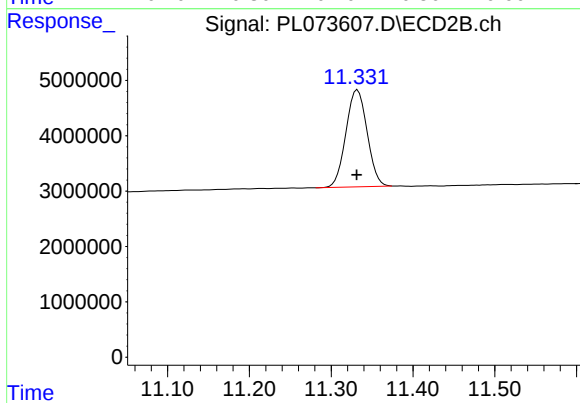

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 31503665
Conc: 17.62 ng/ml