

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 18:31
 Operator : AR\AJ
 Sample : N2031-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:32:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.647	5.489	5342909	28998107	16.682	17.668
28)	SA Decachlor...	10.419	11.332	7354204	26177493	14.463	14.639
Target Compounds							
4)	MA Heptachlor	0.000	7.118f	0	108512	N.D.	0.046 #
7)	B delta-BHC	0.000	6.958	0	460856	N.D.	0.214 #
9)	A Endosulfan I	0.000	8.326	0	152684	N.D.	0.084 #
10)	B gamma-Chl...	7.345f	8.205	55302	253256	0.126	0.124
14)	MA Endrin	8.093f	8.854	161881	100676	0.417	0.065 #
15)	B Endosulfa...	8.356f	0.000	49901	0	0.128	N.D. #
17)	MA 4,4'-DDT	0.000	9.299	0	134856	N.D.	0.083 #
20)	A Methoxychlor	9.097	9.795	48791	28862	0.190	0.032 #
25)	Chlordane-3	7.345f	8.205	55302	253256	1.354	0.934 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 18:31
Operator : AR\AJ
Sample : N2031-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:32:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

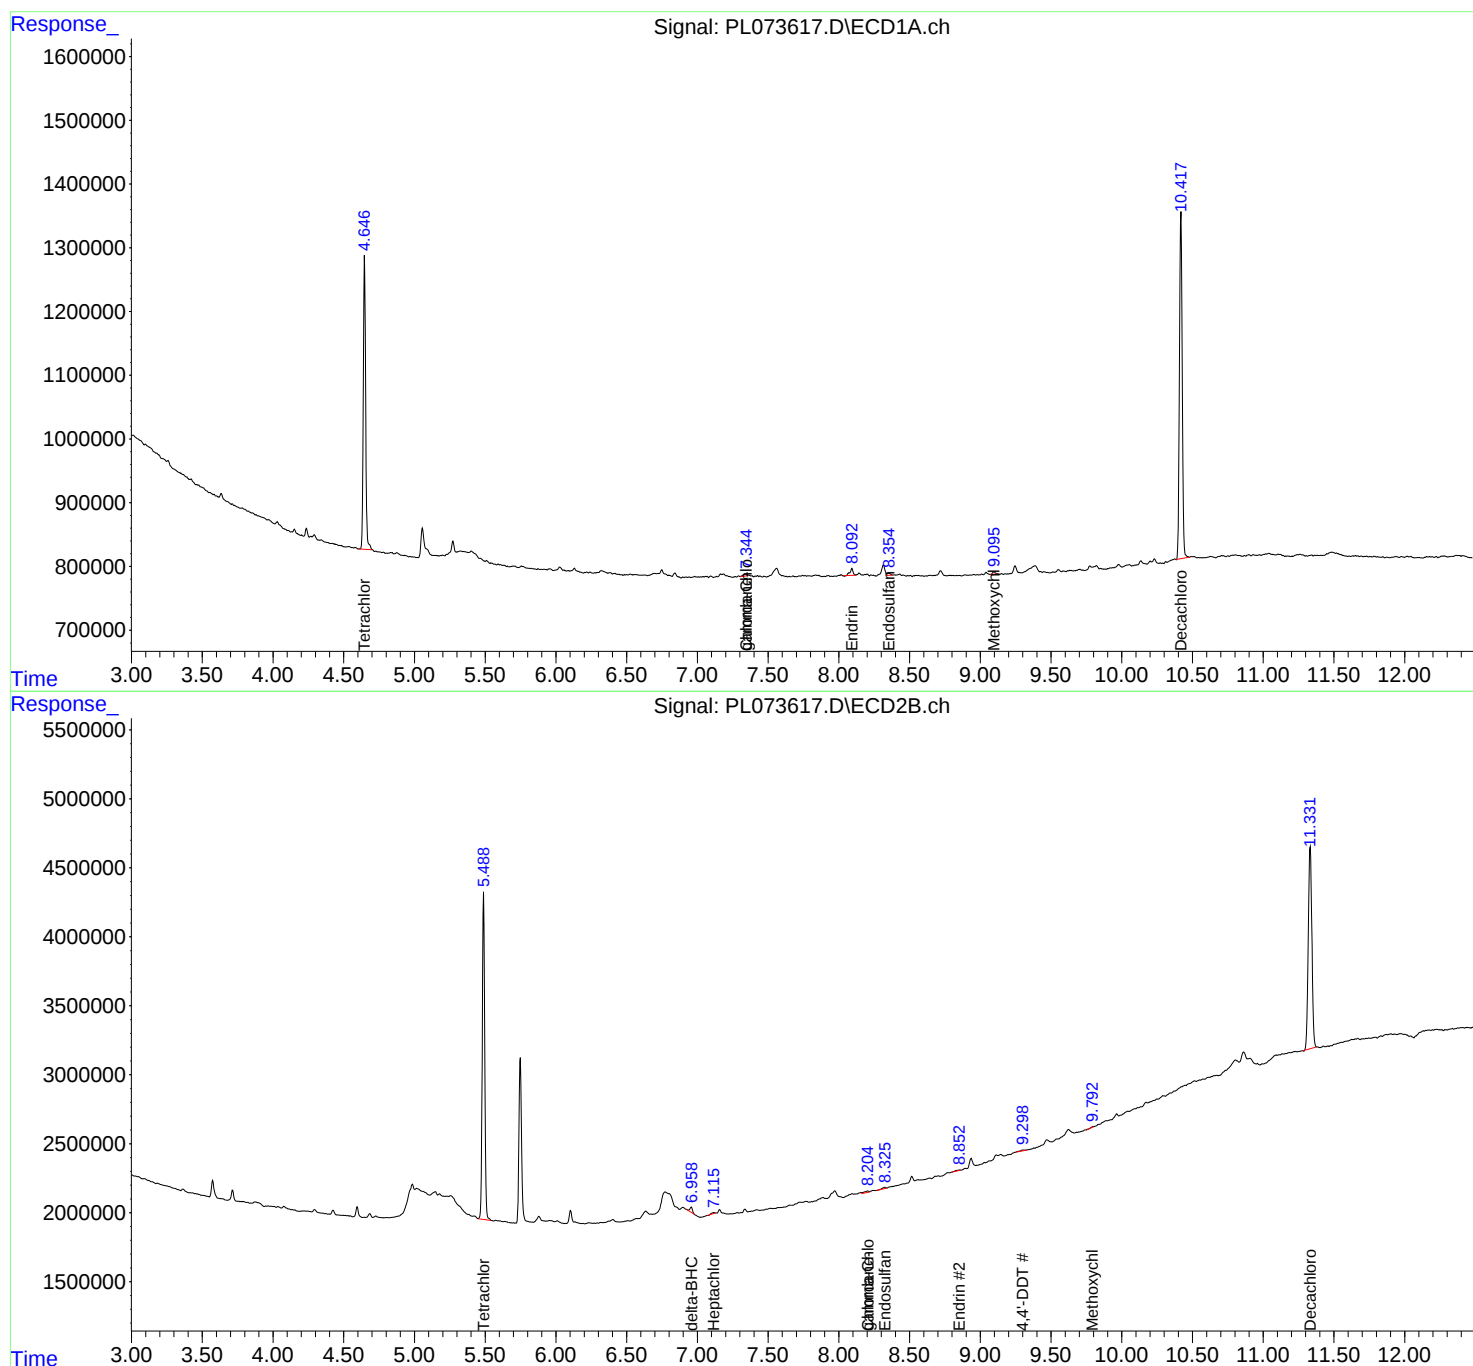


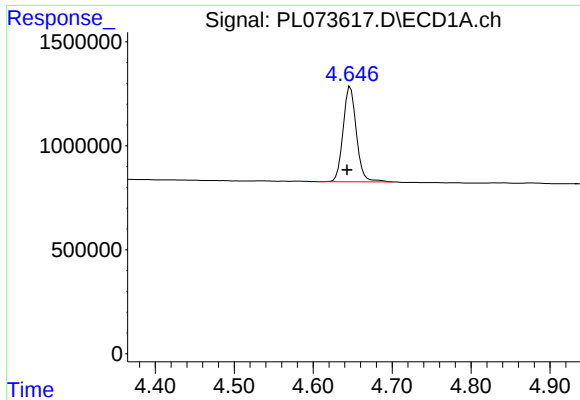

#1 Tetrachloro-m-xylene


R.T.: 4.647 min
Delta R.T.: 0.004 min
Response: 5342909
Conc: 16.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

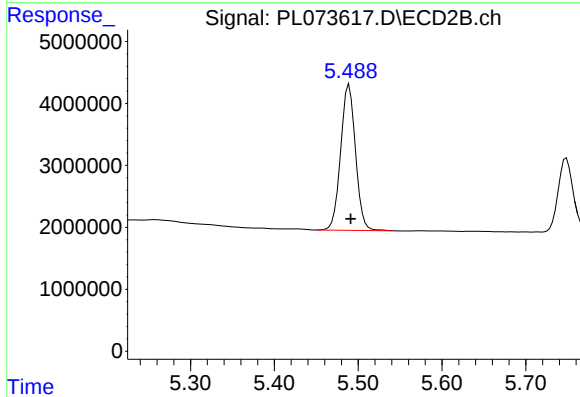


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 28998107
Conc: 17.67 ng/ml

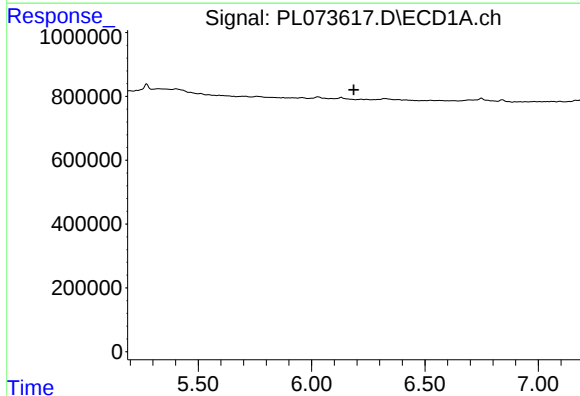


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 6.187 min
Response: 0
Conc: N.D.

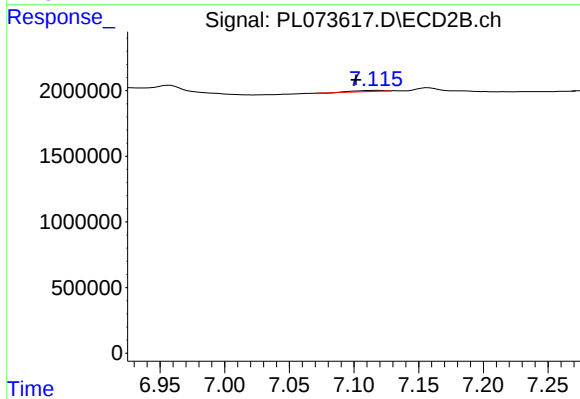

#4 Heptachlor


R.T.: 7.118 min
Delta R.T.: 0.016 min
Response: 108512
Conc: 0.05 ng/ml

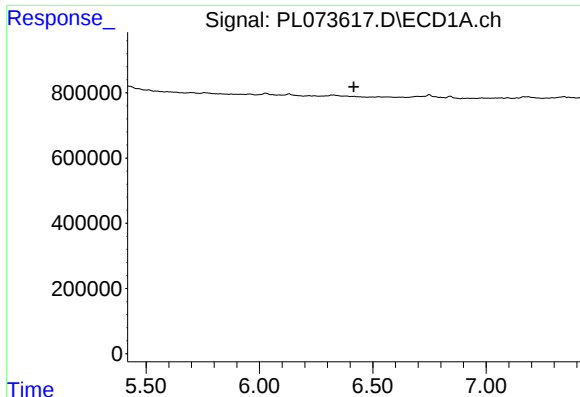

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

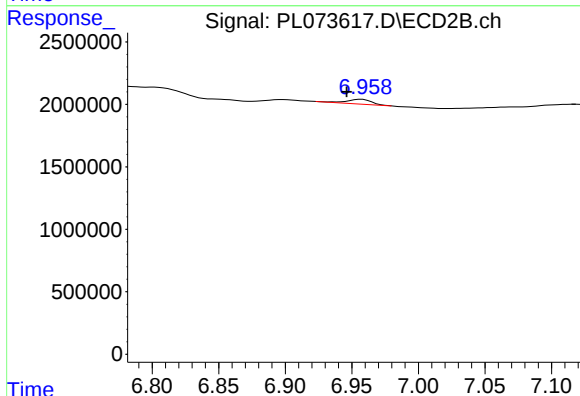


#7 delta-BHC

R.T.: 6.958 min
Delta R.T.: 0.011 min
Response: 460856
Conc: 0.21 ng/ml

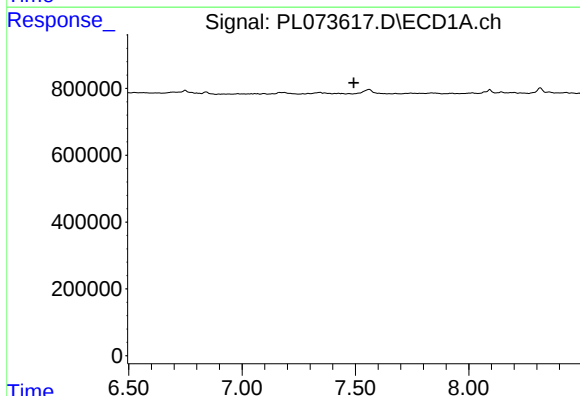


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.493 min
Response: 0
Conc: N.D.

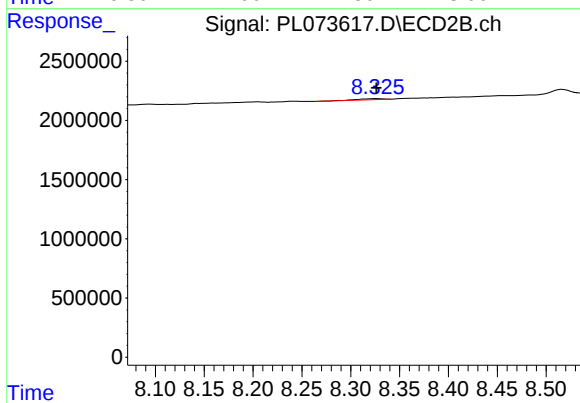

#9 Endosulfan I


R.T.: 8.326 min
Delta R.T.: 0.000 min
Response: 152684
Conc: 0.08 ng/ml

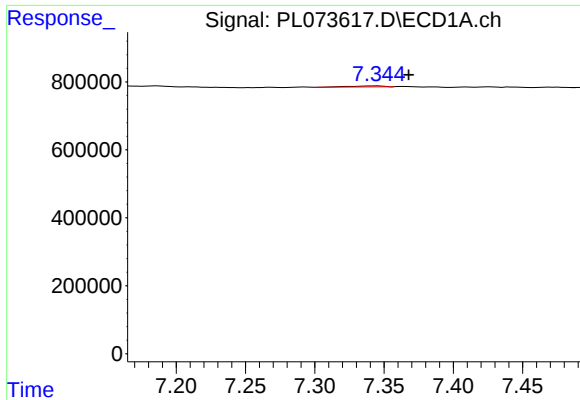

#10 gamma-Chlordane


R.T.: 7.345 min
Delta R.T.: -0.022 min
Response: 55302
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

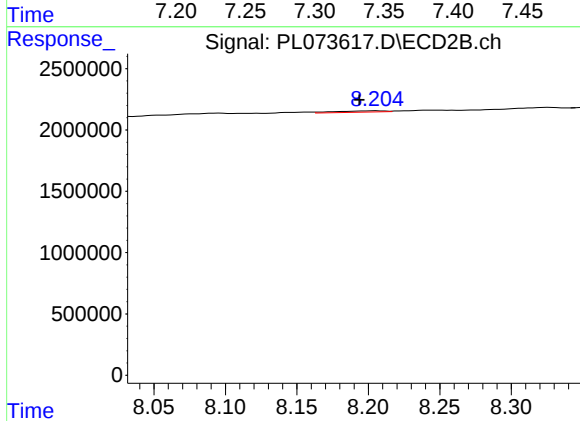


#10 gamma-Chlordane

R.T.: 8.205 min
Delta R.T.: 0.012 min
Response: 253256
Conc: 0.12 ng/ml

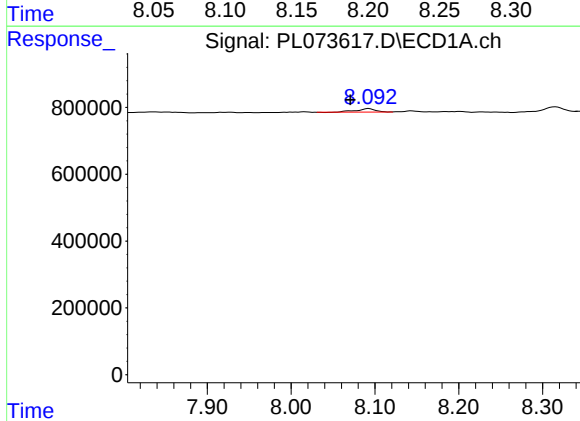


#14 Endrin

R.T.: 8.093 min
Delta R.T.: 0.022 min
Response: 161881
Conc: 0.42 ng/ml

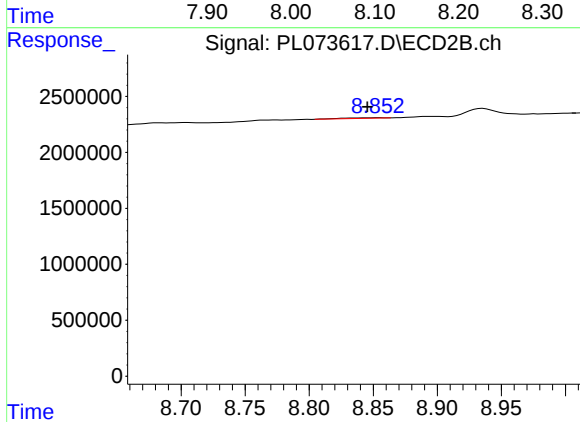

#14 Endrin


R.T.: 8.854 min
Delta R.T.: 0.009 min
Response: 100676
Conc: 0.07 ng/ml

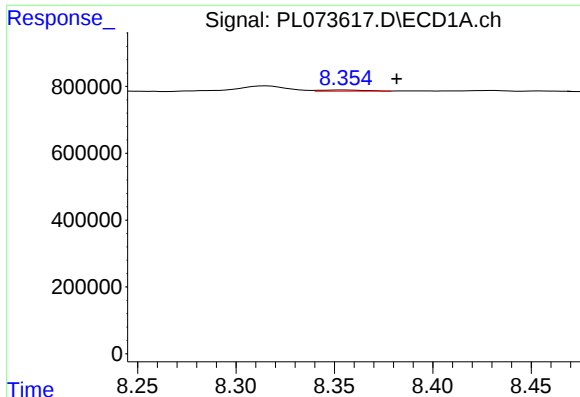

#15 Endosulfan II


R.T.: 8.356 min
Delta R.T.: -0.026 min
Response: 49901
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

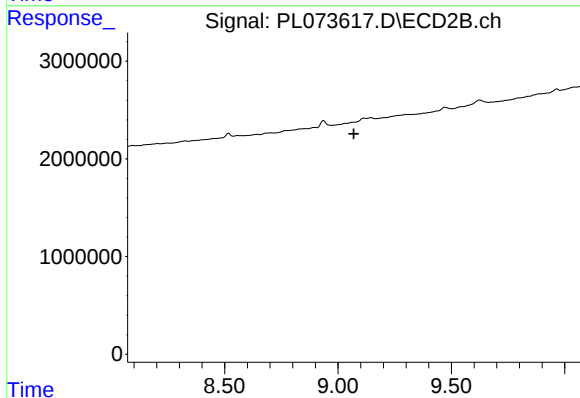


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

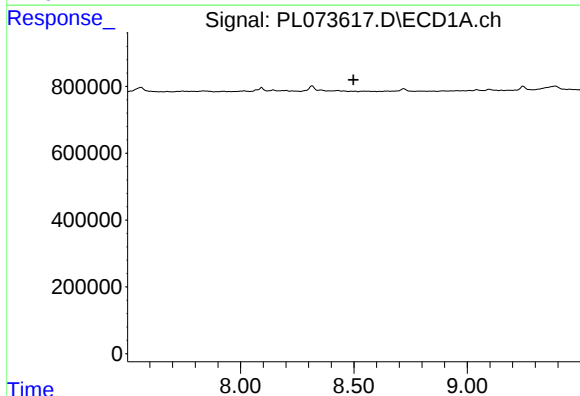


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.499 min
Response: 0
Conc: N.D.

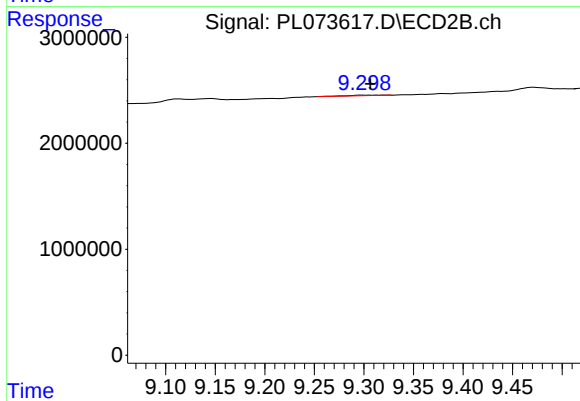

#17 4,4'-DDT


R.T.: 9.299 min
Delta R.T.: -0.007 min
Response: 134856
Conc: 0.08 ng/ml

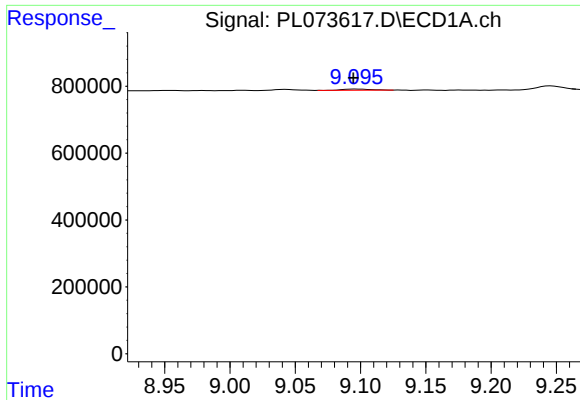

#20 Methoxychlor


R.T.: 9.097 min
Delta R.T.: 0.002 min
Response: 48791
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

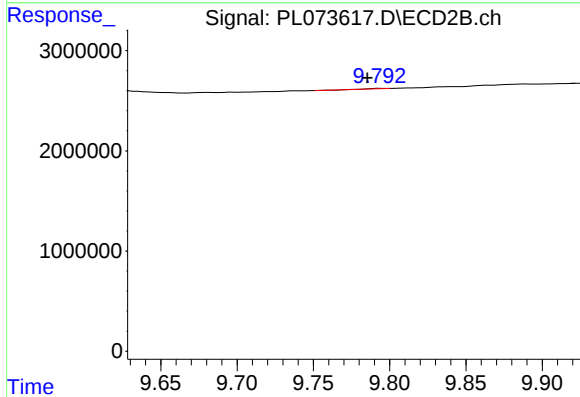


#20 Methoxychlor

R.T.: 9.795 min
Delta R.T.: 0.009 min
Response: 28862
Conc: 0.03 ng/ml

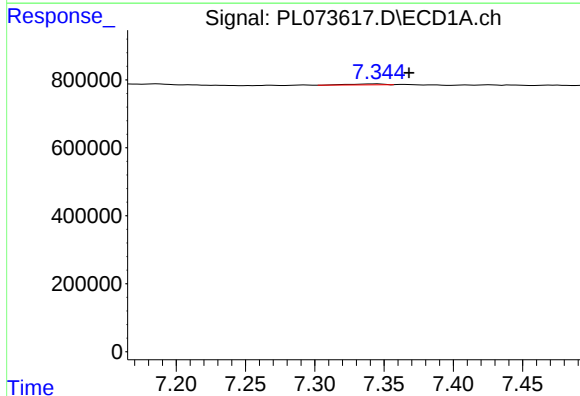


#25 Chlordane-3

R.T.: 7.345 min
Delta R.T.: -0.023 min
Response: 55302
Conc: 1.35 ng/ml

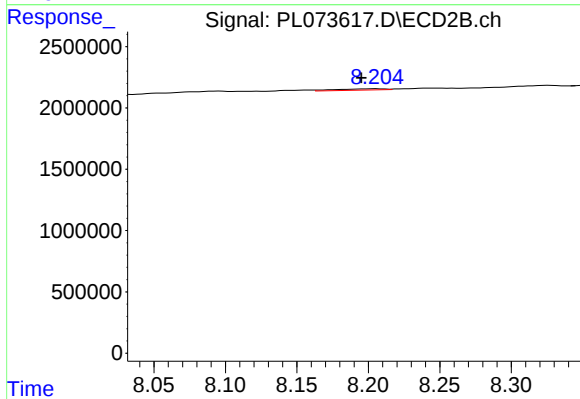

#25 Chlordane-3


R.T.: 8.205 min
Delta R.T.: 0.010 min
Response: 253256
Conc: 0.93 ng/ml

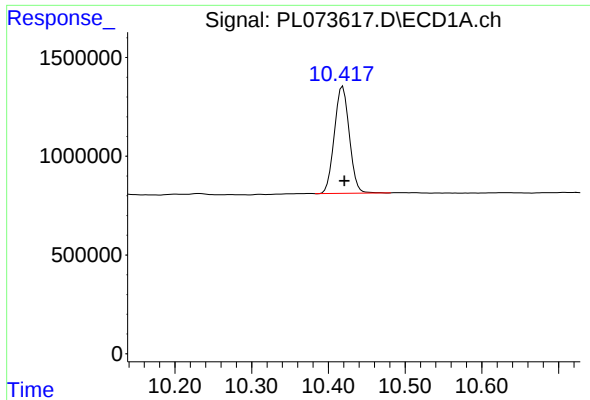

#28 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: -0.002 min
Response: 7354204
Conc: 14.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

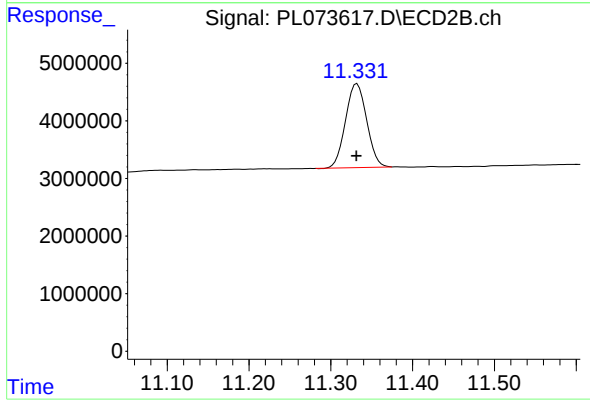

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 26177493
Conc: 14.64 ng/ml