

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 20:09
 Operator : AR\AJ
 Sample : PB143542BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:33:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.640	5.491	5453854	28430369	17.028	17.322
28)	SA Decachlor...	10.415	11.332	9251986	32590035	18.195	18.225
Target Compounds							
2)	A alpha-BHC	5.375f	0.000	88762	0	0.215	N.D. #
6)	B beta-BHC	0.000	6.681	0	879341	N.D.	0.844 #
7)	B delta-BHC	0.000	6.958	0	2316478	N.D.	1.076 #
9)	A Endosulfan I	0.000	8.325	0	25603	N.D.	0.014 #
14)	MA Endrin	8.090f	0.000	111426	0	0.287	N.D. #
15)	B Endosulfa...	0.000	9.054f	0	1162919	N.D.	0.757 #
16)	A 4,4'-DDD	0.000	8.969f	0	64616	N.D.	0.044 #
17)	MA 4,4'-DDT	0.000	9.292	0	96257	N.D.	0.059 #
18)	B Endrin al...	0.000	9.203	0	86051	N.D.	0.070 #
19)	B Endosulfa...	0.000	9.443	0	62084	N.D.	0.039 #
23)	Chlordane-1	0.000	6.849	0	1014529	N.D.	14.851 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 20:09
Operator : AR\AJ
Sample : PB143542BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:33:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

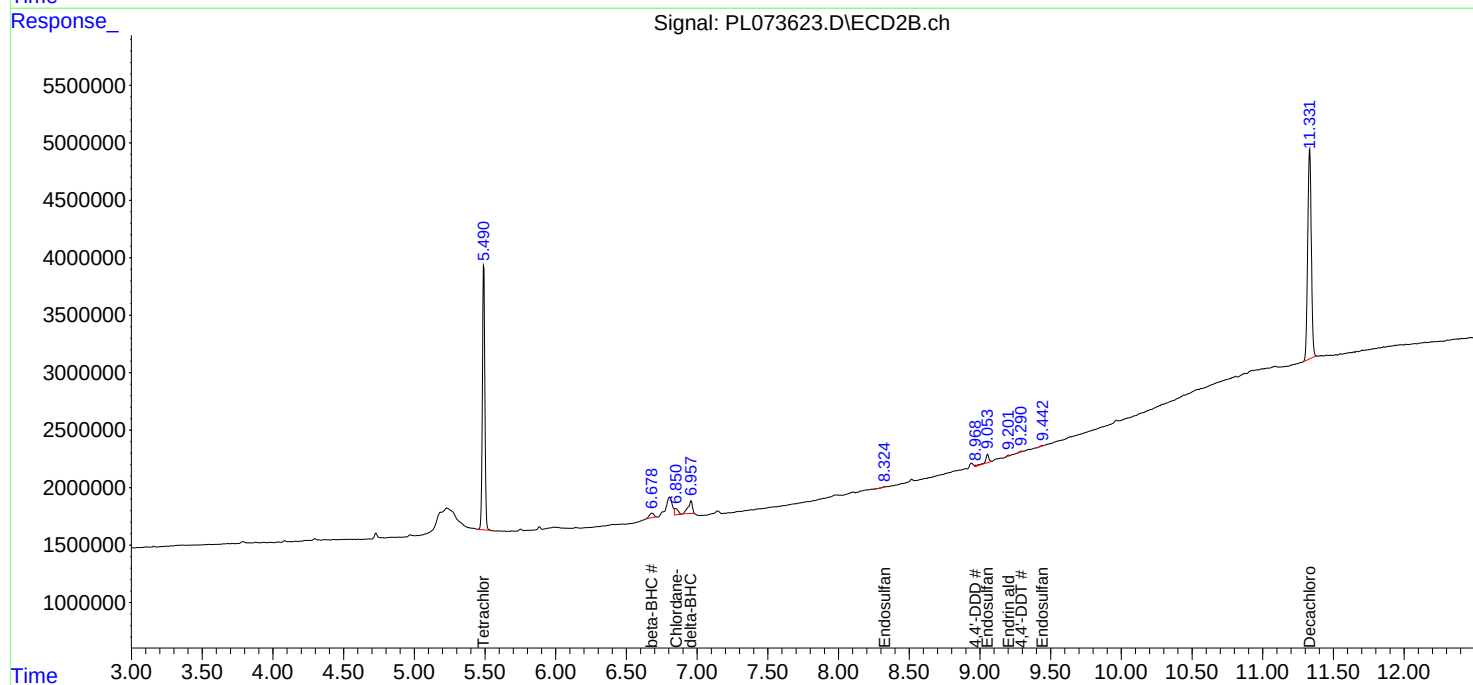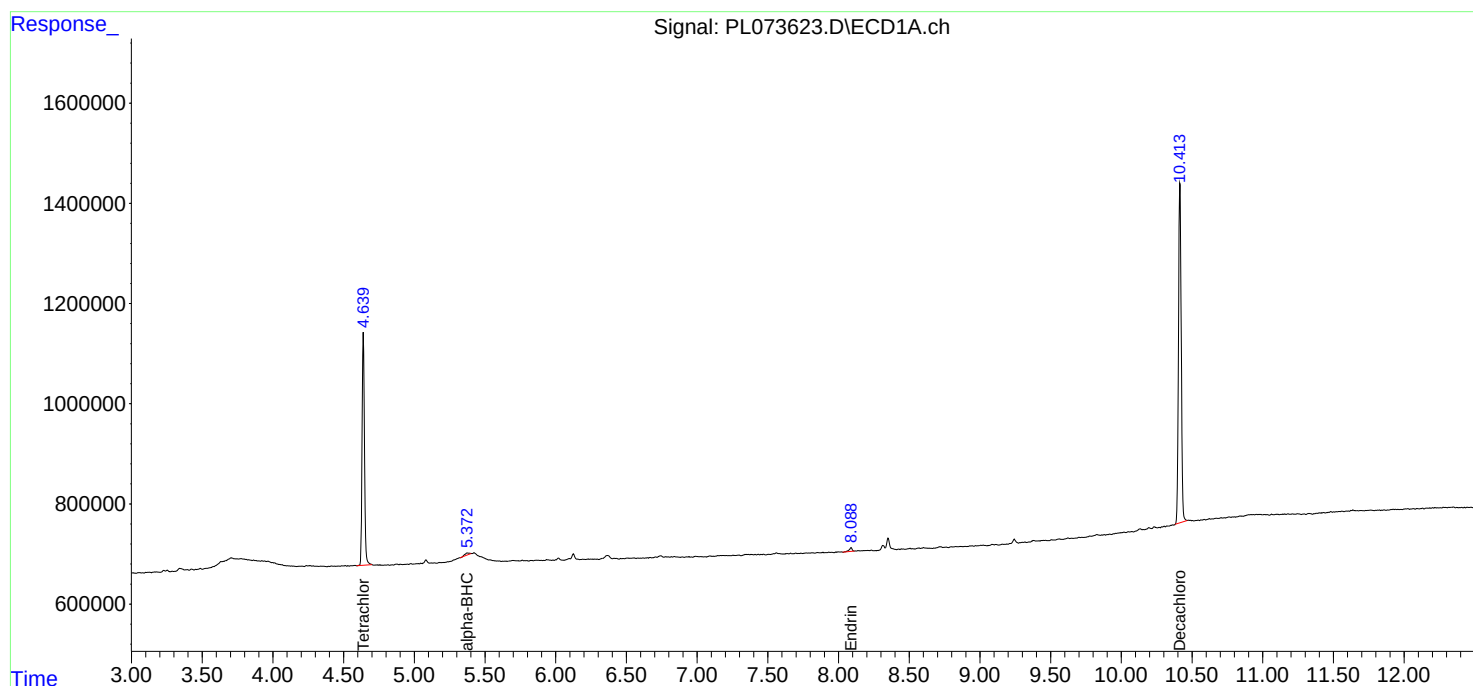


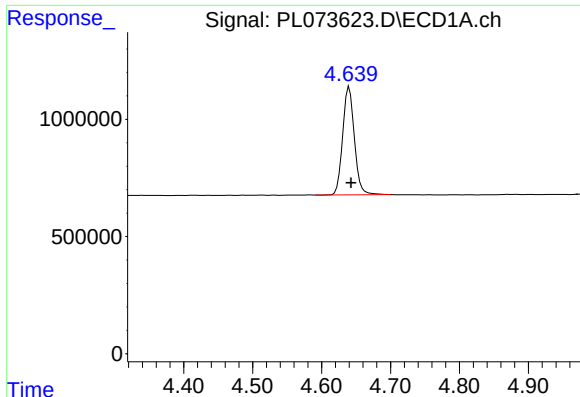

#1 Tetrachloro-m-xylene


R.T.: 4.640 min
Delta R.T.: -0.003 min
Response: 5453854
Conc: 17.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

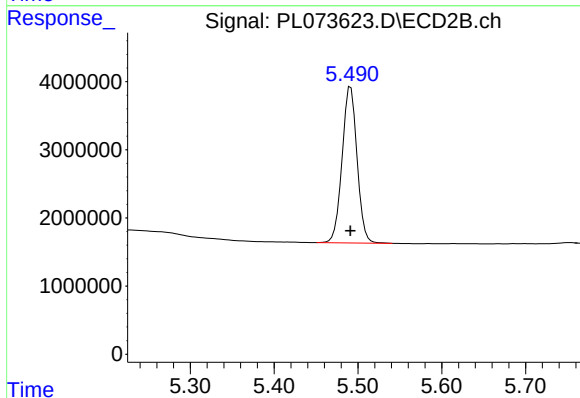


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 28430369
Conc: 17.32 ng/ml

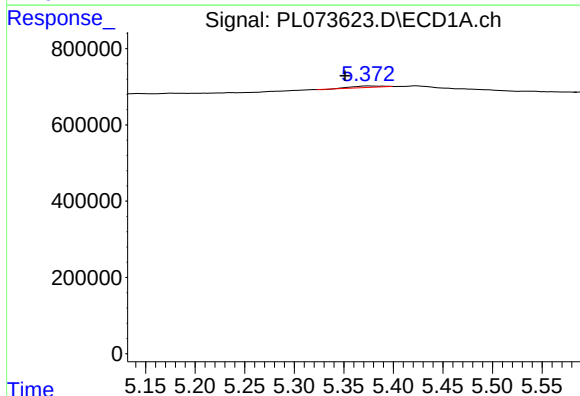


#2 alpha-BHC

R.T.: 5.375 min
Delta R.T.: 0.024 min
Response: 88762
Conc: 0.22 ng/ml

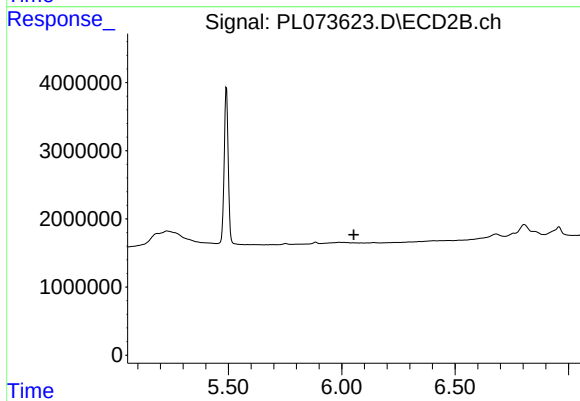

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

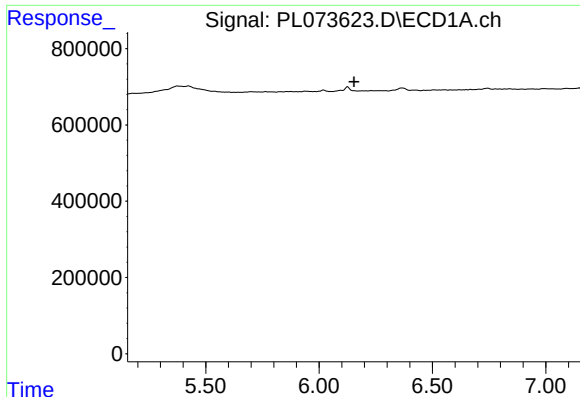

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

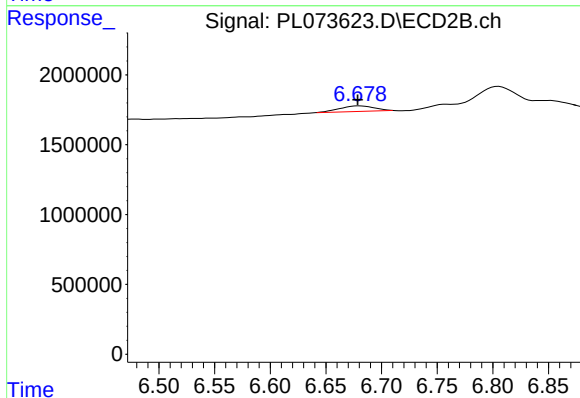


#6 beta-BHC

R.T.: 6.681 min
Delta R.T.: 0.002 min
Response: 879341
Conc: 0.84 ng/ml

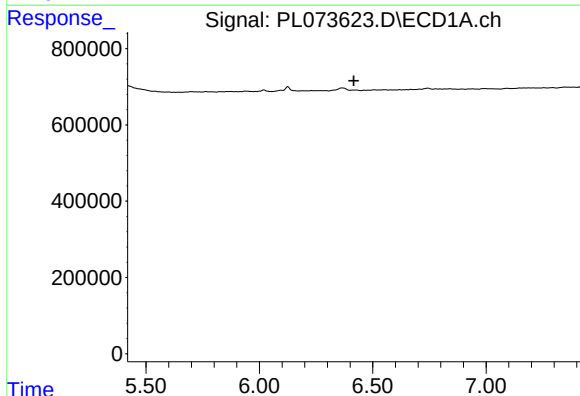


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

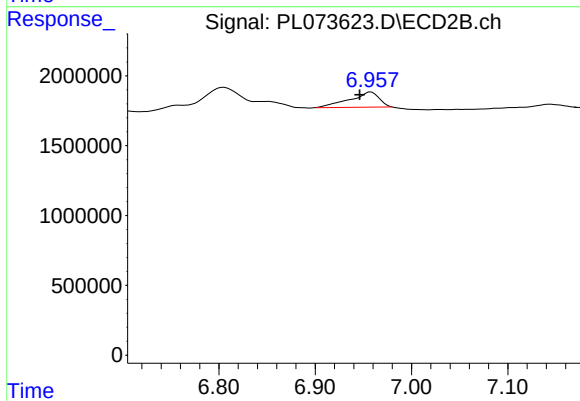

#7 delta-BHC


R.T.: 6.958 min
Delta R.T.: 0.012 min
Response: 2316478
Conc: 1.08 ng/ml

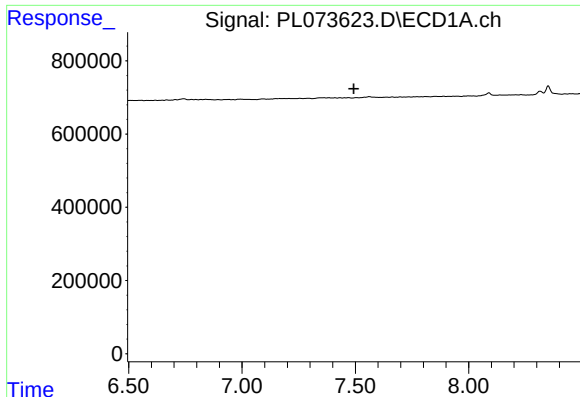

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.493 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

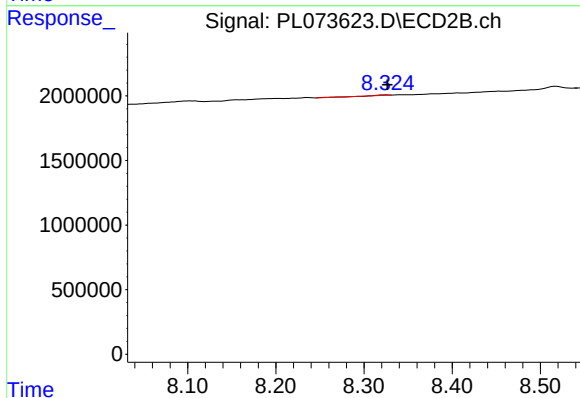


#9 Endosulfan I

R.T.: 8.325 min
Delta R.T.: -0.002 min
Response: 25603
Conc: 0.01 ng/ml

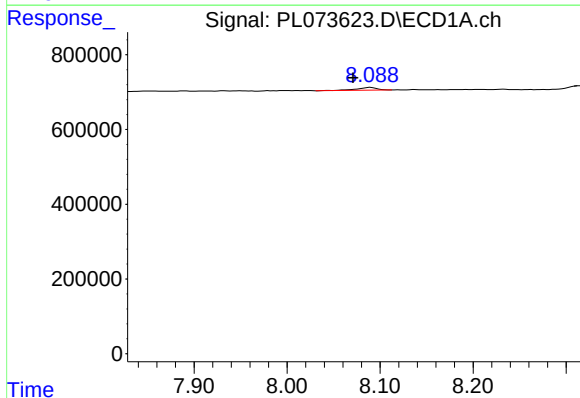


#14 Endrin

R.T.: 8.090 min
Delta R.T.: 0.019 min
Response: 111426
Conc: 0.29 ng/ml

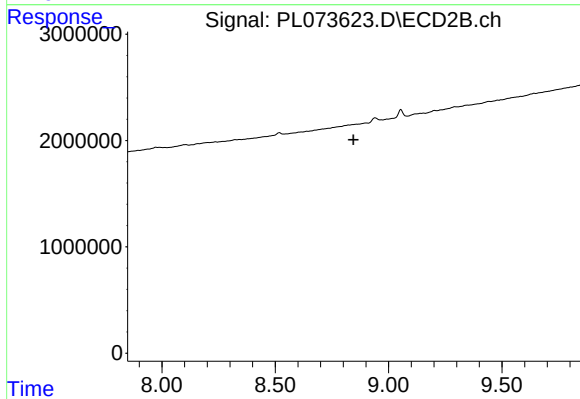

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.845 min
Response: 0
Conc: N.D.

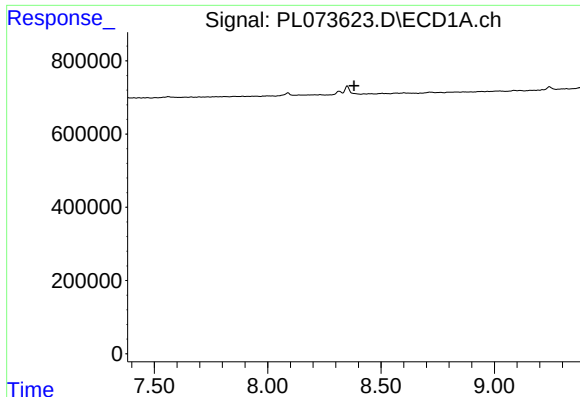

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

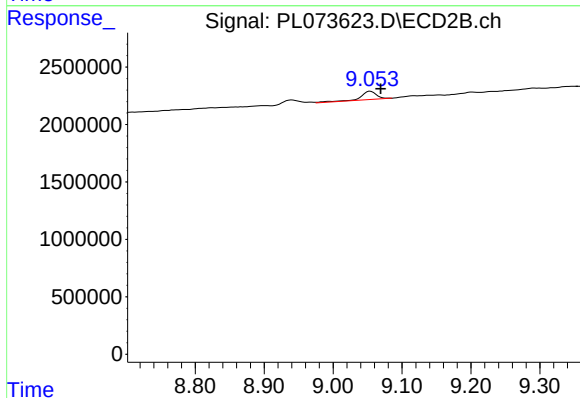


#15 Endosulfan II

R.T.: 9.054 min
Delta R.T.: -0.015 min
Response: 1162919
Conc: 0.76 ng/ml

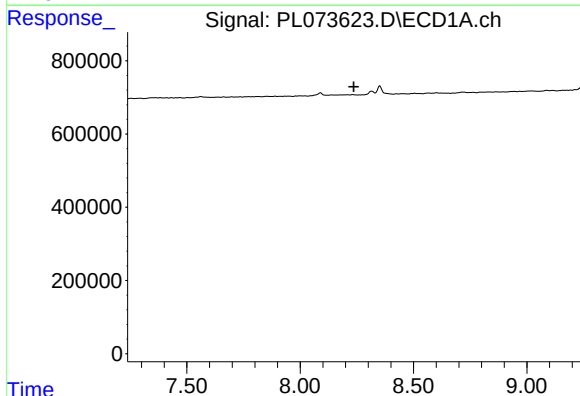


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.237 min
Response: 0
Conc: N.D.

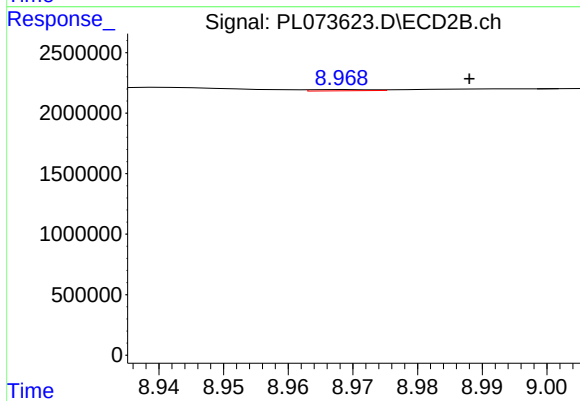

#16 4,4'-DDD


R.T.: 8.969 min
Delta R.T.: -0.019 min
Response: 64616
Conc: 0.04 ng/ml

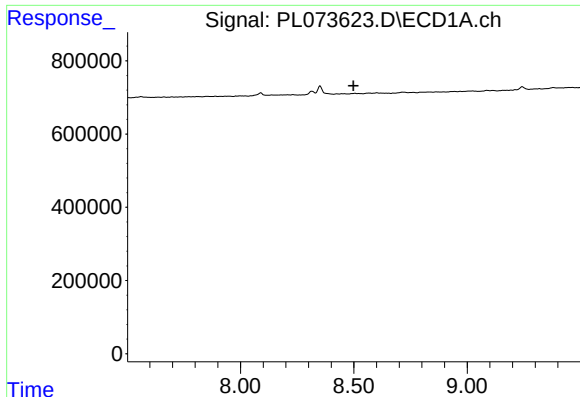

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

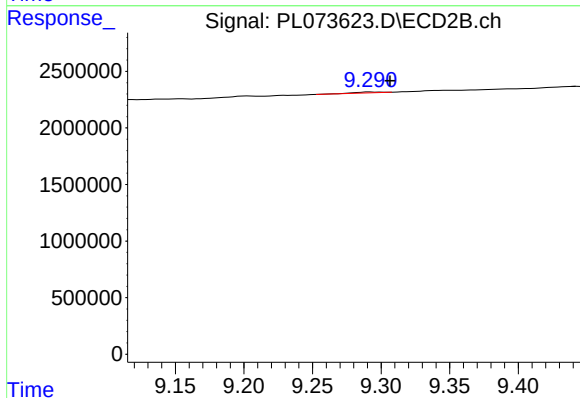


#17 4,4'-DDT

R.T.: 9.292 min
Delta R.T.: -0.015 min
Response: 96257
Conc: 0.06 ng/ml

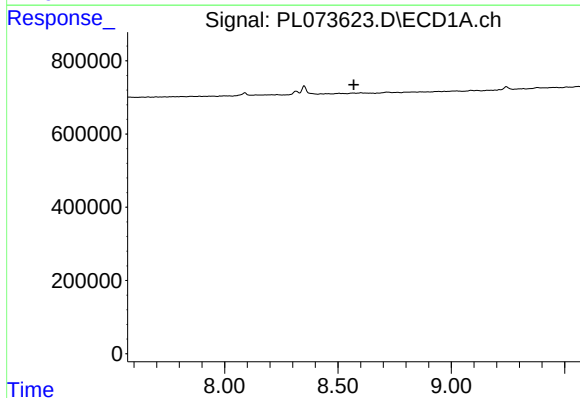


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.570 min
Response: 0
Conc: N.D.

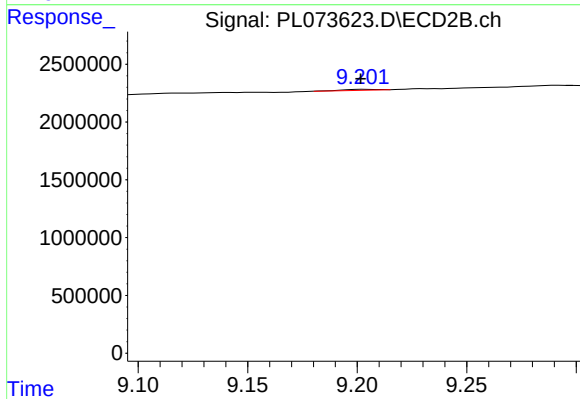

#18 Endrin aldehyde


R.T.: 9.203 min
Delta R.T.: 0.000 min
Response: 86051
Conc: 0.07 ng/ml

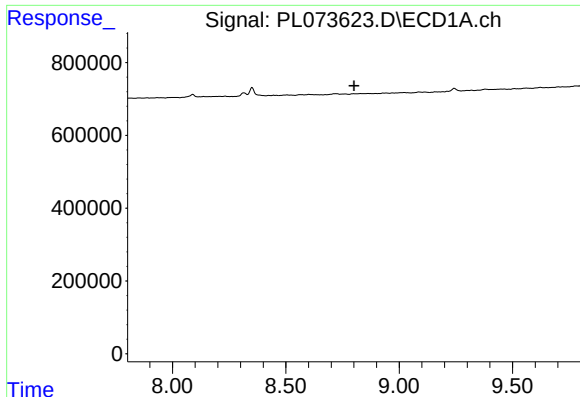

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 8.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

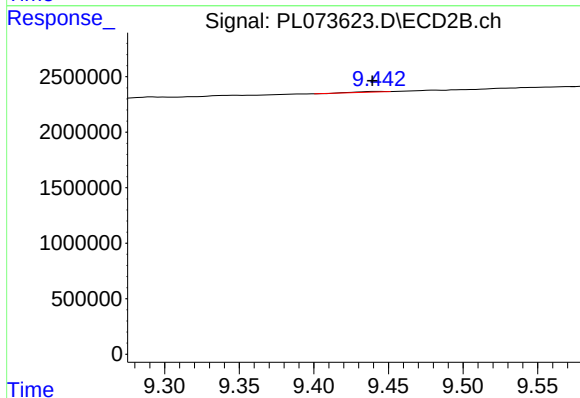


#19 Endosulfan Sulfate

R.T.: 9.443 min
Delta R.T.: 0.004 min
Response: 62084
Conc: 0.04 ng/ml

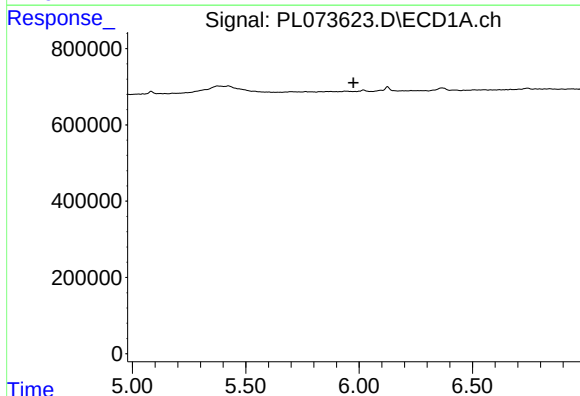


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

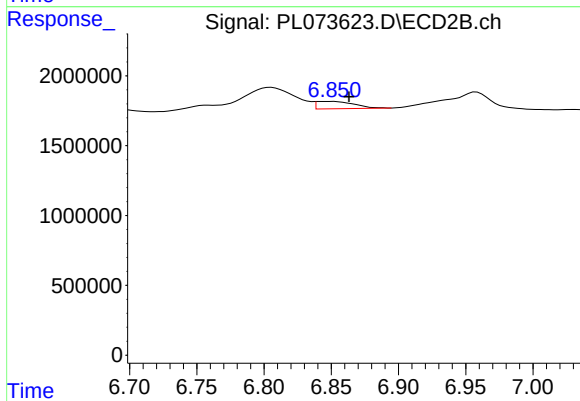

#23 Chlordane-1


R.T.: 6.849 min
Delta R.T.: -0.014 min
Response: 1014529
Conc: 14.85 ng/ml

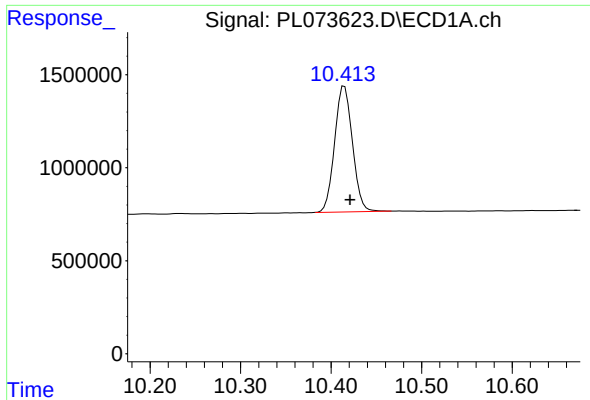

#28 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.006 min
Response: 9251986
Conc: 18.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

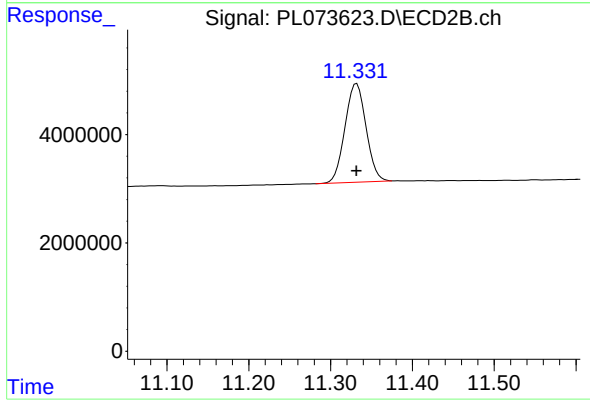

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 32590035
Conc: 18.23 ng/ml