

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073625.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 20:42
 Operator : AR\AJ
 Sample : PB143528TB
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:34:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.640	5.491	5446545	28621622	17.005	17.439
28)	SA Decachlor...	10.414	11.331	9395322	32630175	18.477	18.248
Target Compounds							
6)	B beta-BHC	0.000	6.678	0	714974	N.D.	0.686 #
7)	B delta-BHC	0.000	6.956	0	2257188	N.D.	1.048 #
9)	A Endosulfan I	0.000	8.325	0	158763	N.D.	0.087 #
10)	B gamma-Chl...	7.348f	8.194	34112	666595	0.078	0.326 #
11)	B alpha-Chl...	0.000	8.254f	0	140276	N.D.	0.070 #
14)	MA Endrin	8.089f	0.000	138583	0	0.357	N.D. #
18)	B Endrin al...	0.000	9.200	0	67892	N.D.	0.055 #
20)	A Methoxychlor	0.000	9.786	0	32659	N.D.	0.036 #
23)	Chlordane-1	0.000	6.853	0	1174286	N.D.	17.190 #
25)	Chlordane-3	7.348f	8.194	34112	666595	0.835	2.459 #
26)	Chlordane-4	0.000	8.254f	0	140276	N.D.	0.423 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073625.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 20:42
Operator : AR\AJ
Sample : PB143528TB
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:34:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

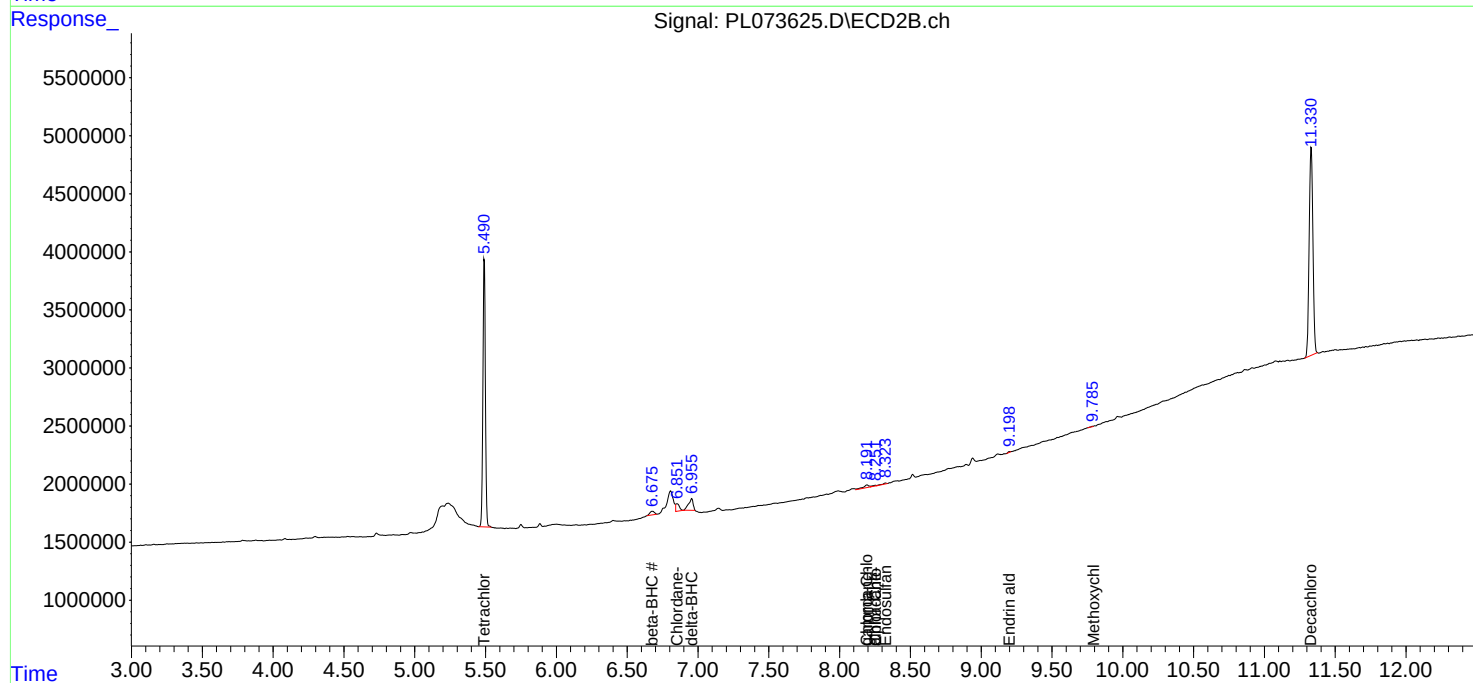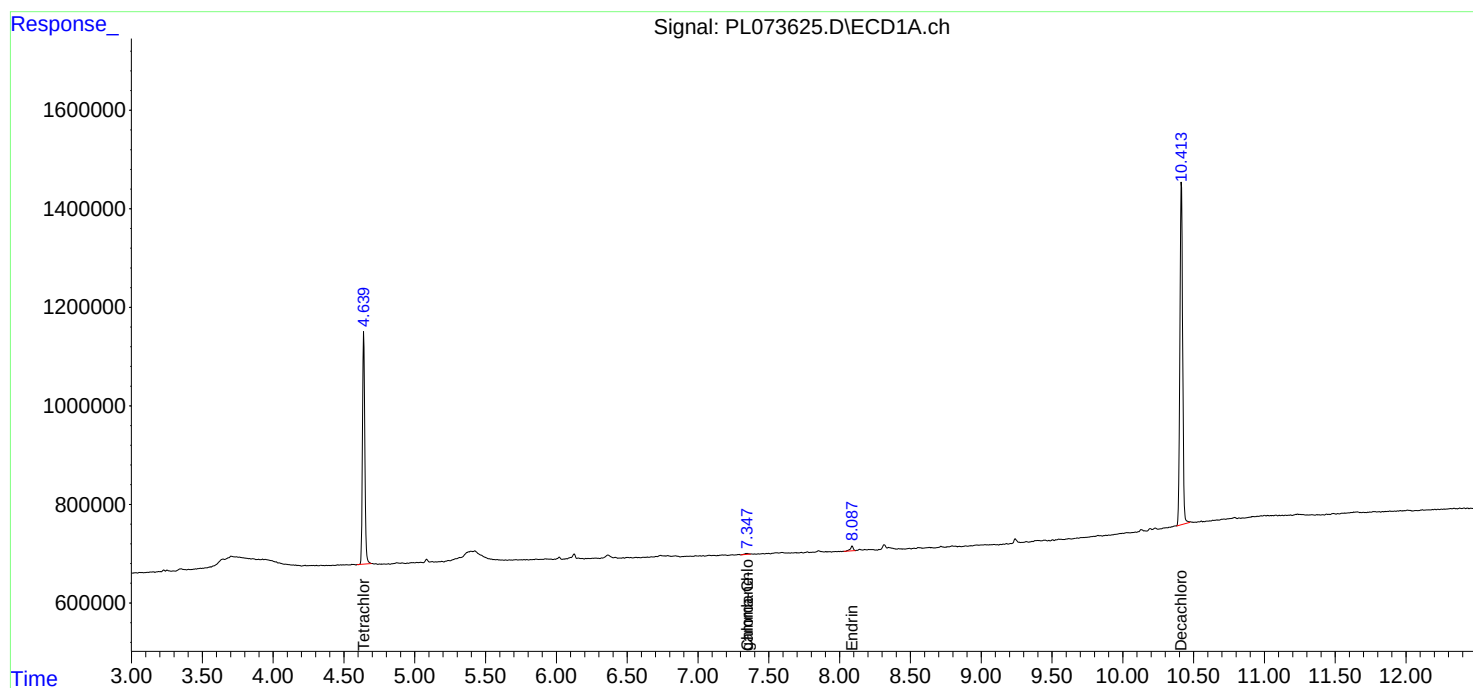


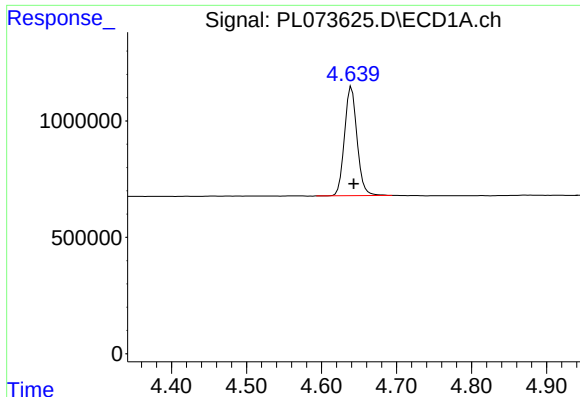

#1 Tetrachloro-m-xylene


R.T.: 4.640 min
Delta R.T.: -0.003 min
Response: 5446545
Conc: 17.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

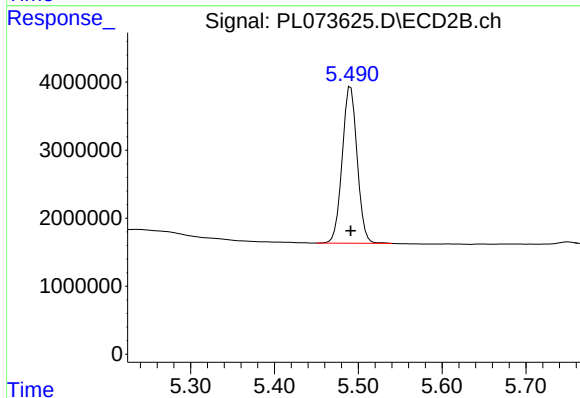


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 28621622
Conc: 17.44 ng/ml

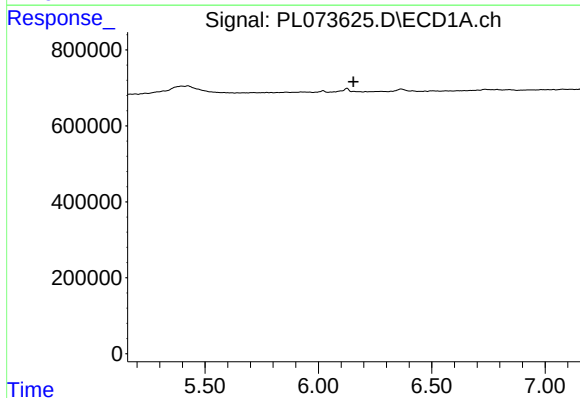


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

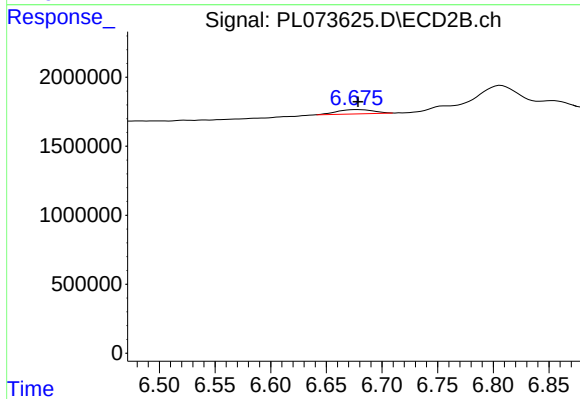

#6 beta-BHC


R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 714974
Conc: 0.69 ng/ml

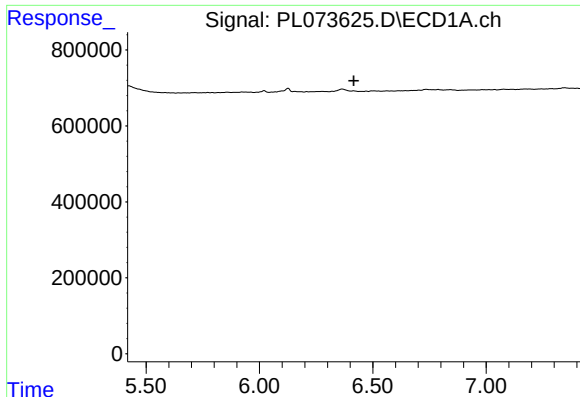

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

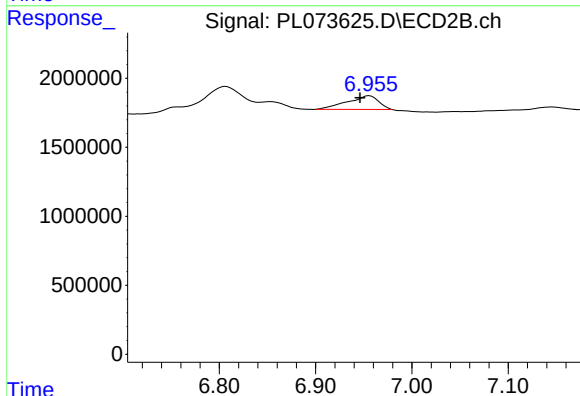


#7 delta-BHC

R.T.: 6.956 min
Delta R.T.: 0.010 min
Response: 2257188
Conc: 1.05 ng/ml

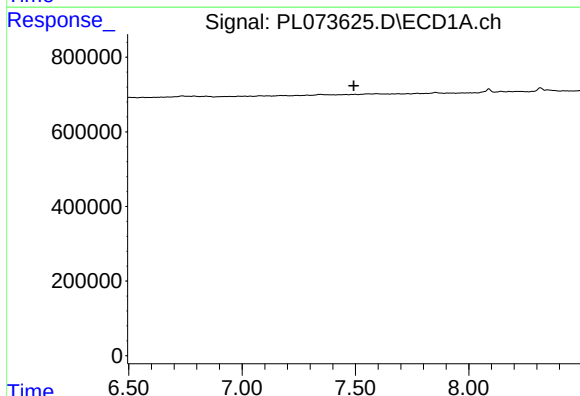


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.493 min
Response: 0
Conc: N.D.

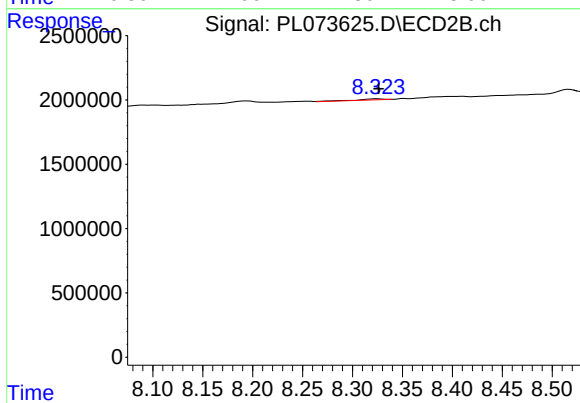

#9 Endosulfan I


R.T.: 8.325 min
Delta R.T.: -0.002 min
Response: 158763
Conc: 0.09 ng/ml

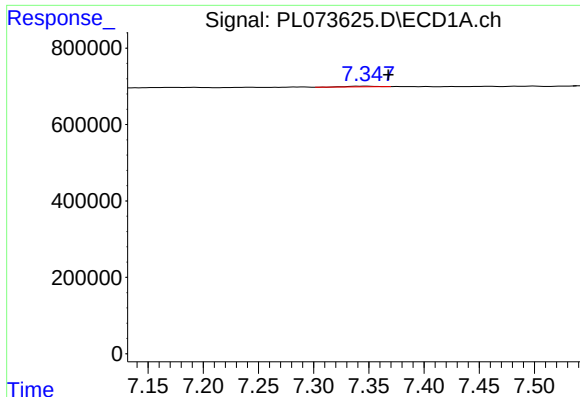

#10 gamma-Chlordane


R.T.: 7.348 min
Delta R.T.: -0.020 min
Response: 34112
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

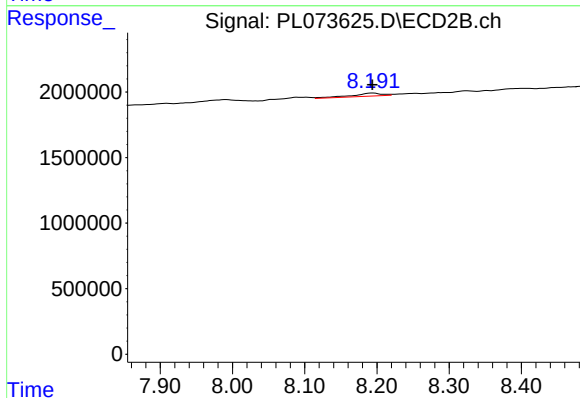


#10 gamma-Chlordane

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 666595
Conc: 0.33 ng/ml

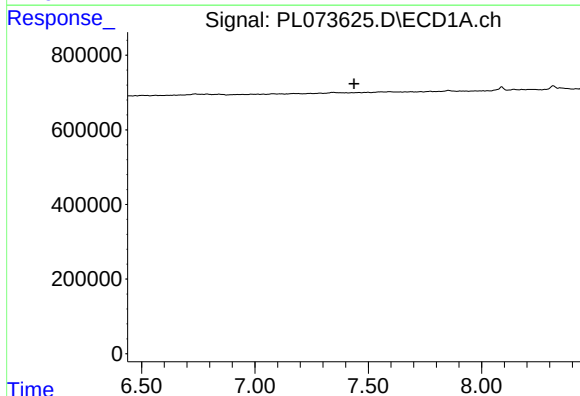


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.437 min
Response: 0
Conc: N.D.

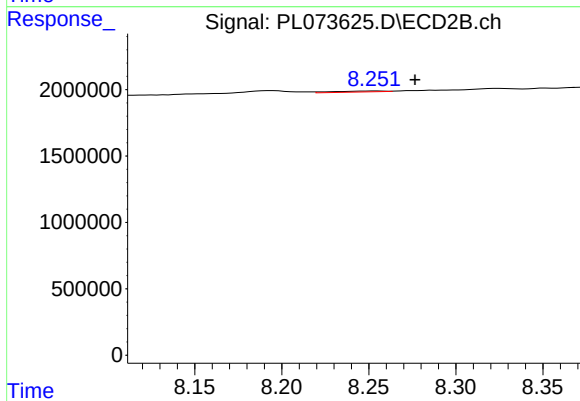

#11 alpha-Chlordane


R.T.: 8.254 min
Delta R.T.: -0.023 min
Response: 140276
Conc: 0.07 ng/ml

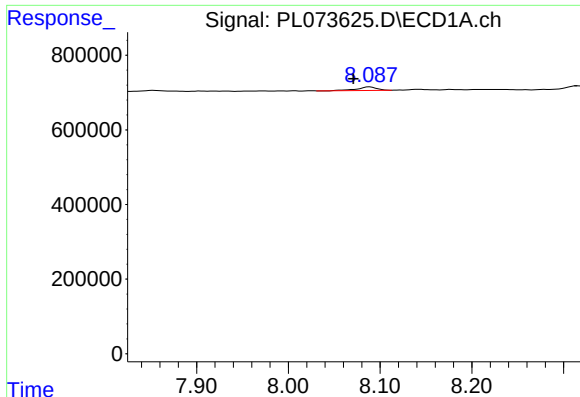

#14 Endrin


R.T.: 8.089 min
Delta R.T.: 0.018 min
Response: 138583
Conc: 0.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

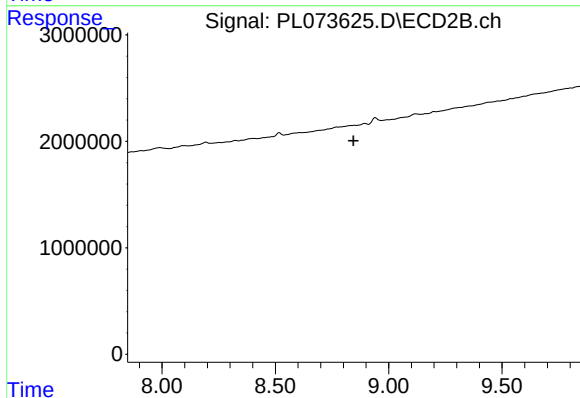


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

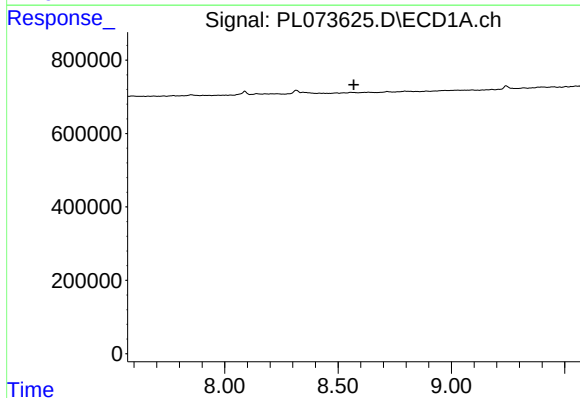


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 8.570 min
Response: 0
Conc: N.D.

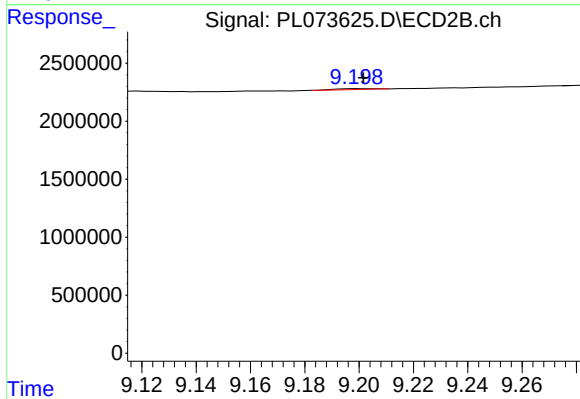

#18 Endrin aldehyde


R.T.: 9.200 min
Delta R.T.: -0.002 min
Response: 67892
Conc: 0.06 ng/ml

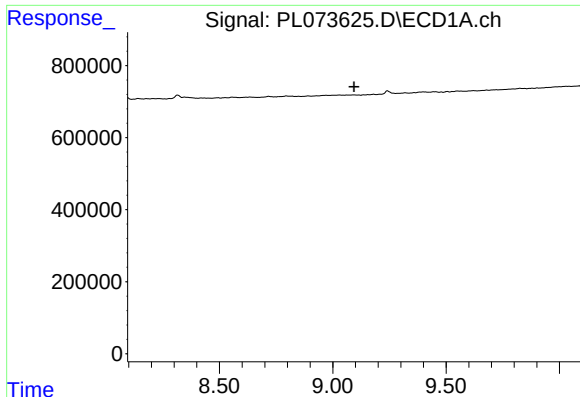

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

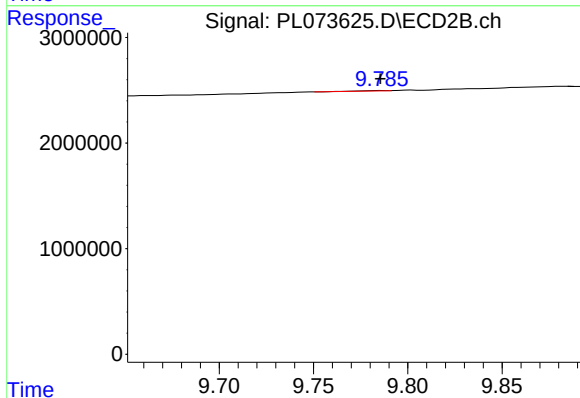


#20 Methoxychlor

R.T.: 9.786 min
Delta R.T.: 0.000 min
Response: 32659
Conc: 0.04 ng/ml

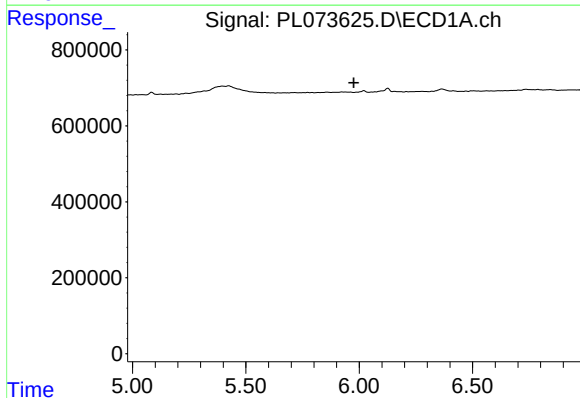


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

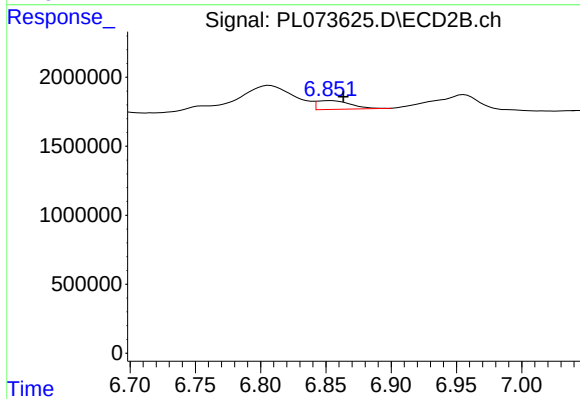

#23 Chlordane-1


R.T.: 6.853 min
Delta R.T.: -0.010 min
Response: 1174286
Conc: 17.19 ng/ml

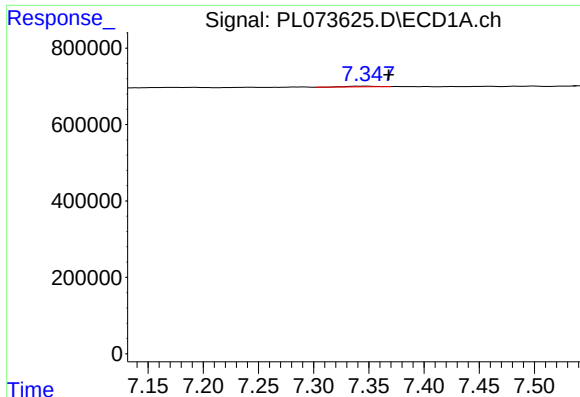

#25 Chlordane-3


R.T.: 7.348 min
Delta R.T.: -0.020 min
Response: 34112
Conc: 0.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

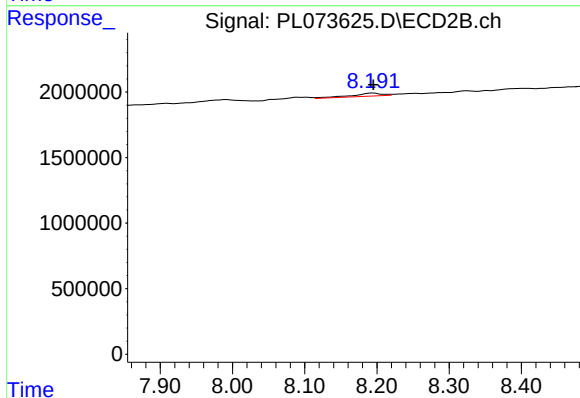


#25 Chlordane-3

R.T.: 8.194 min
Delta R.T.: -0.001 min
Response: 666595
Conc: 2.46 ng/ml

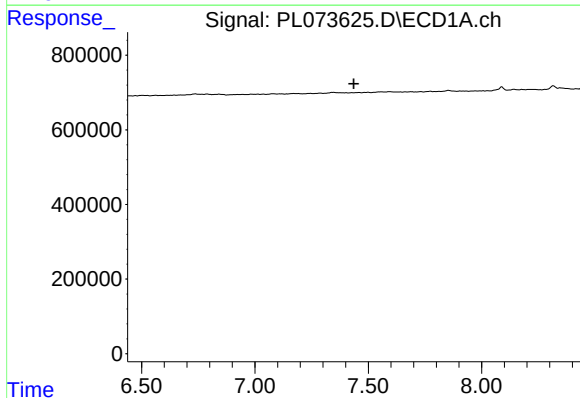


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.437 min
Response: 0
Conc: N.D.

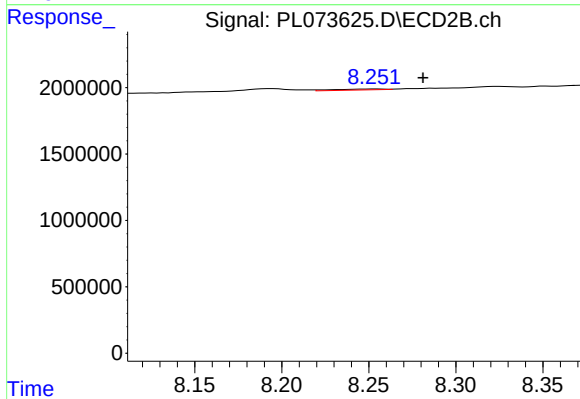

#26 Chlordane-4


R.T.: 8.254 min
Delta R.T.: -0.028 min
Response: 140276
Conc: 0.42 ng/ml

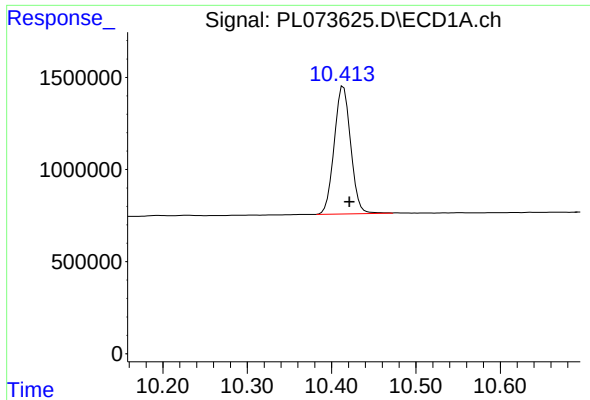

#28 Decachlorobiphenyl

R.T.: 10.414 min
Delta R.T.: -0.007 min
Response: 9395322
Conc: 18.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

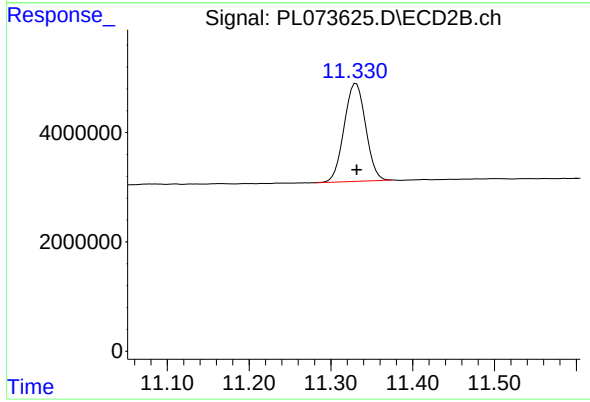

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.000 min
Response: 32630175
Conc: 18.25 ng/ml