

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 23:27
 Operator : AR\AJ
 Sample : N2063-06
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:35:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.492	6067461	32196002	18.944	19.617
2)	SA Decachlor...	10.416	11.332	10218700	35127885	20.096	19.645
Target Compounds							
2)	A alpha-BHC	5.370f	0.000	10134	0	0.025	N.D. #
6)	B beta-BHC	0.000	6.677	0	763331	N.D.	0.732 #
7)	B delta-BHC	6.415	6.940	39846	1324727	0.099	0.615 #
10)	B gamma-Chl...	0.000	8.195	0	375013	N.D.	0.184 #
12)	B 4,4'-DDE	0.000	8.464	0	71523	N.D.	0.040 #
13)	MA Dieldrin	7.782	0.000	24576	0	0.059	N.D. #
14)	MA Endrin	8.091f	0.000	70257	0	0.181	N.D. #
15)	B Endosulfa...	8.375	9.067	33201	134369	0.085	0.087
16)	A 4,4'-DDD	0.000	8.973	0	161513	N.D.	0.111 #
23)	Chlordane-1	0.000	6.852	0	1263537	N.D.	18.496 #
25)	Chlordane-3	0.000	8.195	0	375013	N.D.	1.383 #
27)	Chlordane-5	8.375	0.000	33201	0	2.028	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 23:27
Operator : AR\AJ
Sample : N2063-06
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:35:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

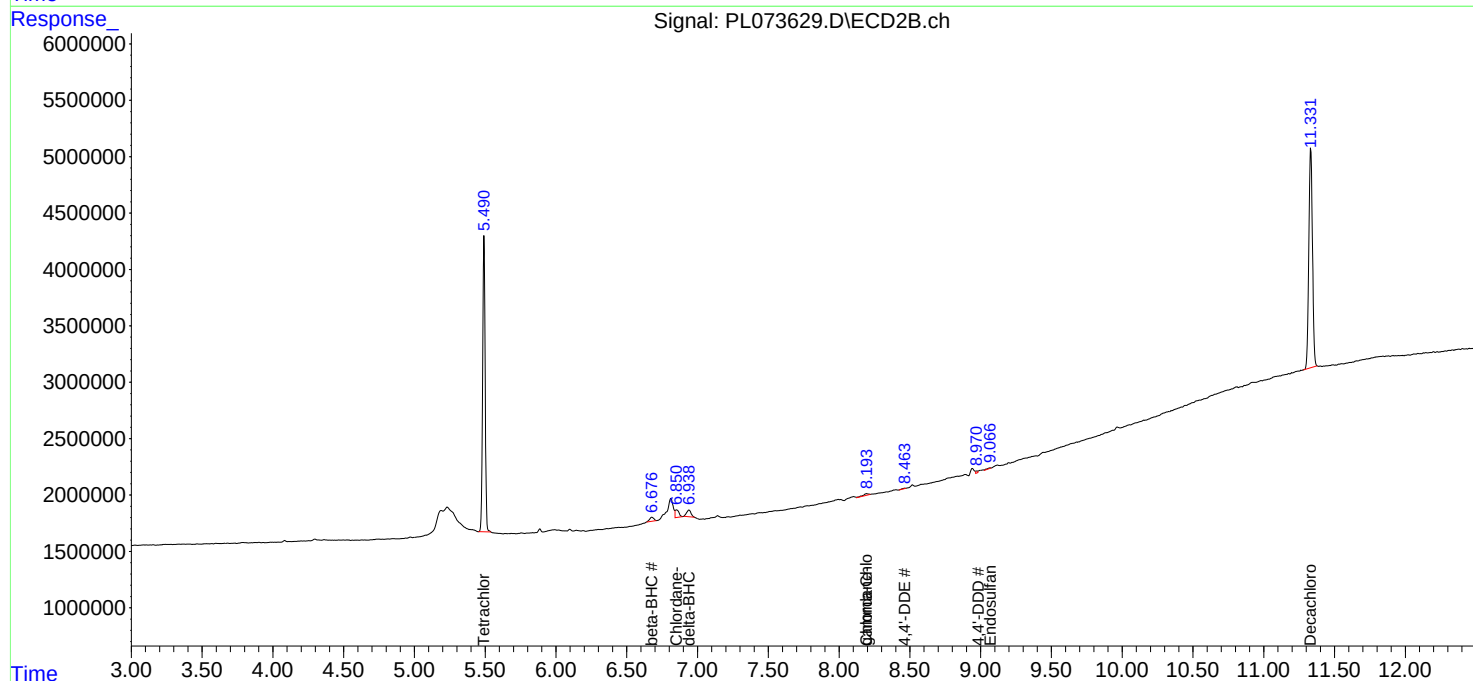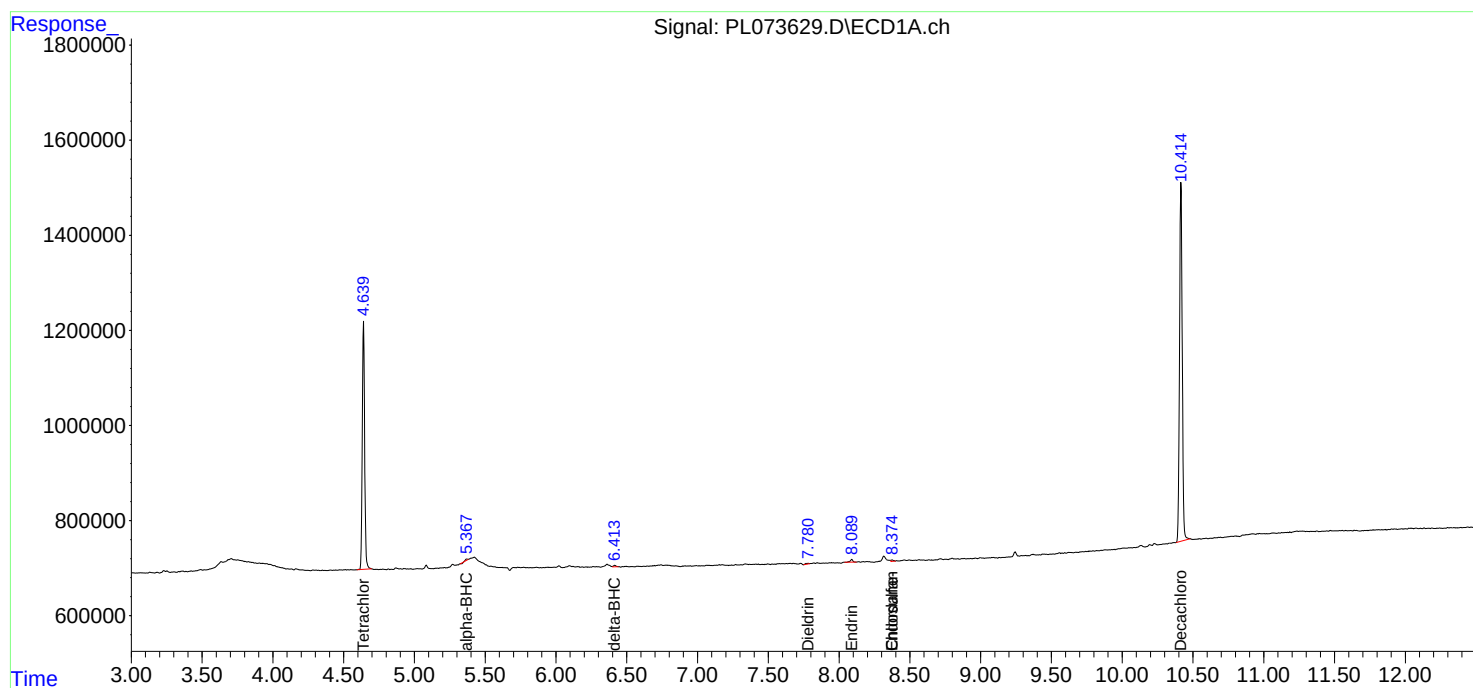


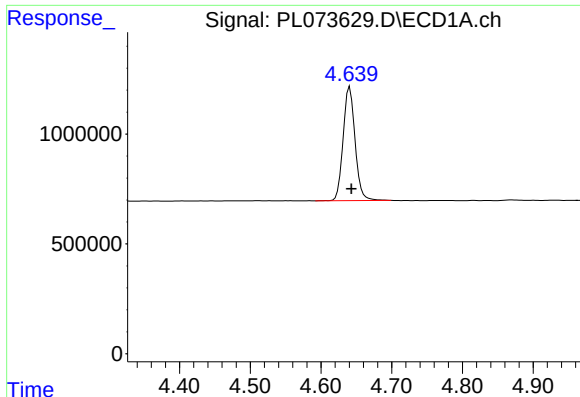

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.002 min
Response: 6067461
Conc: 18.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

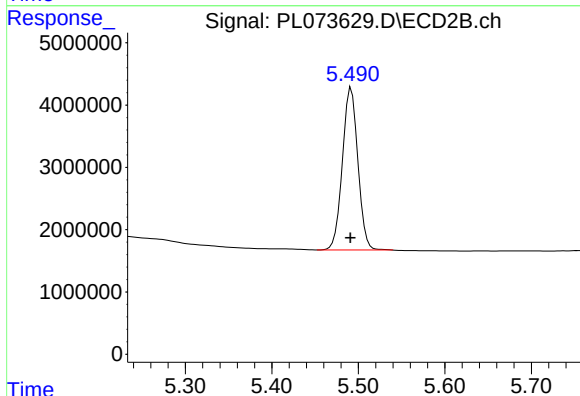


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 32196002
Conc: 19.62 ng/ml

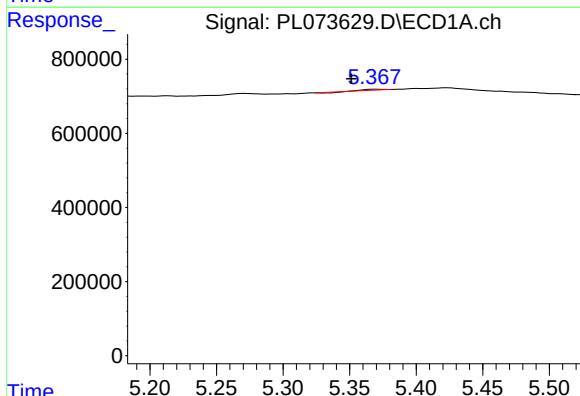


#2 alpha-BHC

R.T.: 5.370 min
Delta R.T.: 0.018 min
Response: 10134
Conc: 0.02 ng/ml

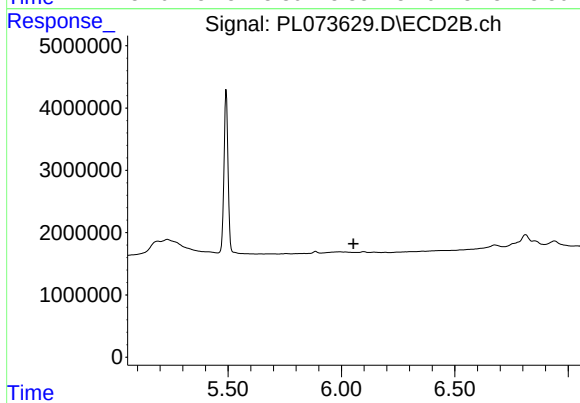

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.054 min
Response: 0
Conc: N.D.

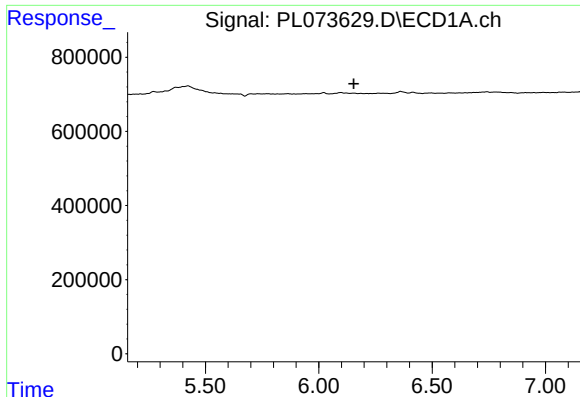

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

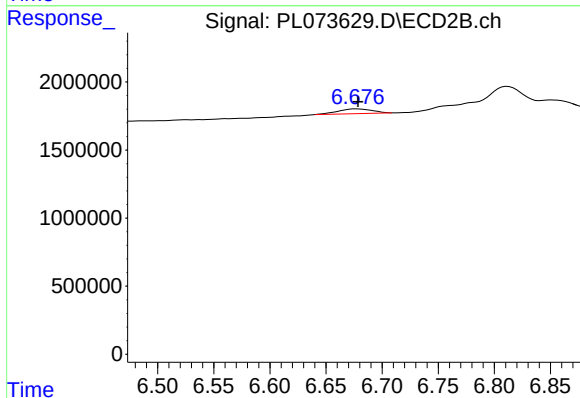


#6 beta-BHC

R.T.: 6.677 min
Delta R.T.: -0.002 min
Response: 763331
Conc: 0.73 ng/ml

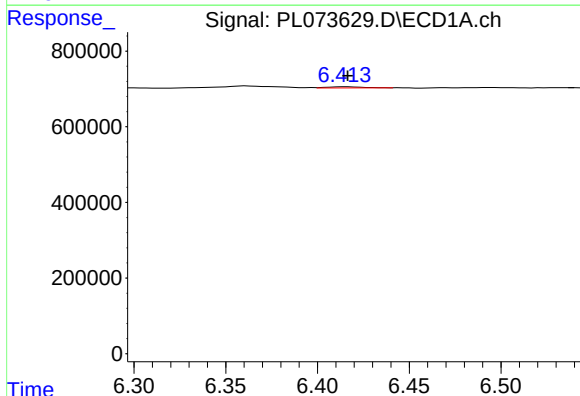


#7 delta-BHC

R.T.: 6.415 min
Delta R.T.: -0.002 min
Response: 39846
Conc: 0.10 ng/ml

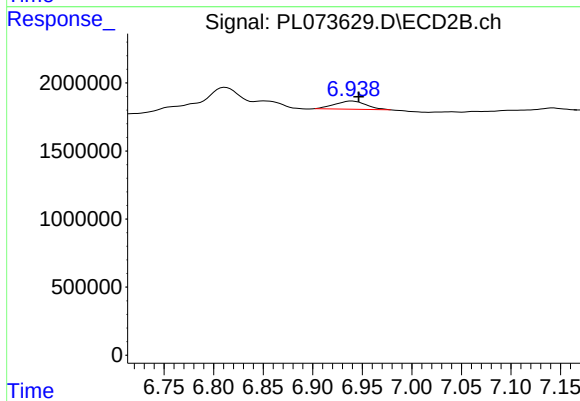

#7 delta-BHC


R.T.: 6.940 min
Delta R.T.: -0.006 min
Response: 1324727
Conc: 0.62 ng/ml

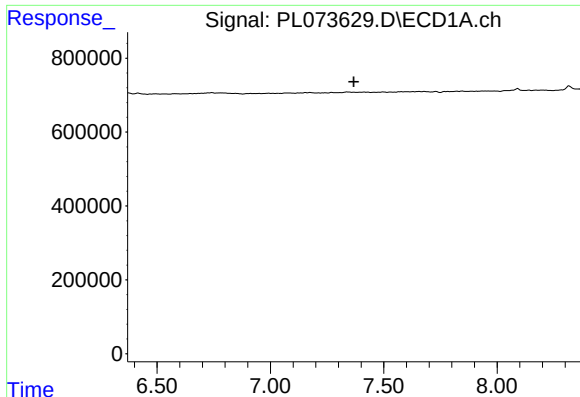

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

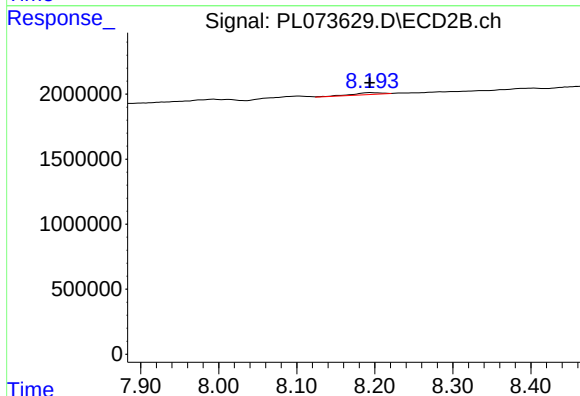


#10 gamma-Chlordane

R.T.: 8.195 min
Delta R.T.: 0.001 min
Response: 375013
Conc: 0.18 ng/ml

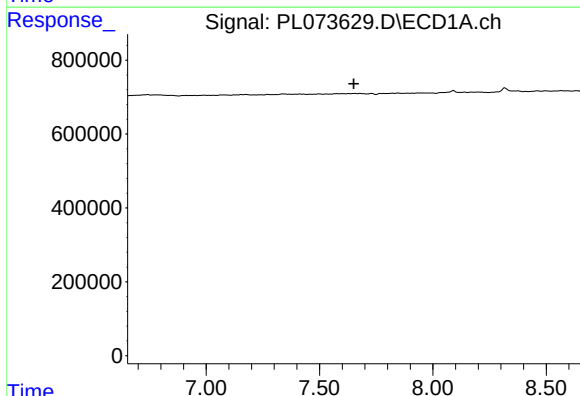


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.651 min
Response: 0
Conc: N.D.

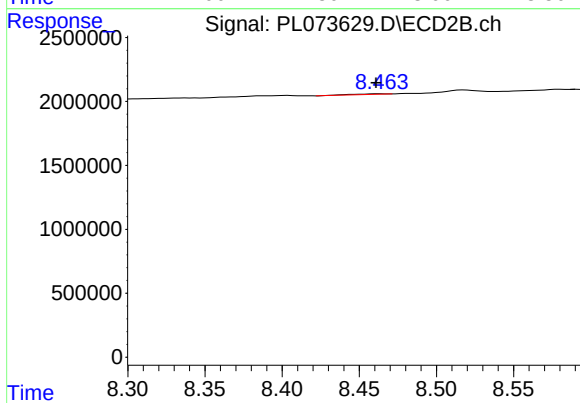

#12 4,4'-DDE


R.T.: 8.464 min
Delta R.T.: 0.003 min
Response: 71523
Conc: 0.04 ng/ml

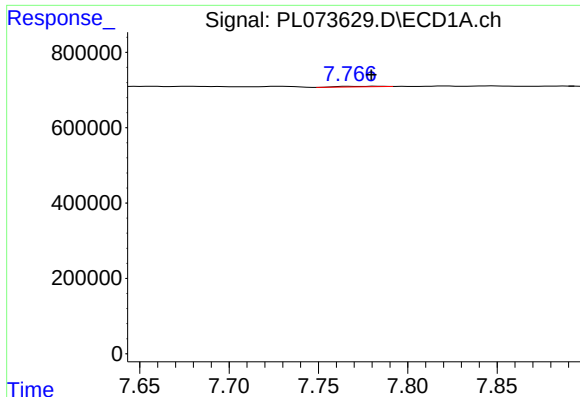

#13 Dieldrin


R.T.: 7.782 min
Delta R.T.: 0.003 min
Response: 24576
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

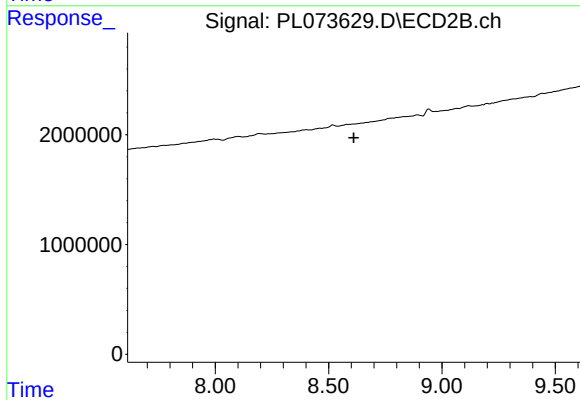


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.611 min
Response: 0
Conc: N.D.

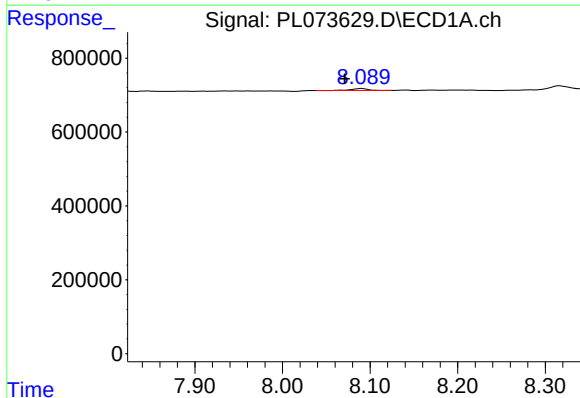


#14 Endrin

R.T.: 8.091 min
Delta R.T.: 0.020 min
Response: 70257
Conc: 0.18 ng/ml

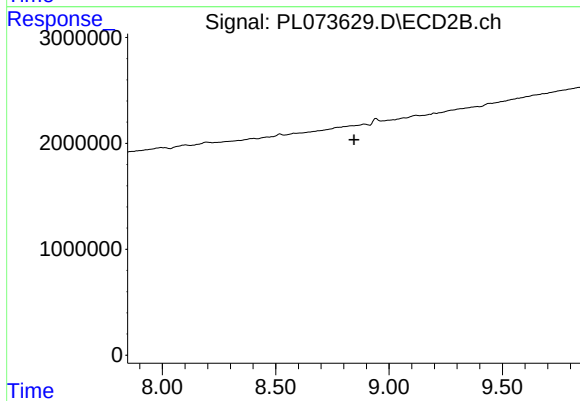

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

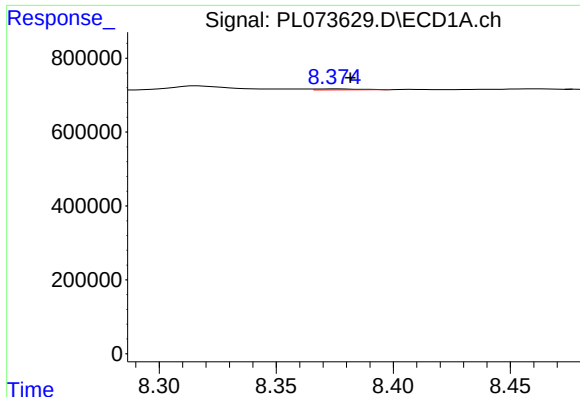

#15 Endosulfan II


R.T.: 8.375 min
Delta R.T.: -0.007 min
Response: 33201
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

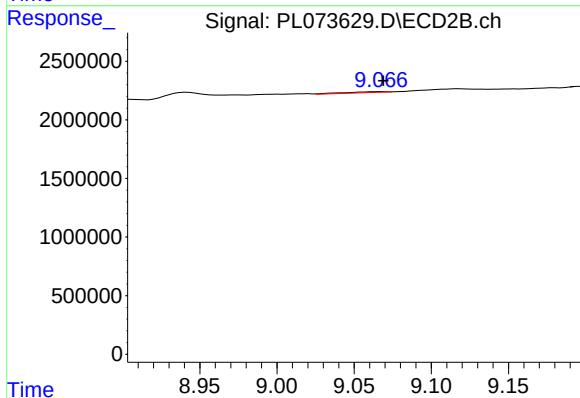


#15 Endosulfan II

R.T.: 9.067 min
Delta R.T.: -0.002 min
Response: 134369
Conc: 0.09 ng/ml

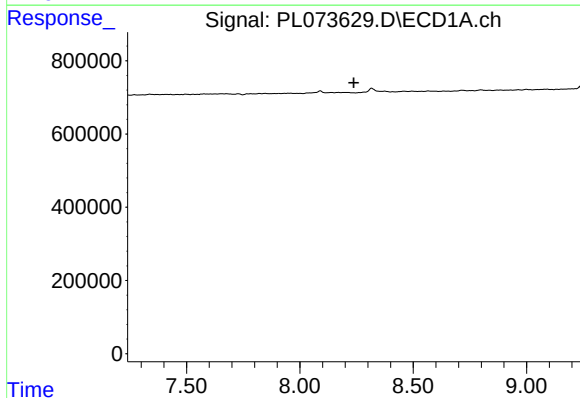


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.237 min
Response: 0
Conc: N.D.

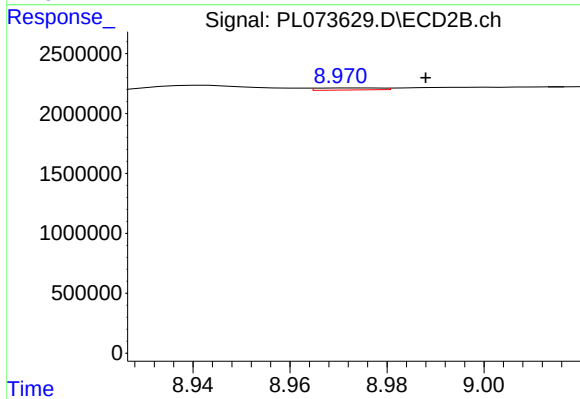

#16 4,4'-DDD


R.T.: 8.973 min
Delta R.T.: -0.015 min
Response: 161513
Conc: 0.11 ng/ml

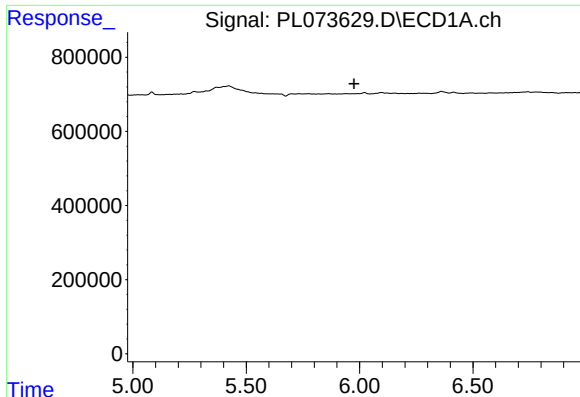

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

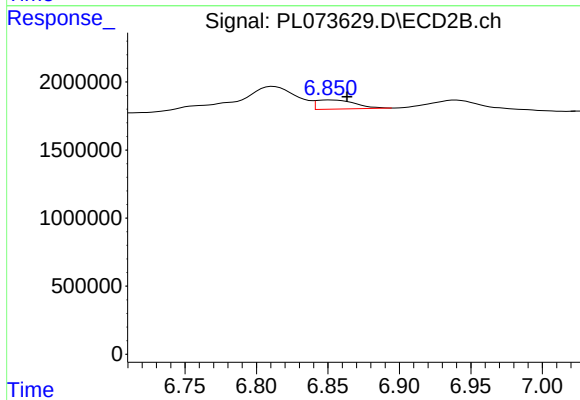


#23 Chlordane-1

R.T.: 6.852 min
Delta R.T.: -0.012 min
Response: 1263537
Conc: 18.50 ng/ml

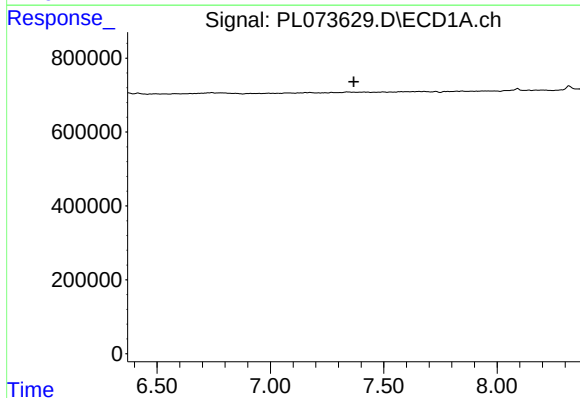


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

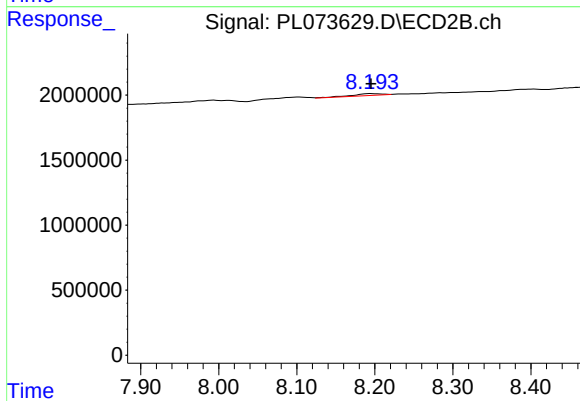

#25 Chlordane-3


R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 375013
Conc: 1.38 ng/ml

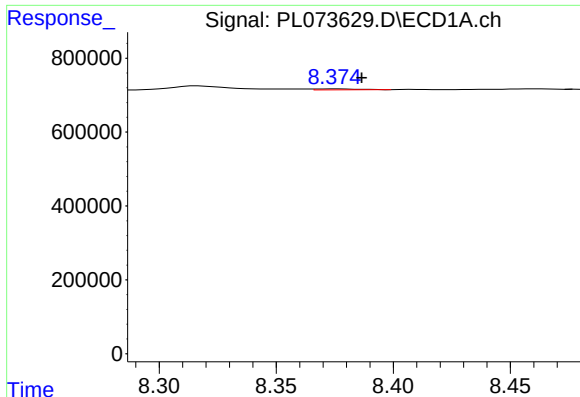

#27 Chlordane-5


R.T.: 8.375 min
Delta R.T.: -0.011 min
Response: 33201
Conc: 2.03 ng/ml

Instrument :
ECD_L
ClientSampleId :

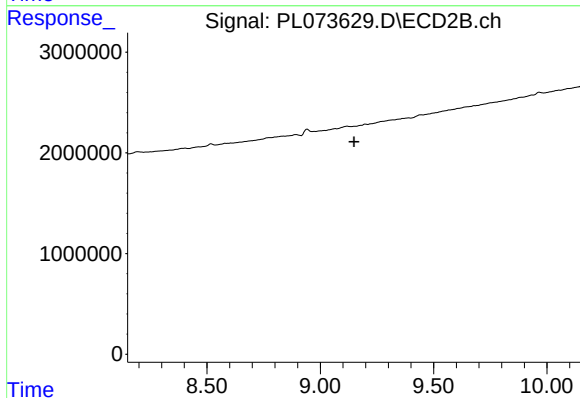


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.149 min
Response: 0
Conc: N.D.

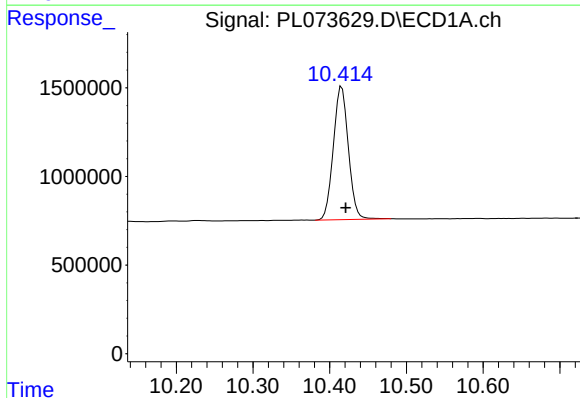

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.005 min
Response: 10218700
Conc: 20.10 ng/ml

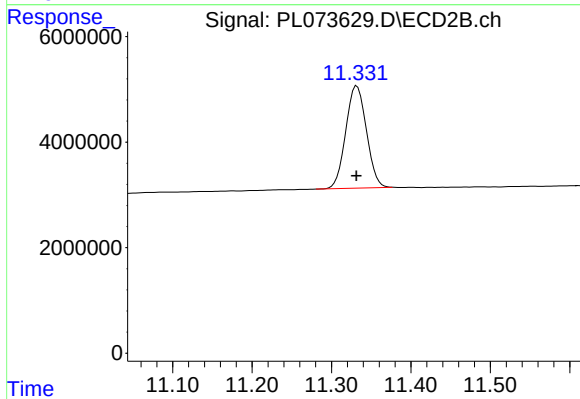

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 35127885
Conc: 19.64 ng/ml