

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073631.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 23:59
 Operator : AR\AJ
 Sample : N2063-08
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:35:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.492	6268176	33122522	19.571	20.181
2)	SA Decachlor...	10.417	11.333	10314227	35815860	20.284	20.029
Target Compounds							
2)	A alpha-BHC	5.373f	0.000	73986	0	0.179	N.D. #
6)	B beta-BHC	0.000	6.677	0	589194	N.D.	0.565 #
7)	B delta-BHC	0.000	6.942	0	1449940	N.D.	0.673 #
9)	A Endosulfan I	0.000	8.297f	0	108763	N.D.	0.060 #
10)	B gamma-Chl...	0.000	8.198	0	497470	N.D.	0.244 #
11)	B alpha-Chl...	0.000	8.297f	0	108763	N.D.	0.054 #
14)	MA Endrin	8.091f	8.855	100602	237594	0.259	0.154 #
15)	B Endosulfa...	8.381	9.067	73175	516150	0.187	0.336 #
16)	A 4,4'-DDD	8.260f	0.000	107041	0	0.330	N.D. #
18)	B Endrin al...	0.000	9.206	0	62828	N.D.	0.051 #
20)	A Methoxychlor	0.000	9.789	0	228321	N.D.	0.253 #
23)	Chlordane-1	0.000	6.851	0	871265	N.D.	12.754 #
25)	Chlordane-3	0.000	8.198	0	497470	N.D.	1.835 #
26)	Chlordane-4	0.000	8.297f	0	108763	N.D.	0.328 #
27)	Chlordane-5	8.381	0.000	73175	0	4.469	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073631.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 23:59
Operator : AR\AJ
Sample : N2063-08
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:35:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

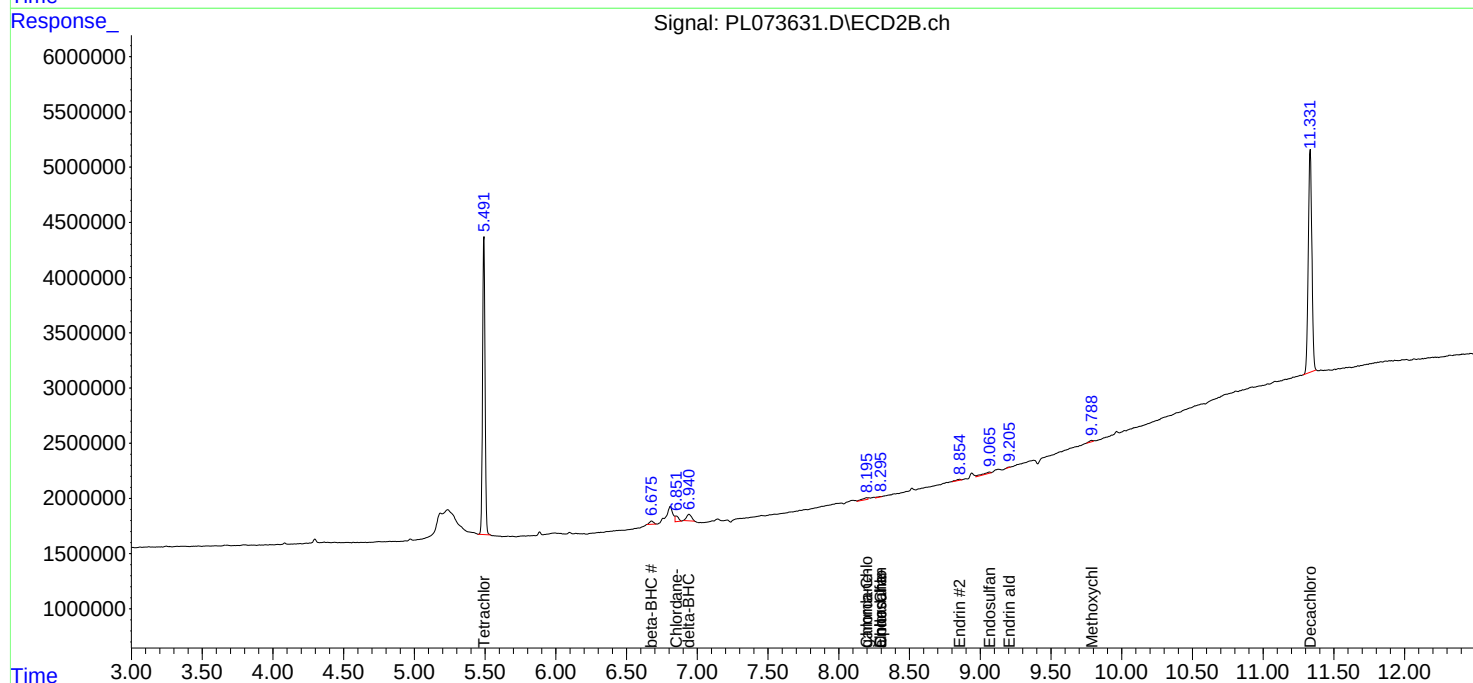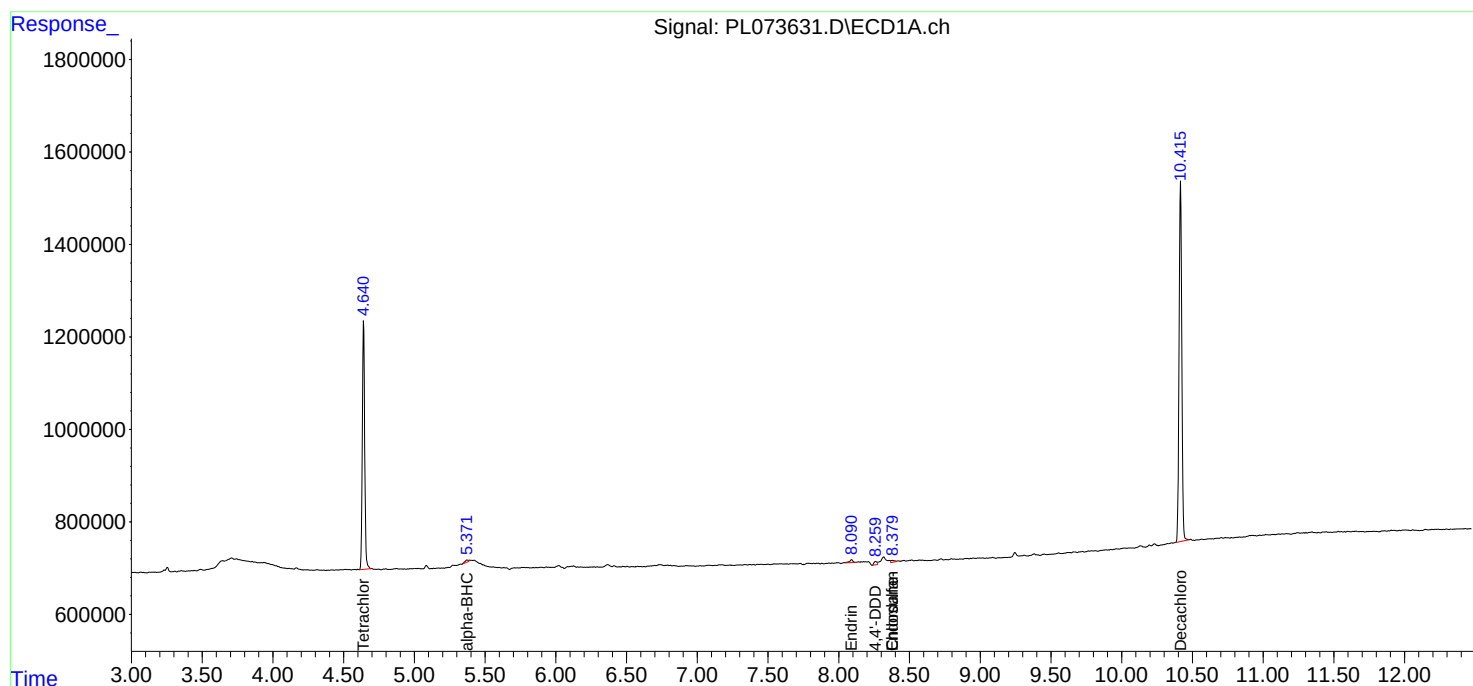


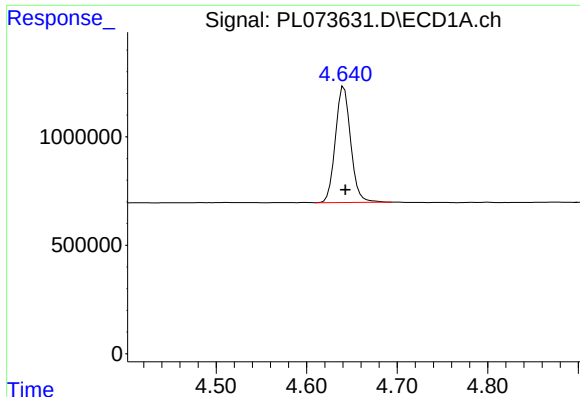

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.002 min
Response: 6268176
Conc: 19.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

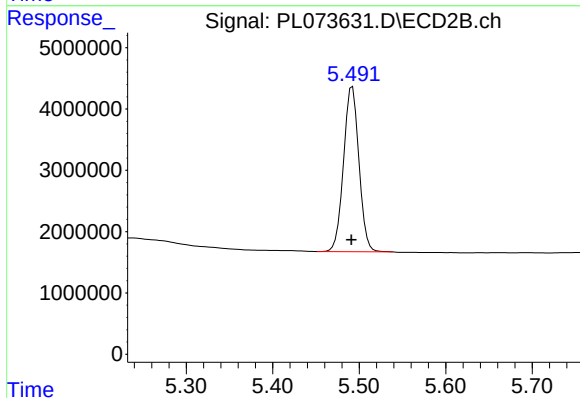


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.001 min
Response: 33122522
Conc: 20.18 ng/ml

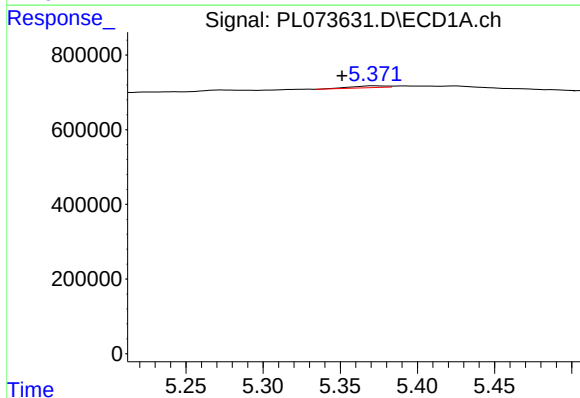


#2 alpha-BHC

R.T.: 5.373 min
Delta R.T.: 0.021 min
Response: 73986
Conc: 0.18 ng/ml

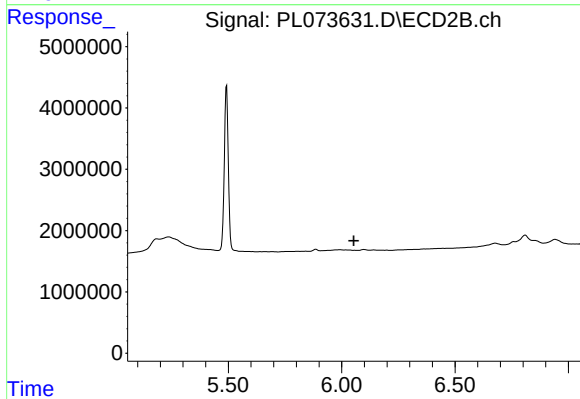

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

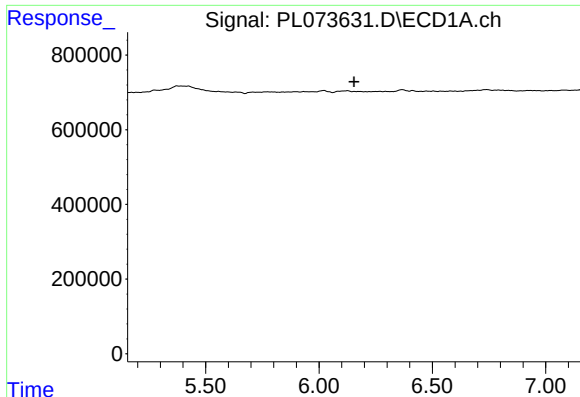

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

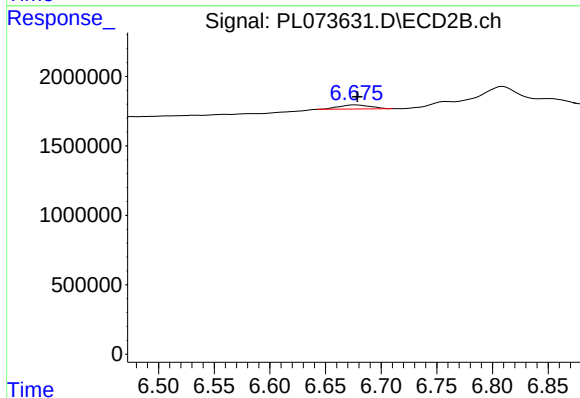


#6 beta-BHC

R.T.: 6.677 min
Delta R.T.: -0.002 min
Response: 589194
Conc: 0.57 ng/ml

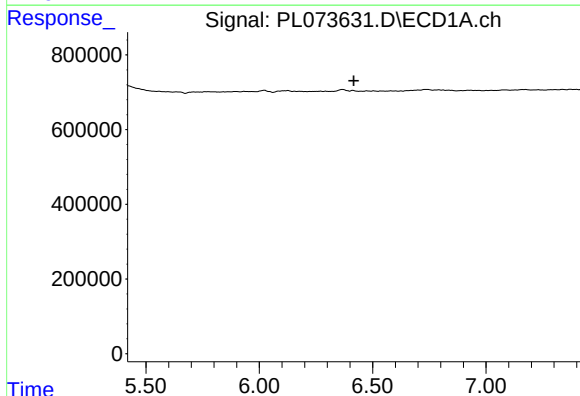


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

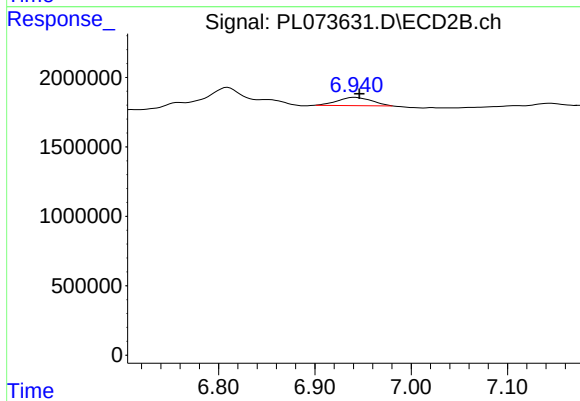

#7 delta-BHC


R.T.: 6.942 min
Delta R.T.: -0.005 min
Response: 1449940
Conc: 0.67 ng/ml

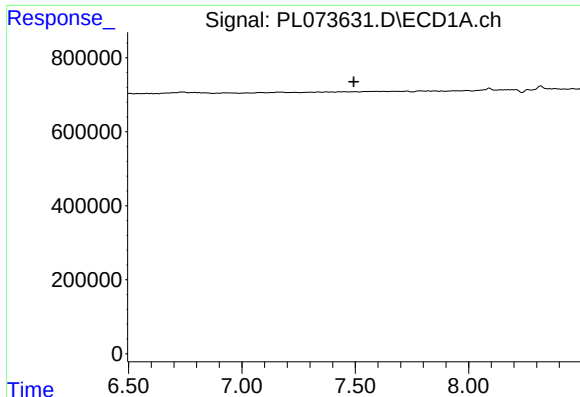

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.493 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

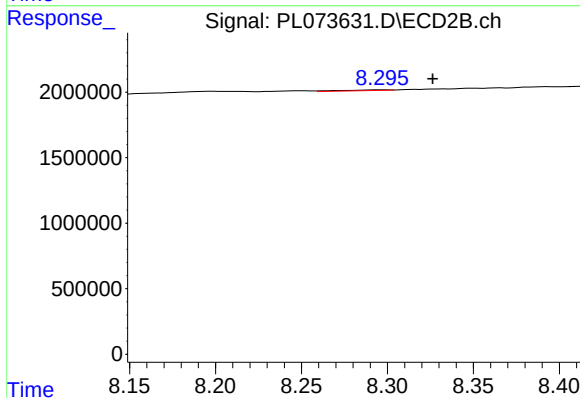


#9 Endosulfan I

R.T.: 8.297 min
Delta R.T.: -0.030 min
Response: 108763
Conc: 0.06 ng/ml

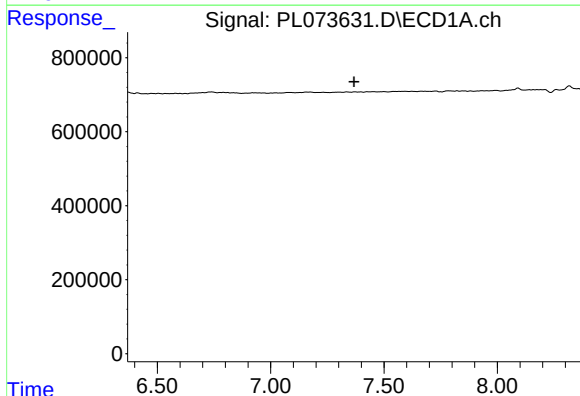


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

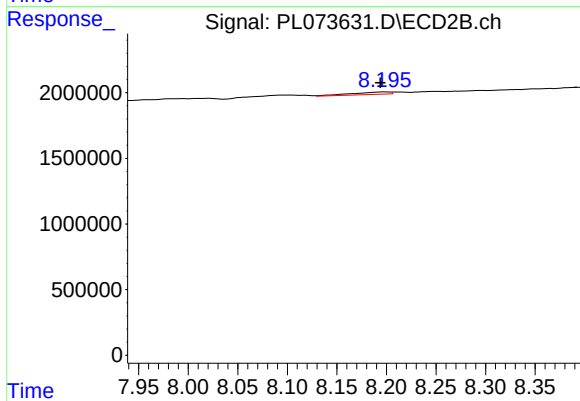

#10 gamma-Chlordane


R.T.: 8.198 min
Delta R.T.: 0.005 min
Response: 497470
Conc: 0.24 ng/ml

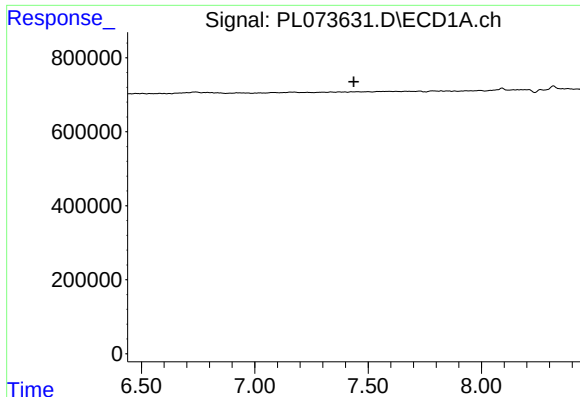

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

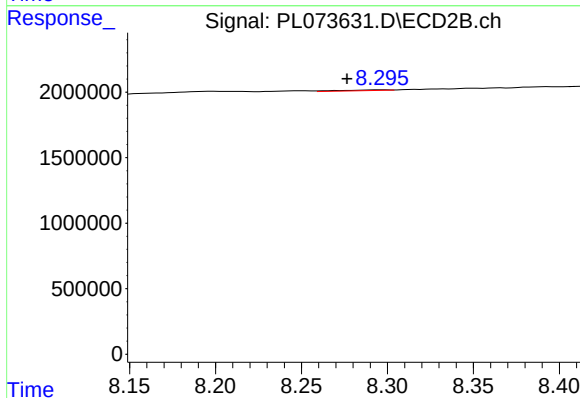


#11 alpha-Chlordane

R.T.: 8.297 min
Delta R.T.: 0.020 min
Response: 108763
Conc: 0.05 ng/ml

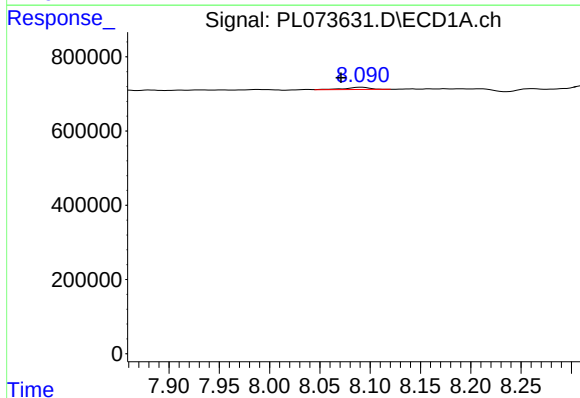


#14 Endrin

R.T.: 8.091 min
Delta R.T.: 0.020 min
Response: 100602
Conc: 0.26 ng/ml

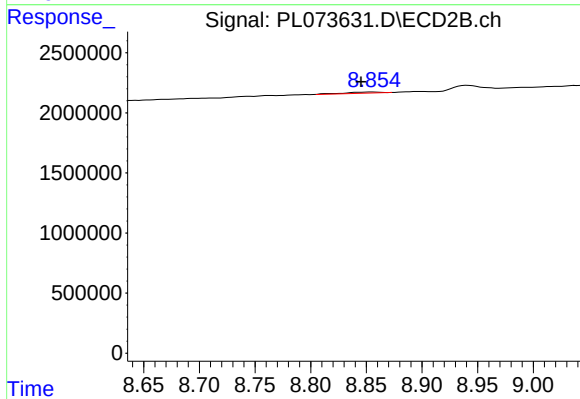

#14 Endrin


R.T.: 8.855 min
Delta R.T.: 0.010 min
Response: 237594
Conc: 0.15 ng/ml

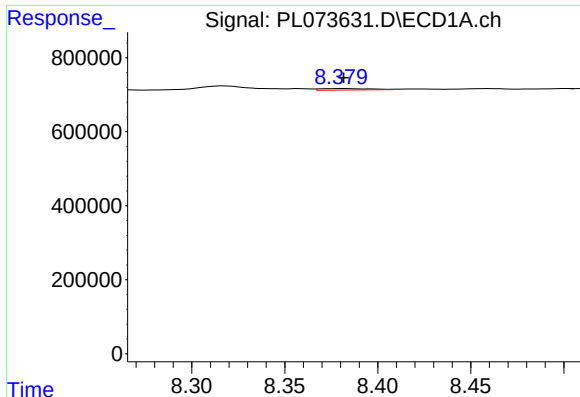

#15 Endosulfan II


R.T.: 8.381 min
Delta R.T.: 0.000 min
Response: 73175
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

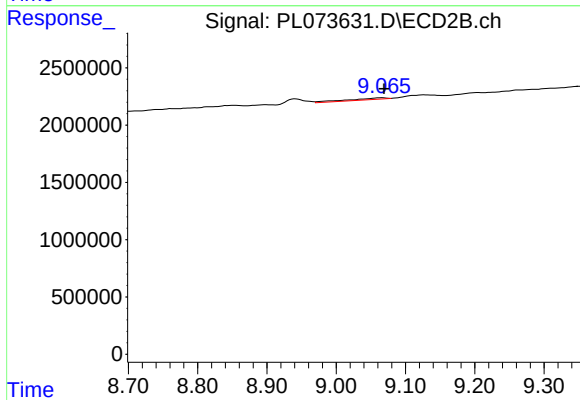


#15 Endosulfan II

R.T.: 9.067 min
Delta R.T.: -0.002 min
Response: 516150
Conc: 0.34 ng/ml

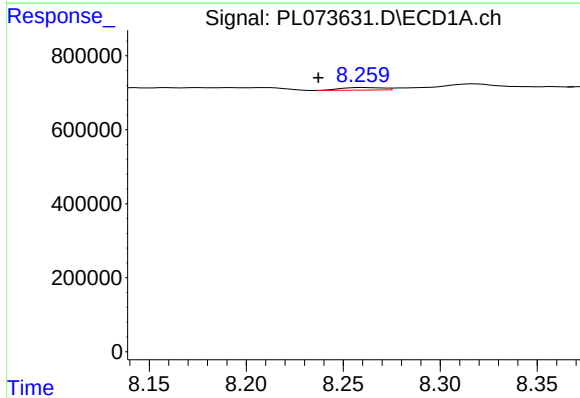


#16 4,4'-DDD

R.T.: 8.260 min
Delta R.T.: 0.023 min
Response: 107041
Conc: 0.33 ng/ml

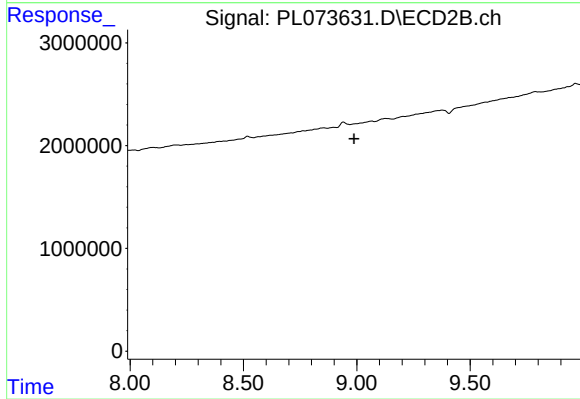

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.988 min
Response: 0
Conc: N.D.

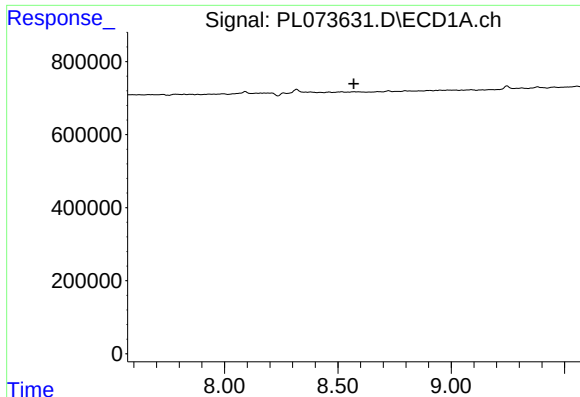

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 8.570 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

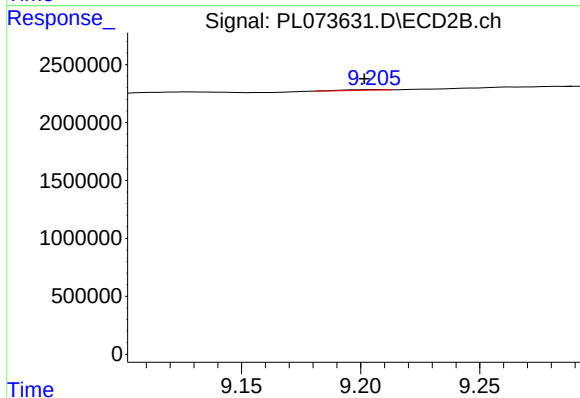


#18 Endrin aldehyde

R.T.: 9.206 min
Delta R.T.: 0.004 min
Response: 62828
Conc: 0.05 ng/ml

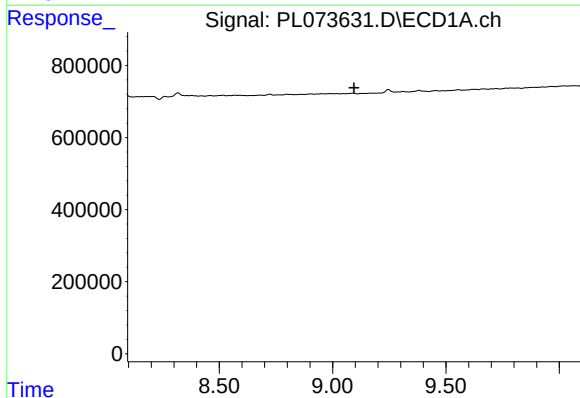


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.095 min
Response: 0
Conc: N.D.

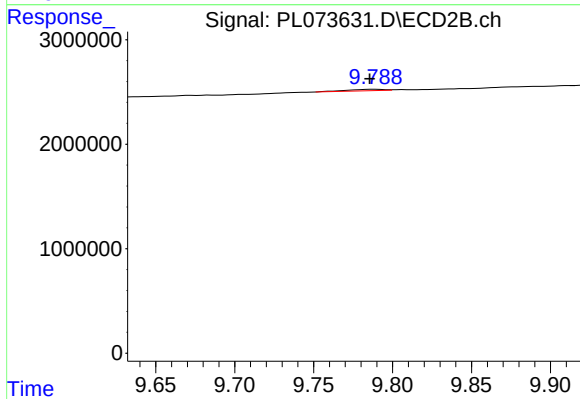

#20 Methoxychlor


R.T.: 9.789 min
Delta R.T.: 0.003 min
Response: 228321
Conc: 0.25 ng/ml

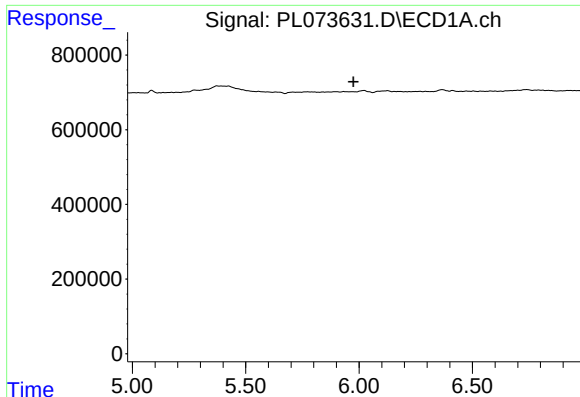

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

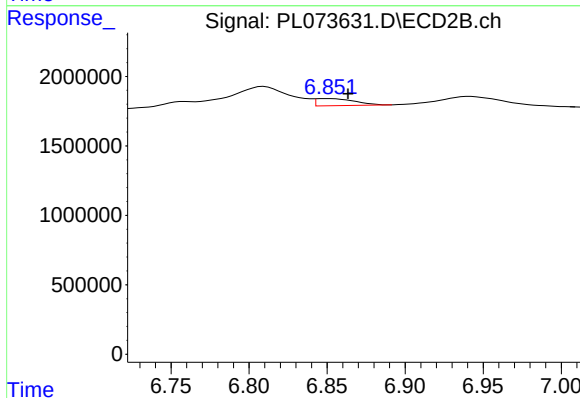


#23 Chlordane-1

R.T.: 6.851 min
Delta R.T.: -0.012 min
Response: 871265
Conc: 12.75 ng/ml

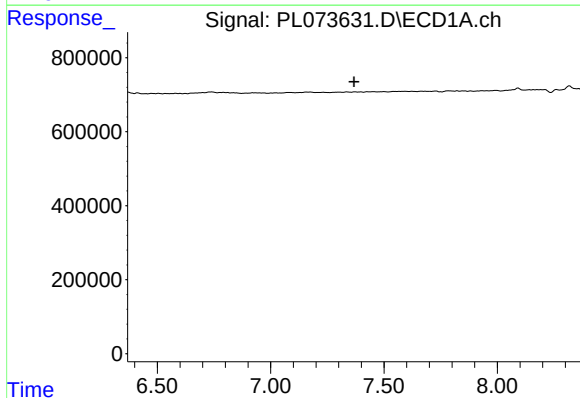


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

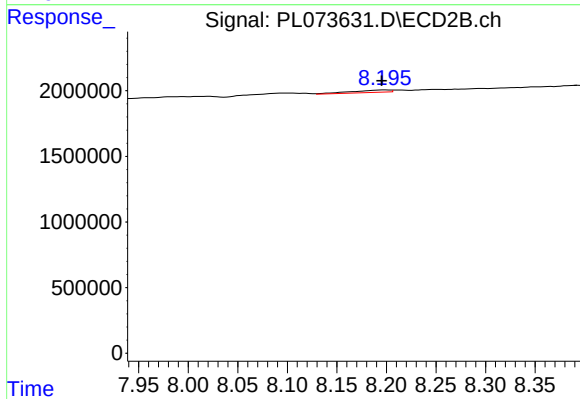

#25 Chlordane-3


R.T.: 8.198 min
Delta R.T.: 0.003 min
Response: 497470
Conc: 1.83 ng/ml

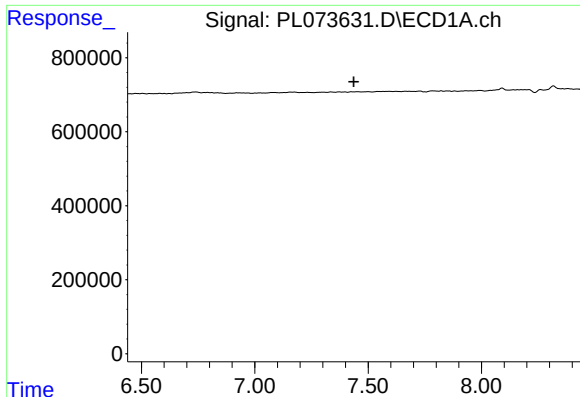

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

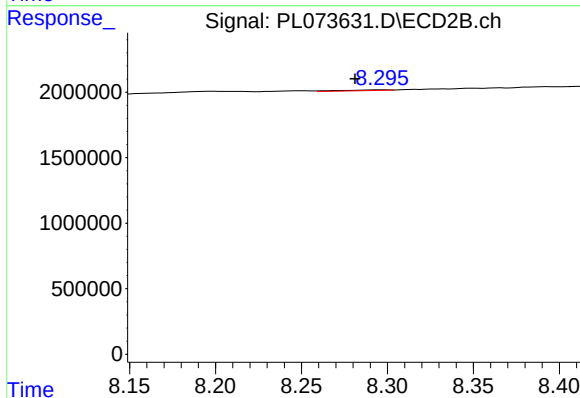


#26 Chlordane-4

R.T.: 8.297 min
Delta R.T.: 0.015 min
Response: 108763
Conc: 0.33 ng/ml

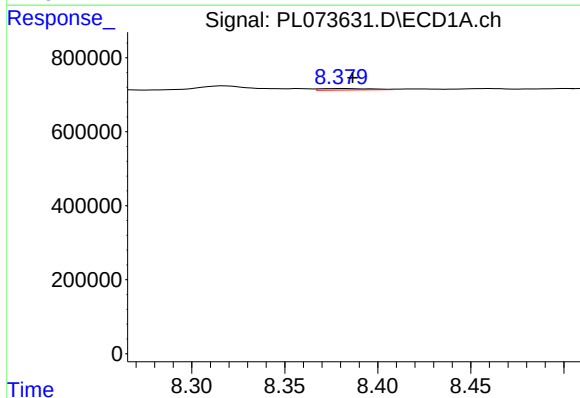


#27 Chlordane-5

R.T.: 8.381 min
Delta R.T.: -0.006 min
Response: 73175
Conc: 4.47 ng/ml

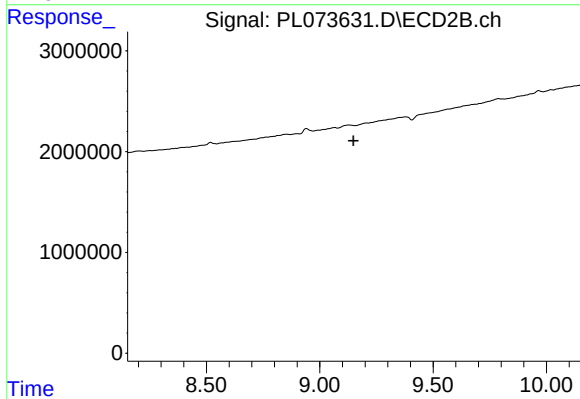

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 9.149 min
Response: 0
Conc: N.D.

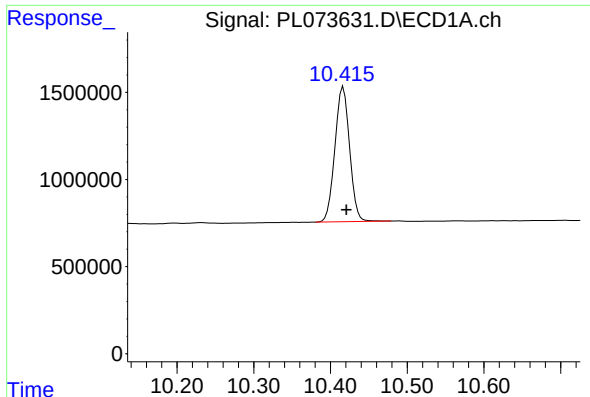

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.004 min
Response: 10314227
Conc: 20.28 ng/ml

Instrument :
ECD_L
ClientSampleId :

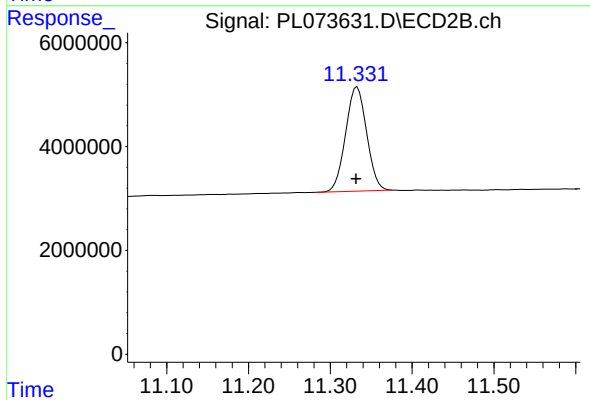

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: 0.001 min
Response: 35815860
Conc: 20.03 ng/ml