

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073632.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 00:16
 Operator : AR\AJ
 Sample : N2063-09
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:36:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.491	5916585	31142213	18.473	18.975
28)	SA Decachlor...	10.415	11.332	9472199	33130292	18.628	18.527
Target Compounds							
6)	B beta-BHC	0.000	6.679	0	622884	N.D.	0.598 #
7)	B delta-BHC	0.000	6.941	0	1445166	N.D.	0.671 #
10)	B gamma-Chl...	0.000	8.200	0	236048	N.D.	0.116 #
12)	B 4,4'-DDE	0.000	8.486f	0	68183	N.D.	0.038 #
14)	MA Endrin	8.091f	8.860	88732	62755	0.229	0.041 #
15)	B Endosulfa...	8.387	9.060	41829	296105	0.107	0.193 #
17)	MA 4,4'-DDT	0.000	9.316	0	5526	N.D.	0.003 #
23)	Chlordane-1	0.000	6.853	0	1197548	N.D.	17.530 #
25)	Chlordane-3	0.000	8.200	0	236048	N.D.	0.871 #
27)	Chlordane-5	8.387	0.000	41829	0	2.554	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073632.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 00:16
Operator : AR\AJ
Sample : N2063-09
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:36:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

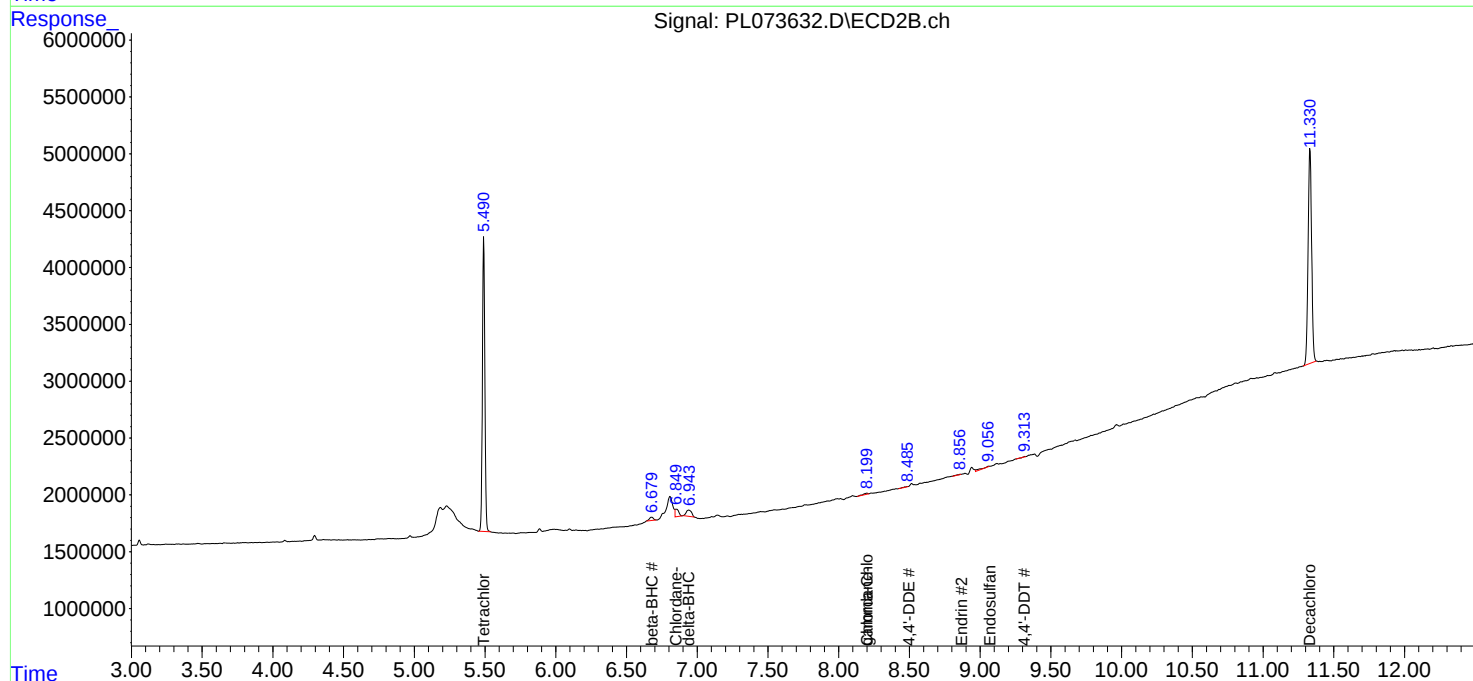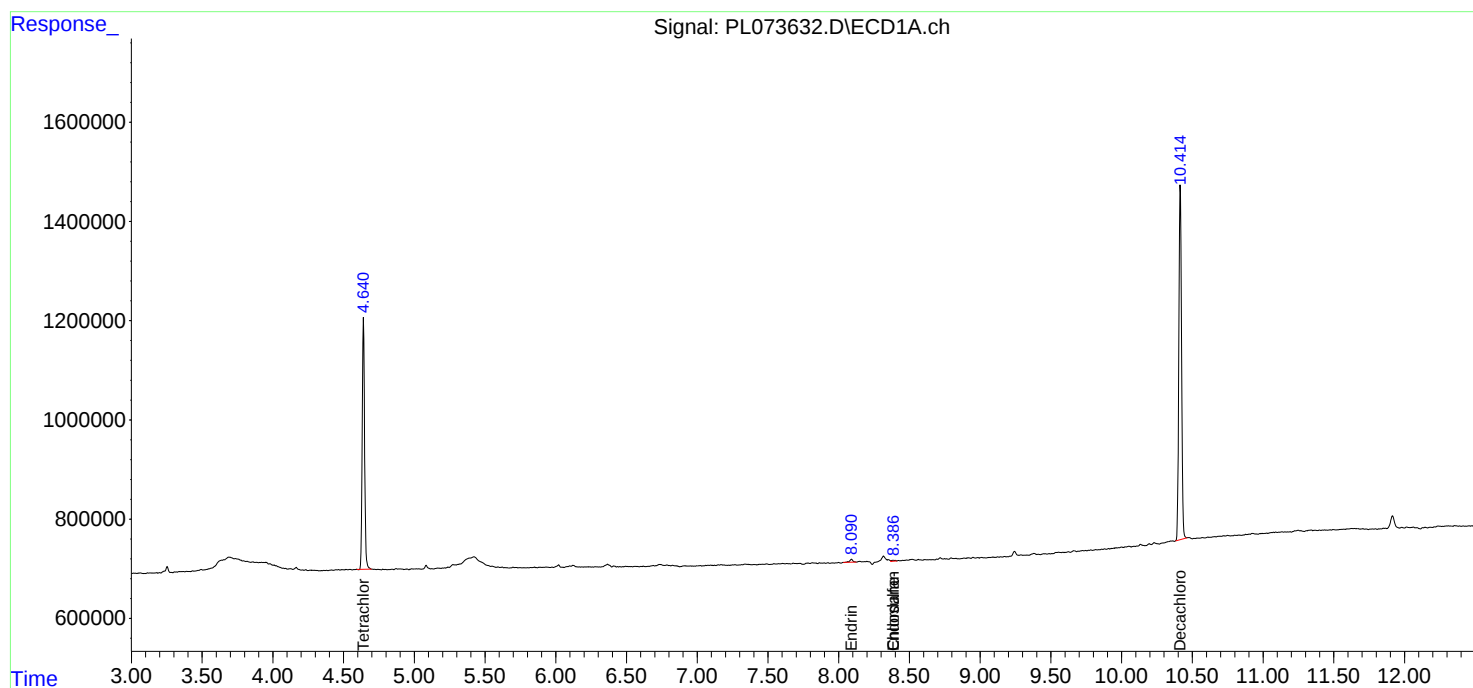


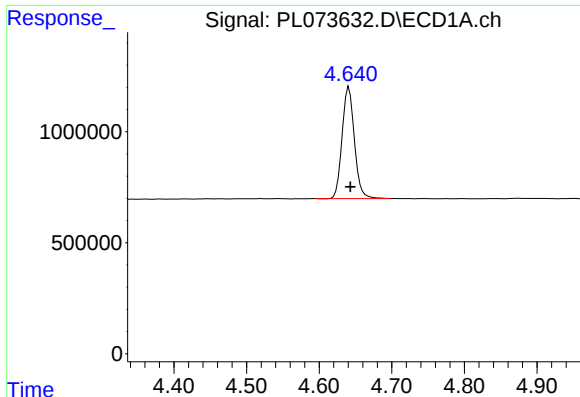

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.002 min
Response: 5916585
Conc: 18.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

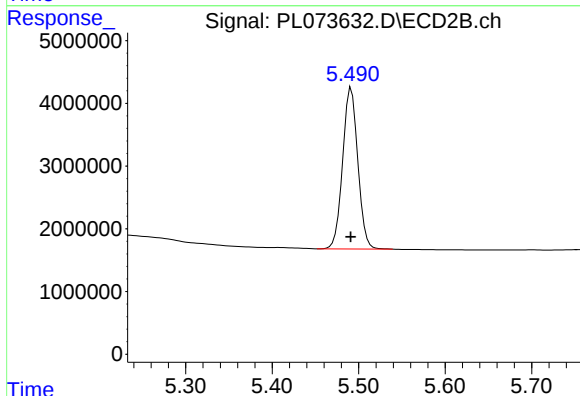


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 31142213
Conc: 18.97 ng/ml

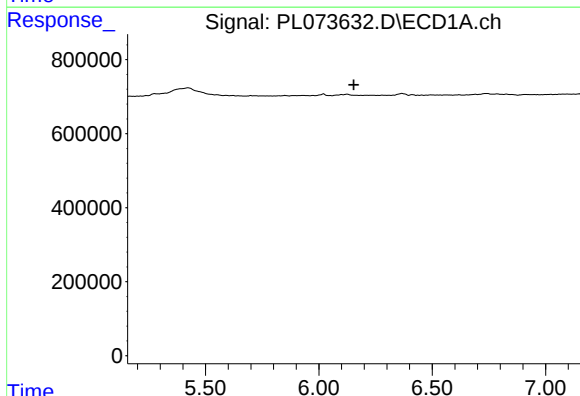


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

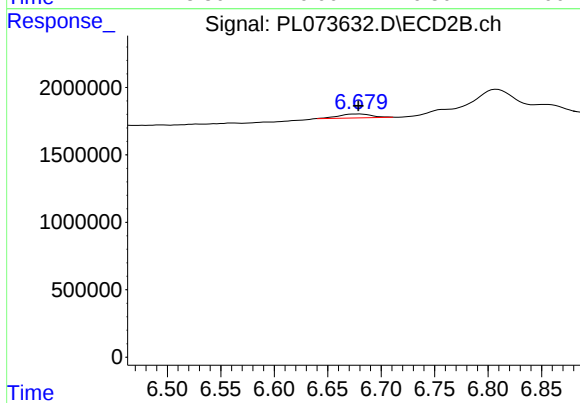

#6 beta-BHC


R.T.: 6.679 min
Delta R.T.: 0.000 min
Response: 622884
Conc: 0.60 ng/ml

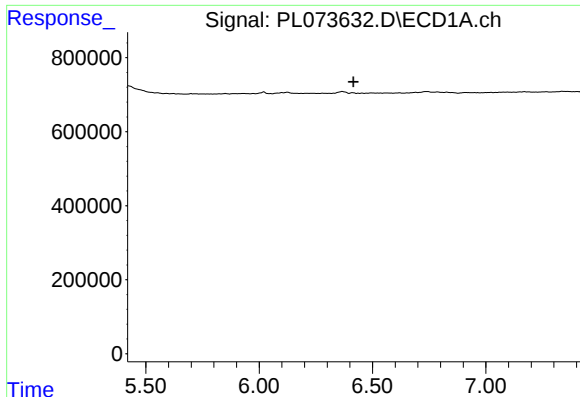

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

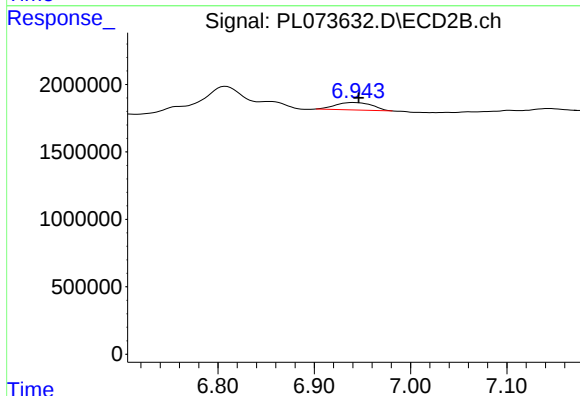


#7 delta-BHC

R.T.: 6.941 min
Delta R.T.: -0.005 min
Response: 1445166
Conc: 0.67 ng/ml

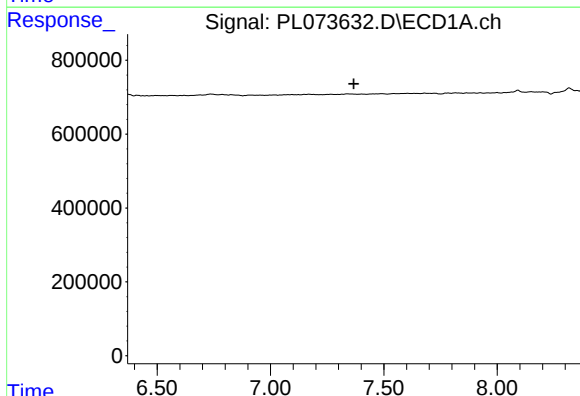


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

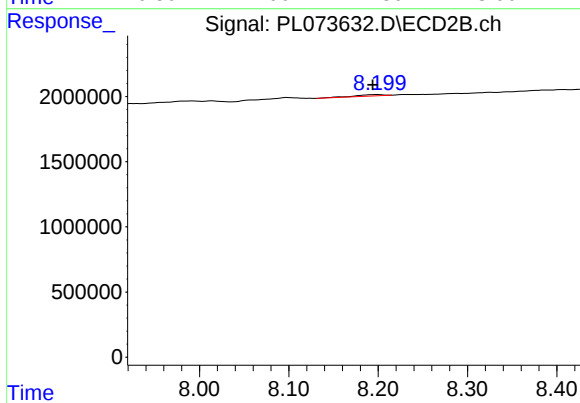

#10 gamma-Chlordane


R.T.: 8.200 min
Delta R.T.: 0.006 min
Response: 236048
Conc: 0.12 ng/ml

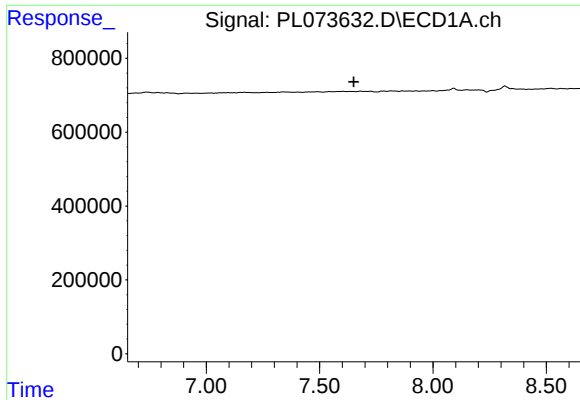

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 7.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

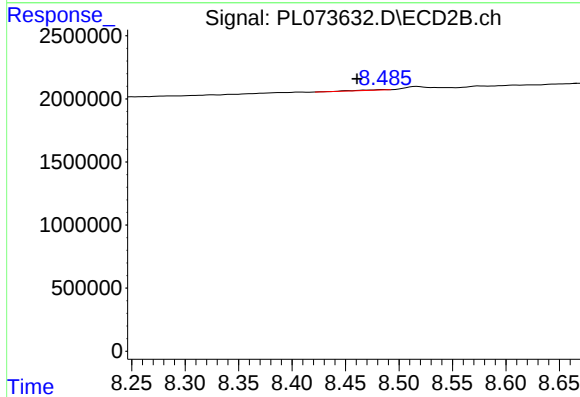


#12 4,4'-DDE

R.T.: 8.486 min
Delta R.T.: 0.026 min
Response: 68183
Conc: 0.04 ng/ml

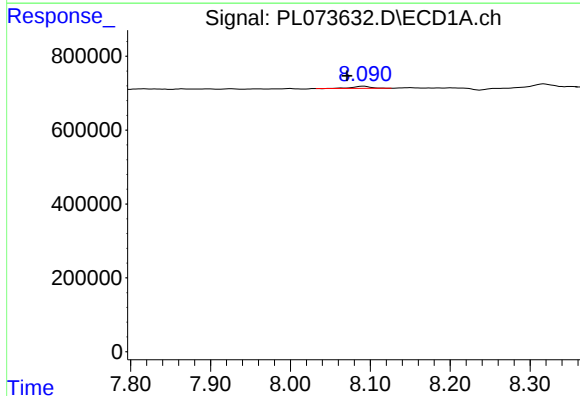


#14 Endrin

R.T.: 8.091 min
Delta R.T.: 0.021 min
Response: 88732
Conc: 0.23 ng/ml

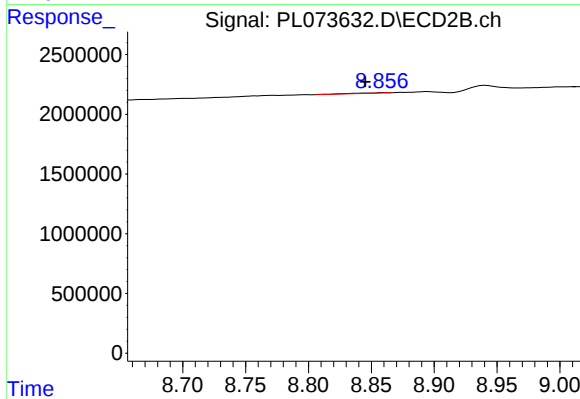

#14 Endrin


R.T.: 8.860 min
Delta R.T.: 0.014 min
Response: 62755
Conc: 0.04 ng/ml

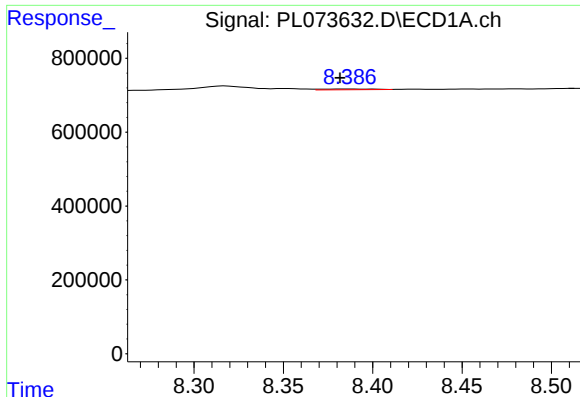

#15 Endosulfan II


R.T.: 8.387 min
Delta R.T.: 0.005 min
Response: 41829
Conc: 0.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

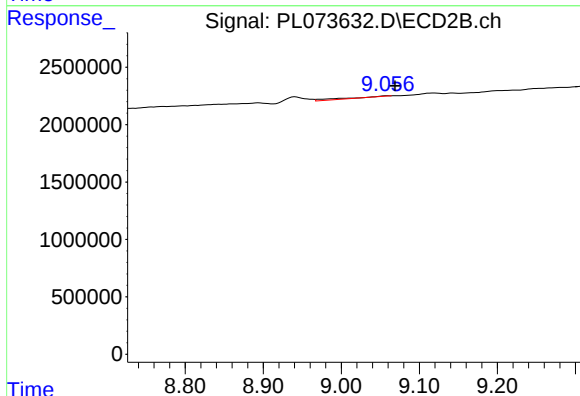


#15 Endosulfan II

R.T.: 9.060 min
Delta R.T.: -0.009 min
Response: 296105
Conc: 0.19 ng/ml

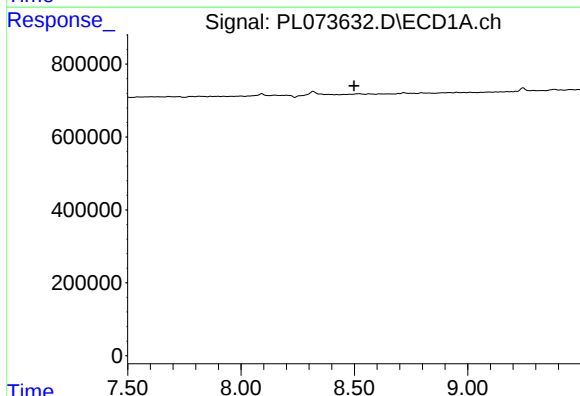


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.499 min
Response: 0
Conc: N.D.

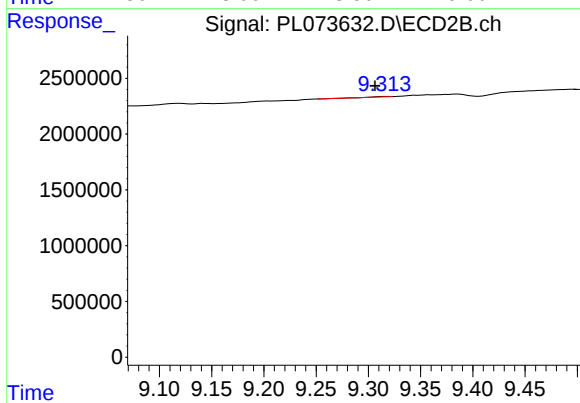

#17 4,4'-DDT


R.T.: 9.316 min
Delta R.T.: 0.009 min
Response: 5526
Conc: 0.00 ng/ml

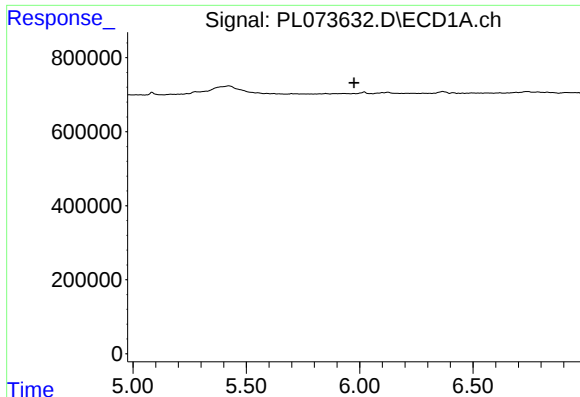

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

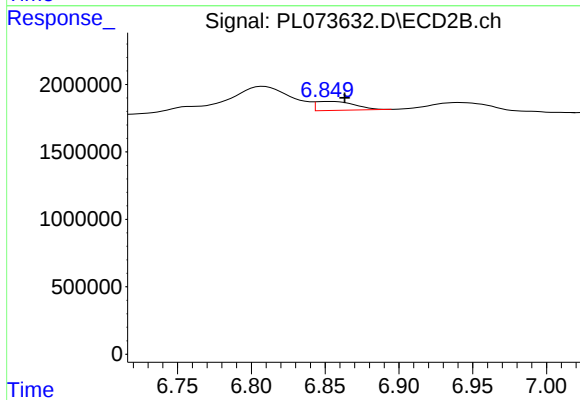


#23 Chlordane-1

R.T.: 6.853 min
Delta R.T.: -0.010 min
Response: 1197548
Conc: 17.53 ng/ml

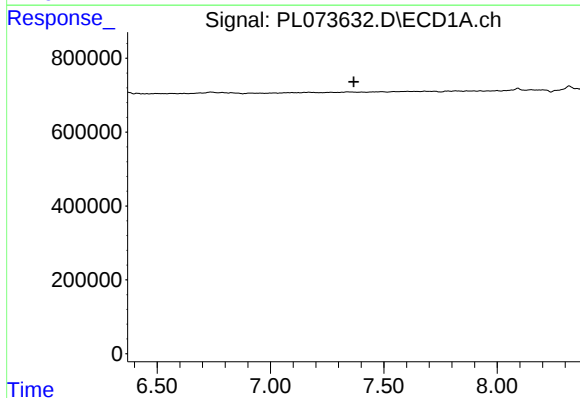


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 7.368 min
Response: 0
Conc: N.D.

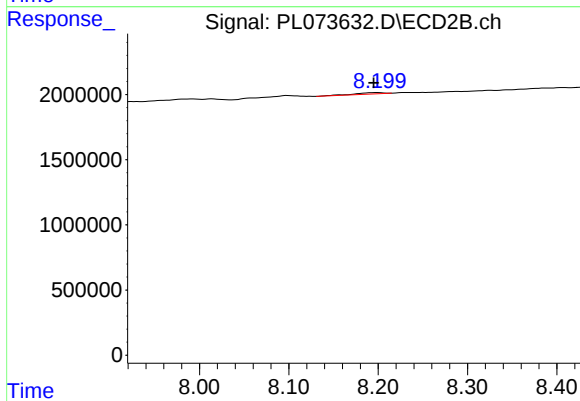

#25 Chlordane-3


R.T.: 8.200 min
Delta R.T.: 0.005 min
Response: 236048
Conc: 0.87 ng/ml

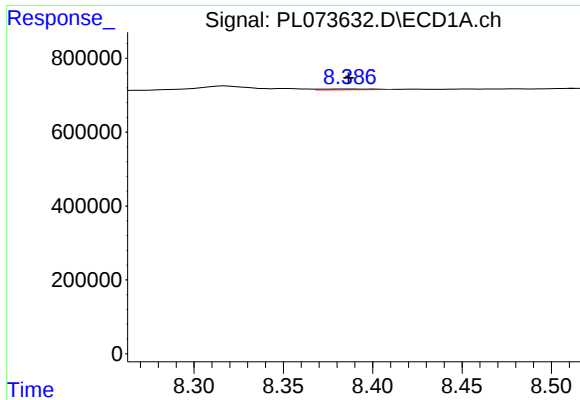

#27 Chlordane-5


R.T.: 8.387 min
Delta R.T.: 0.000 min
Response: 41829
Conc: 2.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

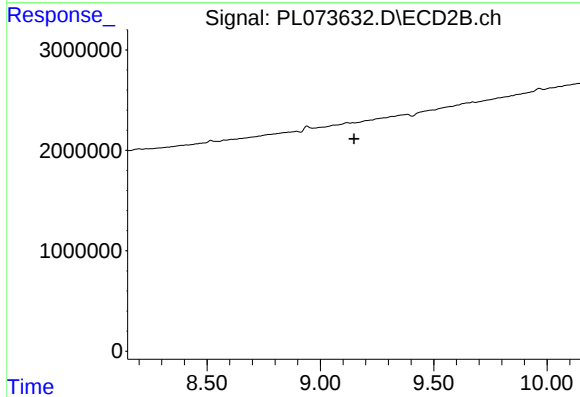


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.149 min
Response: 0
Conc: N.D.

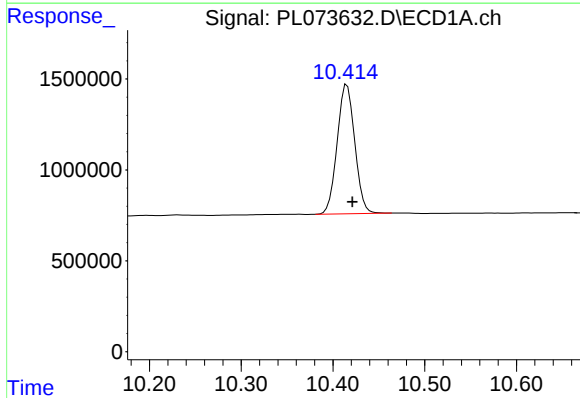

#28 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.006 min
Response: 9472199
Conc: 18.63 ng/ml

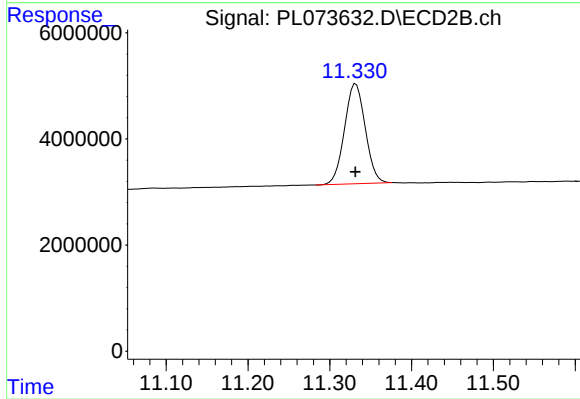

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 33130292
Conc: 18.53 ng/ml