

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073597.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 12:14
 Operator : AR\AJ
 Sample : N1905-16
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-14A-1A-1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/24/2022
 Supervised By : mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 16:58:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.640	5.491	6811563	33179124	21.267m	20.216
28) SA Decachlor...	10.415	11.331	10329614	35030205	20.314	19.590

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 12:14
Operator : AR\AJ
Sample : N1905-16
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-14A-1A-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/24/2022
Supervised By : mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 16:58:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

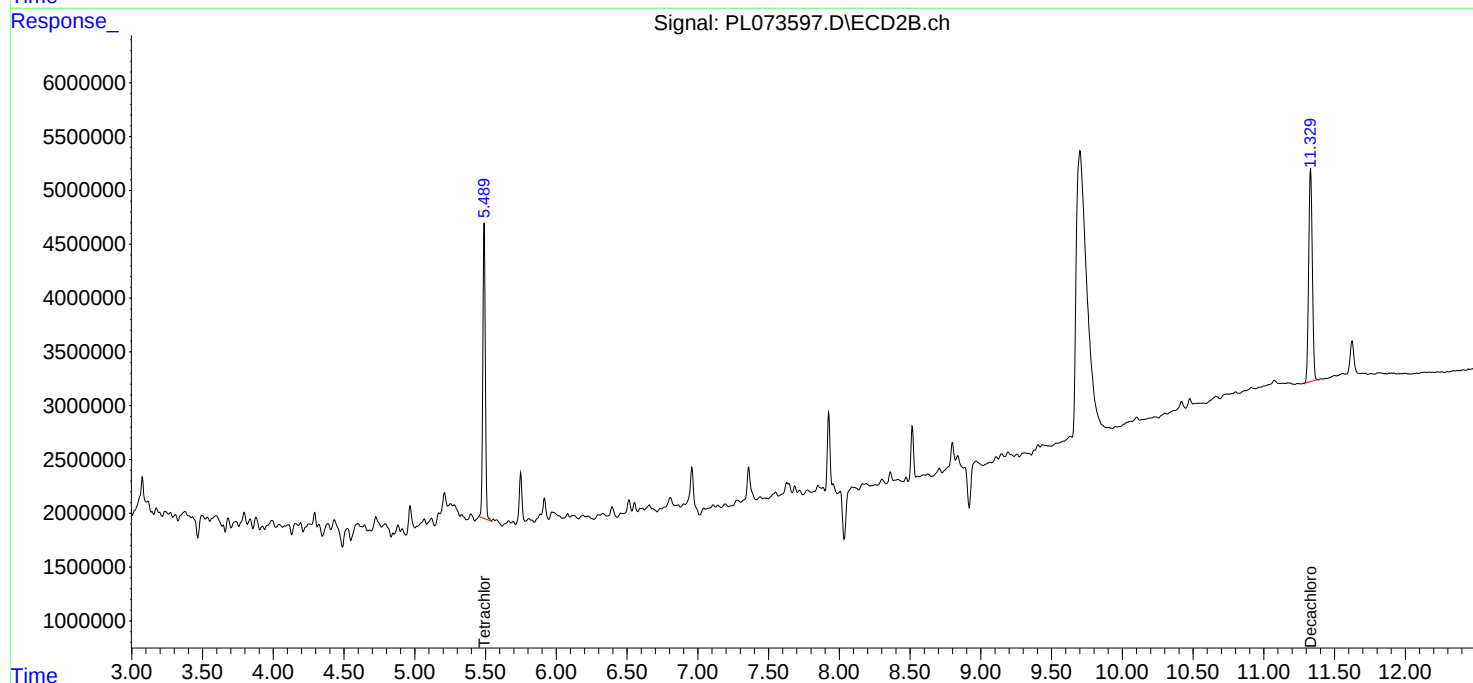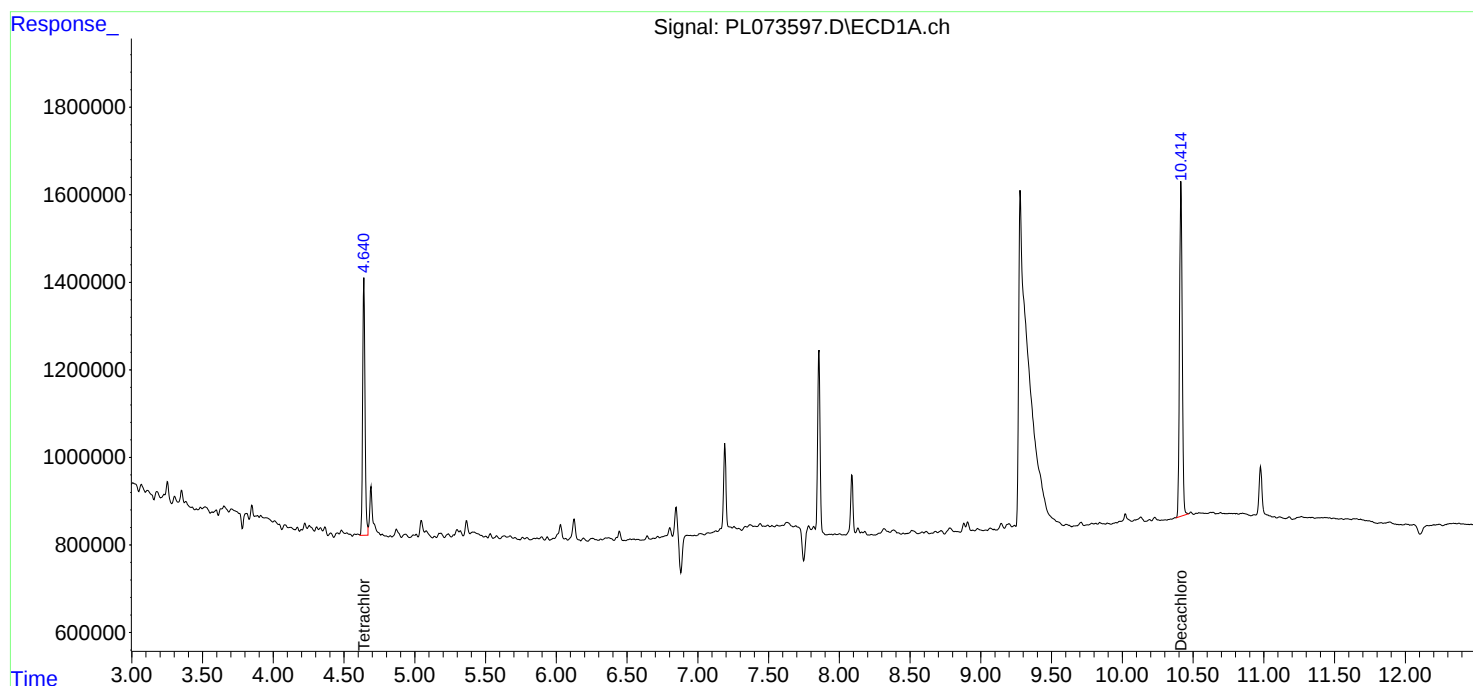

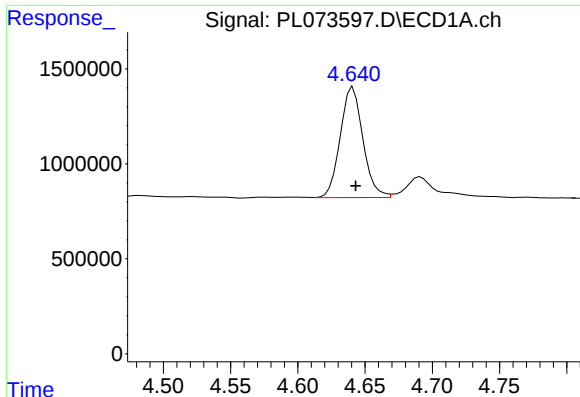


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: -0.003 min
Response: 6811563
Conc: 21.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-14A-1A-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

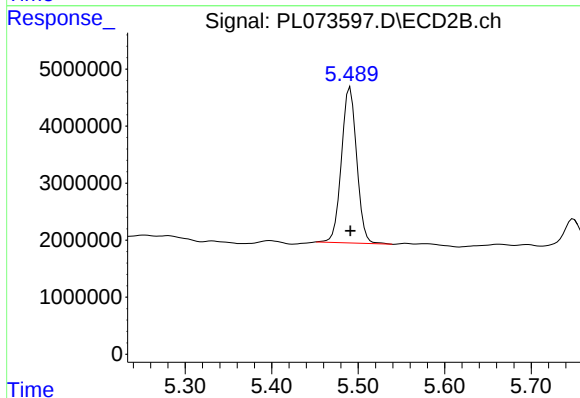


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 33179124
Conc: 20.22 ng/ml

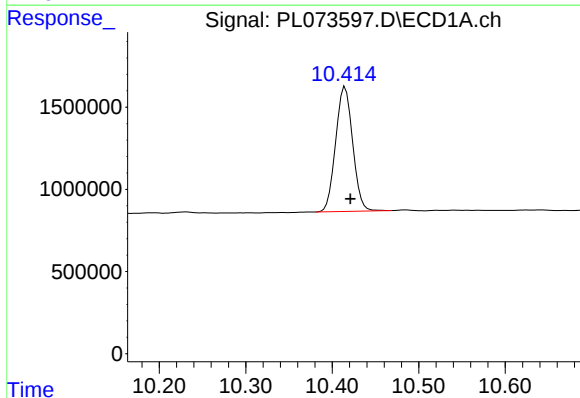

#28 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.006 min
Response: 10329614
Conc: 20.31 ng/ml

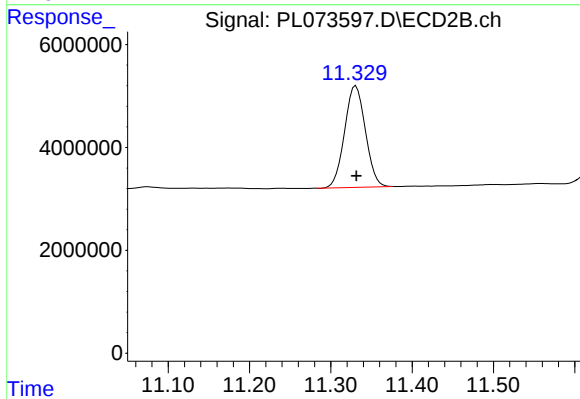

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.000 min
Response: 35030205
Conc: 19.59 ng/ml