

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 14:48
 Operator : AR\AJ
 Sample : N2063-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-4-1-(10-10.5)

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/24/2022
 Supervised By : mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:28:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.639	5.491	6233429	31951173	19.462m	19.468
28) SA Decachlor...	10.415	11.331	9146821	30729583	17.988	17.185

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 14:48
Operator : AR\AJ
Sample : N2063-04
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WC-4-1-(10-10.5)


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/24/2022
Supervised By : mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:28:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

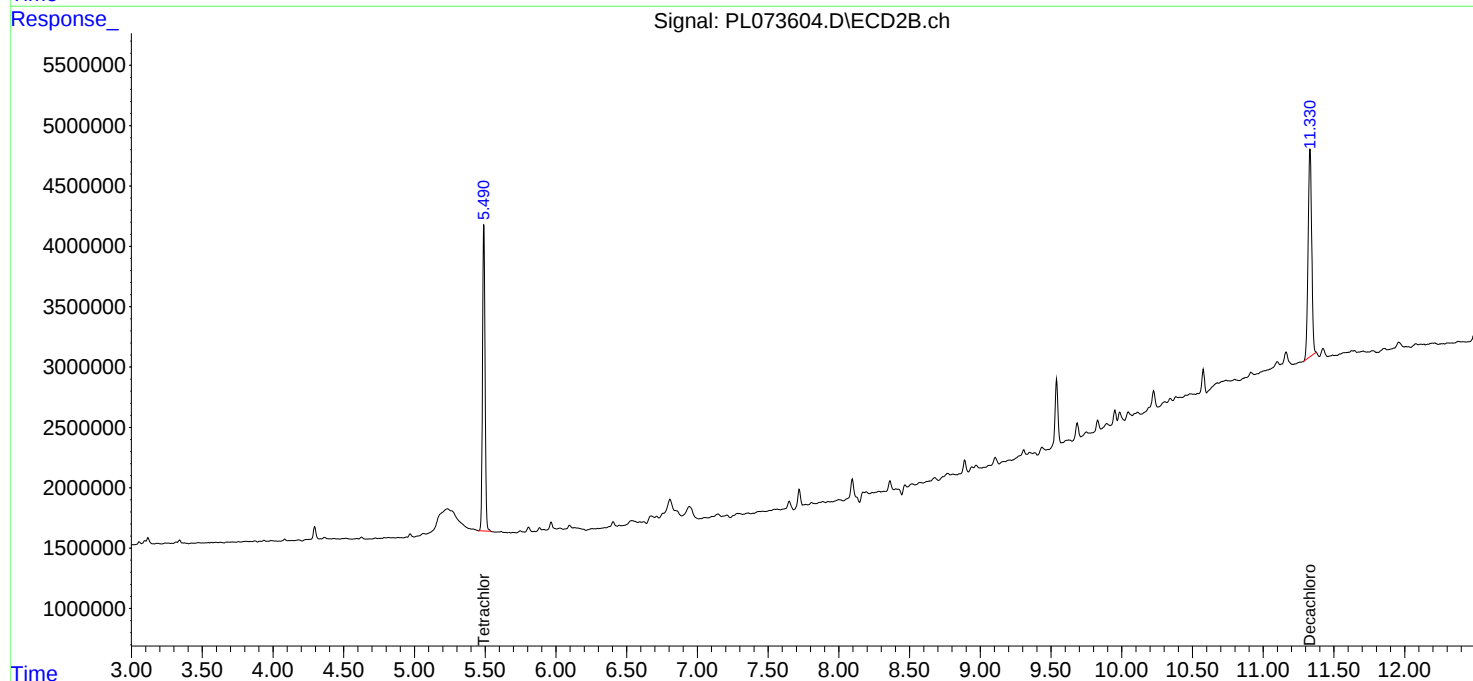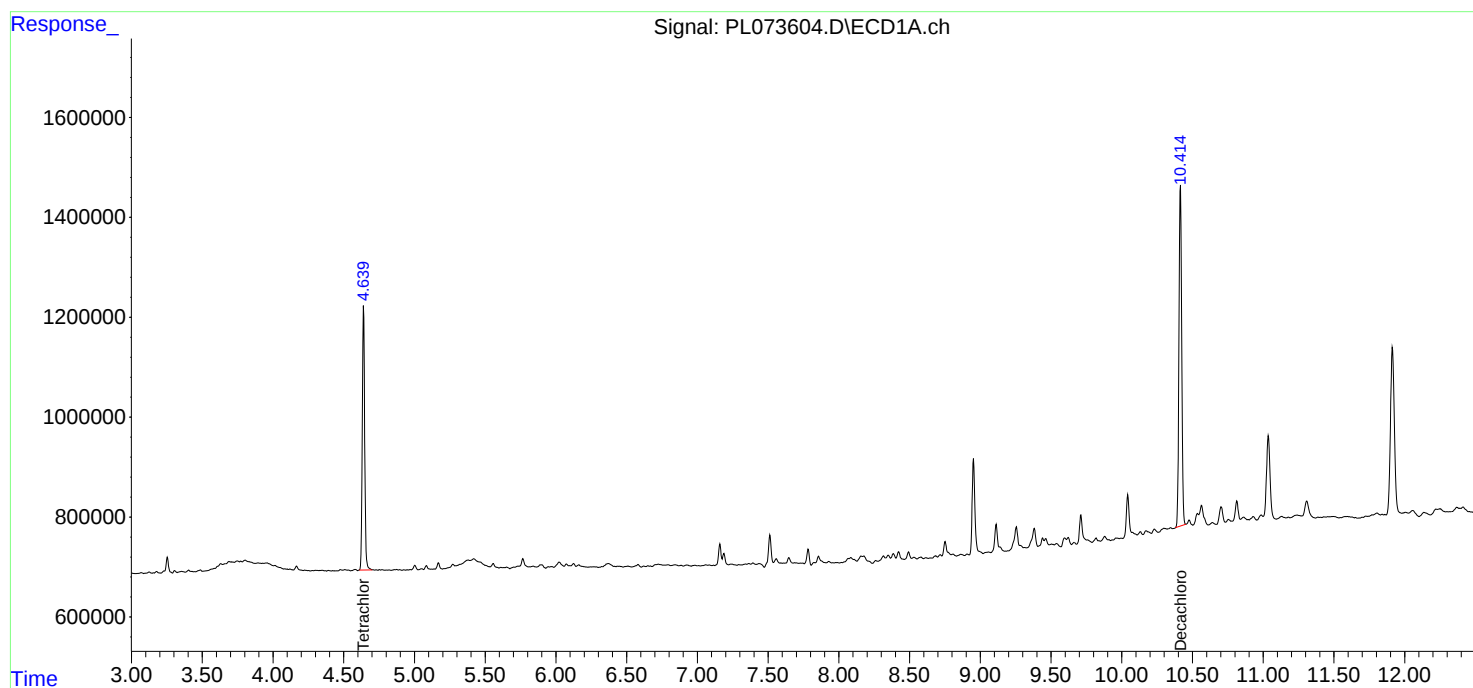

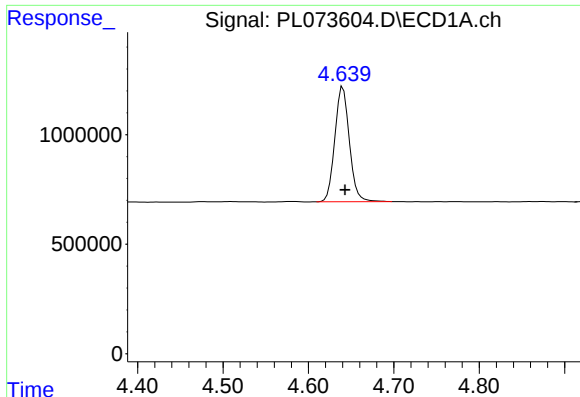


#1 Tetrachloro-m-xylene

R.T.: 4.639 min
Delta R.T.: -0.004 min
Response: 6233429
Conc: 19.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-4-1-(10-10.5)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

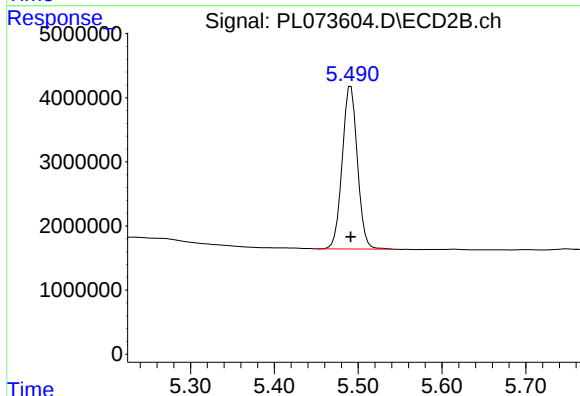


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 31951173
Conc: 19.47 ng/ml

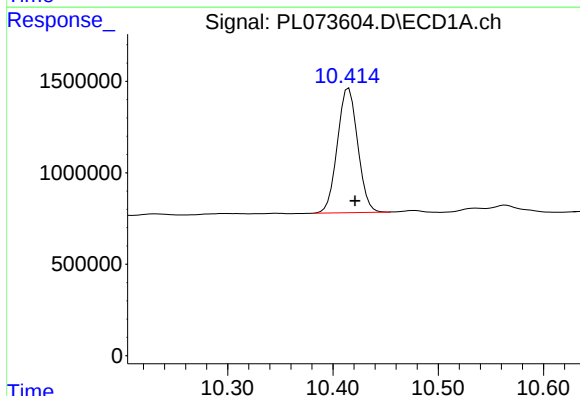

#28 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.006 min
Response: 9146821
Conc: 17.99 ng/ml

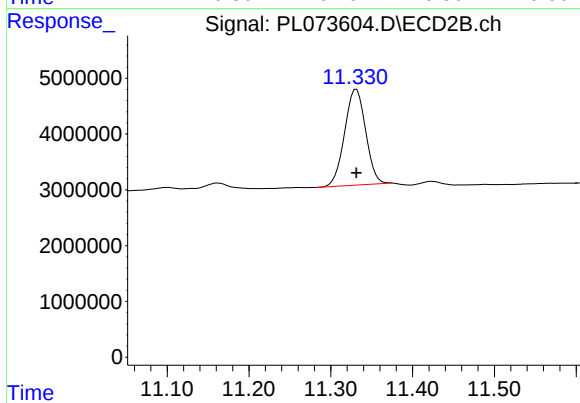

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.000 min
Response: 30729583
Conc: 17.18 ng/ml