

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
 Data File : PL073611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2022 16:47
 Operator : AR\AJ
 Sample : PB143543BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB143543BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/24/2022
 Supervised By : mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 04:30:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.648	5.490	59384	331613	0.185	0.202m
28) SA Decachlor...	10.432	11.313f	673263	364135	1.324m	0.204m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032322\
Data File : PL073611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2022 16:47
Operator : AR\AJ
Sample : PB143543BL
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB143543BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/24/2022
Supervised By : mohammad ahmed 03/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 04:30:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

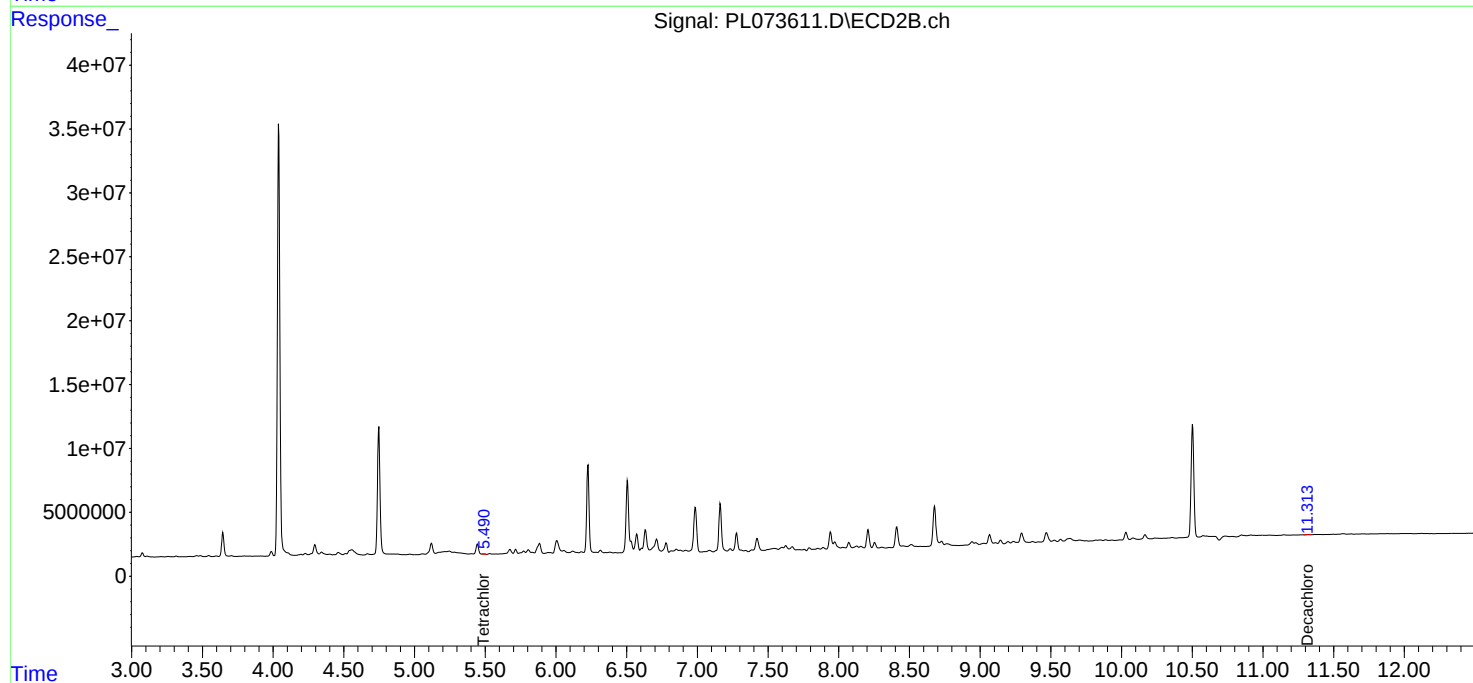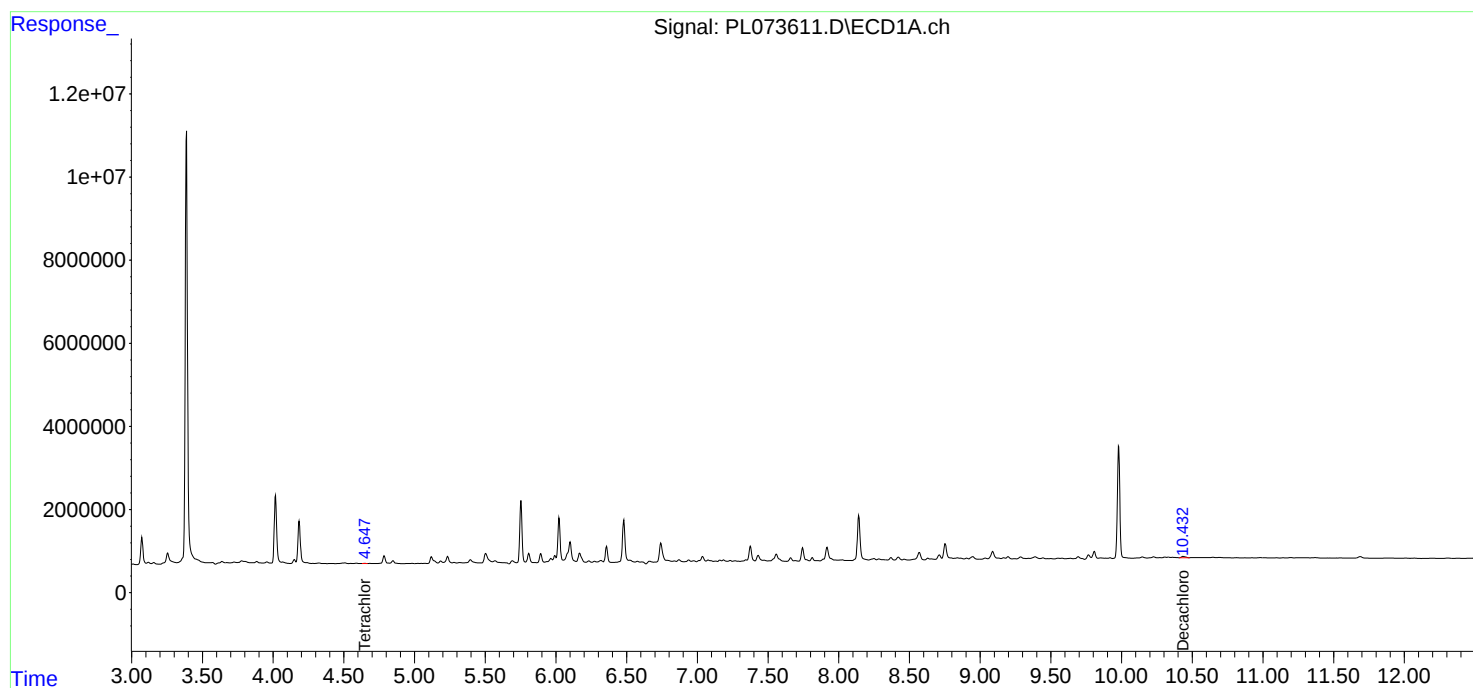

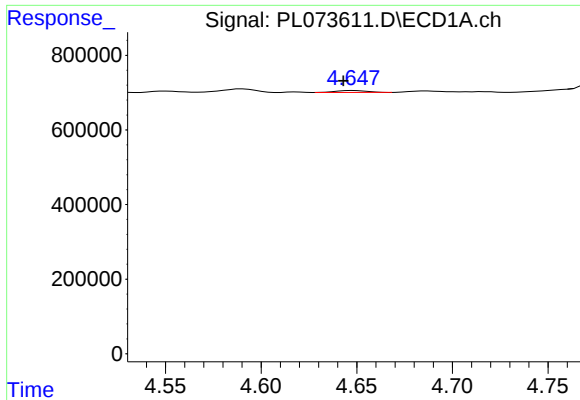


#1 Tetrachloro-m-xylene

R.T.: 4.648 min
Delta R.T.: 0.005 min
Response: 59384
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143543BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/24/2022
Supervised By :mohammad ahmed 03/25/2022

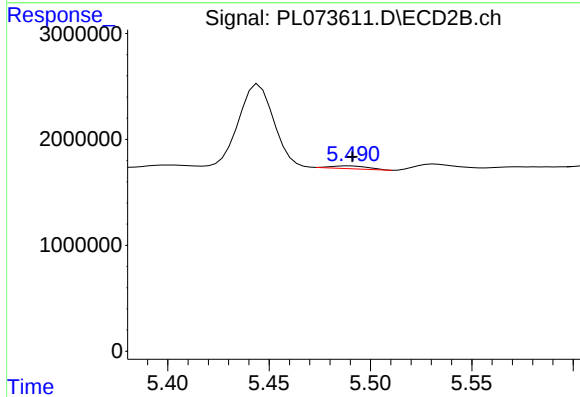


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 331613
Conc: 0.20 ng/ml m

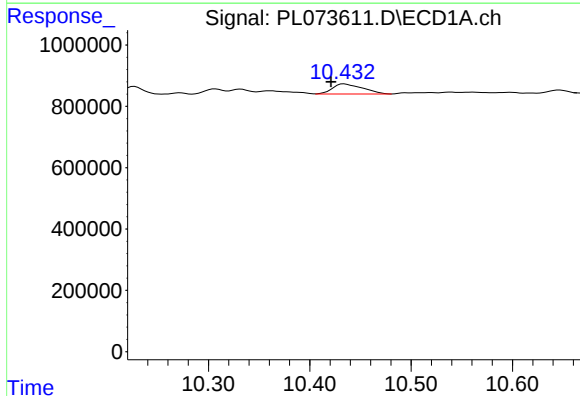

#28 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.011 min
Response: 673263
Conc: 1.32 ng/ml m

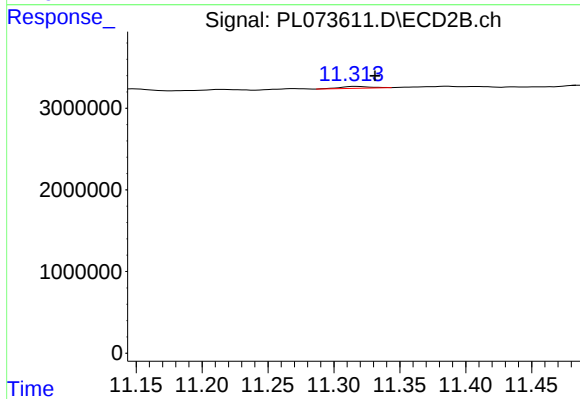

#28 Decachlorobiphenyl

R.T.: 11.313 min
Delta R.T.: -0.018 min
Response: 364135
Conc: 0.20 ng/ml m