

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032323\
 Data File : PL081669.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Mar 2023 12:21
 Operator : AR\AJ
 Sample : 02023-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-11-TEST-PIT-ON-CENTRAL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 03:02:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 23 01:07:33 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.329	2.658	20895467	18335007	8.984	9.185
28) SA Decachlor...	8.751	7.776	17025871	17552471	9.514	8.850

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032323\
Data File : PL081669.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Mar 2023 12:21
Operator : AR\AJ
Sample : 02023-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-11-TEST-PIT-ON-CENTRAL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 03:02:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032223.M
Quant Title : GC Extractables
QLast Update : Thu Mar 23 01:07:33 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

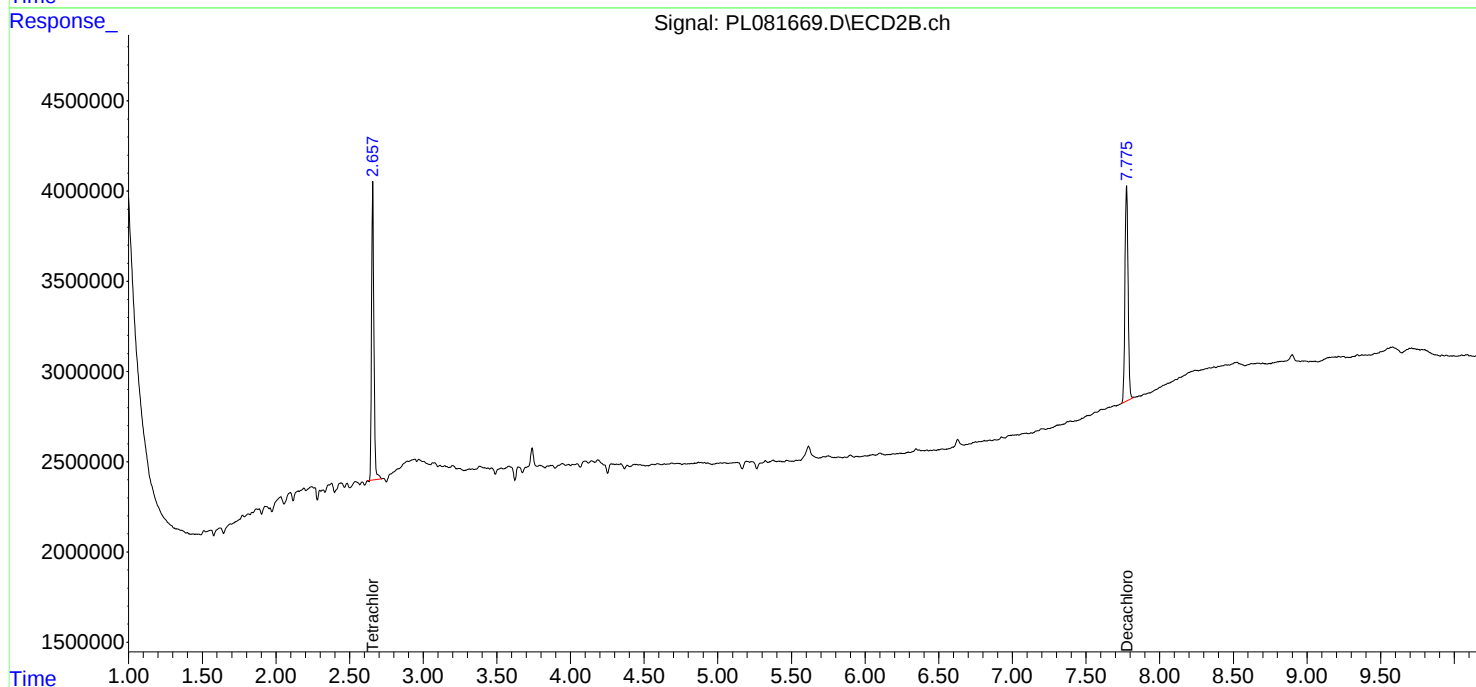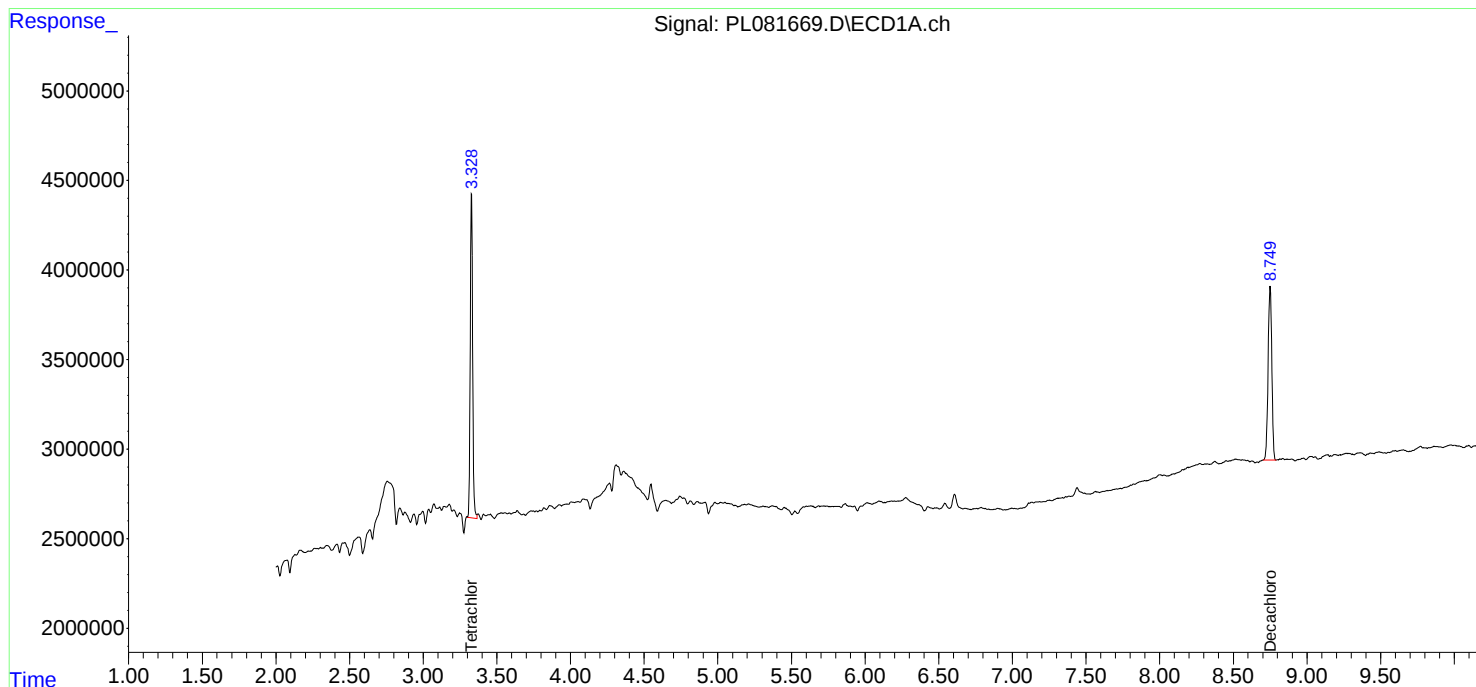


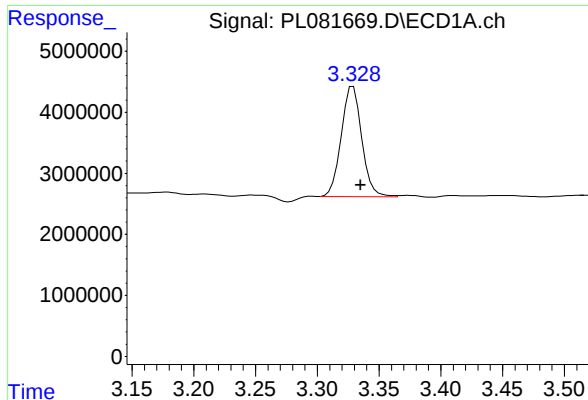

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: -0.006 min
Response: 20895467
Conc: 8.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-11-TEST-PIT-ON-CENTRAL

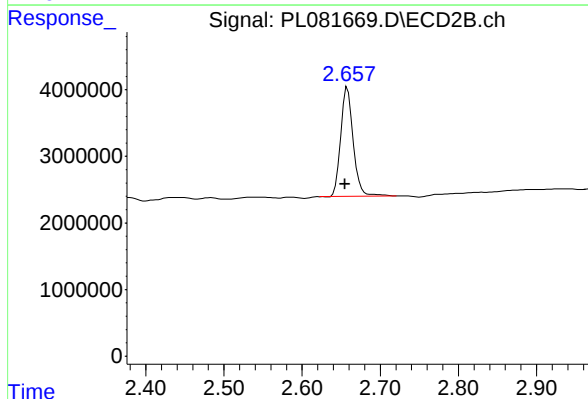


#1 Tetrachloro-m-xylene

R.T.: 2.658 min
Delta R.T.: 0.003 min
Response: 18335007
Conc: 9.19 ng/ml

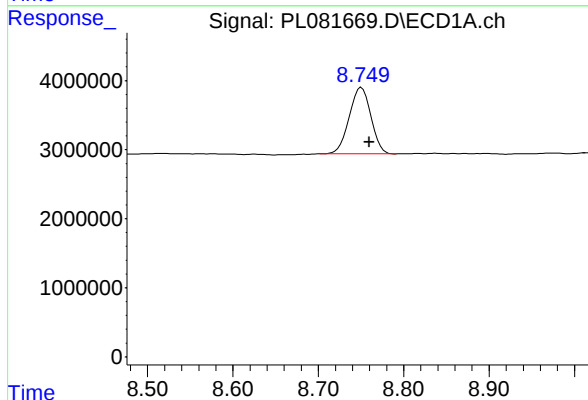

#28 Decachlorobiphenyl

R.T.: 8.751 min
Delta R.T.: -0.009 min
Response: 17025871
Conc: 9.51 ng/ml

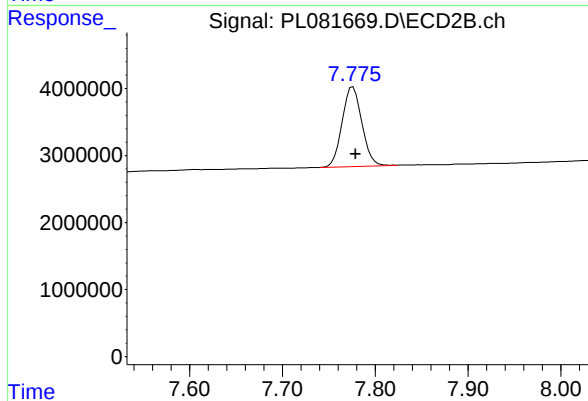

#28 Decachlorobiphenyl

R.T.: 7.776 min
Delta R.T.: -0.003 min
Response: 17552471
Conc: 8.85 ng/ml