

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032420\
 Data File : PL057533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2020 12:58
 Operator : AJ\MA
 Sample : PB127764BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 04:54:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 16 09:40:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.956	191.7E6	42594184	20.681	19.633
28)	SA Decachlor...	8.206	8.977	211.0E6	46098887	19.944	20.790
Target Compounds							
2)	A alpha-BHC	3.896	0.000	3901964	0	0.245	N.D. #
14)	MA Endrin	6.005	0.000	225946	0	0.020	N.D. #
15)	B Endosulfa...	6.289	0.000	640268	0	0.059	N.D. #
16)	A 4,4'-DDD	6.130	0.000	183255	0	0.019	N.D. #
18)	B Endrin al...	6.447	0.000	255213	0	0.028	N.D. #
19)	B Endosulfa...	6.681f	0.000	136123	0	0.014	N.D. #
22)	Mirex	7.340	0.000	393915	0	0.049	N.D. #
23)	Chlordane-1	4.355f	0.000	1740119	0	5.361	N.D. #
24)	Chlordane-2	4.801f	0.000	34239	0	0.094	N.D. #
27)	Chlordane-5	6.289	0.000	640268	0	1.760	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032420\
Data File : PL057533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2020 12:58
Operator : AJ\MA
Sample : PB127764BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 04:54:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031420.M
Quant Title : GC Extractables
QLast Update : Mon Mar 16 09:40:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

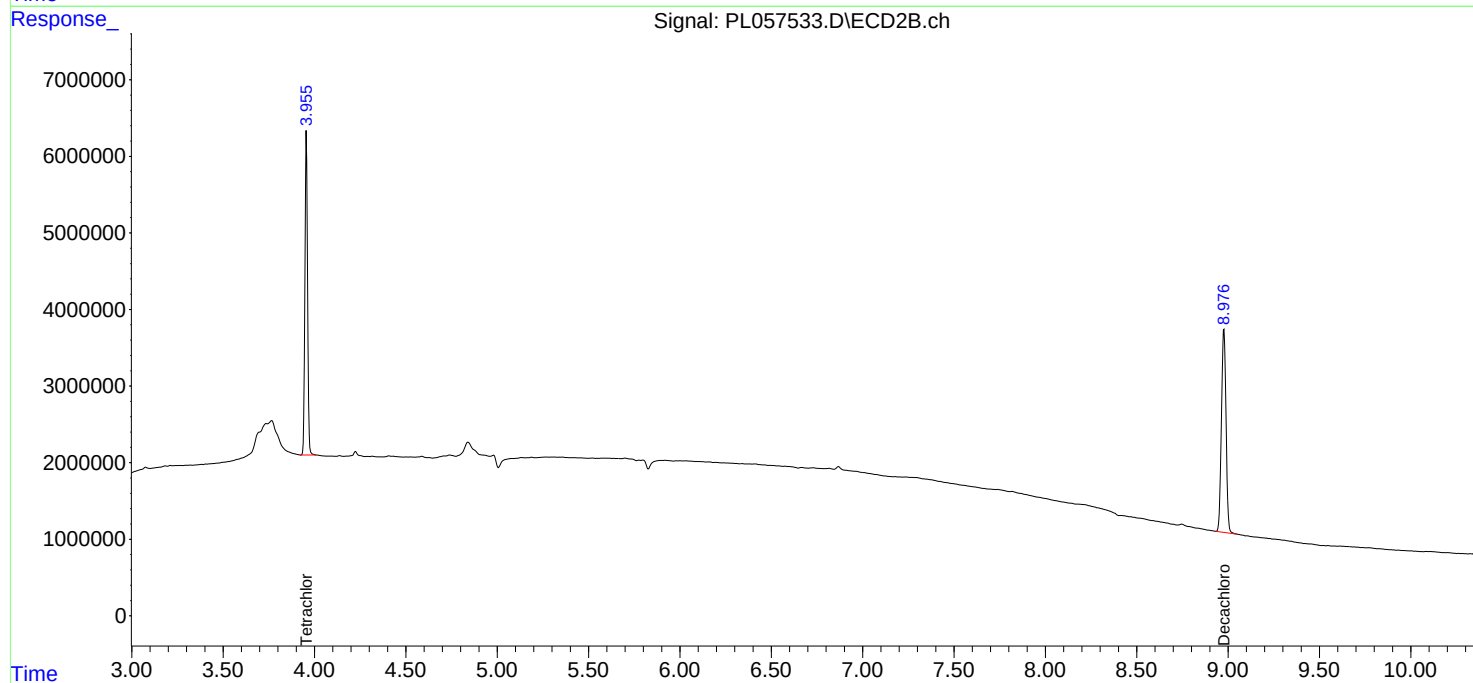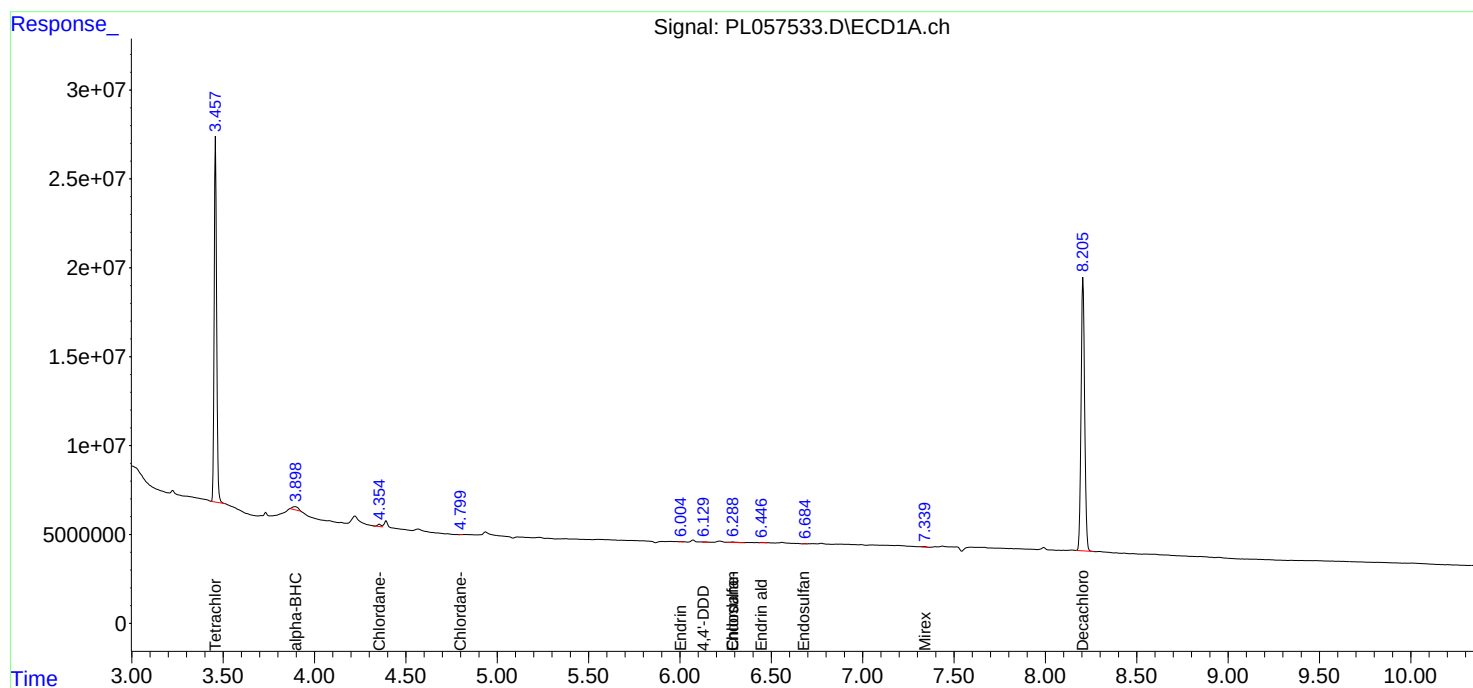


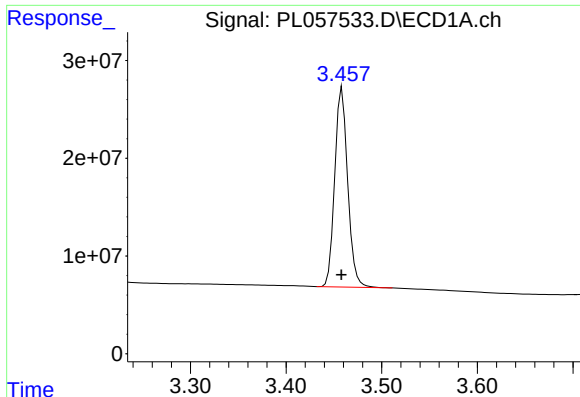

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: 0.000 min
Response: 191702904
Conc: 20.68 ng/ml

Instrument :
ECD_L
ClientSampleId :

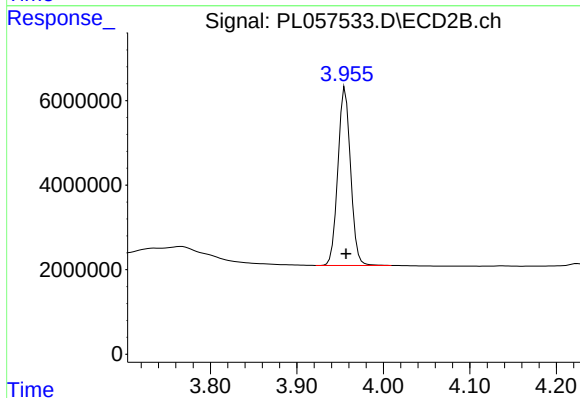


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.001 min
Response: 42594184
Conc: 19.63 ng/ml

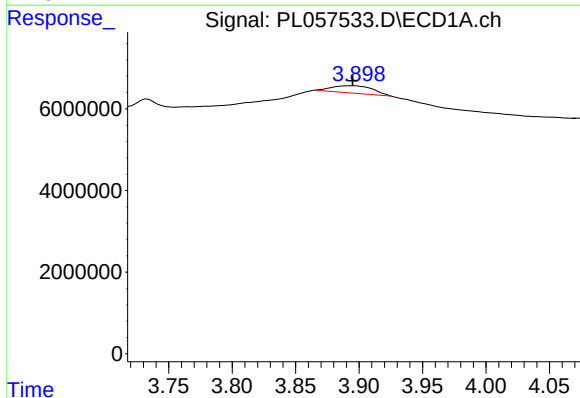


#2 alpha-BHC

R.T.: 3.896 min
Delta R.T.: 0.000 min
Response: 3901964
Conc: 0.24 ng/ml

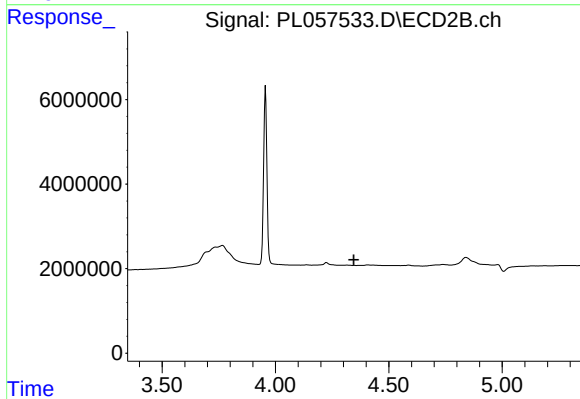

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.345 min
Response: 0
Conc: N.D.

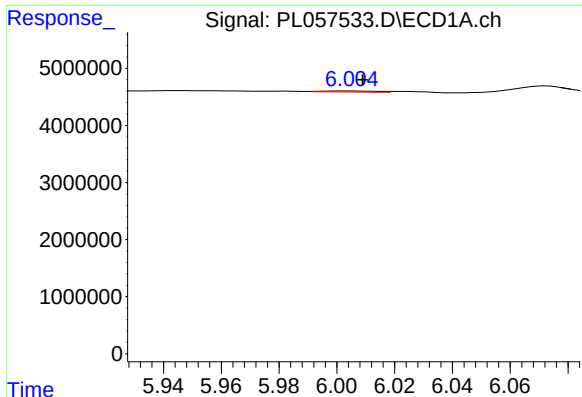

#14 Endrin


R.T.: 6.005 min
Delta R.T.: -0.004 min
Response: 225946
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

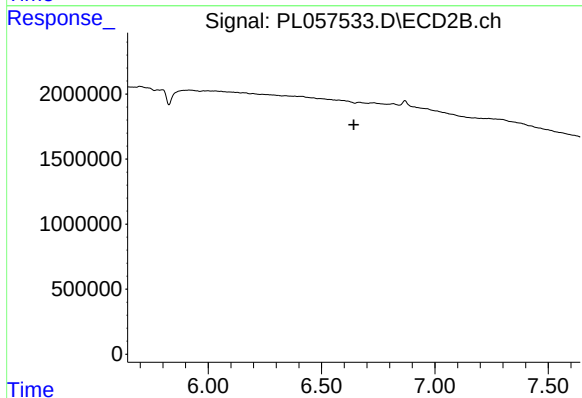


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

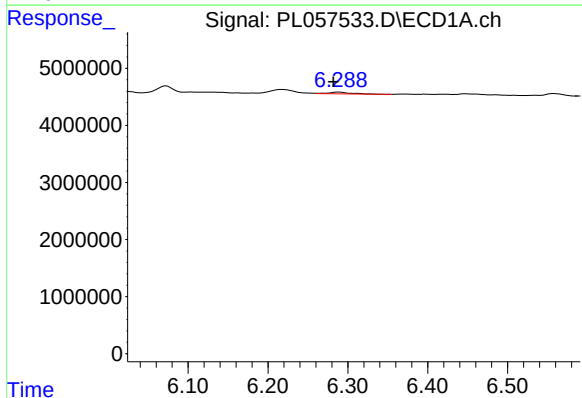


#15 Endosulfan II

R.T.: 6.289 min
Delta R.T.: 0.007 min
Response: 640268
Conc: 0.06 ng/ml

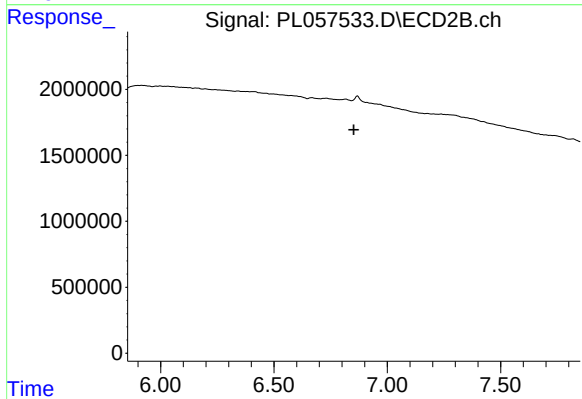

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.852 min
Response: 0
Conc: N.D.

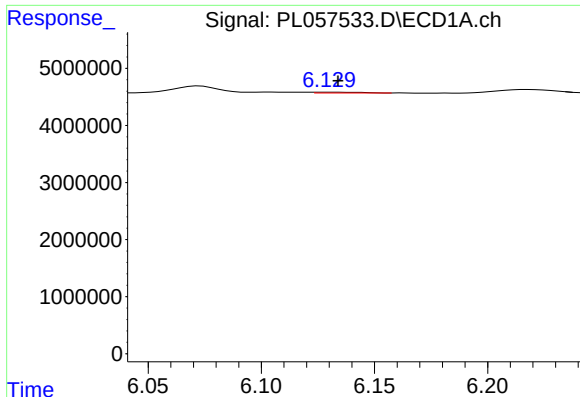

#16 4,4'-DDD


R.T.: 6.130 min
Delta R.T.: -0.004 min
Response: 183255
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

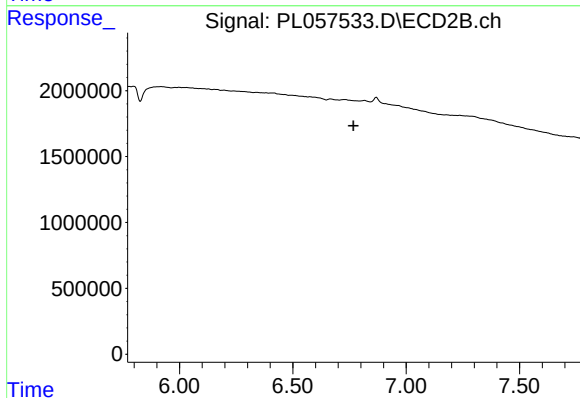


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

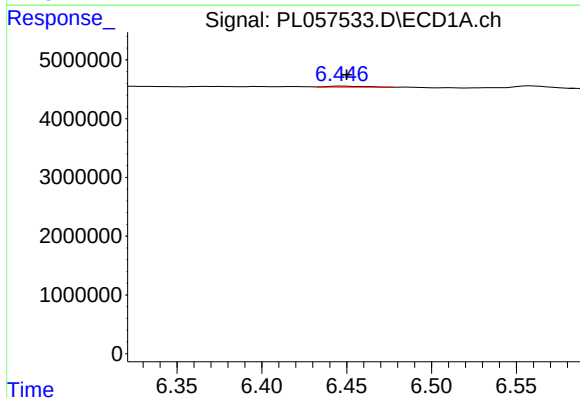


#18 Endrin aldehyde

R.T.: 6.447 min
Delta R.T.: -0.003 min
Response: 255213
Conc: 0.03 ng/ml

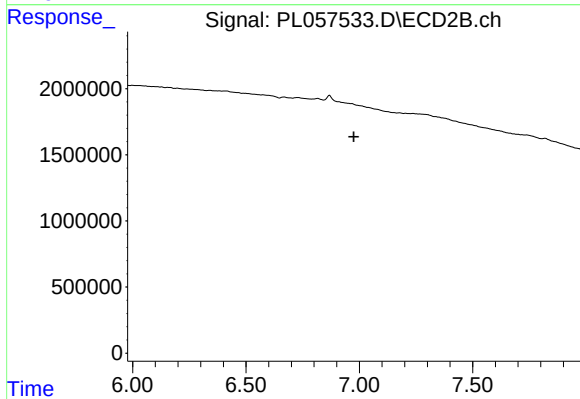

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.976 min
Response: 0
Conc: N.D.

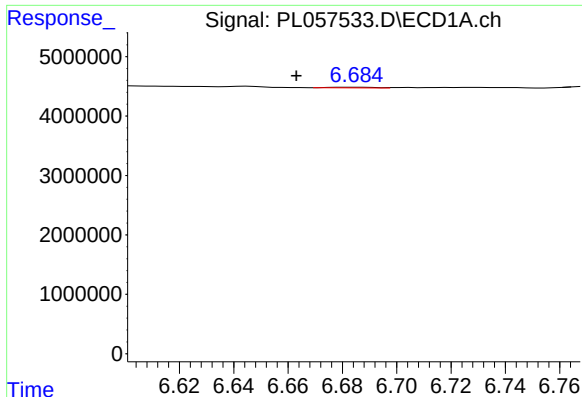

#19 Endosulfan Sulfate


R.T.: 6.681 min
Delta R.T.: 0.018 min
Response: 136123
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

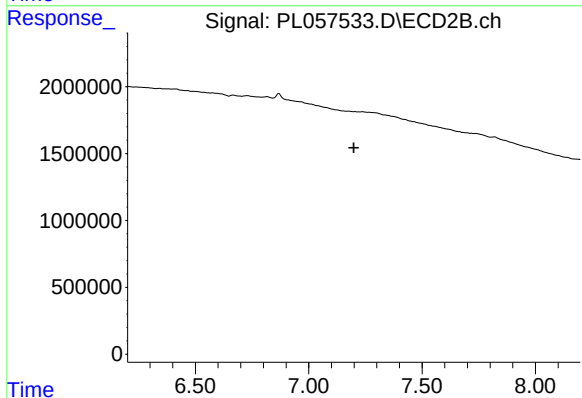


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

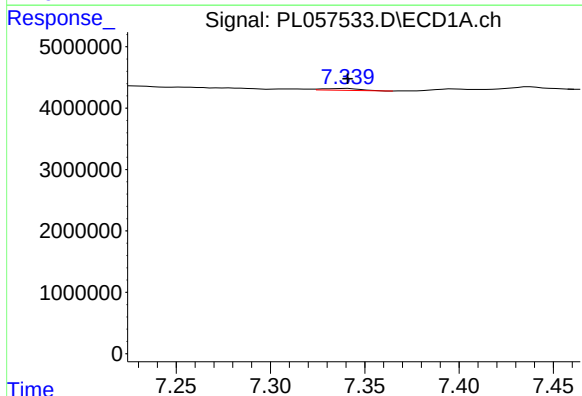


#22 Mirex

R.T.: 7.340 min
Delta R.T.: 0.000 min
Response: 393915
Conc: 0.05 ng/ml

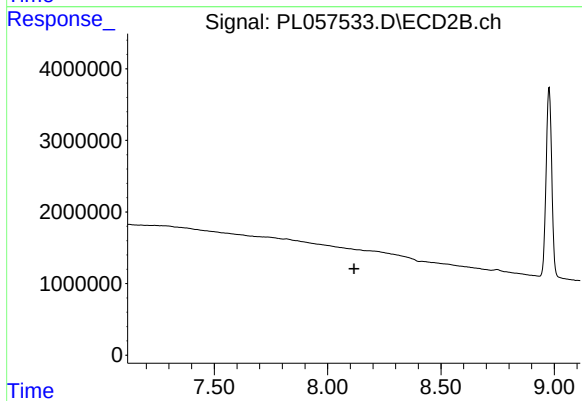

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.116 min
Response: 0
Conc: N.D.

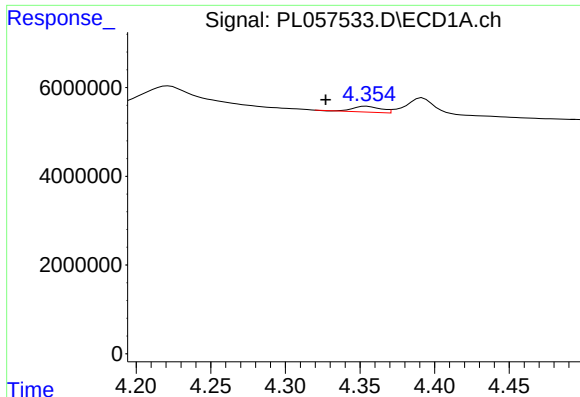

#23 Chlordane-1


R.T.: 4.355 min
Delta R.T.: 0.028 min
Response: 1740119
Conc: 5.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

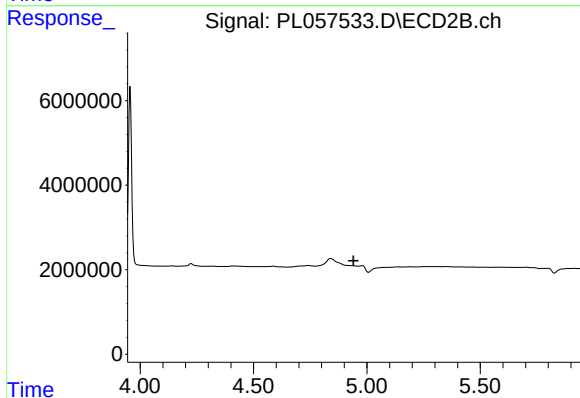


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.941 min
Response: 0
Conc: N.D.

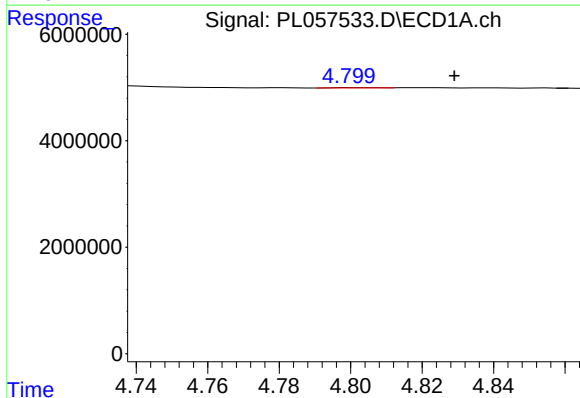


#24 Chlordane-2

R.T.: 4.801 min
Delta R.T.: -0.028 min
Response: 34239
Conc: 0.09 ng/ml

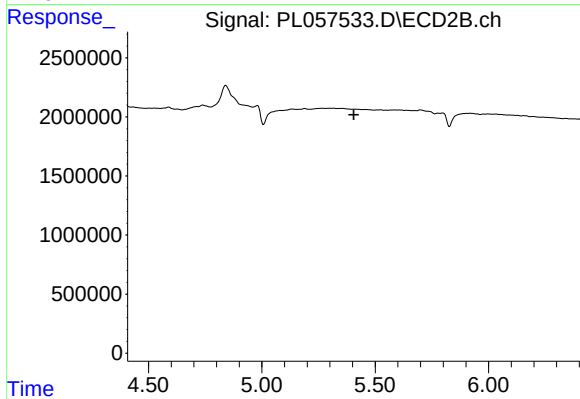

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.406 min
Response: 0
Conc: N.D.

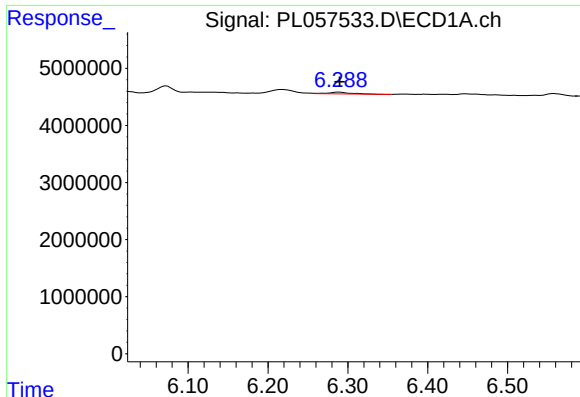

#27 Chlordane-5


R.T.: 6.289 min
Delta R.T.: 0.000 min
Response: 640268
Conc: 1.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

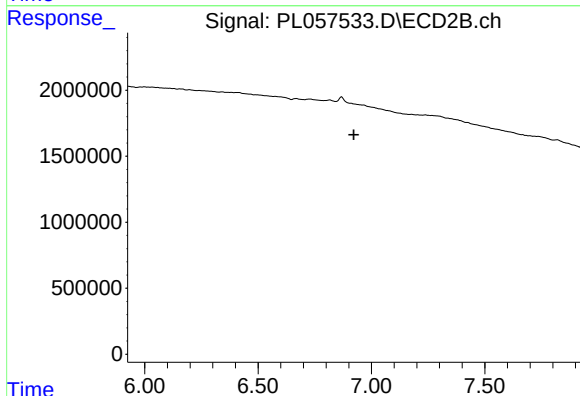


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

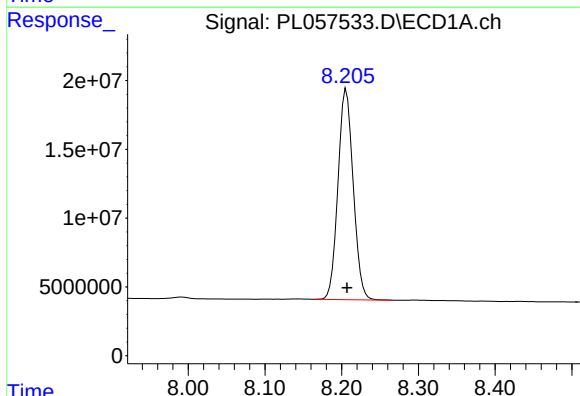

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.001 min
Response: 211032246
Conc: 19.94 ng/ml

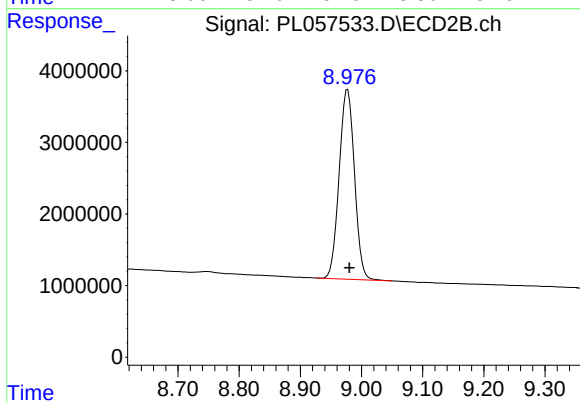

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.003 min
Response: 46098887
Conc: 20.79 ng/ml