

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032422\
 Data File : PL073650.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 11:40
 Operator : AR\AJ
 Sample : N2058-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 01:21:44 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.649	5.488	7417752	41838398	23.160	25.492
28)	SA Decachlor...	10.421	11.333	12595849	43991453	24.771	24.601
Target Compounds							
6)	B beta-BHC	6.134f	0.000	369814	0	1.796	N.D. #
7)	B delta-BHC	0.000	6.958	0	5458873	N.D.	2.535 #
10)	B gamma-Chl...	7.344f	8.192	32701	417185	0.075	0.204 #
11)	B alpha-Chl...	0.000	8.285	0	28527	N.D.	0.014 #
13)	MA Dieldrin	7.752f	0.000	49268	0	0.118	N.D. #
14)	MA Endrin	8.097f	0.000	717784	0	1.850	N.D. #
20)	A Methoxychlor	0.000	9.814f	0	122710	N.D.	0.136 #
25)	Chlordane-3	7.344f	8.192	32701	417185	0.801	1.539 #
26)	Chlordane-4	0.000	8.285	0	28527	N.D.	0.086 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032422\
Data File : PL073650.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 11:40
Operator : AR\AJ
Sample : N2058-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 01:21:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

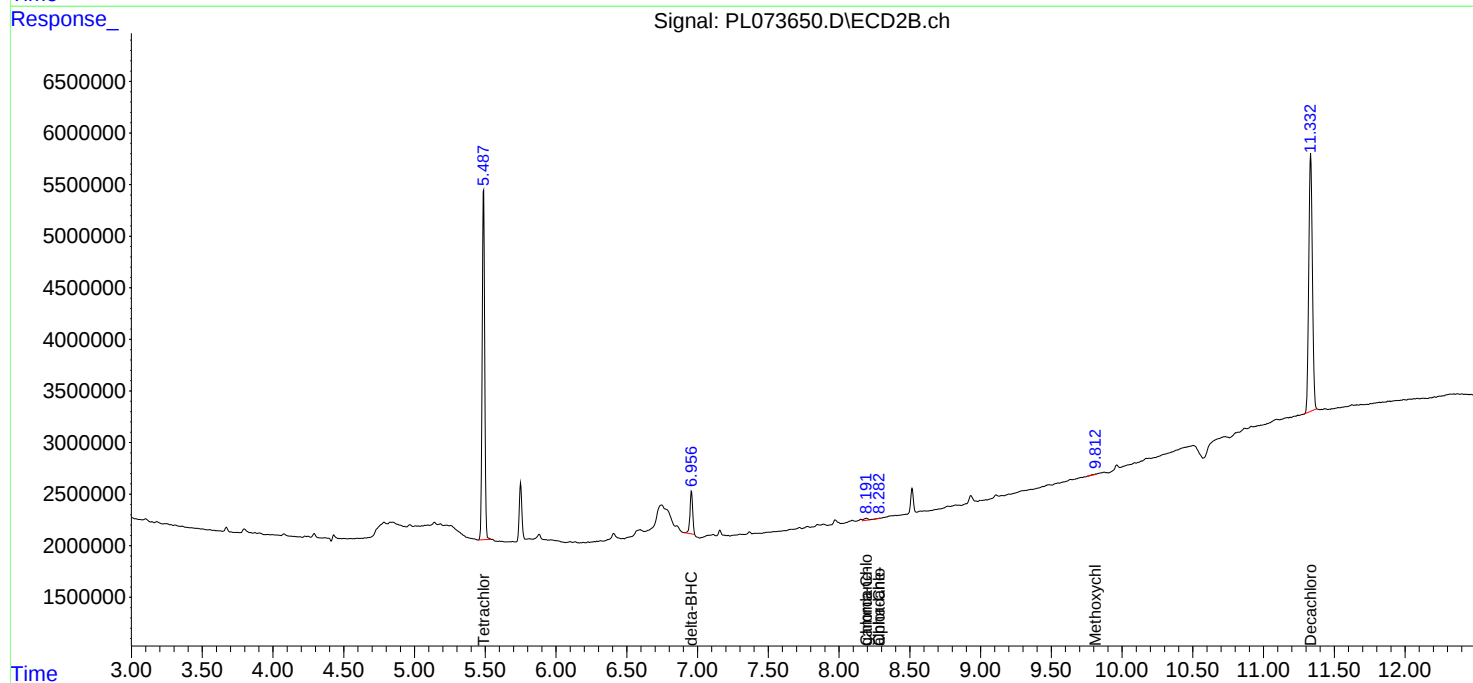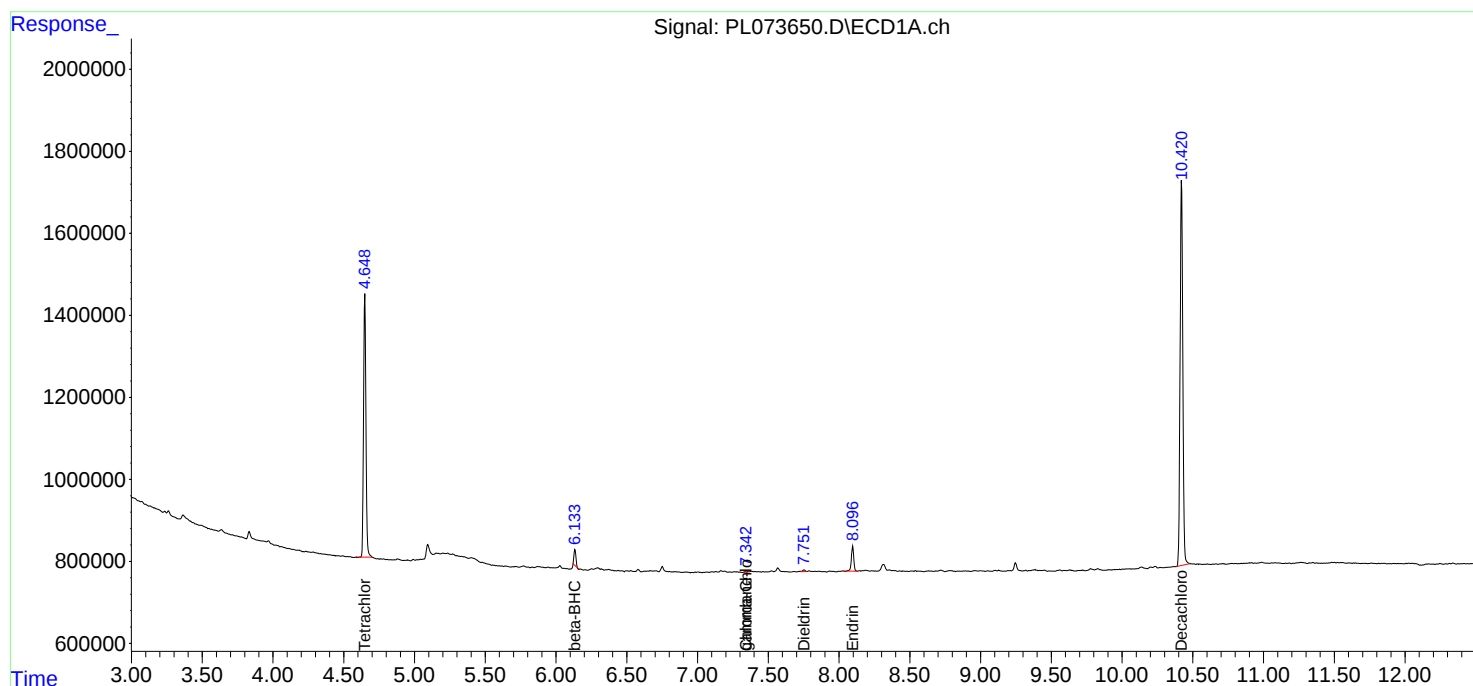


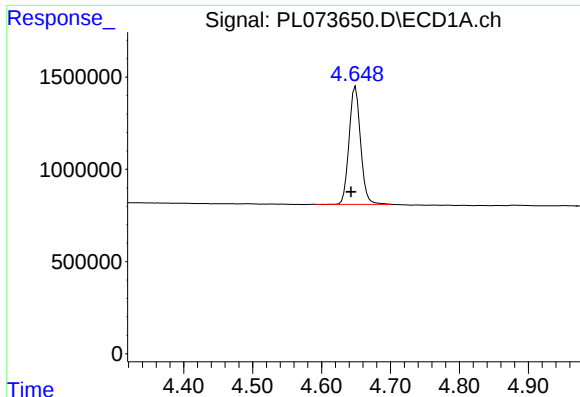

#1 Tetrachloro-m-xylene


R.T.: 4.649 min
Delta R.T.: 0.006 min
Response: 7417752
Conc: 23.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

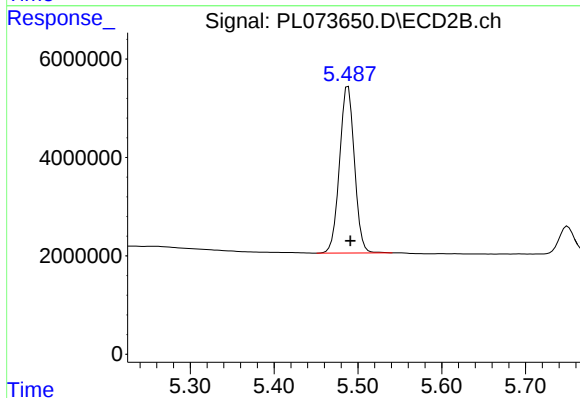


#1 Tetrachloro-m-xylene

R.T.: 5.488 min
Delta R.T.: -0.003 min
Response: 41838398
Conc: 25.49 ng/ml

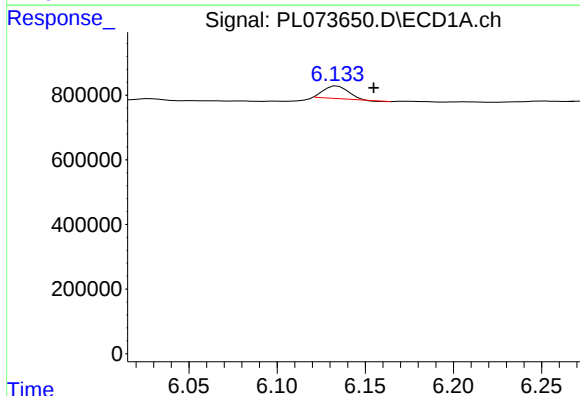


#6 beta-BHC

R.T.: 6.134 min
Delta R.T.: -0.021 min
Response: 369814
Conc: 1.80 ng/ml

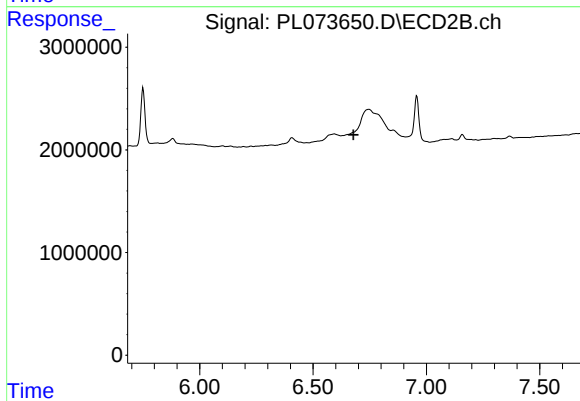

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.679 min
Response: 0
Conc: N.D.

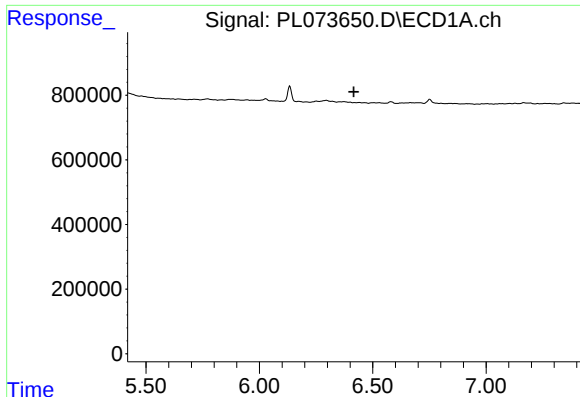

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

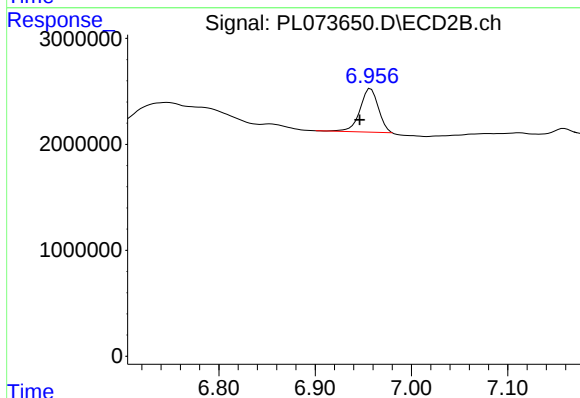


#7 delta-BHC

R.T.: 6.958 min
Delta R.T.: 0.011 min
Response: 5458873
Conc: 2.53 ng/ml

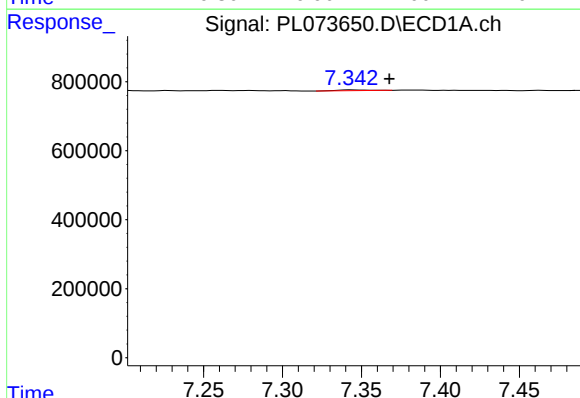


#10 gamma-Chlordane

R.T.: 7.344 min
Delta R.T.: -0.024 min
Response: 32701
Conc: 0.07 ng/ml

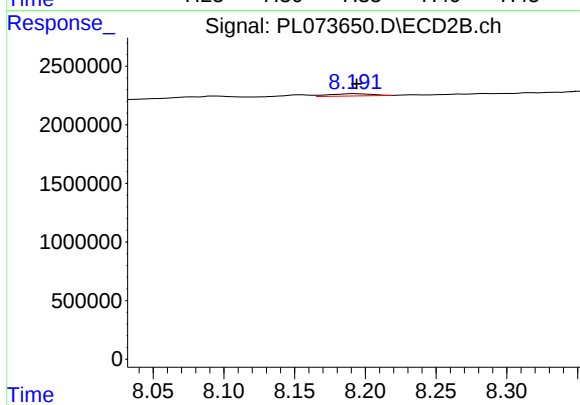

#10 gamma-Chlordane


R.T.: 8.192 min
Delta R.T.: -0.001 min
Response: 417185
Conc: 0.20 ng/ml

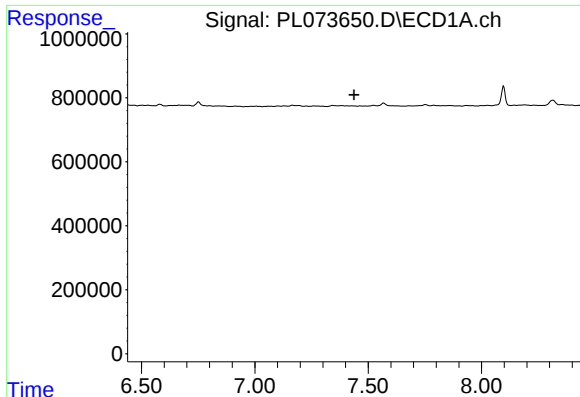

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

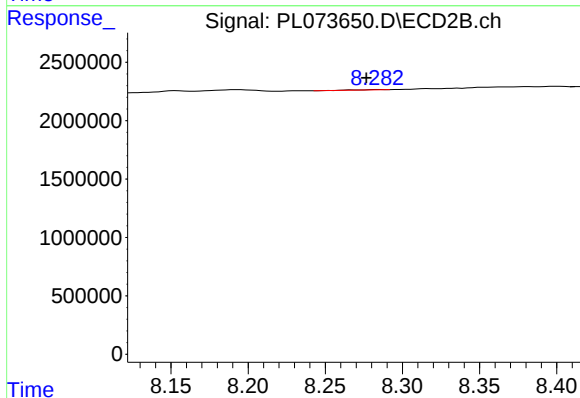


#11 alpha-Chlordane

R.T.: 8.285 min
Delta R.T.: 0.008 min
Response: 28527
Conc: 0.01 ng/ml

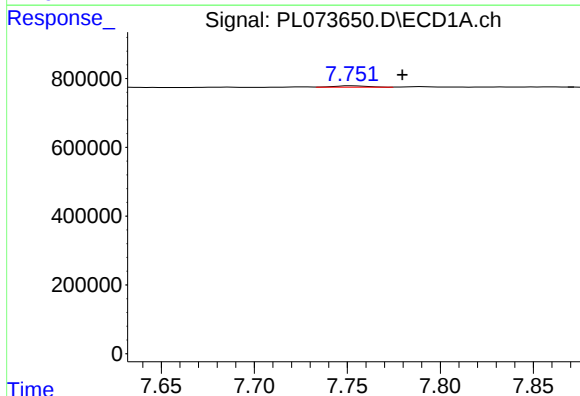


#13 Dieldrin

R.T.: 7.752 min
Delta R.T.: -0.027 min
Response: 49268
Conc: 0.12 ng/ml

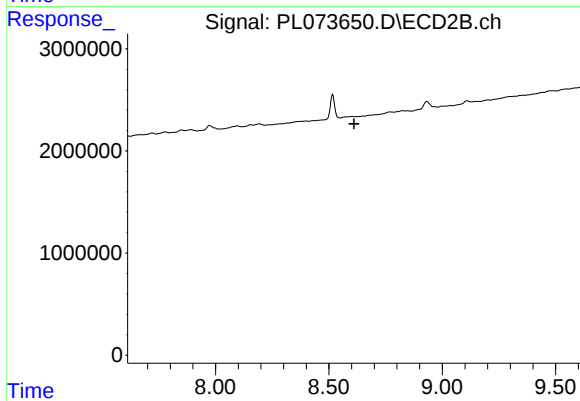

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.611 min
Response: 0
Conc: N.D.

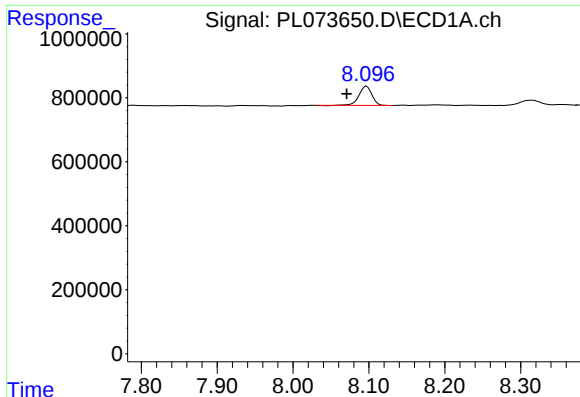

#14 Endrin


R.T.: 8.097 min
Delta R.T.: 0.026 min
Response: 717784
Conc: 1.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

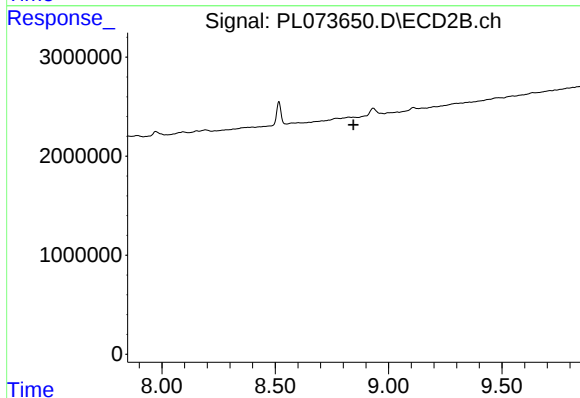


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

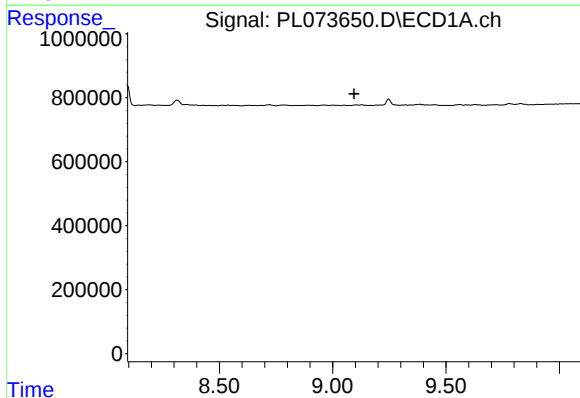


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.095 min
Response: 0
Conc: N.D.

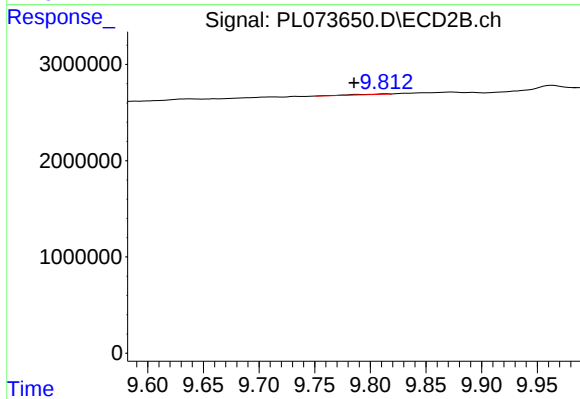

#20 Methoxychlor


R.T.: 9.814 min
Delta R.T.: 0.028 min
Response: 122710
Conc: 0.14 ng/ml

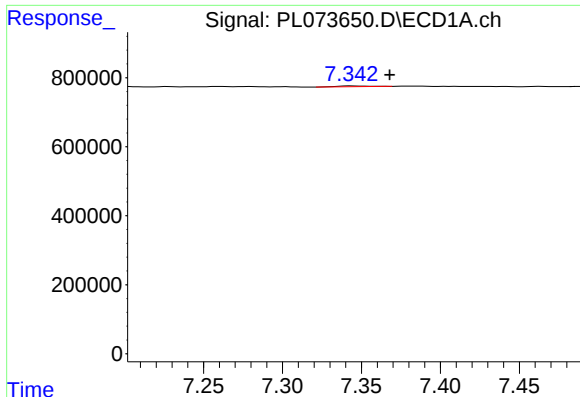

#25 Chlordane-3


R.T.: 7.344 min
Delta R.T.: -0.024 min
Response: 32701
Conc: 0.80 ng/ml

Instrument :
ECD_L
ClientSampleId :

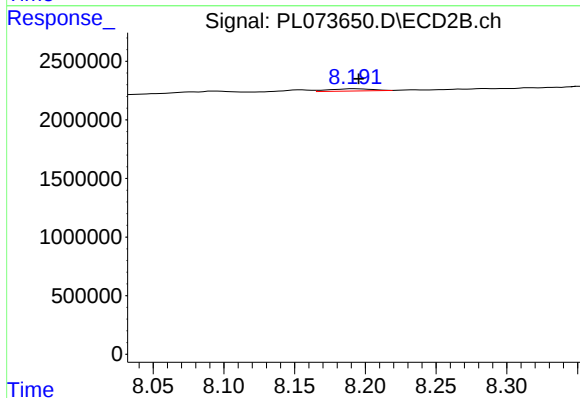


#25 Chlordane-3

R.T.: 8.192 min
Delta R.T.: -0.003 min
Response: 417185
Conc: 1.54 ng/ml

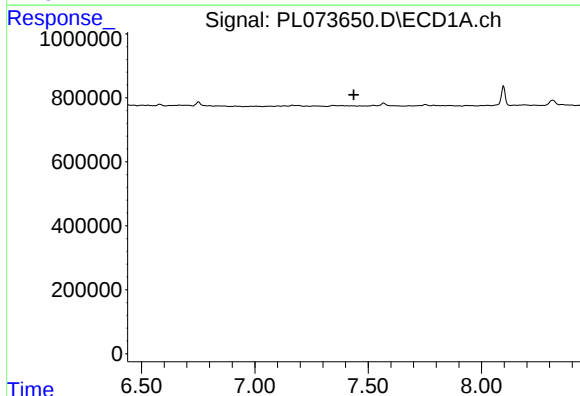


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 7.437 min
Response: 0
Conc: N.D.

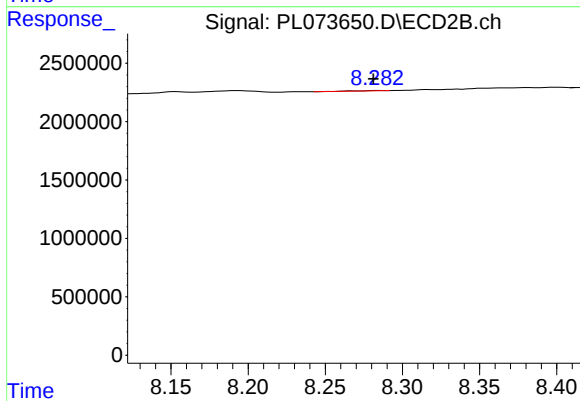

#26 Chlordane-4


R.T.: 8.285 min
Delta R.T.: 0.004 min
Response: 28527
Conc: 0.09 ng/ml

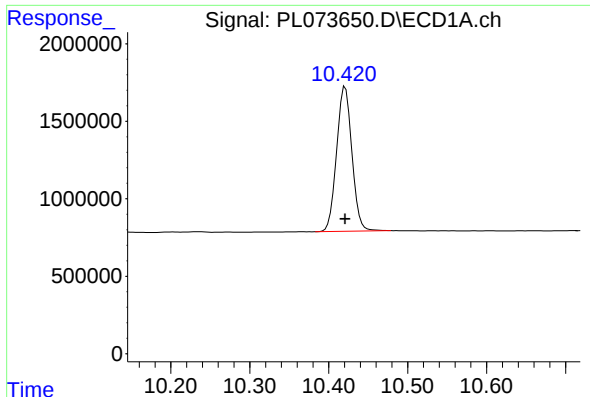

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: 0.000 min
Response: 12595849
Conc: 24.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

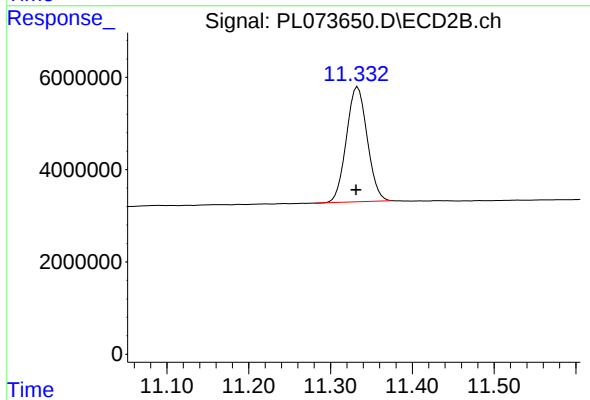

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: 0.002 min
Response: 43991453
Conc: 24.60 ng/ml