

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032422\
 Data File : PL073659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 15:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 01:27:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.491	7514163	40370910	23.461	24.598
28)	SA Decachlor...	10.415	11.333	12124870	41552705	23.844	23.237
Target Compounds							
6)	B beta-BHC	0.000	6.679	0	809110	N.D.	0.776 #
7)	B delta-BHC	0.000	6.941	0	1101074	N.D.	0.511 #
8)	B Heptachlo...	0.000	7.928	0	1236754	N.D.	0.619 #
9)	A Endosulfan I	0.000	8.350f	0	7904670	N.D.	4.330 #
10)	B gamma-Chl...	0.000	8.194	0	12673799	N.D.	6.205 #
13)	MA Dieldrin	7.791	0.000	589907	0	1.416	N.D. #
14)	MA Endrin	8.090f	8.826f	1103589	60034	2.844	0.039 #
15)	B Endosulfa...	0.000	9.058	0	2283930	N.D.	1.487 #
16)	A 4,4'-DDD	0.000	9.006f	0	5879245	N.D.	4.028 #
18)	B Endrin al...	0.000	9.202	0	93705	N.D.	0.076 #
20)	A Methoxychlor	0.000	9.792	0	59807	N.D.	0.066 #
23)	Chlordane-1	0.000	6.855	0	1022590	N.D.	14.969 #
25)	Chlordane-3	0.000	8.194	0	12673799	N.D.	46.744 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032422\
Data File : PL073659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 15:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 01:27:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

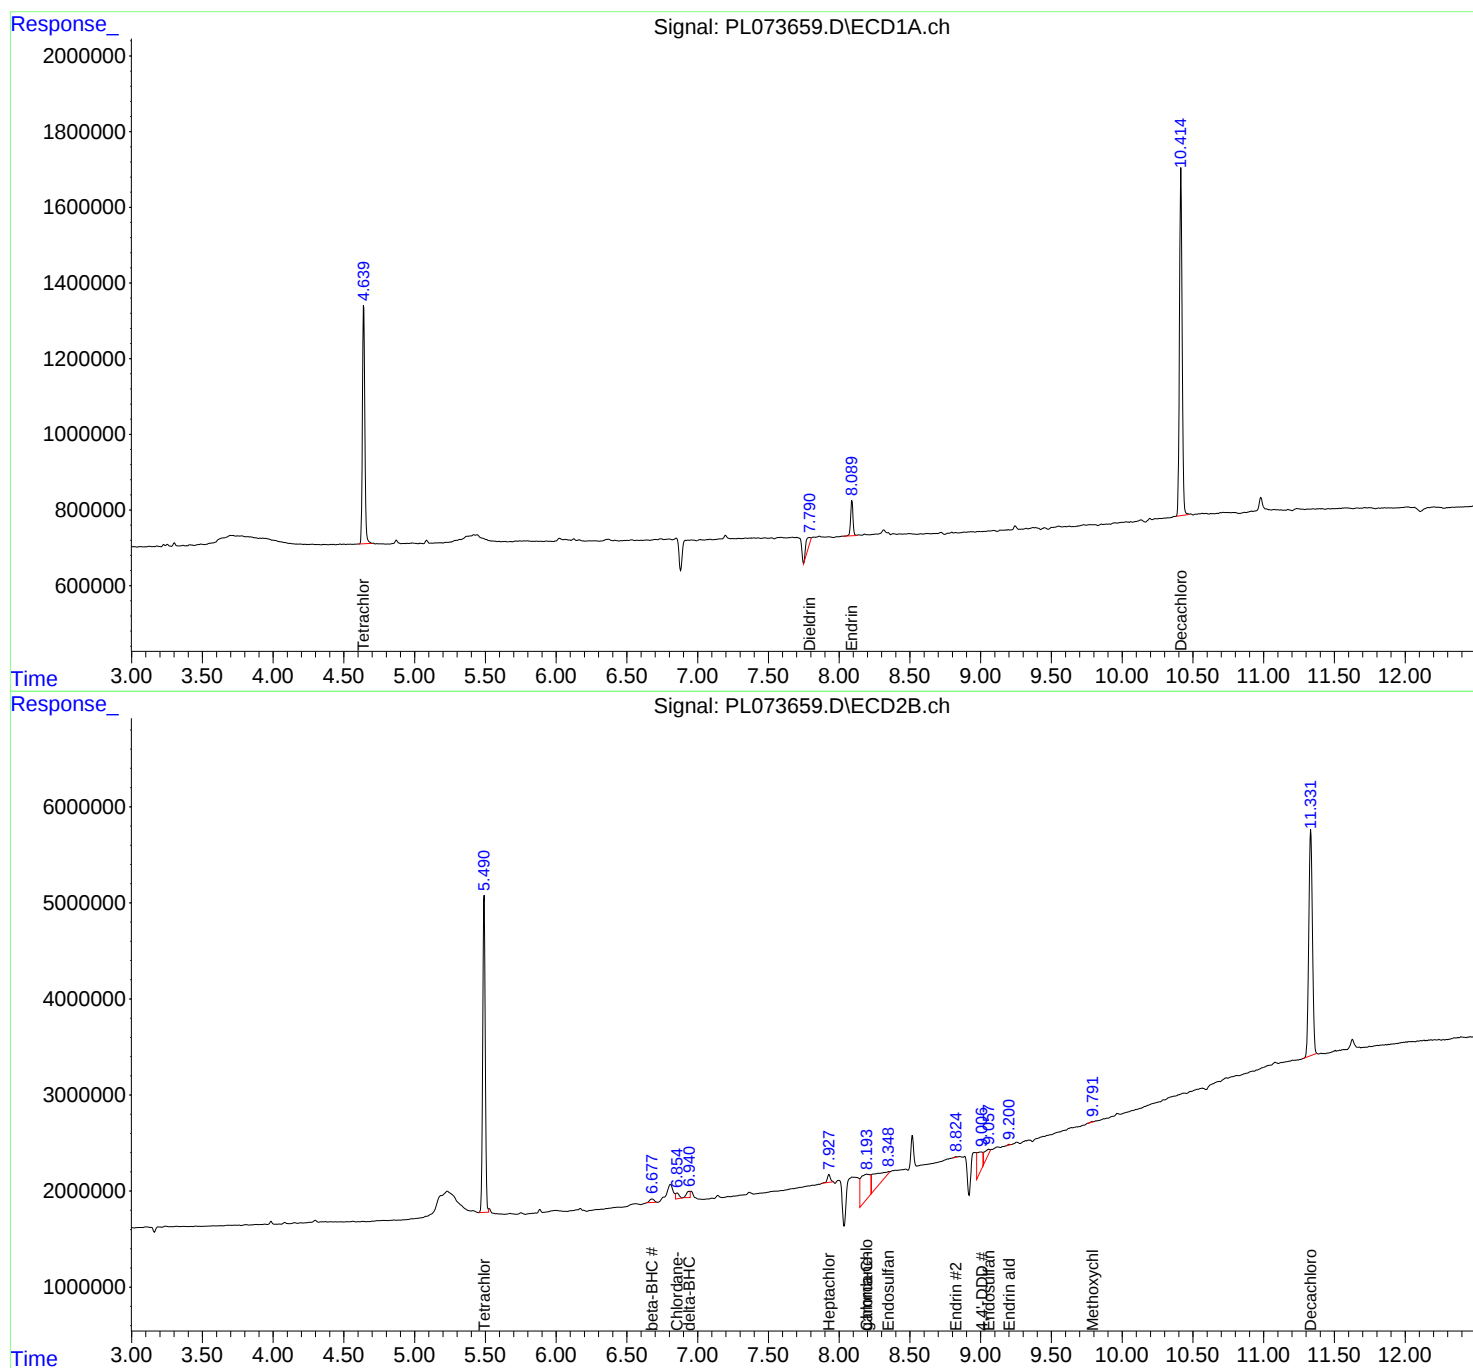


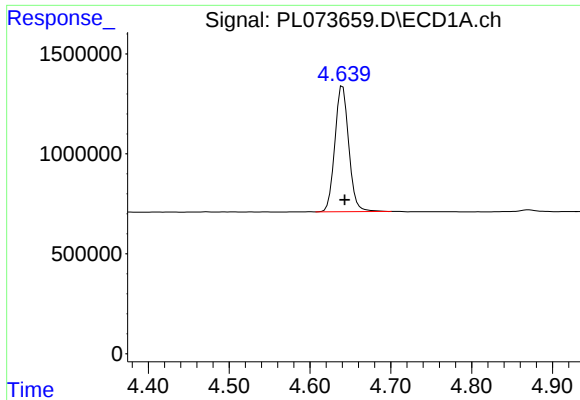

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.002 min
Response: 7514163
Conc: 23.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

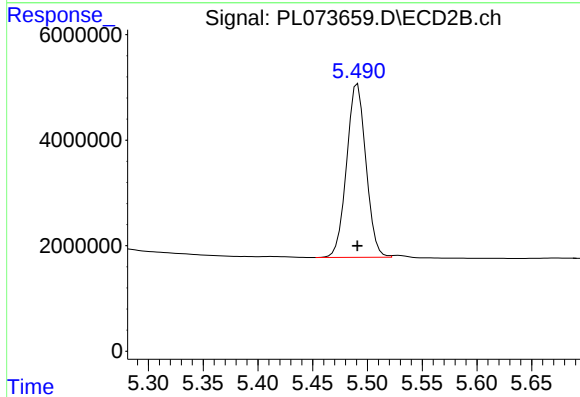


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 40370910
Conc: 24.60 ng/ml

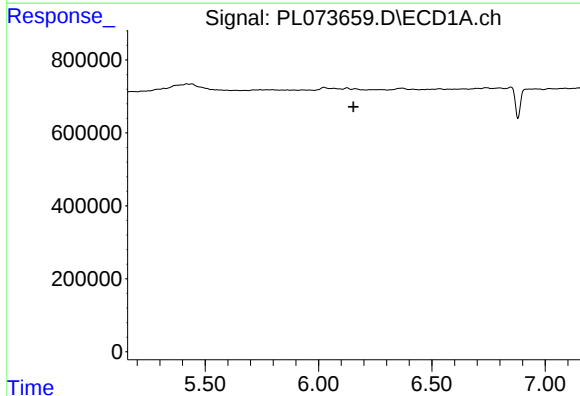


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

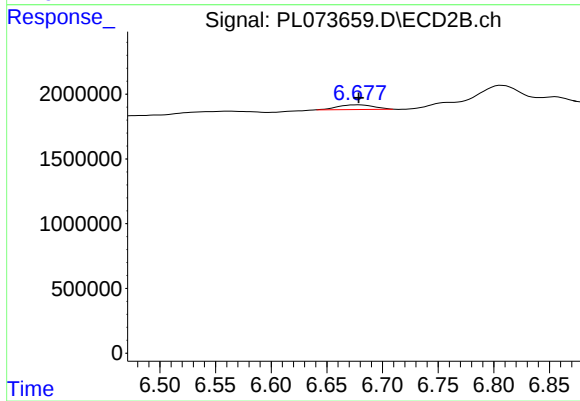

#6 beta-BHC


R.T.: 6.679 min
Delta R.T.: 0.000 min
Response: 809110
Conc: 0.78 ng/ml

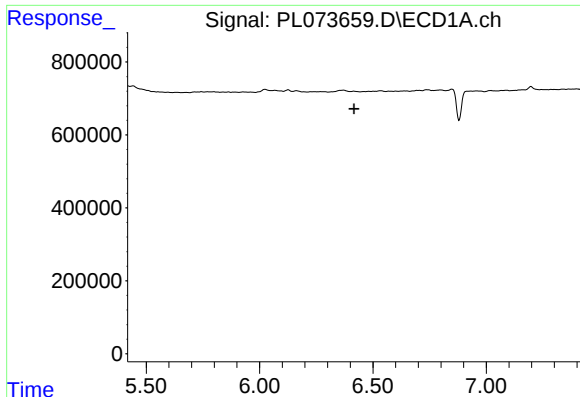

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

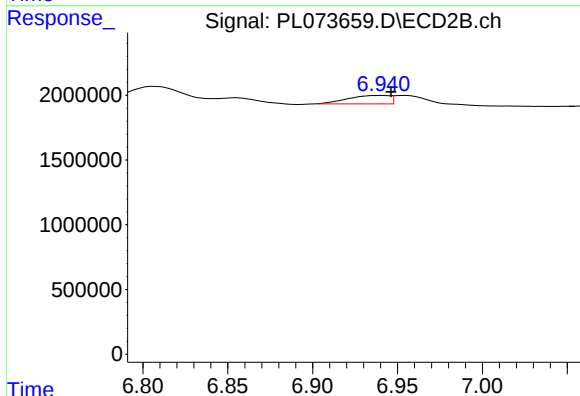


#7 delta-BHC

R.T.: 6.941 min
Delta R.T.: -0.005 min
Response: 1101074
Conc: 0.51 ng/ml

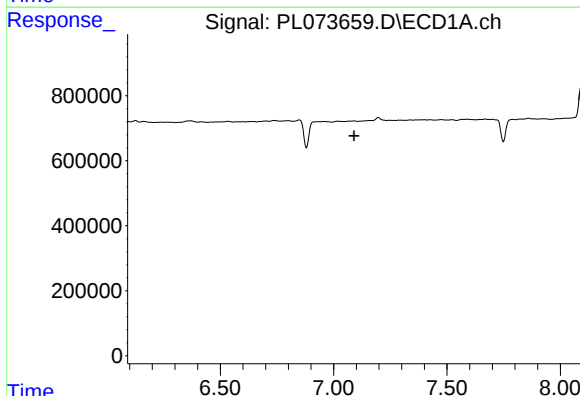


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

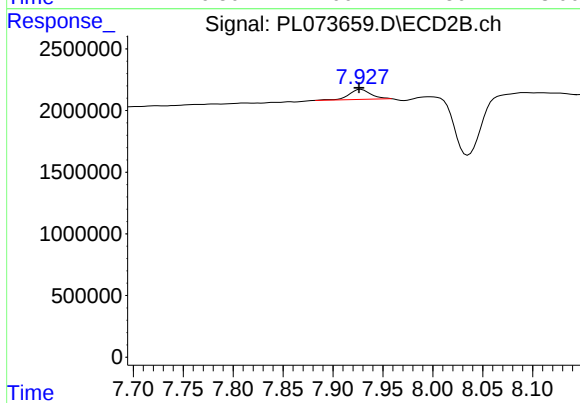

#8 Heptachlor epoxide


R.T.: 7.928 min
Delta R.T.: 0.002 min
Response: 1236754
Conc: 0.62 ng/ml

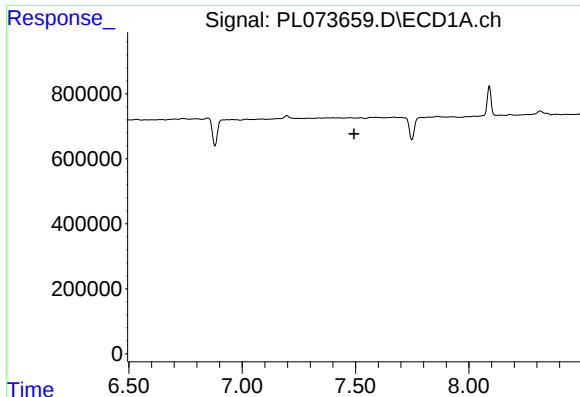

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.493 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

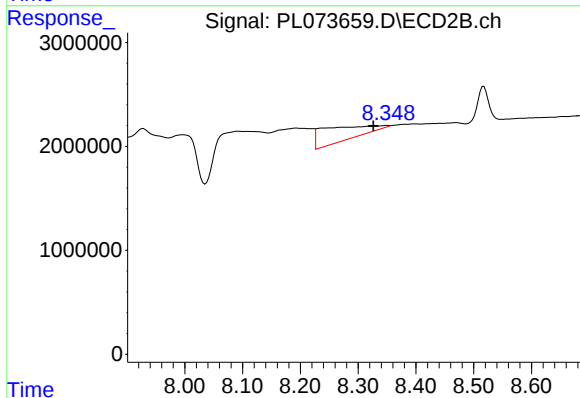


#9 Endosulfan I

R.T.: 8.350 min
Delta R.T.: 0.024 min
Response: 7904670
Conc: 4.33 ng/ml

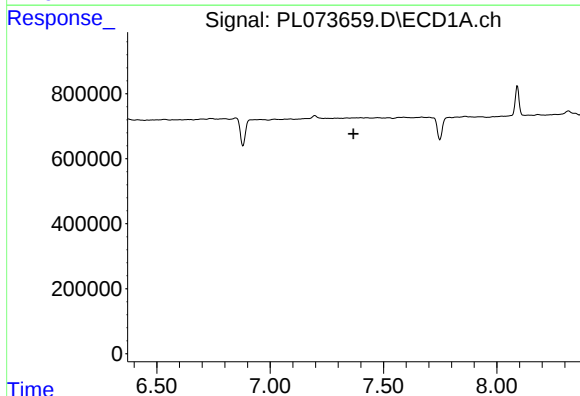


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

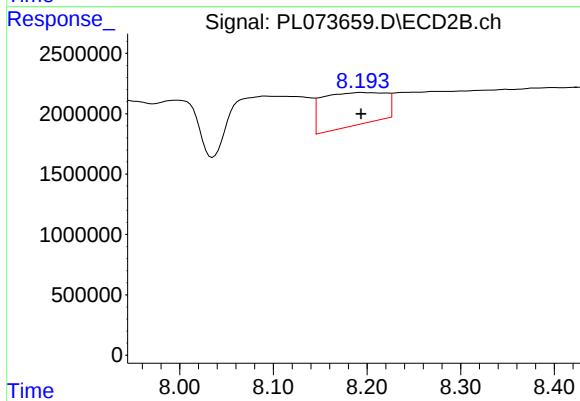

#10 gamma-Chlordane


R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 12673799
Conc: 6.21 ng/ml

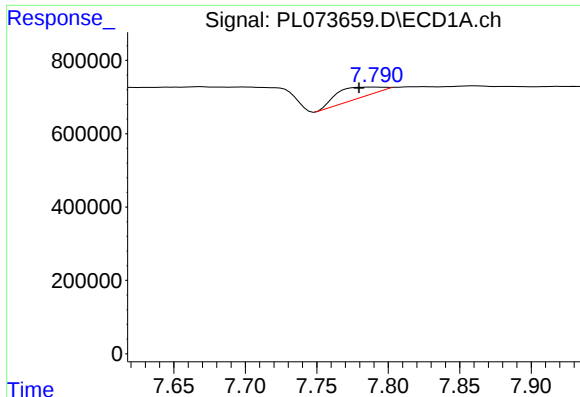

#13 Dieldrin


R.T.: 7.791 min
Delta R.T.: 0.011 min
Response: 589907
Conc: 1.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

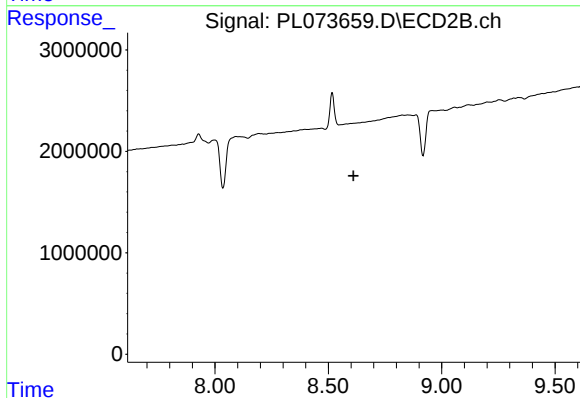


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.611 min
Response: 0
Conc: N.D.

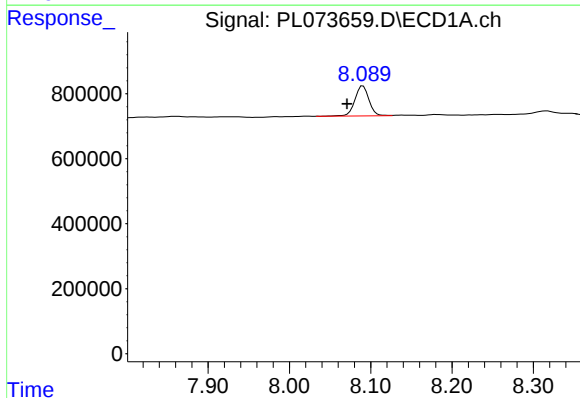


#14 Endrin

R.T.: 8.090 min
Delta R.T.: 0.020 min
Response: 1103589
Conc: 2.84 ng/ml

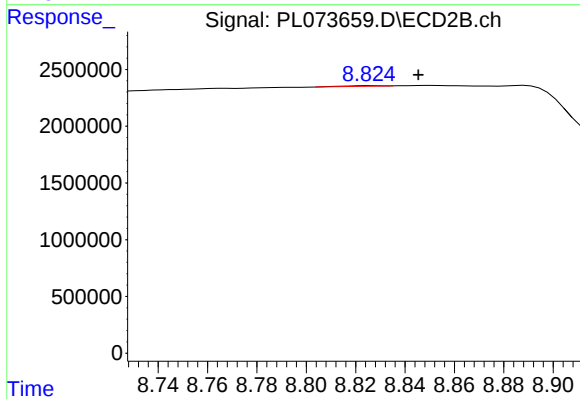

#14 Endrin


R.T.: 8.826 min
Delta R.T.: -0.019 min
Response: 60034
Conc: 0.04 ng/ml

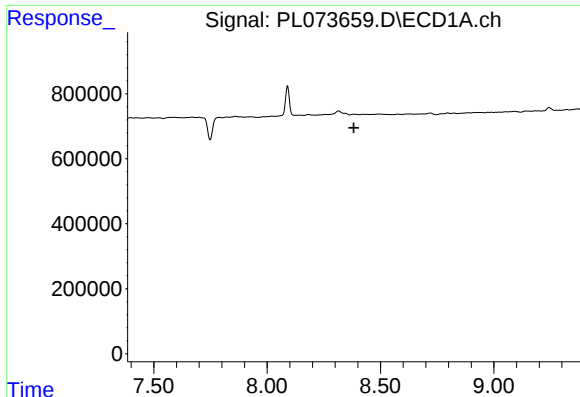

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

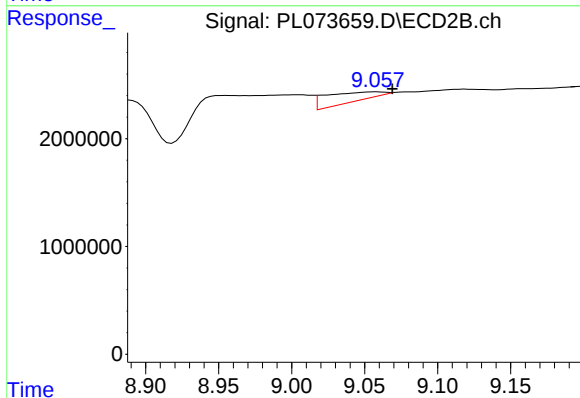


#15 Endosulfan II

R.T.: 9.058 min
Delta R.T.: -0.011 min
Response: 2283930
Conc: 1.49 ng/ml

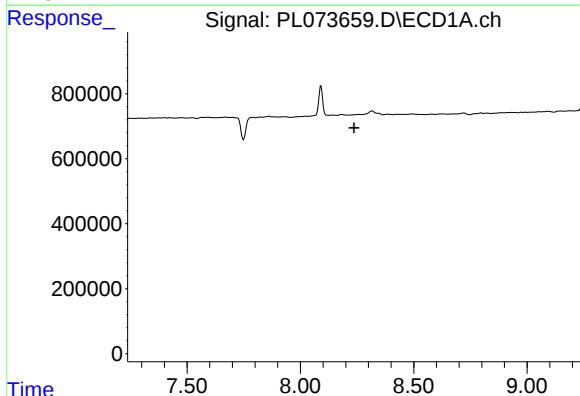


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.237 min
Response: 0
Conc: N.D.

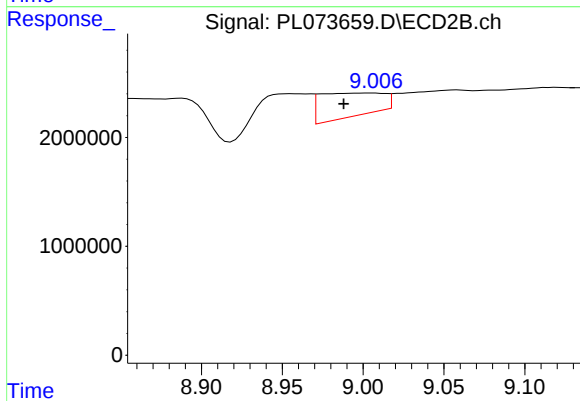

#16 4,4'-DDD


R.T.: 9.006 min
Delta R.T.: 0.018 min
Response: 5879245
Conc: 4.03 ng/ml

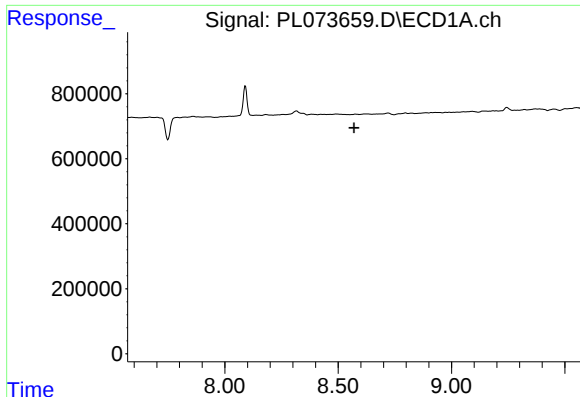

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.570 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

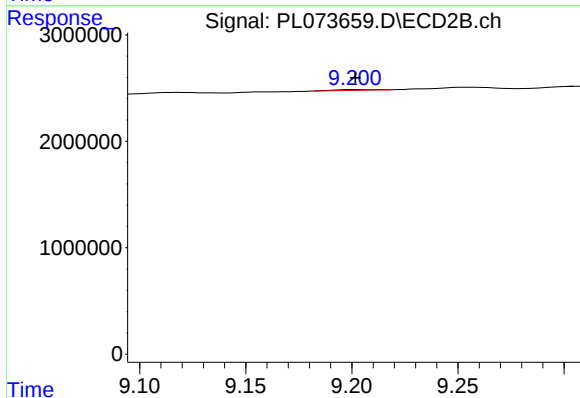


#18 Endrin aldehyde

R.T.: 9.202 min
Delta R.T.: 0.000 min
Response: 93705
Conc: 0.08 ng/ml

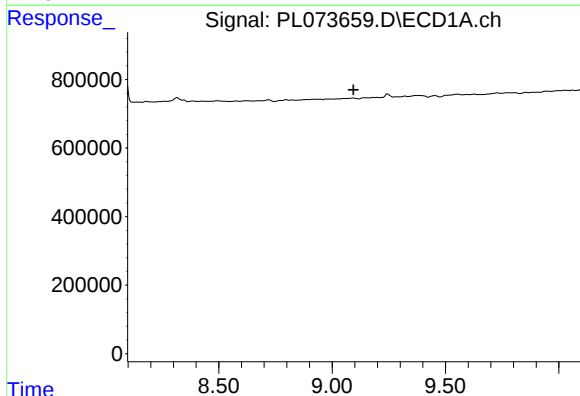


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.095 min
Response: 0
Conc: N.D.

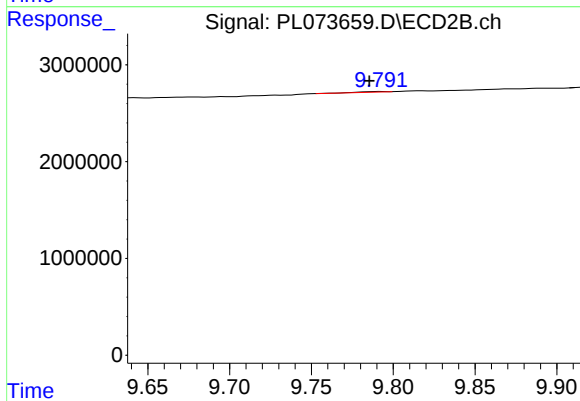

#20 Methoxychlor


R.T.: 9.792 min
Delta R.T.: 0.007 min
Response: 59807
Conc: 0.07 ng/ml

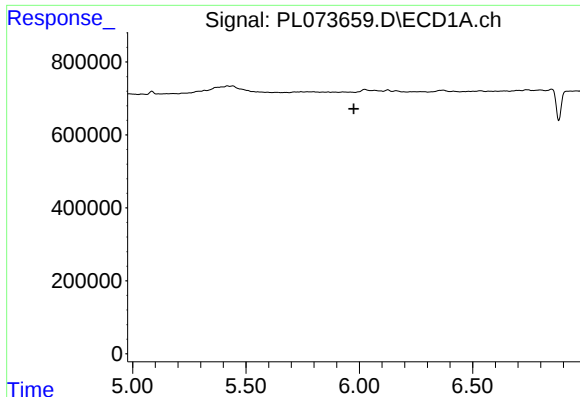

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

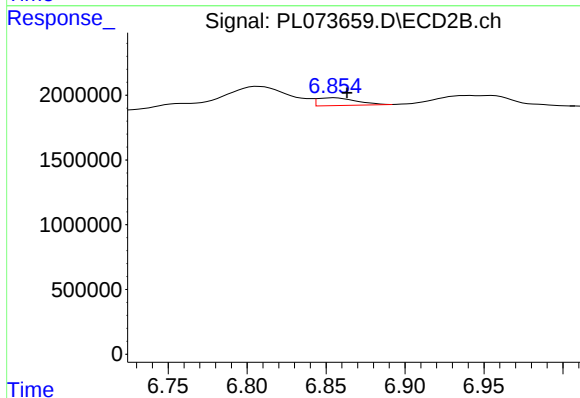


#23 Chlordane-1

R.T.: 6.855 min
Delta R.T.: -0.008 min
Response: 1022590
Conc: 14.97 ng/ml

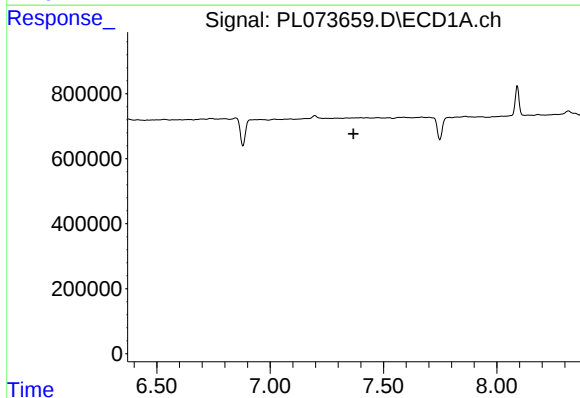


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

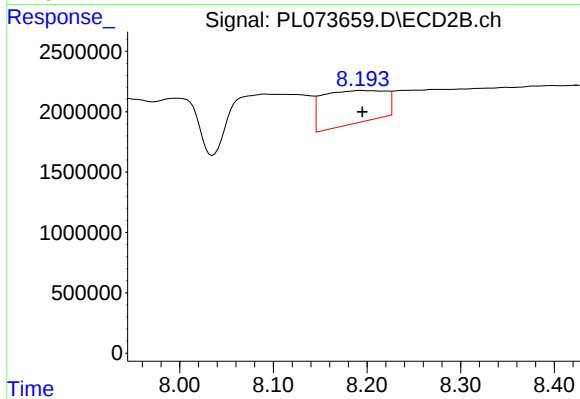

#25 Chlordane-3


R.T.: 8.194 min
Delta R.T.: -0.001 min
Response: 12673799
Conc: 46.74 ng/ml

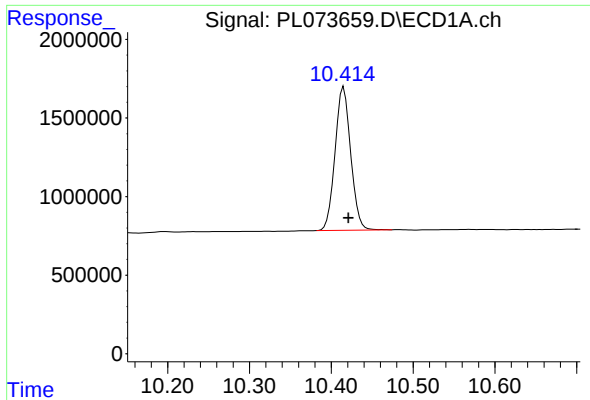

#28 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.006 min
Response: 12124870
Conc: 23.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

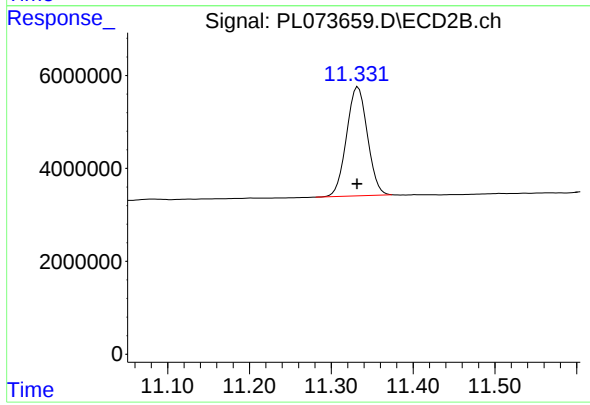

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: 0.001 min
Response: 41552705
Conc: 23.24 ng/ml