

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032422\
 Data File : PL073671.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 18:32
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 01:47:47 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
28)	SA Decachlor...	10.428	11.347f	117388	393615	0.231	0.220
Target Compounds							
6)	B beta-BHC	0.000	6.684	0	487127	N.D.	0.467 #
7)	B delta-BHC	0.000	6.958	0	1193953	N.D.	0.554 #
9)	A Endosulfan I	0.000	8.325	0	1011567	N.D.	0.554 #
10)	B gamma-Chl...	7.341f	8.182	36107	2782941	0.083	1.363 #
11)	B alpha-Chl...	0.000	8.262	0	602806	N.D.	0.301 #
14)	MA Endrin	8.091f	8.824f	13005097	78205	33.518	0.051 #
16)	A 4,4'-DDD	0.000	8.978	0	511630	N.D.	0.351 #
18)	B Endrin al...	0.000	9.206	0	115011	N.D.	0.094 #
19)	B Endosulfa...	0.000	9.467f	0	10620	N.D.	0.007 #
20)	A Methoxychlor	9.120f	0.000	77466	0	0.302	N.D. #
23)	Chlordane-1	0.000	6.854	0	696954	N.D.	10.202 #
24)	Chlordane-2	6.693f	0.000	1007406	0	61.755	N.D. #
25)	Chlordane-3	7.341f	8.182	36107	2782941	0.884	10.264 #
26)	Chlordane-4	0.000	8.262f	0	602806	N.D.	1.820 #
27)	Chlordane-5	0.000	9.125f	0	244249	N.D.	4.500 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032422\
Data File : PL073671.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 18:32
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 01:47:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

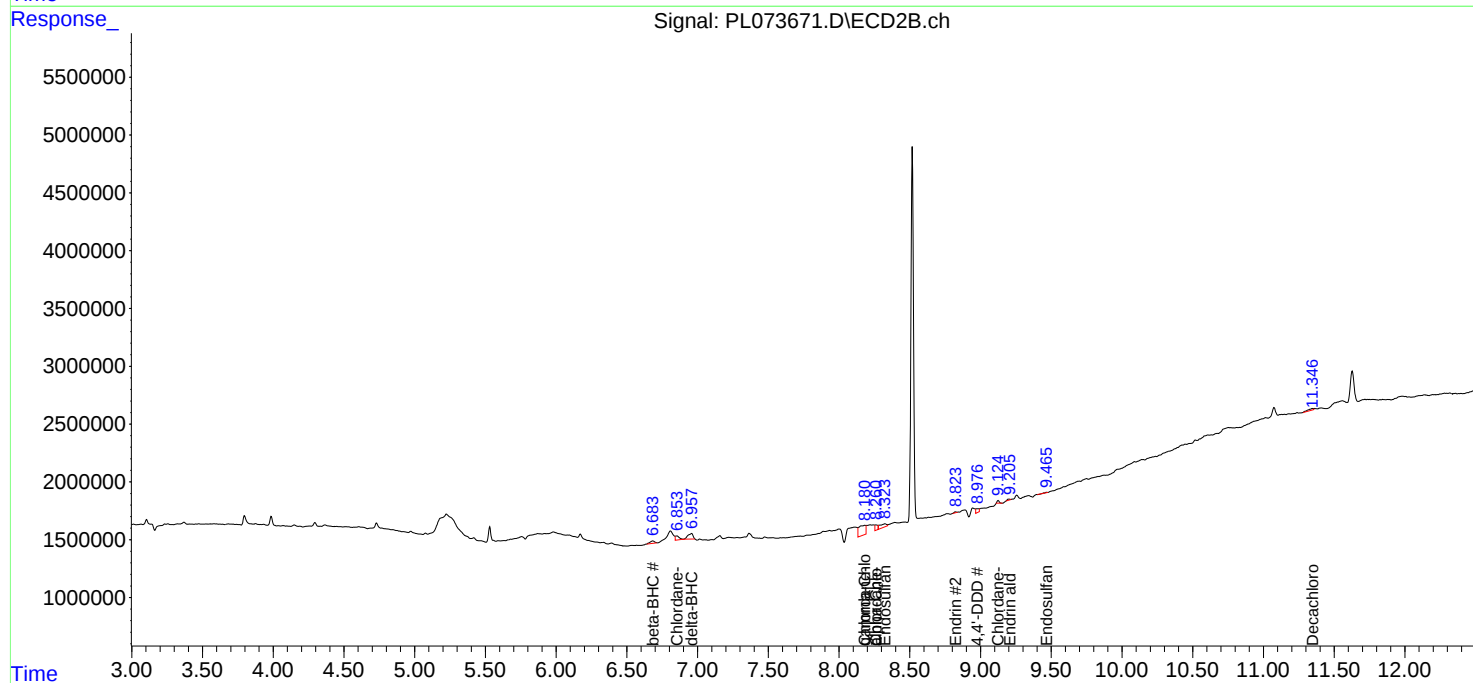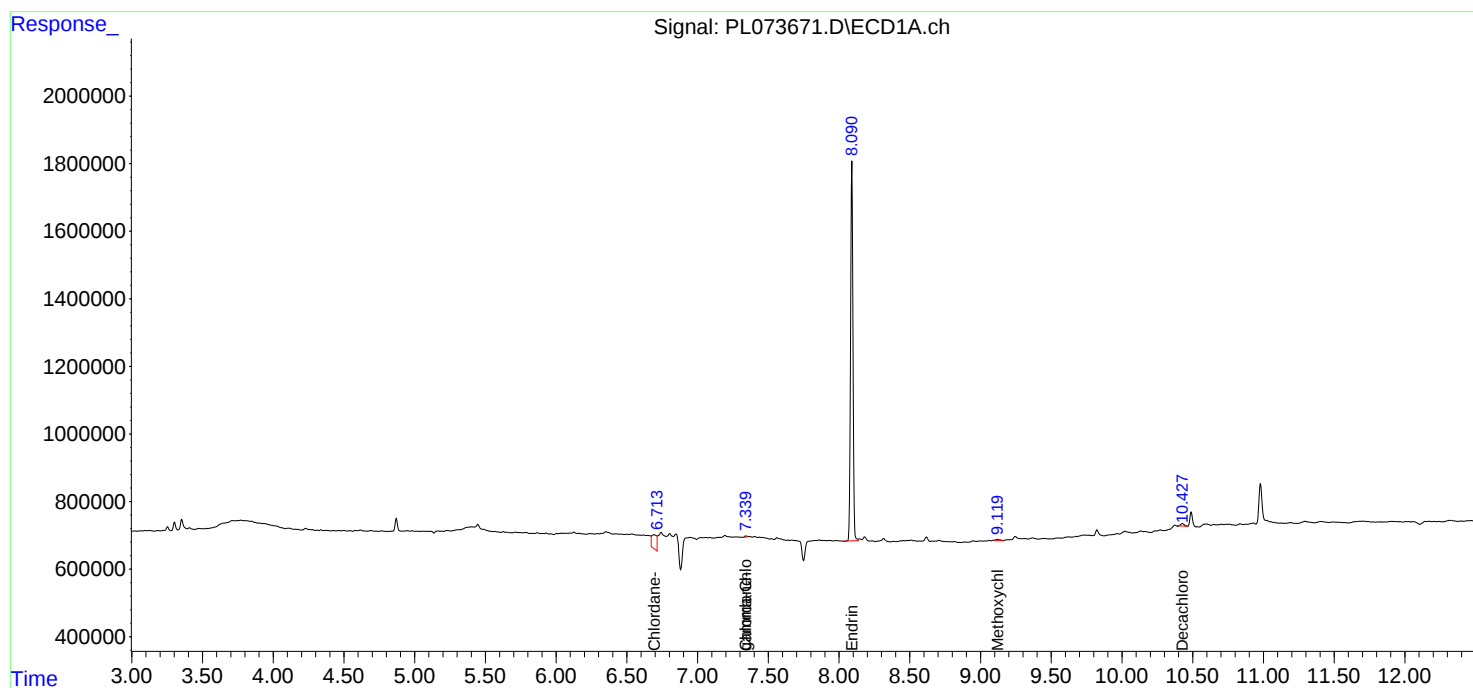


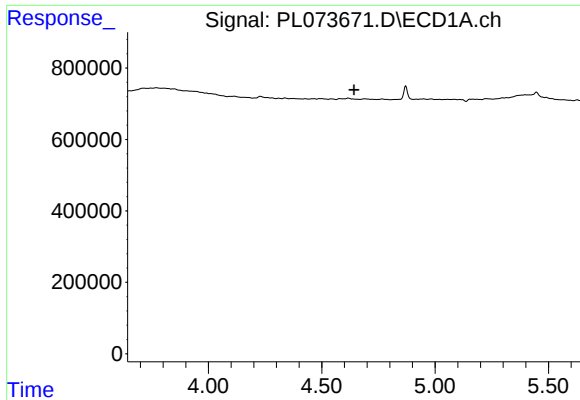

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

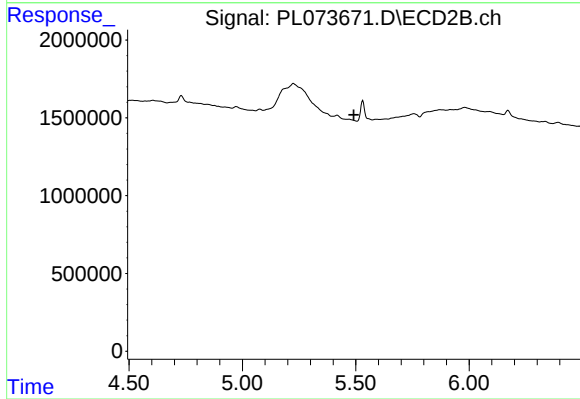


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.491 min
Response: 0
Conc: N.D.

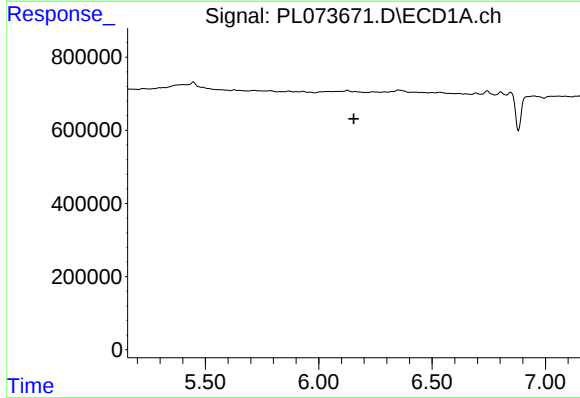


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

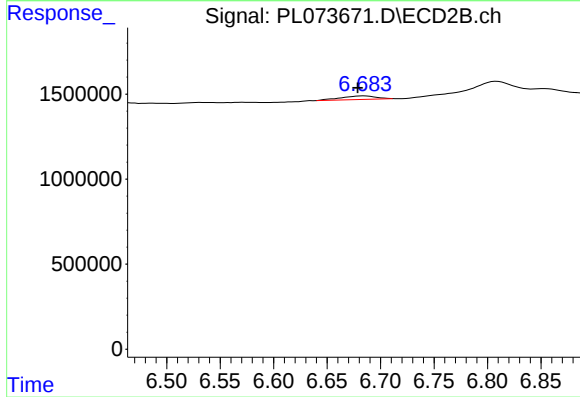

#6 beta-BHC


R.T.: 6.684 min
Delta R.T.: 0.006 min
Response: 487127
Conc: 0.47 ng/ml

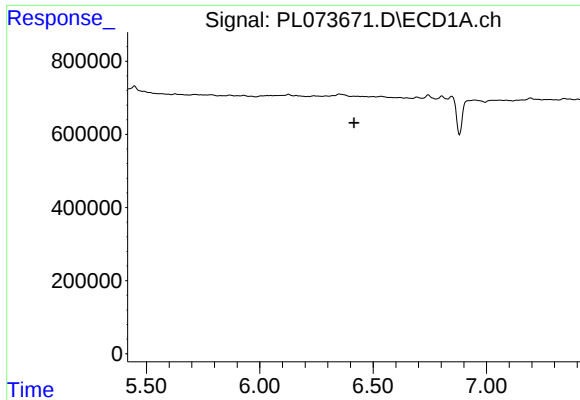

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

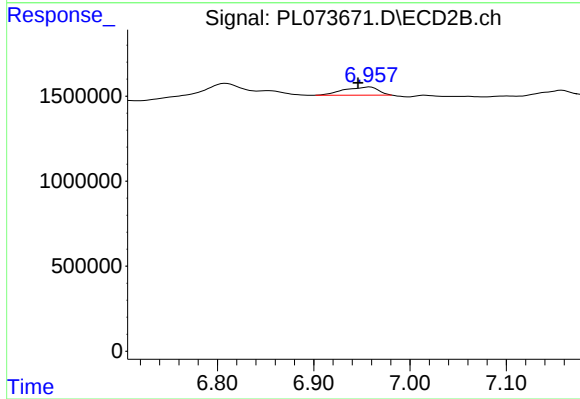


#7 delta-BHC

R.T.: 6.958 min
Delta R.T.: 0.012 min
Response: 1193953
Conc: 0.55 ng/ml

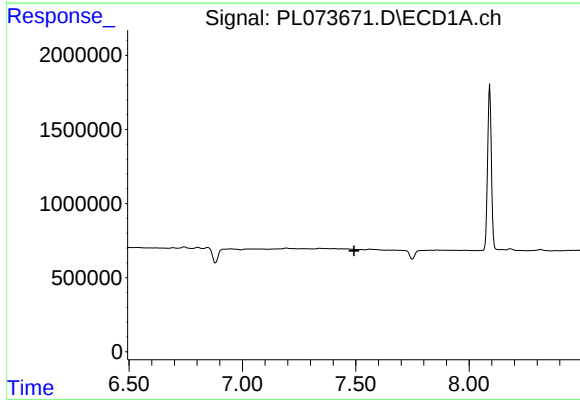


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.493 min
Response: 0
Conc: N.D.

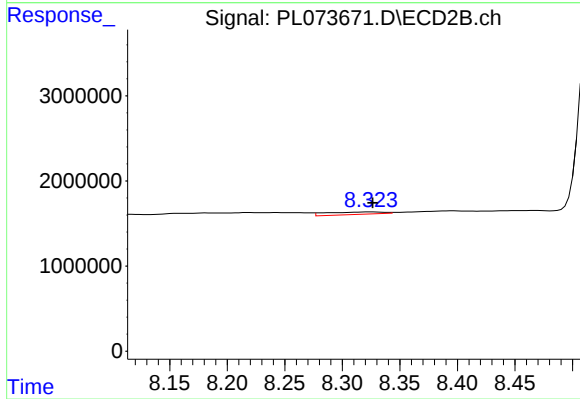

#9 Endosulfan I


R.T.: 8.325 min
Delta R.T.: -0.002 min
Response: 1011567
Conc: 0.55 ng/ml

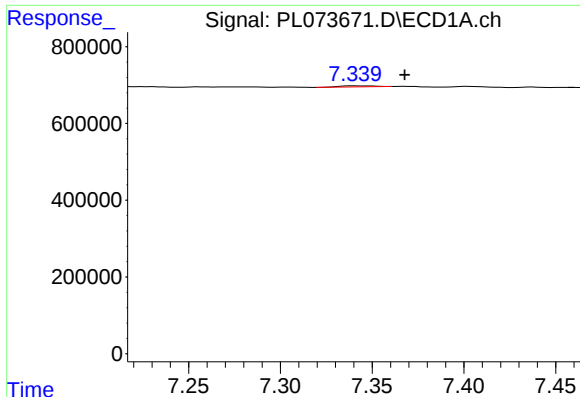

#10 gamma-Chlordane


R.T.: 7.341 min
Delta R.T.: -0.027 min
Response: 36107
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

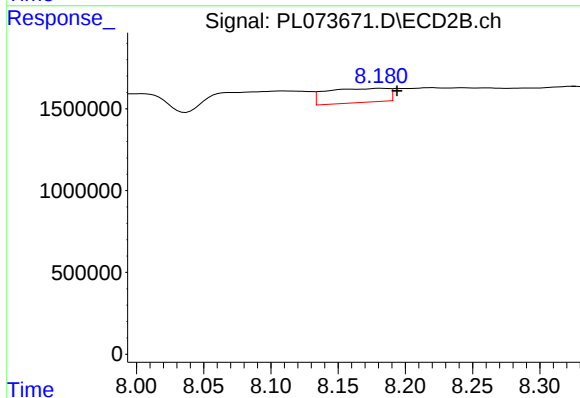


#10 gamma-Chlordane

R.T.: 8.182 min
Delta R.T.: -0.012 min
Response: 2782941
Conc: 1.36 ng/ml

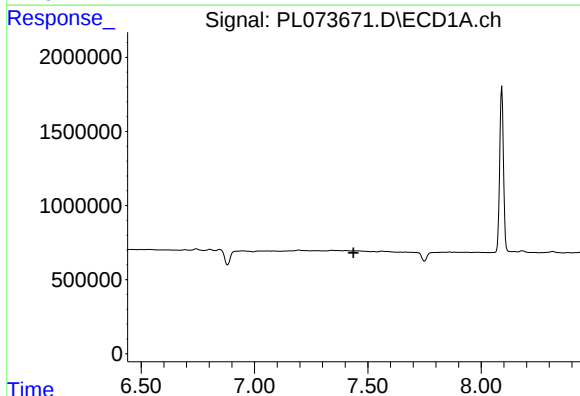


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.437 min
Response: 0
Conc: N.D.

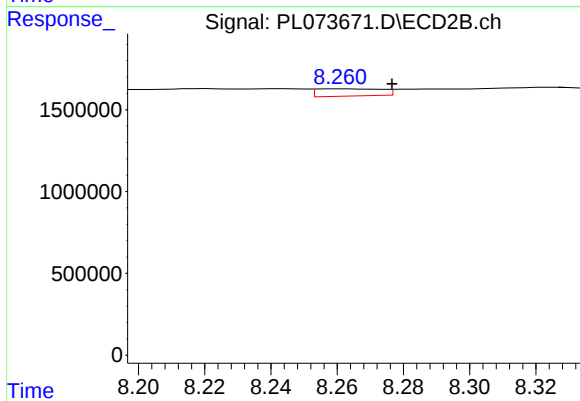

#11 alpha-Chlordane


R.T.: 8.262 min
Delta R.T.: -0.014 min
Response: 602806
Conc: 0.30 ng/ml

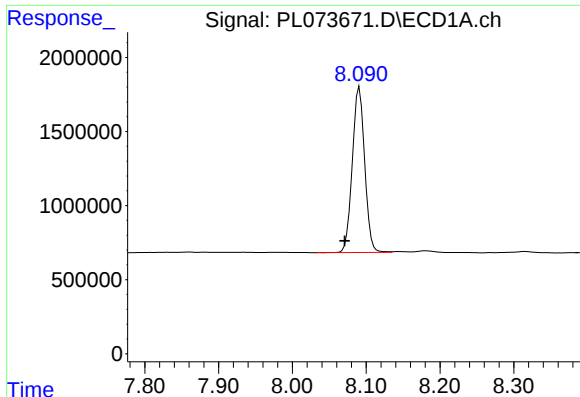

#14 Endrin


R.T.: 8.091 min
Delta R.T.: 0.020 min
Response: 13005097
Conc: 33.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

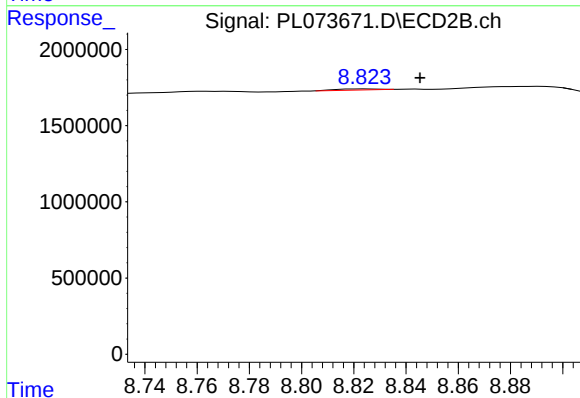


#14 Endrin

R.T.: 8.824 min
Delta R.T.: -0.021 min
Response: 78205
Conc: 0.05 ng/ml

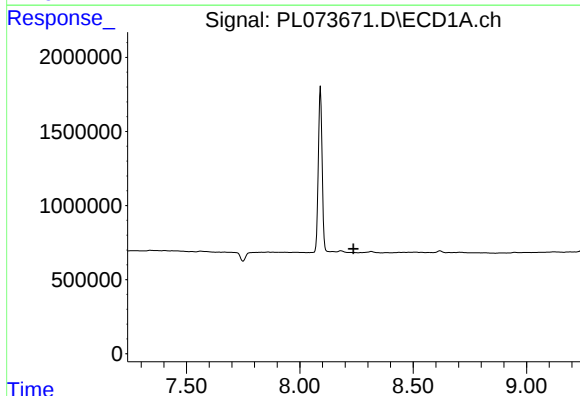


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.237 min
Response: 0
Conc: N.D.

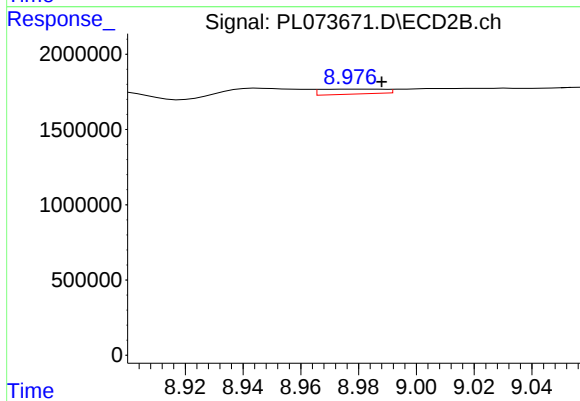

#16 4,4'-DDD


R.T.: 8.978 min
Delta R.T.: -0.010 min
Response: 511630
Conc: 0.35 ng/ml

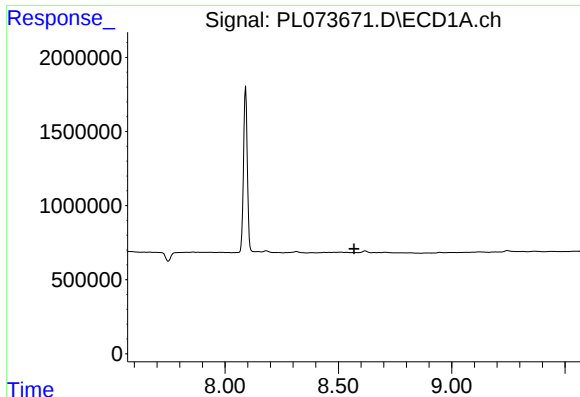

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 8.570 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

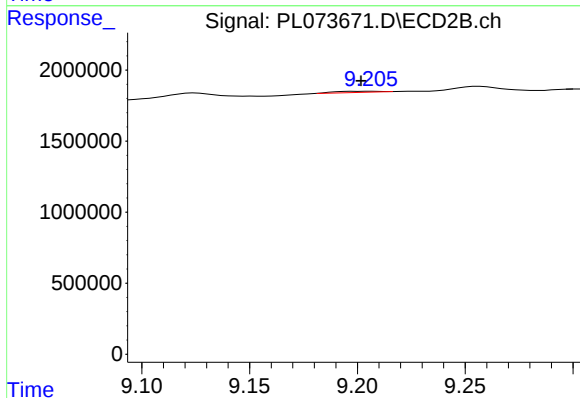


#18 Endrin aldehyde

R.T.: 9.206 min
Delta R.T.: 0.004 min
Response: 115011
Conc: 0.09 ng/ml

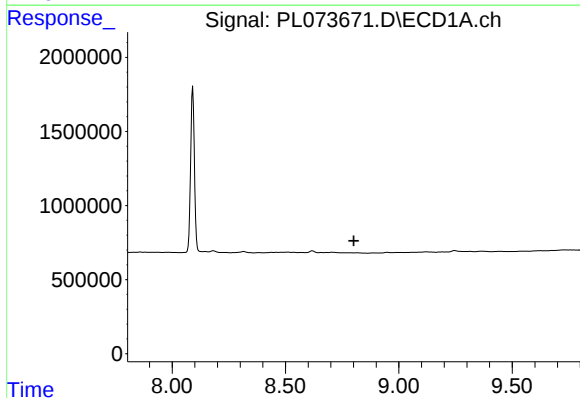


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.801 min
Response: 0
Conc: N.D.

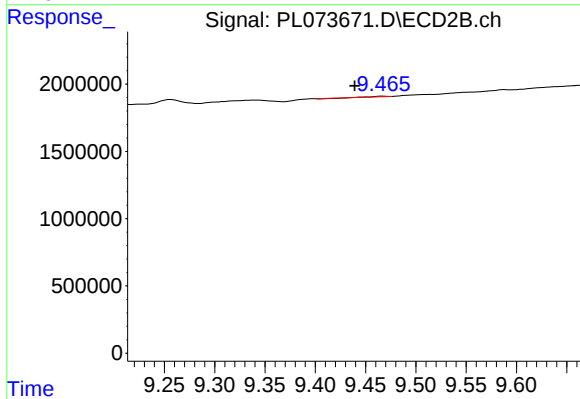

#19 Endosulfan Sulfate


R.T.: 9.467 min
Delta R.T.: 0.028 min
Response: 10620
Conc: 0.01 ng/ml

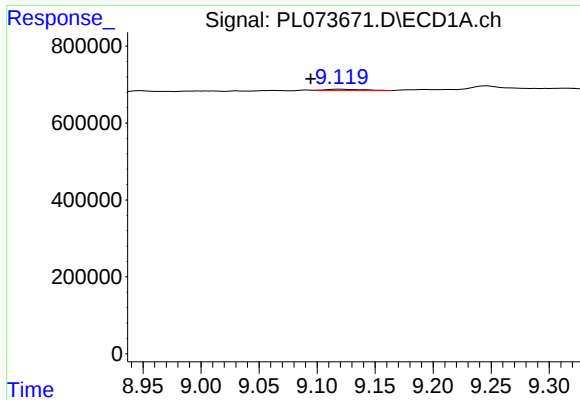

#20 Methoxychlor


R.T.: 9.120 min
Delta R.T.: 0.026 min
Response: 77466
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

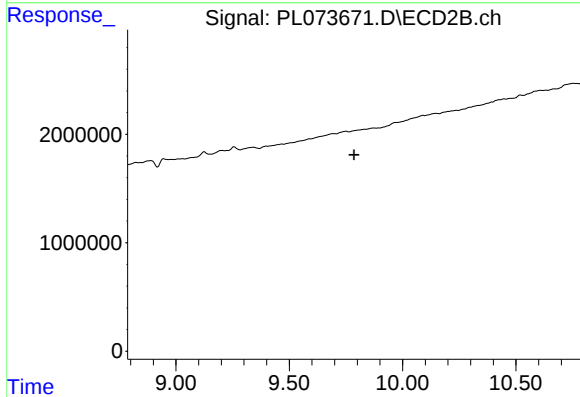


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.786 min
Response: 0
Conc: N.D.

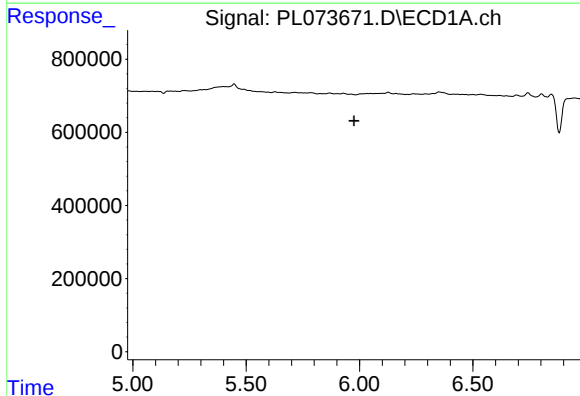


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

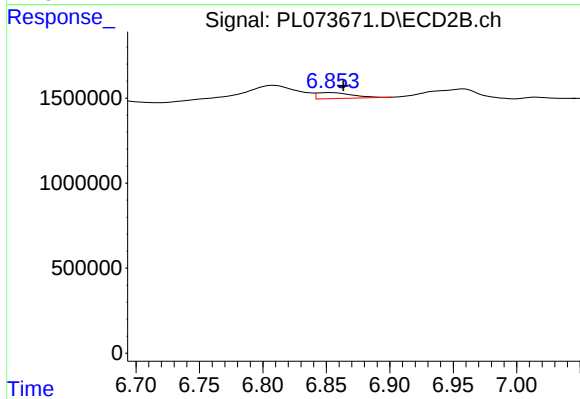

#23 Chlordane-1


R.T.: 6.854 min
Delta R.T.: -0.009 min
Response: 696954
Conc: 10.20 ng/ml

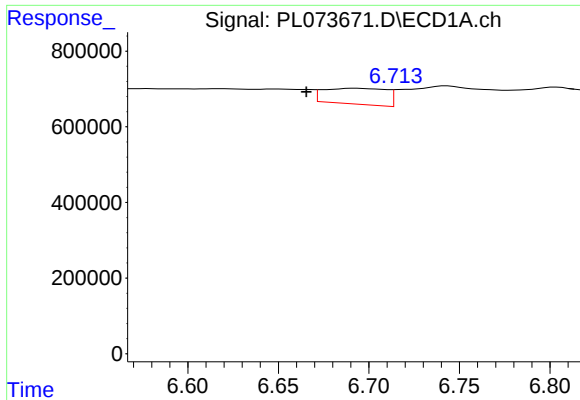

#24 Chlordane-2


R.T.: 6.693 min
Delta R.T.: 0.028 min
Response: 1007406
Conc: 61.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

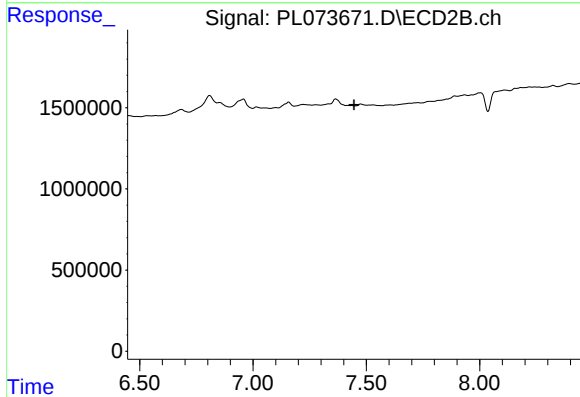


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

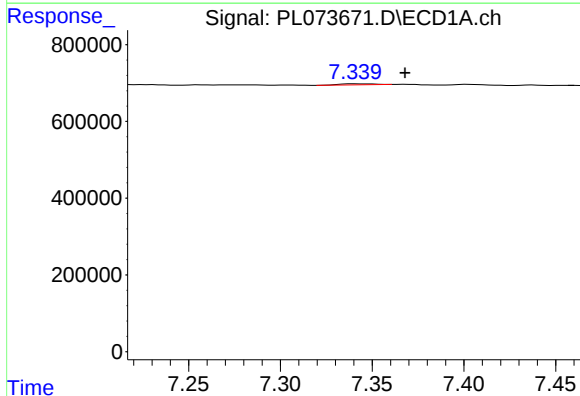


#25 Chlordane-3

R.T.: 7.341 min
Delta R.T.: -0.027 min
Response: 36107
Conc: 0.88 ng/ml

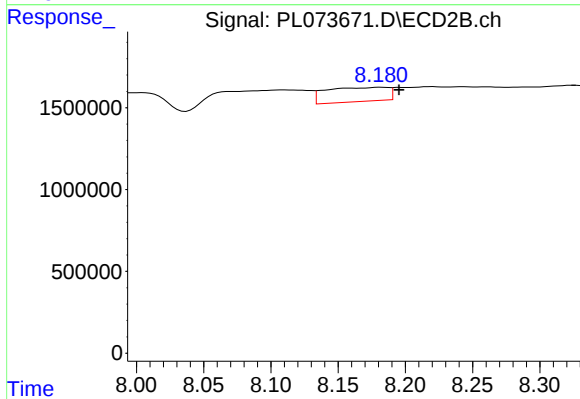

#25 Chlordane-3


R.T.: 8.182 min
Delta R.T.: -0.014 min
Response: 2782941
Conc: 10.26 ng/ml

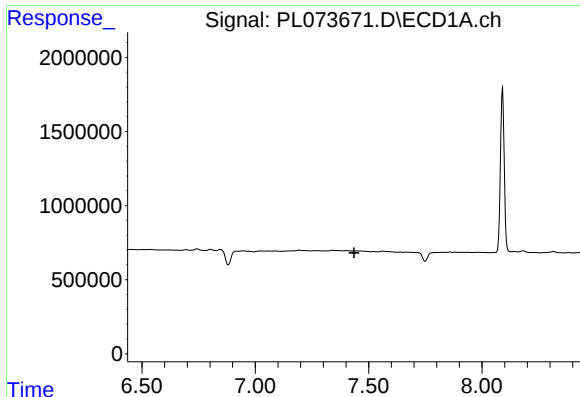

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

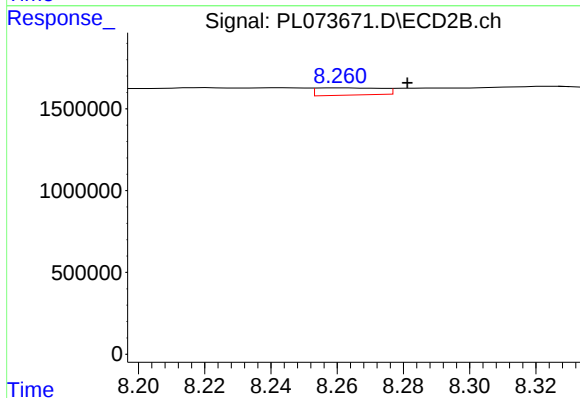


#26 Chlordane-4

R.T.: 8.262 min
Delta R.T.: -0.019 min
Response: 602806
Conc: 1.82 ng/ml

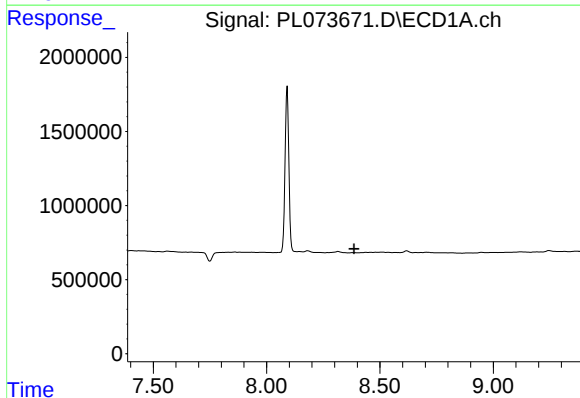


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.387 min
Response: 0
Conc: N.D.

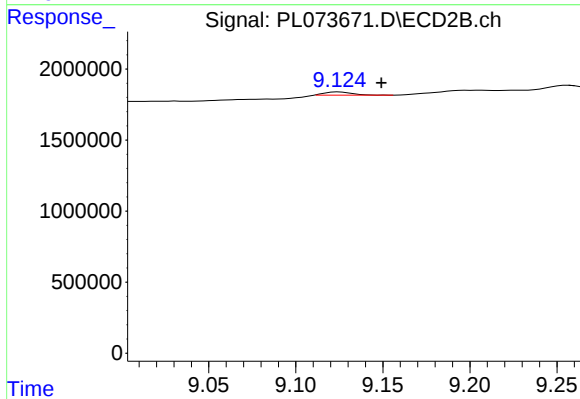

#27 Chlordane-5


R.T.: 9.125 min
Delta R.T.: -0.024 min
Response: 244249
Conc: 4.50 ng/ml

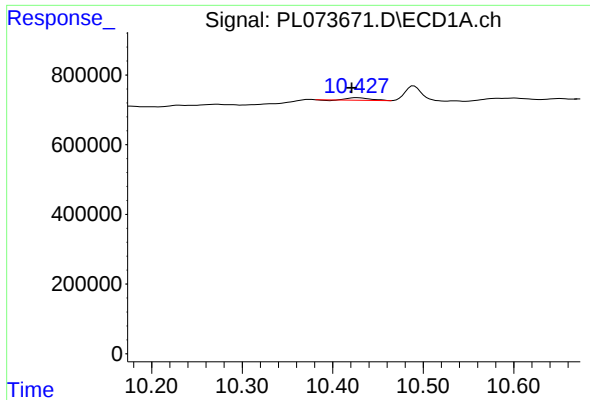

#28 Decachlorobiphenyl

R.T.: 10.428 min
Delta R.T.: 0.007 min
Response: 117388
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

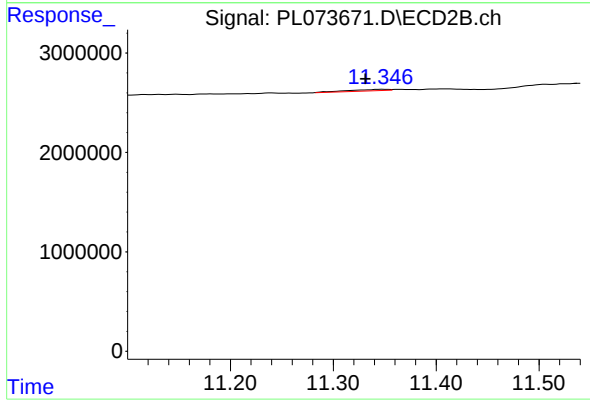

#28 Decachlorobiphenyl

R.T.: 11.347 min
Delta R.T.: 0.016 min
Response: 393615
Conc: 0.22 ng/ml