

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032425\
 Data File : PL094823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2025 17:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 01:52:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.770	50046833	66240929	17.680	18.559
28)	SA Decachlor...	9.055	7.904	45841033	74105054	21.752	18.346
Target Compounds							
14)	MA Endrin	0.000	5.650f	0	11688028	N.D.	2.678 #
18)	B Endrin al...	0.000	6.105	0	28466235	N.D.	8.459 #
24)	Chlordane-2	0.000	4.349	0	10662931	N.D.	60.383 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032425\
Data File : PL094823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2025 17:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 01:52:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

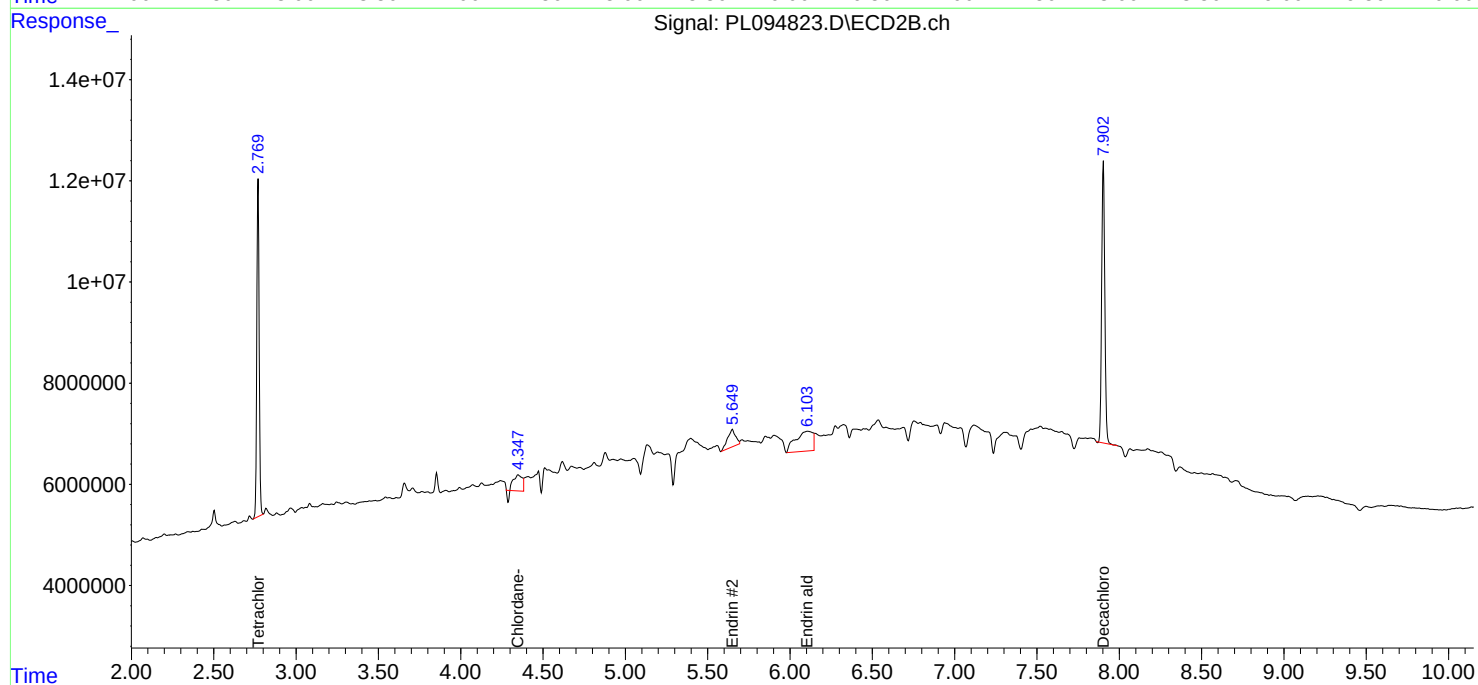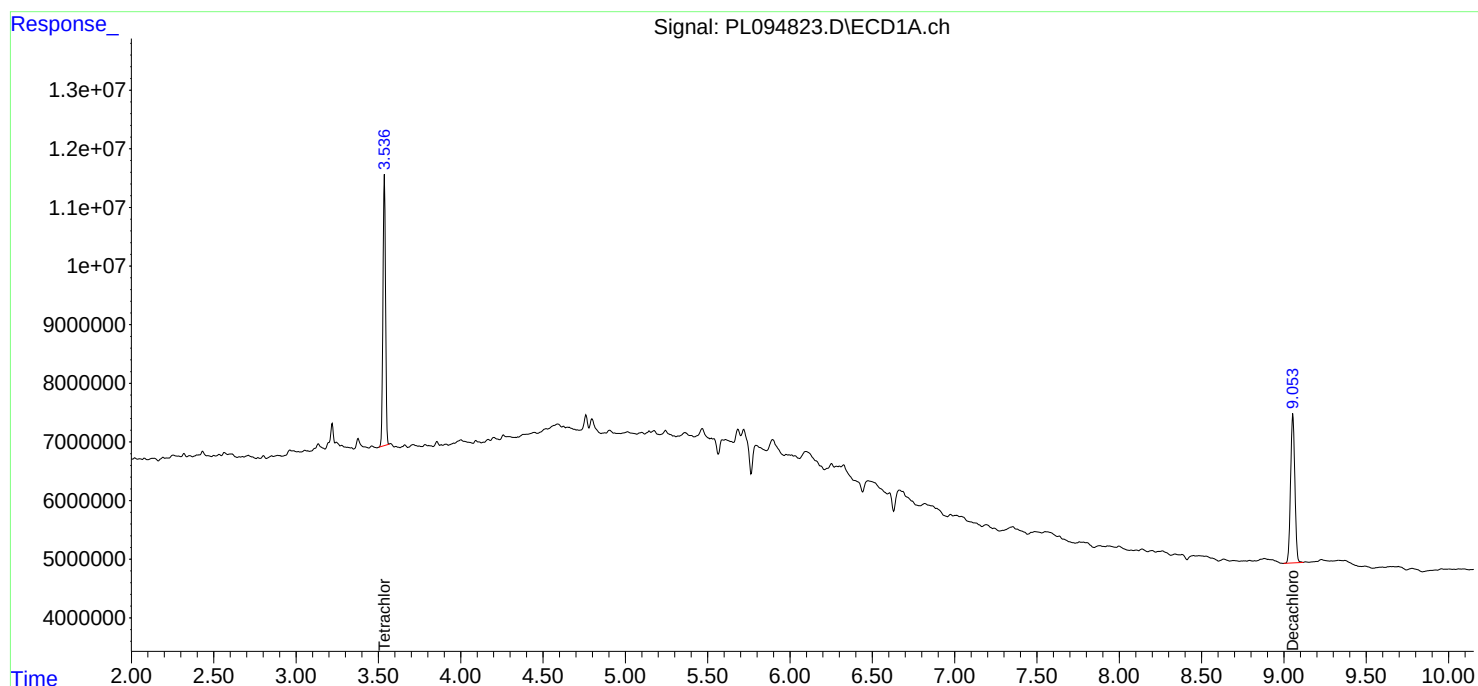


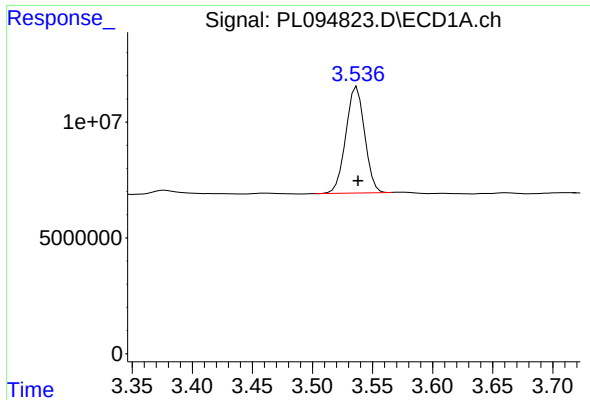

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 50046833
Conc: 17.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

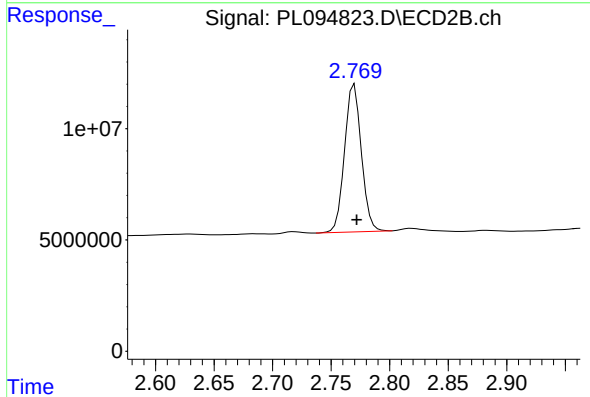


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.002 min
Response: 66240929
Conc: 18.56 ng/ml

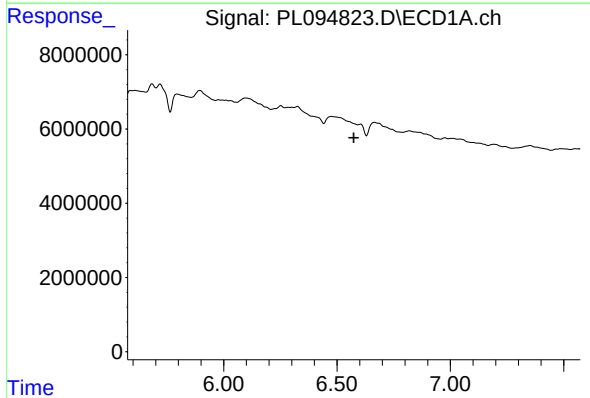


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.574 min
Response: 0
Conc: N.D.

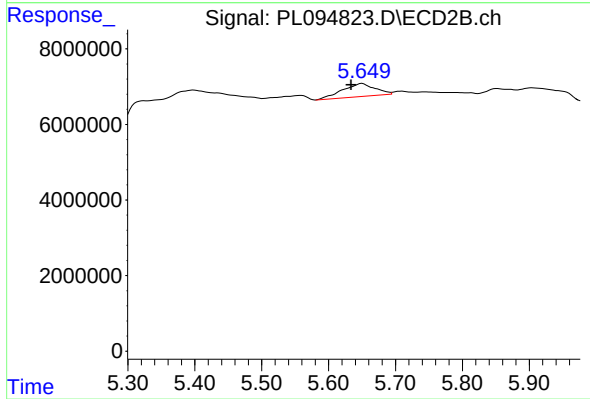

#14 Endrin


R.T.: 5.650 min
Delta R.T.: 0.017 min
Response: 11688028
Conc: 2.68 ng/ml

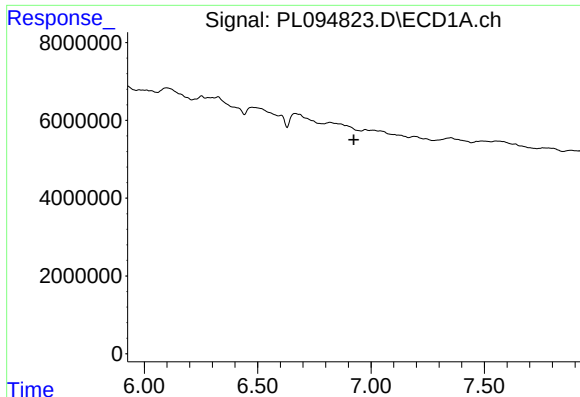

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.924 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

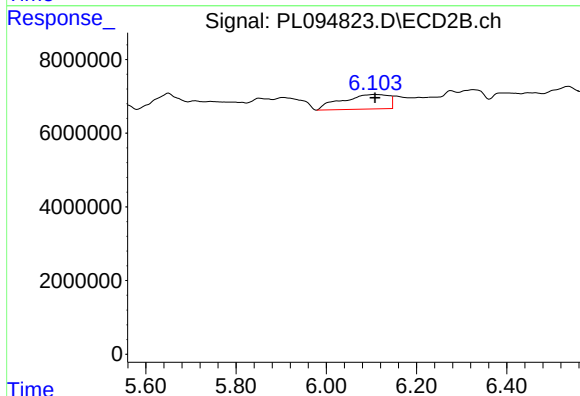


#18 Endrin aldehyde

R.T.: 6.105 min
Delta R.T.: -0.003 min
Response: 28466235
Conc: 8.46 ng/ml

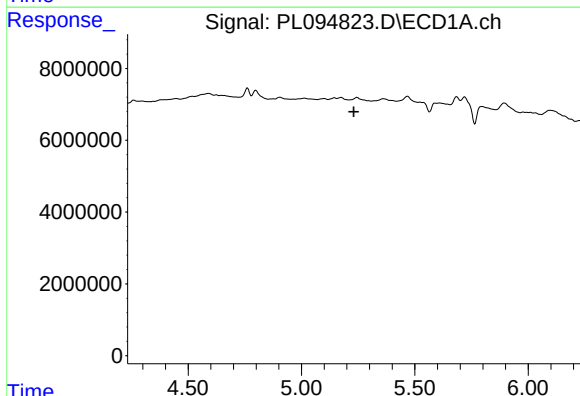


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.230 min
Response: 0
Conc: N.D.

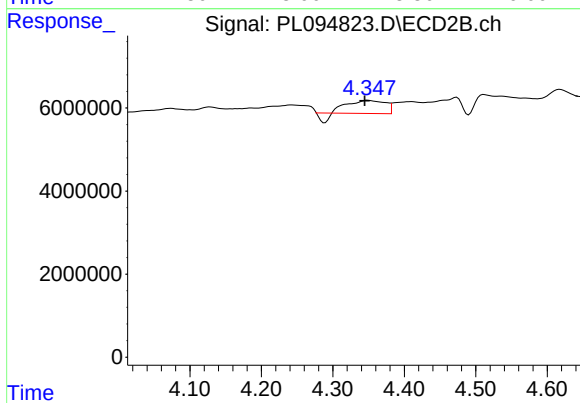

#24 Chlordane-2


R.T.: 4.349 min
Delta R.T.: 0.004 min
Response: 10662931
Conc: 60.38 ng/ml

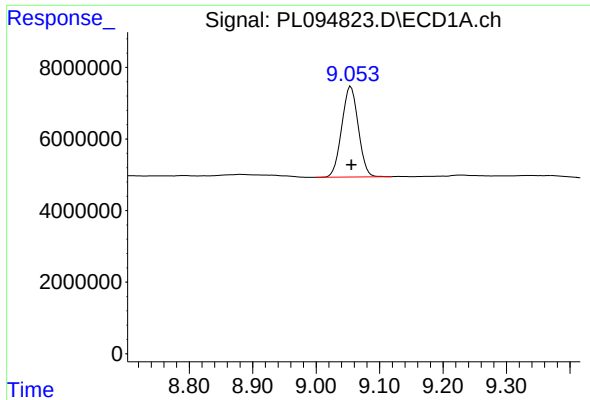

#28 Decachlorobiphenyl

R.T.: 9.055 min
Delta R.T.: 0.000 min
Response: 45841033
Conc: 21.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

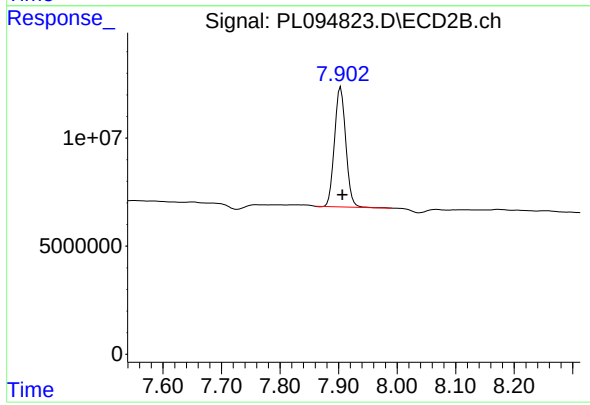

#28 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: -0.003 min
Response: 74105054
Conc: 18.35 ng/ml