

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032519\
 Data File : PL046432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2019 11:39
 Operator : AJ\SJ
 Sample : K2015-07RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-025-SW034-031919

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 01:10:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.978	89777690	29155978	12.341	12.734
28)	SA Decachlor...	8.037	9.031	90695378	26397091	10.783	11.386
Target Compounds							
10)	B gamma-Chl...	5.273f	0.000	12851405	0	1.251	N.D. #
11)	B alpha-Chl...	0.000	6.158	0	4532399	N.D.	1.598 #
12)	B 4,4'-DDE	5.476	6.312	58564567	18114047	6.361	7.297
13)	MA Dieldrin	5.599	0.000	10079509	0	1.004	N.D. #
16)	A 4,4'-DDD	0.000	6.808	0	3205331	N.D.	1.593 #
17)	MA 4,4'-DDT	6.220	7.100	34215293	966408	4.517	0.461 #
25)	Chlordane-3	5.273f	0.000	12851405	0	11.540	N.D. #
26)	Chlordane-4	0.000	6.158	0	4532399	N.D.	9.823 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032519\
Data File : PL046432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2019 11:39
Operator : AJ\SJ
Sample : K2015-07RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EXT-025-SW034-031919

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 01:10:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

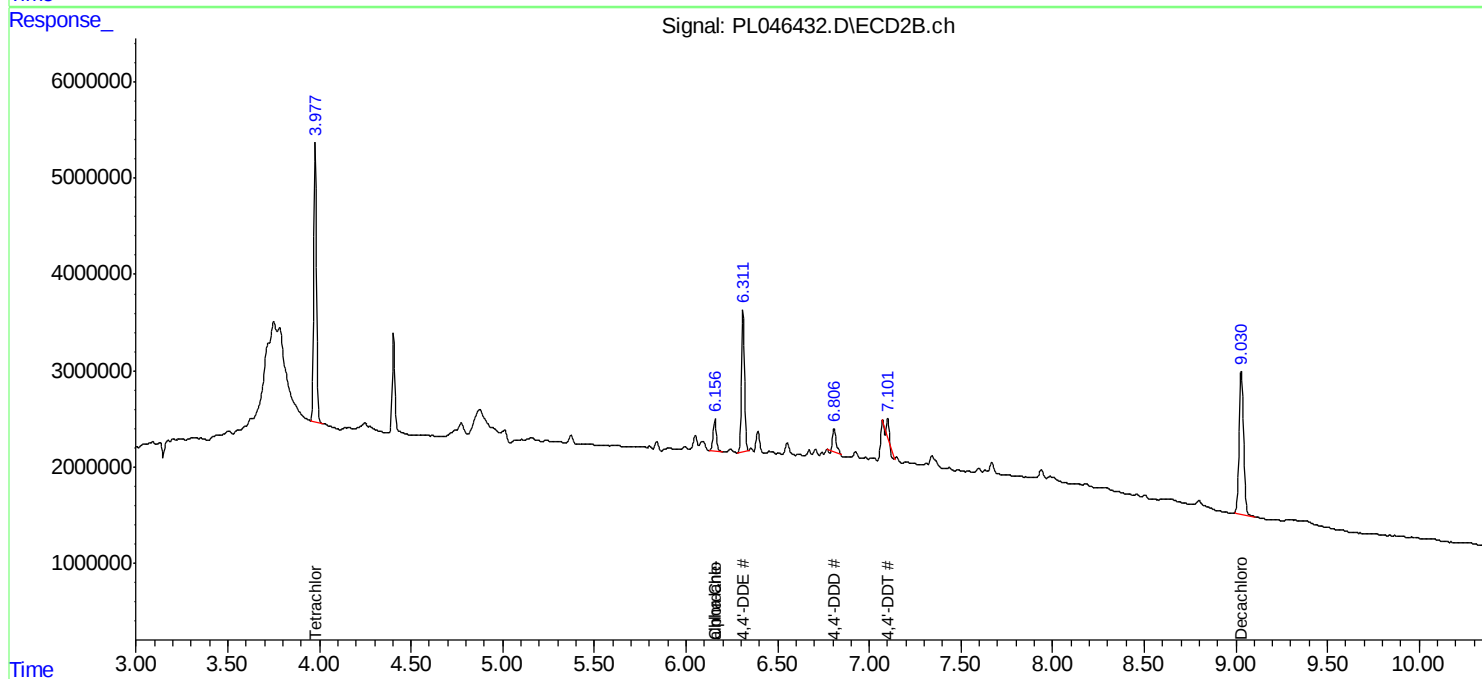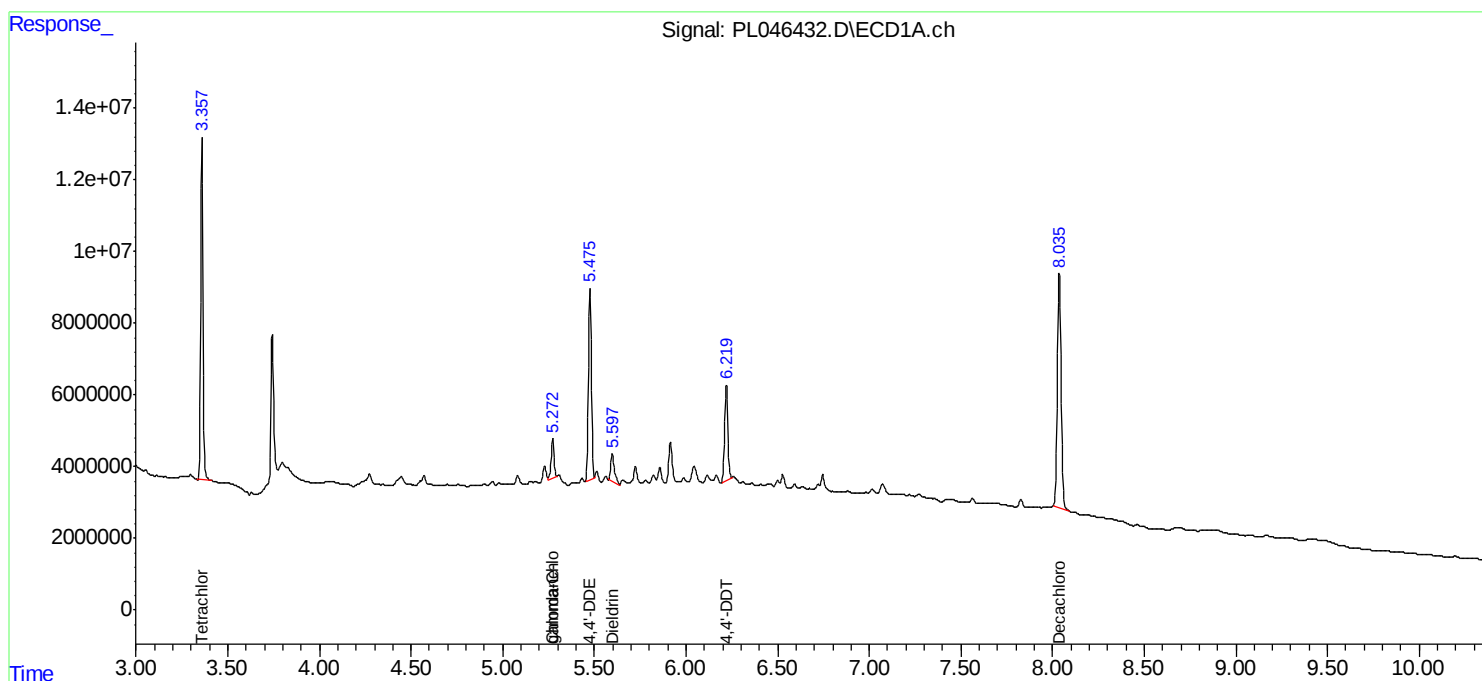


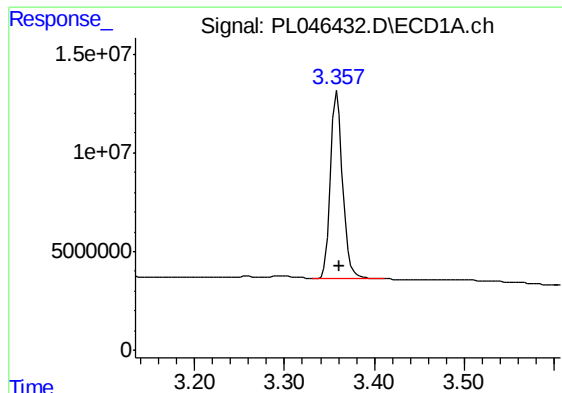

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 89777690
Conc: 12.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-025-SW034-031919

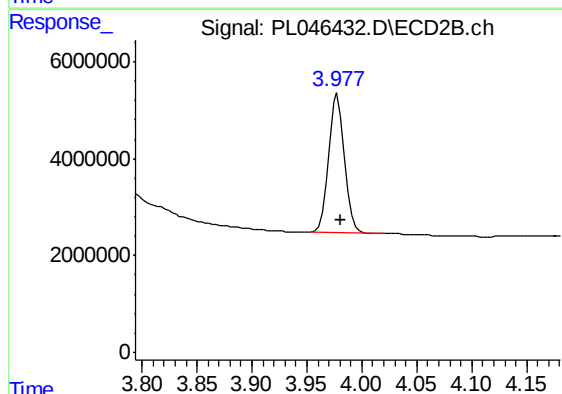


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 29155978
Conc: 12.73 ng/ml

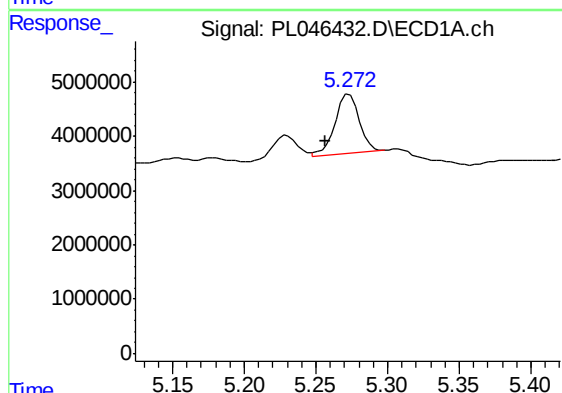


#10 gamma-Chlordane

R.T.: 5.273 min
Delta R.T.: 0.016 min
Response: 12851405
Conc: 1.25 ng/ml

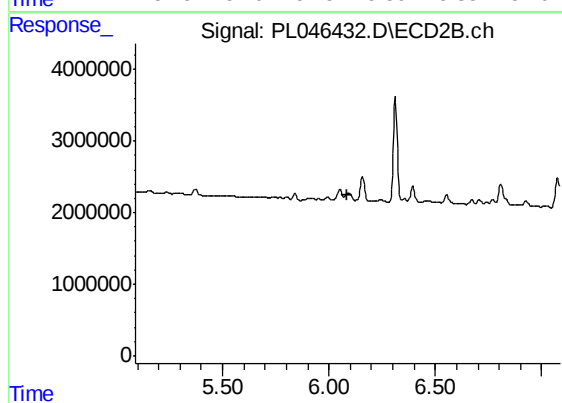

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

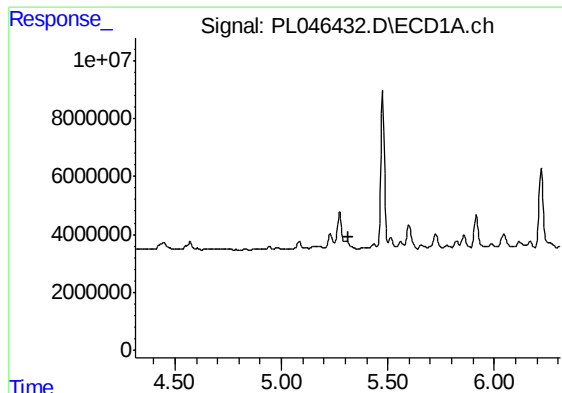

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EXT-025-SW034-031919

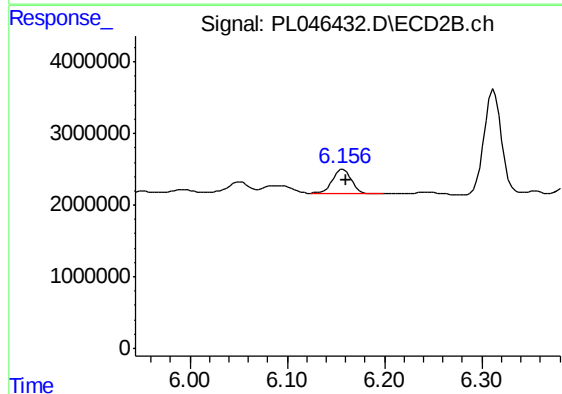


#11 alpha-Chlordane

R.T.: 6.158 min
Delta R.T.: -0.003 min
Response: 4532399
Conc: 1.60 ng/ml

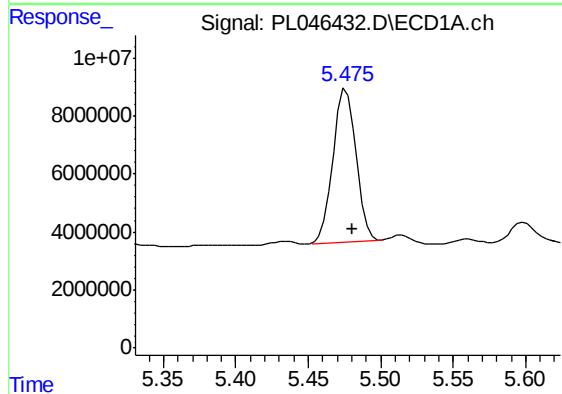


#12 4,4'-DDE

R.T.: 5.476 min
Delta R.T.: -0.005 min
Response: 58564567
Conc: 6.36 ng/ml

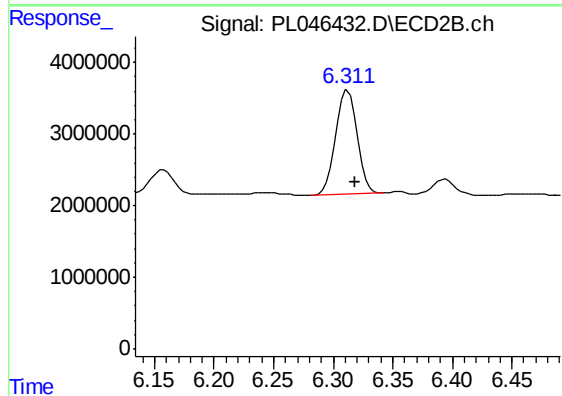

#12 4,4'-DDE


R.T.: 6.312 min
Delta R.T.: -0.006 min
Response: 18114047
Conc: 7.30 ng/ml

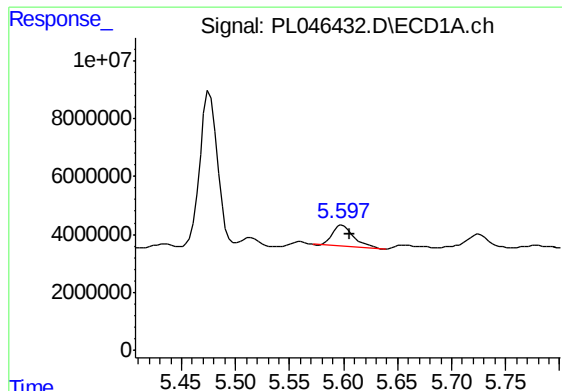

#13 Dieldrin


R.T.: 5.599 min
Delta R.T.: -0.007 min
Response: 10079509
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-025-SW034-031919

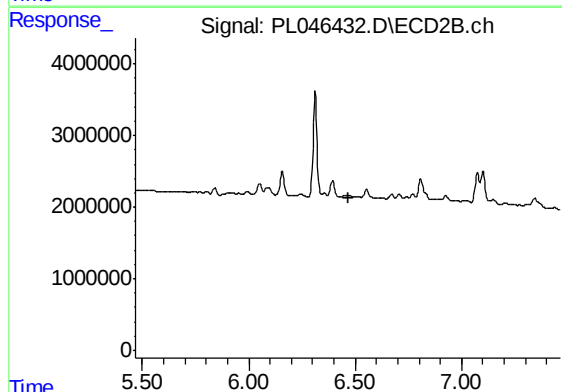


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.467 min
Response: 0
Conc: N.D.

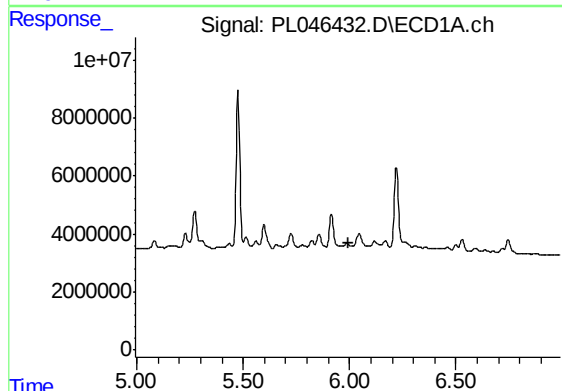


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

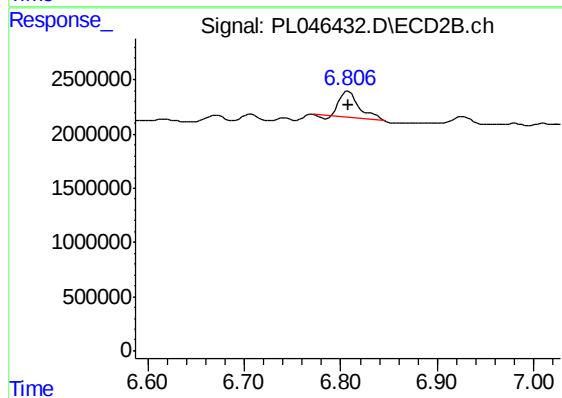

#16 4,4'-DDD


R.T.: 6.808 min
Delta R.T.: 0.000 min
Response: 3205331
Conc: 1.59 ng/ml

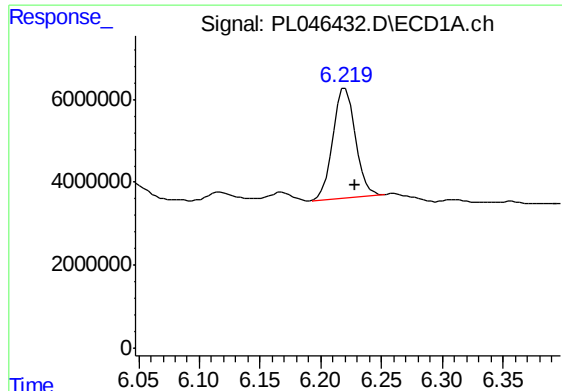

#17 4,4'-DDT


R.T.: 6.220 min
Delta R.T.: -0.007 min
Response: 34215293
Conc: 4.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-025-SW034-031919

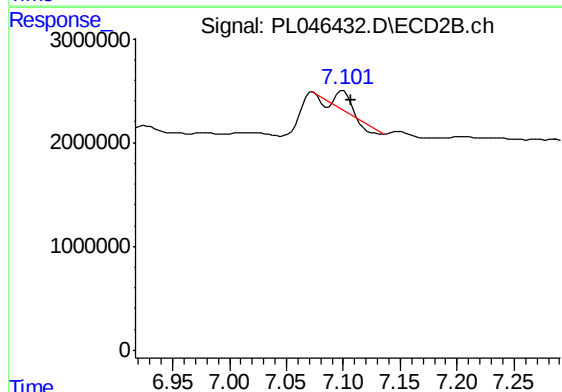


#17 4,4'-DDT

R.T.: 7.100 min
Delta R.T.: -0.007 min
Response: 966408
Conc: 0.46 ng/ml

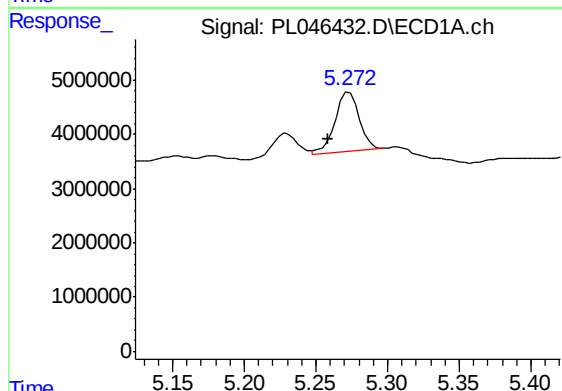


#25 Chlordane-3

R.T.: 5.273 min
Delta R.T.: 0.015 min
Response: 12851405
Conc: 11.54 ng/ml

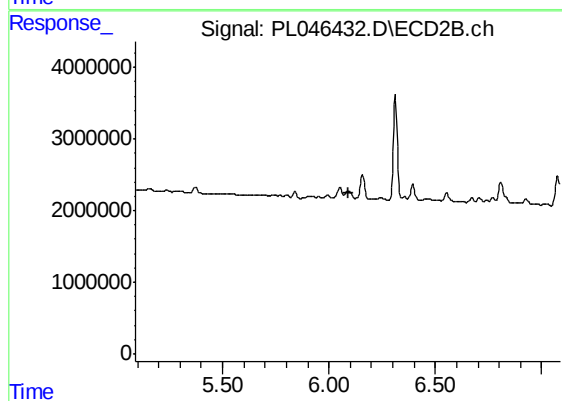

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

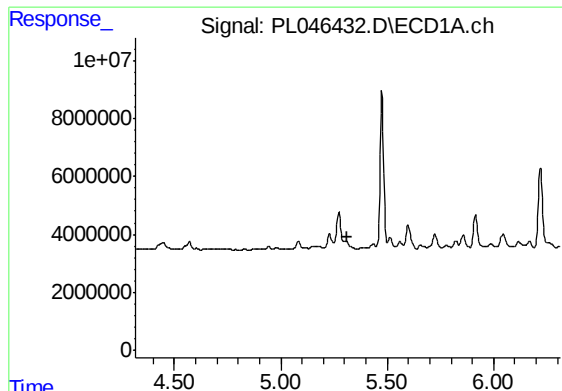

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EXT-025-SW034-031919

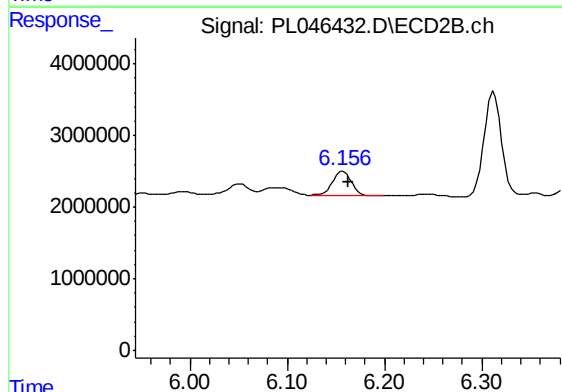


#26 Chlordane-4

R.T.: 6.158 min
Delta R.T.: -0.006 min
Response: 4532399
Conc: 9.82 ng/ml

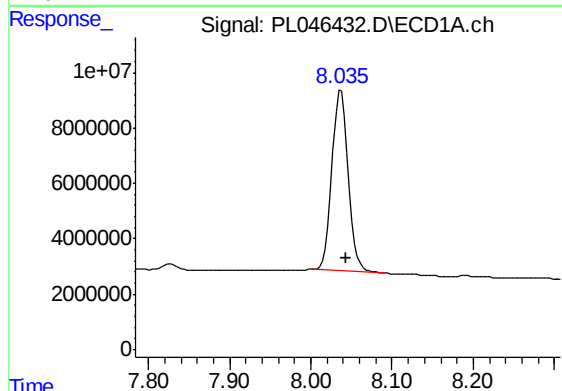

#28 Decachlorobiphenyl

R.T.: 8.037 min
Delta R.T.: -0.007 min
Response: 90695378
Conc: 10.78 ng/ml

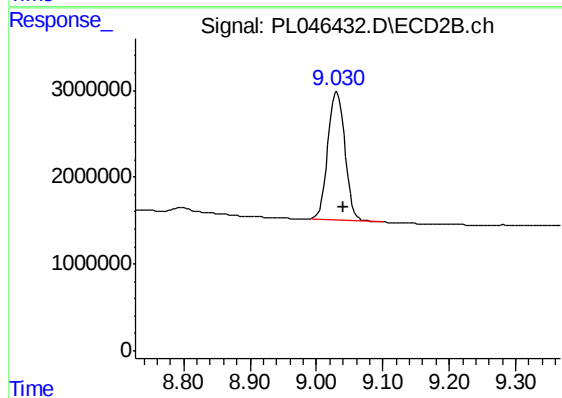

#28 Decachlorobiphenyl

R.T.: 9.031 min
Delta R.T.: -0.009 min
Response: 26397091
Conc: 11.39 ng/ml