

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032519\
 Data File : PL046433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2019 12:08
 Operator : AJ\SJ
 Sample : K2015-14RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-025-B029-031919RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 01:10:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.360	3.979	70992936	23732567	9.759	10.365
28)	SA Decachlor...	8.038	9.033	75317414	25046048	8.955	10.803
Target Compounds							
10)	B gamma-Chl...	0.000	6.088	0	3066112	N.D.	1.080 #
11)	B alpha-Chl...	0.000	6.156	0	1832652	N.D.	0.646 #
12)	B 4,4'-DDE	5.481	0.000	5811400	0	0.631	N.D. #
25)	Chlordane-3	0.000	6.088	0	3066112	N.D.	8.042 #
26)	Chlordane-4	0.000	6.156	0	1832652	N.D.	3.972 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032519\
Data File : PL046433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2019 12:08
Operator : AJ\SJ
Sample : K2015-14RE
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-025-B029-031919RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 01:10:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

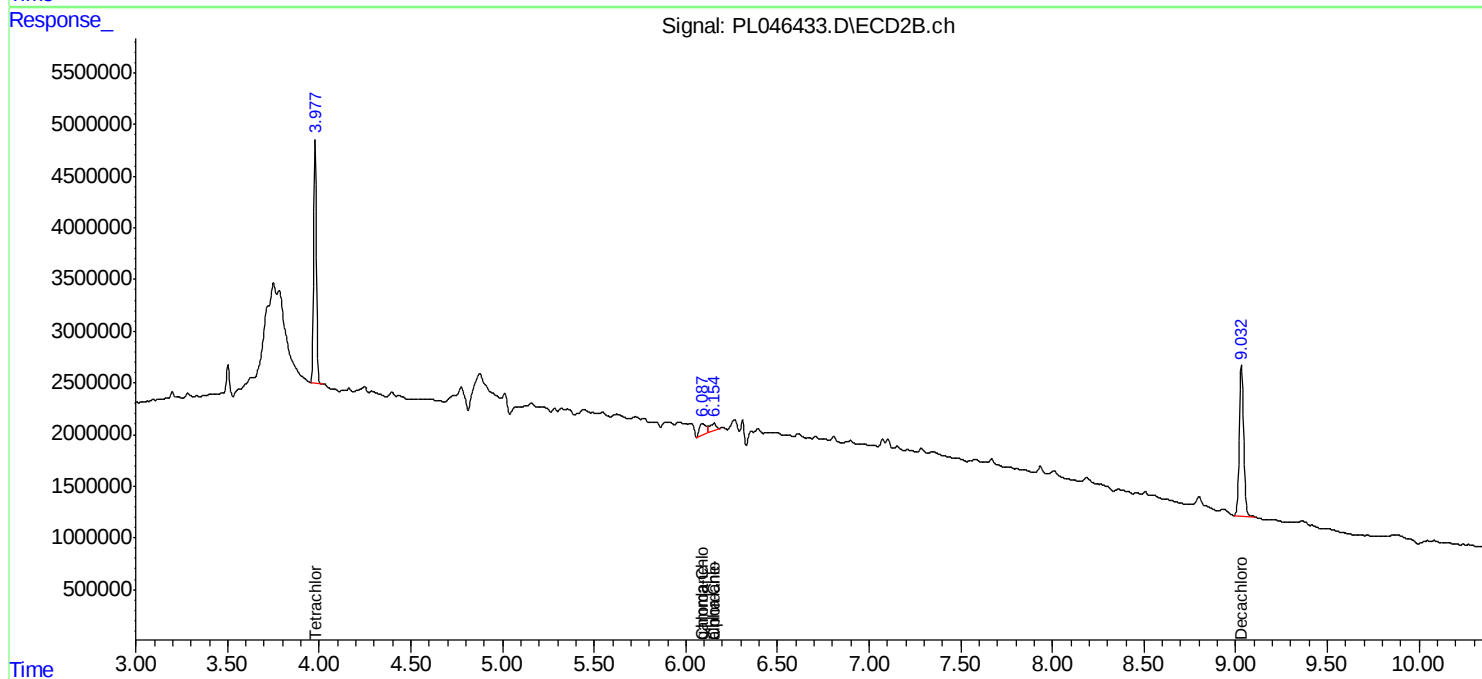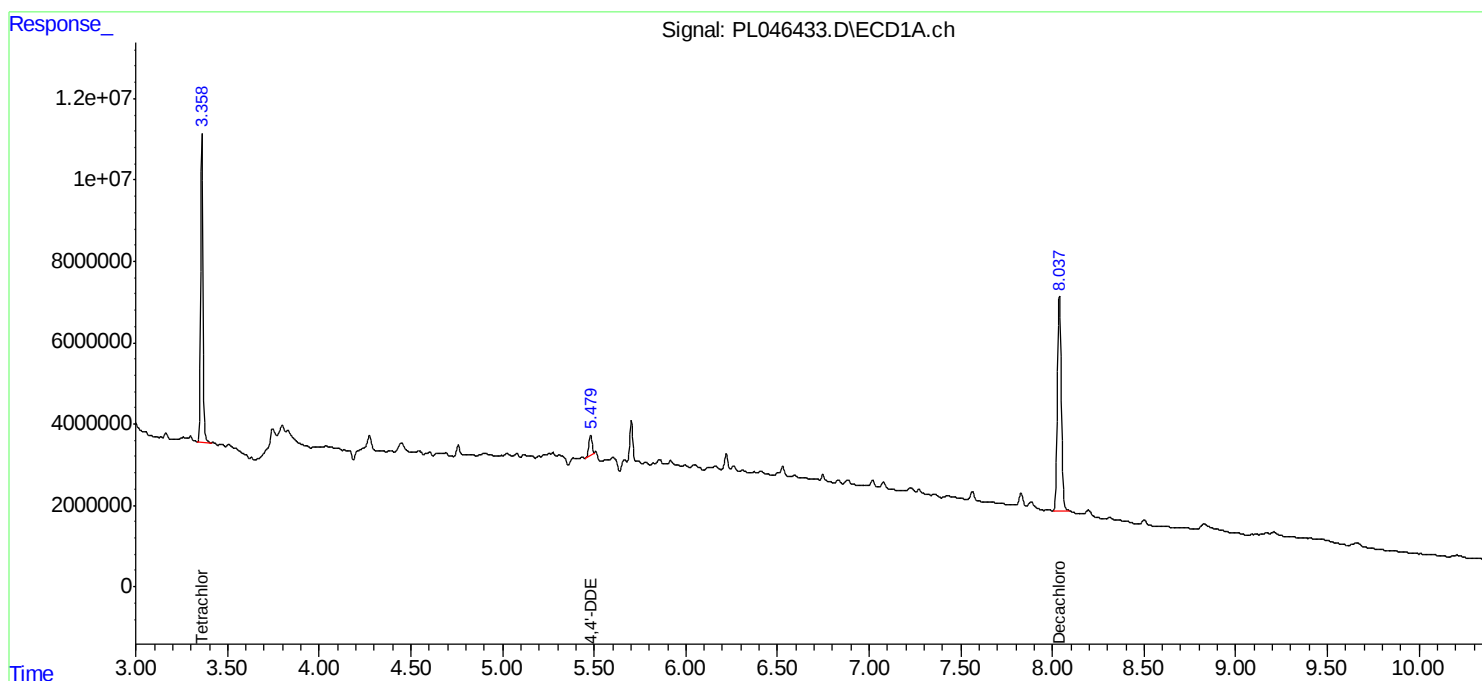


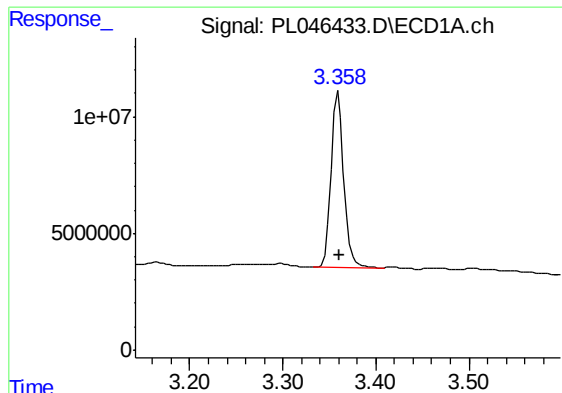

#1 Tetrachloro-m-xylene


R.T.: 3.360 min
Delta R.T.: -0.001 min
Response: 70992936
Conc: 9.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-025-B029-031919RE

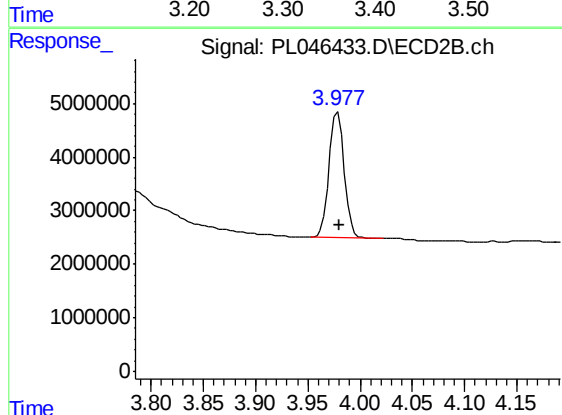


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 23732567
Conc: 10.37 ng/ml

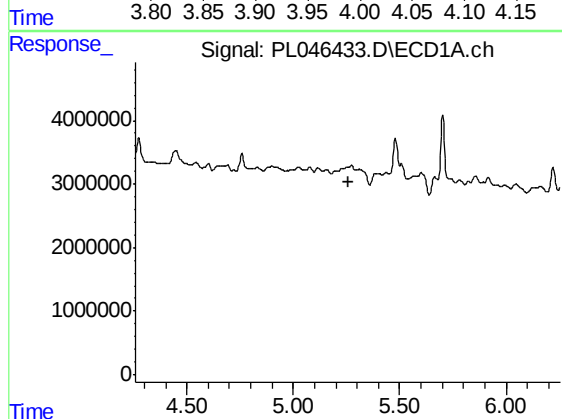


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

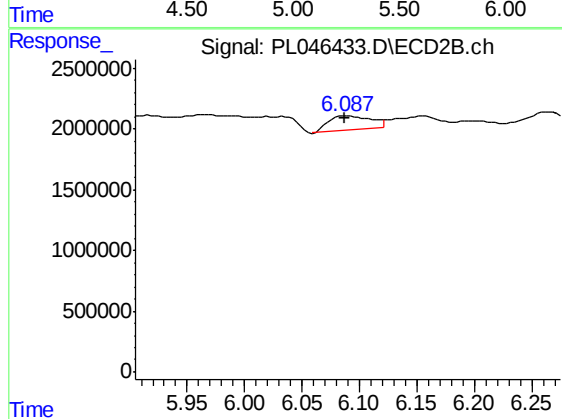

#10 gamma-Chlordane


R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 3066112
Conc: 1.08 ng/ml

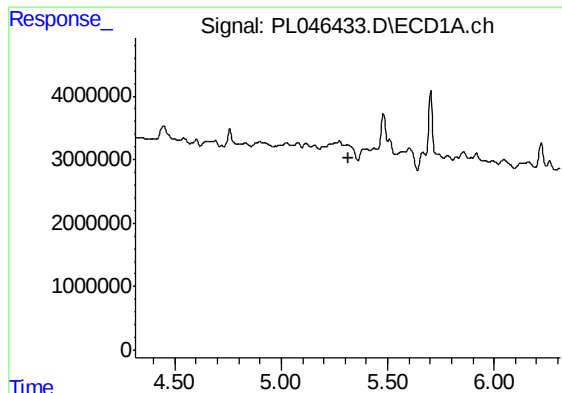

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-025-B029-031919RE

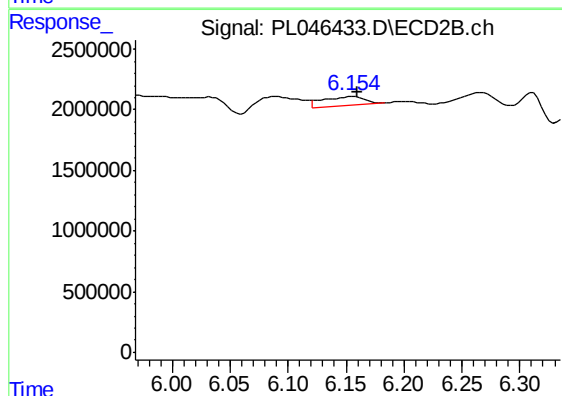


#11 alpha-Chlordane

R.T.: 6.156 min
Delta R.T.: -0.005 min
Response: 1832652
Conc: 0.65 ng/ml

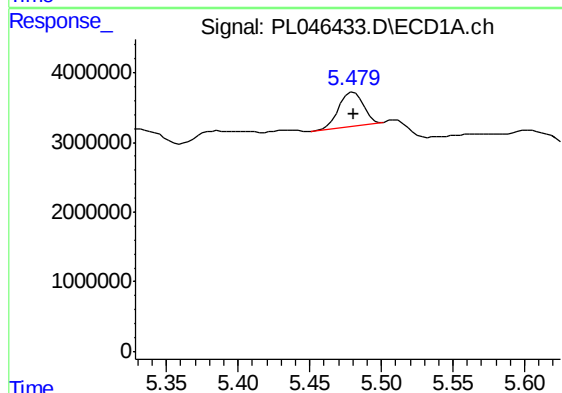


#12 4,4'-DDE

R.T.: 5.481 min
Delta R.T.: 0.000 min
Response: 5811400
Conc: 0.63 ng/ml

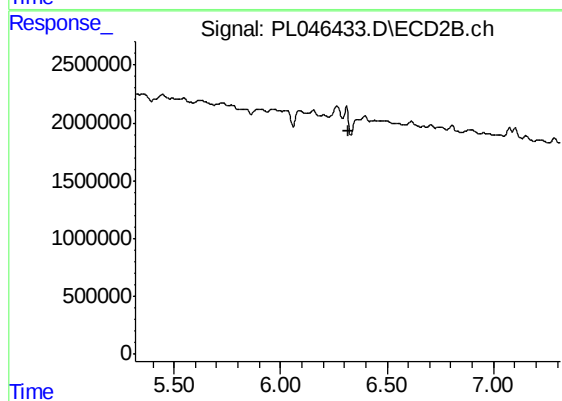

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.318 min
Response: 0
Conc: N.D.

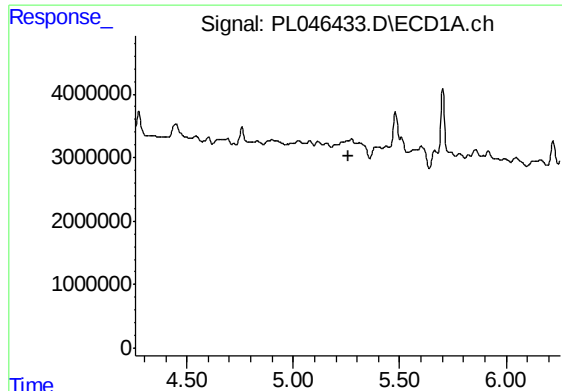

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-025-B029-031919RE

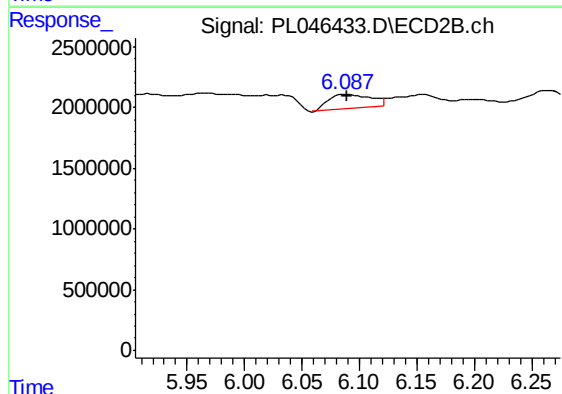


#25 Chlordane-3

R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 3066112
Conc: 8.04 ng/ml

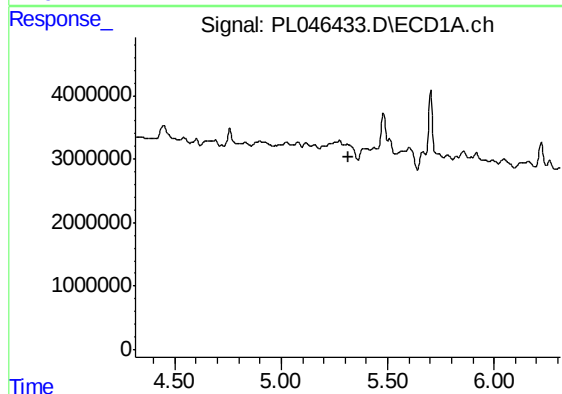


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.314 min
Response: 0
Conc: N.D.

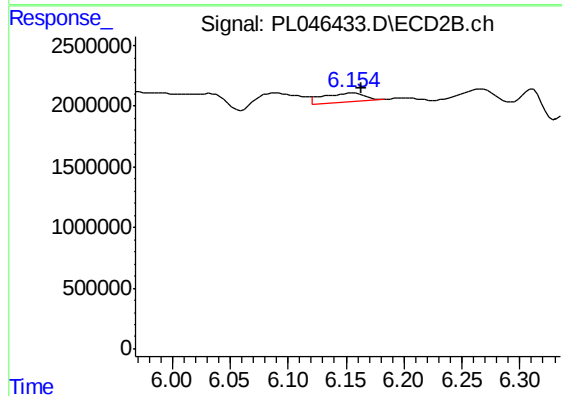

#26 Chlordane-4


R.T.: 6.156 min
Delta R.T.: -0.008 min
Response: 1832652
Conc: 3.97 ng/ml

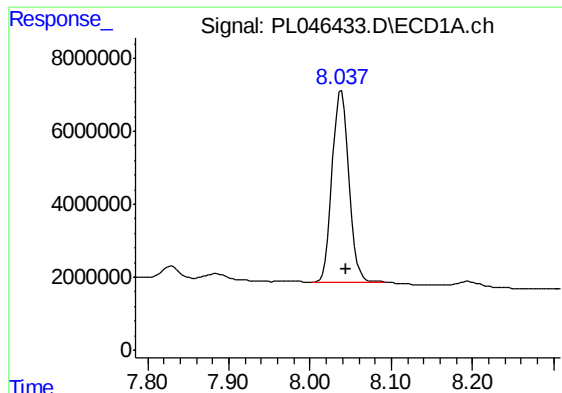

#28 Decachlorobiphenyl

R.T.: 8.038 min
Delta R.T.: -0.006 min
Response: 75317414
Conc: 8.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-025-B029-031919RE

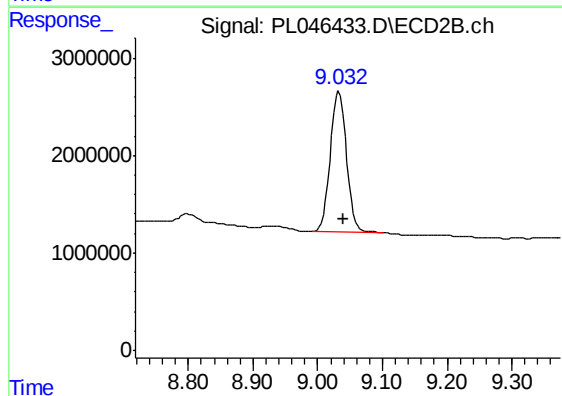

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: -0.007 min
Response: 25046048
Conc: 10.80 ng/ml