

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032519\
 Data File : PL046451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2019 18:09
 Operator : AJ\SJ
 Sample : K2050-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CS-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 01:15:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.360	3.978	123.4E6	40180174	16.968	17.549
28)	SA Decachlor...	8.038	9.033	151.5E6	46591281	18.012	20.096
Target Compounds							
10)	B gamma-Chl...	0.000	6.070f	0	2489896	N.D.	0.877 #
25)	Chlordane-3	0.000	6.070f	0	2489896	N.D.	6.531 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032519\
Data File : PL046451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2019 18:09
Operator : AJ\SJ
Sample : K2050-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CS-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 01:15:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

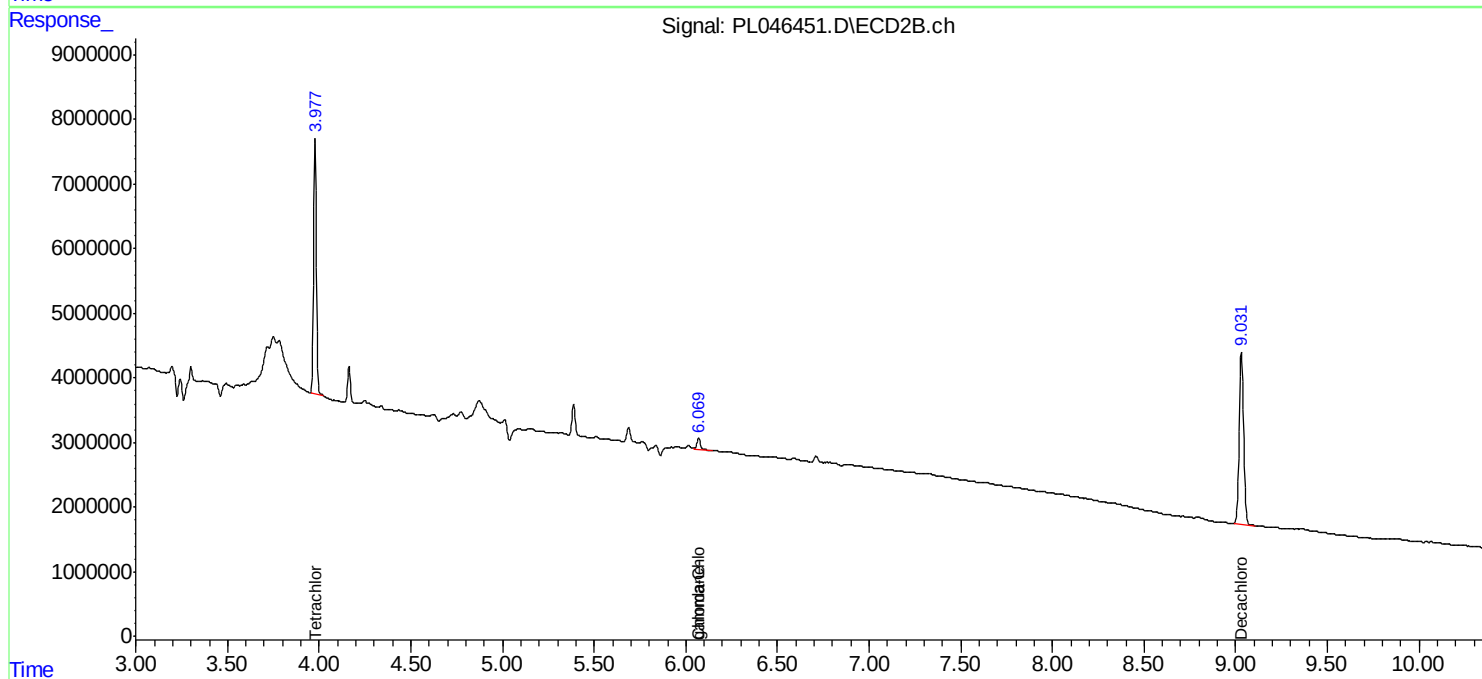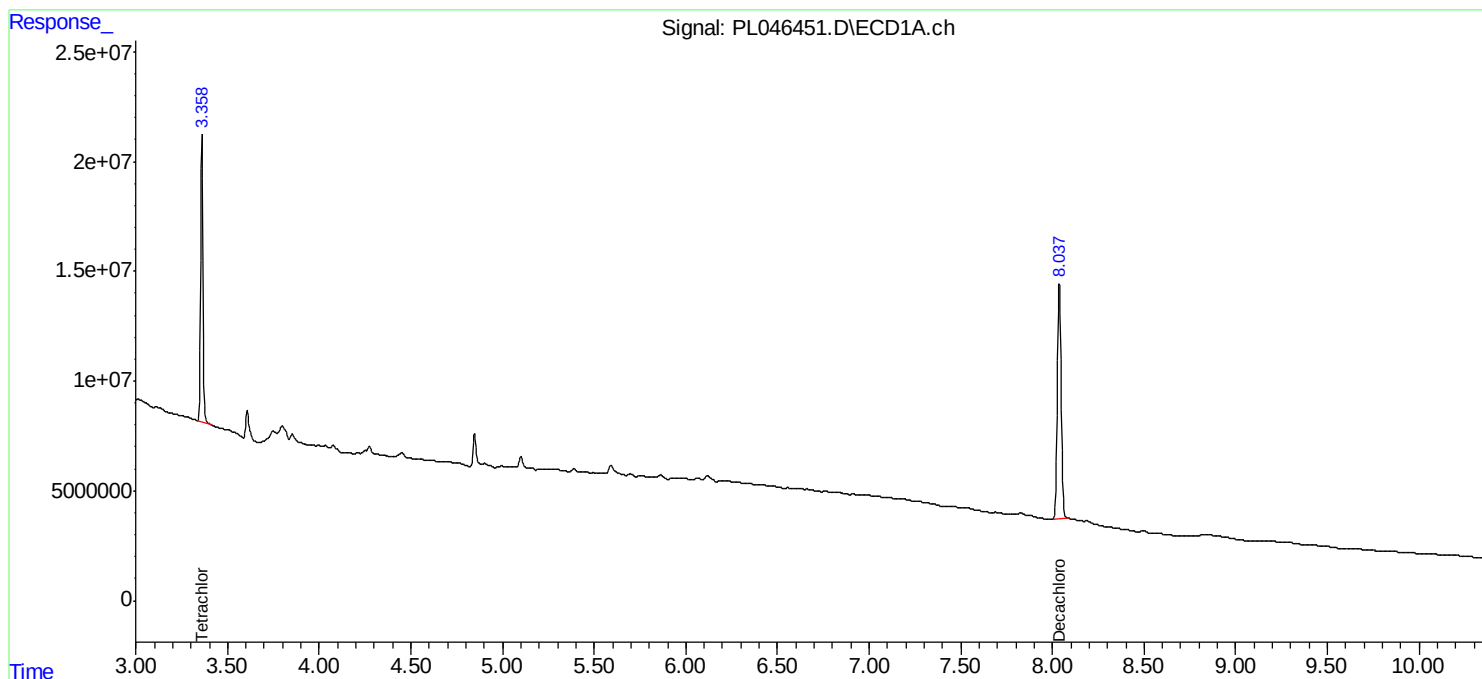


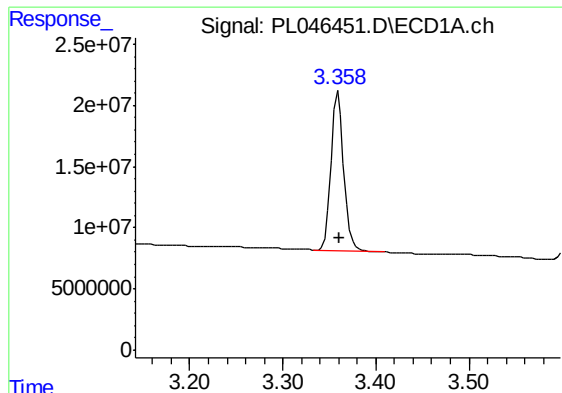

#1 Tetrachloro-m-xylene


R.T.: 3.360 min
Delta R.T.: -0.001 min
Response: 123437834
Conc: 16.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
CS-5

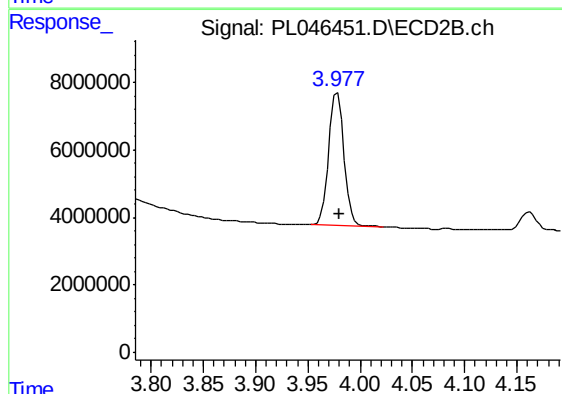


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.002 min
Response: 40180174
Conc: 17.55 ng/ml

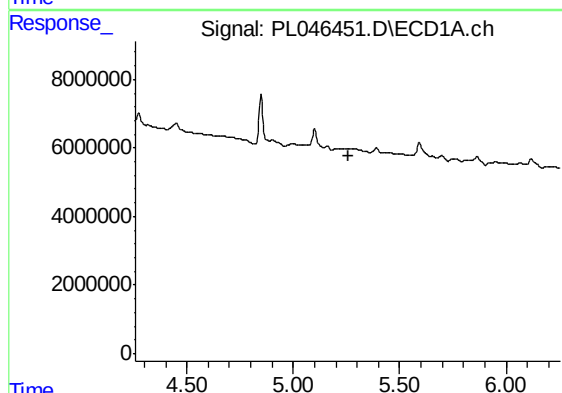


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.257 min
Response: 0
Conc: N.D.

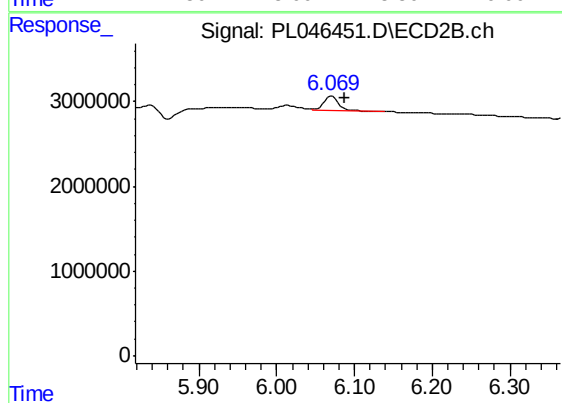

#10 gamma-Chlordane


R.T.: 6.070 min
Delta R.T.: -0.017 min
Response: 2489896
Conc: 0.88 ng/ml

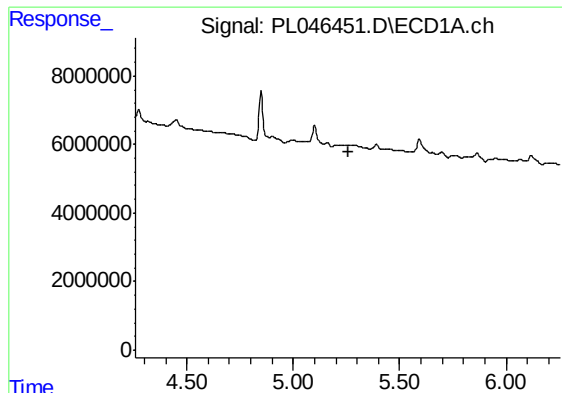

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CS-5

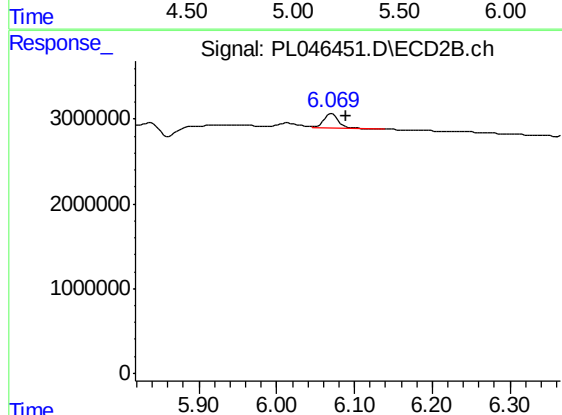


#25 Chlordane-3

R.T.: 6.070 min
Delta R.T.: -0.019 min
Response: 2489896
Conc: 6.53 ng/ml

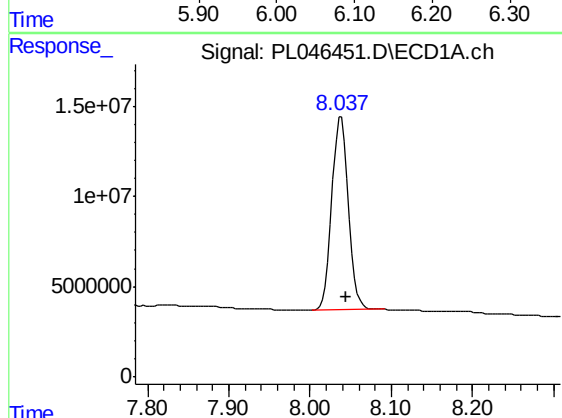

#28 Decachlorobiphenyl

R.T.: 8.038 min
Delta R.T.: -0.006 min
Response: 151496789
Conc: 18.01 ng/ml

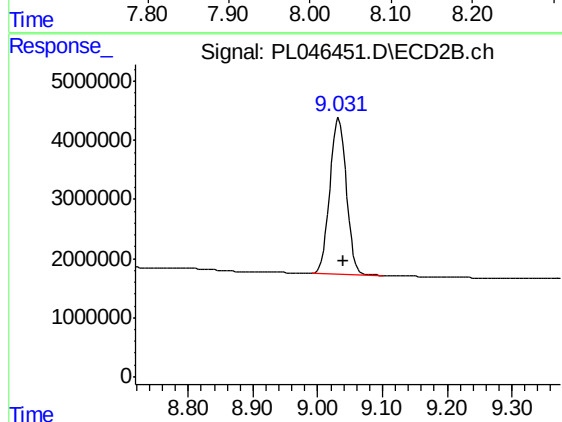

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: -0.007 min
Response: 46591281
Conc: 20.10 ng/ml