

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032521\
 Data File : PL065553.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2021 11:45
 Operator : AR\AJ
 Sample : PB135321BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB135321BL

Manual Integrations
 APPROVED

Ankita
 3/26/2021 11:06:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 13:49:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.784	47897717	49787655	20.169	18.139
28)	SA Decachlor...	7.922	8.733	28639394	35762413	11.854m	18.042 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032521\
Data File : PL065553.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2021 11:45
Operator : AR\AJ
Sample : PB135321BL
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PB135321BL


Manual Integrations
APPROVED

Ankita
3/26/2021 11:06:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 13:49:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

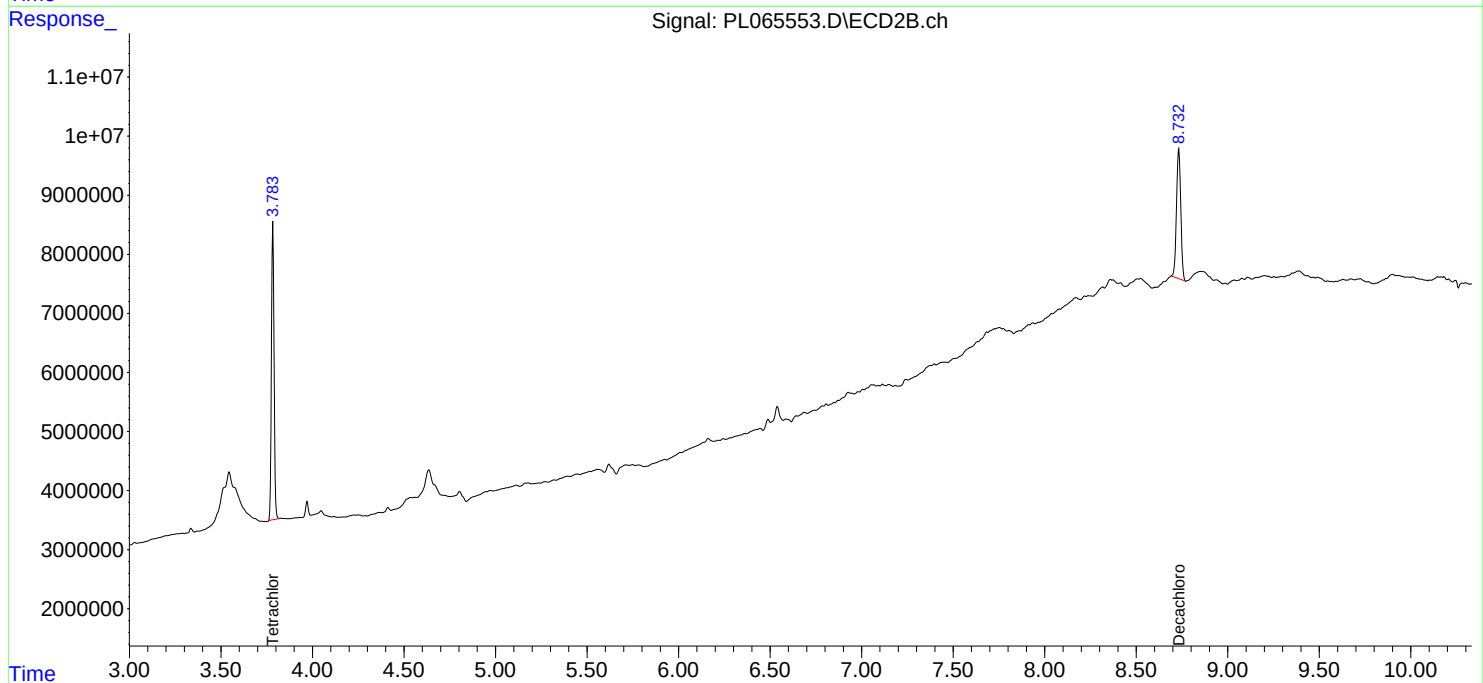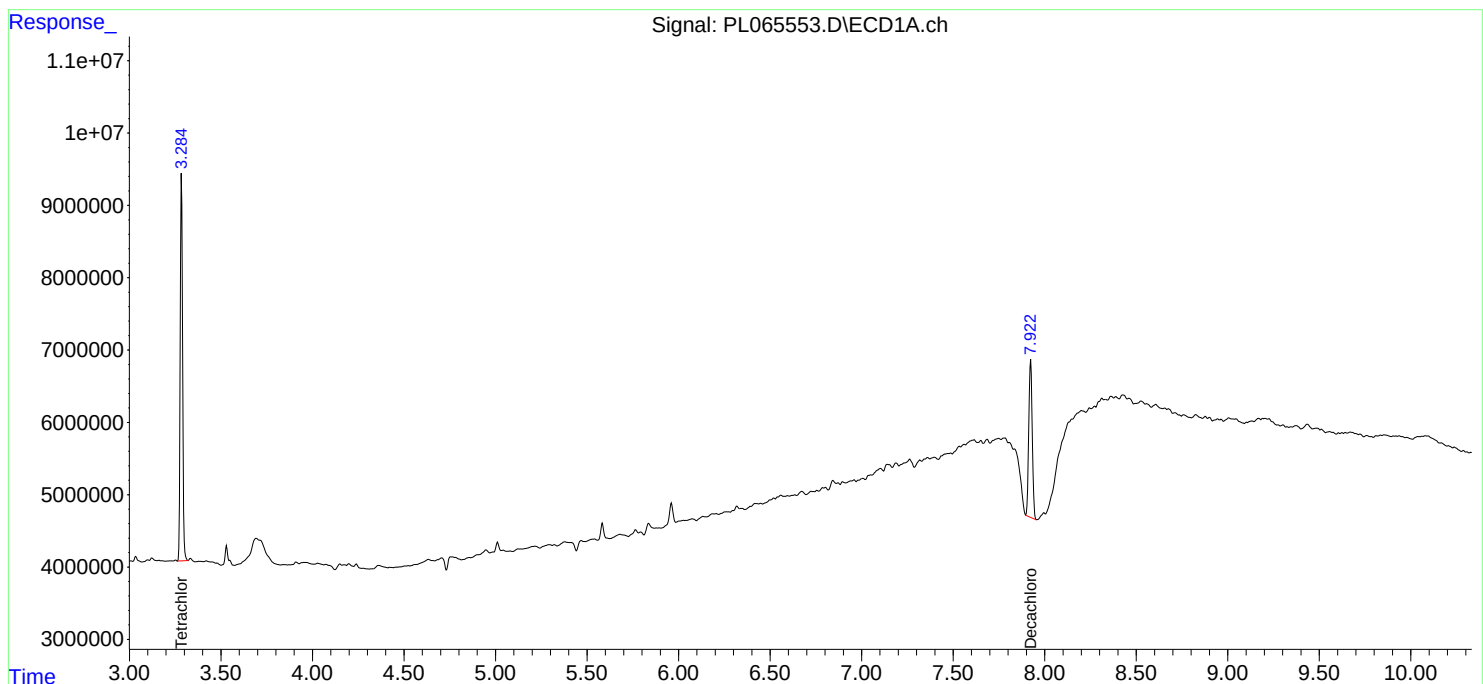

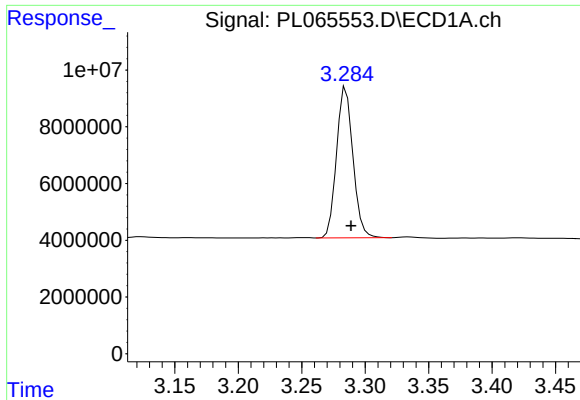


#1 Tetrachloro-m-xylene

R.T.: 3.285 min
Delta R.T.: -0.004 min
Response: 47897717
Conc: 20.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135321BL


Manual Integrations
APPROVED

Ankita
3/26/2021 11:06:46 AM

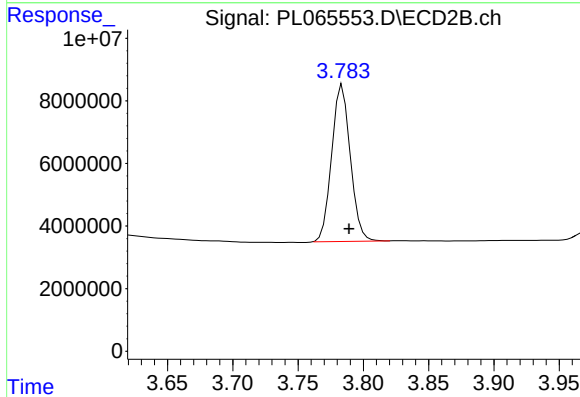


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: -0.005 min
Response: 49787655
Conc: 18.14 ng/ml

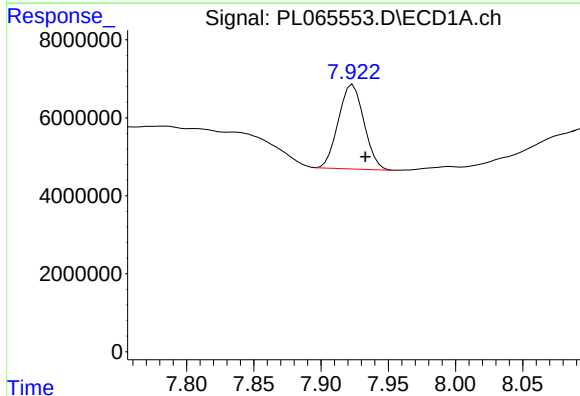

#28 Decachlorobiphenyl

R.T.: 7.922 min
Delta R.T.: -0.011 min
Response: 28639394
Conc: 11.85 ng/ml m

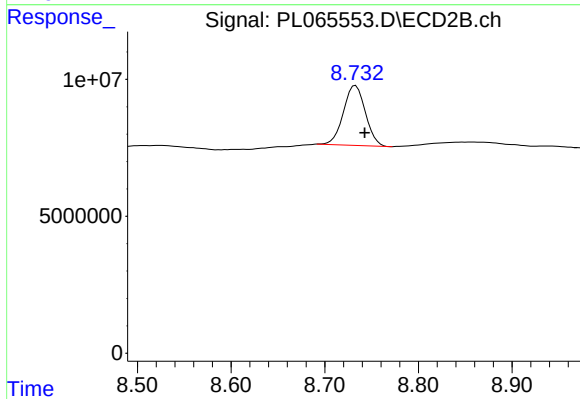

#28 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: -0.010 min
Response: 35762413
Conc: 18.04 ng/ml