

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032521\
 Data File : PL065560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2021 14:26
 Operator : AR\AJ
 Sample : M1786-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP-1

Manual Integrations
 APPROVED

Ankita
 3/26/2021 11:06:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 02:17:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.285	3.784	59360401	63523779	24.996	23.144
28)	SA Decachlor...	7.923	8.732	45995840	42462561	19.038	21.423
Target Compounds							
10)	B gamma-Chl...	5.156	5.845	6443225	6577084	2.182m	2.357m
11)	B alpha-Chl...	5.211	5.916	10371449	12662846	3.564	4.563 #
16)	A 4,4'-DDD	5.898	6.568	2404296	3544443	1.088m	1.611m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032521\
Data File : PL065560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2021 14:26
Operator : AR\AJ
Sample : M1786-01
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
SP-1


Manual Integrations
APPROVED

Ankita
3/26/2021 11:06:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 02:17:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

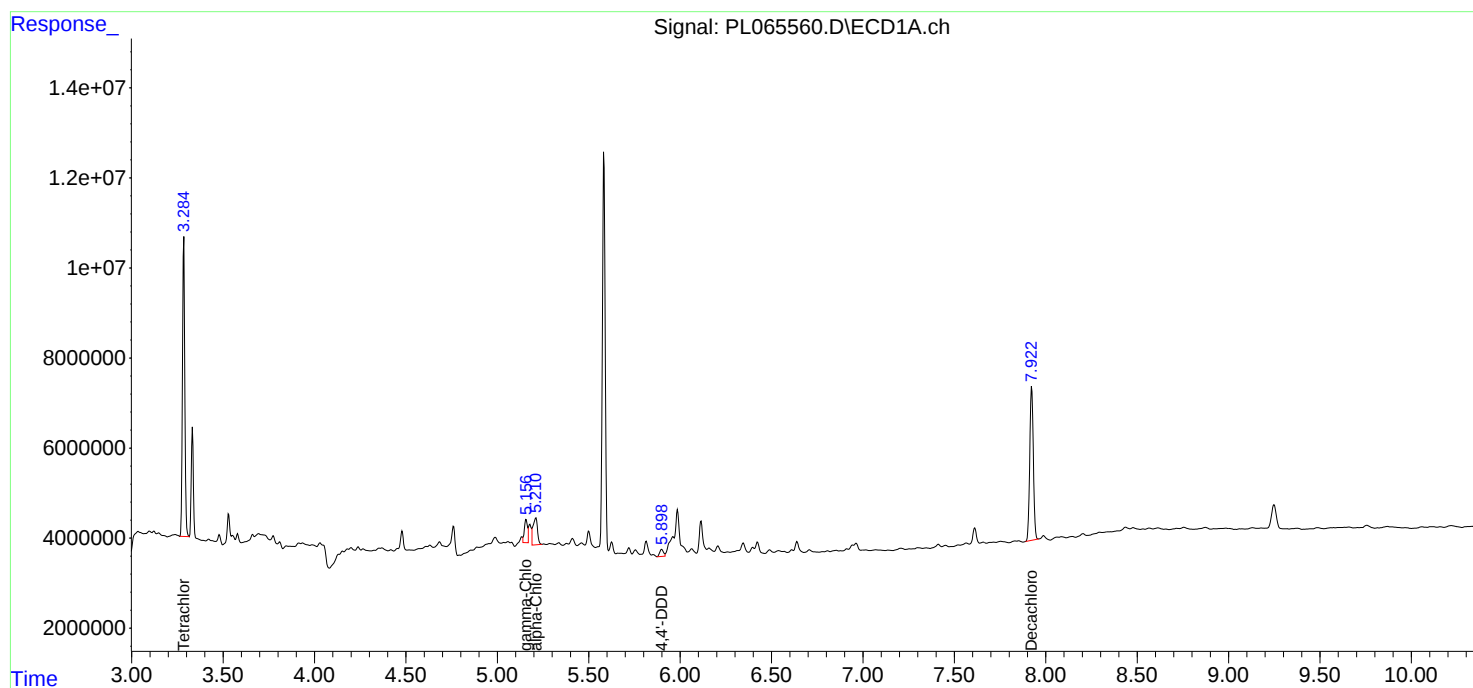

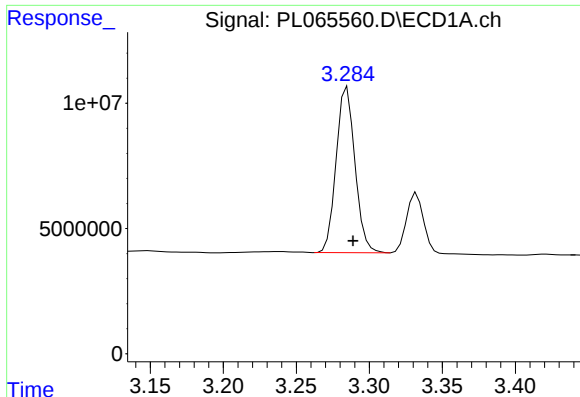


#1 Tetrachloro-m-xylene

R.T.: 3.285 min
Delta R.T.: -0.004 min
Response: 59360401
Conc: 25.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1


Manual Integrations
APPROVED

Ankita
3/26/2021 11:06:55 AM

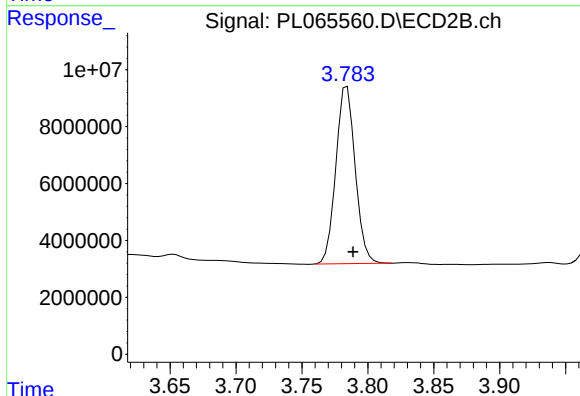


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: -0.005 min
Response: 63523779
Conc: 23.14 ng/ml

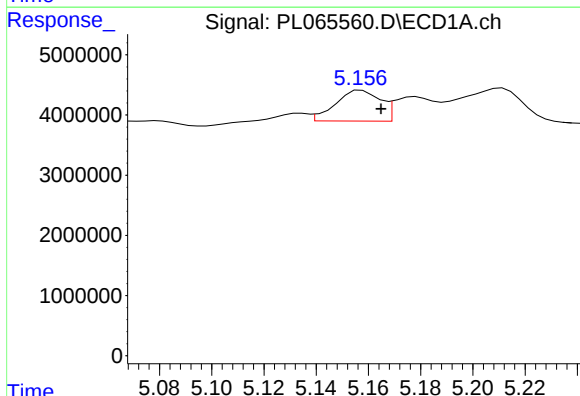


#10 gamma-Chlordane

R.T.: 5.156 min
Delta R.T.: -0.009 min
Response: 6443225
Conc: 2.18 ng/ml m

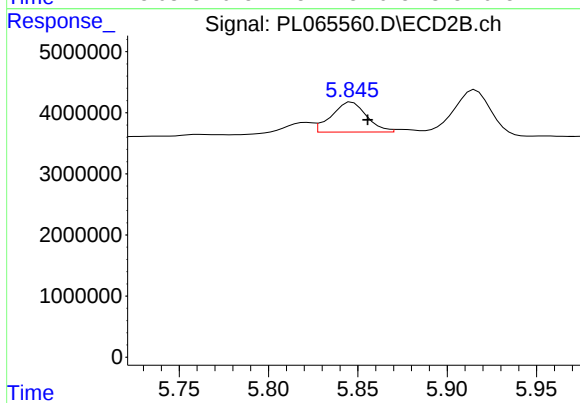

#10 gamma-Chlordane

R.T.: 5.845 min
Delta R.T.: -0.010 min
Response: 6577084
Conc: 2.36 ng/ml m

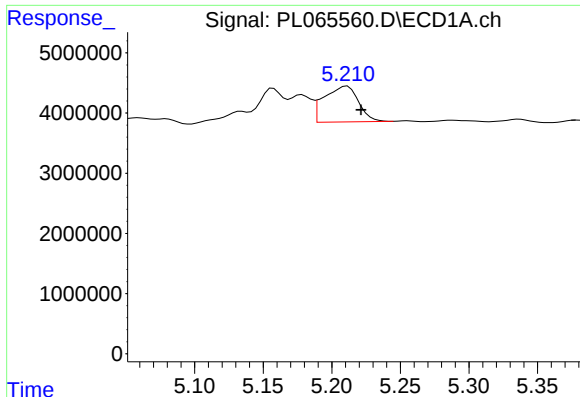


#11 alpha-Chlordane

R.T.: 5.211 min
Delta R.T.: -0.010 min
Response: 10371449
Conc: 3.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1


Manual Integrations
APPROVED

Ankita
3/26/2021 11:06:55 AM

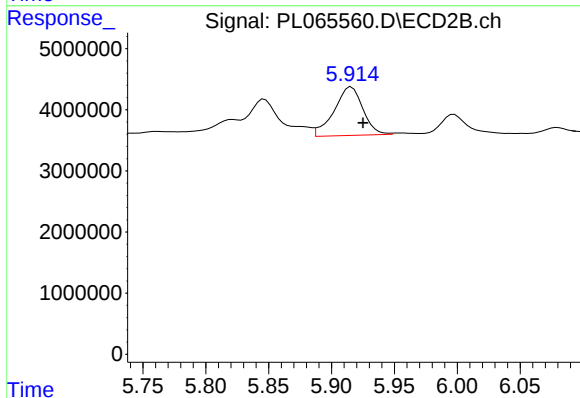


#11 alpha-Chlordane

R.T.: 5.916 min
Delta R.T.: -0.009 min
Response: 12662846
Conc: 4.56 ng/ml

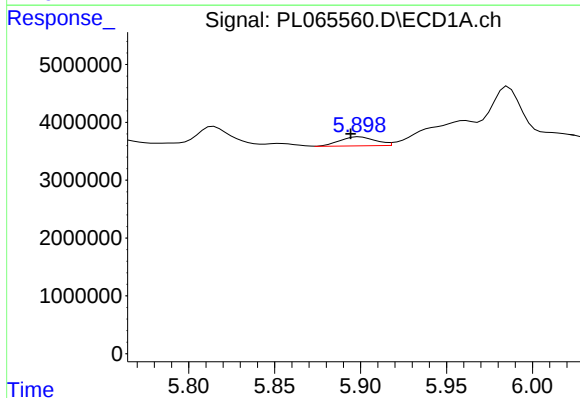


#16 4,4'-DDD

R.T.: 5.898 min
Delta R.T.: 0.003 min
Response: 2404296
Conc: 1.09 ng/ml m

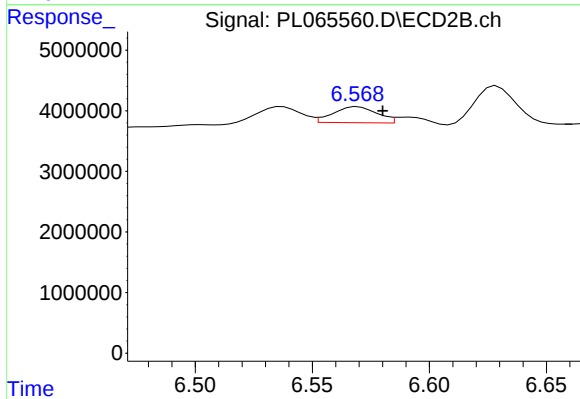

#16 4,4'-DDD

R.T.: 6.568 min
Delta R.T.: -0.012 min
Response: 3544443
Conc: 1.61 ng/ml m

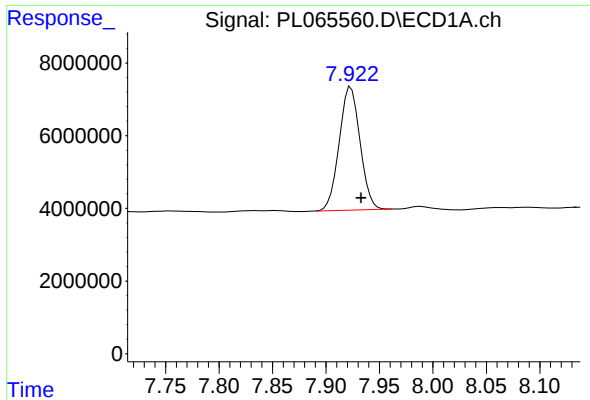


#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: -0.010 min
Response: 45995840
Conc: 19.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP-1

Manual Integrations
APPROVED

Ankita
3/26/2021 11:06:55 AM

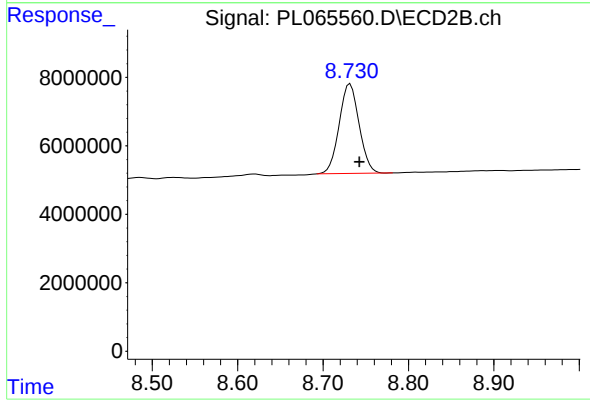

#28 Decachlorobiphenyl

R.T.: 8.732 min
Delta R.T.: -0.011 min
Response: 42462561
Conc: 21.42 ng/ml