

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032521\
 Data File : PL065565.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2021 16:05
 Operator : AR\AJ
 Sample : M1792-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5

Manual Integrations
 APPROVED

Ankita
 3/26/2021 11:07:03 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 02:18:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.290	3.785	30895522	45561015	13.010	16.599 #
28)	SA Decachlor...	7.928	8.735	17702968	15385459	7.327	7.762
Target Compounds							
12)	B 4,4'-DDE	5.369f	6.080	4924409	5948237	1.871	2.388m#
17)	MA 4,4'-DDT	6.119	6.860	4330631	1692575	2.288	0.862m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032521\
Data File : PL065565.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2021 16:05
Operator : AR\AJ
Sample : M1792-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
TP-5


Manual Integrations
APPROVED

Ankita
3/26/2021 11:07:03 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 02:18:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

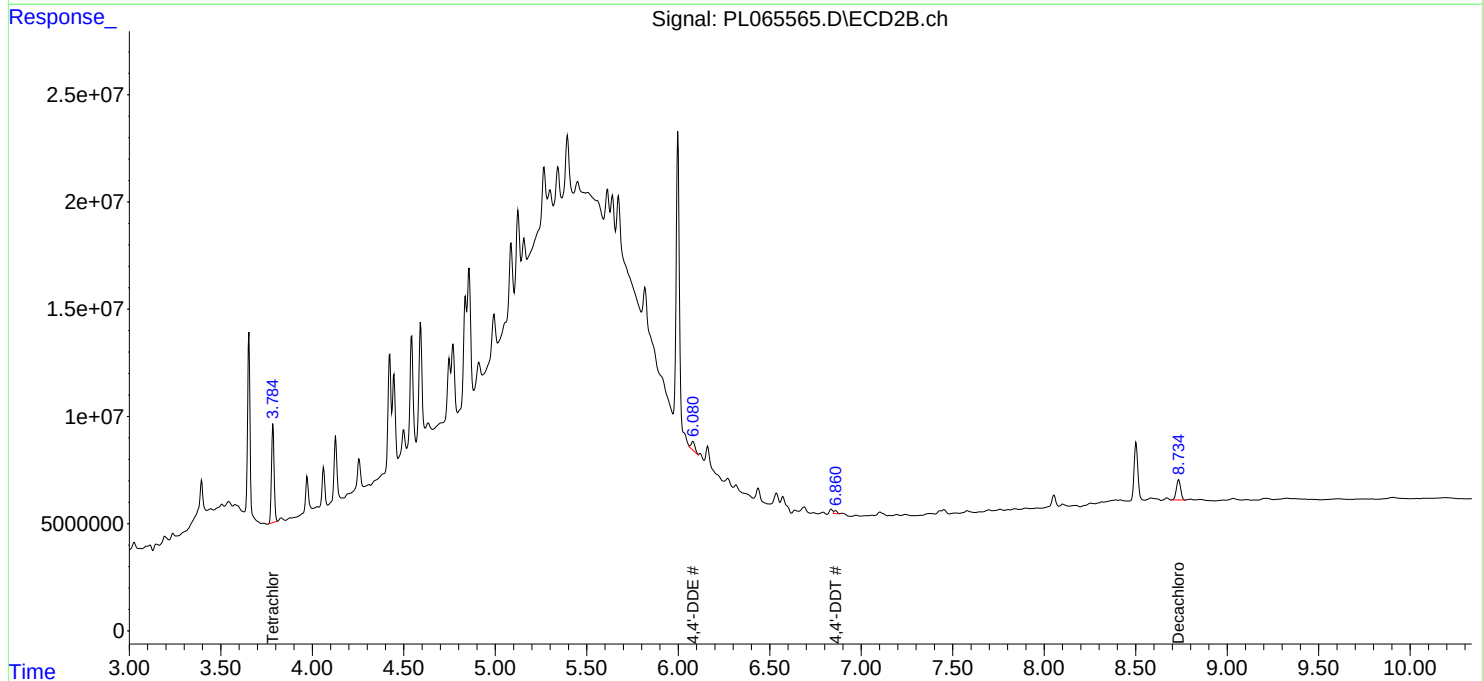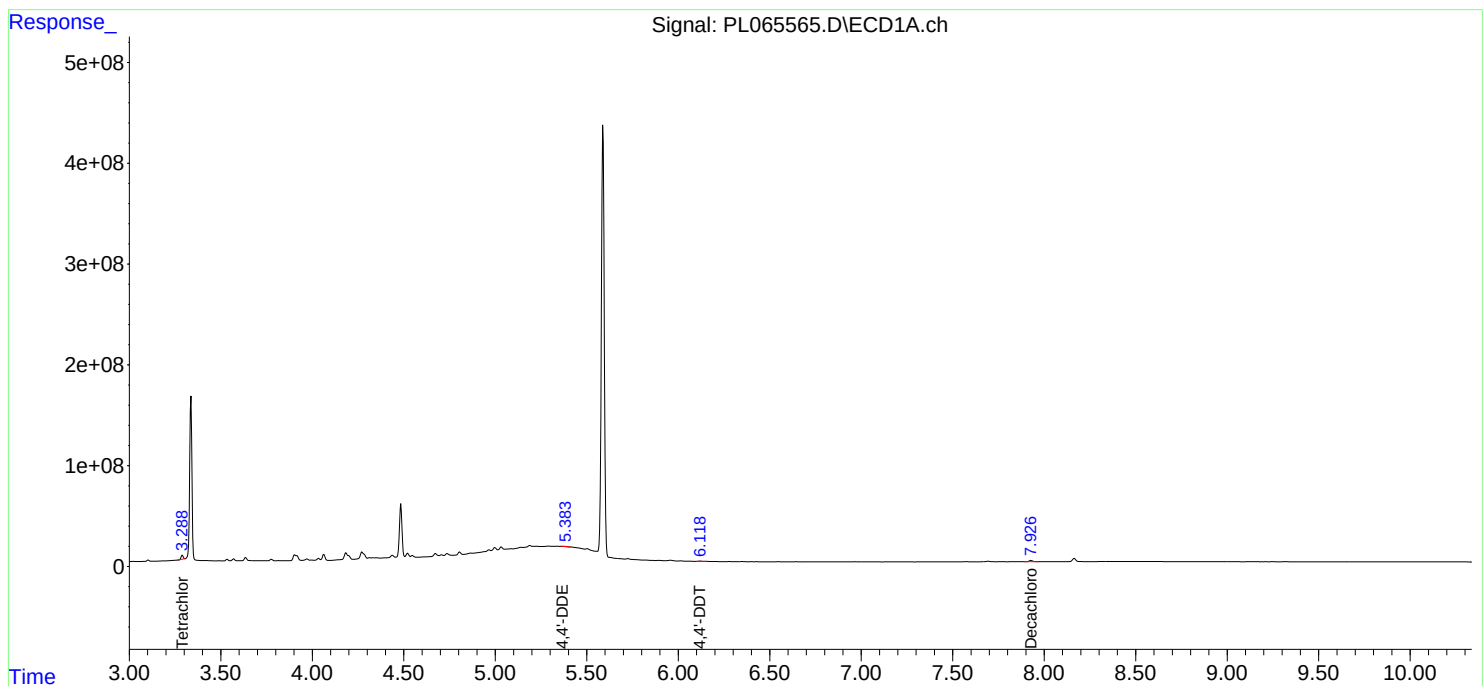

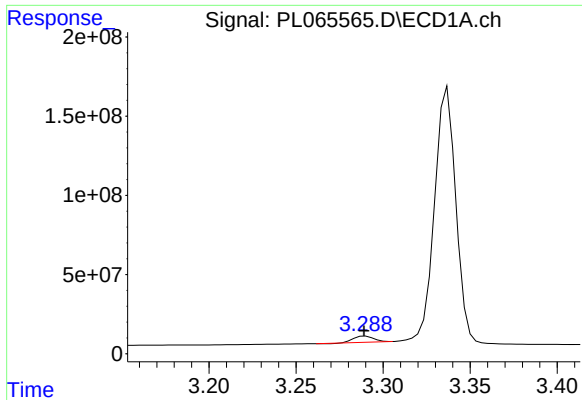


#1 Tetrachloro-m-xylene

R.T.: 3.290 min
Delta R.T.: 0.000 min
Response: 30895522
Conc: 13.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
3/26/2021 11:07:03 AM

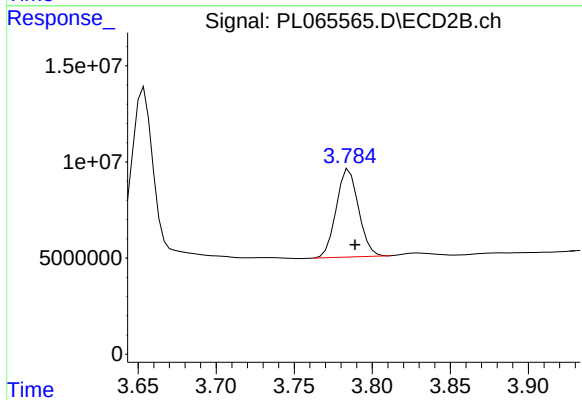


#1 Tetrachloro-m-xylene

R.T.: 3.785 min
Delta R.T.: -0.004 min
Response: 45561015
Conc: 16.60 ng/ml

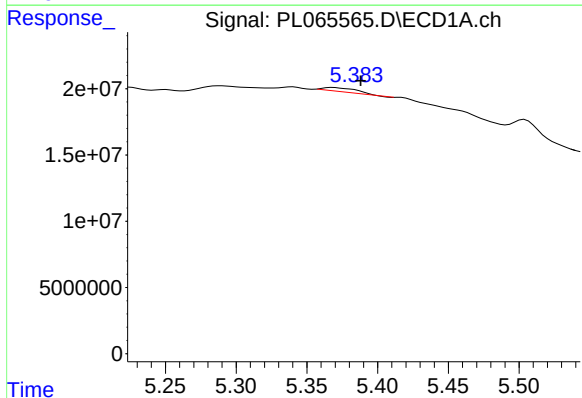


#12 4,4'-DDE

R.T.: 5.369 min
Delta R.T.: -0.019 min
Response: 4924409
Conc: 1.87 ng/ml

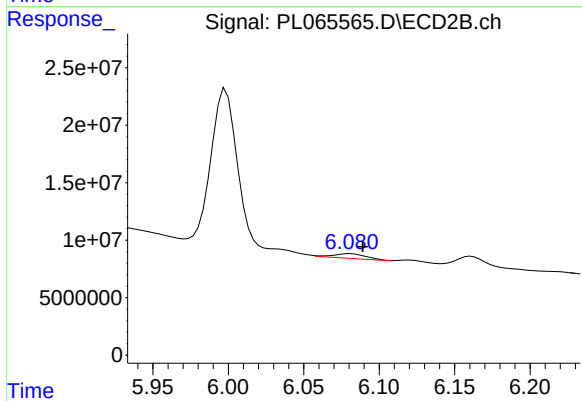

#12 4,4'-DDE

R.T.: 6.080 min
Delta R.T.: -0.009 min
Response: 5948237
Conc: 2.39 ng/ml m

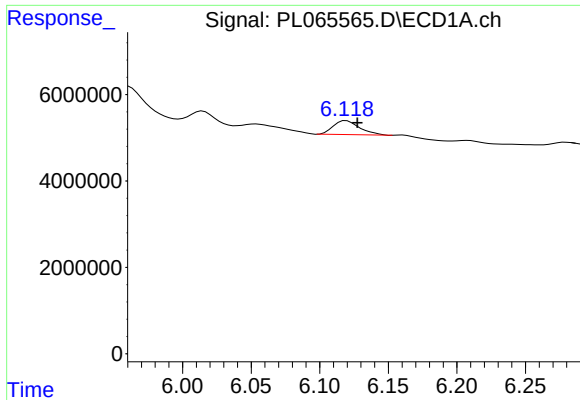


#17 4,4'-DDT

R.T.: 6.119 min
Delta R.T.: -0.008 min
Response: 4330631
Conc: 2.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5


Manual Integrations
APPROVED

Ankita
3/26/2021 11:07:03 AM

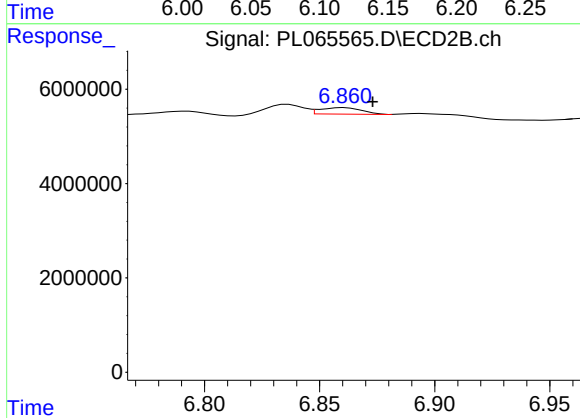


#17 4,4'-DDT

R.T.: 6.860 min
Delta R.T.: -0.013 min
Response: 1692575
Conc: 0.86 ng/ml m

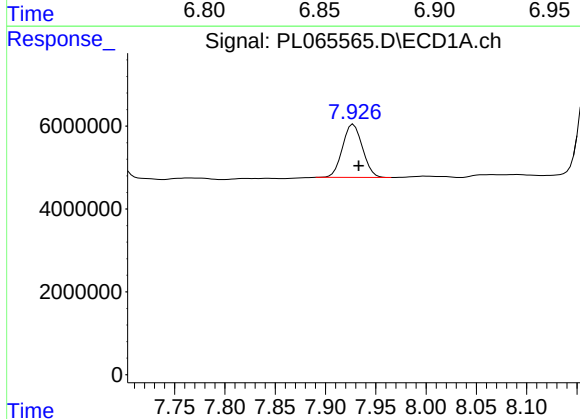

#28 Decachlorobiphenyl

R.T.: 7.928 min
Delta R.T.: -0.005 min
Response: 17702968
Conc: 7.33 ng/ml

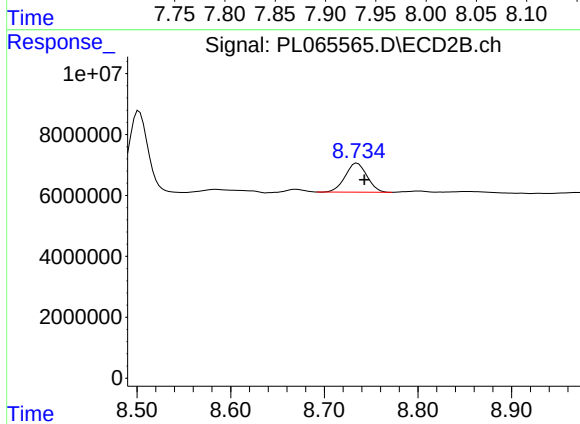

#28 Decachlorobiphenyl

R.T.: 8.735 min
Delta R.T.: -0.008 min
Response: 15385459
Conc: 7.76 ng/ml