

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032525\
 Data File : PL094829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2025 10:05
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 01:16:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.678	0.000	22023486	0	6.584	N.D. #
10) B	gamma-Chl...	5.951	0.000	2115879	0	0.628	N.D. #
13) MA	Dieldrin	0.000	5.369	0	13818645	N.D.	2.848 #
14) MA	Endrin	0.000	5.647	0	8519736	N.D.	1.952 #
23)	Chlordane-1	4.679f	0.000	9619574	0	68.653	N.D. #
25)	Chlordane-3	5.951	0.000	2115879	0	4.233	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032525\
Data File : PL094829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2025 10:05
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 01:16:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

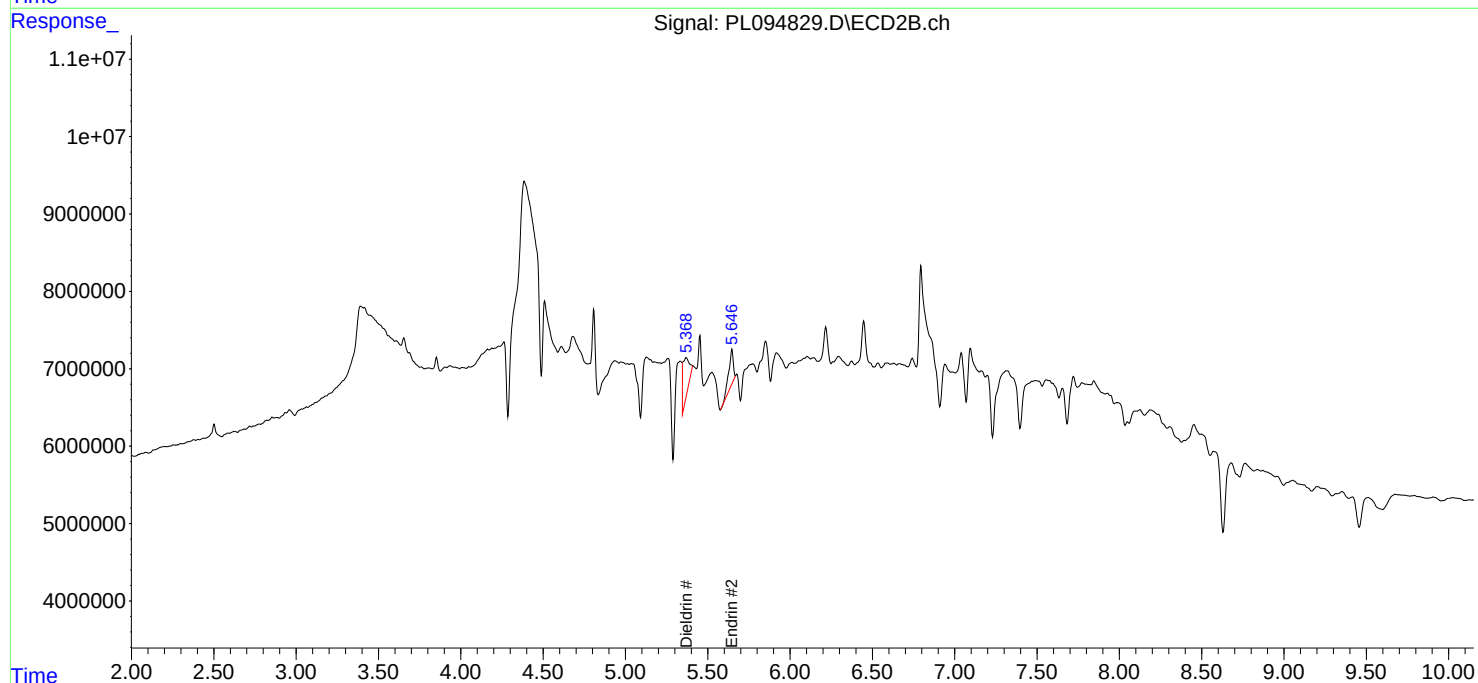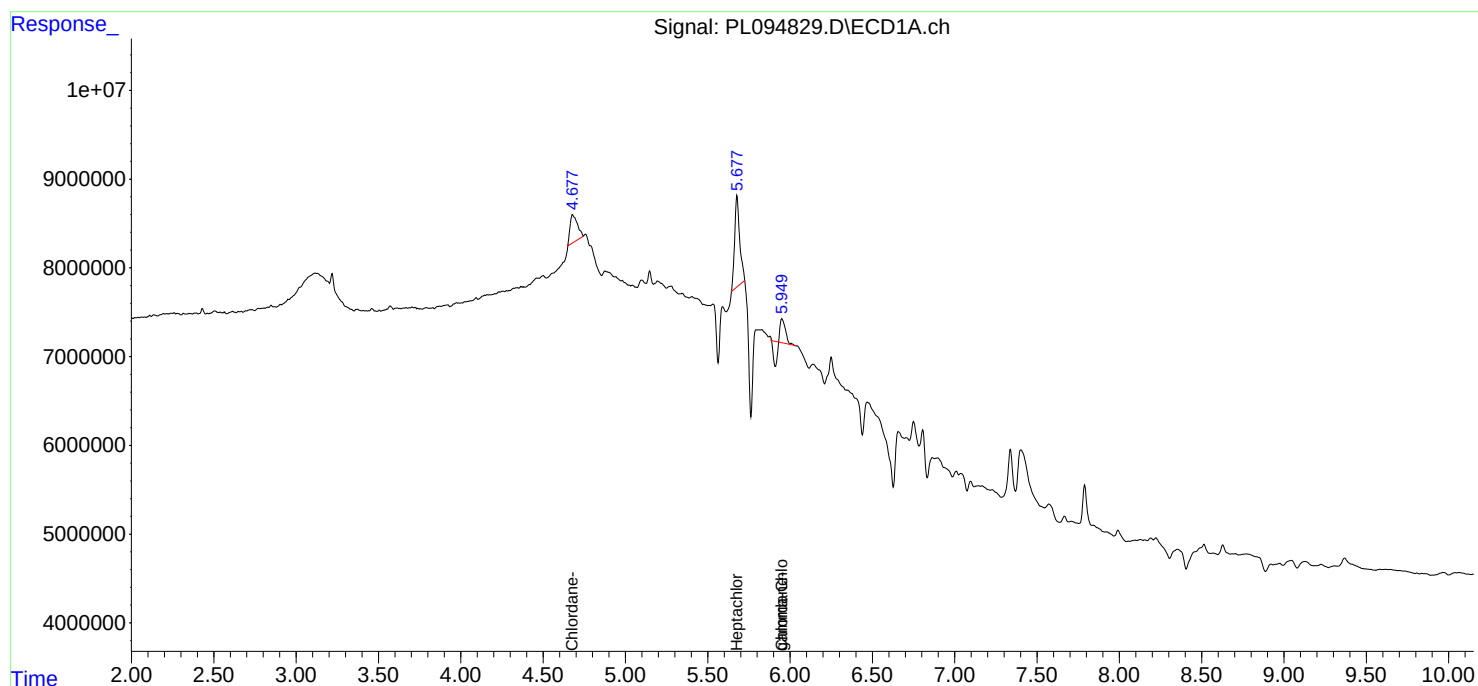


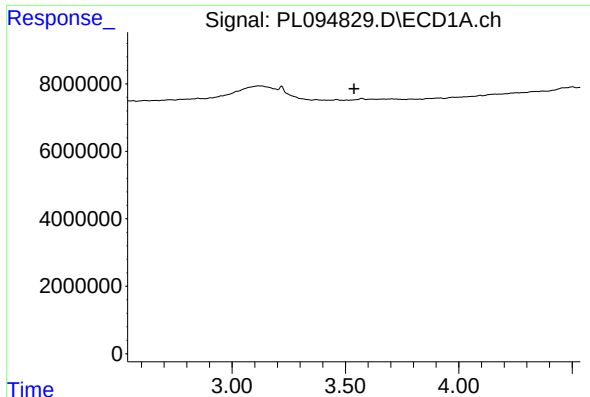

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.538 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

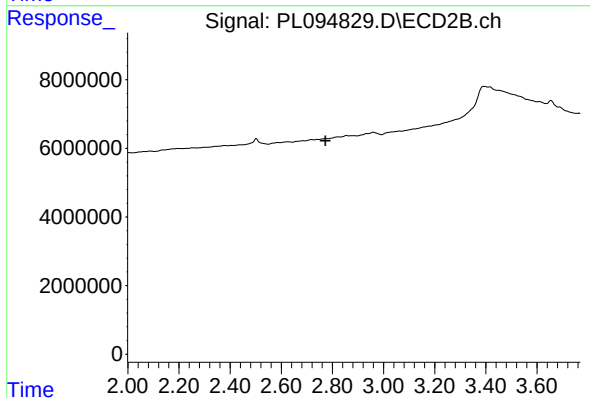


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.772 min
Response: 0
Conc: N.D.

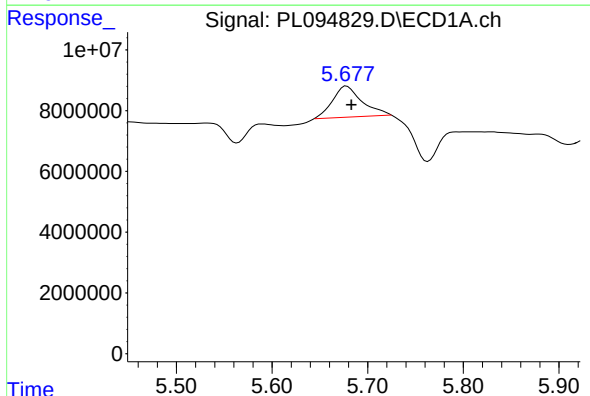


#8 Heptachlor epoxide

R.T.: 5.678 min
Delta R.T.: -0.005 min
Response: 22023486
Conc: 6.58 ng/ml

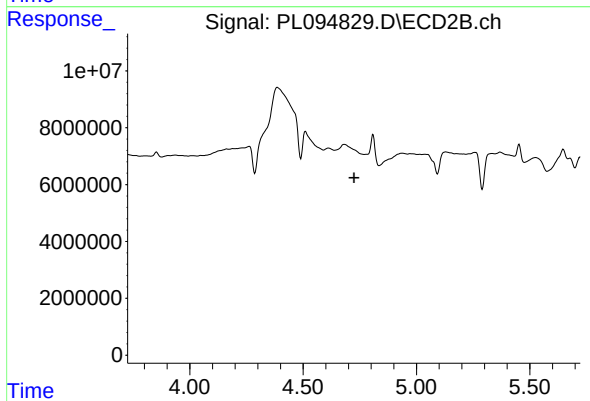

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.725 min
Response: 0
Conc: N.D.

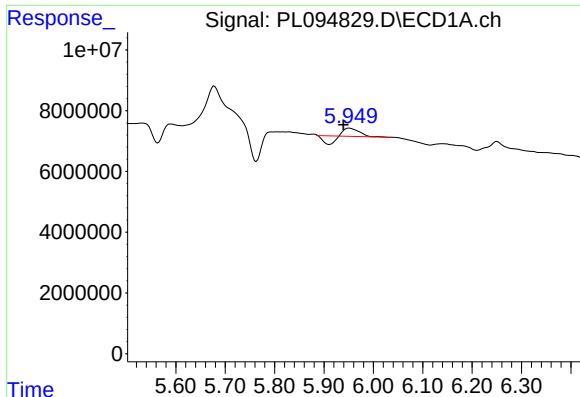

#10 gamma-Chlordane


R.T.: 5.951 min
Delta R.T.: 0.011 min
Response: 2115879
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

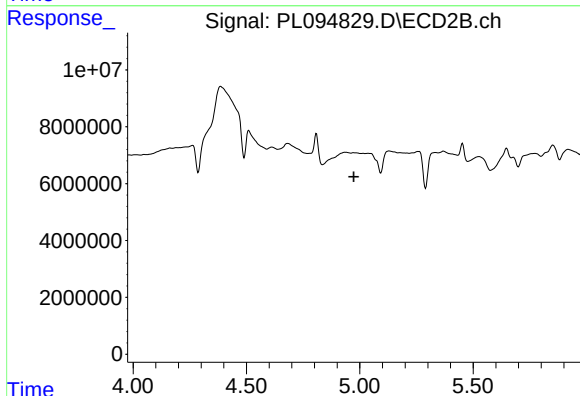


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

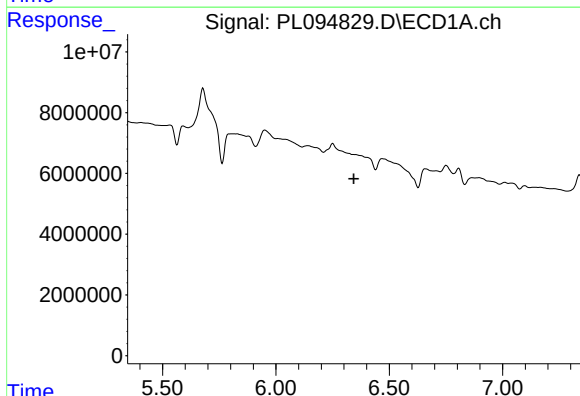


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

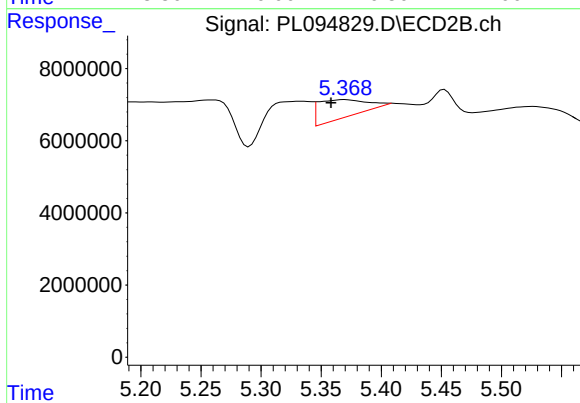

#13 Dieldrin


R.T.: 5.369 min
Delta R.T.: 0.011 min
Response: 13818645
Conc: 2.85 ng/ml

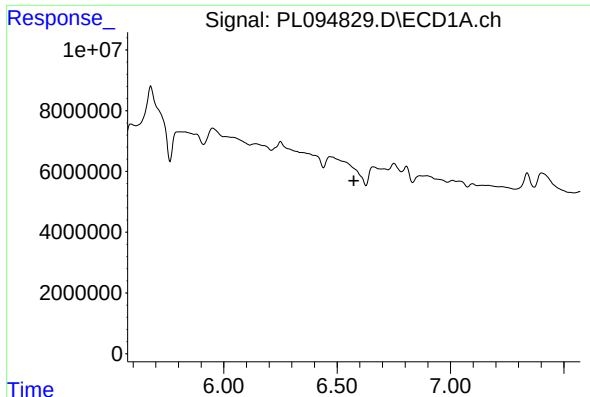

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

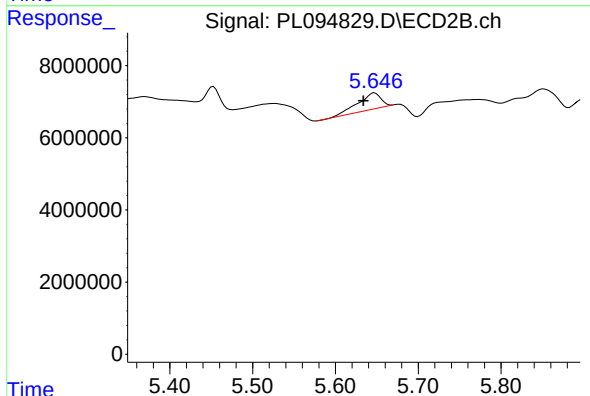


#14 Endrin

R.T.: 5.647 min
Delta R.T.: 0.014 min
Response: 8519736
Conc: 1.95 ng/ml

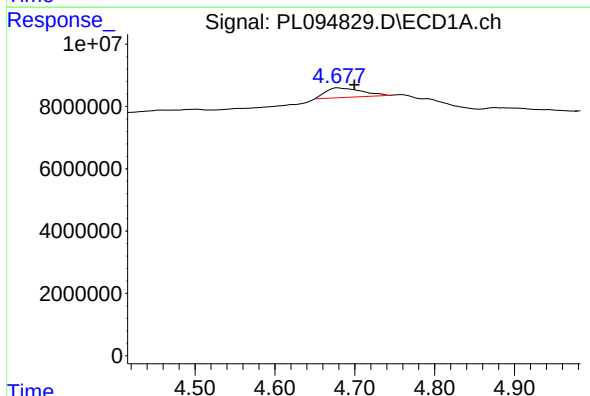


#23 Chlordane-1

R.T.: 4.679 min
Delta R.T.: -0.021 min
Response: 9619574
Conc: 68.65 ng/ml

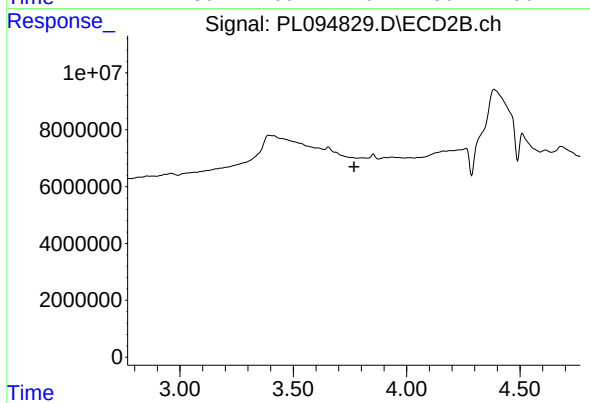

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 3.768 min
Response: 0
Conc: N.D.

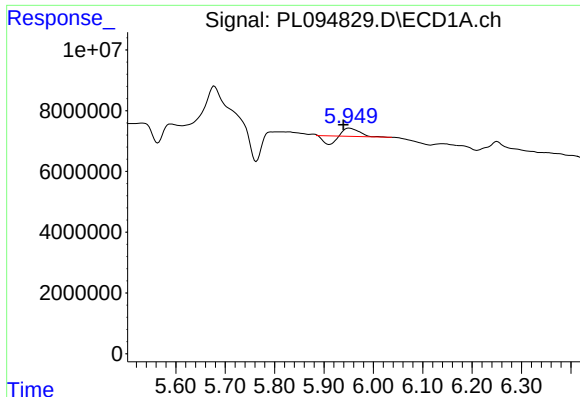

#25 Chlordane-3


R.T.: 5.951 min
Delta R.T.: 0.011 min
Response: 2115879
Conc: 4.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

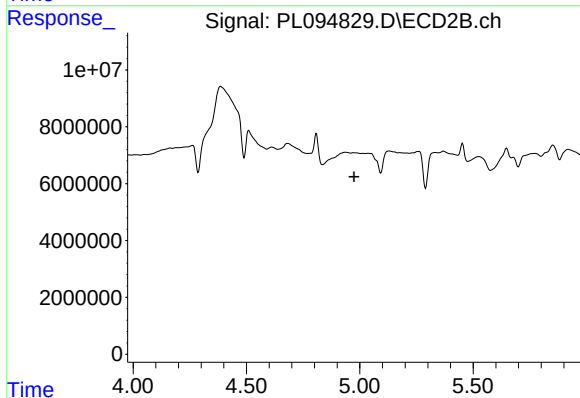


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

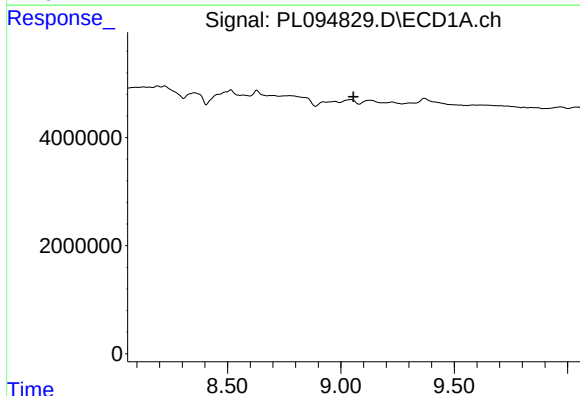

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.056 min
Response: 0
Conc: N.D.

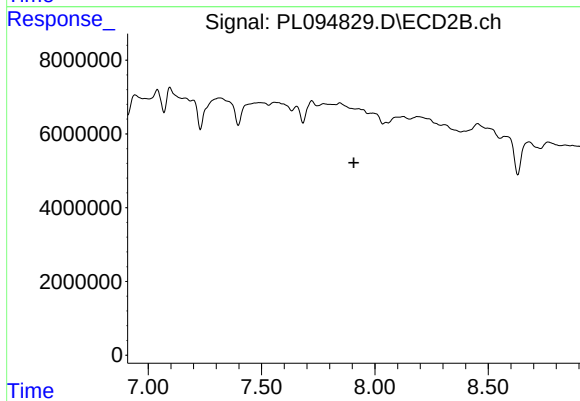

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.907 min
Response: 0
Conc: N.D.