

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032525\
 Data File : PL094847.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2025 18:09
 Operator : AR\AJ
 Sample : Q1634-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HR-04-032425

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 02:16:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.770	22439902	30184587	7.927	8.457
28)	SA Decachlor...	9.054	7.903	25525587	33894965	12.112	8.391 #
Target Compounds							
7)	B delta-BHC	4.760	0.000	6202331	0	1.593	N.D. #
10)	B gamma-Chl...	5.937	4.994f	8133135	4707488	2.414	0.975 #
11)	B alpha-Chl...	6.019	0.000	12370433	0	3.752	N.D. #
25)	Chlordane-3	5.937	4.994f	8133135	4707488	16.272	8.849 #
26)	Chlordane-4	6.019	0.000	12370433	0	20.999	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032525\
Data File : PL094847.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2025 18:09
Operator : AR\AJ
Sample : Q1634-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HR-04-032425

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 02:16:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

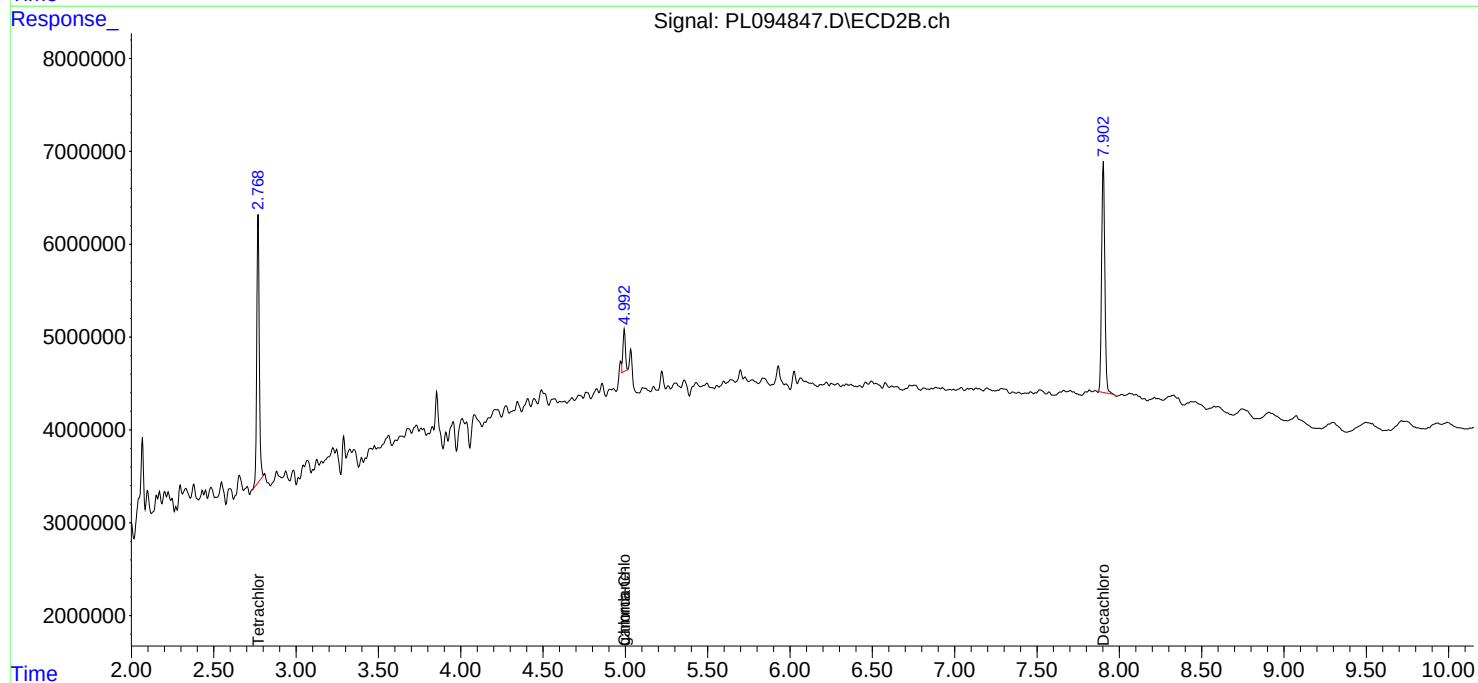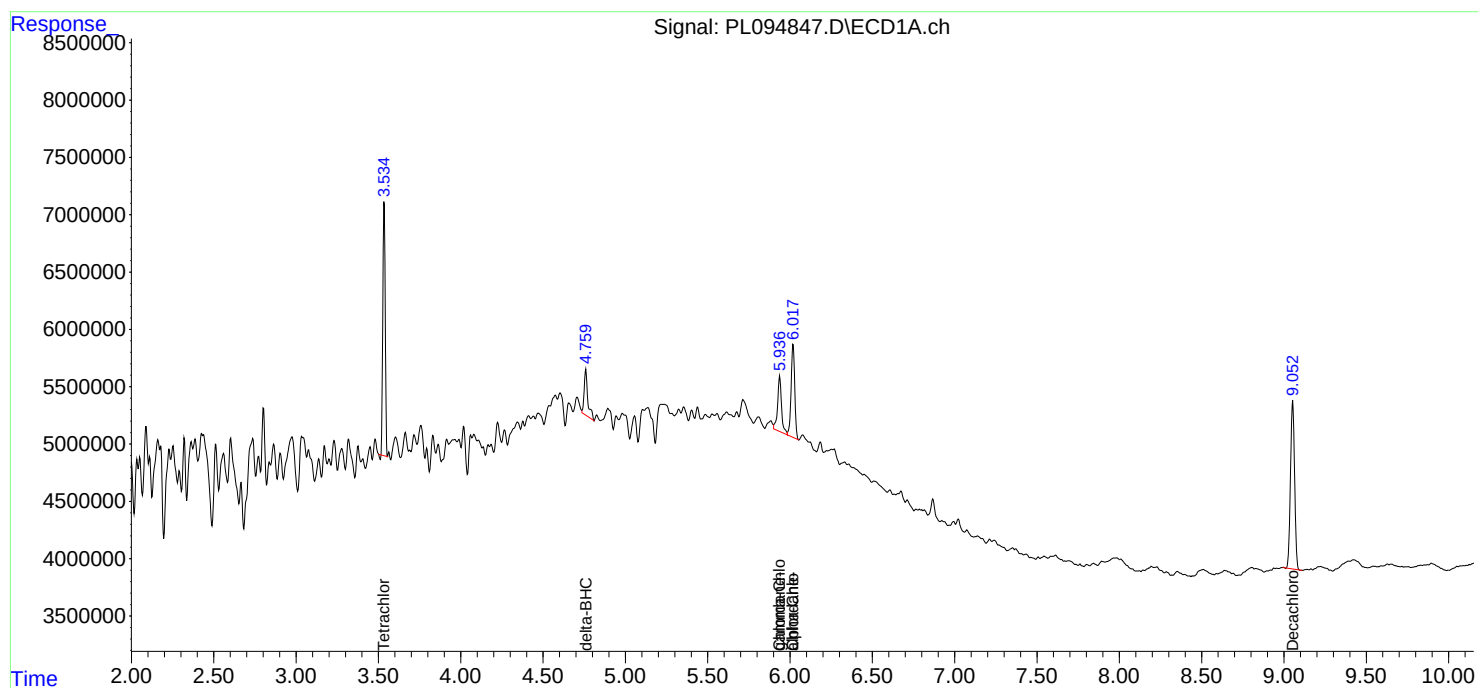


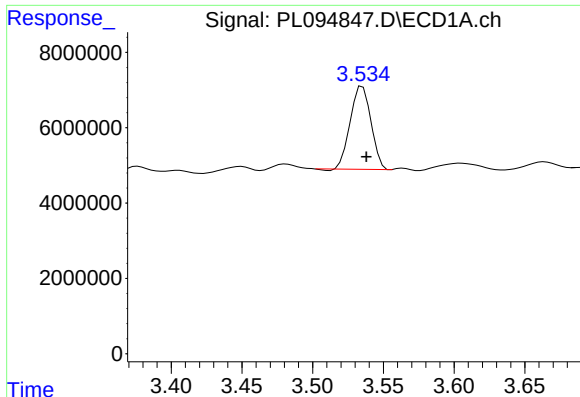

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 22439902
Conc: 7.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-04-032425

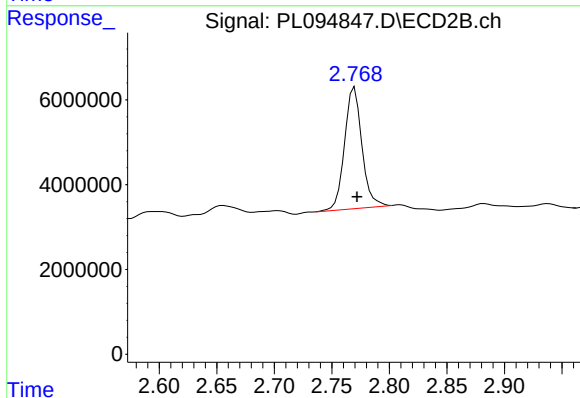


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.002 min
Response: 30184587
Conc: 8.46 ng/ml

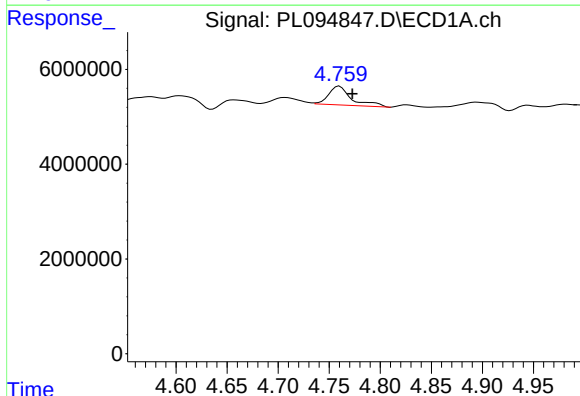


#7 delta-BHC

R.T.: 4.760 min
Delta R.T.: -0.013 min
Response: 6202331
Conc: 1.59 ng/ml

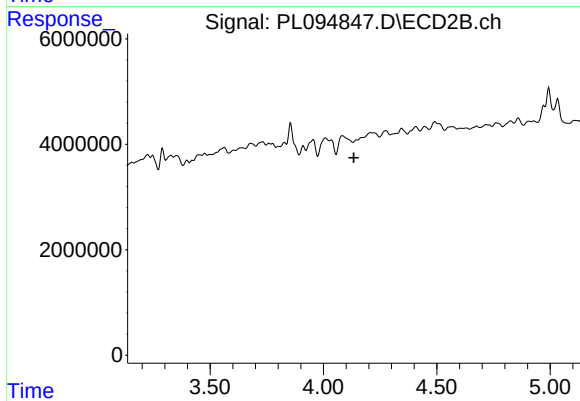

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

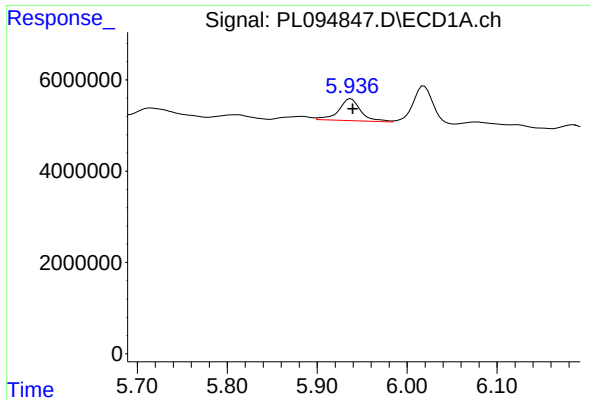

#10 gamma-Chlordane


R.T.: 5.937 min
Delta R.T.: -0.002 min
Response: 8133135
Conc: 2.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-04-032425

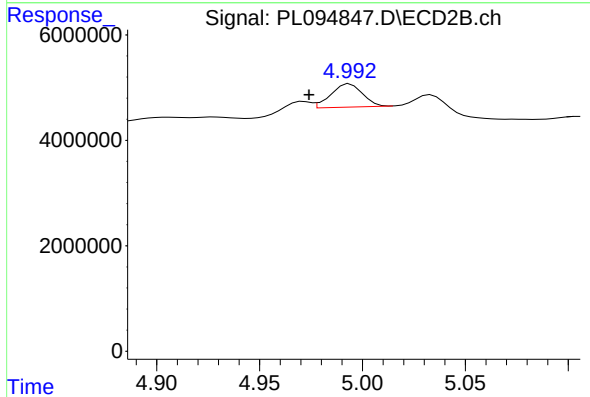


#10 gamma-Chlordane

R.T.: 4.994 min
Delta R.T.: 0.020 min
Response: 4707488
Conc: 0.97 ng/ml

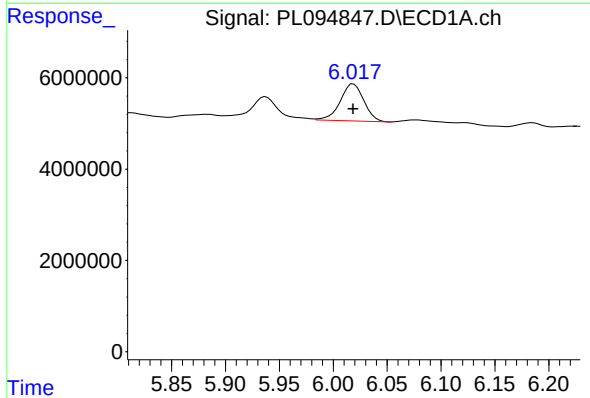


#11 alpha-Chlordane

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 12370433
Conc: 3.75 ng/ml

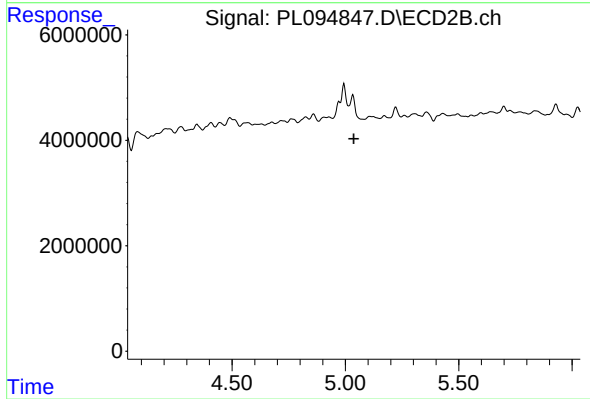

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.038 min
Response: 0
Conc: N.D.

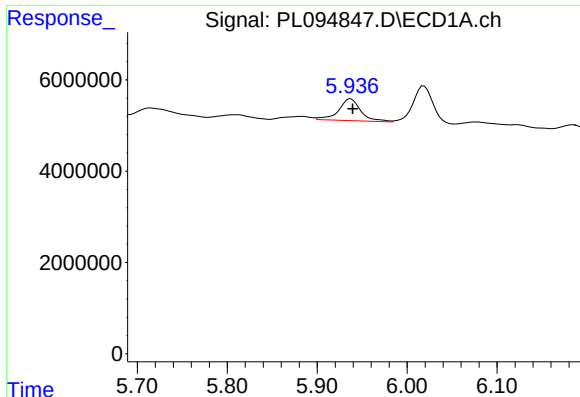

#25 Chlordane-3


R.T.: 5.937 min
Delta R.T.: -0.002 min
Response: 8133135
Conc: 16.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-04-032425

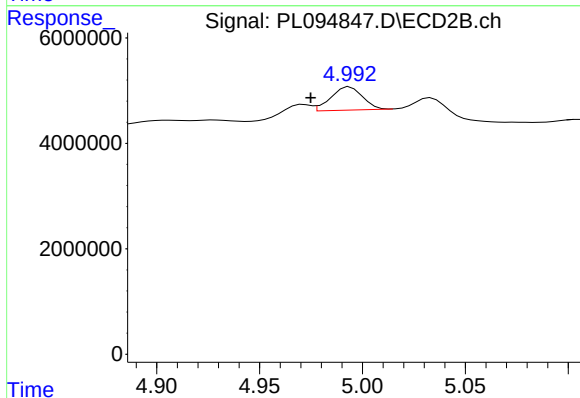


#25 Chlordane-3

R.T.: 4.994 min
Delta R.T.: 0.019 min
Response: 4707488
Conc: 8.85 ng/ml

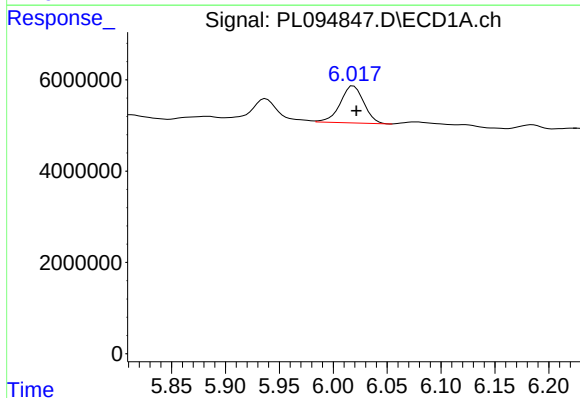


#26 Chlordane-4

R.T.: 6.019 min
Delta R.T.: -0.003 min
Response: 12370433
Conc: 21.00 ng/ml

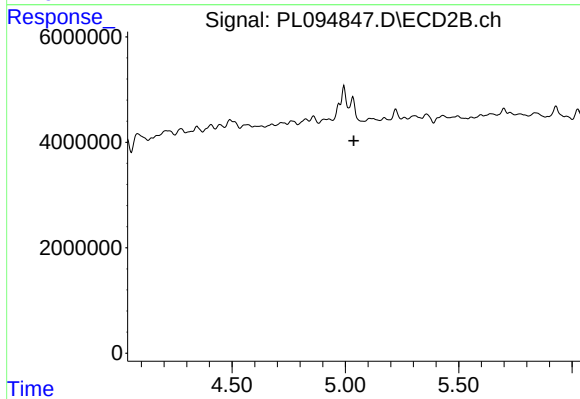

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.037 min
Response: 0
Conc: N.D.

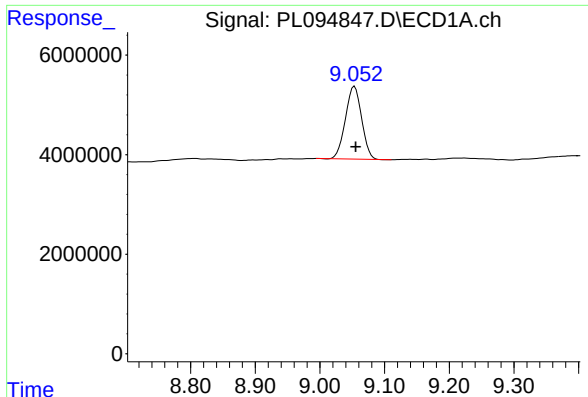

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.002 min
Response: 25525587
Conc: 12.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
HR-04-032425

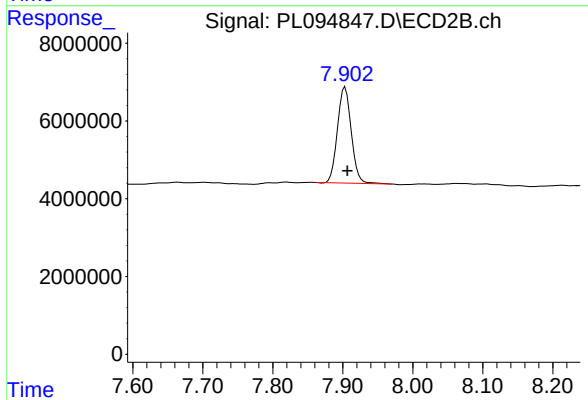

#28 Decachlorobiphenyl

R.T.: 7.903 min
Delta R.T.: -0.003 min
Response: 33894965
Conc: 8.39 ng/ml