

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032525\
 Data File : PL094856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2025 20:26
 Operator : AR\AJ
 Sample : Q1609-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-SCRN-01-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 02:19:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.770	55732042	75283878	19.689	21.092
28)	SA Decachlor...	9.050	7.902	49049366	87156628	23.274	21.577
Target Compounds							
3)	MA gamma-BHC...	0.000	3.612	0	25216785	N.D.	4.907 #
7)	B delta-BHC	4.762	0.000	38818314	0	9.968	N.D. #
9)	A Endosulfan I	0.000	5.123f	0	9468384	N.D.	2.157 #
10)	B gamma-Chl...	5.914f	0.000	8565192	0	2.542	N.D. #
13)	MA Dieldrin	0.000	5.345	0	393858	N.D.	0.081 #
15)	B Endosulfa...	0.000	5.917	0	7126282	N.D.	1.646 #
23)	Chlordane-1	0.000	3.764	0	6949105	N.D.	46.011 #
25)	Chlordane-3	5.914f	0.000	8565192	0	17.137	N.D. #
27)	Chlordane-5	0.000	5.917	0	7126282	N.D.	37.148 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032525\
Data File : PL094856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2025 20:26
Operator : AR\AJ
Sample : Q1609-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WC-SCRN-01-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 02:19:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

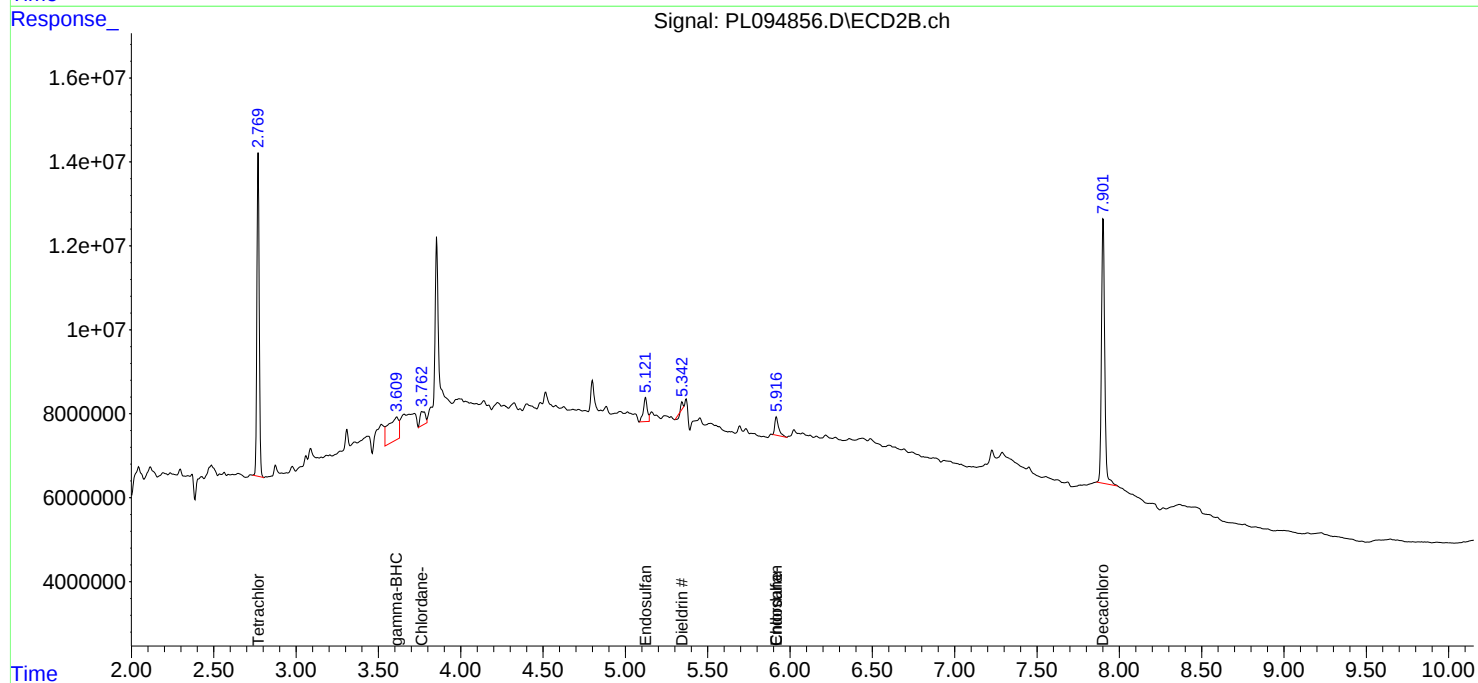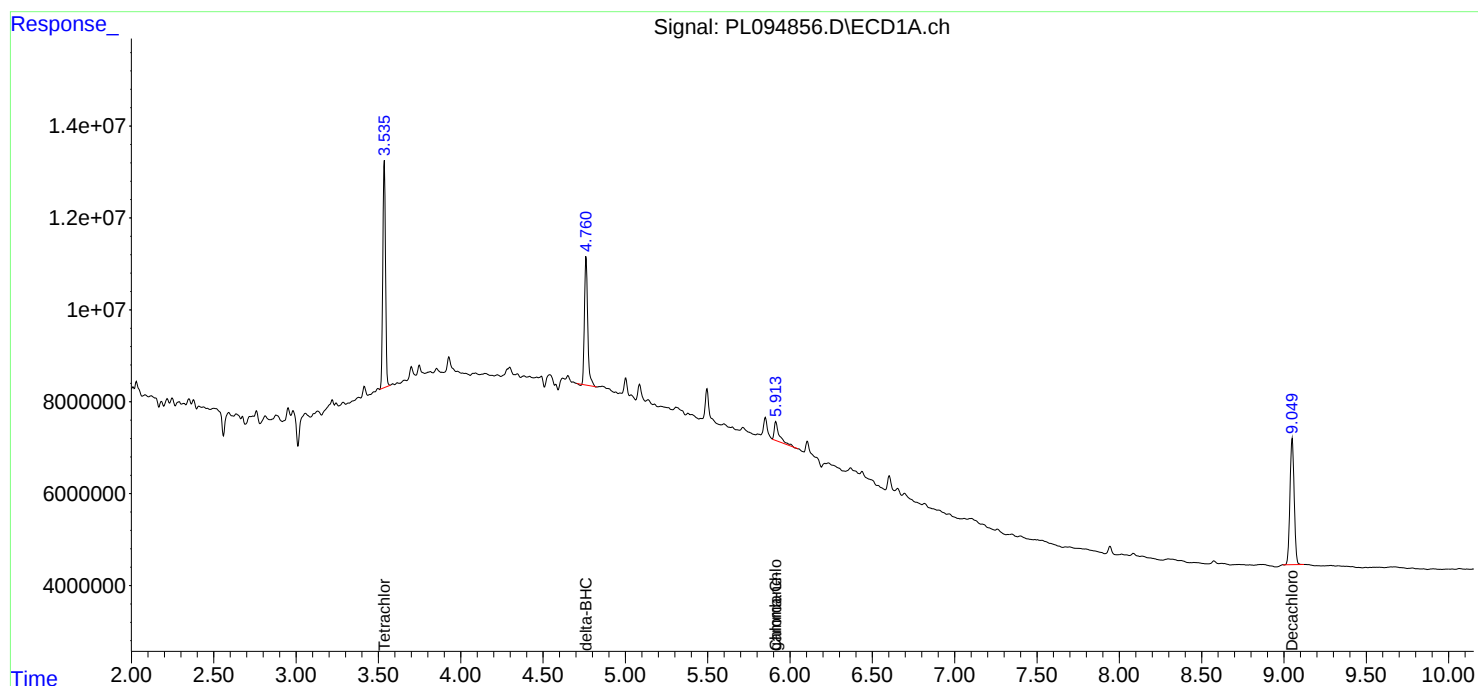


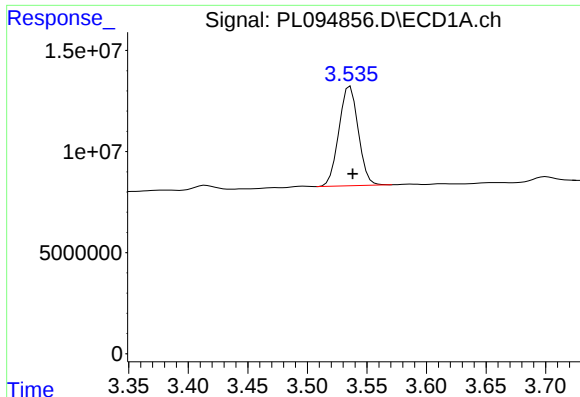

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 55732042
Conc: 19.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-SCRN-01-C

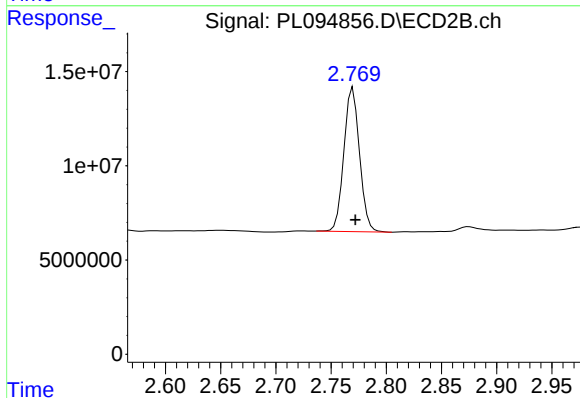


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.002 min
Response: 75283878
Conc: 21.09 ng/ml

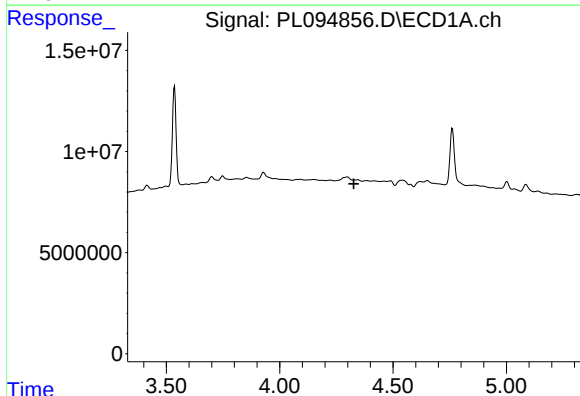


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.327 min
Response: 0
Conc: N.D.

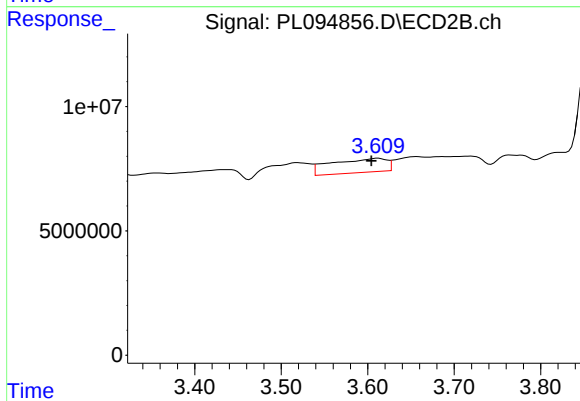

#3 gamma-BHC (Lindane)


R.T.: 3.612 min
Delta R.T.: 0.007 min
Response: 25216785
Conc: 4.91 ng/ml

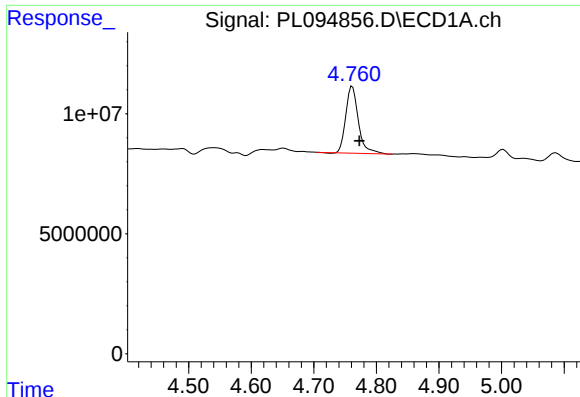

#7 delta-BHC


R.T.: 4.762 min
Delta R.T.: -0.011 min
Response: 38818314
Conc: 9.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-SCRN-01-C

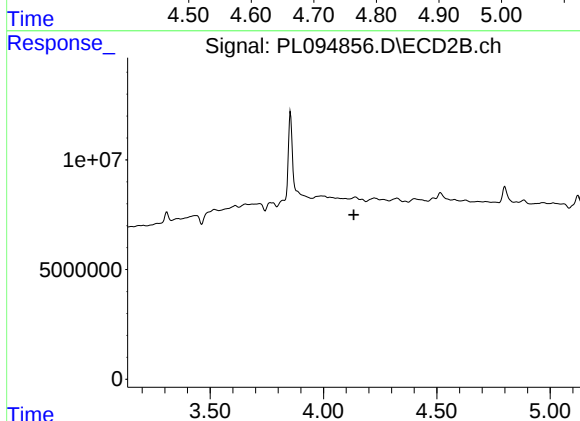


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

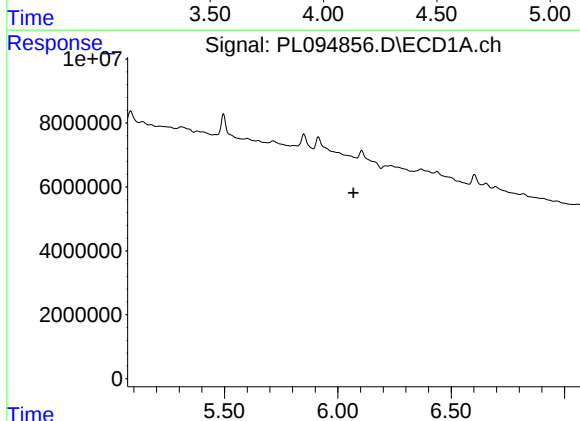


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.069 min
Response: 0
Conc: N.D.

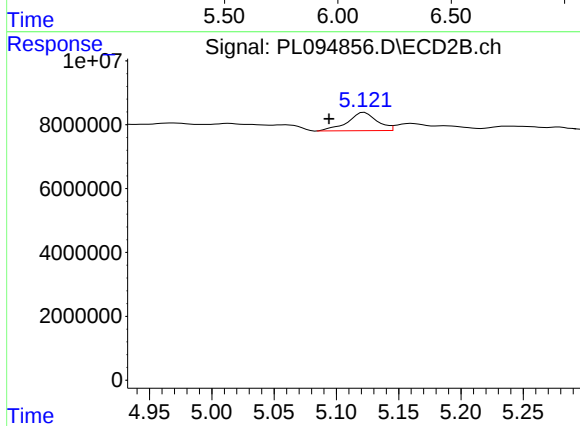

#9 Endosulfan I


R.T.: 5.123 min
Delta R.T.: 0.029 min
Response: 9468384
Conc: 2.16 ng/ml

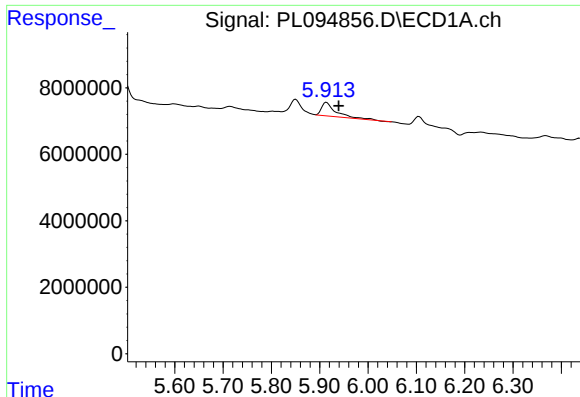

#10 gamma-Chlordane


R.T.: 5.914 min
Delta R.T.: -0.025 min
Response: 8565192
Conc: 2.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-SCRN-01-C

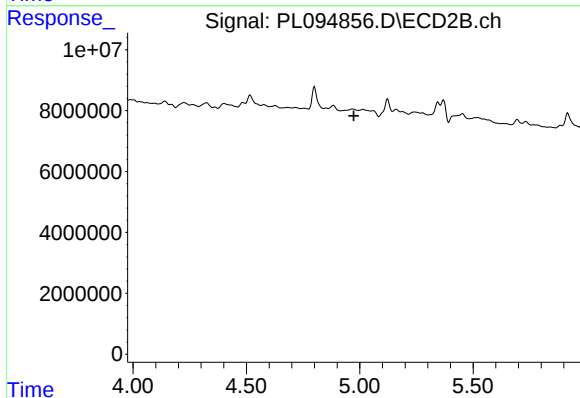


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

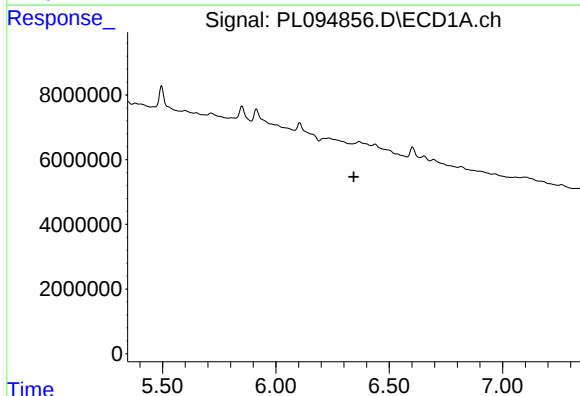


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

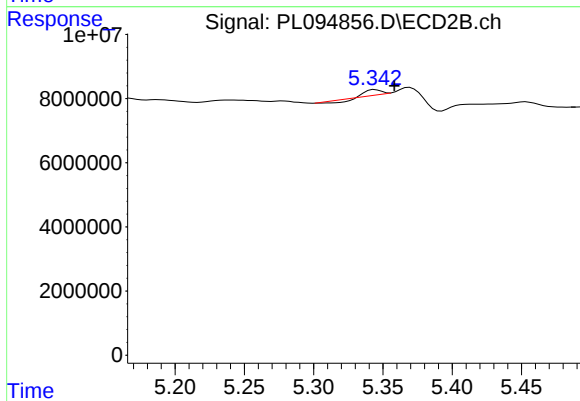

#13 Dieldrin


R.T.: 5.345 min
Delta R.T.: -0.014 min
Response: 393858
Conc: 0.08 ng/ml

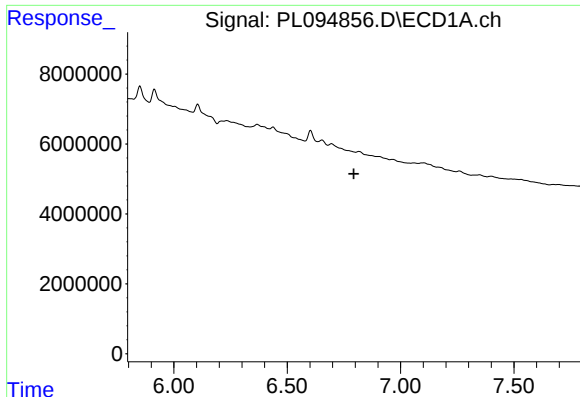

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WC-SCRN-01-C

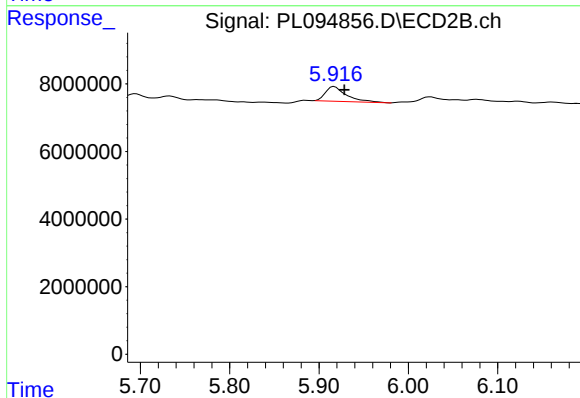


#15 Endosulfan II

R.T.: 5.917 min
Delta R.T.: -0.011 min
Response: 7126282
Conc: 1.65 ng/ml

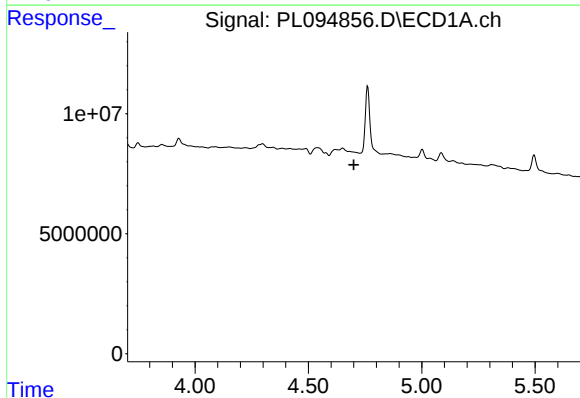


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.700 min
Response: 0
Conc: N.D.

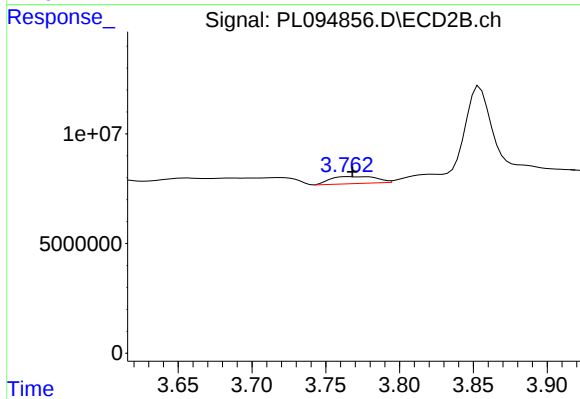

#23 Chlordane-1


R.T.: 3.764 min
Delta R.T.: -0.004 min
Response: 6949105
Conc: 46.01 ng/ml

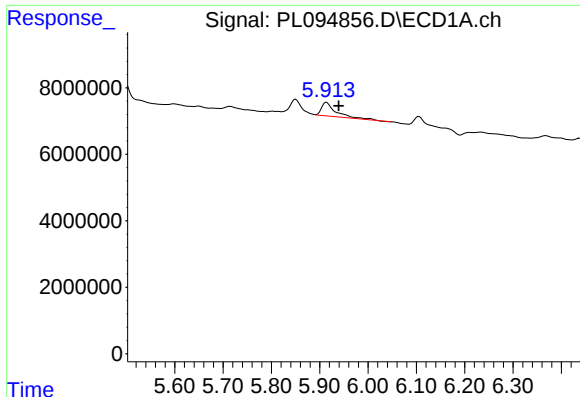

#25 Chlordane-3


R.T.: 5.914 min
Delta R.T.: -0.026 min
Response: 8565192
Conc: 17.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-SCRN-01-C

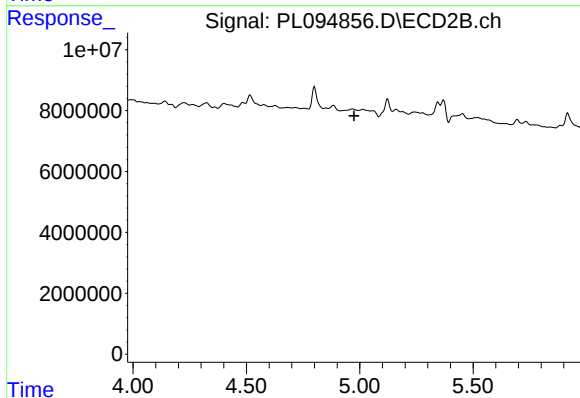


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

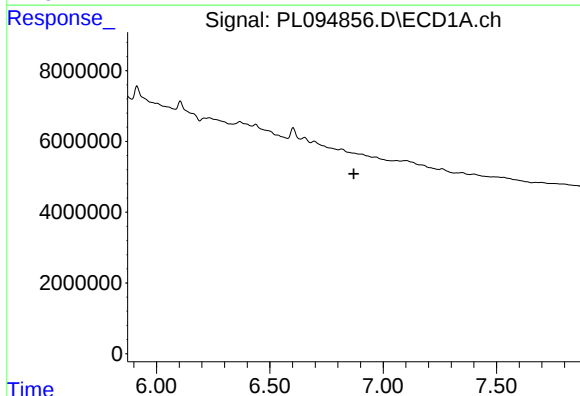


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.871 min
Response: 0
Conc: N.D.

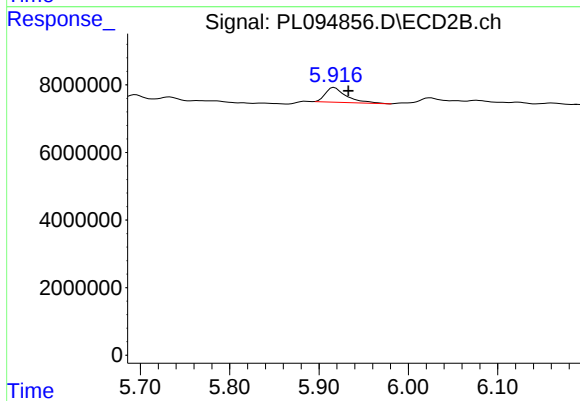

#27 Chlordane-5


R.T.: 5.917 min
Delta R.T.: -0.016 min
Response: 7126282
Conc: 37.15 ng/ml

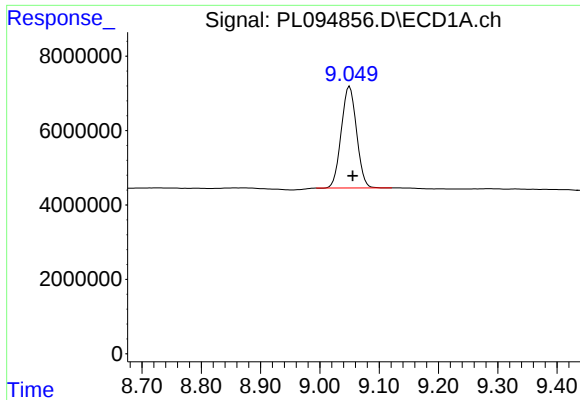

#28 Decachlorobiphenyl

R.T.: 9.050 min
Delta R.T.: -0.005 min
Response: 49049366
Conc: 23.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-SCRN-01-C

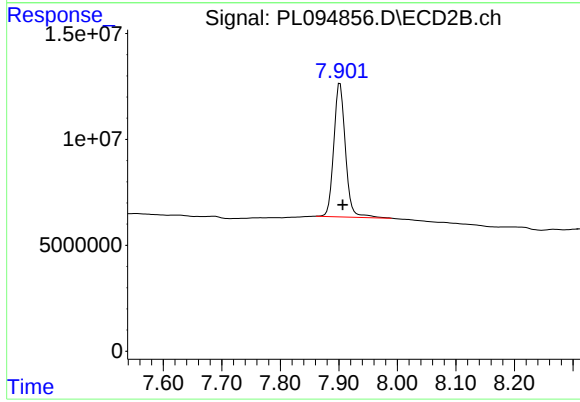

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.005 min
Response: 87156628
Conc: 21.58 ng/ml