

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
 Data File : PL046504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 21:52
 Operator : AJ\SJ
 Sample : K1693-13
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-01-032519-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:10:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	78963063	25842002	10.855	11.287
28)	SA Decachlor...	8.035	9.028	90098963	30013942	10.712	12.946
Target Compounds							
2)	A alpha-BHC	3.797	0.000	4420871	0	0.379	N.D. #
10)	B gamma-Chl...	5.253	6.081	9804406	5276995	0.954	1.859 #
11)	B alpha-Chl...	5.308	6.155	16602439	8097586	1.637	2.855 #
12)	B 4,4'-DDE	5.474	6.309	7073068	3279165	0.768	1.321 #
16)	A 4,4'-DDD	0.000	6.803	0	1481247	N.D.	0.736 #
24)	Chlordane-2	0.000	5.434	0	2779192	N.D.	23.793 #
25)	Chlordane-3	5.253	6.081	9804406	5276995	8.804	13.841 #
26)	Chlordane-4	5.308	6.155	16602439	8097586	16.056	17.549



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
Data File : PL046504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 21:52
Operator : AJ\SJ
Sample : K1693-13
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:10:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

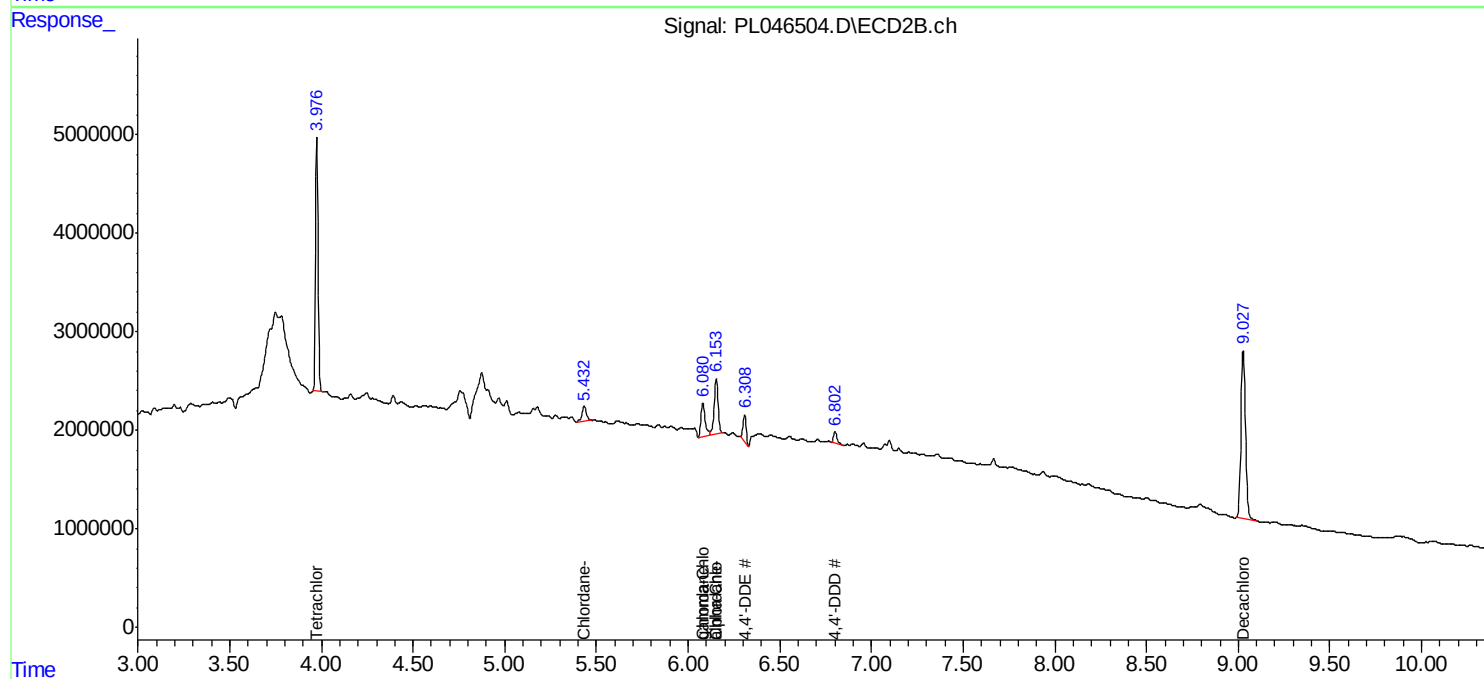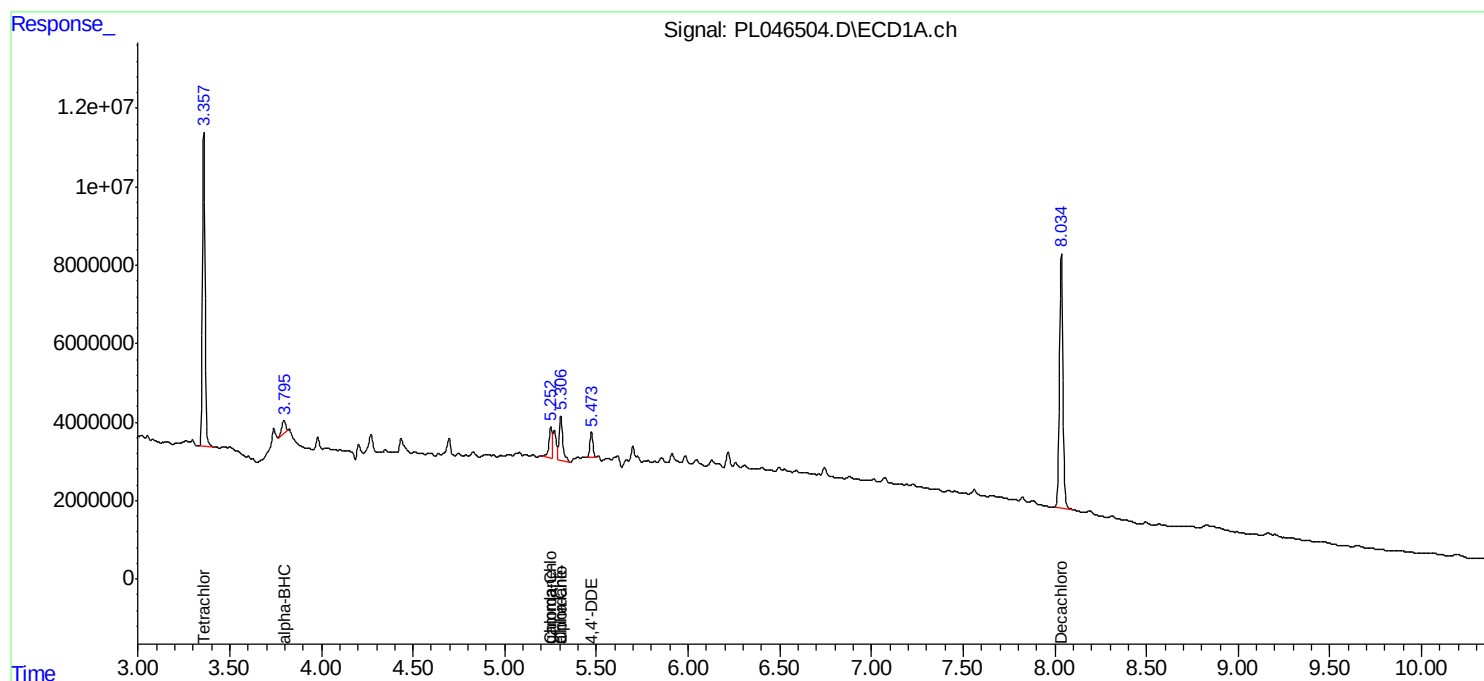


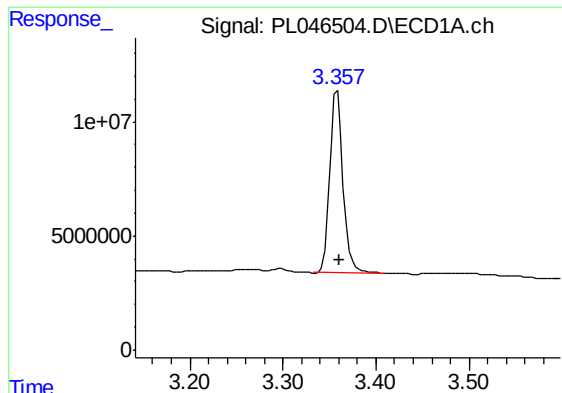

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 78963063
Conc: 10.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-A

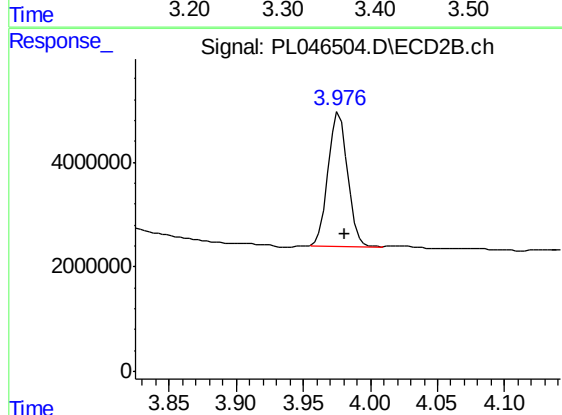


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 25842002
Conc: 11.29 ng/ml

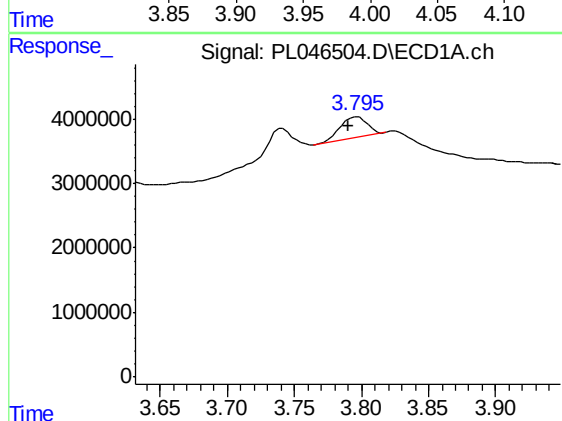


#2 alpha-BHC

R.T.: 3.797 min
Delta R.T.: 0.006 min
Response: 4420871
Conc: 0.38 ng/ml

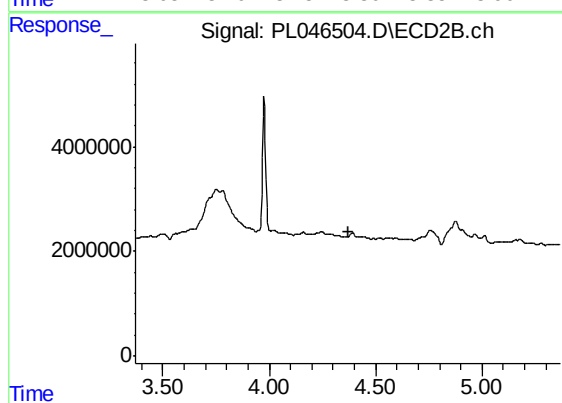

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

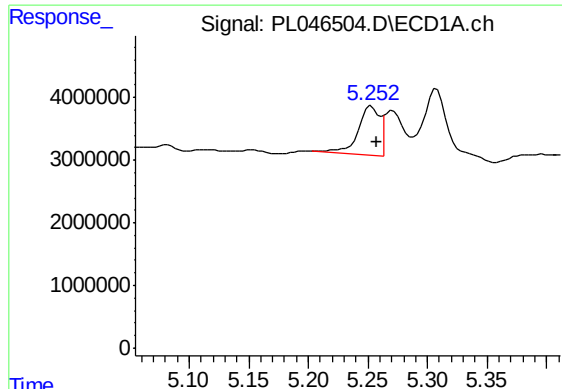

#10 gamma-Chlordane


R.T.: 5.253 min
Delta R.T.: -0.004 min
Response: 9804406
Conc: 0.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-A

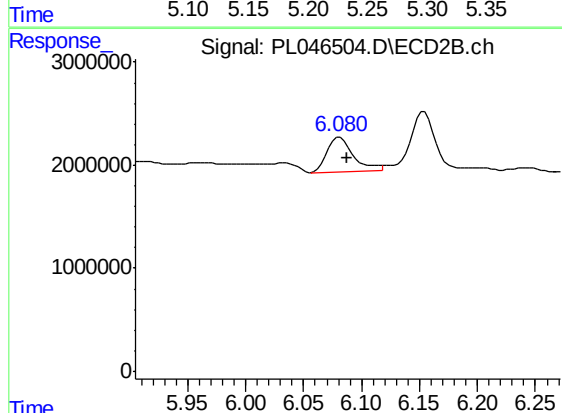


#10 gamma-Chlordane

R.T.: 6.081 min
Delta R.T.: -0.007 min
Response: 5276995
Conc: 1.86 ng/ml

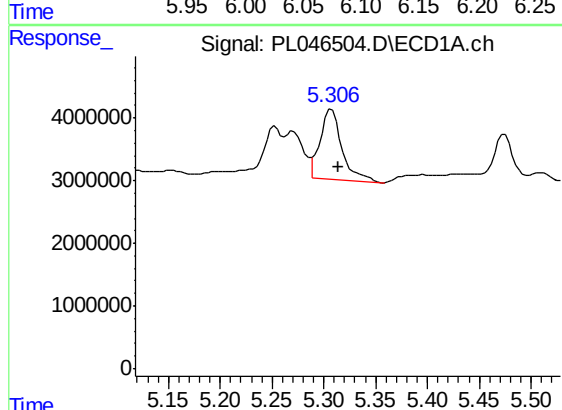


#11 alpha-Chlordane

R.T.: 5.308 min
Delta R.T.: -0.006 min
Response: 16602439
Conc: 1.64 ng/ml

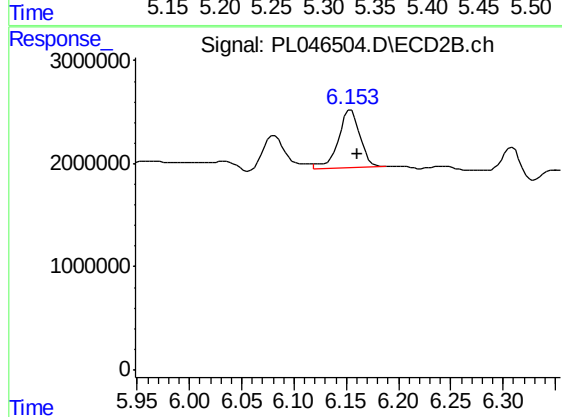

#11 alpha-Chlordane


R.T.: 6.155 min
Delta R.T.: -0.006 min
Response: 8097586
Conc: 2.85 ng/ml

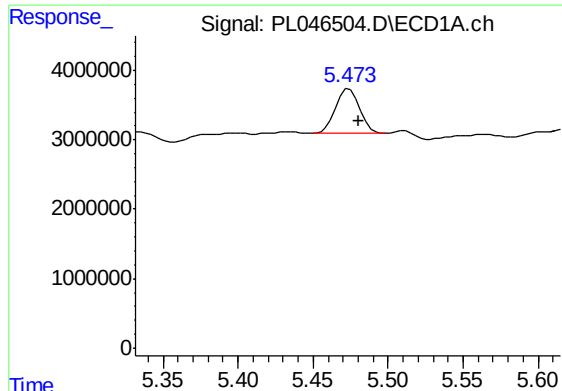

#12 4,4'-DDE


R.T.: 5.474 min
Delta R.T.: -0.007 min
Response: 7073068
Conc: 0.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-A

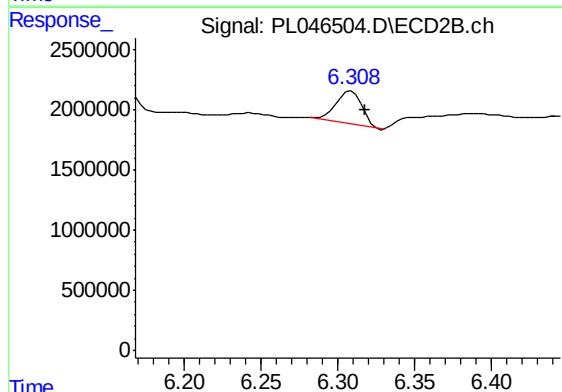


#12 4,4'-DDE

R.T.: 6.309 min
Delta R.T.: -0.009 min
Response: 3279165
Conc: 1.32 ng/ml

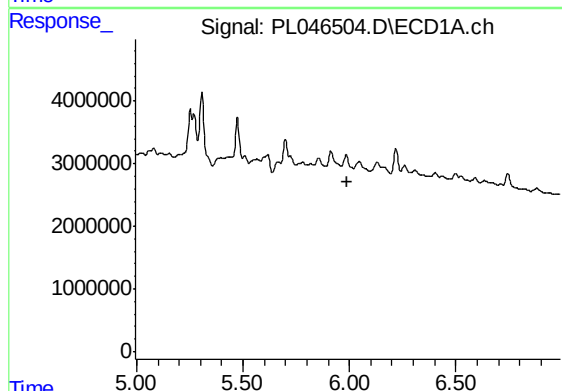


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.993 min
Response: 0
Conc: N.D.

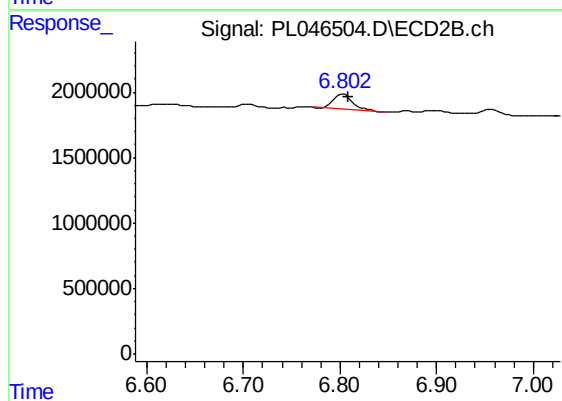

#16 4,4'-DDD


R.T.: 6.803 min
Delta R.T.: -0.005 min
Response: 1481247
Conc: 0.74 ng/ml

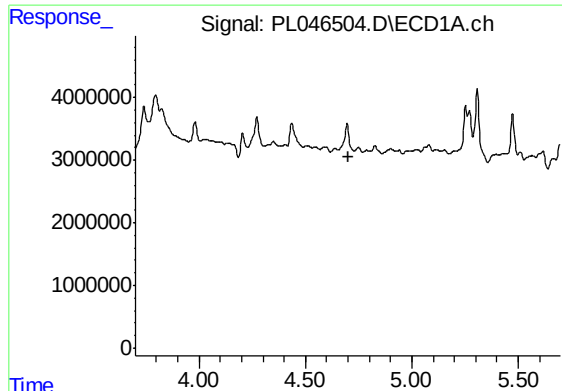

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.701 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-A

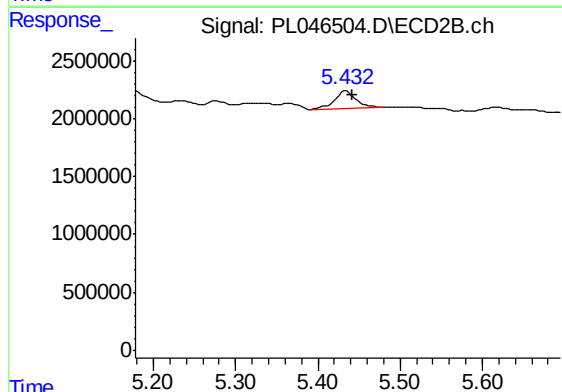


#24 Chlordane-2

R.T.: 5.434 min
Delta R.T.: -0.009 min
Response: 2779192
Conc: 23.79 ng/ml

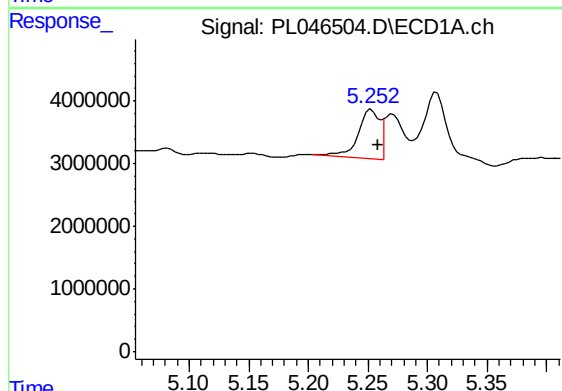


#25 Chlordane-3

R.T.: 5.253 min
Delta R.T.: -0.005 min
Response: 9804406
Conc: 8.80 ng/ml

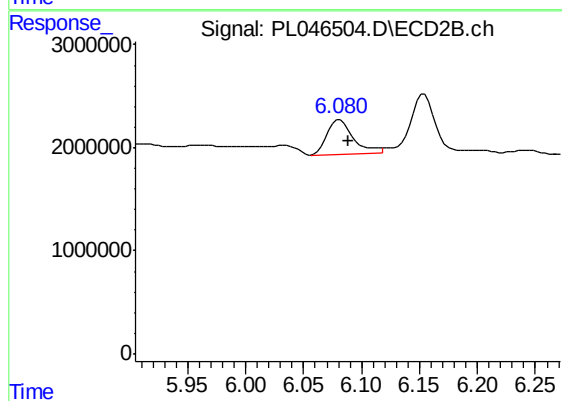

#25 Chlordane-3


R.T.: 6.081 min
Delta R.T.: -0.008 min
Response: 5276995
Conc: 13.84 ng/ml

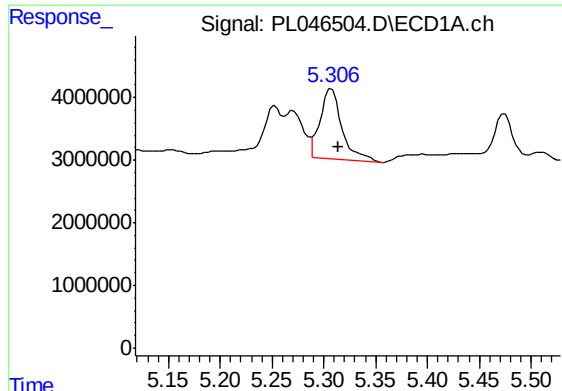

#26 Chlordane-4


R.T.: 5.308 min
Delta R.T.: -0.007 min
Response: 16602439
Conc: 16.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-A

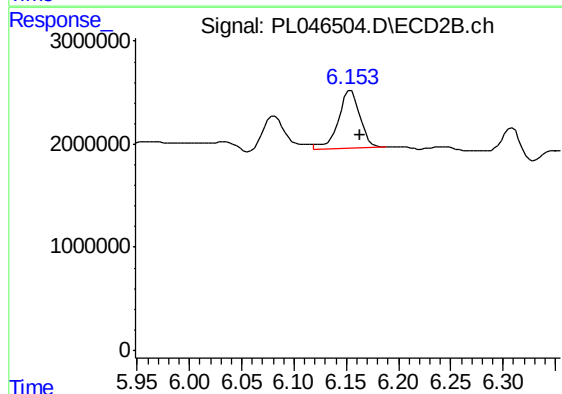


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: -0.009 min
Response: 8097586
Conc: 17.55 ng/ml

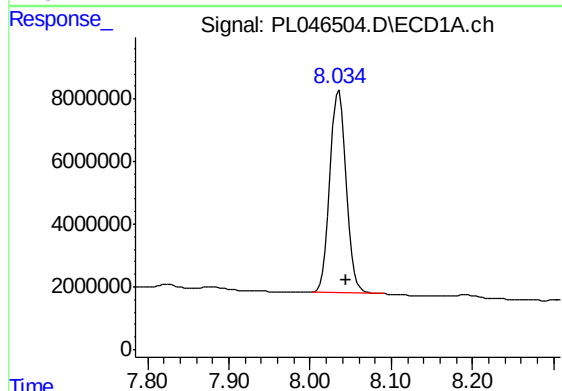

#28 Decachlorobiphenyl

R.T.: 8.035 min
Delta R.T.: -0.009 min
Response: 90098963
Conc: 10.71 ng/ml

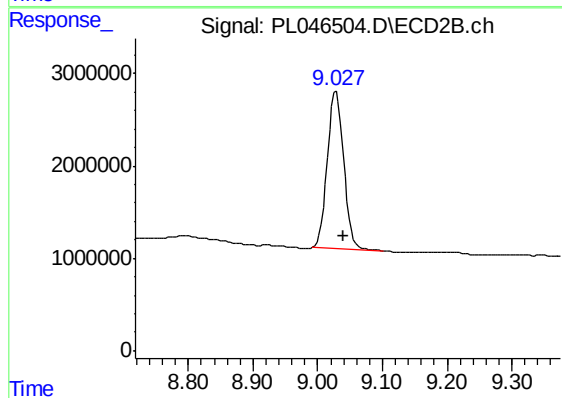

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.011 min
Response: 30013942
Conc: 12.95 ng/ml