

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
 Data File : PL046505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 22:06
 Operator : AJ\SJ
 Sample : K1693-15
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-01-032519-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:10:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.358	3.977	76989436	24323949	10.583	10.624
28)	SA Decachlor...	8.034	9.028	83984501	27572927	9.985	11.893
Target Compounds							
6)	B beta-BHC	0.000	4.847f	0	1400611	N.D.	1.057 #
10)	B gamma-Chl...	0.000	6.083	0	4065949	N.D.	1.433 #
11)	B alpha-Chl...	0.000	6.155	0	4541960	N.D.	1.601 #
12)	B 4,4'-DDE	5.474	6.308	9149253	3377015	0.994	1.360 #
17)	MA 4,4'-DDT	6.220	7.099	8333823	2947379	1.100	1.406 #
24)	Chlordane-2	0.000	5.435	0	2746178	N.D.	23.510 #
25)	Chlordane-3	0.000	6.083	0	4065949	N.D.	10.664 #
26)	Chlordane-4	0.000	6.155	0	4541960	N.D.	9.843 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
Data File : PL046505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 22:06
Operator : AJ\SJ
Sample : K1693-15
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:10:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

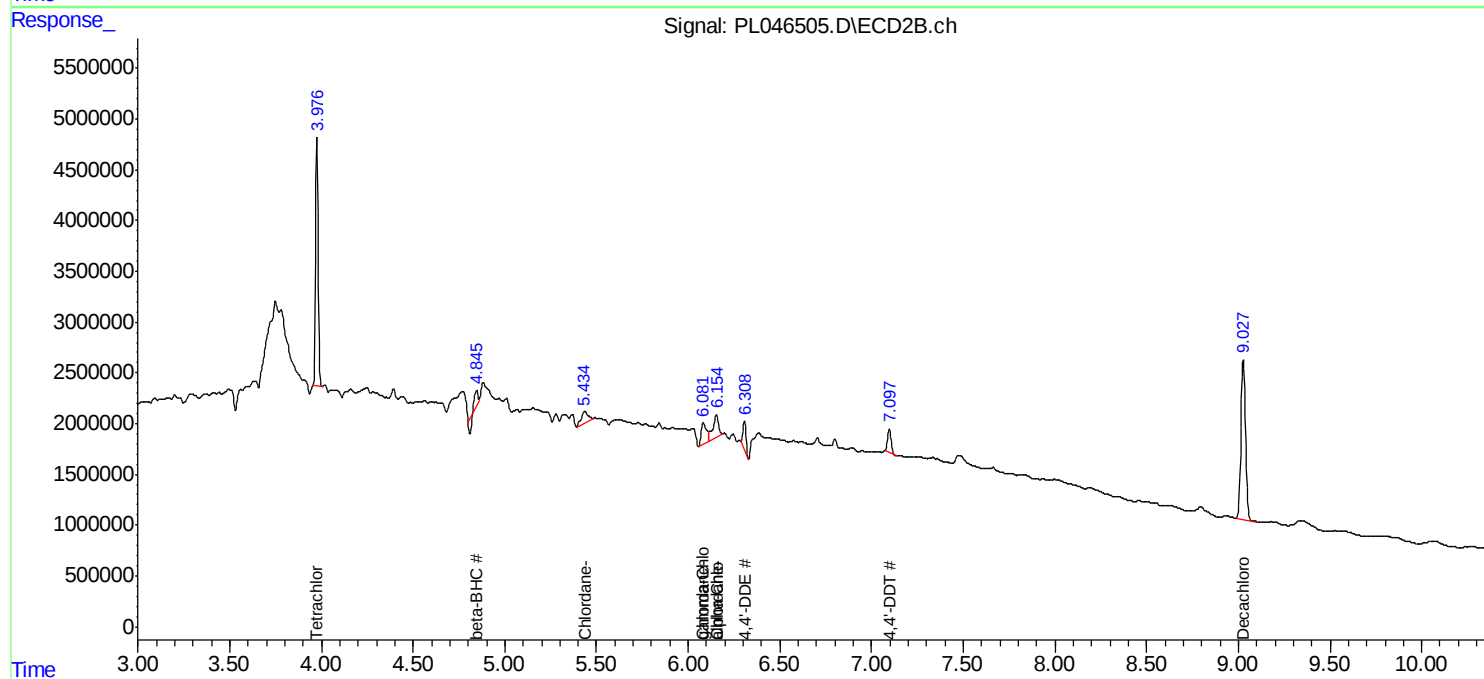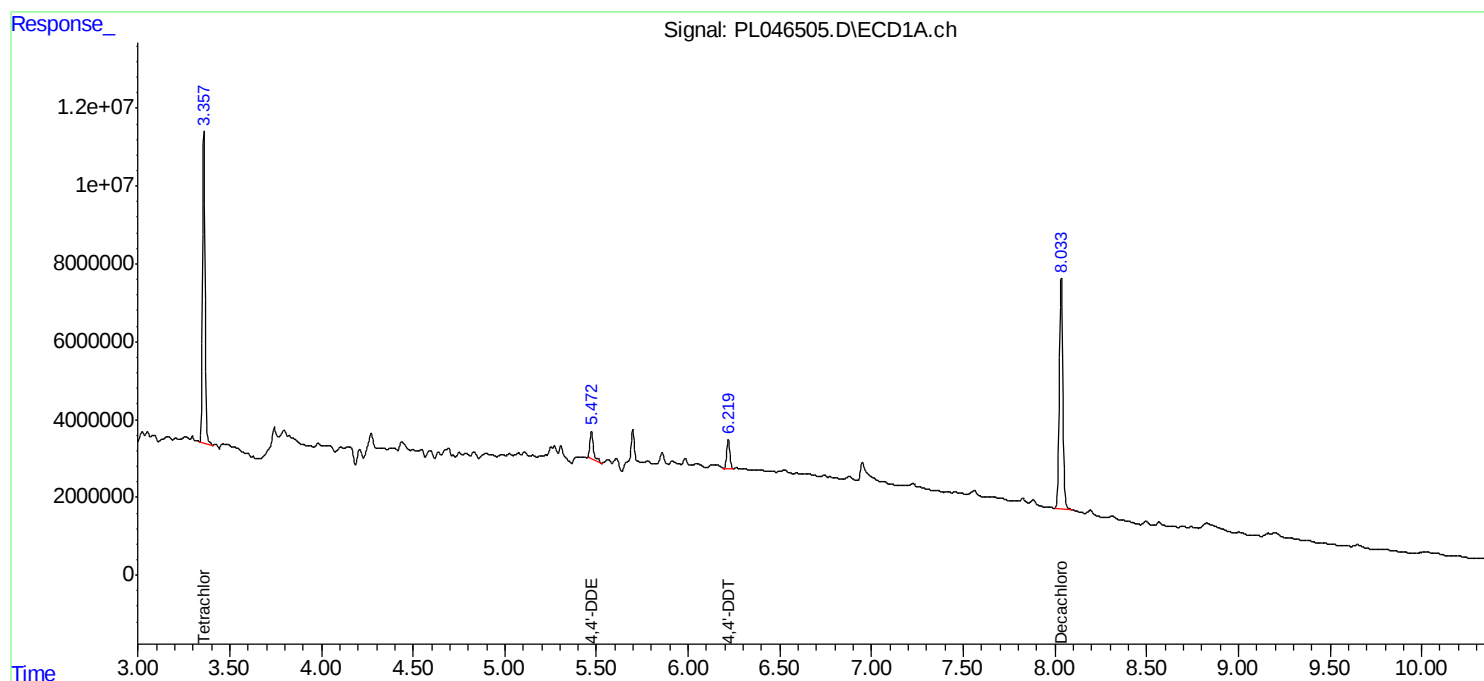


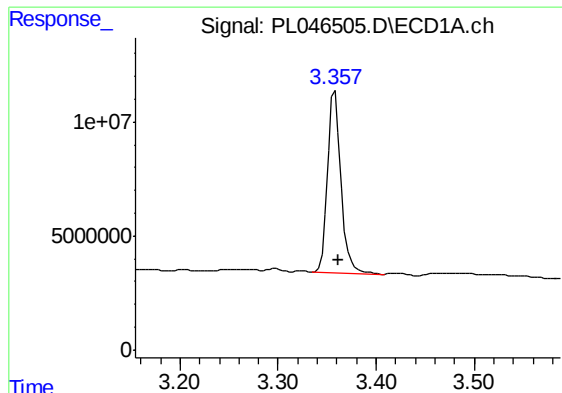

#1 Tetrachloro-m-xylene


R.T.: 3.358 min
Delta R.T.: -0.003 min
Response: 76989436
Conc: 10.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

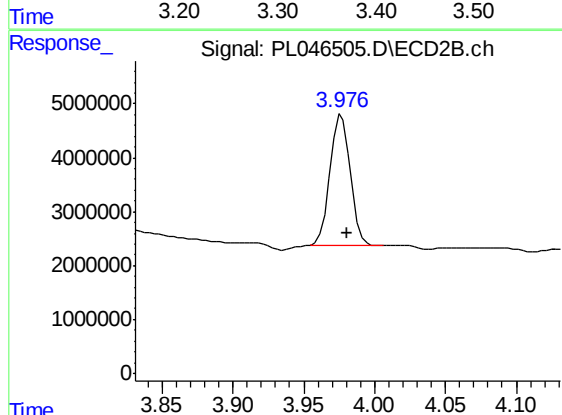


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.004 min
Response: 24323949
Conc: 10.62 ng/ml

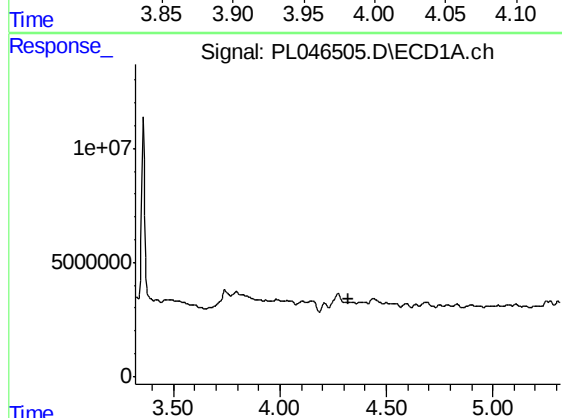


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.321 min
Response: 0
Conc: N.D.

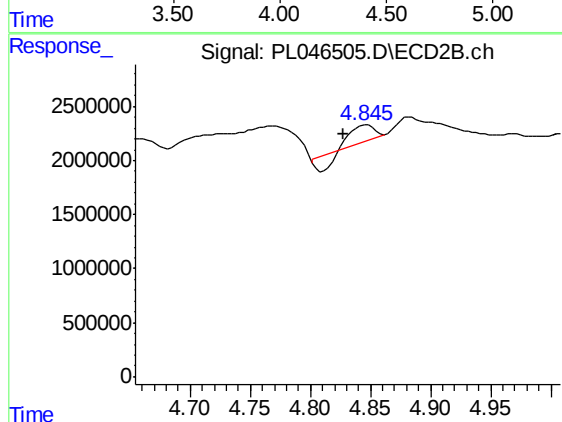

#6 beta-BHC


R.T.: 4.847 min
Delta R.T.: 0.020 min
Response: 1400611
Conc: 1.06 ng/ml

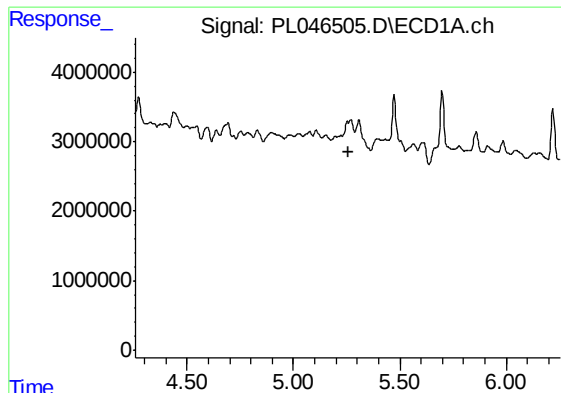

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.257 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

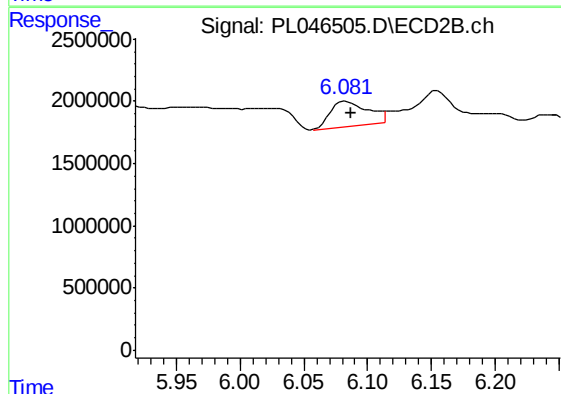


#10 gamma-Chlordane

R.T.: 6.083 min
Delta R.T.: -0.005 min
Response: 4065949
Conc: 1.43 ng/ml

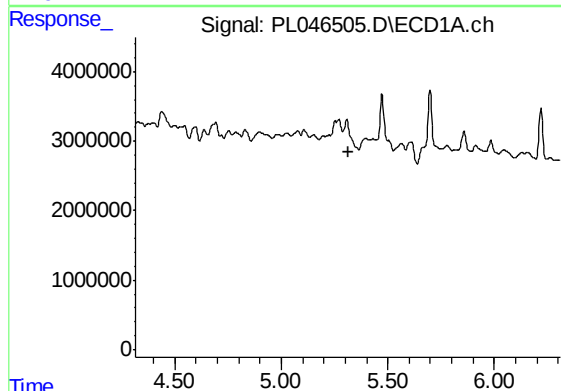


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

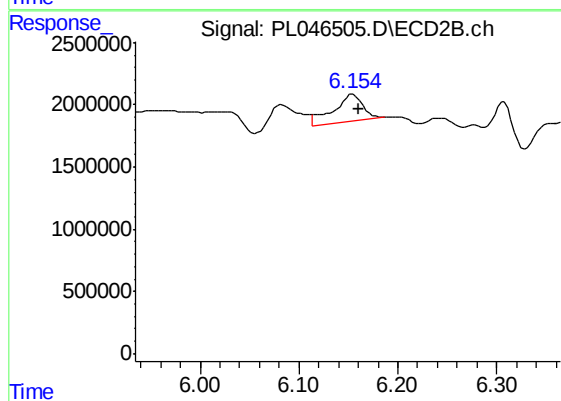

#11 alpha-Chlordane


R.T.: 6.155 min
Delta R.T.: -0.005 min
Response: 4541960
Conc: 1.60 ng/ml

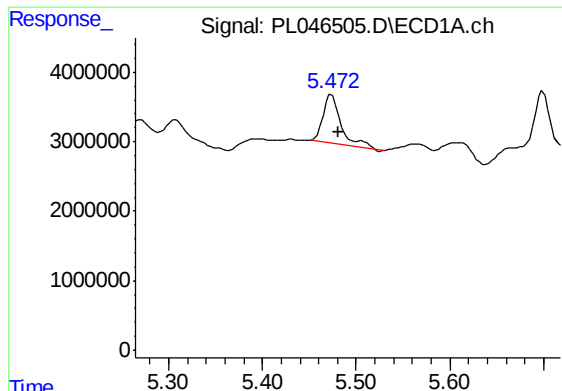

#12 4,4'-DDE


R.T.: 5.474 min
Delta R.T.: -0.007 min
Response: 9149253
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

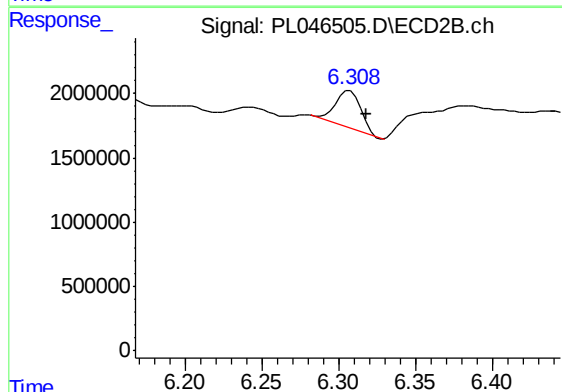


#12 4,4'-DDE

R.T.: 6.308 min
Delta R.T.: -0.010 min
Response: 3377015
Conc: 1.36 ng/ml

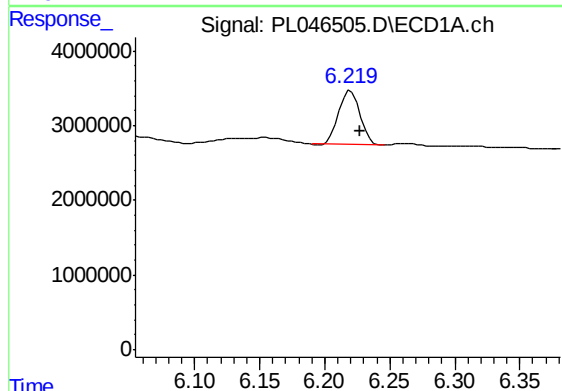


#17 4,4'-DDT

R.T.: 6.220 min
Delta R.T.: -0.008 min
Response: 8333823
Conc: 1.10 ng/ml

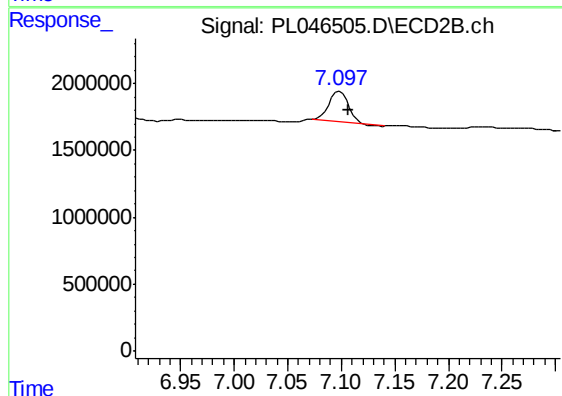

#17 4,4'-DDT


R.T.: 7.099 min
Delta R.T.: -0.008 min
Response: 2947379
Conc: 1.41 ng/ml

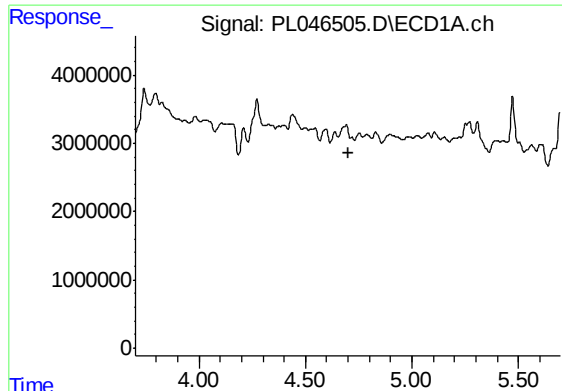

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.701 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

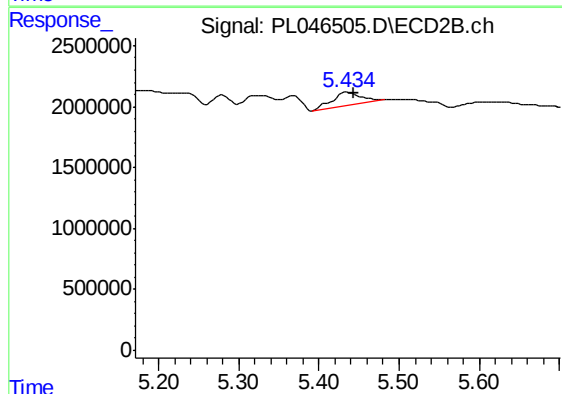


#24 Chlordane-2

R.T.: 5.435 min
Delta R.T.: -0.008 min
Response: 2746178
Conc: 23.51 ng/ml

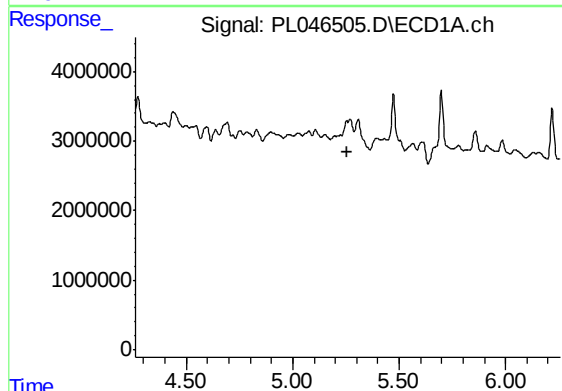


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.258 min
Response: 0
Conc: N.D.

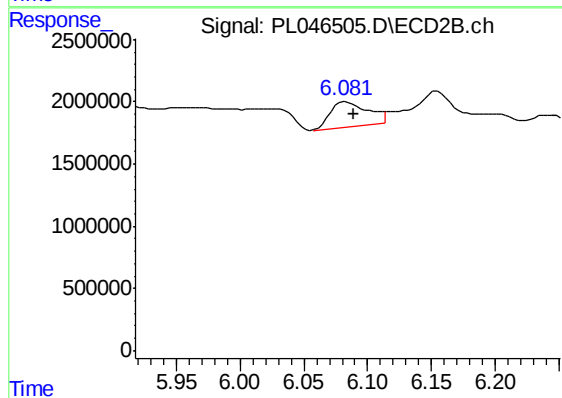

#25 Chlordane-3


R.T.: 6.083 min
Delta R.T.: -0.006 min
Response: 4065949
Conc: 10.66 ng/ml

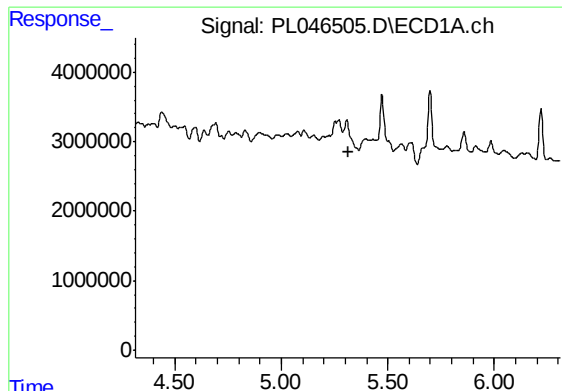

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-01-032519-B

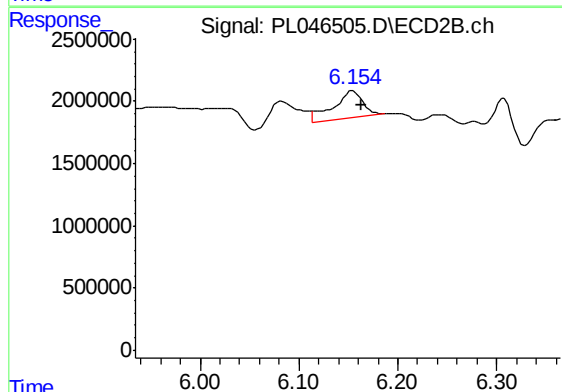


#26 Chlordane-4

R.T.: 6.155 min
Delta R.T.: -0.008 min
Response: 4541960
Conc: 9.84 ng/ml

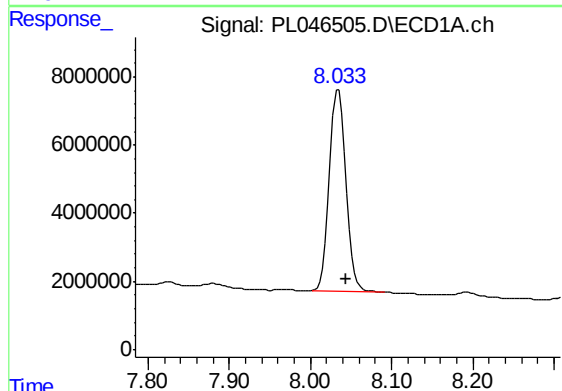

#28 Decachlorobiphenyl

R.T.: 8.034 min
Delta R.T.: -0.010 min
Response: 83984501
Conc: 9.99 ng/ml

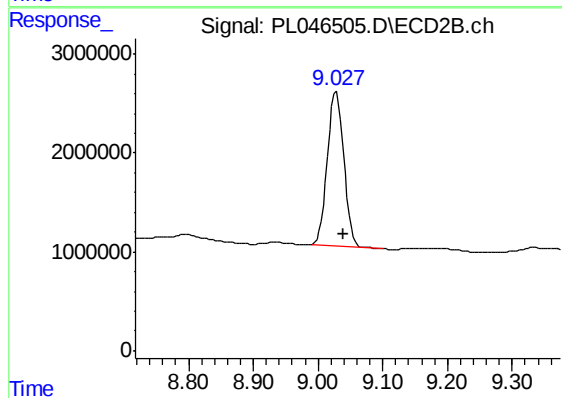

#28 Decachlorobiphenyl

R.T.: 9.028 min
Delta R.T.: -0.012 min
Response: 27572927
Conc: 11.89 ng/ml