

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
 Data File : PL046466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 11:56
 Operator : AJ\SJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:04:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.359	3.978	385.6E6	114.6E6	53.007	50.068
28)	SA Decachlor...	8.037	9.032	398.8E6	111.1E6	47.411	47.926
Target Compounds							
23)	Chlordane-1	4.205	4.970	167.2E6	53016376	497.242	489.908
24)	Chlordane-2	4.697	5.438	182.6E6	56859138	481.193	486.769
25)	Chlordane-3	5.254	6.083	548.3E6	188.5E6	492.358	494.466
26)	Chlordane-4	5.310	6.157	505.2E6	225.6E6	488.553	488.998
27)	Chlordane-5	6.135	6.960	161.5E6	41195795	473.279	458.558



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
Data File : PL046466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 11:56
Operator : AJ\SJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:04:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

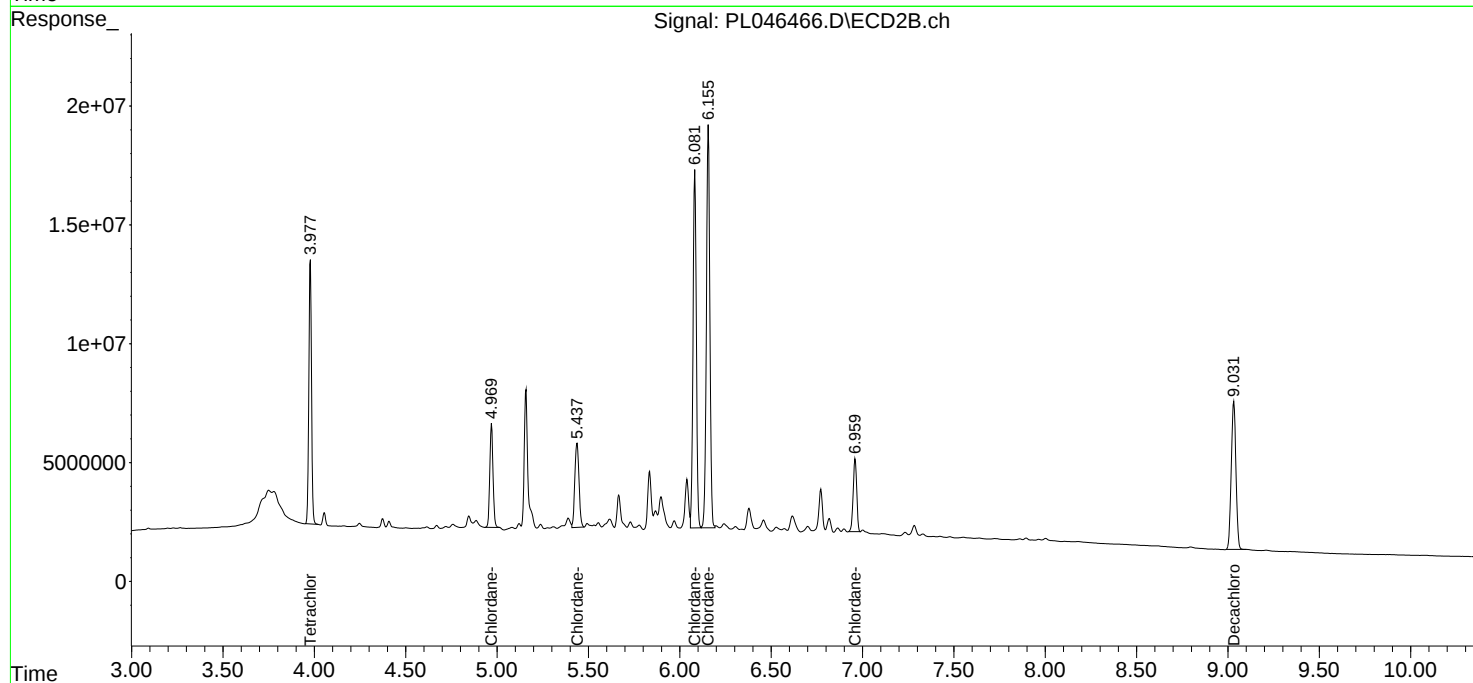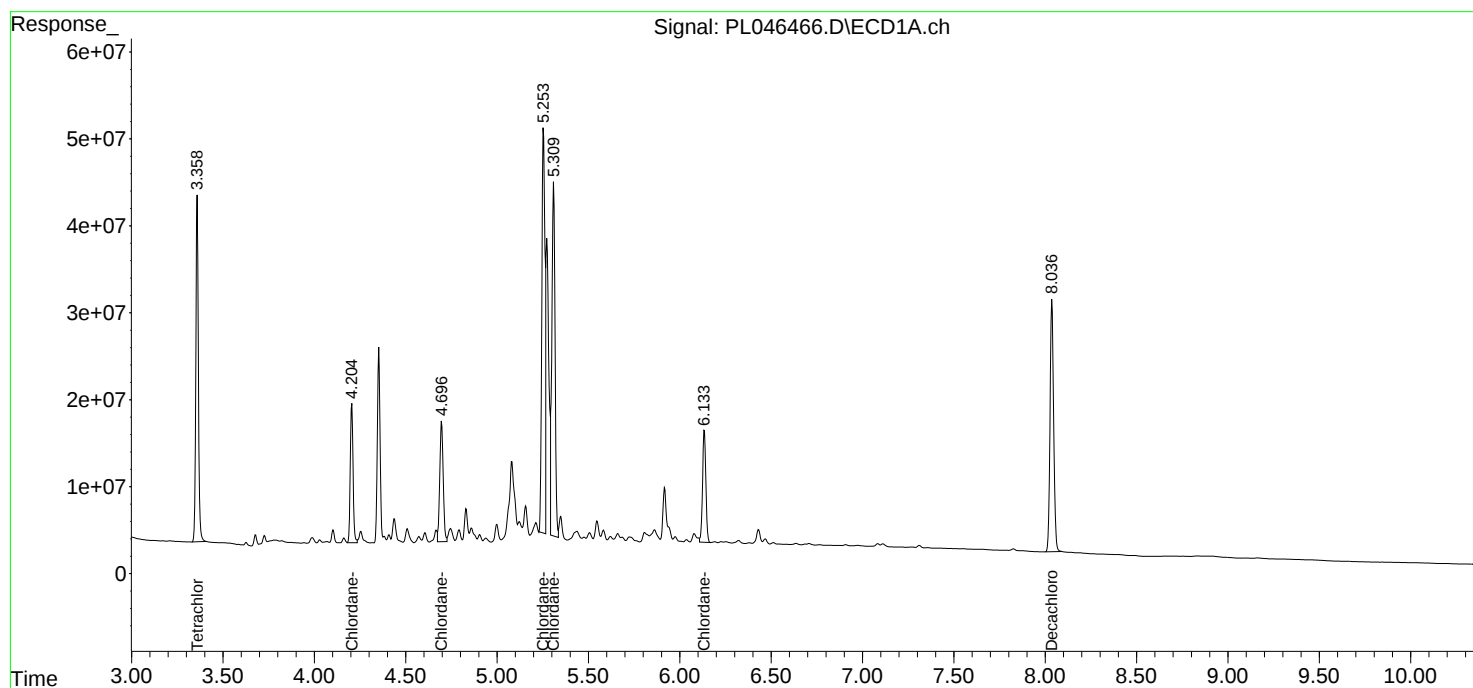


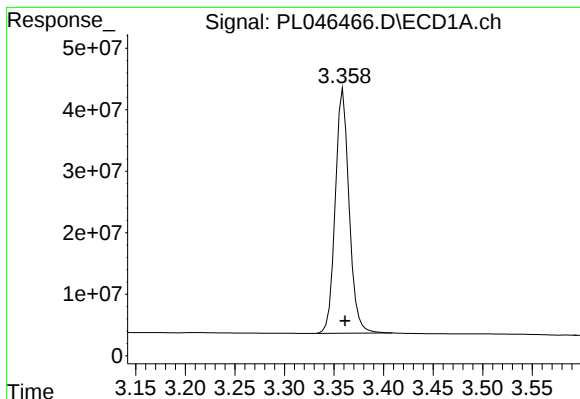

#1 Tetrachloro-m-xylene


R.T.: 3.359 min
Delta R.T.: -0.002 min
Response: 385608201
Conc: 53.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

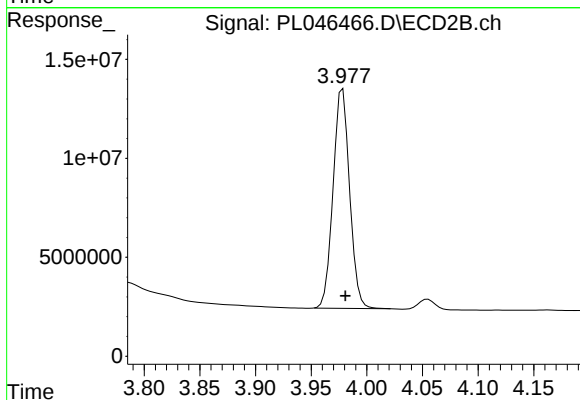


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.002 min
Response: 114635694
Conc: 50.07 ng/ml

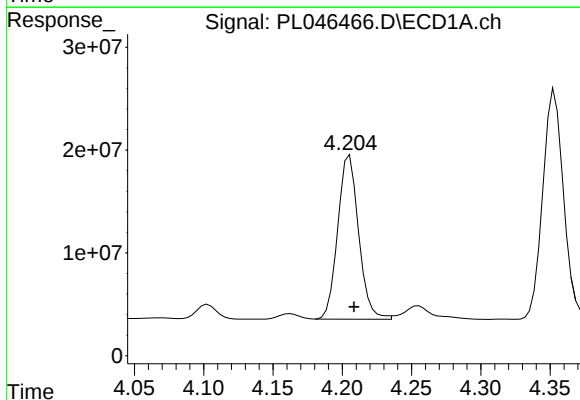


#23 Chlordane-1

R.T.: 4.205 min
Delta R.T.: -0.003 min
Response: 167220266
Conc: 497.24 ng/ml

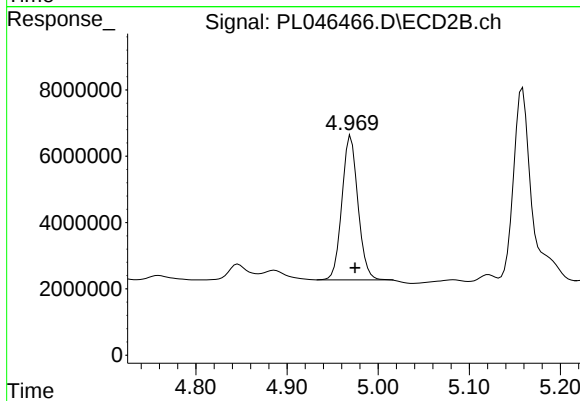

#23 Chlordane-1


R.T.: 4.970 min
Delta R.T.: -0.005 min
Response: 53016376
Conc: 489.91 ng/ml

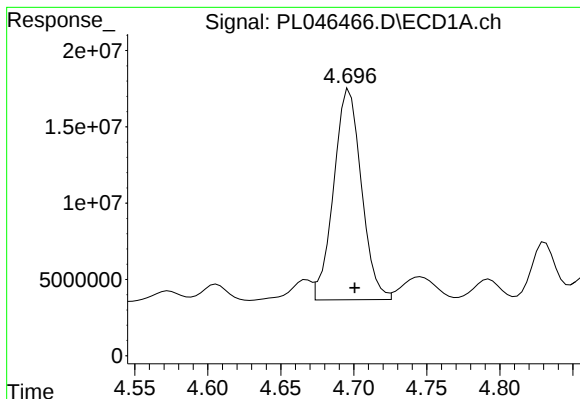

#24 Chlordane-2


R.T.: 4.697 min
Delta R.T.: -0.004 min
Response: 182573631
Conc: 481.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

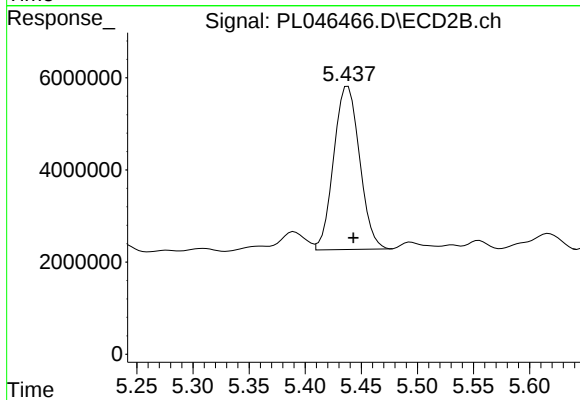


#24 Chlordane-2

R.T.: 5.438 min
Delta R.T.: -0.005 min
Response: 56859138
Conc: 486.77 ng/ml

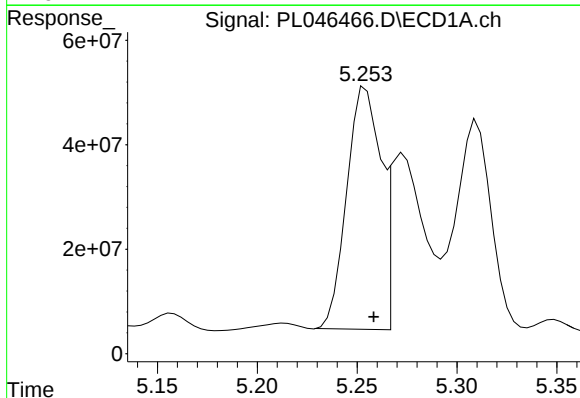


#25 Chlordane-3

R.T.: 5.254 min
Delta R.T.: -0.004 min
Response: 548325754
Conc: 492.36 ng/ml

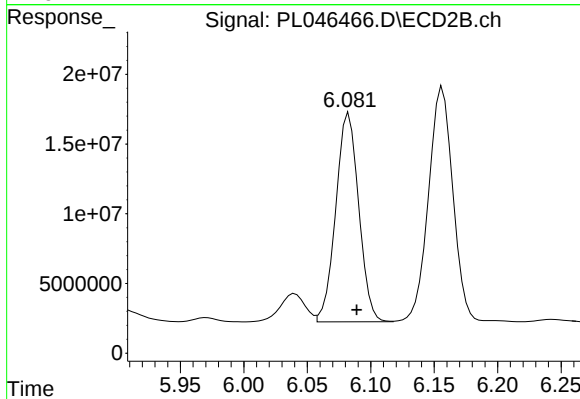

#25 Chlordane-3


R.T.: 6.083 min
Delta R.T.: -0.006 min
Response: 188523782
Conc: 494.47 ng/ml

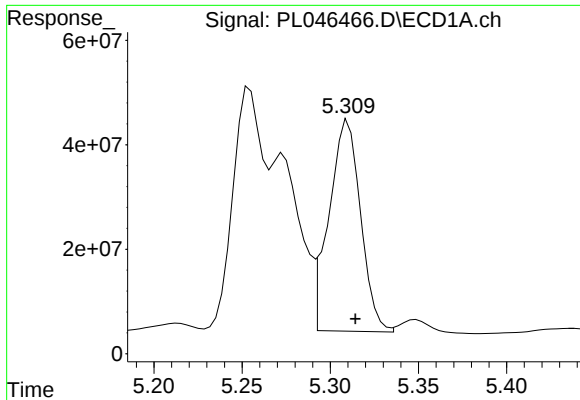

#26 Chlordane-4


R.T.: 5.310 min
Delta R.T.: -0.004 min
Response: 505192809
Conc: 488.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

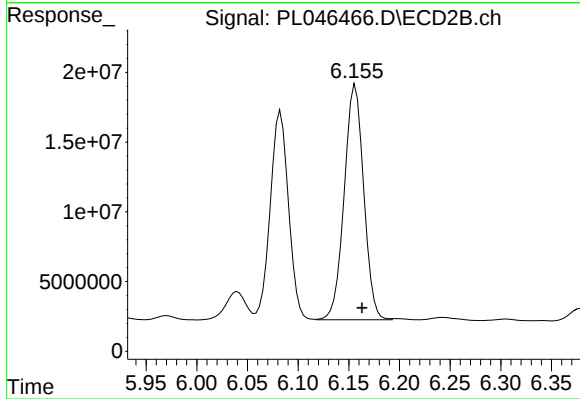


#26 Chlordane-4

R.T.: 6.157 min
Delta R.T.: -0.007 min
Response: 225636084
Conc: 489.00 ng/ml

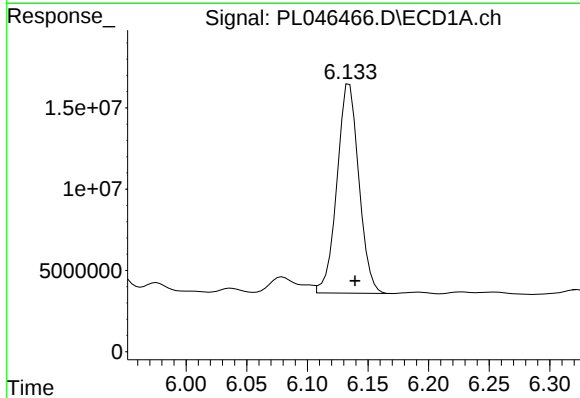


#27 Chlordane-5

R.T.: 6.135 min
Delta R.T.: -0.005 min
Response: 161514638
Conc: 473.28 ng/ml

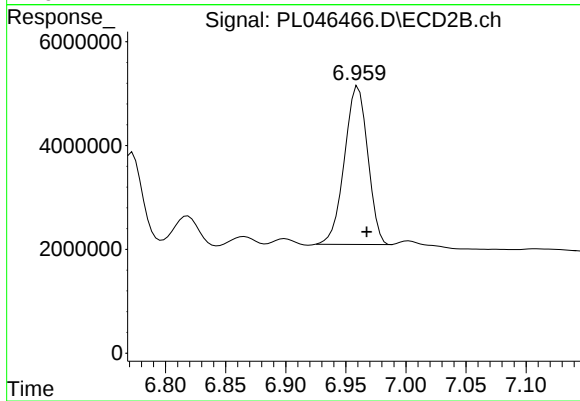

#27 Chlordane-5

R.T.: 6.960 min
Delta R.T.: -0.007 min
Response: 41195795
Conc: 458.56 ng/ml

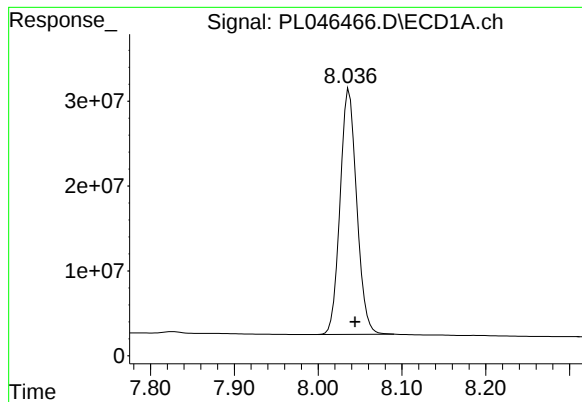

#28 Decachlorobiphenyl


R.T.: 8.037 min

Delta R.T.: -0.007 min

Response: 398779530

Conc: 47.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

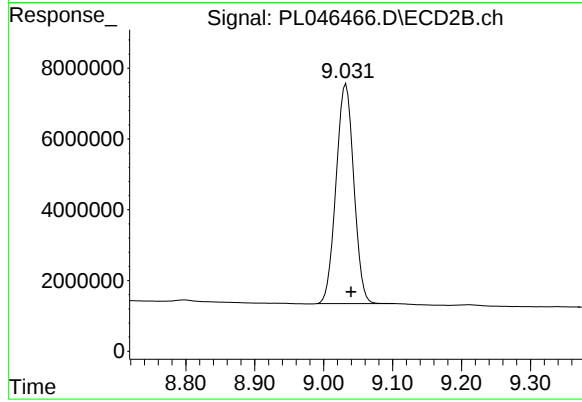

#28 Decachlorobiphenyl

R.T.: 9.032 min

Delta R.T.: -0.007 min

Response: 111115715

Conc: 47.93 ng/ml