

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
 Data File : PL046468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 12:26
 Operator : AJ\SJ
 Sample : MDL-CHL-S-02
 Misc : 25 PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 MDL-CHL-S-02

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:05:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.360	3.978	134.8E6	43550014	18.533	19.021
28)	SA Decachlor...	8.037	9.031	165.7E6	48105465	19.705	20.749
Target Compounds							
23)	Chlordane-1	4.206	4.969	6545824	2280088	19.465	21.070
24)	Chlordane-2	4.697	5.437	9017442	2991524	23.766	25.610
25)	Chlordane-3	5.254	6.082	21508064	9103587	19.313	23.877
26)	Chlordane-4	5.310	6.156	20406049	11264512	19.734	24.412
27)	Chlordane-5	6.134	6.959	6098964	1896517	17.872	21.110



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032619\
Data File : PL046468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 12:26
Operator : AJ\SJ
Sample : MDL-CHL-S-02
Misc : 25 PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-02

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:05:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

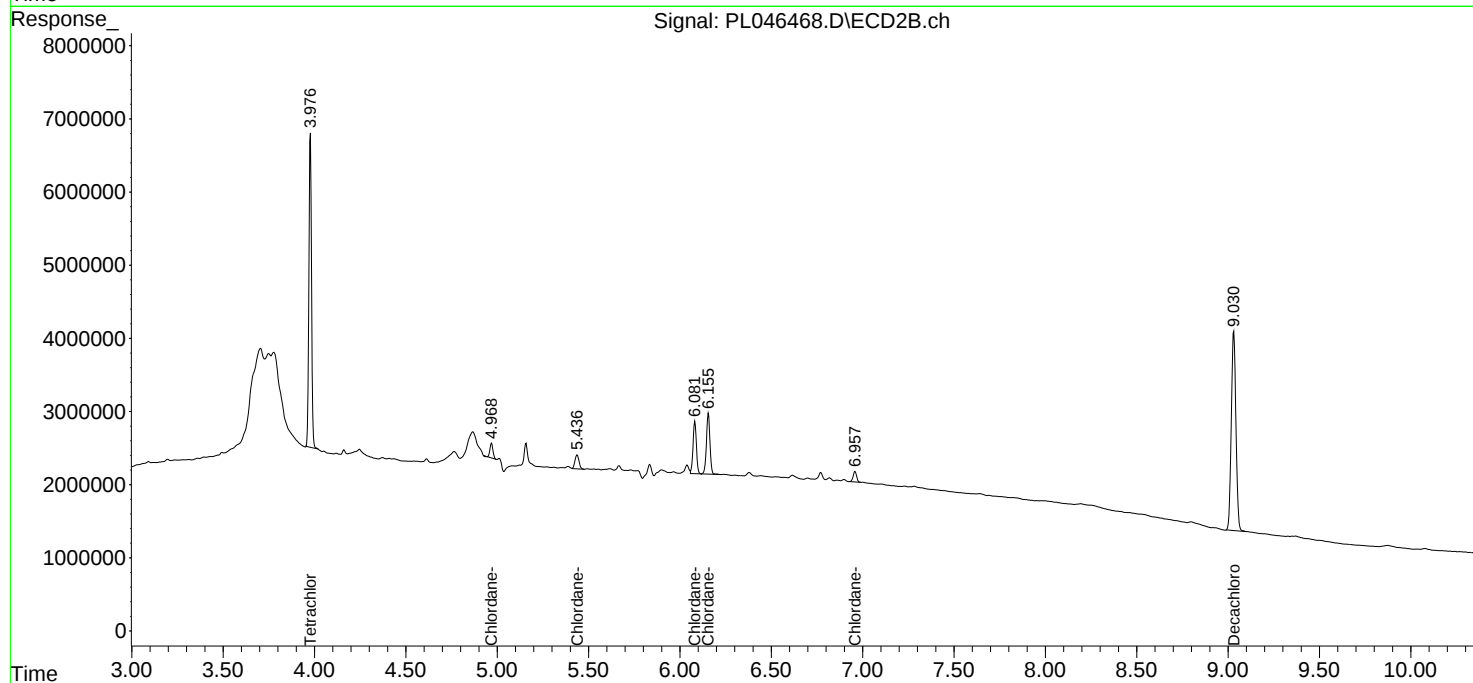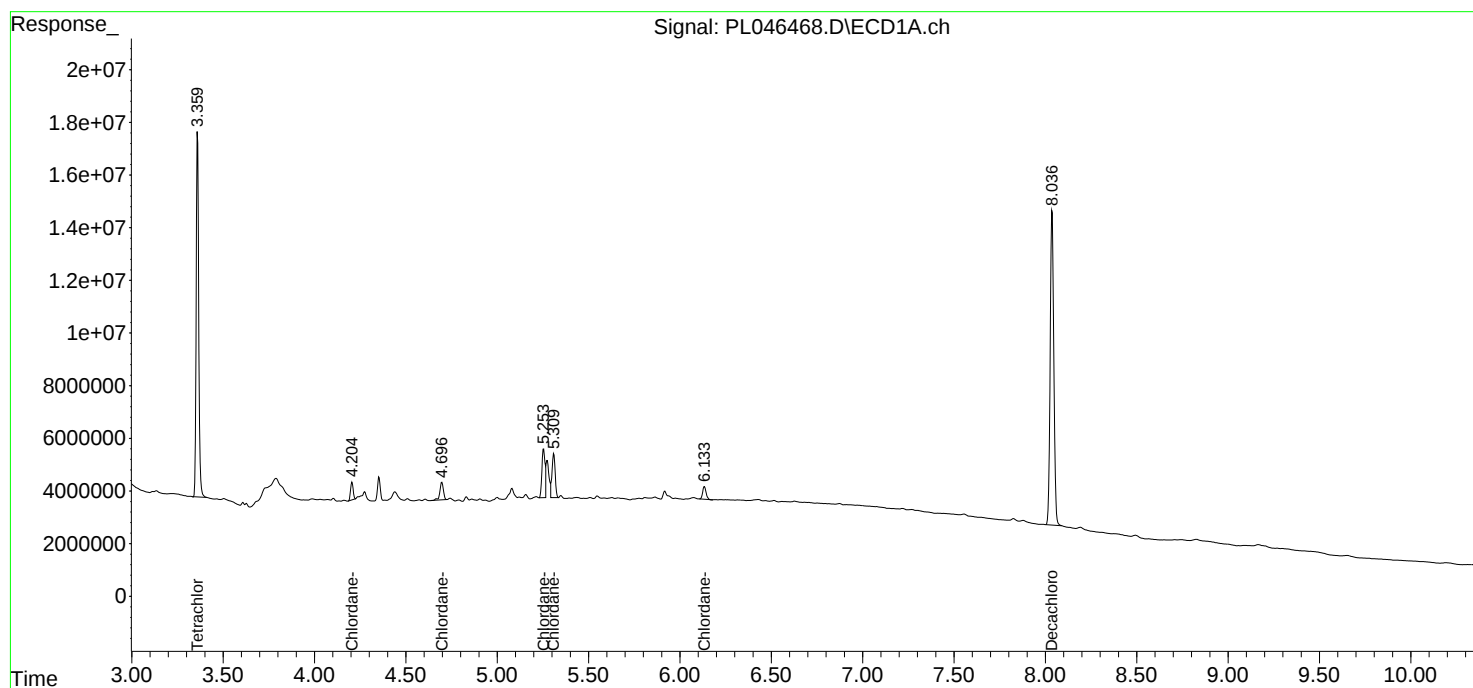


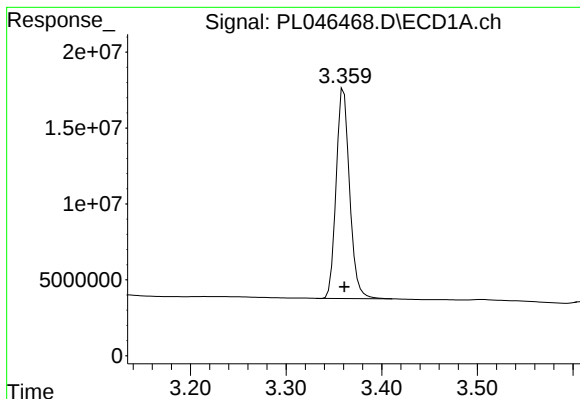

#1 Tetrachloro-m-xylene


R.T.: 3.360 min
Delta R.T.: 0.000 min
Response: 134822038
Conc: 18.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-02

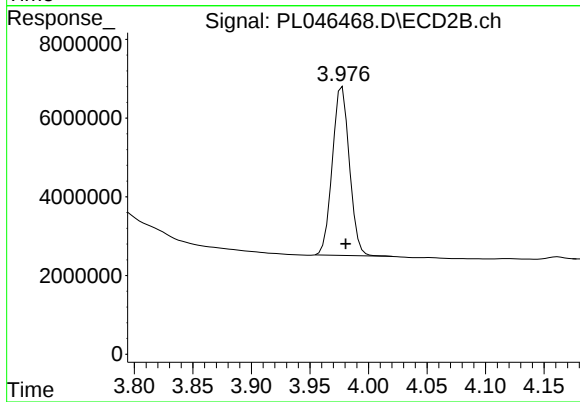


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.003 min
Response: 43550014
Conc: 19.02 ng/ml

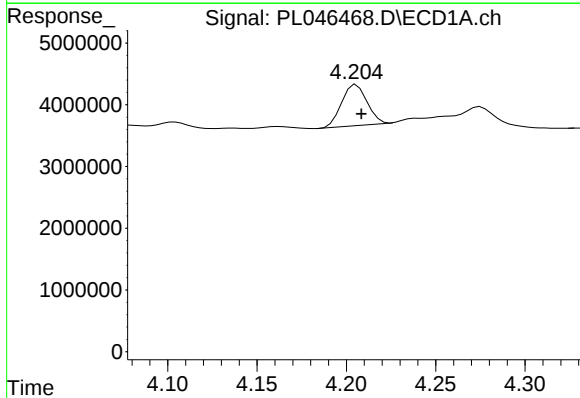


#23 Chlordane-1

R.T.: 4.206 min
Delta R.T.: -0.003 min
Response: 6545824
Conc: 19.46 ng/ml

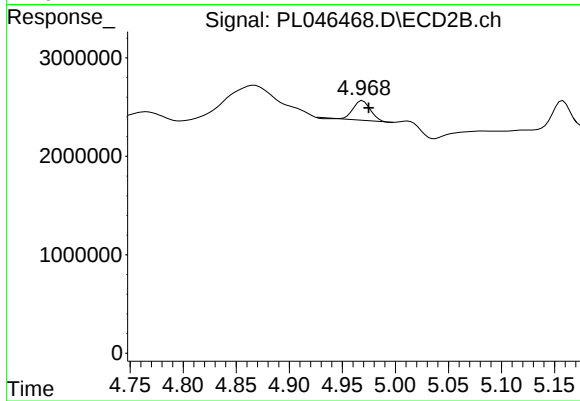

#23 Chlordane-1


R.T.: 4.969 min
Delta R.T.: -0.006 min
Response: 2280088
Conc: 21.07 ng/ml

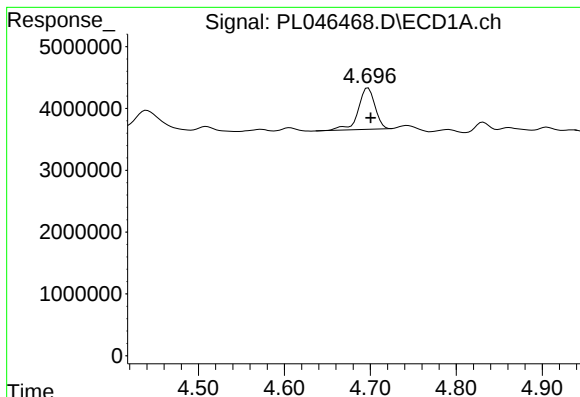

#24 Chlordane-2


R.T.: 4.697 min
Delta R.T.: -0.003 min
Response: 9017442
Conc: 23.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-02

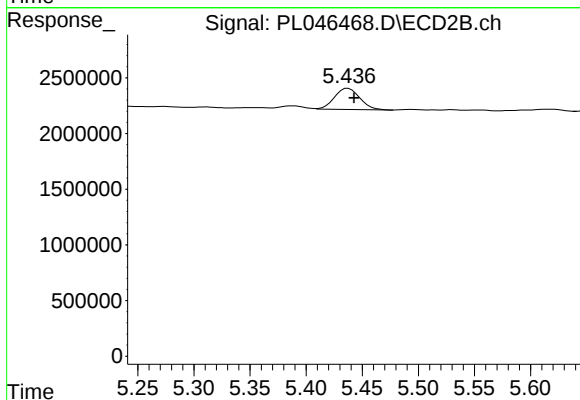


#24 Chlordane-2

R.T.: 5.437 min
Delta R.T.: -0.005 min
Response: 2991524
Conc: 25.61 ng/ml

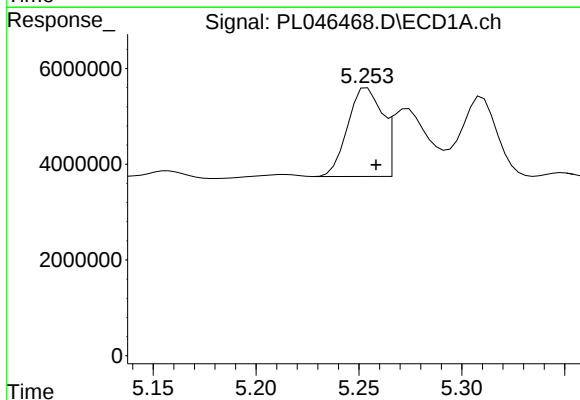


#25 Chlordane-3

R.T.: 5.254 min
Delta R.T.: -0.004 min
Response: 21508064
Conc: 19.31 ng/ml

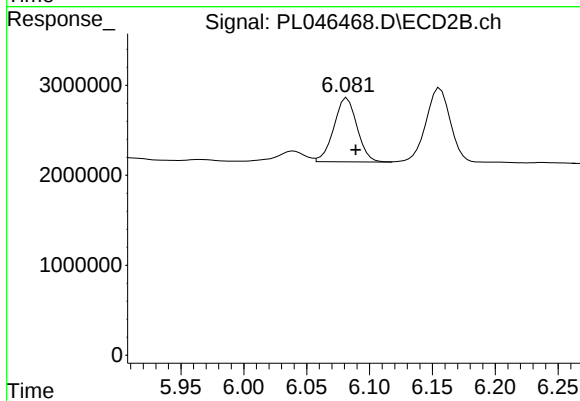

#25 Chlordane-3


R.T.: 6.082 min
Delta R.T.: -0.007 min
Response: 9103587
Conc: 23.88 ng/ml

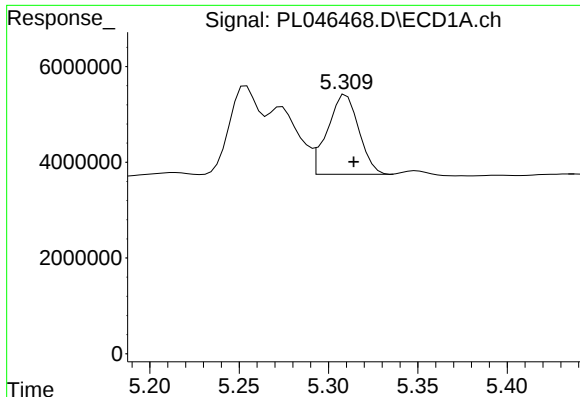

#26 Chlordane-4


R.T.: 5.310 min
Delta R.T.: -0.004 min
Response: 20406049
Conc: 19.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-02

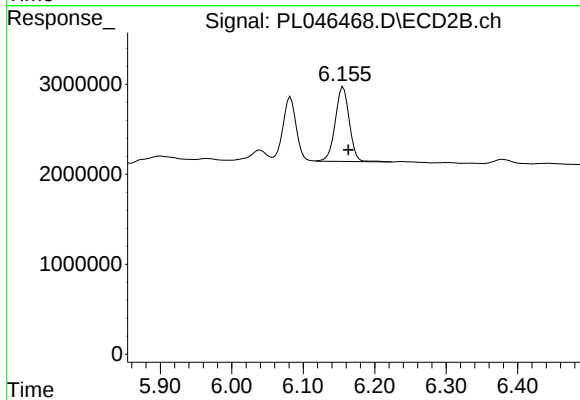


#26 Chlordane-4

R.T.: 6.156 min
Delta R.T.: -0.007 min
Response: 11264512
Conc: 24.41 ng/ml

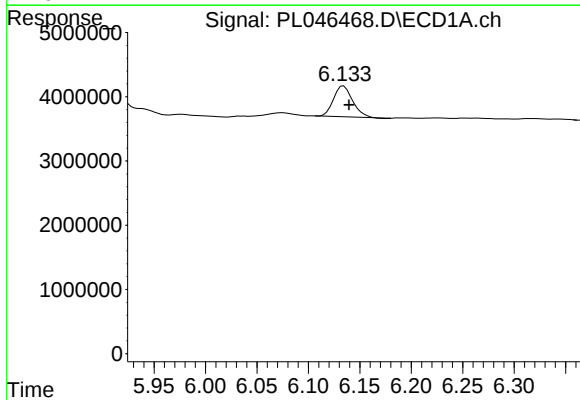


#27 Chlordane-5

R.T.: 6.134 min
Delta R.T.: -0.005 min
Response: 6098964
Conc: 17.87 ng/ml

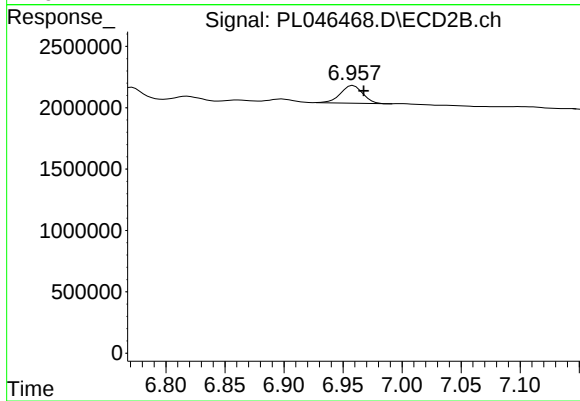

#27 Chlordane-5

R.T.: 6.959 min
Delta R.T.: -0.009 min
Response: 1896517
Conc: 21.11 ng/ml

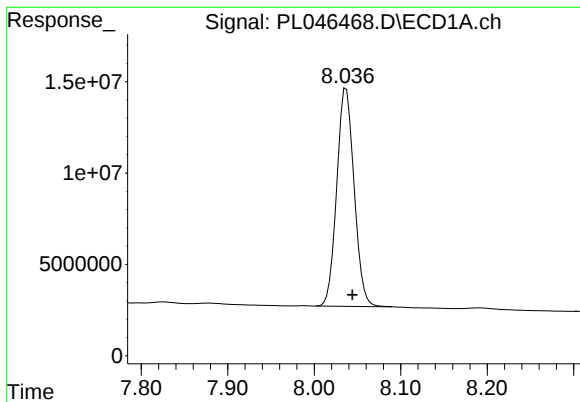

#28 Decachlorobiphenyl


R.T.: 8.037 min

Delta R.T.: -0.007 min

Response: 165742334

Conc: 19.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
MDL-CHL-S-02

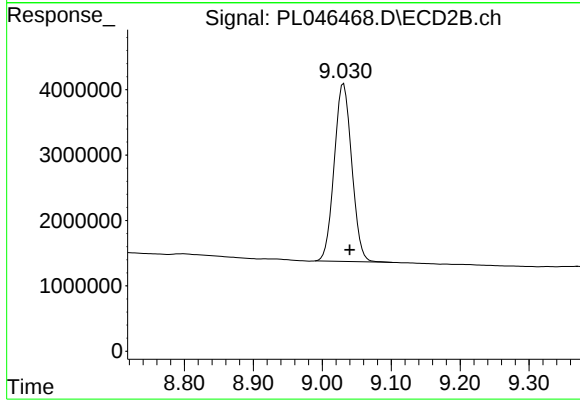

#28 Decachlorobiphenyl

R.T.: 9.031 min

Delta R.T.: -0.009 min

Response: 48105465

Conc: 20.75 ng/ml